

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081224\
 Data File : P0105453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 01:20
 Operator : YP/AJ
 Sample : P3390-07
 Misc : AR1268 LOD 40 PPB
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:43:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.427	3.536	170.9E6	65808365	19.563	20.952
2)	SA Decachlor...	10.217	8.425	136.9E6	43035997	23.800	24.309
Target Compounds							
3)	L1 AR-1016-1	5.594	4.612	84752	287097	0.280	2.555 #
4)	L1 AR-1016-2	5.622	4.612	155284	287097	0.363	1.844 #
5)	L1 AR-1016-3	5.668	4.779	242445	52750	0.945	0.630 #
6)	L1 AR-1016-4	5.787	4.831	1005215	56178	4.596	0.834 #
7)	L1 AR-1016-5	6.073	5.031	511637	308060	2.391	3.681 #
8)	L2 AR-1221-1	4.634	3.756	2841504	85099	25.338	2.156 #
9)	L2 AR-1221-2	4.732	3.825	4135363	1772768	48.789	57.703
10)	L2 AR-1221-3	4.774	3.895	1733227	42560	7.124	0.476 #
11)	L3 AR-1232-1	4.774	3.895	1733227	42560	8.669	0.583 #
12)	L3 AR-1232-2	5.320	4.612	332931	287097	3.145	4.089 #
13)	L3 AR-1232-3	5.622	4.779	155284	52750	0.811	1.380 #
14)	L3 AR-1232-4	5.787	4.861	1005215	78262	10.306	2.250 #
15)	L3 AR-1232-5	5.880	5.031	96585	308060	1.340	8.727 #
16)	L4 AR-1242-1	5.594	4.612	84752	287097	0.365	3.255 #
17)	L4 AR-1242-2	5.622	4.612	155284	287097	0.476	2.418 #
18)	L4 AR-1242-3	5.668	4.779	242445	52750	1.229	0.812 #
19)	L4 AR-1242-4	5.787	4.861	1005215	78262	5.891	1.180 #
20)	L4 AR-1242-5	6.538	5.374	1439296	309724	8.236	3.769 #
21)	L5 AR-1248-1	5.594	4.612	84752	287097	0.464	4.111 #
22)	L5 AR-1248-2	5.880	4.831	96585	56178	0.383	0.592 #
23)	L5 AR-1248-3	6.073	4.861	511637	78262	1.810	0.784 #
24)	L5 AR-1248-4	6.483	5.031	1487906	308060	4.653	2.729 #
25)	L5 AR-1248-5	6.515	5.399	225045	879020	0.728	7.806 #
26)	L6 AR-1254-1	6.462	5.374	2381513	309724	7.594	1.902 #
27)	L6 AR-1254-2	6.684	5.529	170159	366027	0.377	2.502 #
28)	L6 AR-1254-3	7.052	5.910	3565838	511162	7.517	2.266 #
29)	L6 AR-1254-4	7.332	6.139	2033662	397665	5.677	2.818 #
30)	L6 AR-1254-5	7.769	6.552	2301394	127883	5.797	0.638 #
31)	L7 AR-1260-1	7.237	6.039	1503673	147150	4.103	0.943 #
32)	L7 AR-1260-2	7.483	6.214	1809022	871307	4.345	4.610
33)	L7 AR-1260-3	7.835	6.387	10029649	3198159	38.752	17.312 #
34)	L7 AR-1260-4	8.083	6.842	16217637	2985424	49.155	24.425 #
35)	L7 AR-1260-5	8.386	7.085	6747260	1759534	11.342	6.322 #
36)	L8 AR-1262-1	7.769	6.552	2301394	127883	7.245	1.202 #
37)	L8 AR-1262-2	8.386	6.842	6747260	2985424	8.970	17.569 #
38)	L8 AR-1262-3	8.699	7.364	24067575	10909362	48.909	86.410 #
39)	L8 AR-1262-4	8.794	7.429	22652853	9997665	61.689	43.189 #
40)	L8 AR-1262-5	9.456	7.917	6884470	3342566	25.706	33.259 #
41)	L9 AR-1268-1	8.699	7.364	24067575	10909362	29.592	31.248

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081224\
 Data File : P0105453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 01:20
 Operator : YP/AJ
 Sample : P3390-07
 Misc : AR1268 LOD 40 PPB
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:43:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.794	7.429	22652853	9997665	31.162	32.046
43) L9	AR-1268-3	9.025	7.632	18891168	8205792	29.262	32.466
44) L9	AR-1268-4	9.456	7.917	6884470	3342566	24.724	31.078 #
45) L9	AR-1268-5	9.873	8.190	58074950	20210825	27.776	30.215

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-OT3-2024

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

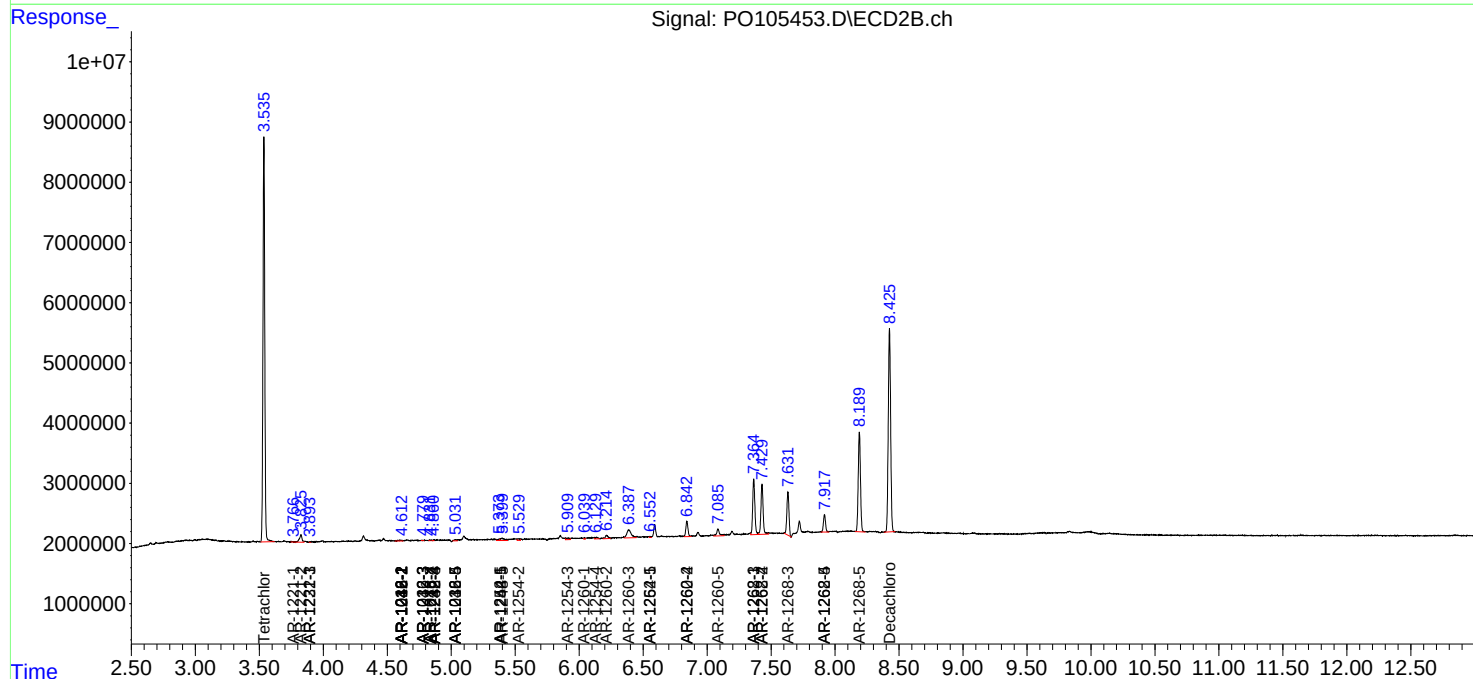


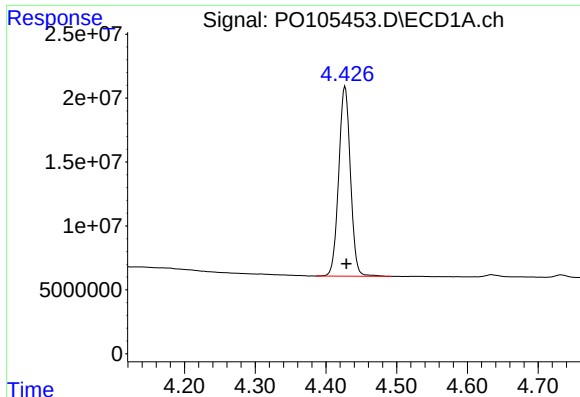

#1 Tetrachloro-m-xylene


R.T.: 4.427 min
Delta R.T.: -0.002 min
Response: 170870627
Conc: 19.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

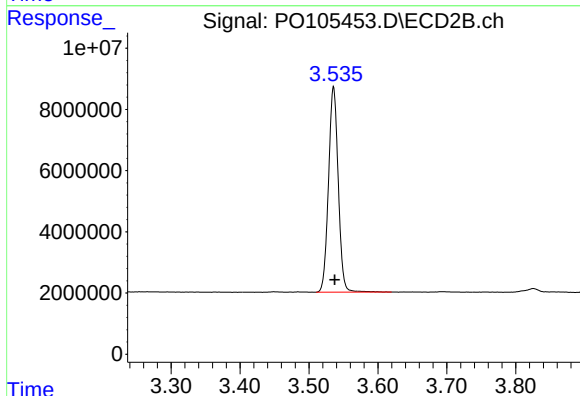


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 65808365
Conc: 20.95 ng/ml

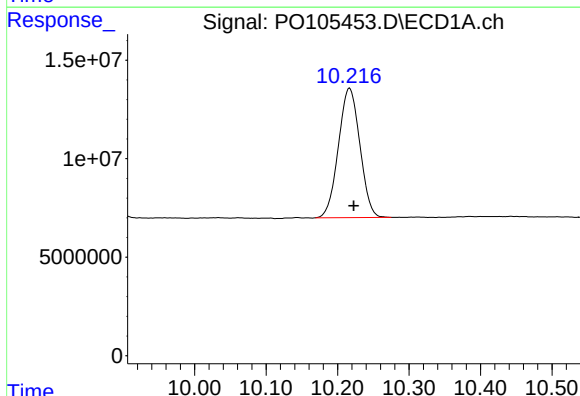


#2 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: -0.006 min
Response: 136907302
Conc: 23.80 ng/ml

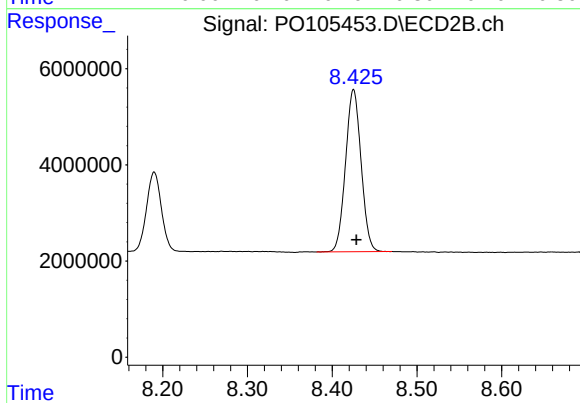

#2 Decachlorobiphenyl


R.T.: 8.425 min
Delta R.T.: -0.003 min
Response: 43035997
Conc: 24.31 ng/ml

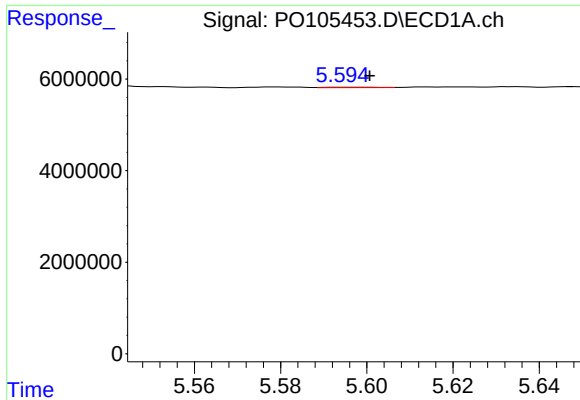

#3 AR-1016-1


R.T.: 5.594 min
Delta R.T.: -0.007 min
Response: 84752
Conc: 0.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

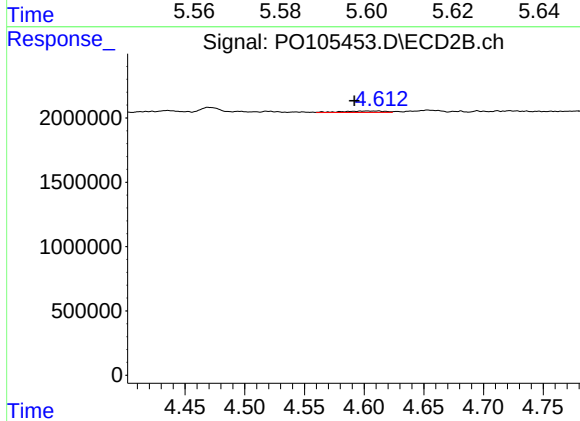


#3 AR-1016-1

R.T.: 4.612 min
Delta R.T.: 0.020 min
Response: 287097
Conc: 2.55 ng/ml

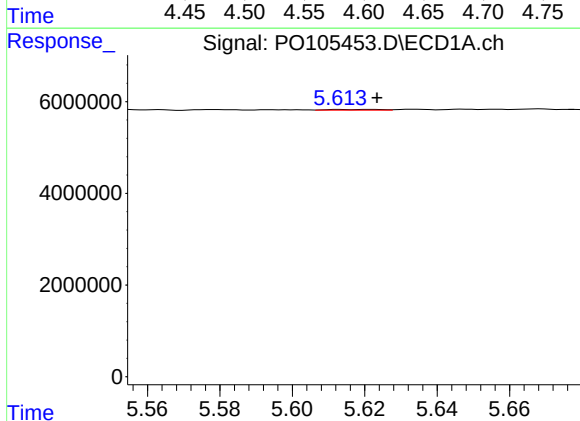


#4 AR-1016-2

R.T.: 5.622 min
Delta R.T.: -0.002 min
Response: 155284
Conc: 0.36 ng/ml

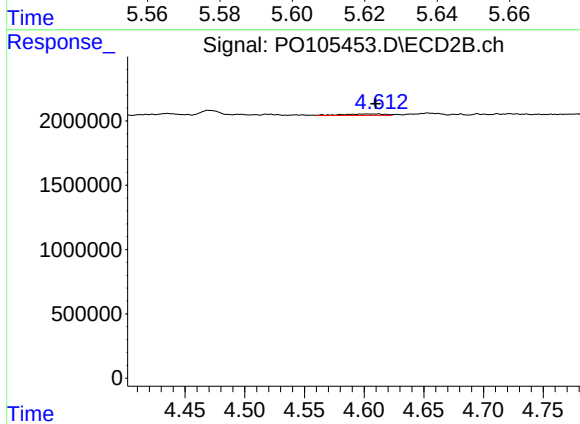

#4 AR-1016-2


R.T.: 4.612 min
Delta R.T.: 0.002 min
Response: 287097
Conc: 1.84 ng/ml

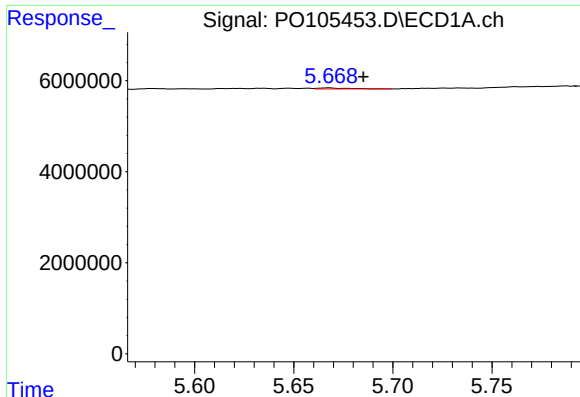

#5 AR-1016-3


R.T.: 5.668 min
Delta R.T.: -0.017 min
Response: 242445
Conc: 0.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

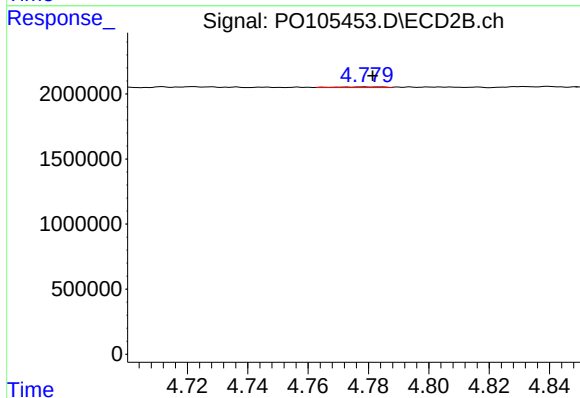


#5 AR-1016-3

R.T.: 4.779 min
Delta R.T.: -0.003 min
Response: 52750
Conc: 0.63 ng/ml

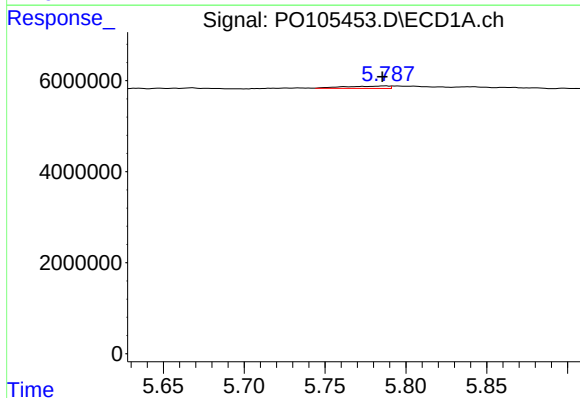


#6 AR-1016-4

R.T.: 5.787 min
Delta R.T.: 0.002 min
Response: 1005215
Conc: 4.60 ng/ml

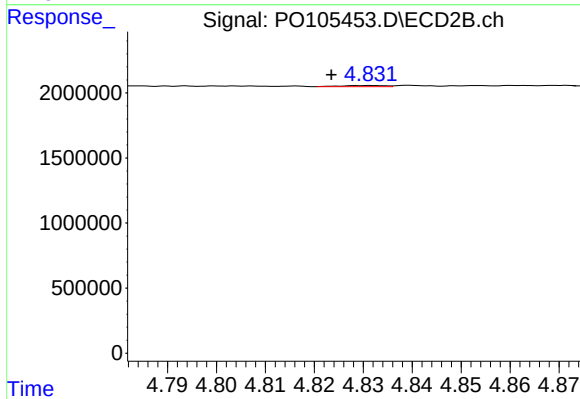

#6 AR-1016-4


R.T.: 4.831 min
Delta R.T.: 0.007 min
Response: 56178
Conc: 0.83 ng/ml

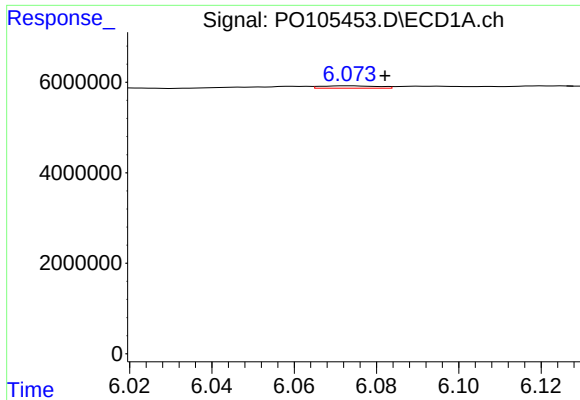

#7 AR-1016-5


R.T.: 6.073 min
Delta R.T.: -0.009 min
Response: 511637
Conc: 2.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

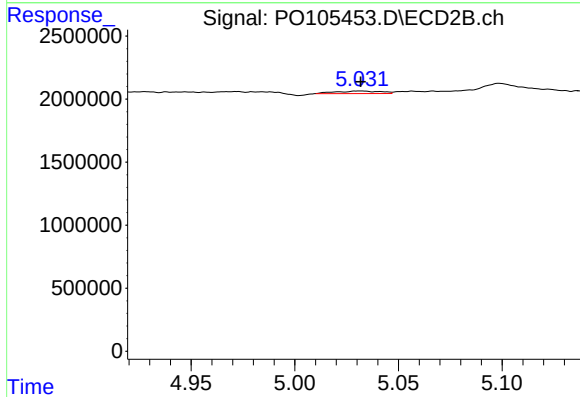


#7 AR-1016-5

R.T.: 5.031 min
Delta R.T.: 0.000 min
Response: 308060
Conc: 3.68 ng/ml

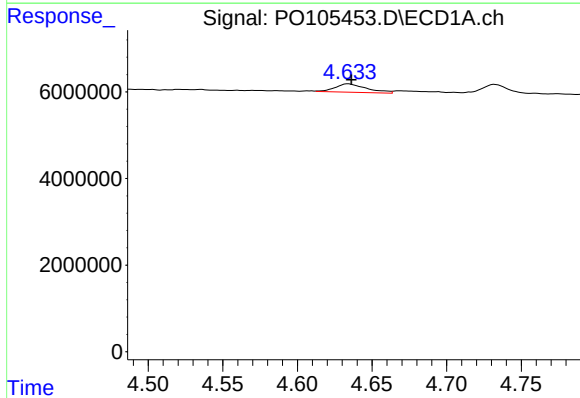


#8 AR-1221-1

R.T.: 4.634 min
Delta R.T.: -0.002 min
Response: 2841504
Conc: 25.34 ng/ml

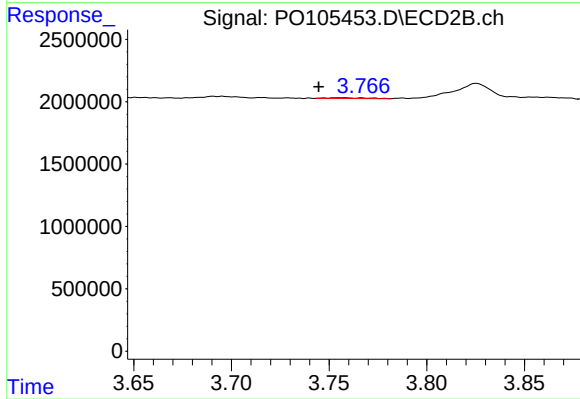

#8 AR-1221-1


R.T.: 3.756 min
Delta R.T.: 0.011 min
Response: 85099
Conc: 2.16 ng/ml

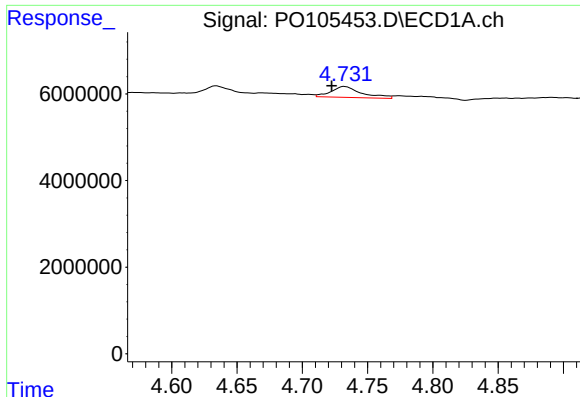

#9 AR-1221-2


R.T.: 4.732 min
Delta R.T.: 0.010 min
Response: 4135363
Conc: 48.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

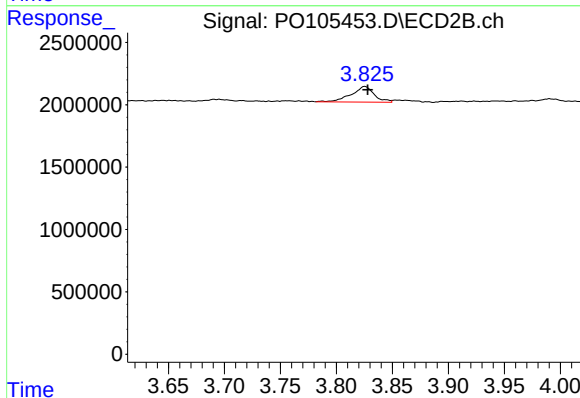


#9 AR-1221-2

R.T.: 3.825 min
Delta R.T.: -0.003 min
Response: 1772768
Conc: 57.70 ng/ml

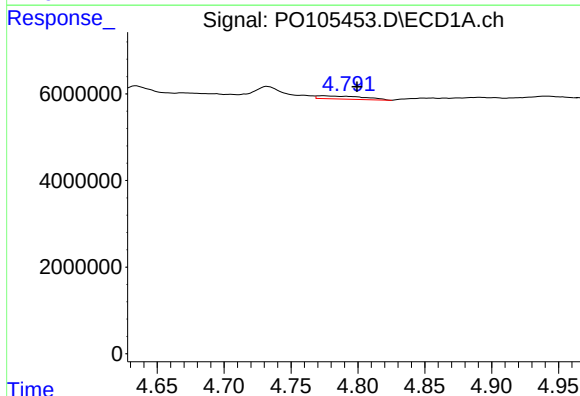


#10 AR-1221-3

R.T.: 4.774 min
Delta R.T.: -0.025 min
Response: 1733227
Conc: 7.12 ng/ml

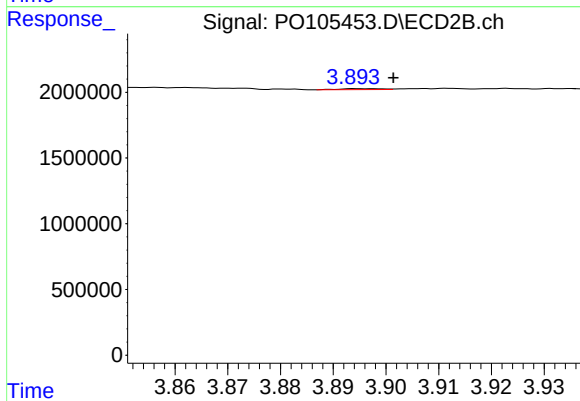

#10 AR-1221-3


R.T.: 3.895 min
Delta R.T.: -0.006 min
Response: 42560
Conc: 0.48 ng/ml

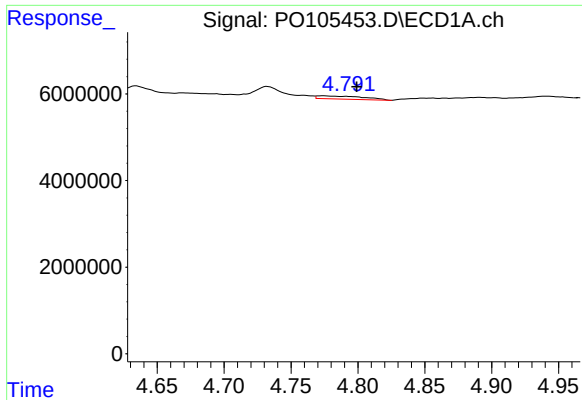

#11 AR-1232-1


R.T.: 4.774 min
Delta R.T.: -0.025 min
Response: 1733227
Conc: 8.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

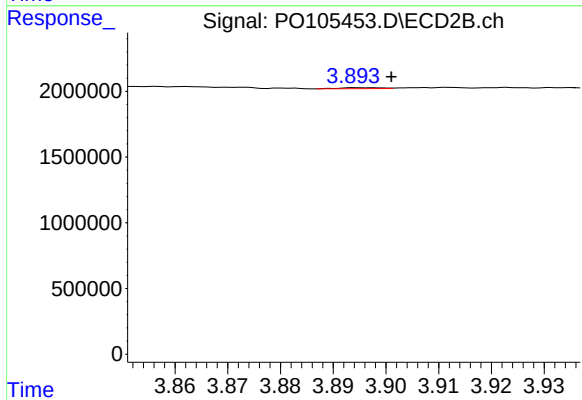


#11 AR-1232-1

R.T.: 3.895 min
Delta R.T.: -0.006 min
Response: 42560
Conc: 0.58 ng/ml

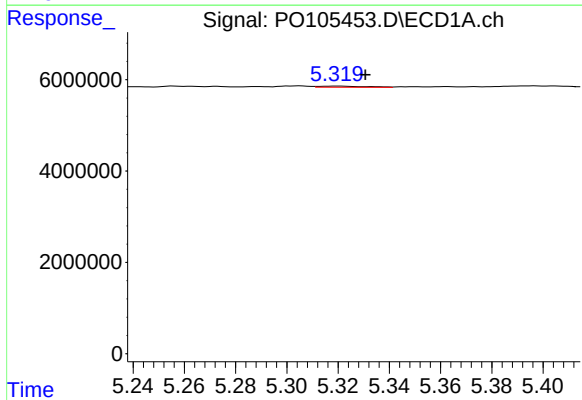


#12 AR-1232-2

R.T.: 5.320 min
Delta R.T.: -0.011 min
Response: 332931
Conc: 3.15 ng/ml

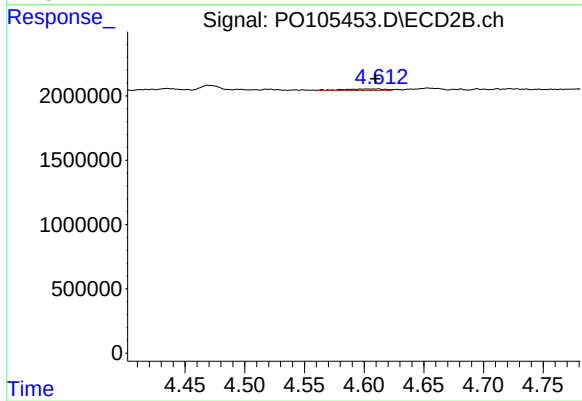

#12 AR-1232-2


R.T.: 4.612 min
Delta R.T.: 0.002 min
Response: 287097
Conc: 4.09 ng/ml

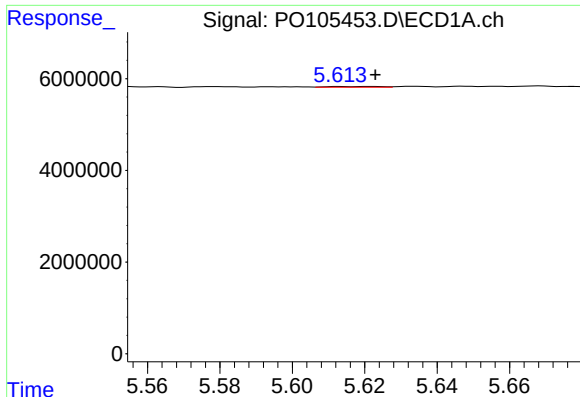

#13 AR-1232-3


R.T.: 5.622 min
Delta R.T.: -0.001 min
Response: 155284
Conc: 0.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

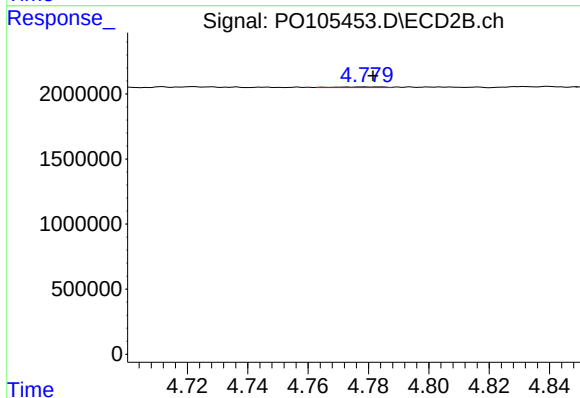


#13 AR-1232-3

R.T.: 4.779 min
Delta R.T.: -0.003 min
Response: 52750
Conc: 1.38 ng/ml

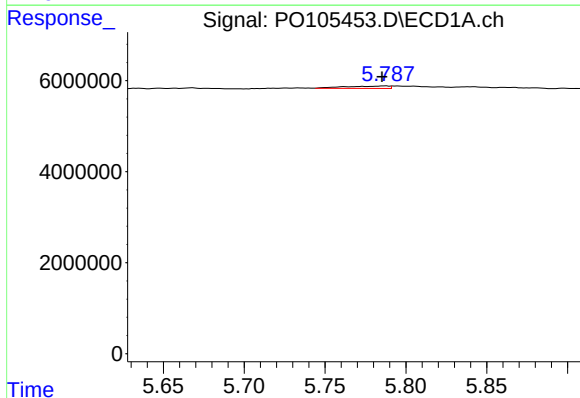


#14 AR-1232-4

R.T.: 5.787 min
Delta R.T.: 0.002 min
Response: 1005215
Conc: 10.31 ng/ml

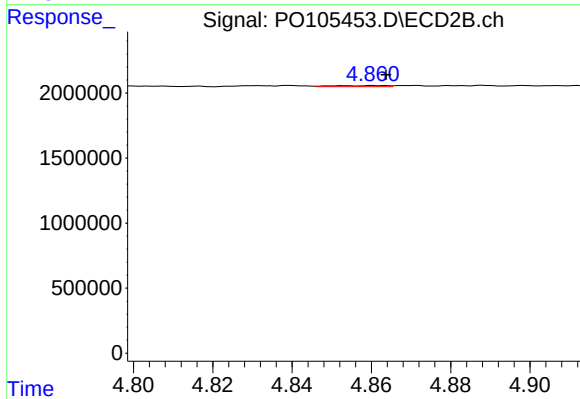

#14 AR-1232-4


R.T.: 4.861 min
Delta R.T.: -0.003 min
Response: 78262
Conc: 2.25 ng/ml

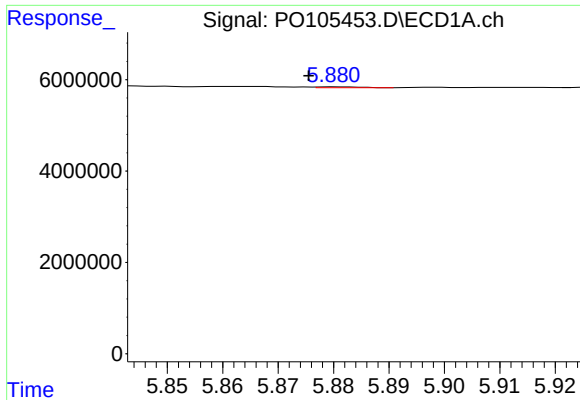

#15 AR-1232-5


R.T.: 5.880 min
Delta R.T.: 0.005 min
Response: 96585
Conc: 1.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

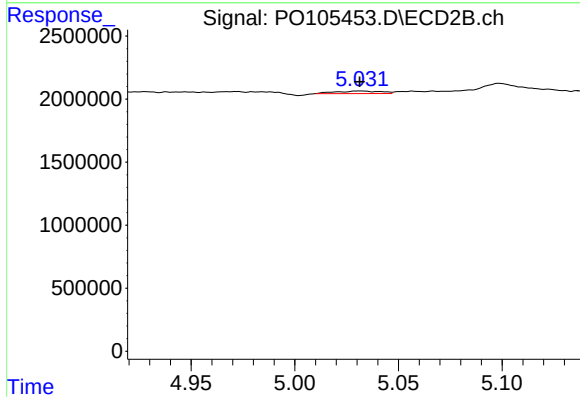


#15 AR-1232-5

R.T.: 5.031 min
Delta R.T.: 0.000 min
Response: 308060
Conc: 8.73 ng/ml

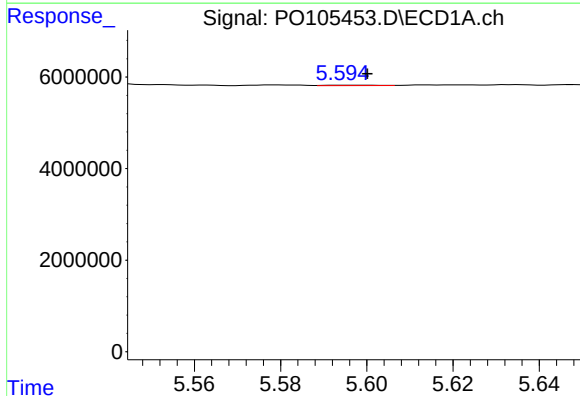


#16 AR-1242-1

R.T.: 5.594 min
Delta R.T.: -0.006 min
Response: 84752
Conc: 0.36 ng/ml

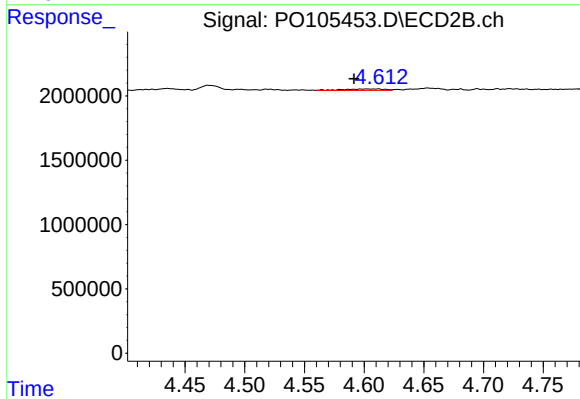

#16 AR-1242-1


R.T.: 4.612 min
Delta R.T.: 0.020 min
Response: 287097
Conc: 3.26 ng/ml

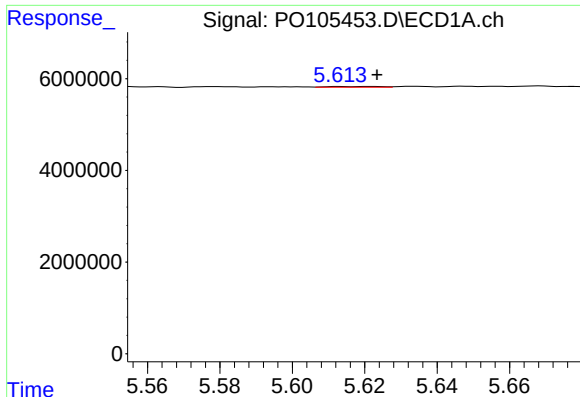

#17 AR-1242-2


R.T.: 5.622 min
Delta R.T.: -0.002 min
Response: 155284
Conc: 0.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

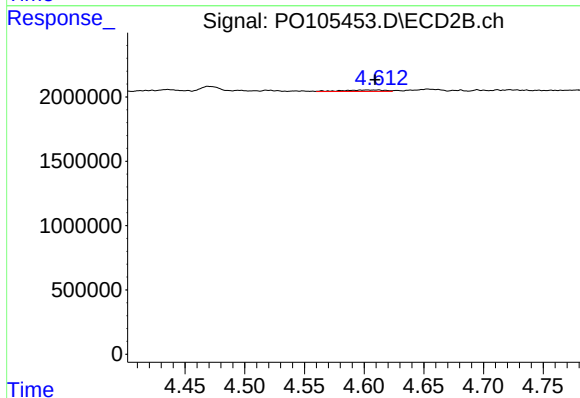


#17 AR-1242-2

R.T.: 4.612 min
Delta R.T.: 0.003 min
Response: 287097
Conc: 2.42 ng/ml

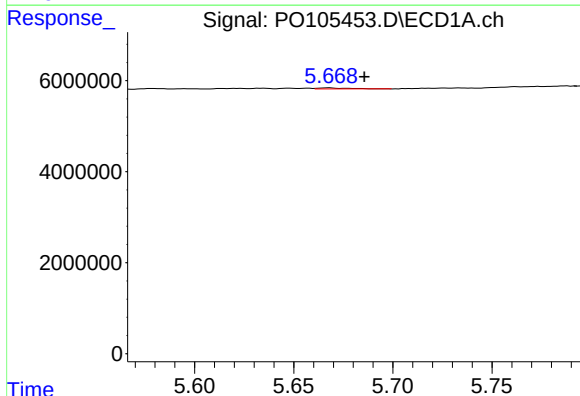


#18 AR-1242-3

R.T.: 5.668 min
Delta R.T.: -0.018 min
Response: 242445
Conc: 1.23 ng/ml

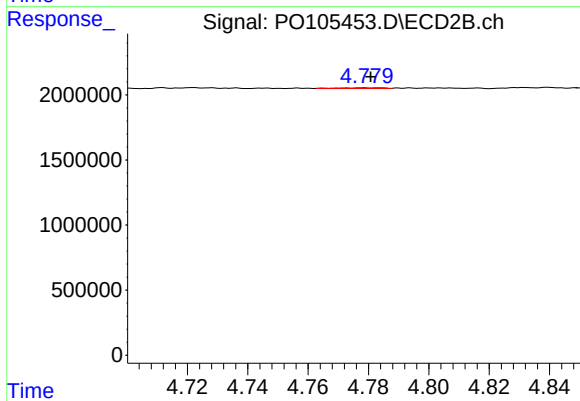

#18 AR-1242-3


R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 52750
Conc: 0.81 ng/ml

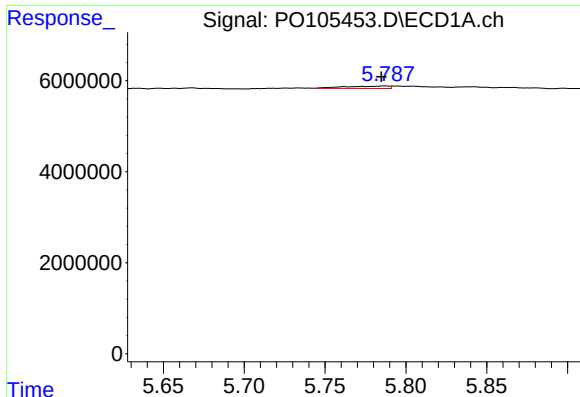

#19 AR-1242-4


R.T.: 5.787 min
Delta R.T.: 0.002 min
Response: 1005215
Conc: 5.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

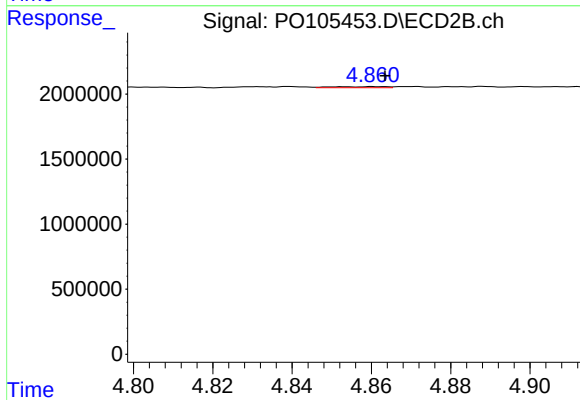


#19 AR-1242-4

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 78262
Conc: 1.18 ng/ml

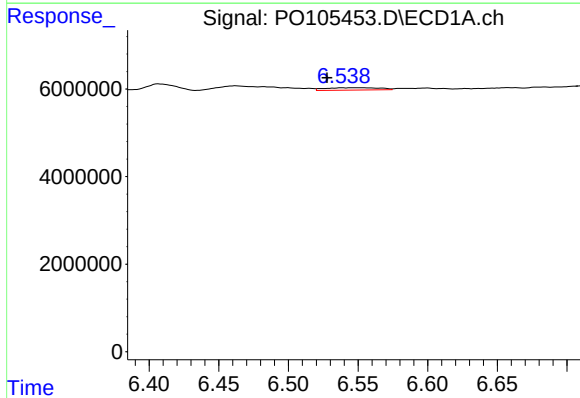


#20 AR-1242-5

R.T.: 6.538 min
Delta R.T.: 0.011 min
Response: 1439296
Conc: 8.24 ng/ml

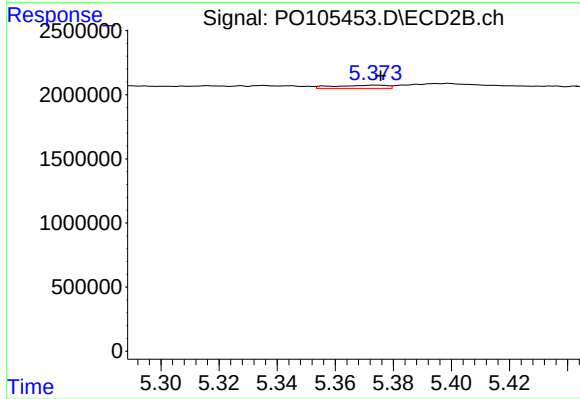

#20 AR-1242-5


R.T.: 5.374 min
Delta R.T.: -0.002 min
Response: 309724
Conc: 3.77 ng/ml

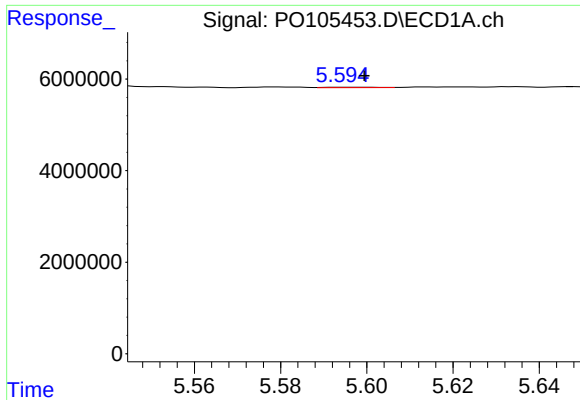

#21 AR-1248-1


R.T.: 5.594 min
Delta R.T.: -0.006 min
Response: 84752
Conc: 0.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

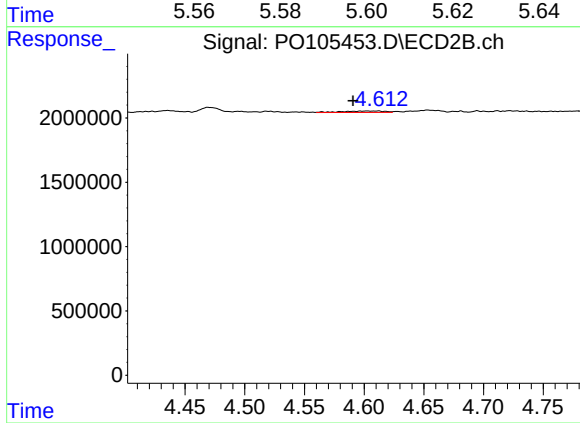


#21 AR-1248-1

R.T.: 4.612 min
Delta R.T.: 0.021 min
Response: 287097
Conc: 4.11 ng/ml

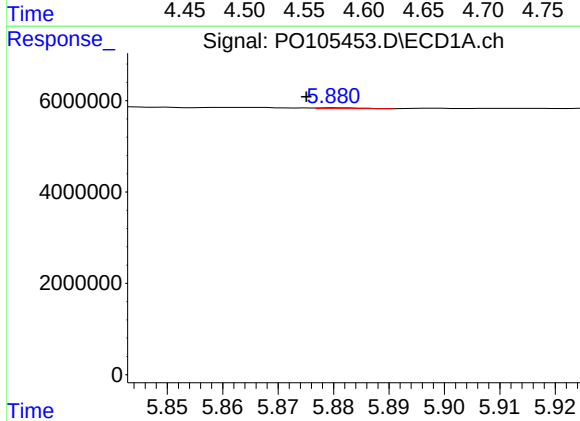


#22 AR-1248-2

R.T.: 5.880 min
Delta R.T.: 0.005 min
Response: 96585
Conc: 0.38 ng/ml

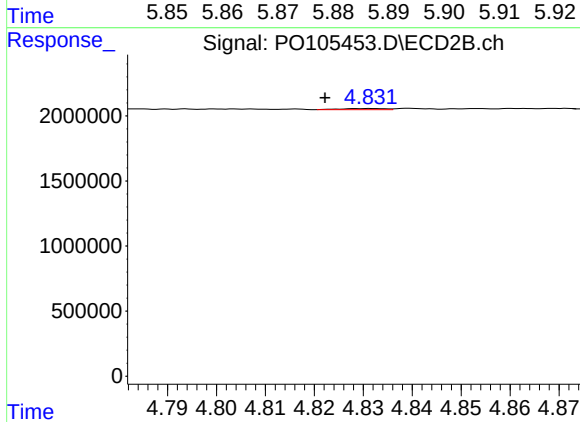

#22 AR-1248-2


R.T.: 4.831 min
Delta R.T.: 0.009 min
Response: 56178
Conc: 0.59 ng/ml

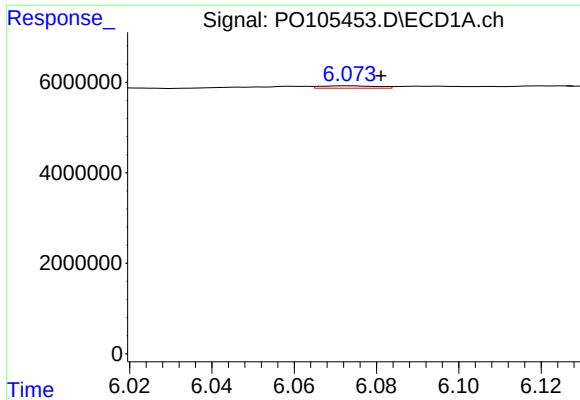

#23 AR-1248-3


R.T.: 6.073 min
Delta R.T.: -0.008 min
Response: 511637
Conc: 1.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

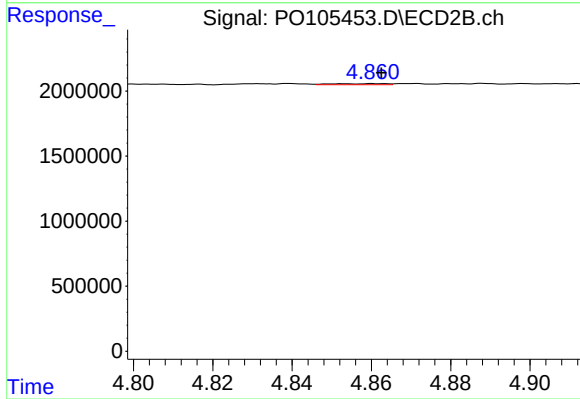


#23 AR-1248-3

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 78262
Conc: 0.78 ng/ml

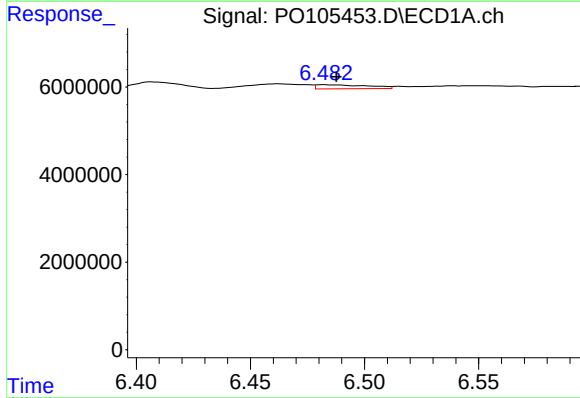


#24 AR-1248-4

R.T.: 6.483 min
Delta R.T.: -0.005 min
Response: 1487906
Conc: 4.65 ng/ml

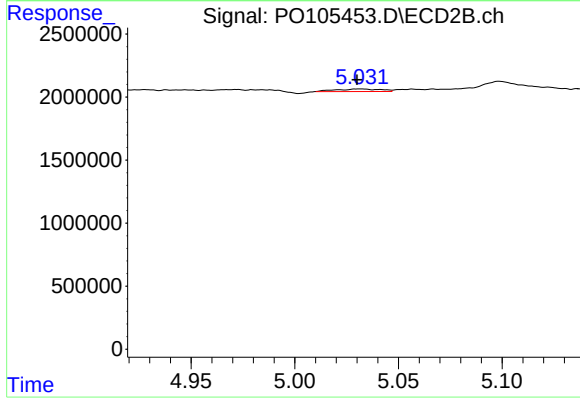

#24 AR-1248-4


R.T.: 5.031 min
Delta R.T.: 0.001 min
Response: 308060
Conc: 2.73 ng/ml

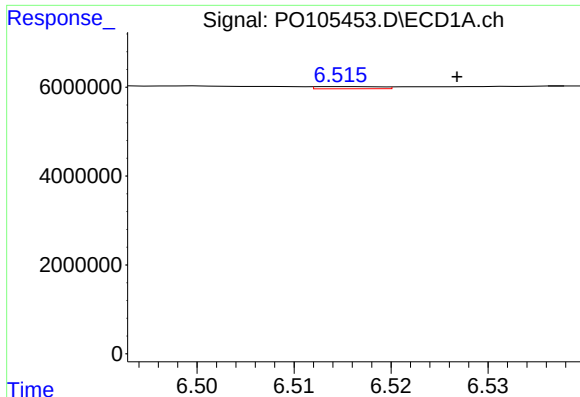

#25 AR-1248-5


R.T.: 6.515 min
Delta R.T.: -0.012 min
Response: 225045
Conc: 0.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

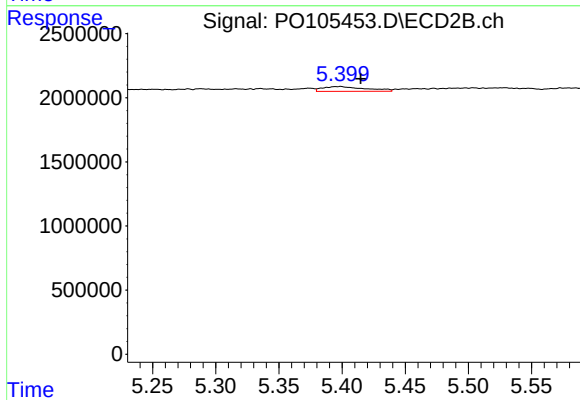


#25 AR-1248-5

R.T.: 5.399 min
Delta R.T.: -0.016 min
Response: 879020
Conc: 7.81 ng/ml

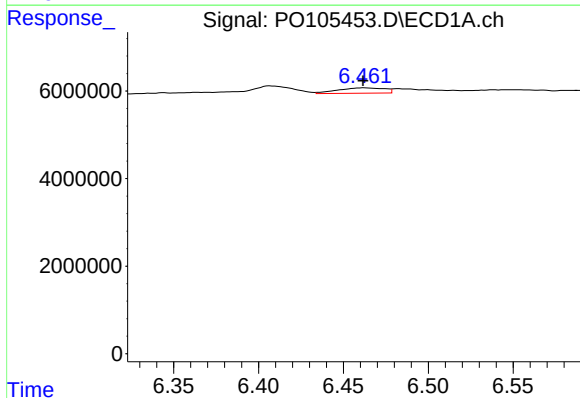


#26 AR-1254-1

R.T.: 6.462 min
Delta R.T.: 0.000 min
Response: 2381513
Conc: 7.59 ng/ml

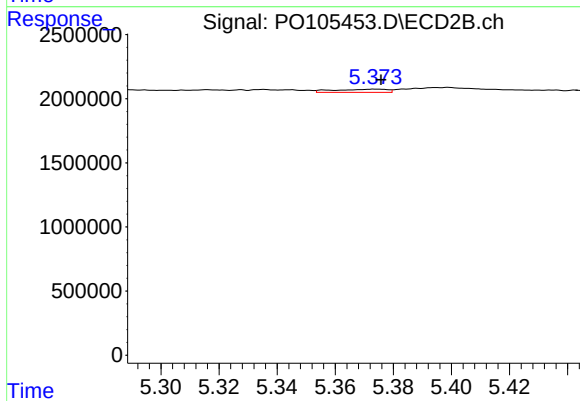

#26 AR-1254-1


R.T.: 5.374 min
Delta R.T.: -0.002 min
Response: 309724
Conc: 1.90 ng/ml

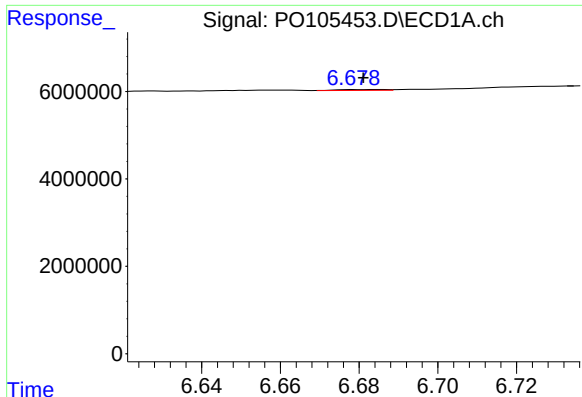

#27 AR-1254-2


R.T.: 6.684 min
Delta R.T.: 0.003 min
Response: 170159
Conc: 0.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

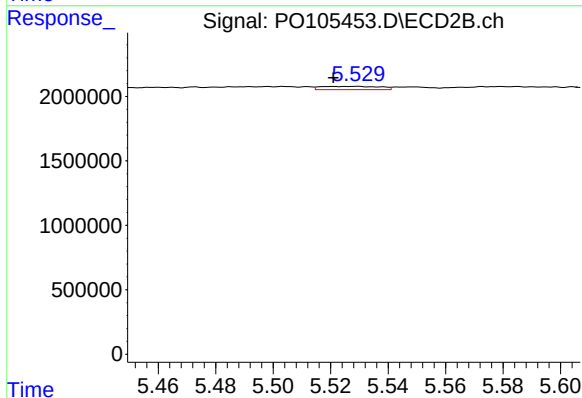


#27 AR-1254-2

R.T.: 5.529 min
Delta R.T.: 0.008 min
Response: 366027
Conc: 2.50 ng/ml

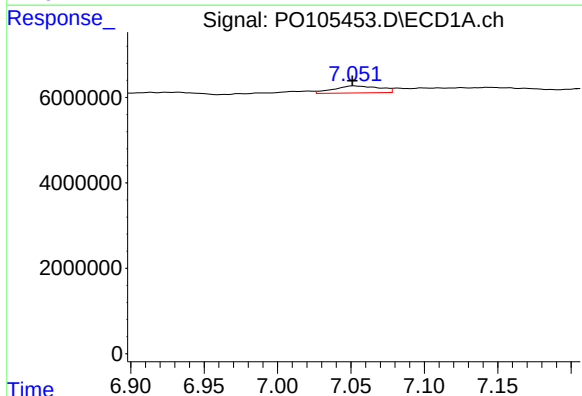


#28 AR-1254-3

R.T.: 7.052 min
Delta R.T.: 0.000 min
Response: 3565838
Conc: 7.52 ng/ml

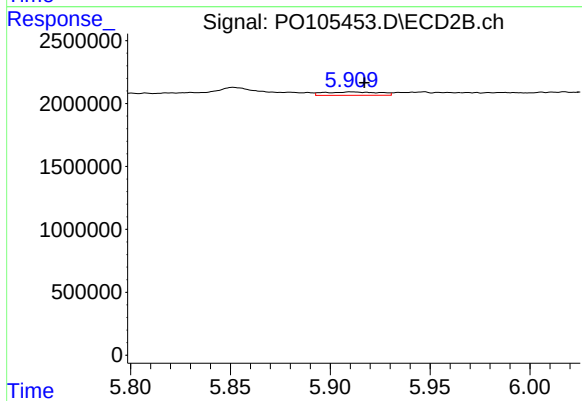

#28 AR-1254-3


R.T.: 5.910 min
Delta R.T.: -0.007 min
Response: 511162
Conc: 2.27 ng/ml

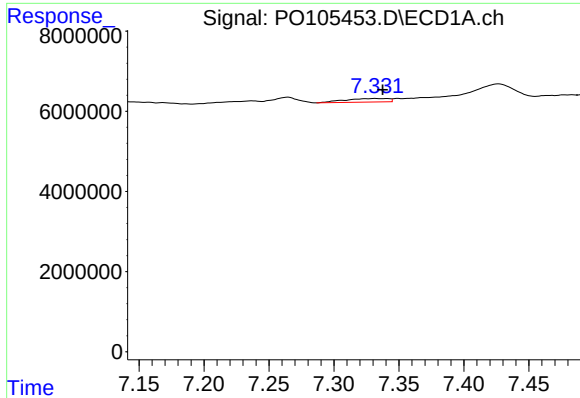

#29 AR-1254-4


R.T.: 7.332 min
Delta R.T.: -0.005 min
Response: 2033662
Conc: 5.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

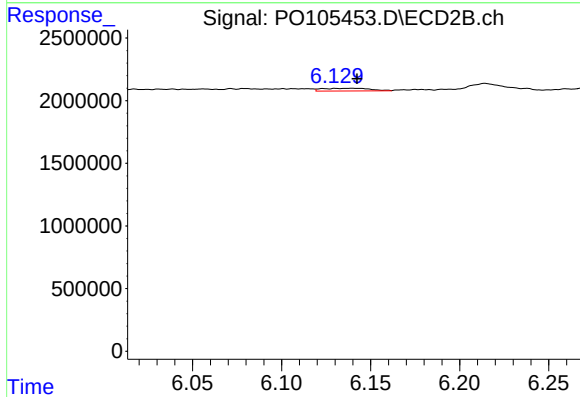


#29 AR-1254-4

R.T.: 6.139 min
Delta R.T.: -0.003 min
Response: 397665
Conc: 2.82 ng/ml

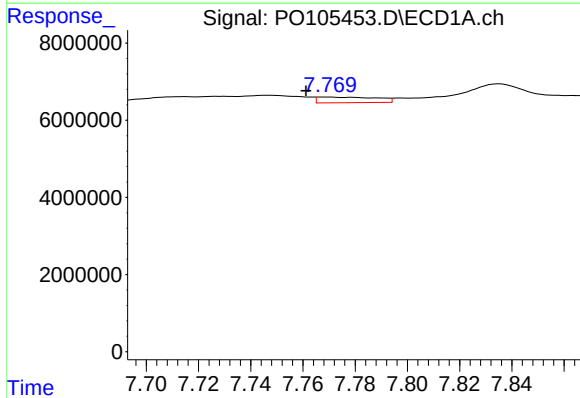


#30 AR-1254-5

R.T.: 7.769 min
Delta R.T.: 0.008 min
Response: 2301394
Conc: 5.80 ng/ml

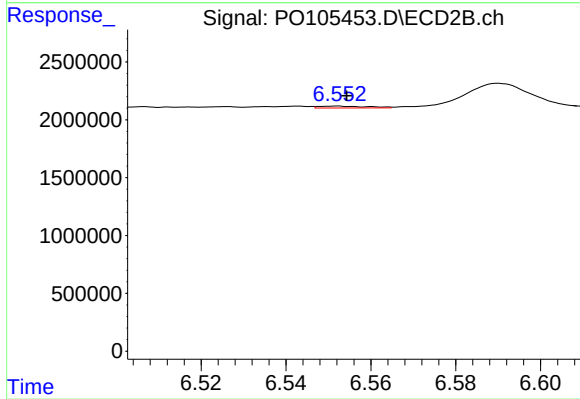

#30 AR-1254-5


R.T.: 6.552 min
Delta R.T.: -0.002 min
Response: 127883
Conc: 0.64 ng/ml

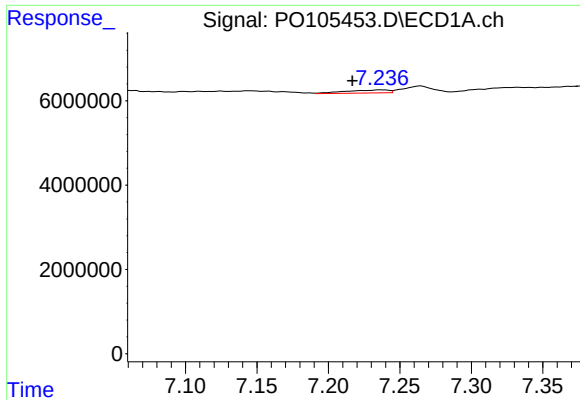

#31 AR-1260-1


R.T.: 7.237 min
Delta R.T.: 0.020 min
Response: 1503673
Conc: 4.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

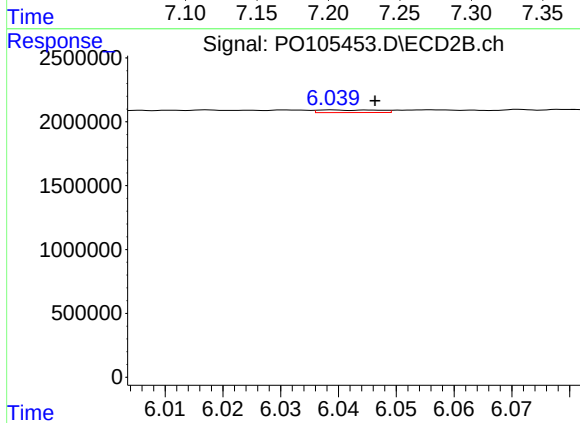


#31 AR-1260-1

R.T.: 6.039 min
Delta R.T.: -0.008 min
Response: 147150
Conc: 0.94 ng/ml

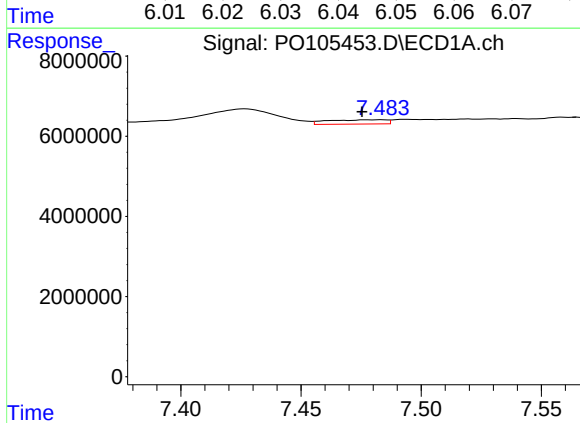


#32 AR-1260-2

R.T.: 7.483 min
Delta R.T.: 0.008 min
Response: 1809022
Conc: 4.34 ng/ml

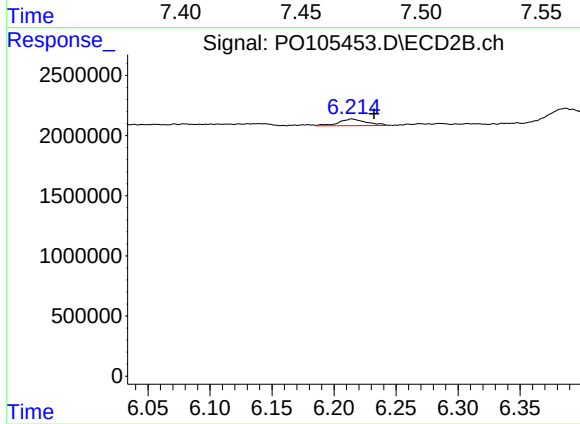

#32 AR-1260-2


R.T.: 6.214 min
Delta R.T.: -0.018 min
Response: 871307
Conc: 4.61 ng/ml

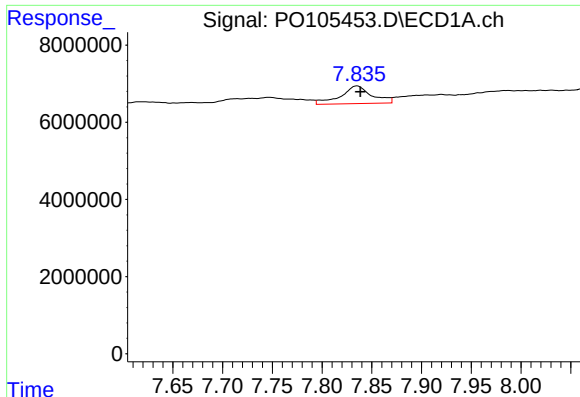

#33 AR-1260-3


R.T.: 7.835 min
Delta R.T.: -0.003 min
Response: 10029649
Conc: 38.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

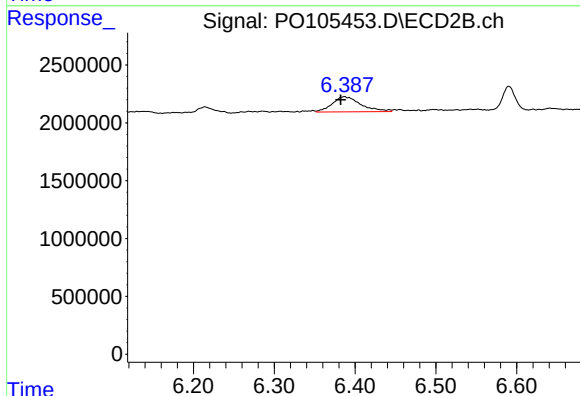


#33 AR-1260-3

R.T.: 6.387 min
Delta R.T.: 0.005 min
Response: 3198159
Conc: 17.31 ng/ml

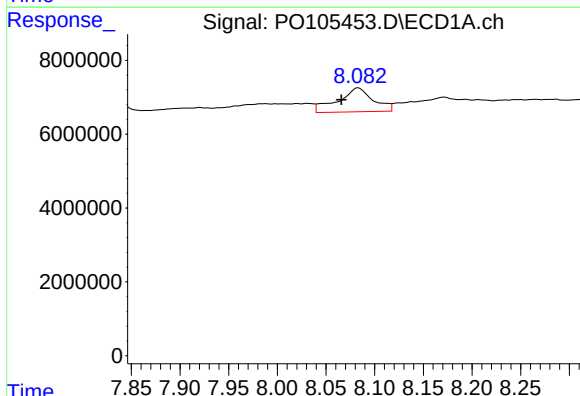


#34 AR-1260-4

R.T.: 8.083 min
Delta R.T.: 0.017 min
Response: 16217637
Conc: 49.15 ng/ml

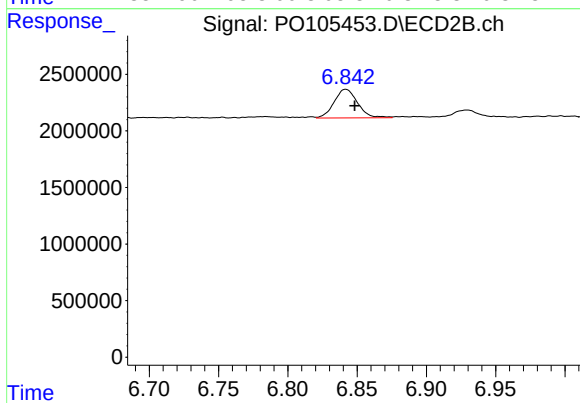

#34 AR-1260-4


R.T.: 6.842 min
Delta R.T.: -0.006 min
Response: 2985424
Conc: 24.42 ng/ml

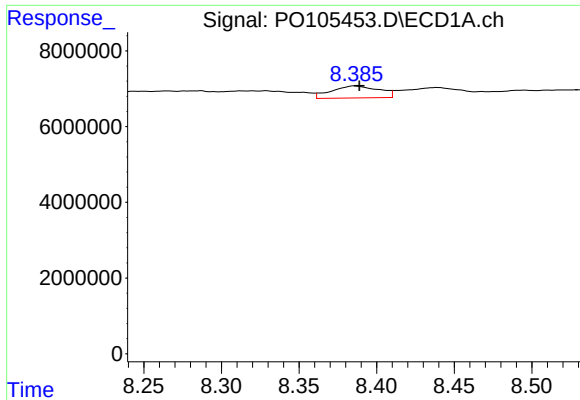

#35 AR-1260-5


R.T.: 8.386 min
Delta R.T.: -0.003 min
Response: 6747260
Conc: 11.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

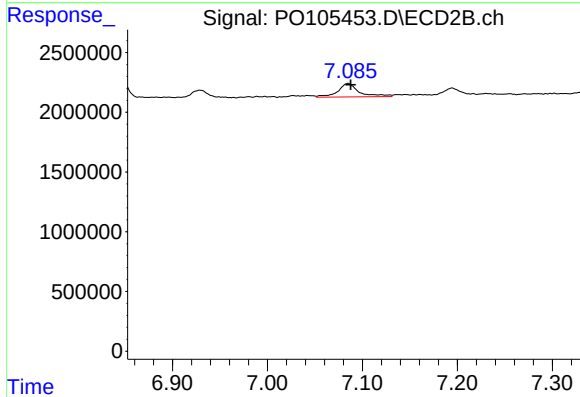


#35 AR-1260-5

R.T.: 7.085 min
Delta R.T.: -0.003 min
Response: 1759534
Conc: 6.32 ng/ml

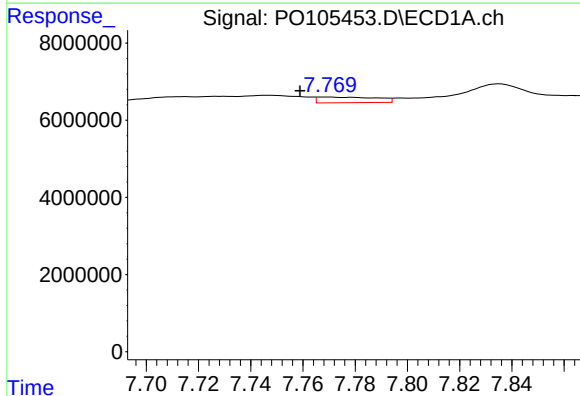


#36 AR-1262-1

R.T.: 7.769 min
Delta R.T.: 0.010 min
Response: 2301394
Conc: 7.25 ng/ml

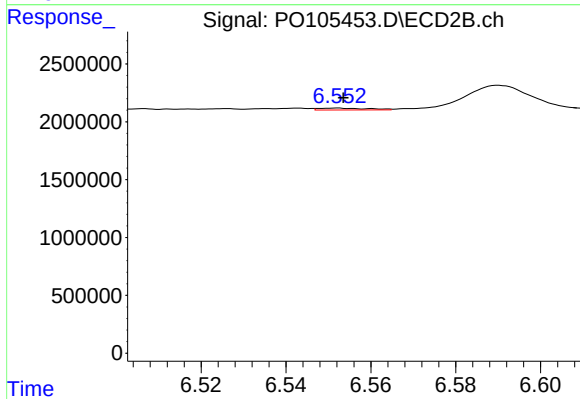

#36 AR-1262-1


R.T.: 6.552 min
Delta R.T.: -0.002 min
Response: 127883
Conc: 1.20 ng/ml

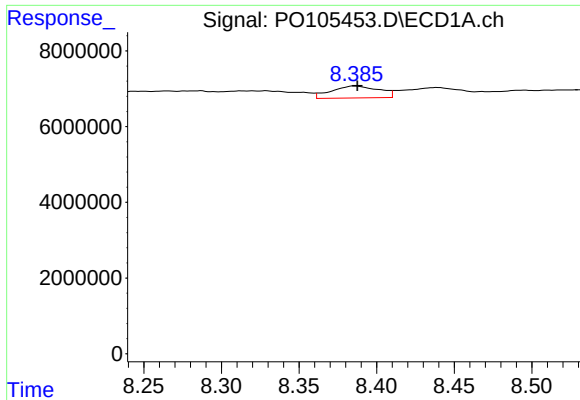

#37 AR-1262-2


R.T.: 8.386 min
Delta R.T.: -0.002 min
Response: 6747260
Conc: 8.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

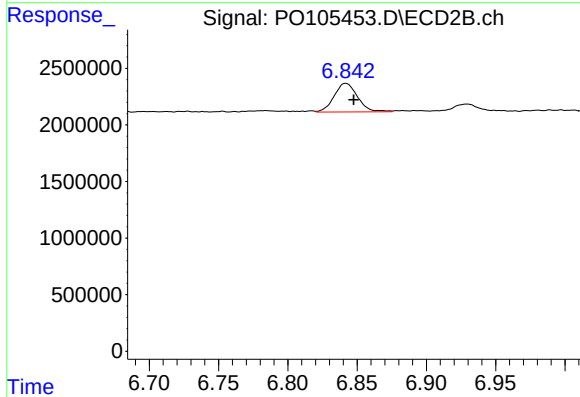


#37 AR-1262-2

R.T.: 6.842 min
Delta R.T.: -0.006 min
Response: 2985424
Conc: 17.57 ng/ml

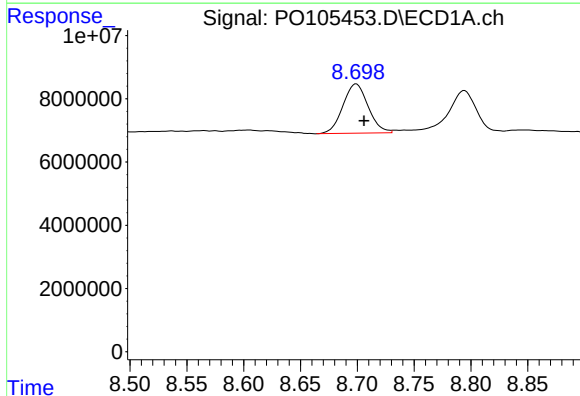


#38 AR-1262-3

R.T.: 8.699 min
Delta R.T.: -0.007 min
Response: 24067575
Conc: 48.91 ng/ml

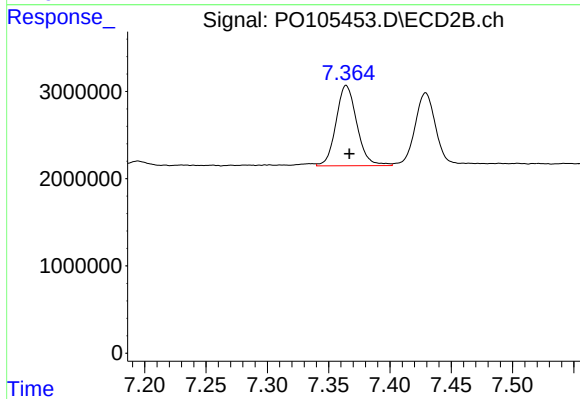

#38 AR-1262-3


R.T.: 7.364 min
Delta R.T.: -0.002 min
Response: 10909362
Conc: 86.41 ng/ml

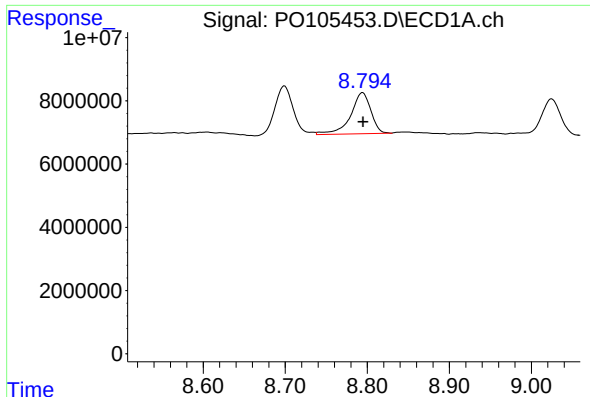

#39 AR-1262-4


R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 22652853
Conc: 61.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

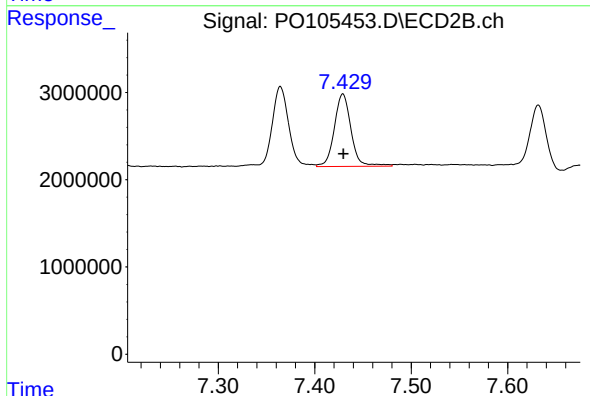


#39 AR-1262-4

R.T.: 7.429 min
Delta R.T.: 0.000 min
Response: 9997665
Conc: 43.19 ng/ml

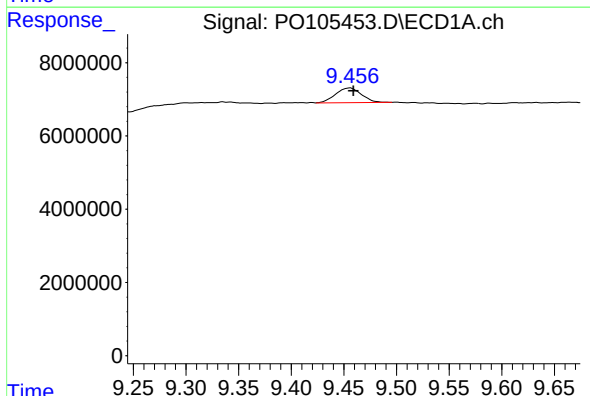


#40 AR-1262-5

R.T.: 9.456 min
Delta R.T.: -0.003 min
Response: 6884470
Conc: 25.71 ng/ml

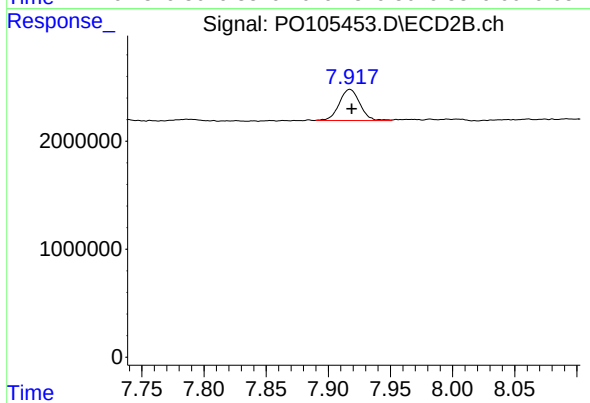

#40 AR-1262-5


R.T.: 7.917 min
Delta R.T.: -0.001 min
Response: 3342566
Conc: 33.26 ng/ml

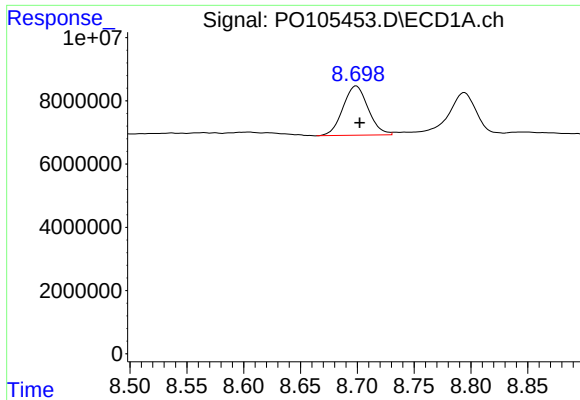

#41 AR-1268-1


R.T.: 8.699 min
Delta R.T.: -0.003 min
Response: 24067575
Conc: 29.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

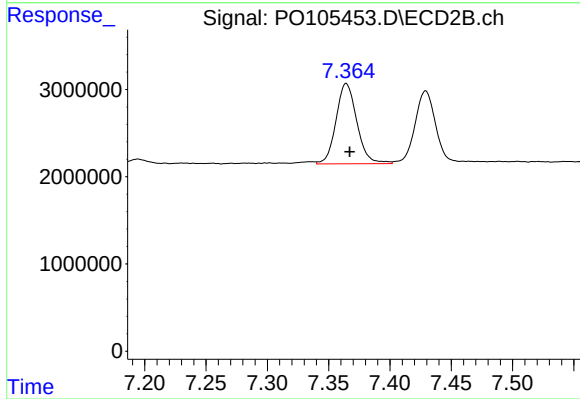


#41 AR-1268-1

R.T.: 7.364 min
Delta R.T.: -0.003 min
Response: 10909362
Conc: 31.25 ng/ml

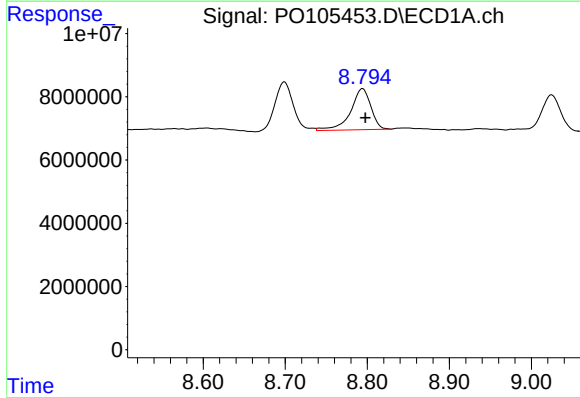


#42 AR-1268-2

R.T.: 8.794 min
Delta R.T.: -0.003 min
Response: 22652853
Conc: 31.16 ng/ml

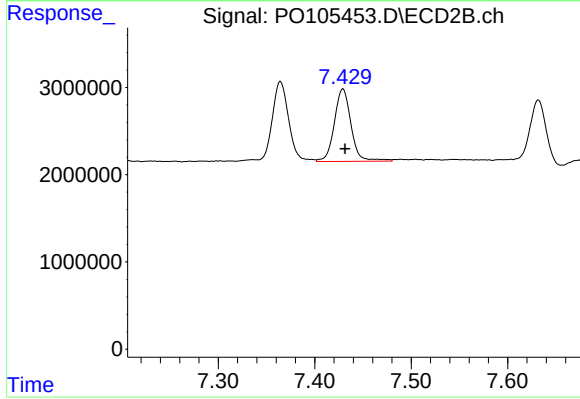

#42 AR-1268-2


R.T.: 7.429 min
Delta R.T.: -0.002 min
Response: 9997665
Conc: 32.05 ng/ml

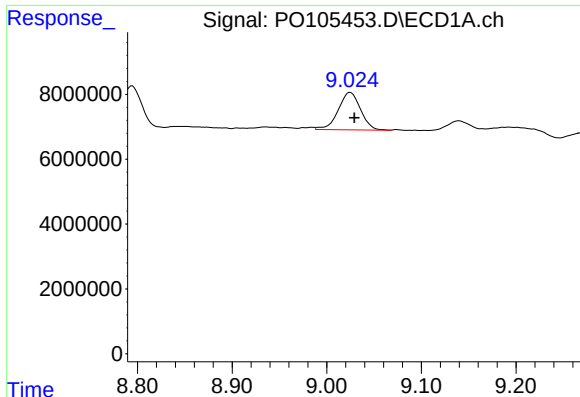

#43 AR-1268-3


R.T.: 9.025 min
Delta R.T.: -0.005 min
Response: 18891168
Conc: 29.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

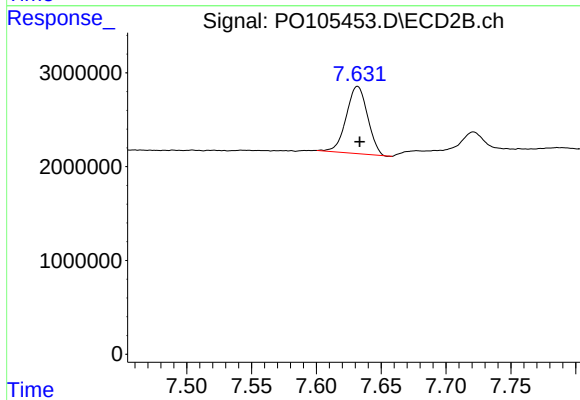


#43 AR-1268-3

R.T.: 7.632 min
Delta R.T.: -0.002 min
Response: 8205792
Conc: 32.47 ng/ml

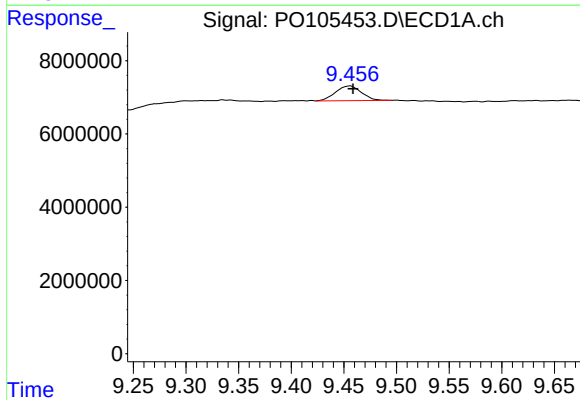


#44 AR-1268-4

R.T.: 9.456 min
Delta R.T.: -0.003 min
Response: 6884470
Conc: 24.72 ng/ml

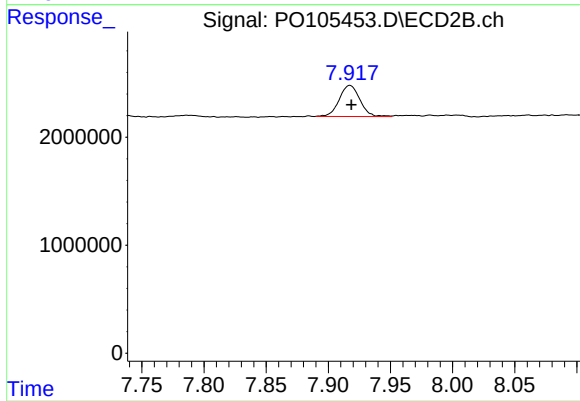

#44 AR-1268-4


R.T.: 7.917 min
Delta R.T.: -0.001 min
Response: 3342566
Conc: 31.08 ng/ml

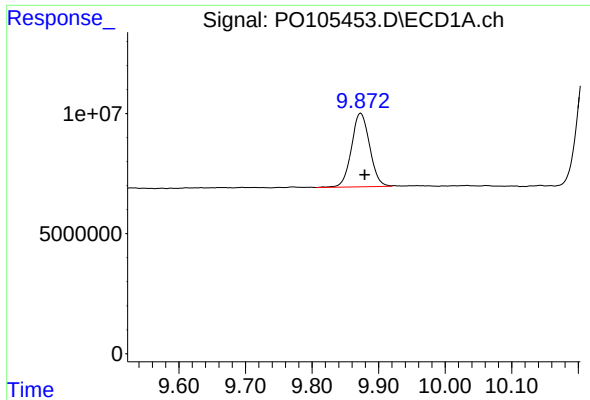

#45 AR-1268-5

R.T.: 9.873 min
Delta R.T.: -0.006 min
Response: 58074950
Conc: 27.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

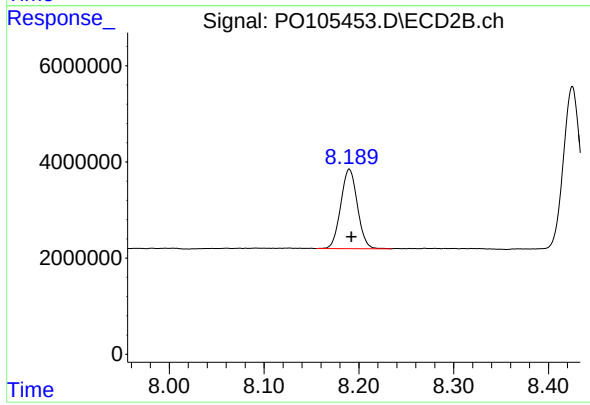

#45 AR-1268-5

R.T.: 8.190 min
Delta R.T.: -0.002 min
Response: 20210825
Conc: 30.21 ng/ml