

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081225\
 Data File : P0112855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 10:24
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 11:06:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.709f	3.695f	1440972	34673	0.177	0.007 #
2)	SA Decachlor...	8.690	8.633	756514	124519	0.103	0.070 #
Target Compounds							
3)	L1 AR-1016-1	4.757	4.728	863010	1853808	3.216	10.593 #
4)	L1 AR-1016-2	4.785	4.766	1039230	1075541	2.559	4.129 #
5)	L1 AR-1016-3	4.833	4.929	274859	2501827	1.050	18.400 #
6)	L1 AR-1016-4	4.951	4.972	7301813	13170205	34.468	118.560 #
7)	L1 AR-1016-5	5.195	5.168	18049320	3517596	82.240	24.547 #
8)	L2 AR-1221-1	3.887	3.877	2018955	3462630	20.887	51.477 #
9)	L2 AR-1221-2	3.976	3.965	2935244	4704568	40.846	92.741 #
10)	L2 AR-1221-3	4.044	4.031	562499	905372	2.366	5.711 #
11)	L3 AR-1232-1	4.044	4.031	562499	905372	3.008	7.154 #
12)	L3 AR-1232-2	4.523	4.766	7625757	1075541	70.855	8.201 #
13)	L3 AR-1232-3	4.785	4.929	1039230	2501827	5.025	37.231 #
14)	L3 AR-1232-4	4.951	5.051f	7301813	12444494	69.714	208.001 #
15)	L3 AR-1232-5	5.010	5.168	24099169	3517596	355.021	53.948 #
16)	L4 AR-1242-1	4.757	4.728	863010	1853808	3.486	11.704 #
17)	L4 AR-1242-2	4.785	4.766	1039230	1075541	2.810	4.603 #
18)	L4 AR-1242-3	4.833	4.929	274859	2501827	1.161	20.644 #
19)	L4 AR-1242-4	4.951	5.051f	7301813	12444494	37.584	101.390 #
20)	L4 AR-1242-5	5.600	5.542	9928981	1857767	46.415	11.541 #
21)	L5 AR-1248-1	4.757	4.728	863010	1853808	4.610	15.257 #
22)	L5 AR-1248-2	5.010	4.972	24099169	13170205	94.465	77.801
23)	L5 AR-1248-3	5.195	5.051f	18049320	12444494	52.515	70.052 #
24)	L5 AR-1248-4	5.569	5.168	11542515	3517596	22.718	16.883 #
25)	L5 AR-1248-5	5.600	5.559	9928981	4801278	28.402	22.356
26)	L6 AR-1254-1	5.569	5.542	11542515	1857767	21.026	5.653 #
27)	L6 AR-1254-2	5.727	5.698	47506034	23495232	97.765	81.161
28)	L6 AR-1254-3	6.126	6.095	13000508	17463248	17.467	40.853 #
29)	L6 AR-1254-4	6.359	6.323	287582	1588603	0.523	5.820 #
30)	L6 AR-1254-5	6.754	6.720	2965.5E6	1476.8E6	4189.633	4421.438
31)	L7 AR-1260-1	6.248	6.207	1240784	2592458	2.824	10.432 #
32)	L7 AR-1260-2	6.432	6.398	16382875	7723031	23.816	23.439
33)	L7 AR-1260-3	6.829	6.585	3293611	389525	5.601	1.516 #
34)	L7 AR-1260-4	7.016f	7.011	27346622	604175	60.635	3.158 #
35)	L7 AR-1260-5	7.316	7.202f	796083	6155488	0.642	14.933 #
36)	L8 AR-1262-1	6.829	6.720f	3293611	1476.8E6	3.545	3560.144 #
37)	L8 AR-1262-2	7.316	7.202f	796083	6155488	0.535	11.940 #
38)	L8 AR-1262-3	7.611	7.543	12079313	126135	20.465	0.676 #
39)	L8 AR-1262-4	7.658	7.557f	4339200	568206	4.365	1.972 #
40)	L8 AR-1262-5	8.145	0.000	1270847	0	2.928	N.D. #
41)	L9 AR-1268-1	7.611	7.543	12079313	126135	6.898	0.244 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081225\
 Data File : P0112855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 10:24
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 11:06:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.658	7.557f	4339200	568206	2.946	1.337 #
43) L9	AR-1268-3	7.838	7.834	1510572	-280578	1.206	N.D. #
44) L9	AR-1268-4	8.145	0.000	1270847	0	2.637	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081225\
Data File : PO112855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 10:24
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 11:06:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

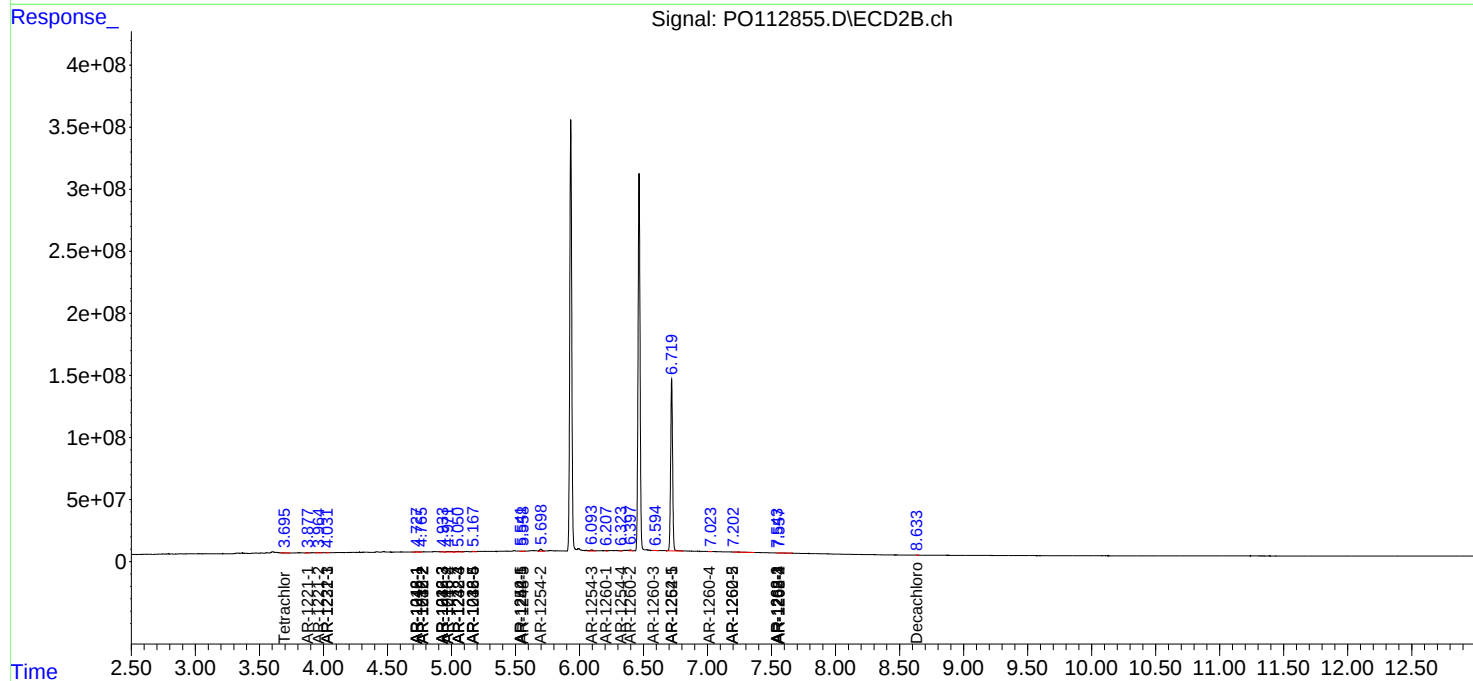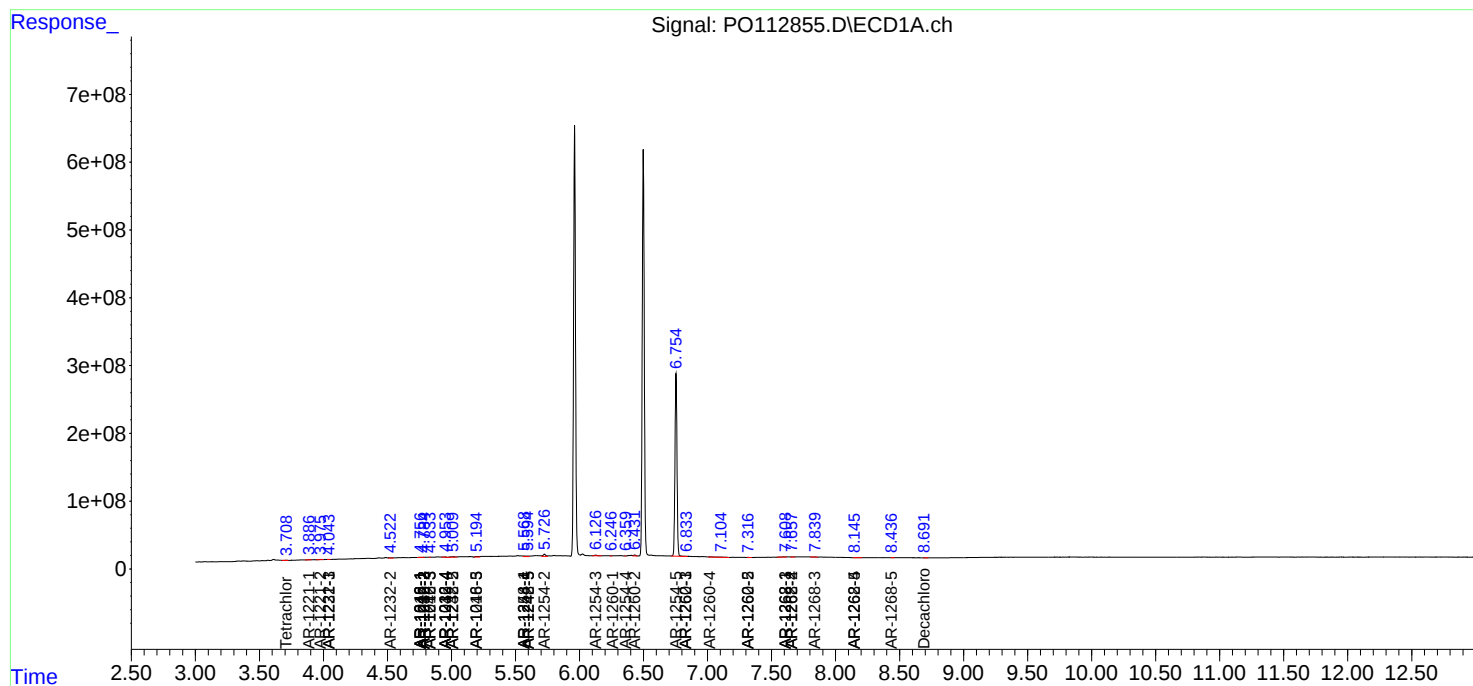


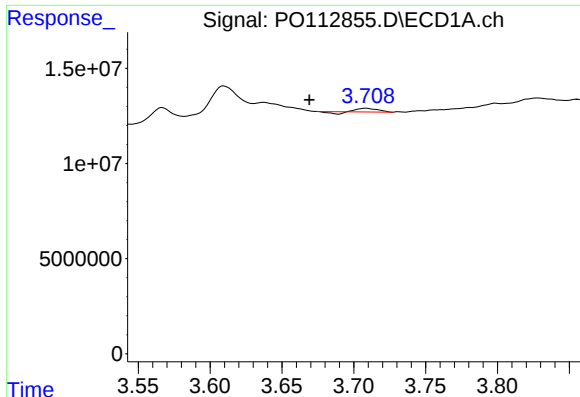

#1 Tetrachloro-m-xylene


R.T.: 3.709 min
Delta R.T.: 0.040 min
Response: 1440972
Conc: 0.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

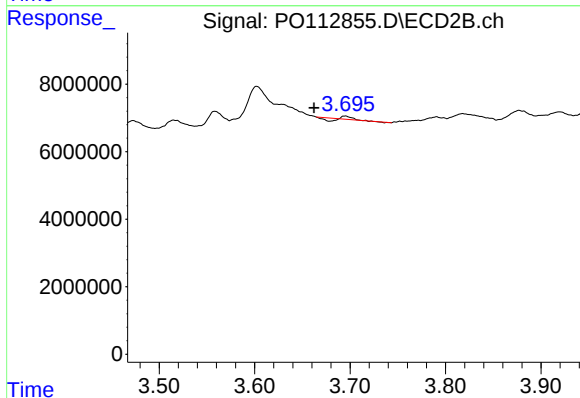


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: 0.033 min
Response: 34673
Conc: 0.01 ng/ml

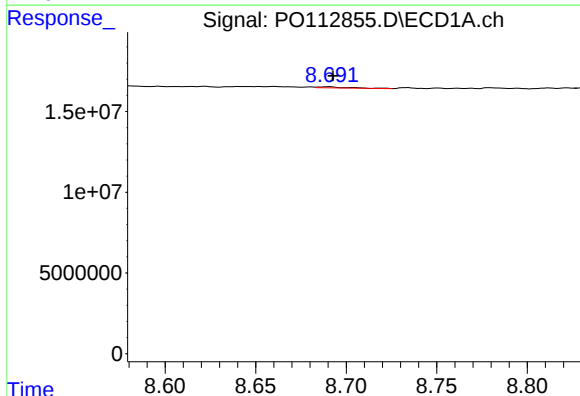


#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.003 min
Response: 756514
Conc: 0.10 ng/ml

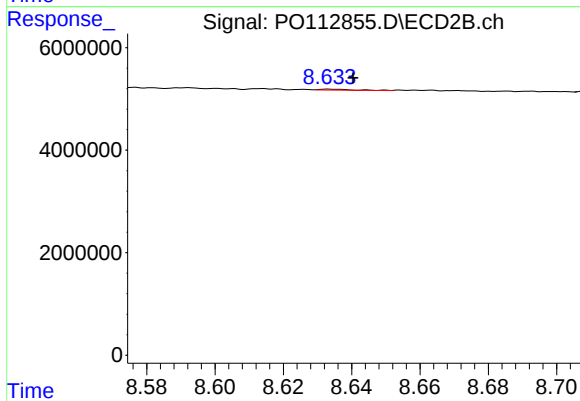

#2 Decachlorobiphenyl


R.T.: 8.633 min
Delta R.T.: -0.007 min
Response: 124519
Conc: 0.07 ng/ml

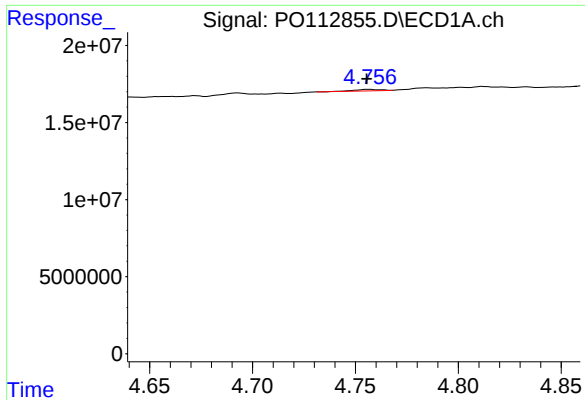

#3 AR-1016-1


R.T.: 4.757 min
Delta R.T.: 0.001 min
Response: 863010
Conc: 3.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

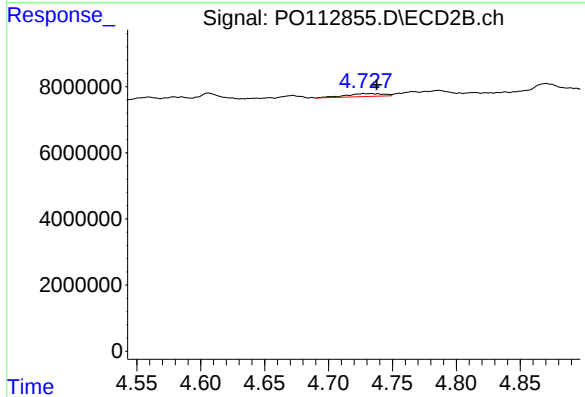


#3 AR-1016-1

R.T.: 4.728 min
Delta R.T.: -0.010 min
Response: 1853808
Conc: 10.59 ng/ml

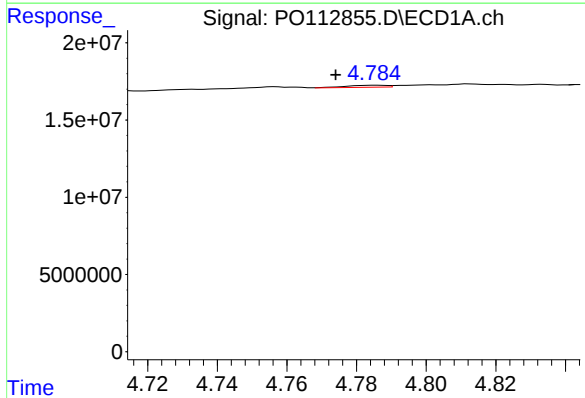


#4 AR-1016-2

R.T.: 4.785 min
Delta R.T.: 0.011 min
Response: 1039230
Conc: 2.56 ng/ml

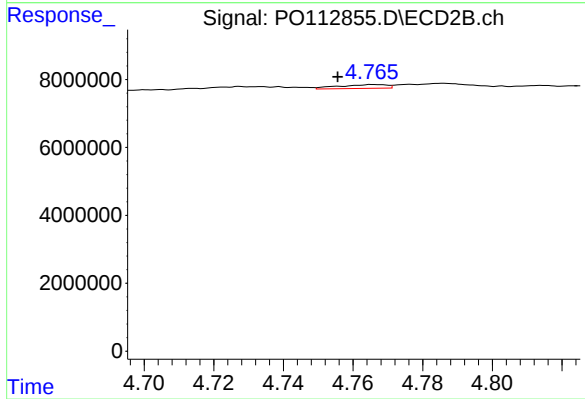

#4 AR-1016-2


R.T.: 4.766 min
Delta R.T.: 0.011 min
Response: 1075541
Conc: 4.13 ng/ml

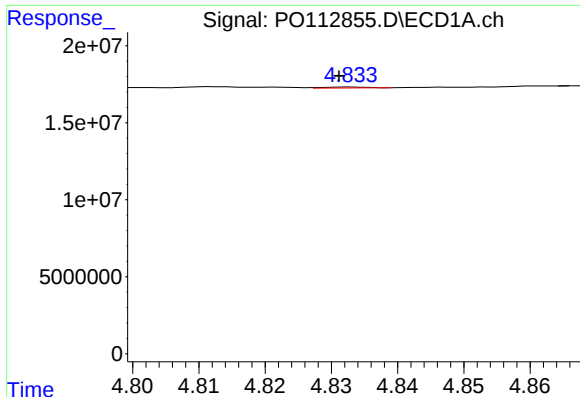

#5 AR-1016-3


R.T.: 4.833 min
Delta R.T.: 0.002 min
Response: 274859
Conc: 1.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

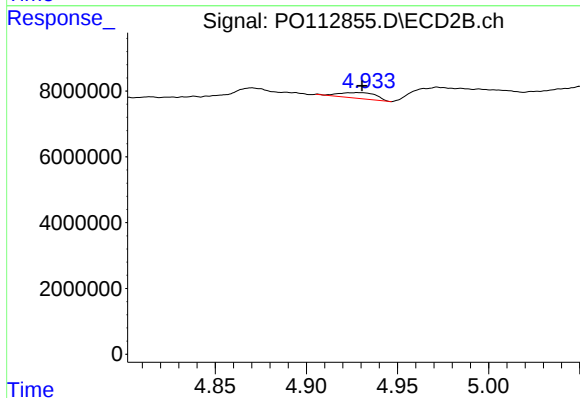


#5 AR-1016-3

R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 2501827
Conc: 18.40 ng/ml

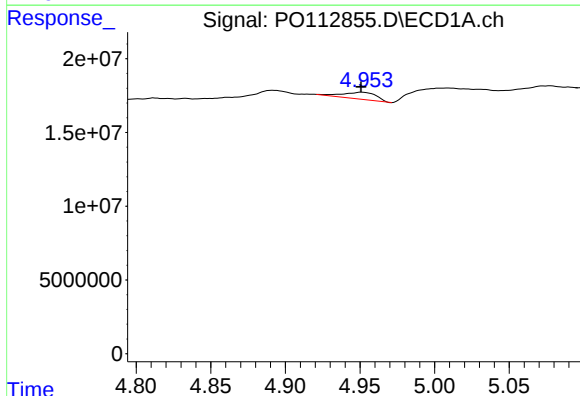


#6 AR-1016-4

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 7301813
Conc: 34.47 ng/ml

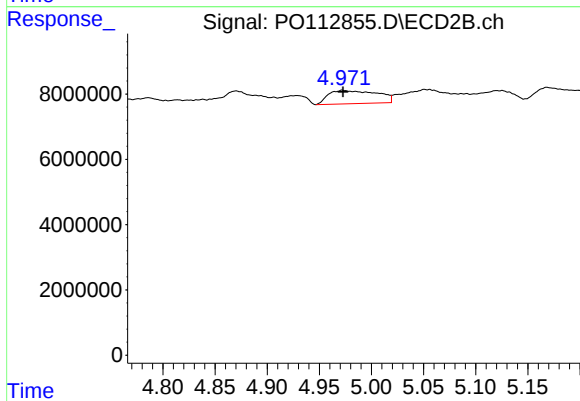

#6 AR-1016-4


R.T.: 4.972 min
Delta R.T.: 0.000 min
Response: 13170205
Conc: 118.56 ng/ml

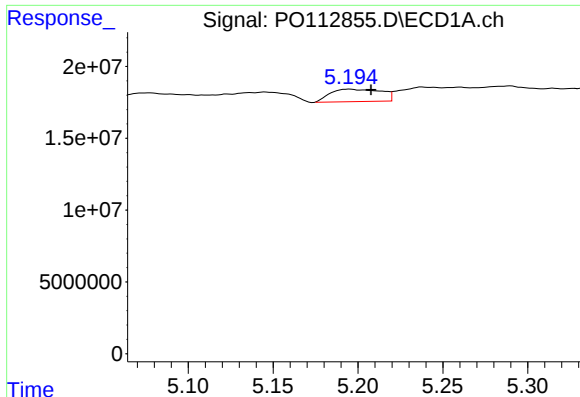

#7 AR-1016-5


R.T.: 5.195 min
Delta R.T.: -0.013 min
Response: 18049320
Conc: 82.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

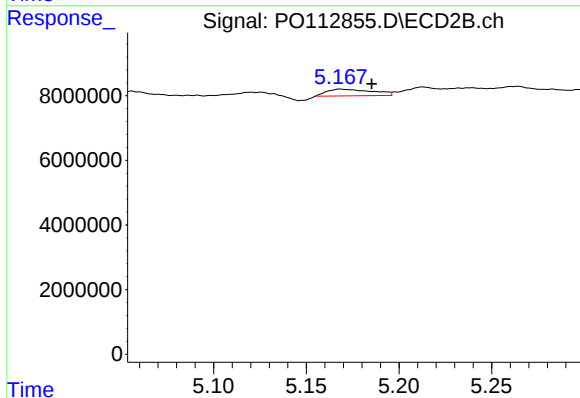


#7 AR-1016-5

R.T.: 5.168 min
Delta R.T.: -0.017 min
Response: 3517596
Conc: 24.55 ng/ml

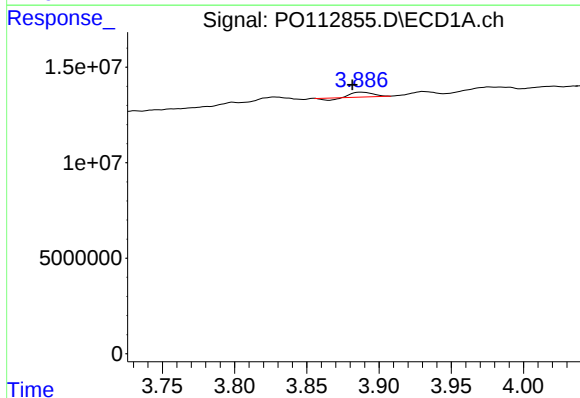


#8 AR-1221-1

R.T.: 3.887 min
Delta R.T.: 0.006 min
Response: 2018955
Conc: 20.89 ng/ml

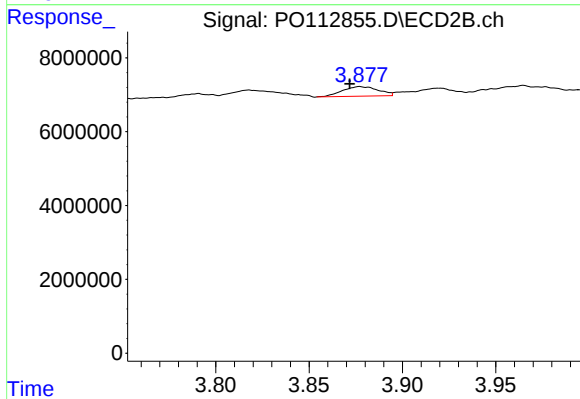

#8 AR-1221-1


R.T.: 3.877 min
Delta R.T.: 0.005 min
Response: 3462630
Conc: 51.48 ng/ml

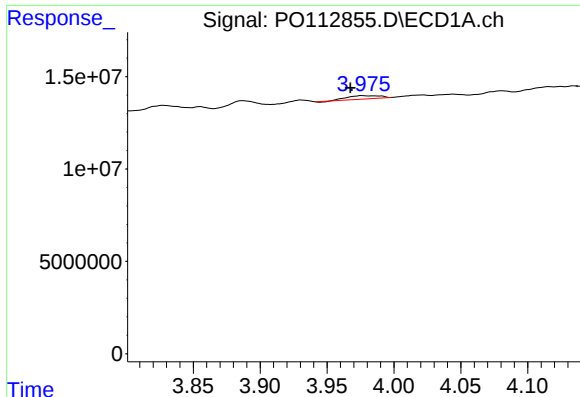

#9 AR-1221-2


R.T.: 3.976 min
Delta R.T.: 0.009 min
Response: 2935244
Conc: 40.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

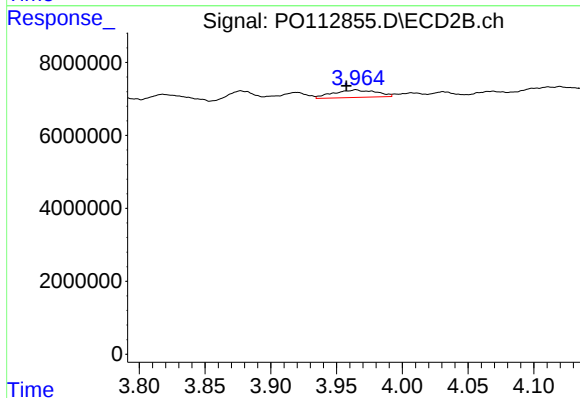


#9 AR-1221-2

R.T.: 3.965 min
Delta R.T.: 0.007 min
Response: 4704568
Conc: 92.74 ng/ml

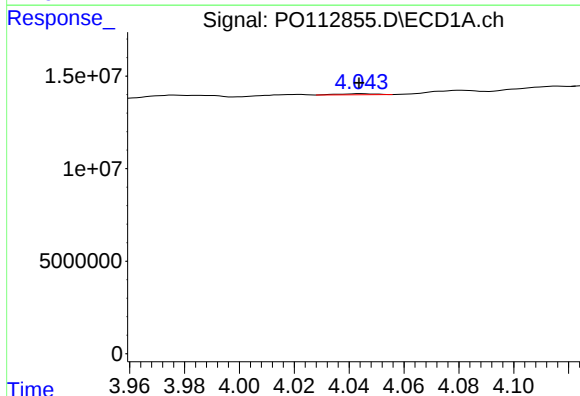


#10 AR-1221-3

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 562499
Conc: 2.37 ng/ml

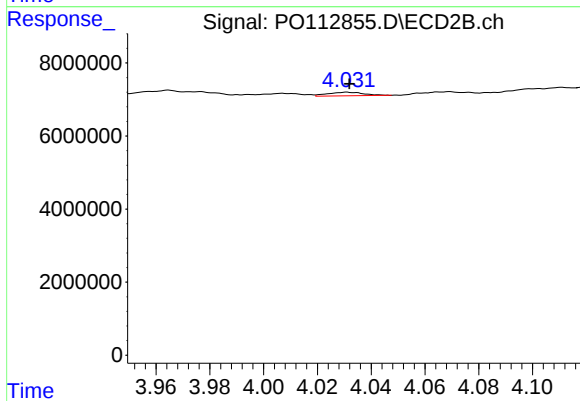

#10 AR-1221-3


R.T.: 4.031 min
Delta R.T.: 0.000 min
Response: 905372
Conc: 5.71 ng/ml

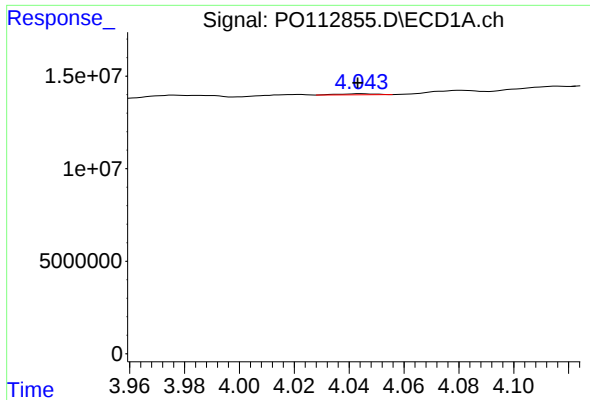

#11 AR-1232-1


R.T.: 4.044 min
Delta R.T.: 0.001 min
Response: 562499
Conc: 3.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

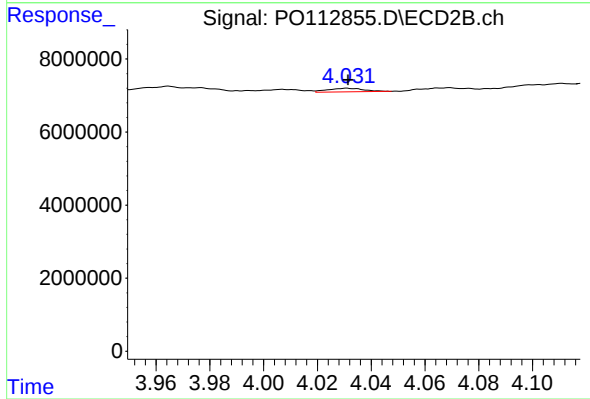


#11 AR-1232-1

R.T.: 4.031 min
Delta R.T.: 0.000 min
Response: 905372
Conc: 7.15 ng/ml

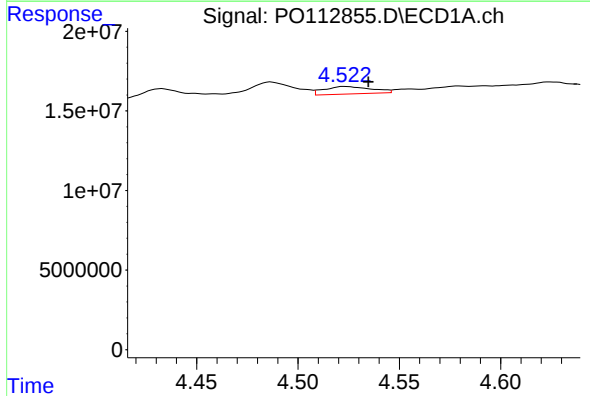


#12 AR-1232-2

R.T.: 4.523 min
Delta R.T.: -0.011 min
Response: 7625757
Conc: 70.86 ng/ml

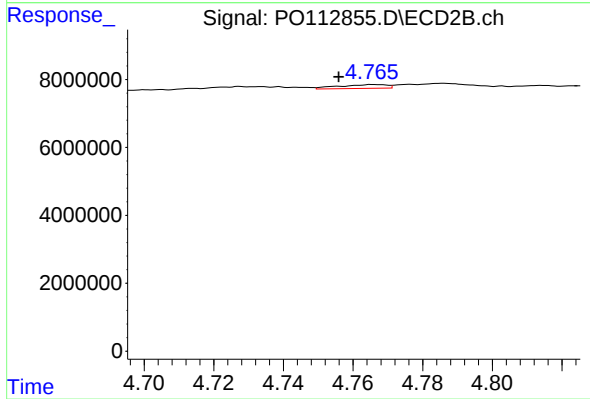

#12 AR-1232-2


R.T.: 4.766 min
Delta R.T.: 0.010 min
Response: 1075541
Conc: 8.20 ng/ml

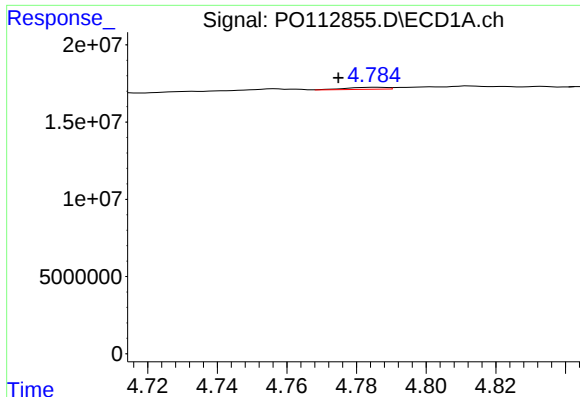

#13 AR-1232-3


R.T.: 4.785 min
Delta R.T.: 0.010 min
Response: 1039230
Conc: 5.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

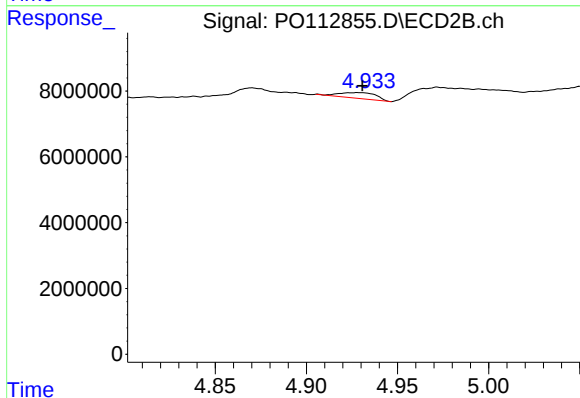


#13 AR-1232-3

R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 2501827
Conc: 37.23 ng/ml

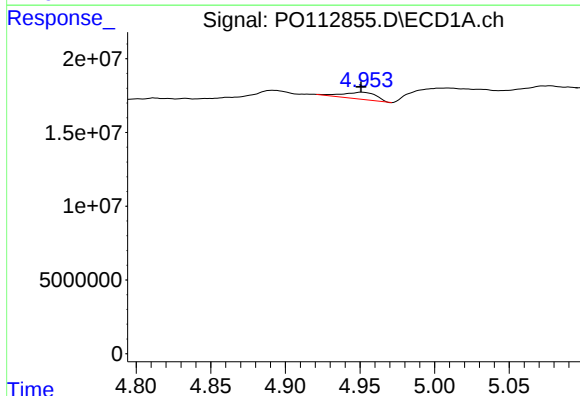


#14 AR-1232-4

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 7301813
Conc: 69.71 ng/ml

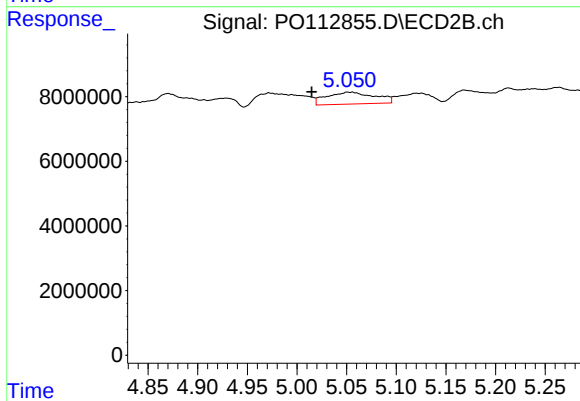

#14 AR-1232-4


R.T.: 5.051 min
Delta R.T.: 0.036 min
Response: 12444494
Conc: 208.00 ng/ml

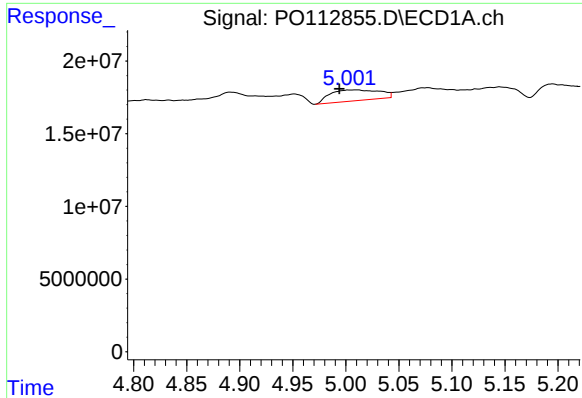

#15 AR-1232-5


R.T.: 5.010 min
Delta R.T.: 0.016 min
Response: 24099169
Conc: 355.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

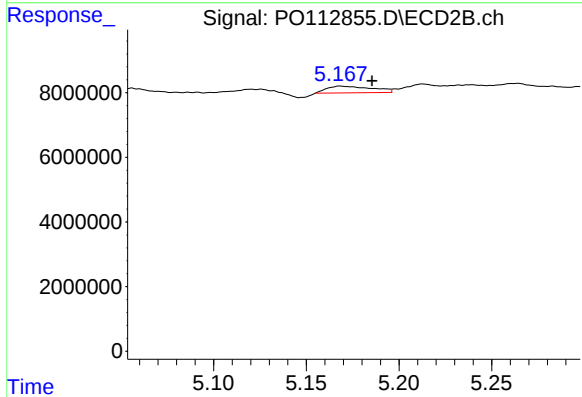


#15 AR-1232-5

R.T.: 5.168 min
Delta R.T.: -0.017 min
Response: 3517596
Conc: 53.95 ng/ml

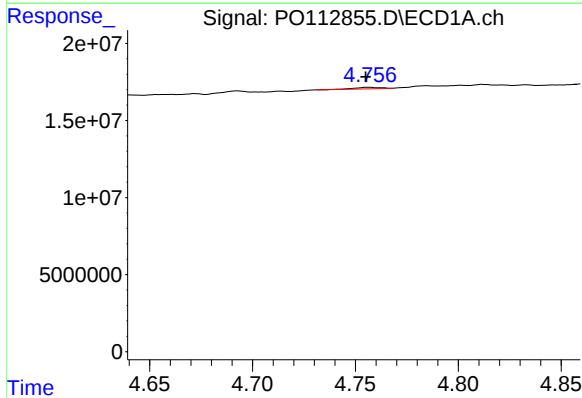


#16 AR-1242-1

R.T.: 4.757 min
Delta R.T.: 0.002 min
Response: 863010
Conc: 3.49 ng/ml

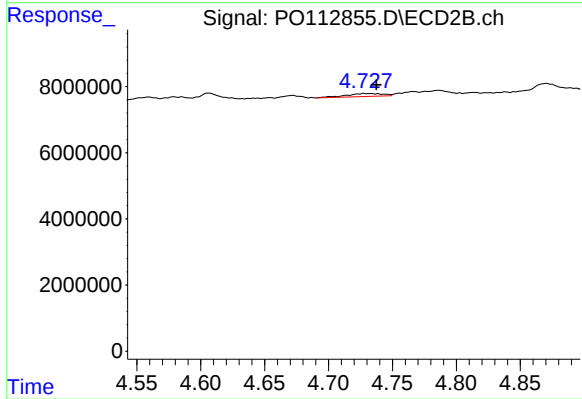

#16 AR-1242-1


R.T.: 4.728 min
Delta R.T.: -0.009 min
Response: 1853808
Conc: 11.70 ng/ml

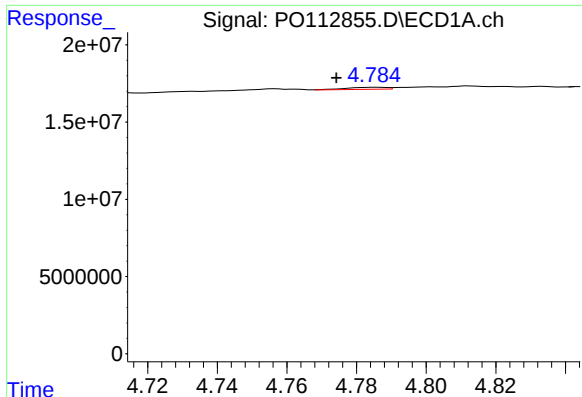

#17 AR-1242-2


R.T.: 4.785 min
Delta R.T.: 0.011 min
Response: 1039230
Conc: 2.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

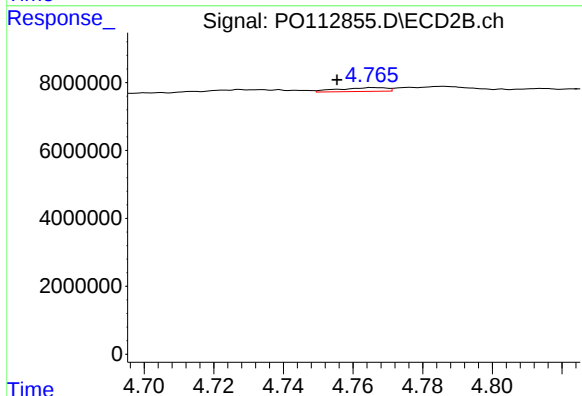


#17 AR-1242-2

R.T.: 4.766 min
Delta R.T.: 0.011 min
Response: 1075541
Conc: 4.60 ng/ml

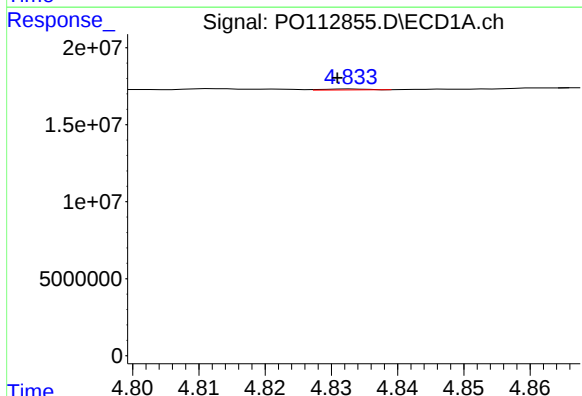


#18 AR-1242-3

R.T.: 4.833 min
Delta R.T.: 0.002 min
Response: 274859
Conc: 1.16 ng/ml

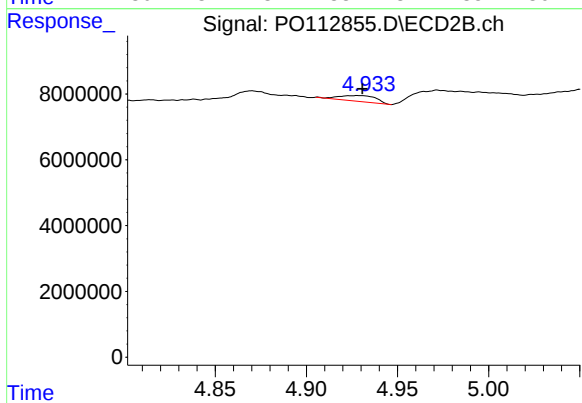

#18 AR-1242-3


R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 2501827
Conc: 20.64 ng/ml

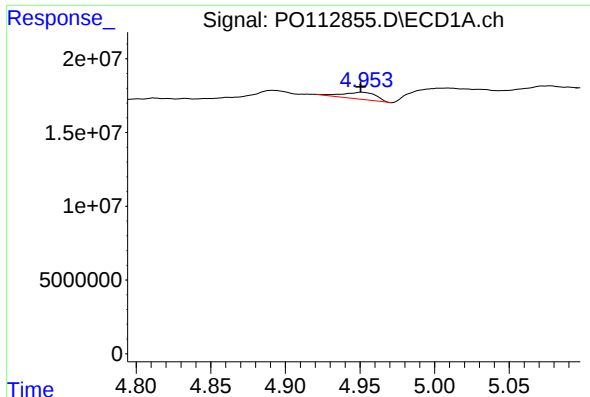

#19 AR-1242-4


R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 7301813
Conc: 37.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

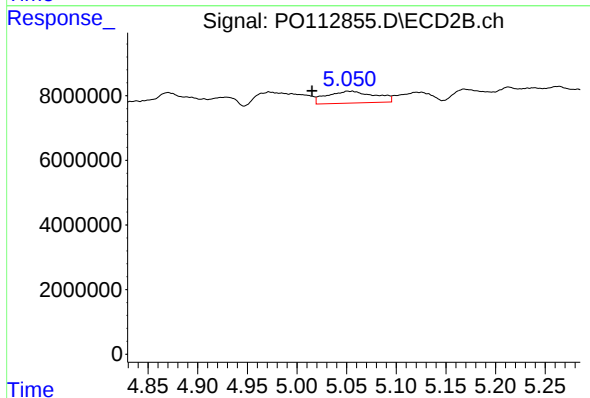


#19 AR-1242-4

R.T.: 5.051 min
Delta R.T.: 0.036 min
Response: 12444494
Conc: 101.39 ng/ml

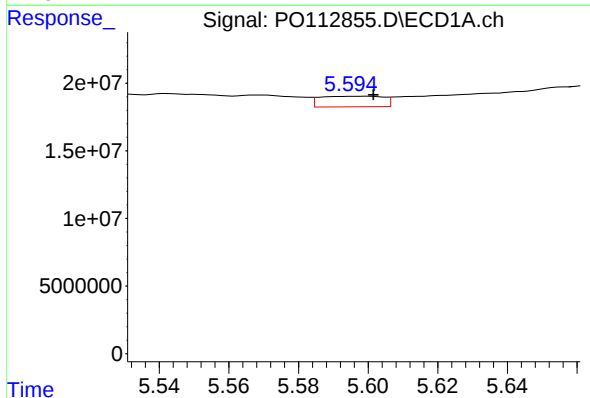


#20 AR-1242-5

R.T.: 5.600 min
Delta R.T.: -0.002 min
Response: 9928981
Conc: 46.42 ng/ml

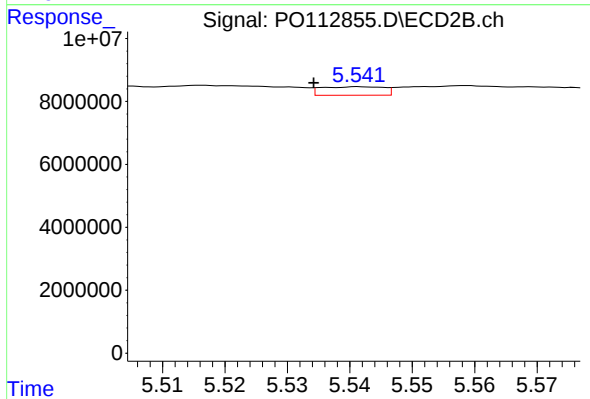

#20 AR-1242-5


R.T.: 5.542 min
Delta R.T.: 0.008 min
Response: 1857767
Conc: 11.54 ng/ml

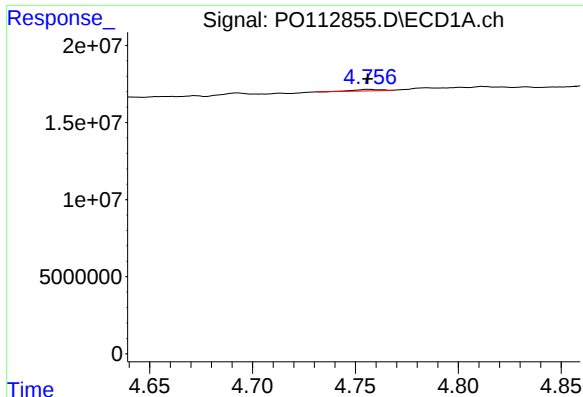

#21 AR-1248-1


R.T.: 4.757 min
Delta R.T.: 0.000 min
Response: 863010
Conc: 4.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

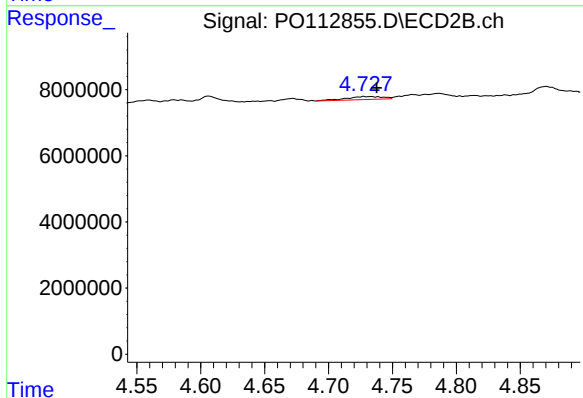


#21 AR-1248-1

R.T.: 4.728 min
Delta R.T.: -0.010 min
Response: 1853808
Conc: 15.26 ng/ml

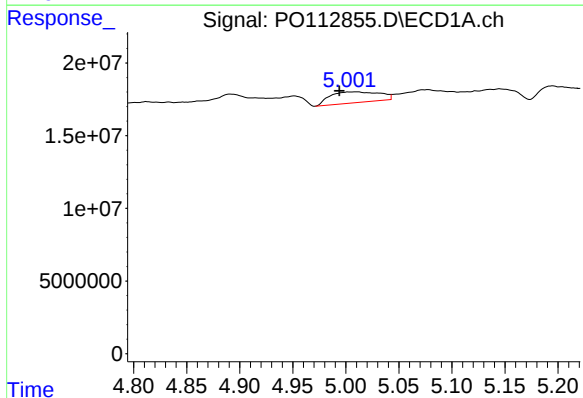


#22 AR-1248-2

R.T.: 5.010 min
Delta R.T.: 0.016 min
Response: 24099169
Conc: 94.46 ng/ml

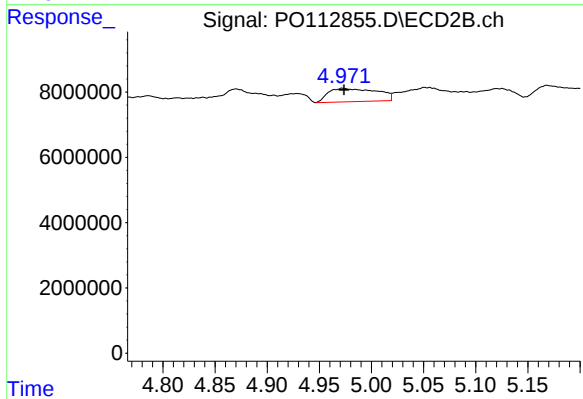

#22 AR-1248-2


R.T.: 4.972 min
Delta R.T.: -0.002 min
Response: 13170205
Conc: 77.80 ng/ml

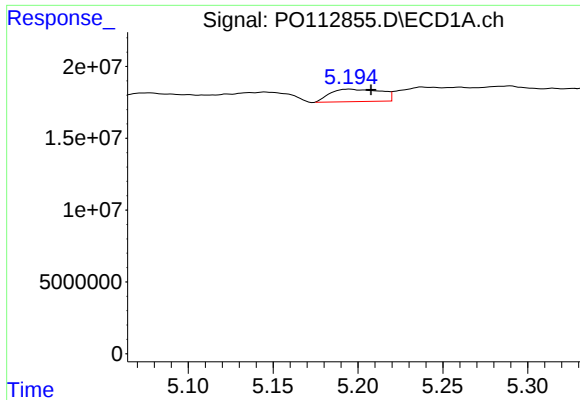

#23 AR-1248-3


R.T.: 5.195 min
Delta R.T.: -0.013 min
Response: 18049320
Conc: 52.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

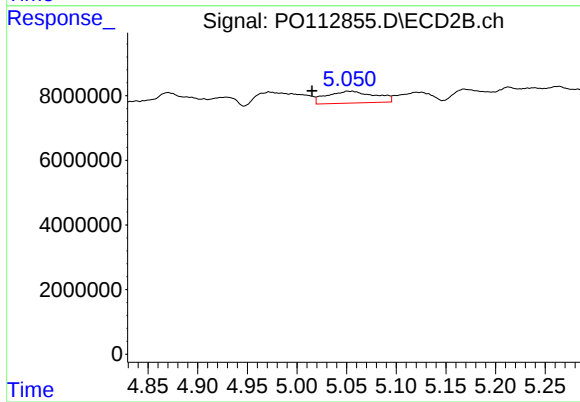


#23 AR-1248-3

R.T.: 5.051 min
Delta R.T.: 0.036 min
Response: 12444494
Conc: 70.05 ng/ml

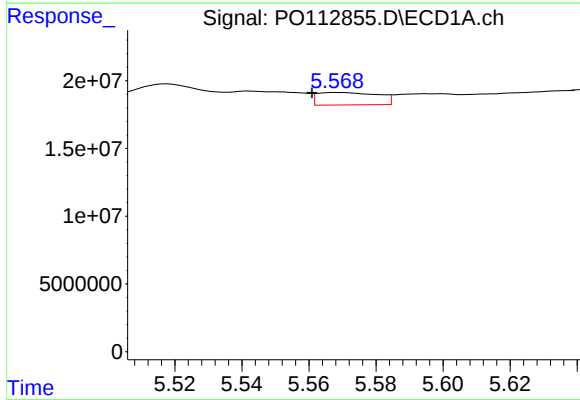


#24 AR-1248-4

R.T.: 5.569 min
Delta R.T.: 0.008 min
Response: 11542515
Conc: 22.72 ng/ml

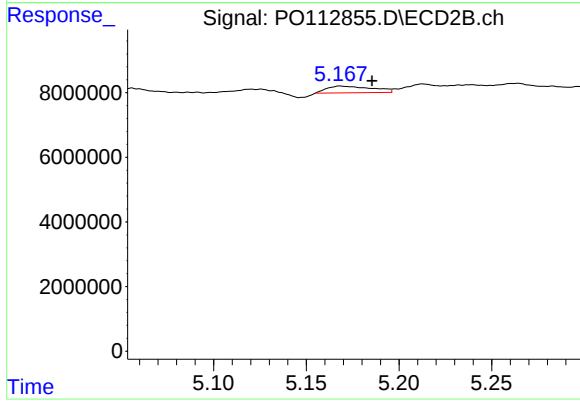

#24 AR-1248-4


R.T.: 5.168 min
Delta R.T.: -0.017 min
Response: 3517596
Conc: 16.88 ng/ml

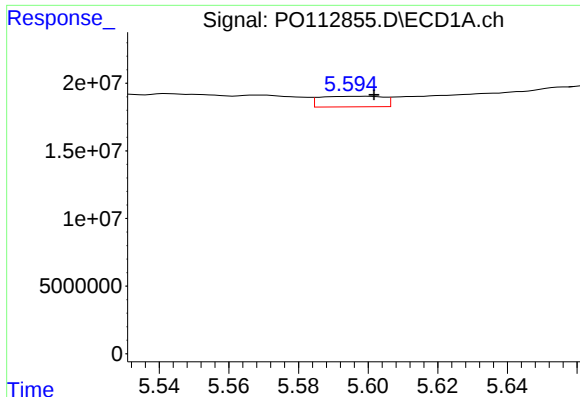

#25 AR-1248-5


R.T.: 5.600 min
Delta R.T.: -0.002 min
Response: 9928981
Conc: 28.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

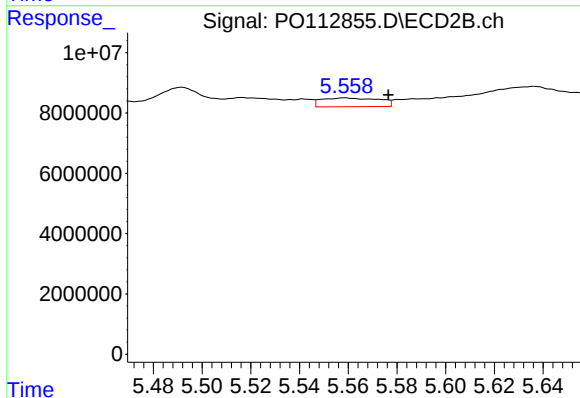


#25 AR-1248-5

R.T.: 5.559 min
Delta R.T.: -0.018 min
Response: 4801278
Conc: 22.36 ng/ml

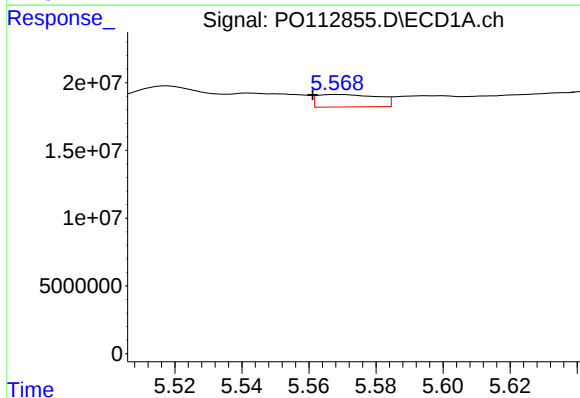


#26 AR-1254-1

R.T.: 5.569 min
Delta R.T.: 0.008 min
Response: 11542515
Conc: 21.03 ng/ml

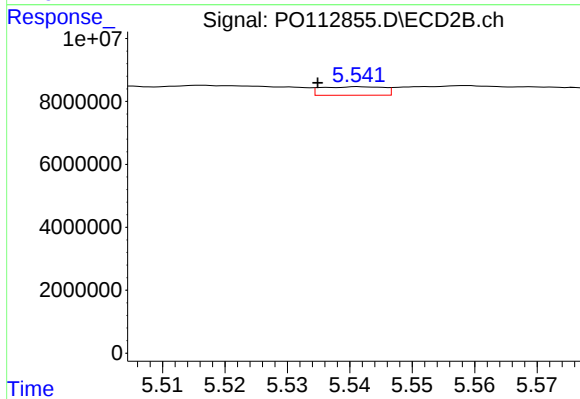

#26 AR-1254-1


R.T.: 5.542 min
Delta R.T.: 0.007 min
Response: 1857767
Conc: 5.65 ng/ml

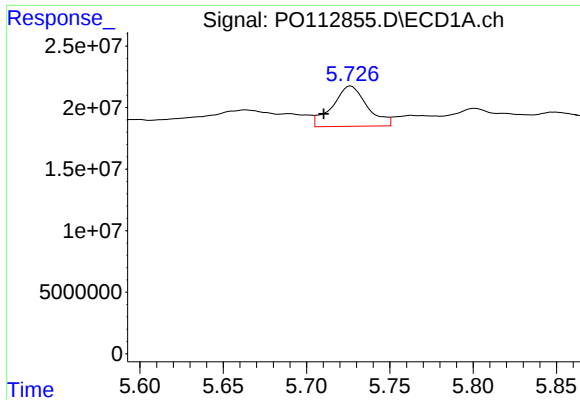

#27 AR-1254-2


R.T.: 5.727 min
Delta R.T.: 0.016 min
Response: 47506034
Conc: 97.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

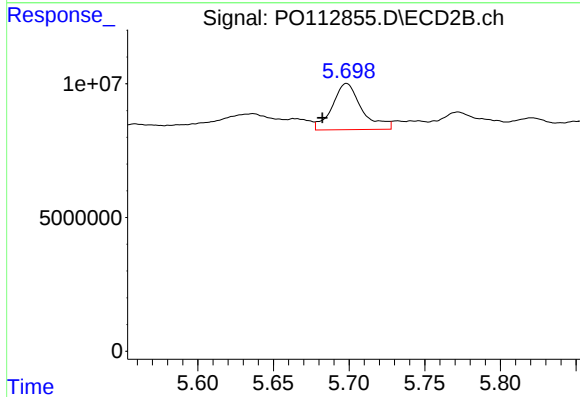


#27 AR-1254-2

R.T.: 5.698 min
Delta R.T.: 0.016 min
Response: 23495232
Conc: 81.16 ng/ml

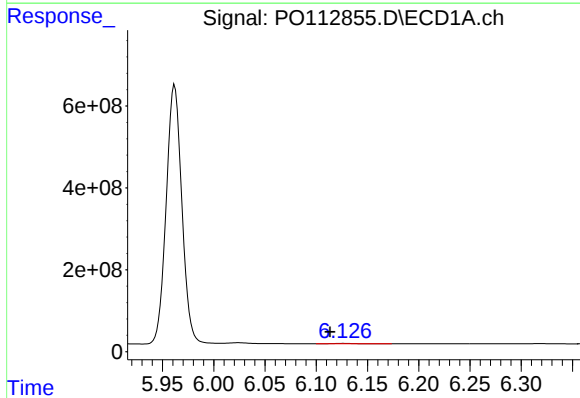


#28 AR-1254-3

R.T.: 6.126 min
Delta R.T.: 0.013 min
Response: 13000508
Conc: 17.47 ng/ml

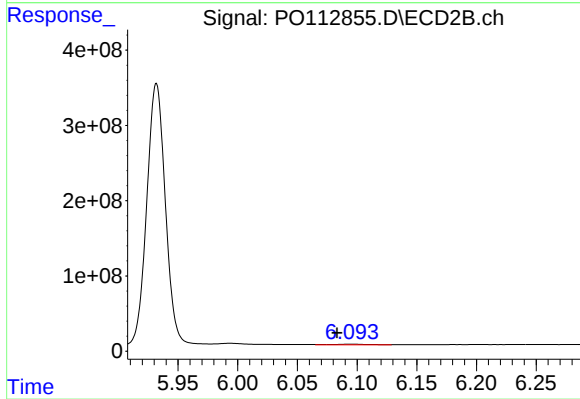

#28 AR-1254-3


R.T.: 6.095 min
Delta R.T.: 0.011 min
Response: 17463248
Conc: 40.85 ng/ml

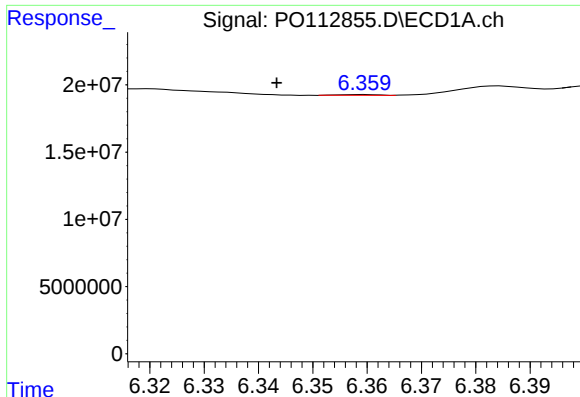

#29 AR-1254-4


R.T.: 6.359 min
Delta R.T.: 0.016 min
Response: 287582
Conc: 0.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

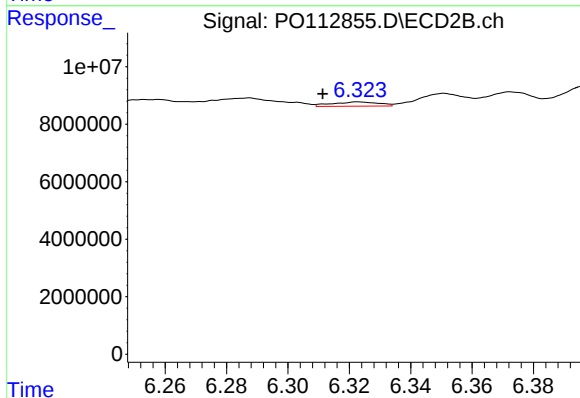


#29 AR-1254-4

R.T.: 6.323 min
Delta R.T.: 0.012 min
Response: 1588603
Conc: 5.82 ng/ml

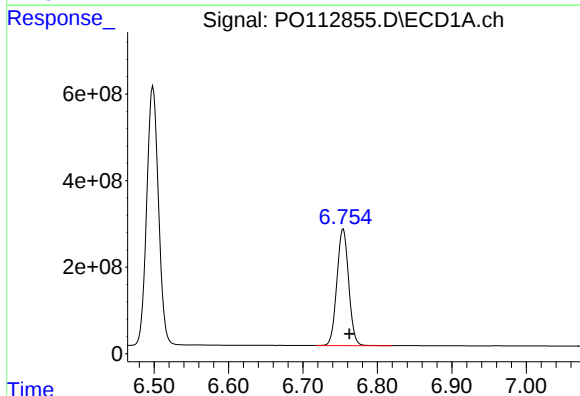


#30 AR-1254-5

R.T.: 6.754 min
Delta R.T.: -0.008 min
Response: 2965524021
Conc: 4189.63 ng/ml

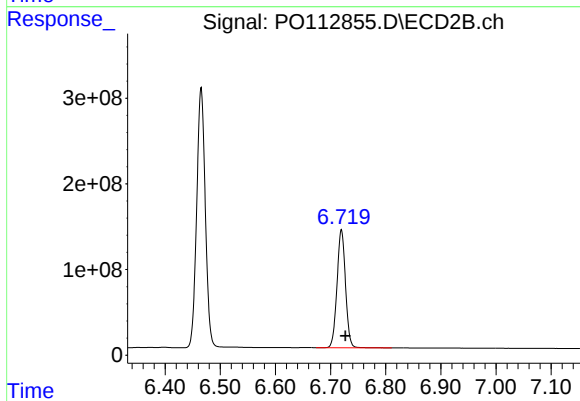

#30 AR-1254-5


R.T.: 6.720 min
Delta R.T.: -0.008 min
Response: 1476847068
Conc: 4421.44 ng/ml

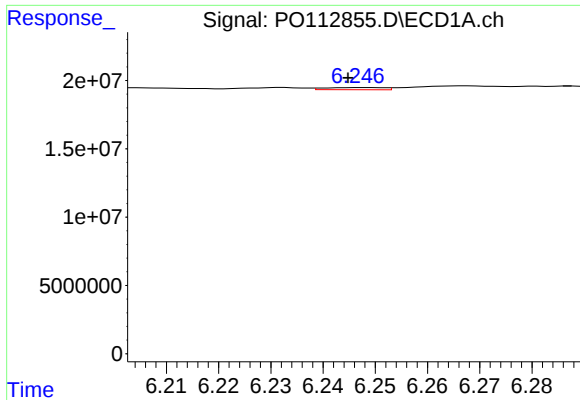

#31 AR-1260-1


R.T.: 6.248 min
Delta R.T.: 0.003 min
Response: 1240784
Conc: 2.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

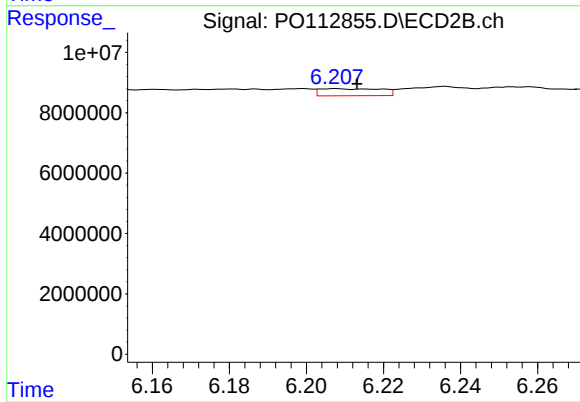


#31 AR-1260-1

R.T.: 6.207 min
Delta R.T.: -0.006 min
Response: 2592458
Conc: 10.43 ng/ml

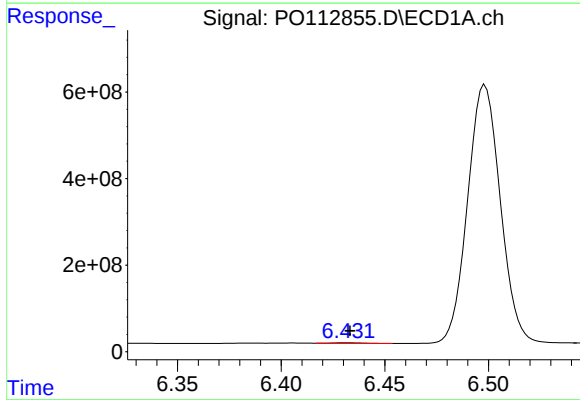


#32 AR-1260-2

R.T.: 6.432 min
Delta R.T.: -0.001 min
Response: 16382875
Conc: 23.82 ng/ml

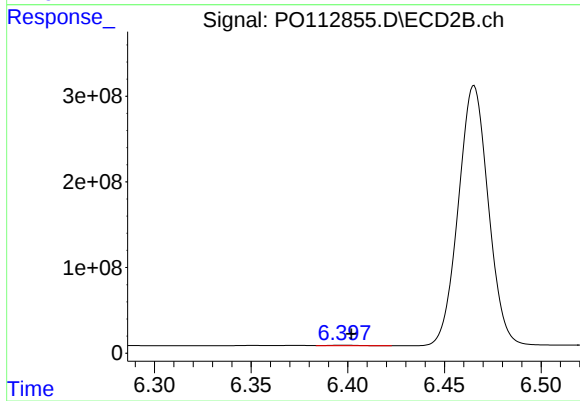

#32 AR-1260-2


R.T.: 6.398 min
Delta R.T.: -0.004 min
Response: 7723031
Conc: 23.44 ng/ml

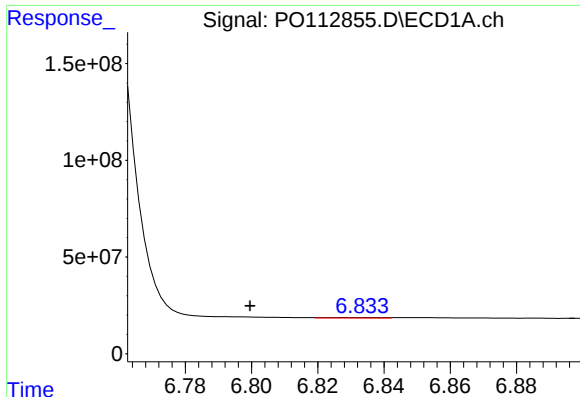

#33 AR-1260-3


R.T.: 6.829 min
Delta R.T.: 0.029 min
Response: 3293611
Conc: 5.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

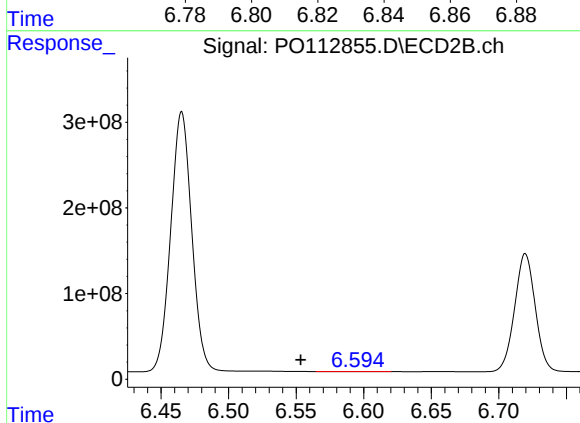


#33 AR-1260-3

R.T.: 6.585 min
Delta R.T.: 0.032 min
Response: 389525
Conc: 1.52 ng/ml

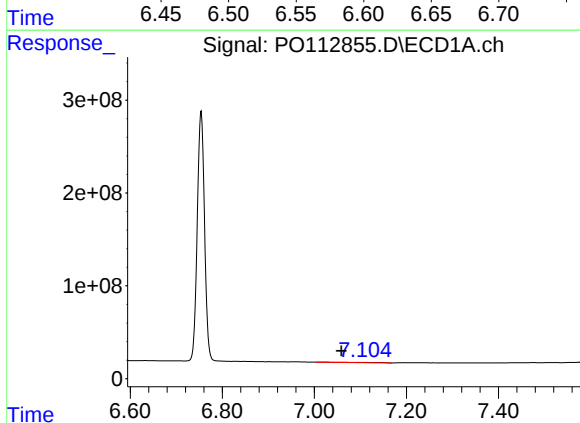


#34 AR-1260-4

R.T.: 7.016 min
Delta R.T.: -0.043 min
Response: 27346622
Conc: 60.63 ng/ml

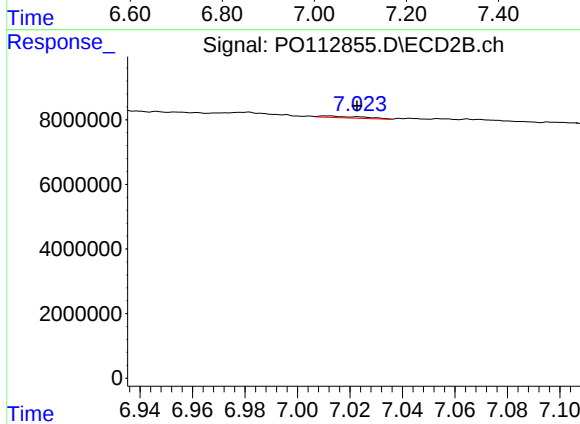

#34 AR-1260-4


R.T.: 7.011 min
Delta R.T.: -0.011 min
Response: 604175
Conc: 3.16 ng/ml

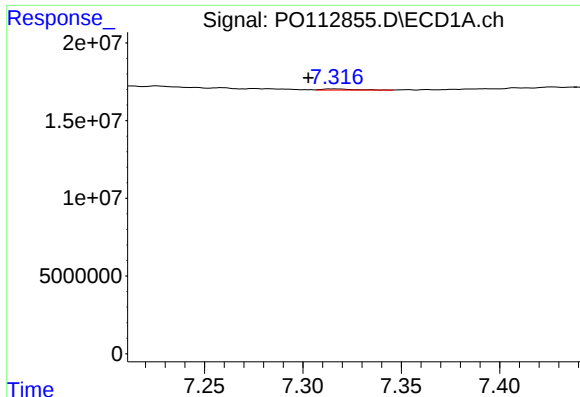

#35 AR-1260-5


R.T.: 7.316 min
Delta R.T.: 0.014 min
Response: 796083
Conc: 0.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

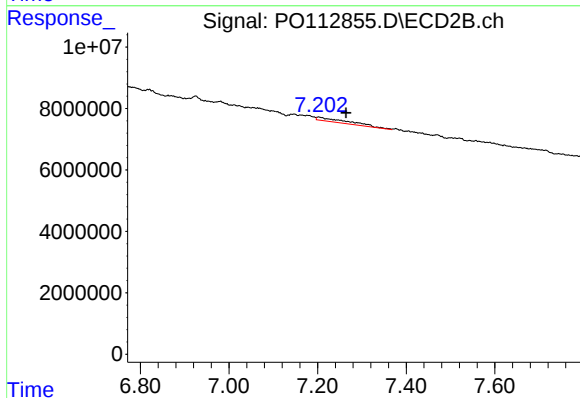


#35 AR-1260-5

R.T.: 7.202 min
Delta R.T.: -0.062 min
Response: 6155488
Conc: 14.93 ng/ml

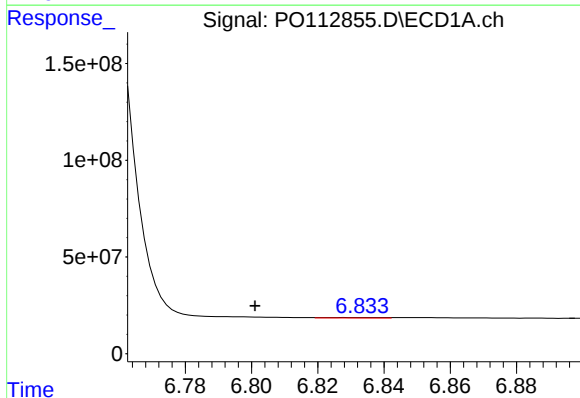


#36 AR-1262-1

R.T.: 6.829 min
Delta R.T.: 0.027 min
Response: 3293611
Conc: 3.54 ng/ml

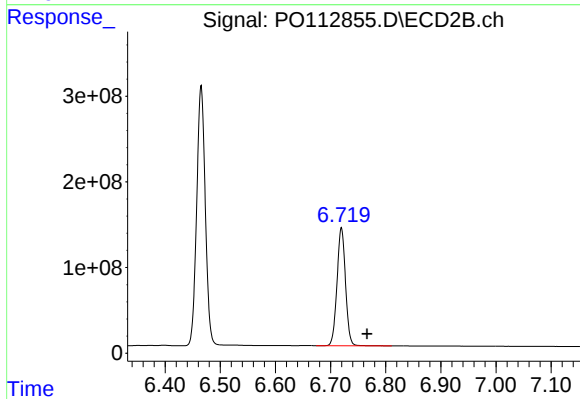

#36 AR-1262-1


R.T.: 6.720 min
Delta R.T.: -0.046 min
Response: 1476847068
Conc: 3560.14 ng/ml

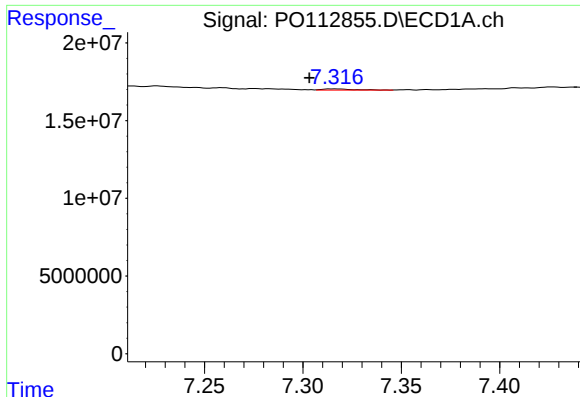

#37 AR-1262-2


R.T.: 7.316 min
Delta R.T.: 0.013 min
Response: 796083
Conc: 0.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

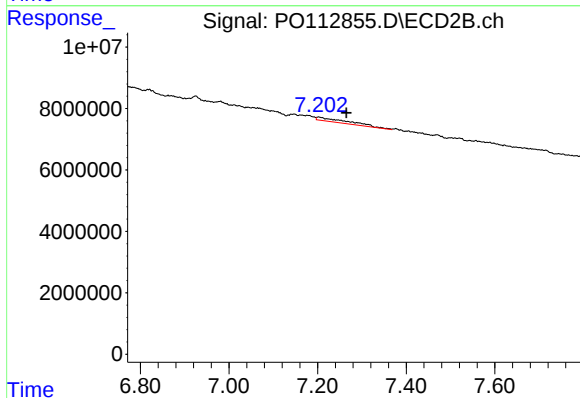


#37 AR-1262-2

R.T.: 7.202 min
Delta R.T.: -0.063 min
Response: 6155488
Conc: 11.94 ng/ml

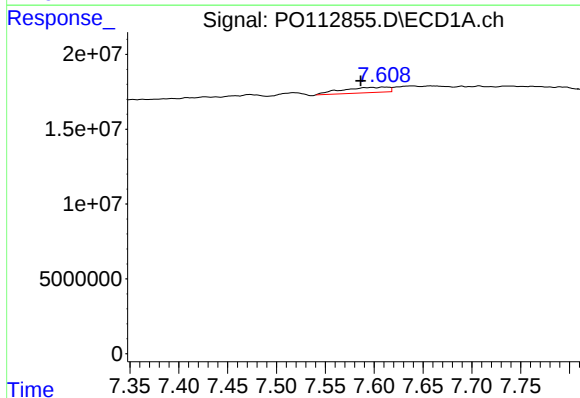


#38 AR-1262-3

R.T.: 7.611 min
Delta R.T.: 0.024 min
Response: 12079313
Conc: 20.46 ng/ml

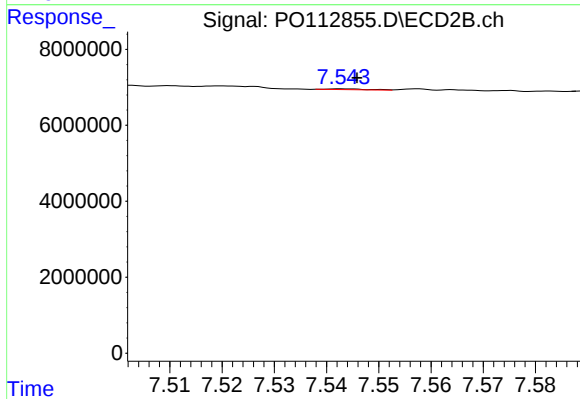

#38 AR-1262-3


R.T.: 7.543 min
Delta R.T.: -0.003 min
Response: 126135
Conc: 0.68 ng/ml

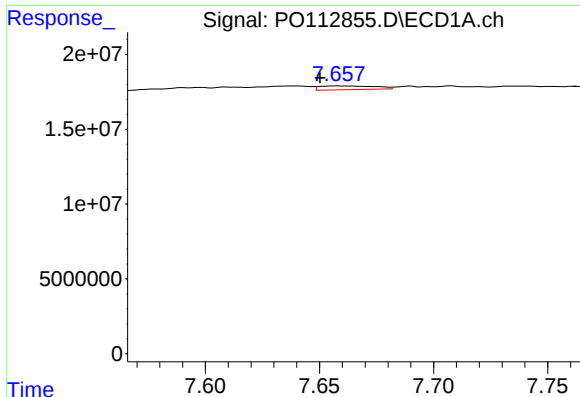

#39 AR-1262-4


R.T.: 7.658 min
Delta R.T.: 0.008 min
Response: 4339200
Conc: 4.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

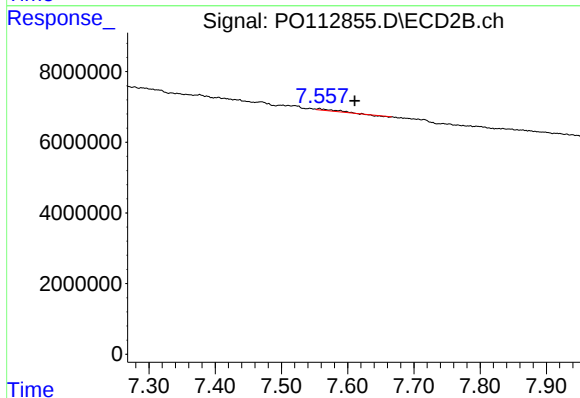


#39 AR-1262-4

R.T.: 7.557 min
Delta R.T.: -0.053 min
Response: 568206
Conc: 1.97 ng/ml

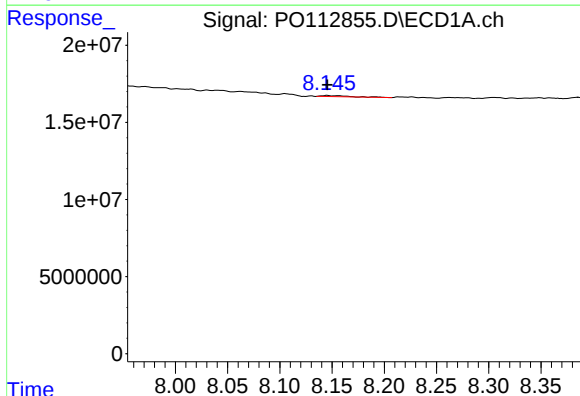


#40 AR-1262-5

R.T.: 8.145 min
Delta R.T.: 0.000 min
Response: 1270847
Conc: 2.93 ng/ml

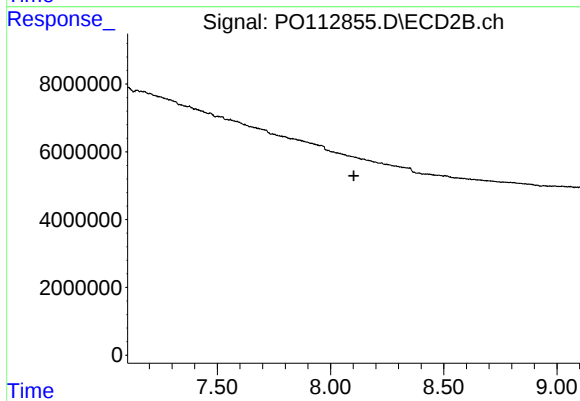

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 8.103 min
Response: 0
Conc: N.D.

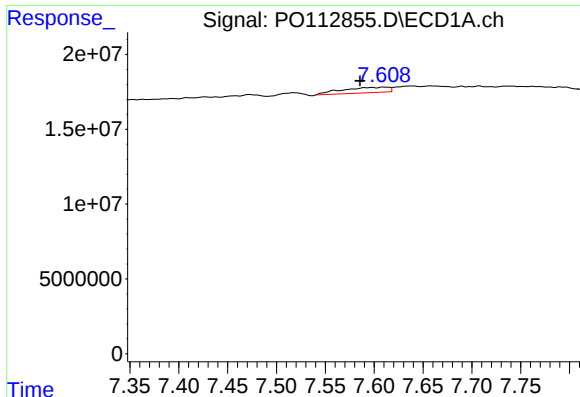

#41 AR-1268-1


R.T.: 7.611 min
Delta R.T.: 0.025 min
Response: 12079313
Conc: 6.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

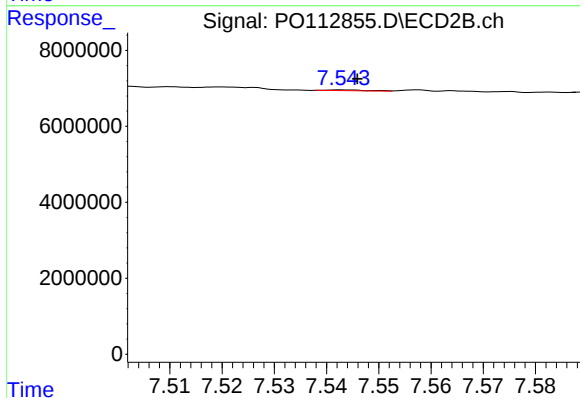


#41 AR-1268-1

R.T.: 7.543 min
Delta R.T.: -0.003 min
Response: 126135
Conc: 0.24 ng/ml

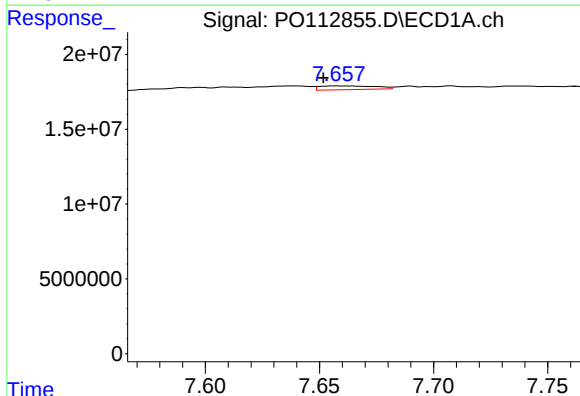


#42 AR-1268-2

R.T.: 7.658 min
Delta R.T.: 0.007 min
Response: 4339200
Conc: 2.95 ng/ml

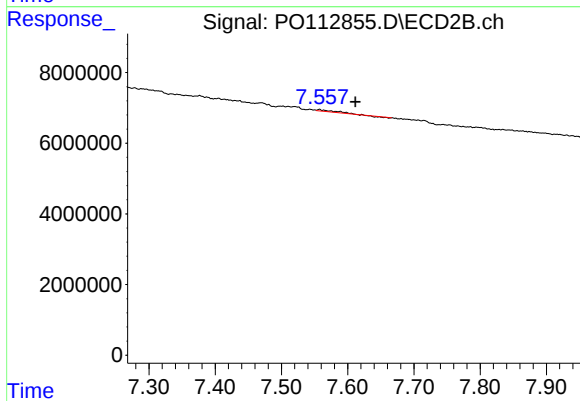

#42 AR-1268-2


R.T.: 7.557 min
Delta R.T.: -0.054 min
Response: 568206
Conc: 1.34 ng/ml

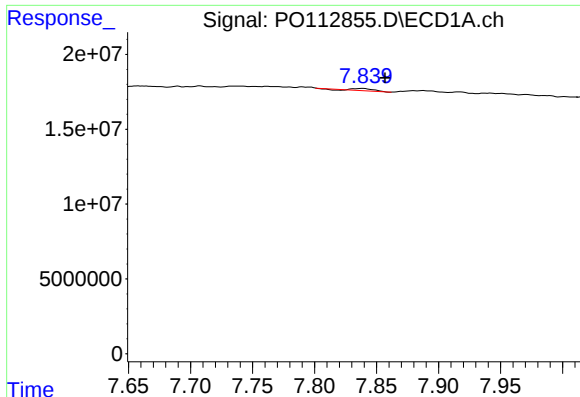

#43 AR-1268-3


R.T.: 7.838 min
Delta R.T.: -0.018 min
Response: 1510572
Conc: 1.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

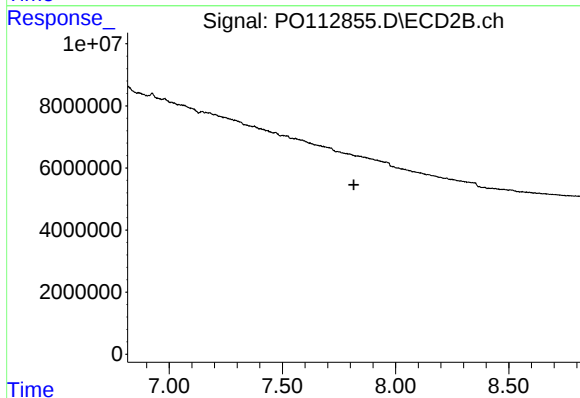


#43 AR-1268-3

R.T.: 7.834 min
Delta R.T.: 0.019 min
Response: -280578
Conc: N.D.

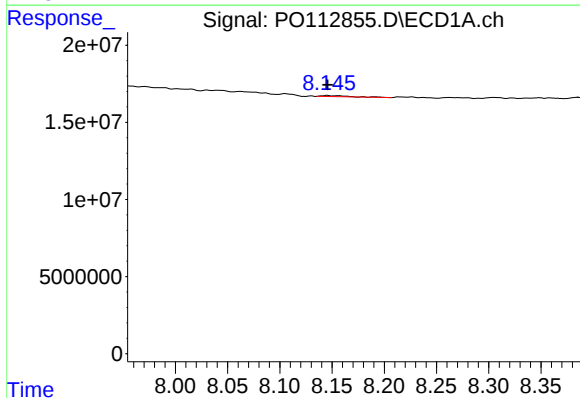


#44 AR-1268-4

R.T.: 8.145 min
Delta R.T.: 0.000 min
Response: 1270847
Conc: 2.64 ng/ml

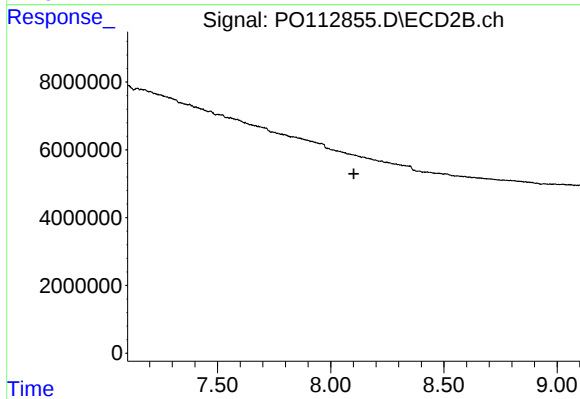

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 8.103 min
Response: 0
Conc: N.D.

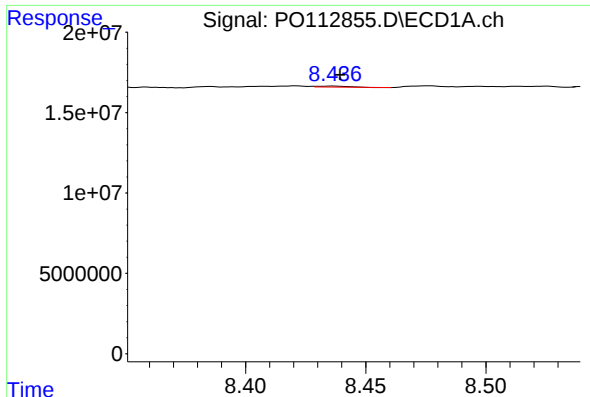

#45 AR-1268-5

R.T.: 8.437 min
Delta R.T.: -0.002 min
Response: 525722
Conc: 0.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

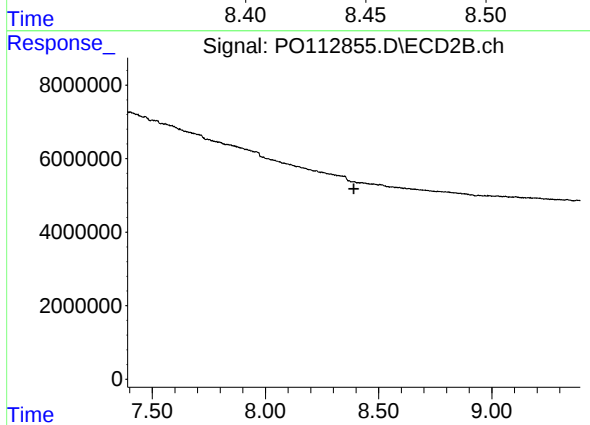

#45 AR-1268-5

R.T.: 8.392 min
Delta R.T.: 0.000 min
Response: -532504
Conc: N.D.