

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081319\
 Data File : P0059242.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2019 14:39
 Operator : SM/SJ
 Sample : K4096-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-04-081219

Manual Integrations
 APPROVED

Ankita
 8/14/2019 2:47:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 08:36:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.150	3.511	1015131	894291	24.054m	22.385
2) SA Decachlor...	9.649	8.388	1177551	831433	21.744	21.063

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081319\
Data File : PO059242.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2019 14:39
Operator : SM/SJ
Sample : K4096-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-04-081219


Manual Integrations
APPROVED

Ankita
8/14/2019 2:47:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 08:36:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

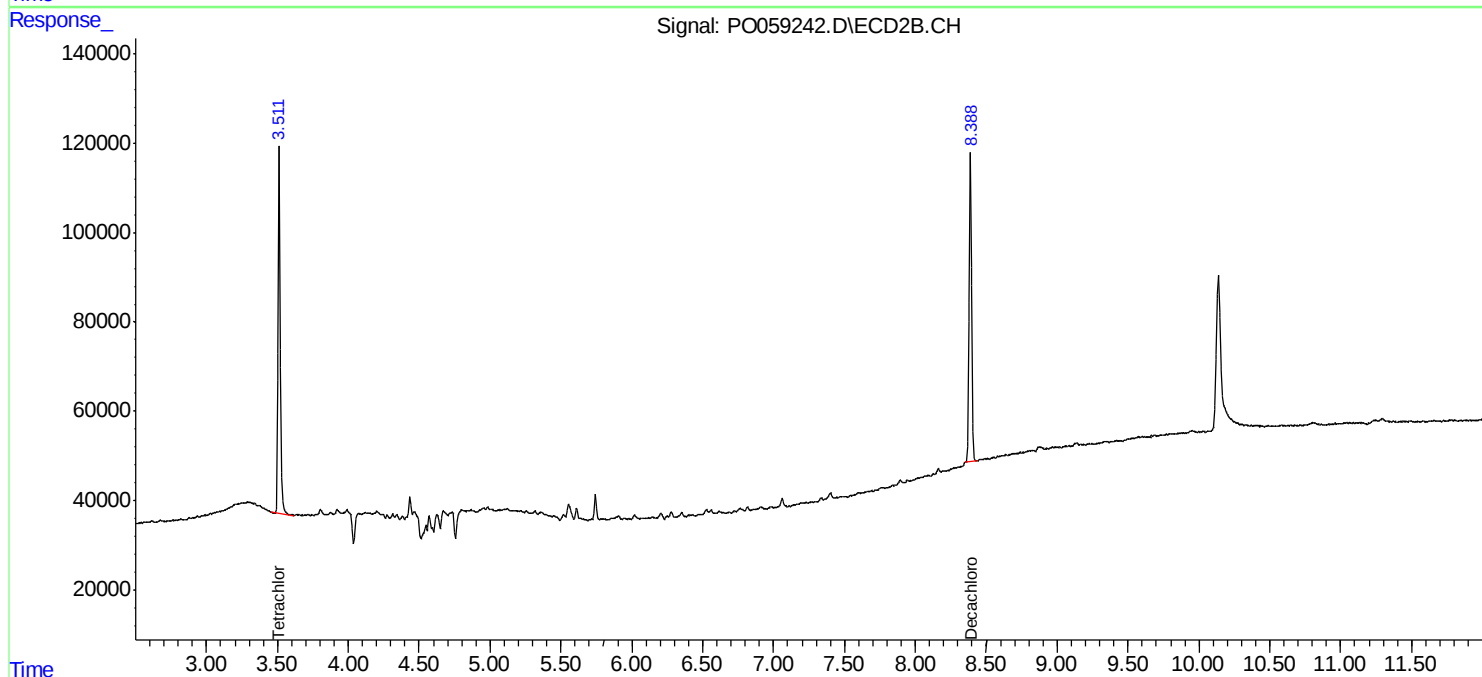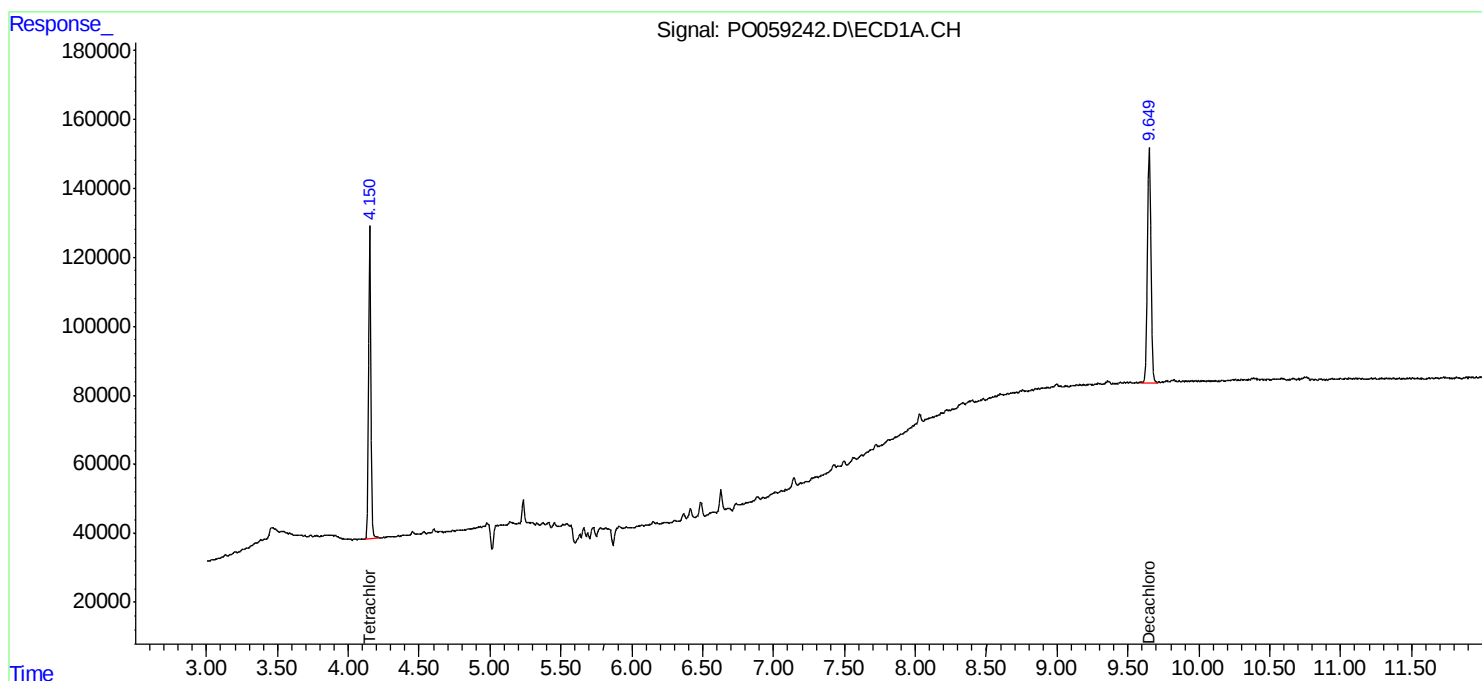

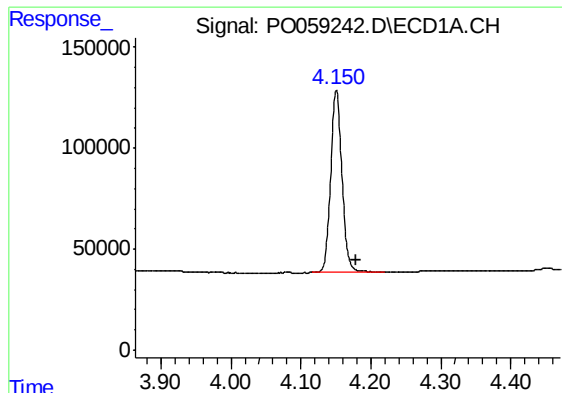


#1 Tetrachloro-m-xylene

R.T.: 4.150 min
Delta R.T.: -0.029 min
Response: 1015131
Conc: 24.05 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TR-04-081219


Manual Integrations
APPROVED

Ankita
8/14/2019 2:47:51 PM

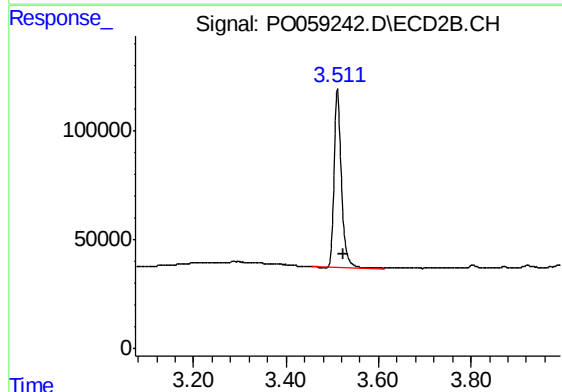


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: -0.014 min
Response: 894291
Conc: 22.39 ng/ml

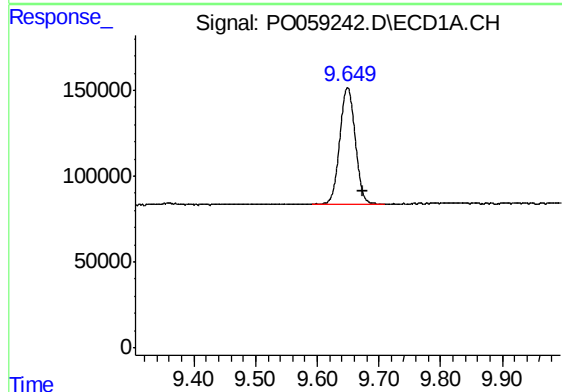

#2 Decachlorobiphenyl

R.T.: 9.649 min
Delta R.T.: -0.023 min
Response: 1177551
Conc: 21.74 ng/ml

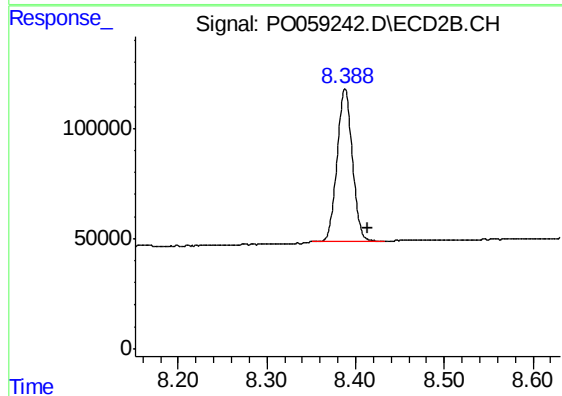

#2 Decachlorobiphenyl

R.T.: 8.388 min
Delta R.T.: -0.026 min
Response: 831433
Conc: 21.06 ng/ml