

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081319\
 Data File : P0059246.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2019 15:46
 Operator : SM/SJ
 Sample : K4319-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRANSFORMER-CONTAINMENT-S

Manual Integrations
 APPROVED

Ankita
 8/14/2019 2:48:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 18:08:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.150	3.511	746608	687635	17.691m	17.212
2)	SA Decachlor...	9.649	8.387	974960	695695	18.003	17.625
Target Compounds							
31)	L7 AR-1260-1	6.884	6.016	229655	167294	79.765	70.290
32)	L7 AR-1260-2	7.140	6.203	271987	162313	65.381m	53.581
33)	L7 AR-1260-3	7.496	6.352	299006	177462	80.292	65.731
34)	L7 AR-1260-4	7.721	6.815	314155	196828	92.188	87.110m
35)	L7 AR-1260-5	8.029	7.059	660812	496860	89.848	92.261

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081319\
Data File : PO059246.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2019 15:46
Operator : SM/SJ
Sample : K4319-04
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TRANSFORMER-CONTAINMENT-S


Manual Integrations
APPROVED

Ankita
8/14/2019 2:48:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 18:08:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

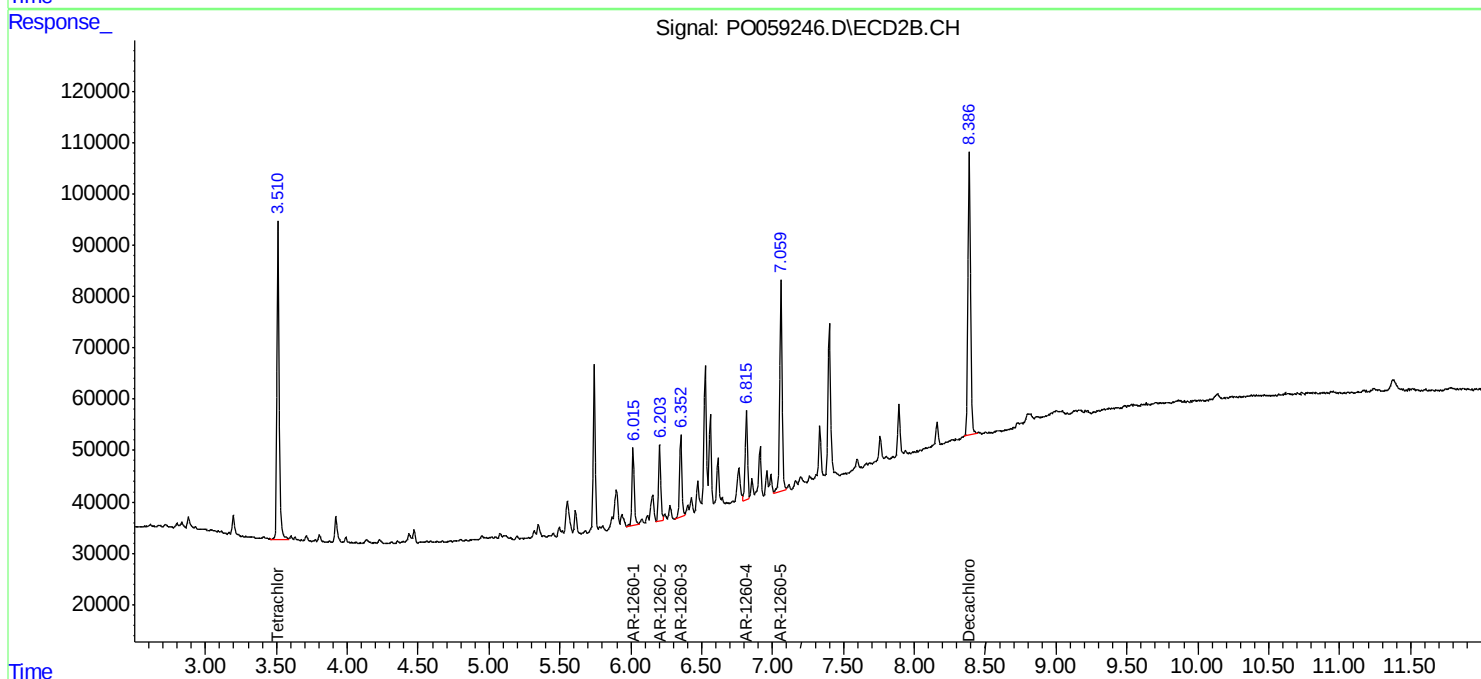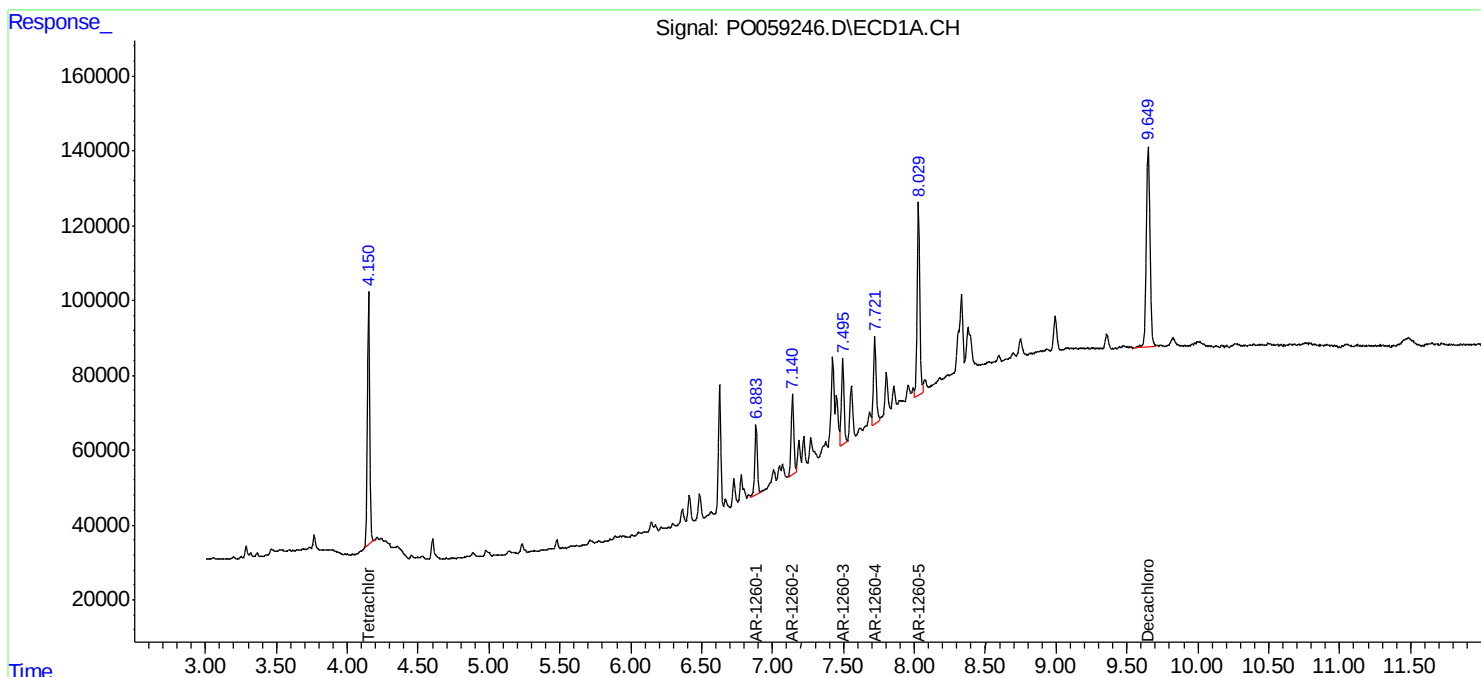

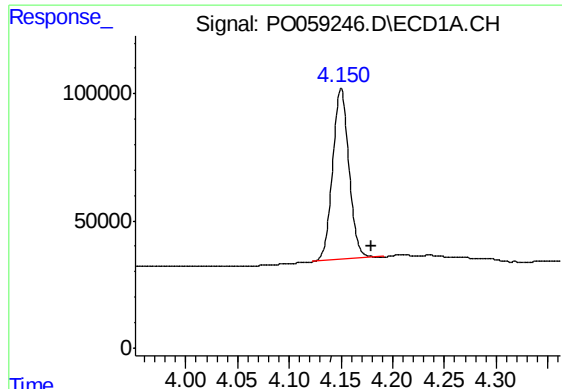


#1 Tetrachloro-m-xylene

R.T.: 4.150 min
Delta R.T.: -0.029 min
Response: 746608
Conc: 17.69 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TRANSFORMER-CONTAINMENT-S


Manual Integrations
APPROVED

Ankita
8/14/2019 2:48:51 PM

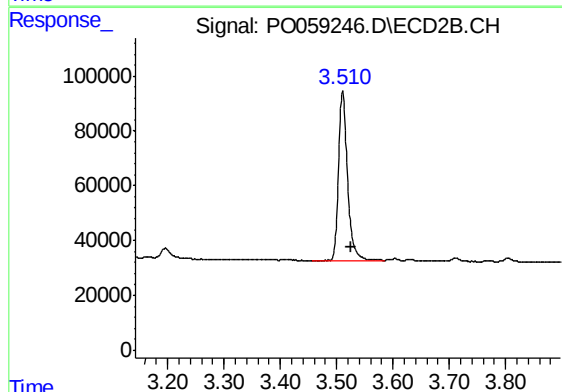


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: -0.014 min
Response: 687635
Conc: 17.21 ng/ml

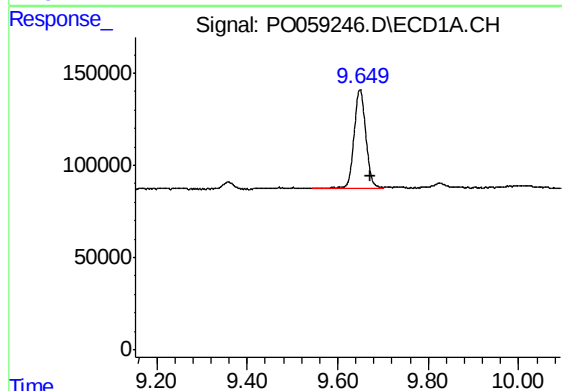


#2 Decachlorobiphenyl

R.T.: 9.649 min
Delta R.T.: -0.024 min
Response: 974960
Conc: 18.00 ng/ml

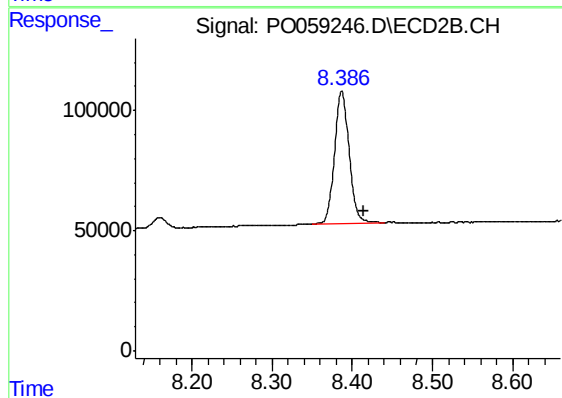

#2 Decachlorobiphenyl

R.T.: 8.387 min
Delta R.T.: -0.027 min
Response: 695695
Conc: 17.62 ng/ml

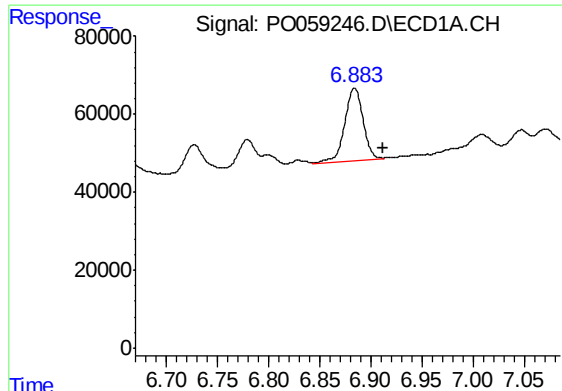


#31 AR-1260-1

R.T.: 6.884 min
Delta R.T.: -0.028 min
Response: 229655
Conc: 79.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRANSFORMER-CONTAINMENT-S


Manual Integrations
APPROVED

Ankita
8/14/2019 2:48:51 PM

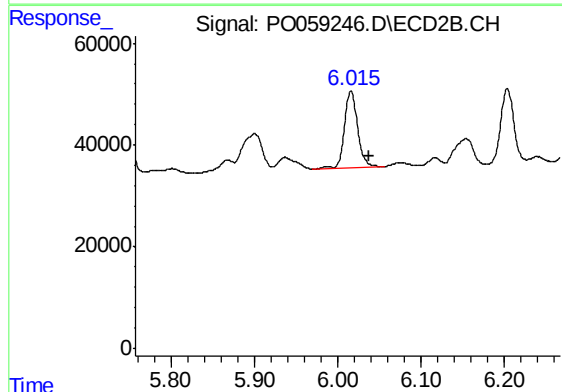


#31 AR-1260-1

R.T.: 6.016 min
Delta R.T.: -0.021 min
Response: 167294
Conc: 70.29 ng/ml

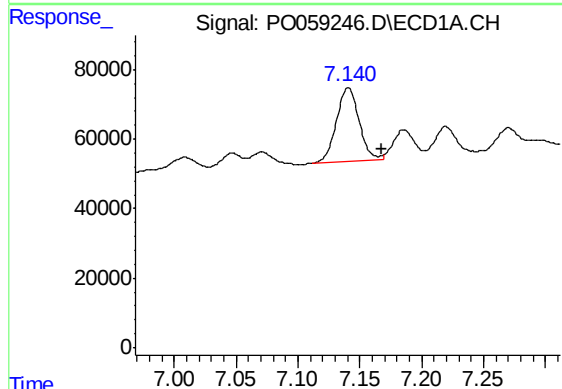


#32 AR-1260-2

R.T.: 7.140 min
Delta R.T.: -0.027 min
Response: 271987
Conc: 65.38 ng/ml m

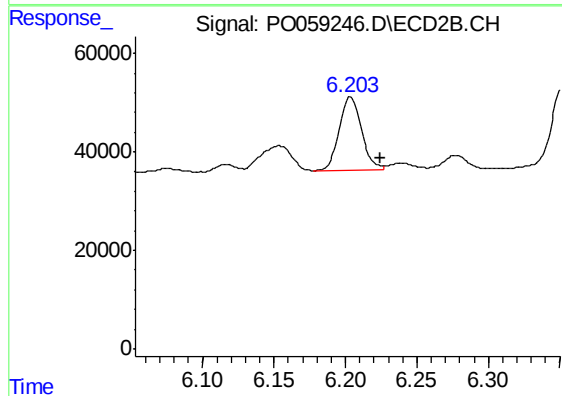

#32 AR-1260-2

R.T.: 6.203 min
Delta R.T.: -0.021 min
Response: 162313
Conc: 53.58 ng/ml

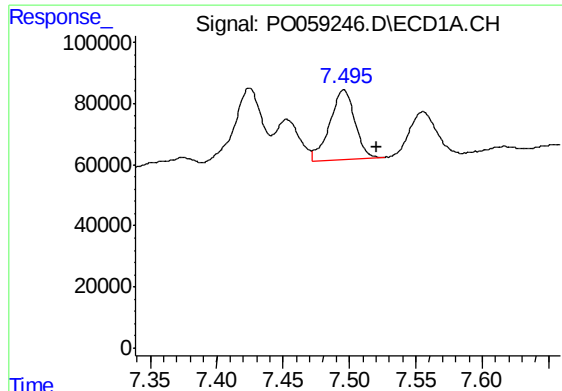


#33 AR-1260-3

R.T.: 7.496 min
Delta R.T.: -0.025 min
Response: 299006
Conc: 80.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRANSFORMER-CONTAINMENT-S


Manual Integrations
APPROVED

Ankita
8/14/2019 2:48:51 PM

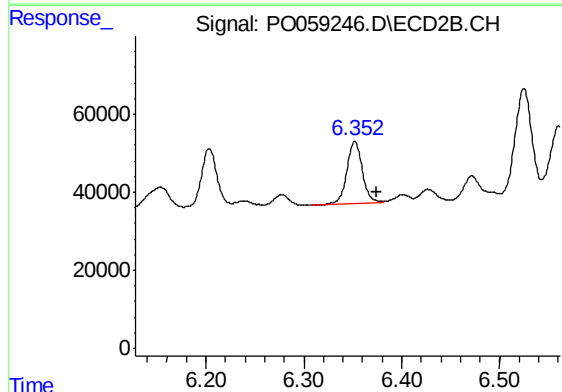


#33 AR-1260-3

R.T.: 6.352 min
Delta R.T.: -0.022 min
Response: 177462
Conc: 65.73 ng/ml

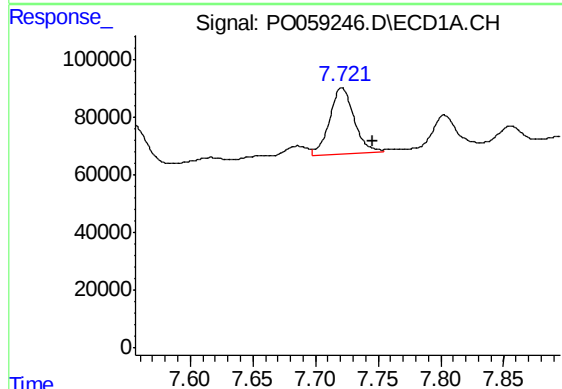


#34 AR-1260-4

R.T.: 7.721 min
Delta R.T.: -0.025 min
Response: 314155
Conc: 92.19 ng/ml

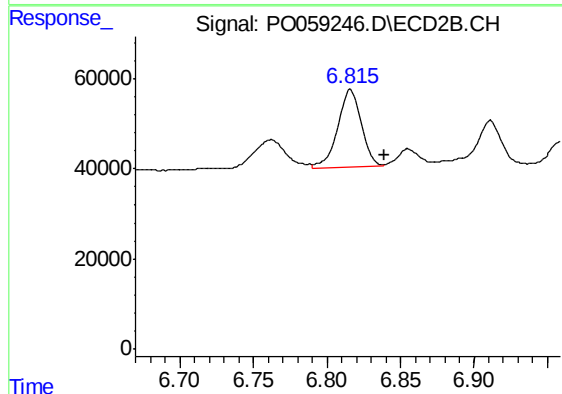

#34 AR-1260-4

R.T.: 6.815 min
Delta R.T.: -0.024 min
Response: 196828
Conc: 87.11 ng/ml m

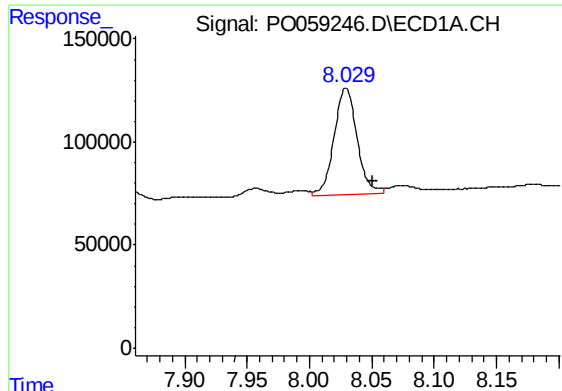


#35 AR-1260-5

R.T.: 8.029 min
Delta R.T.: -0.022 min
Response: 660812
Conc: 89.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRANSFORMER-CONTAINMENT-S

Manual Integrations
APPROVED

Ankita
8/14/2019 2:48:51 PM

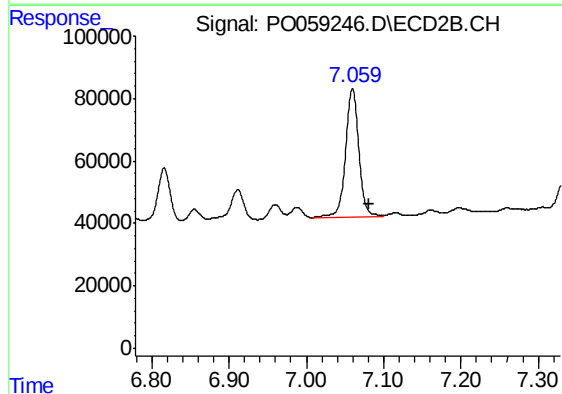

#35 AR-1260-5

R.T.: 7.059 min
Delta R.T.: -0.022 min
Response: 496860
Conc: 92.26 ng/ml