

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081319\
 Data File : P0059254.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2019 17:59
 Operator : SM/SJ
 Sample : K4319-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TEST-PIT-2

Manual Integrations
 APPROVED

Ankita
 8/14/2019 2:49:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:40:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.146	3.511	853275	793146	20.218m	19.853
2)	SA Decachlor...	9.648	8.388	1127533	811235	20.820	20.552
Target Compounds							
31)	L7 AR-1260-1	6.883	6.016	46189	38173	16.043m	16.039
32)	L7 AR-1260-2	7.139	6.203	100475	60145	24.152m	19.854
33)	L7 AR-1260-3	7.493	6.352	75131	50079	20.175	18.549
34)	L7 AR-1260-4	7.720	6.816	85268	37915	25.021m	16.780 #
35)	L7 AR-1260-5	8.029	7.059	138468	119117	18.827m	22.119

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081319\
Data File : PO059254.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2019 17:59
Operator : SM/SJ
Sample : K4319-07
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TEST-PIT-2


Manual Integrations
APPROVED

Ankita
8/14/2019 2:49:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:40:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

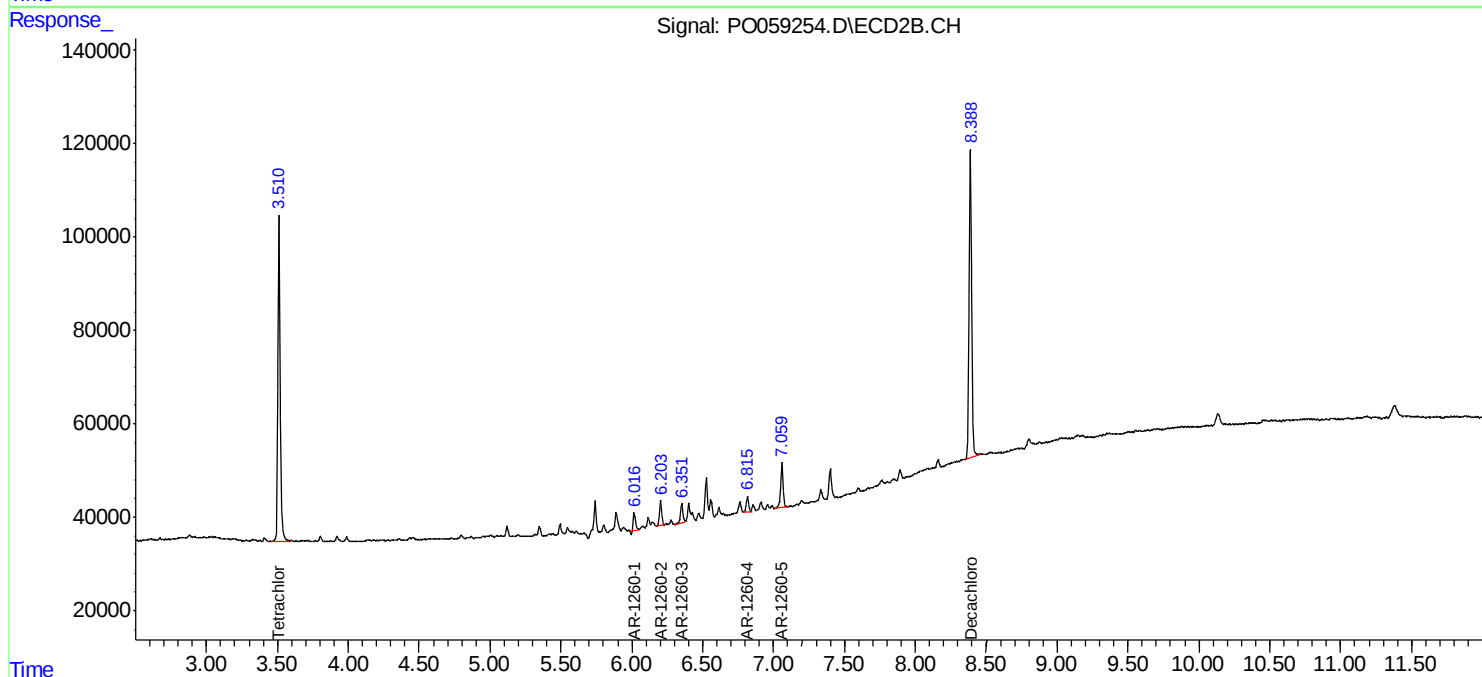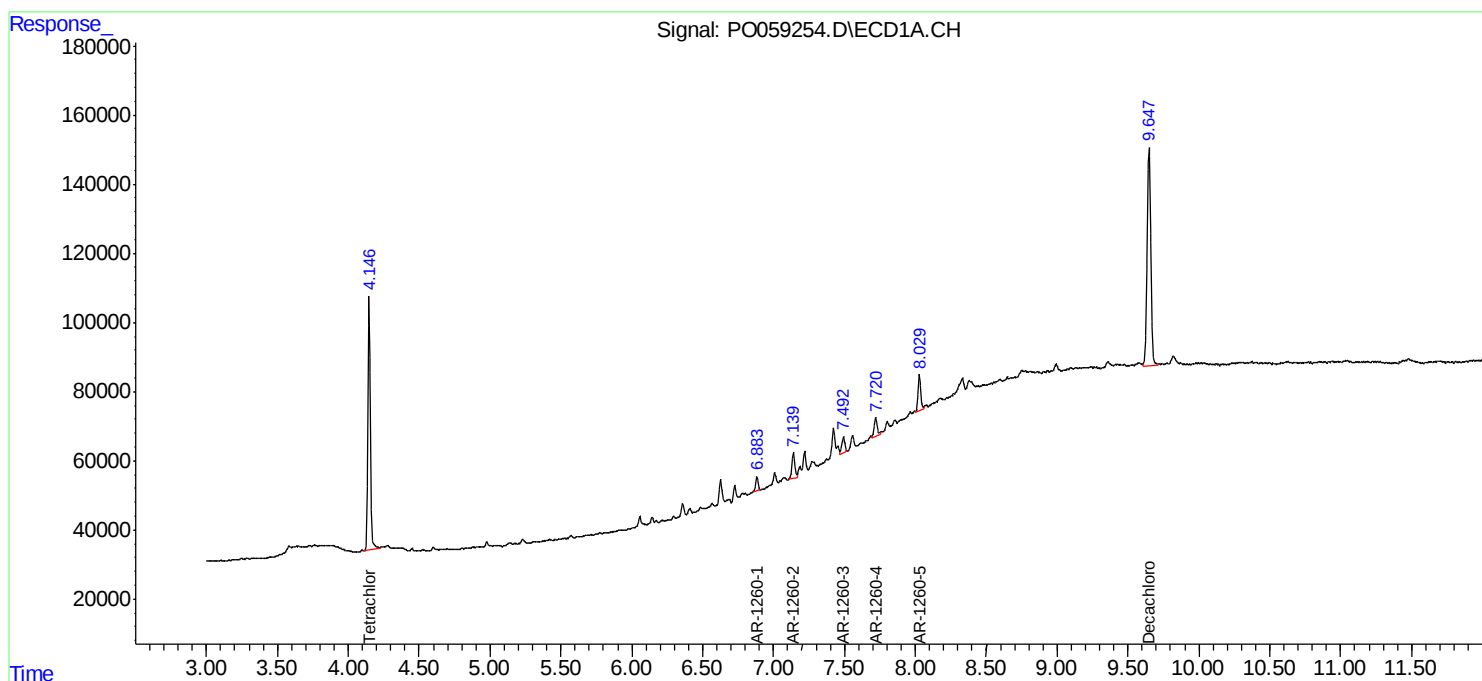

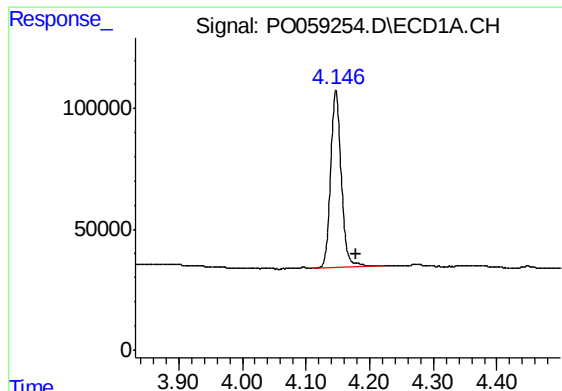


#1 Tetrachloro-m-xylene

R.T.: 4.146 min
Delta R.T.: -0.033 min
Response: 853275
Conc: 20.22 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-2


Manual Integrations
APPROVED

Ankita
8/14/2019 2:49:12 PM

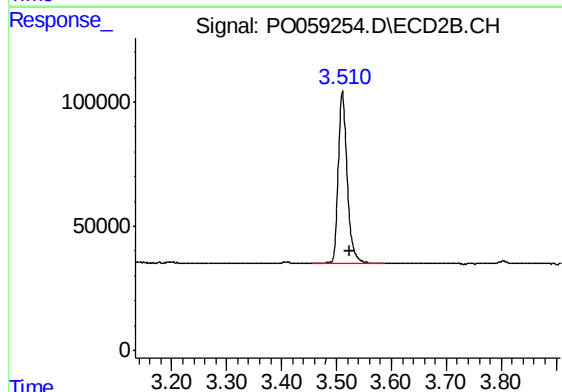


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: -0.014 min
Response: 793146
Conc: 19.85 ng/ml

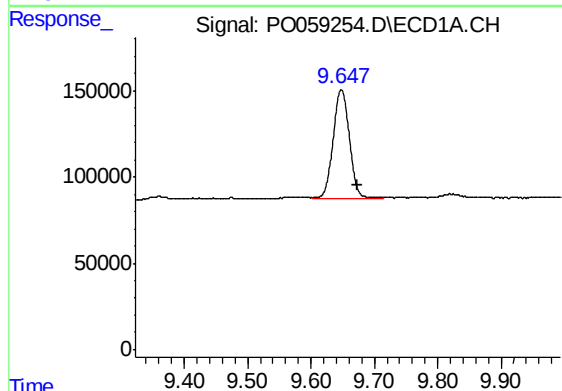


#2 Decachlorobiphenyl

R.T.: 9.648 min
Delta R.T.: -0.025 min
Response: 1127533
Conc: 20.82 ng/ml

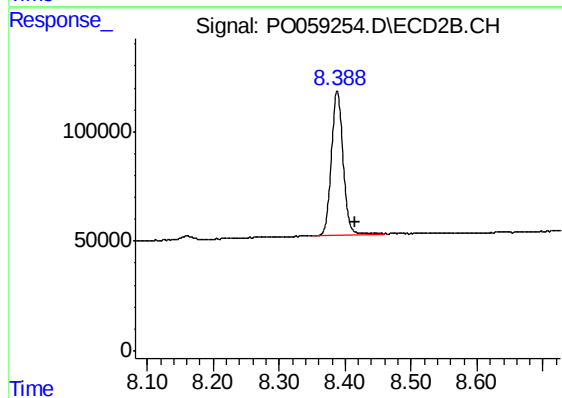

#2 Decachlorobiphenyl

R.T.: 8.388 min
Delta R.T.: -0.026 min
Response: 811235
Conc: 20.55 ng/ml

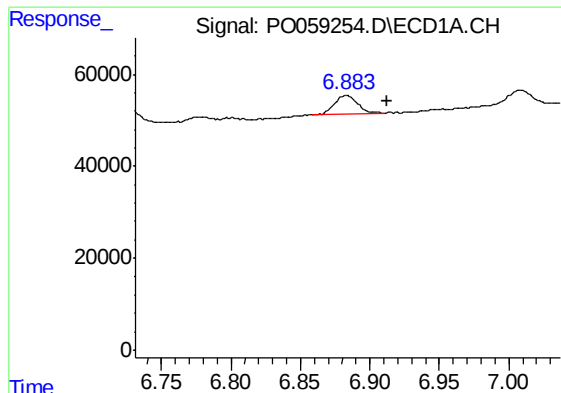


#31 AR-1260-1

R.T.: 6.883 min
Delta R.T.: -0.029 min
Response: 46189
Conc: 16.04 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-2


Manual Integrations
APPROVED

Ankita
8/14/2019 2:49:12 PM

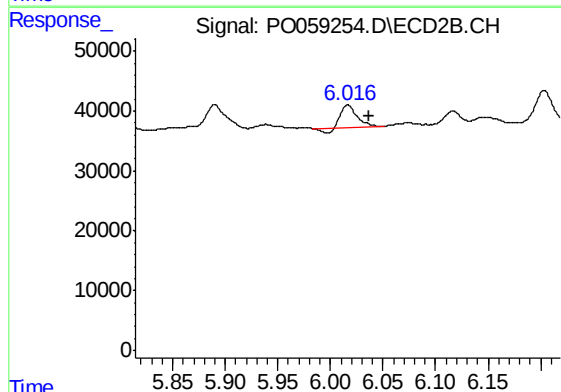


#31 AR-1260-1

R.T.: 6.016 min
Delta R.T.: -0.021 min
Response: 38173
Conc: 16.04 ng/ml

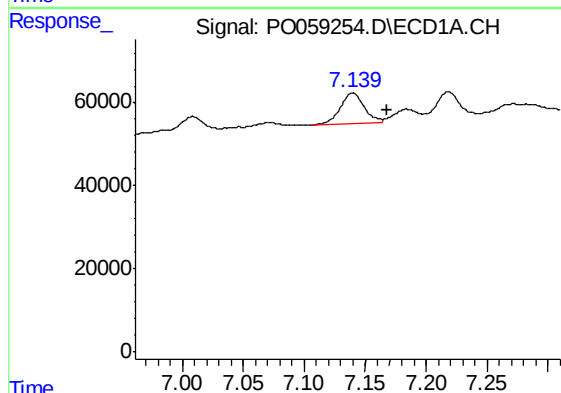


#32 AR-1260-2

R.T.: 7.139 min
Delta R.T.: -0.028 min
Response: 100475
Conc: 24.15 ng/ml m

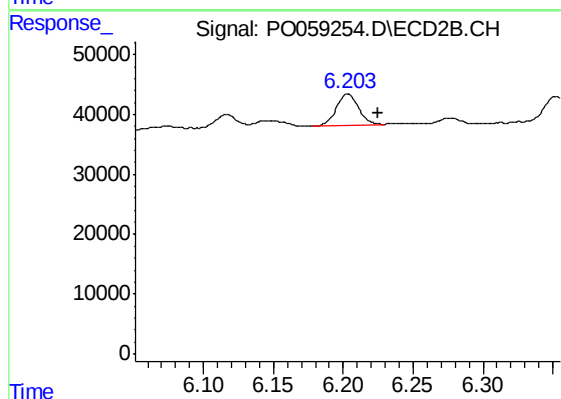

#32 AR-1260-2

R.T.: 6.203 min
Delta R.T.: -0.021 min
Response: 60145
Conc: 19.85 ng/ml

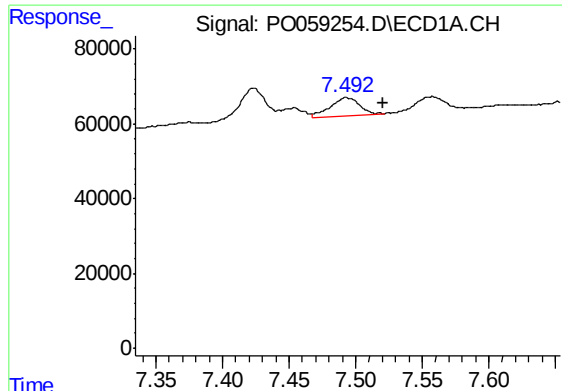


#33 AR-1260-3

R.T.: 7.493 min
Delta R.T.: -0.027 min
Response: 75131
Conc: 20.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-2


Manual Integrations
APPROVED

Ankita
8/14/2019 2:49:12 PM

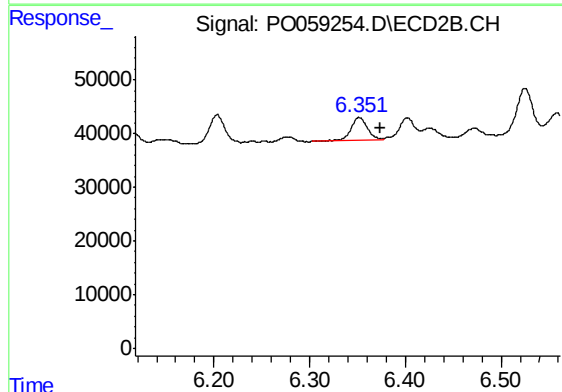


#33 AR-1260-3

R.T.: 6.352 min
Delta R.T.: -0.023 min
Response: 50079
Conc: 18.55 ng/ml

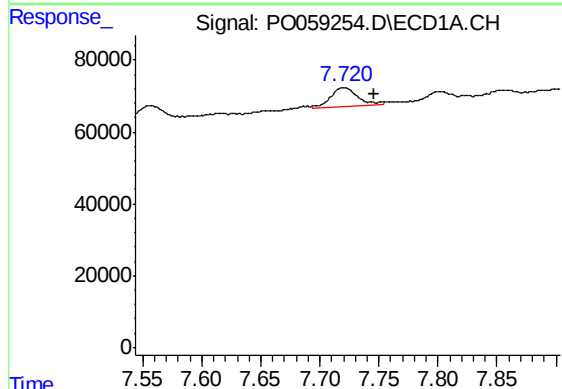


#34 AR-1260-4

R.T.: 7.720 min
Delta R.T.: -0.027 min
Response: 85268
Conc: 25.02 ng/ml m

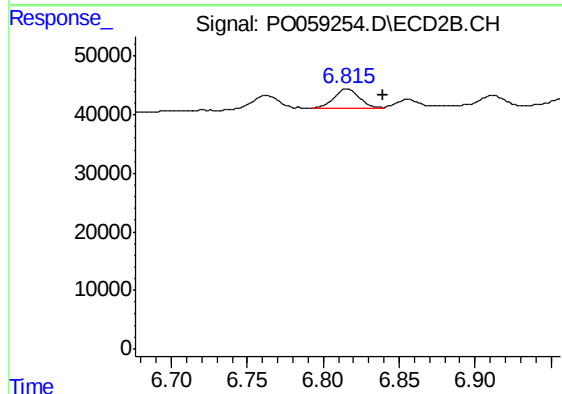

#34 AR-1260-4

R.T.: 6.816 min
Delta R.T.: -0.023 min
Response: 37915
Conc: 16.78 ng/ml

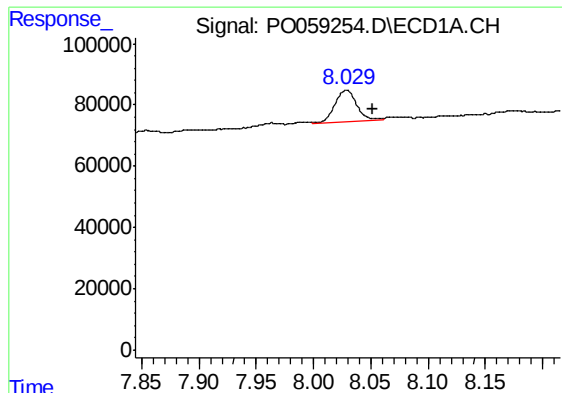


#35 AR-1260-5

R.T.: 8.029 min
Delta R.T.: -0.023 min
Response: 138468
Conc: 18.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-2

Manual Integrations
APPROVED

Ankita
8/14/2019 2:49:12 PM

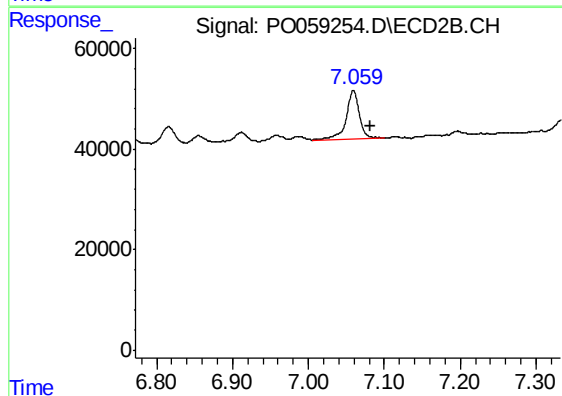

#35 AR-1260-5

R.T.: 7.059 min
Delta R.T.: -0.022 min
Response: 119117
Conc: 22.12 ng/ml