

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081320\
 Data File : P0070547.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2020 15:50
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 16:08:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.367	3.551	1675821	957007	25.343	21.721
2)	SA Decachlor...	9.994	8.742	1937226	1153954	22.625	20.789
Target Compounds							
9)	L2 AR-1221-2	4.710f	0.000	23278	0	37.001	N.D. #
24)	L5 AR-1248-4	6.580f	0.000	45935	0	13.501	N.D. #
26)	L6 AR-1254-1	6.580	0.000	45935	0	12.909	N.D. #
34)	L7 AR-1260-4	8.171f	0.000	1998	0	0.411	N.D. #
39)	L8 AR-1262-4	8.833f	0.000	1778	0	0.563	N.D. #
42)	L9 AR-1268-2	8.833f	0.000	1778	0	0.131	N.D. #
45)	L9 AR-1268-5	9.733	0.000	7962	0	0.253	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081320\
Data File : P0070547.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2020 15:50
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 16:08:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

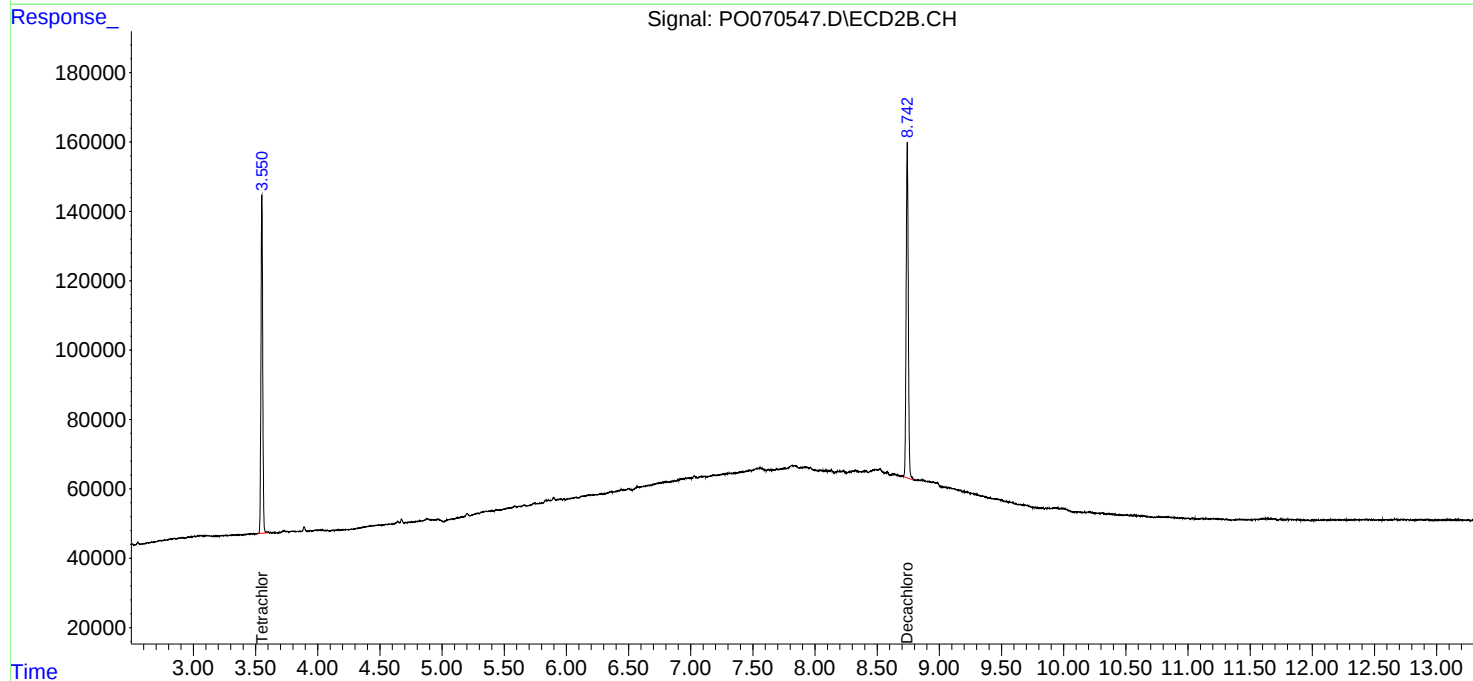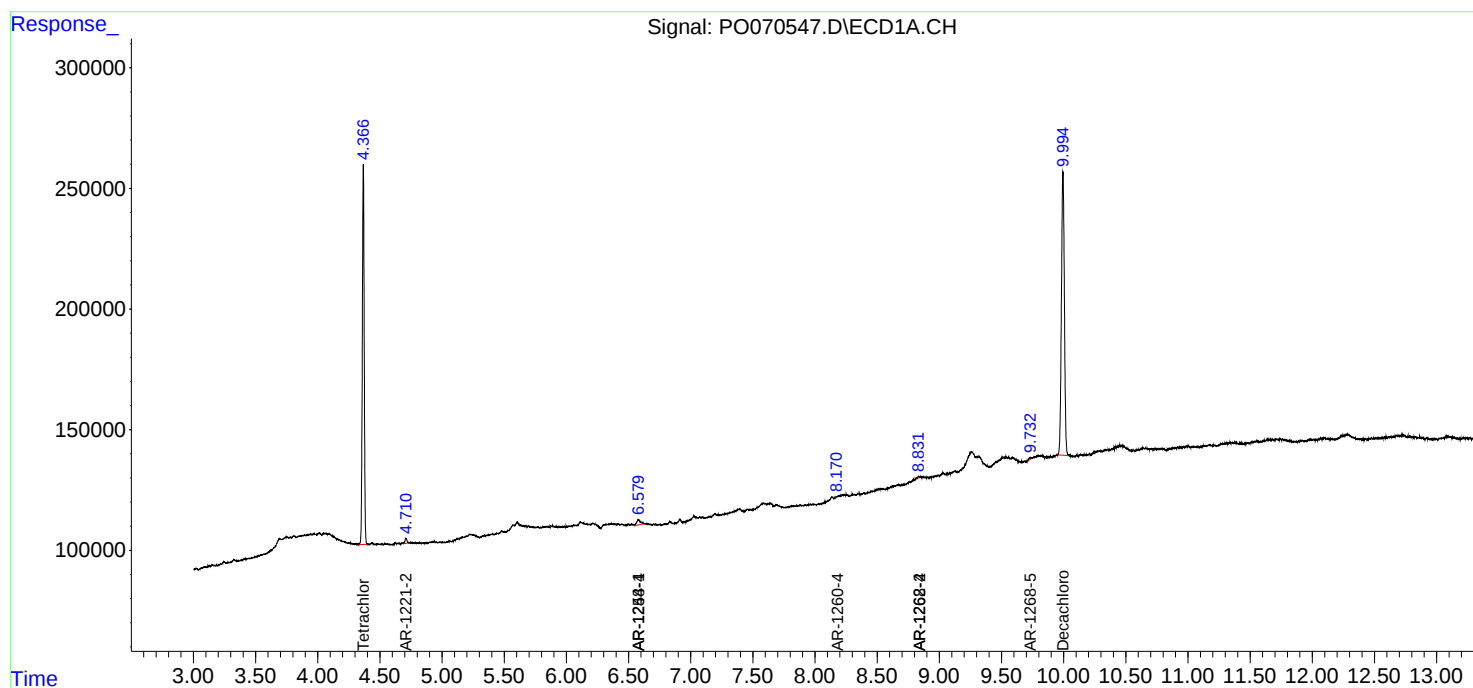


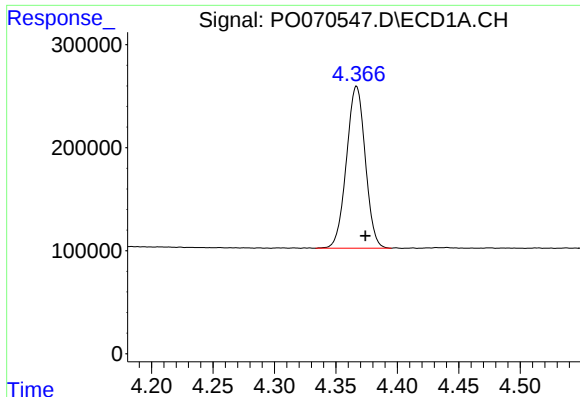

#1 Tetrachloro-m-xylene


R.T.: 4.367 min
Delta R.T.: -0.007 min
Response: 1675821
Conc: 25.34 ng/ml

Instrument :
ECD_O
ClientSampleId :

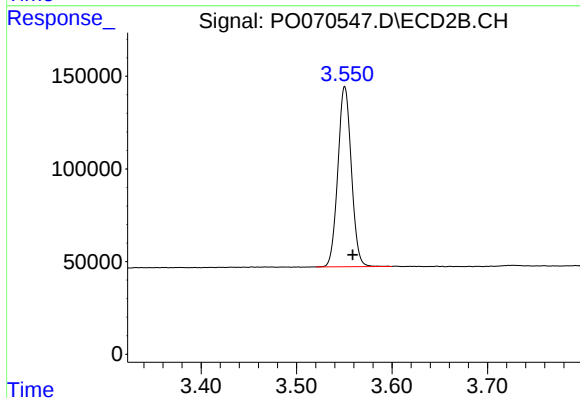


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: -0.008 min
Response: 957007
Conc: 21.72 ng/ml

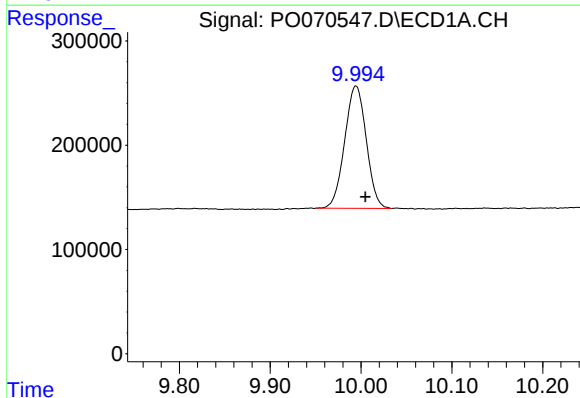


#2 Decachlorobiphenyl

R.T.: 9.994 min
Delta R.T.: -0.011 min
Response: 1937226
Conc: 22.62 ng/ml

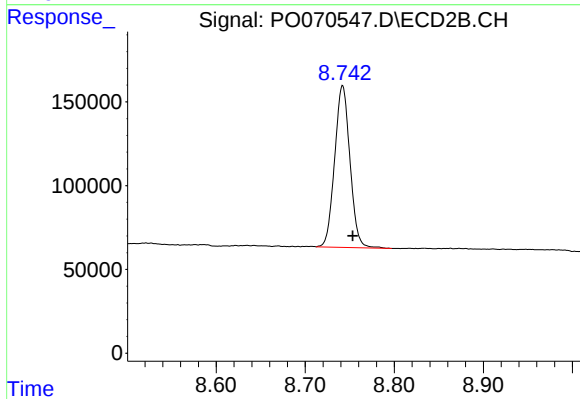

#2 Decachlorobiphenyl


R.T.: 8.742 min
Delta R.T.: -0.011 min
Response: 1153954
Conc: 20.79 ng/ml

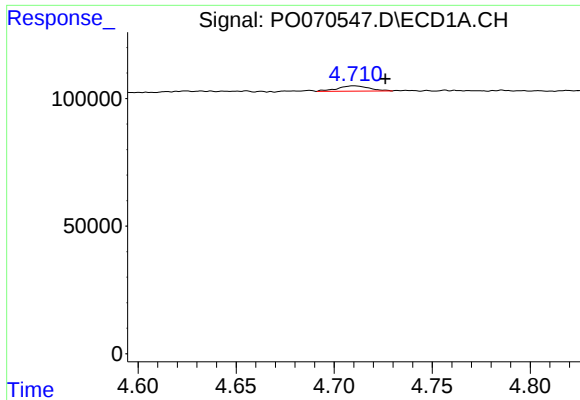

#9 AR-1221-2


R.T.: 4.710 min
Delta R.T.: -0.016 min
Response: 23278
Conc: 37.00 ng/ml

Instrument :
ECD_O
ClientSampleId :

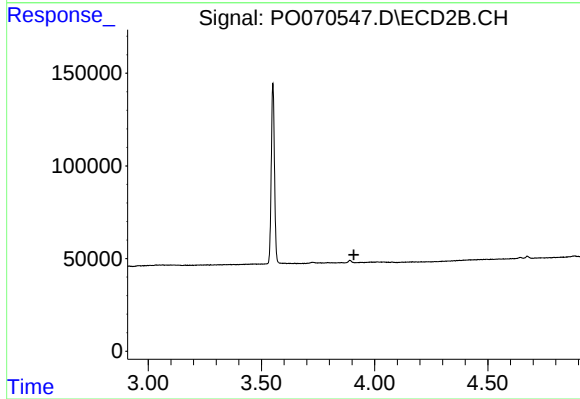


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.908 min
Response: 0
Conc: N.D.

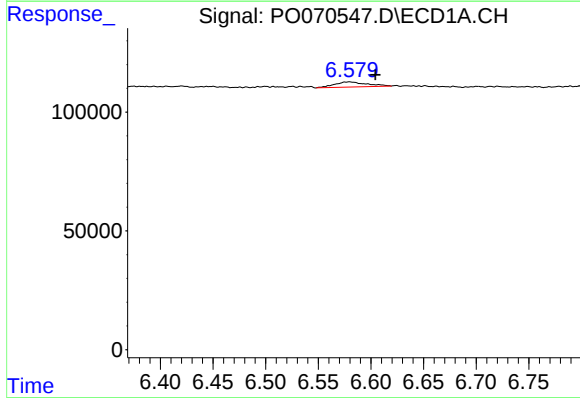


#24 AR-1248-4

R.T.: 6.580 min
Delta R.T.: -0.025 min
Response: 45935
Conc: 13.50 ng/ml

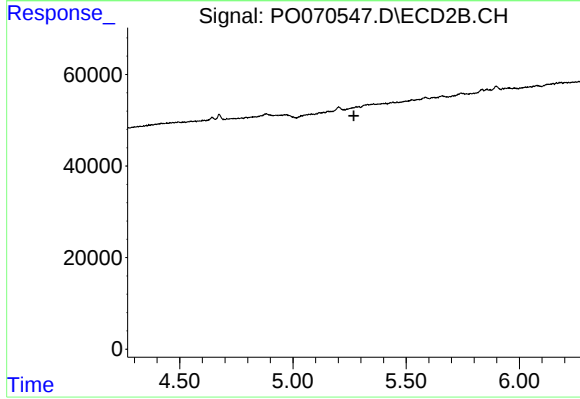

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.269 min
Response: 0
Conc: N.D.

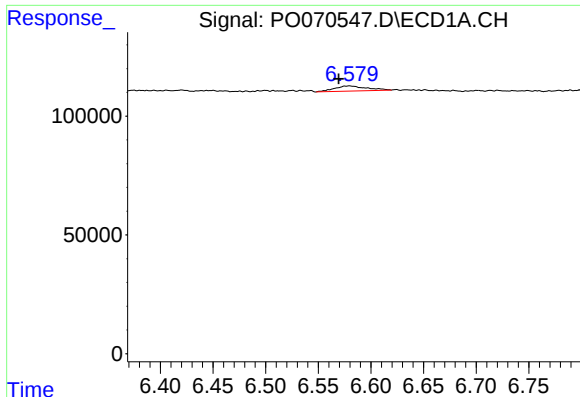

#26 AR-1254-1


R.T.: 6.580 min
Delta R.T.: 0.010 min
Response: 45935
Conc: 12.91 ng/ml

Instrument :
ECD_O
ClientSampleId :

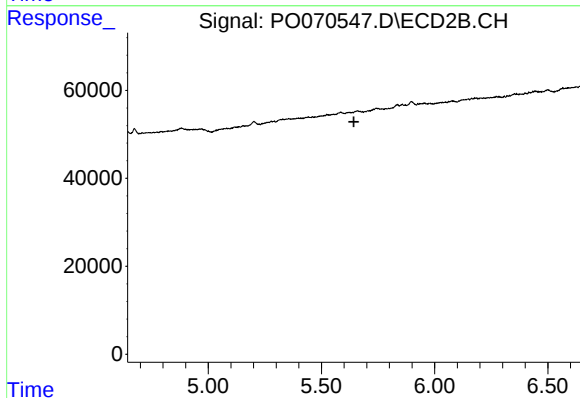


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.644 min
Response: 0
Conc: N.D.

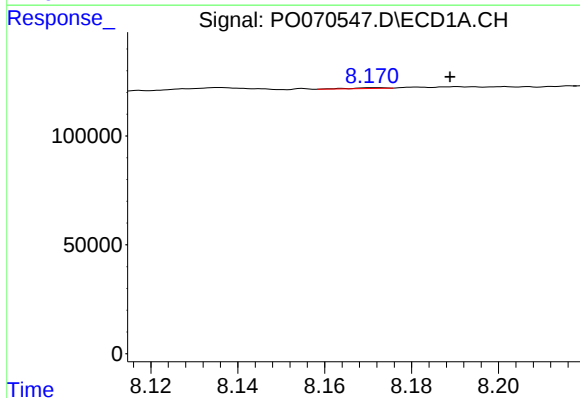


#34 AR-1260-4

R.T.: 8.171 min
Delta R.T.: -0.018 min
Response: 1998
Conc: 0.41 ng/ml

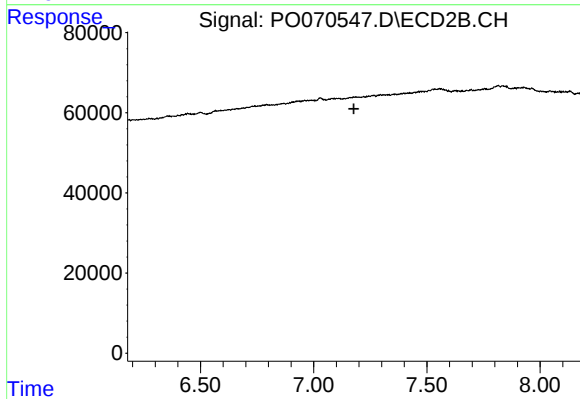

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.177 min
Response: 0
Conc: N.D.

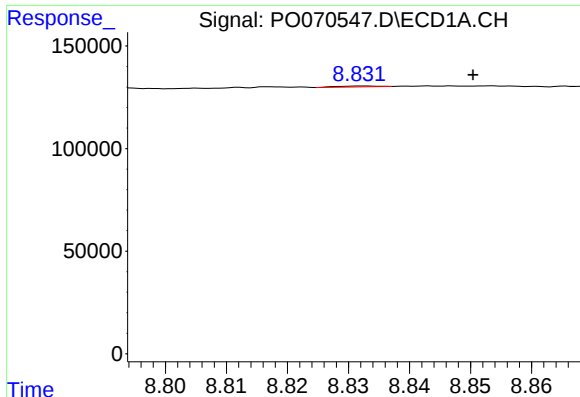

#39 AR-1262-4


R.T.: 8.833 min
Delta R.T.: -0.018 min
Response: 1778
Conc: 0.56 ng/ml

Instrument :
ECD_O
ClientSampleId :

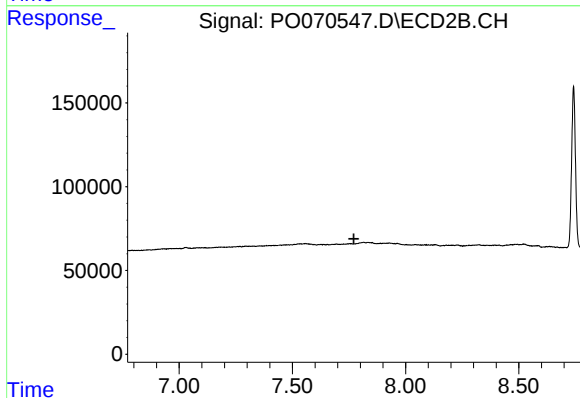


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.772 min
Response: 0
Conc: N.D.

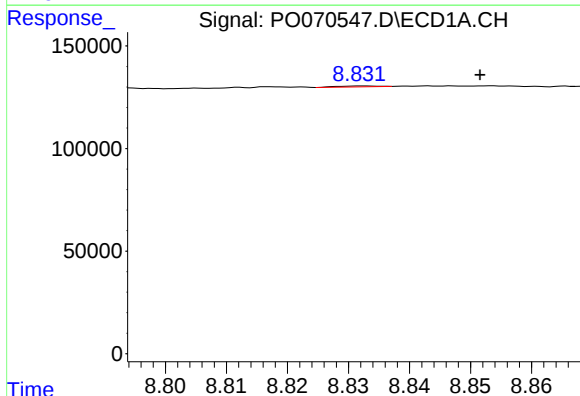


#42 AR-1268-2

R.T.: 8.833 min
Delta R.T.: -0.019 min
Response: 1778
Conc: 0.13 ng/ml

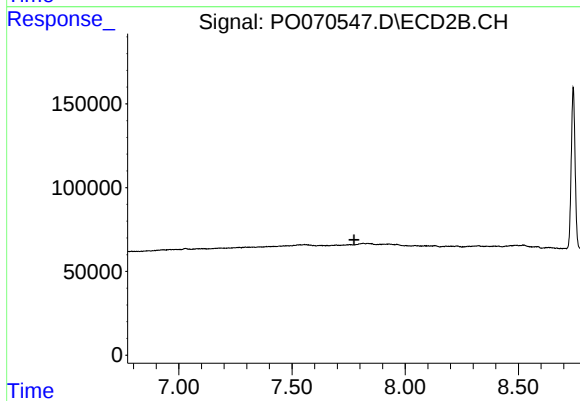

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 7.774 min
Response: 0
Conc: N.D.

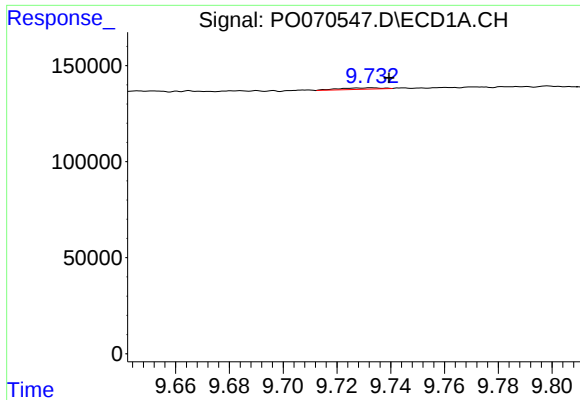

#45 AR-1268-5

R.T.: 9.733 min
Delta R.T.: -0.007 min
Response: 7962
Conc: 0.25 ng/ml

Instrument :
ECD_O
ClientSampleId :

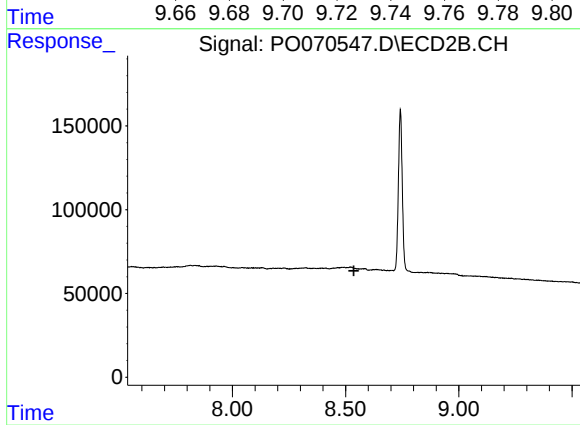

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.536 min
Response: 0
Conc: N.D.