

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081321\
 Data File : P0080420.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2021 11:25
 Operator : DD\AJ
 Sample : M3386-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRANSFO-MAIN-(21-04881)

Manual Integrations
 APPROVED

mohammad
 8/17/2021 11:43:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:58:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.002	4.123	1024854	537731	14.800m	21.575m#
2) SA Decachlor...	11.100	9.512	878554	386367	16.973	17.035

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081321\
Data File : PO080420.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2021 11:25
Operator : DD\AJ
Sample : M3386-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TRANSFO-MAIN-(21-04881)


Manual Integrations
APPROVED

mohammad
8/17/2021 11:43:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:58:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

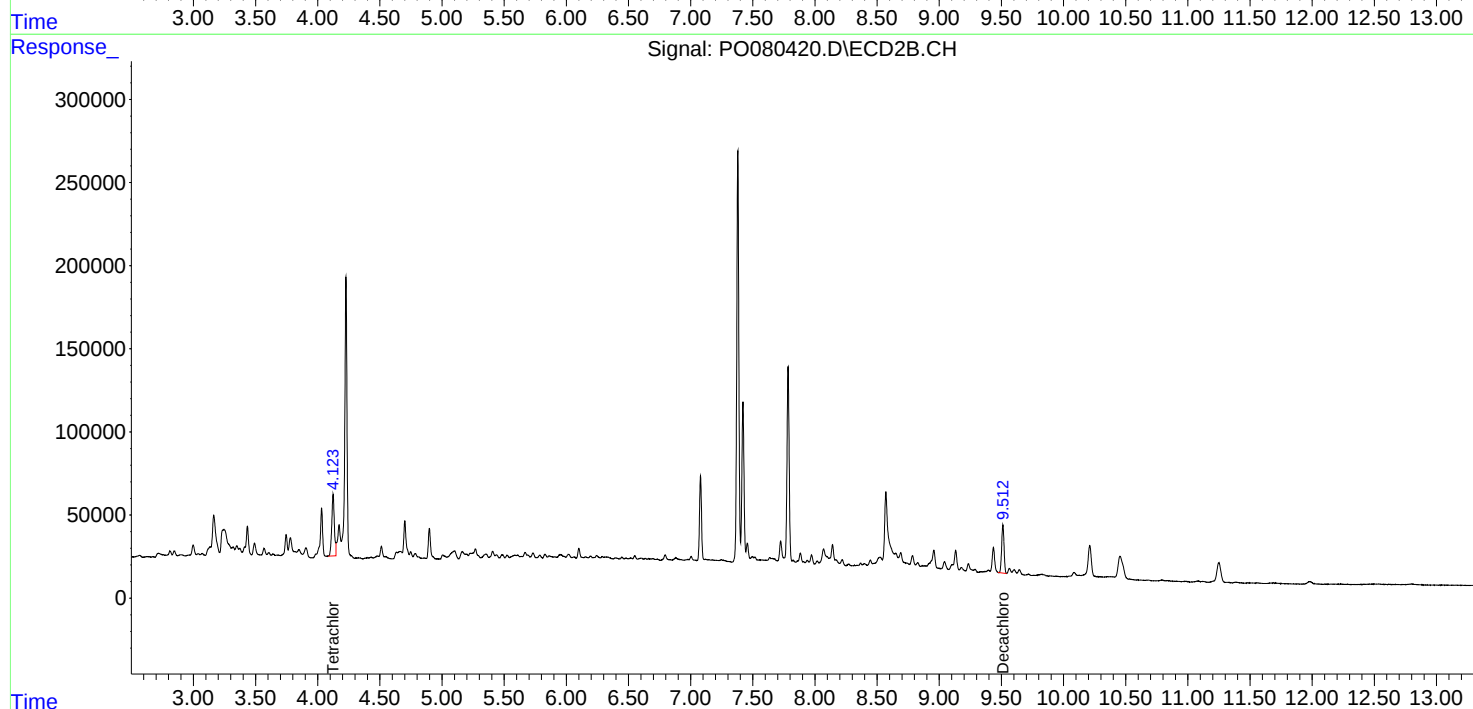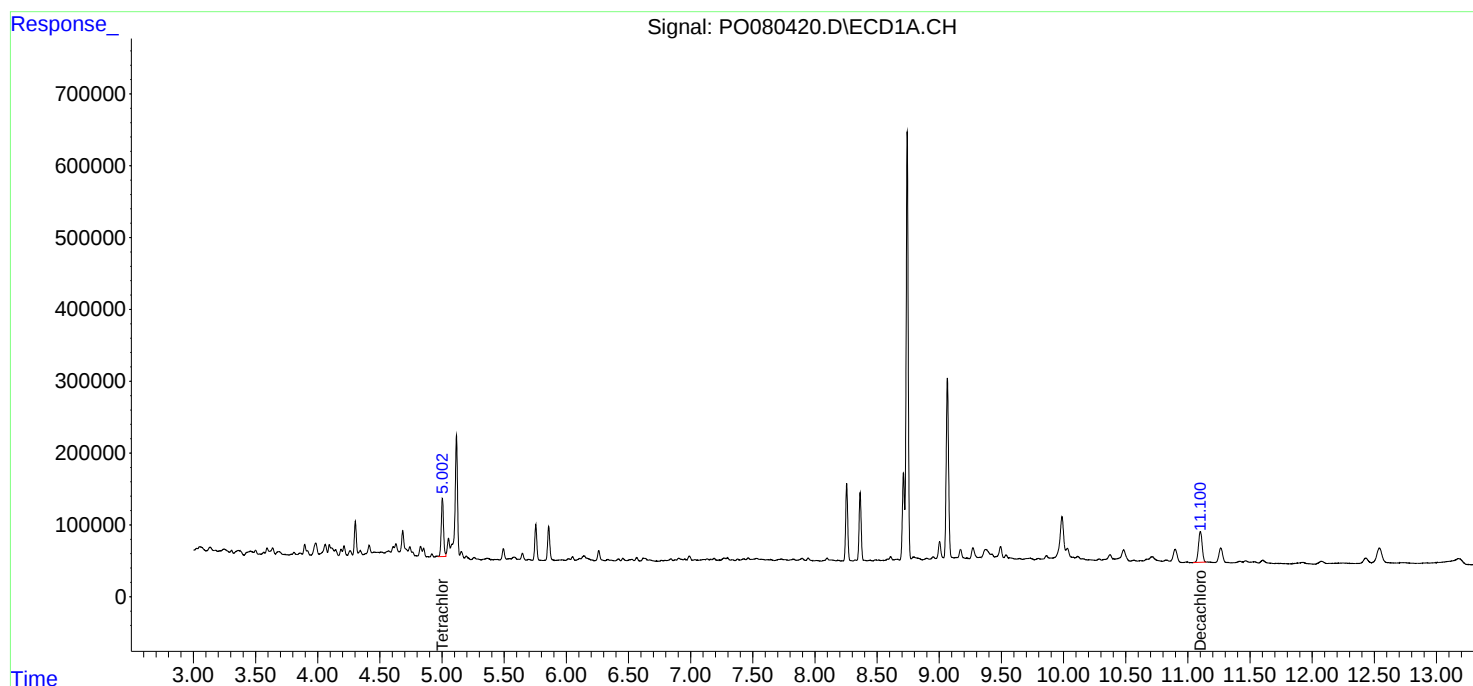

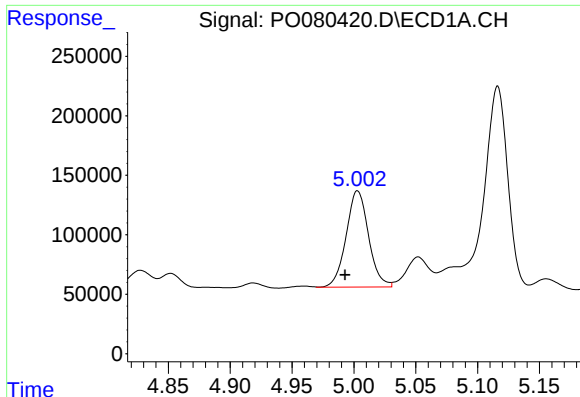


#1 Tetrachloro-m-xylene

R.T.: 5.002 min
Delta R.T.: 0.009 min
Response: 1024854
Conc: 14.80 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TRANSFO-MAIN-(21-04881)


Manual Integrations
APPROVED

mohammad
8/17/2021 11:43:49 AM

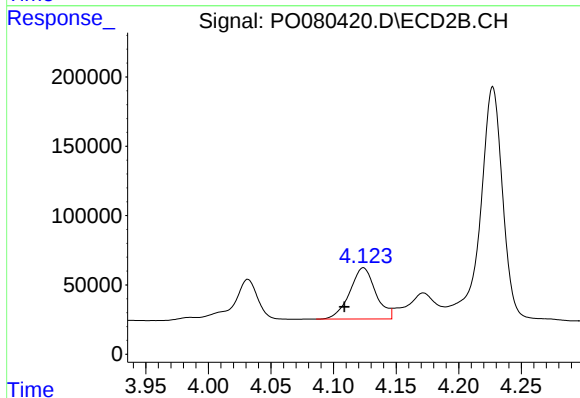


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.015 min
Response: 537731
Conc: 21.58 ng/ml m

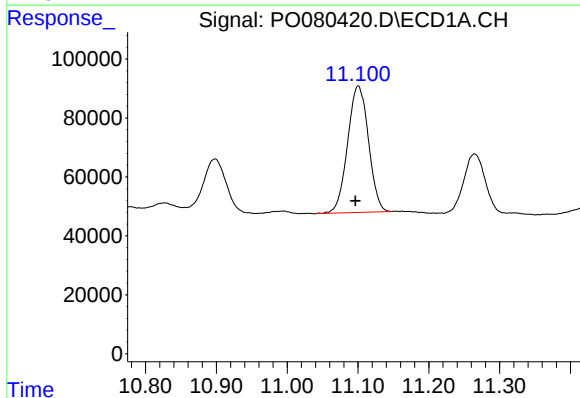

#2 Decachlorobiphenyl

R.T.: 11.100 min
Delta R.T.: 0.004 min
Response: 878554
Conc: 16.97 ng/ml

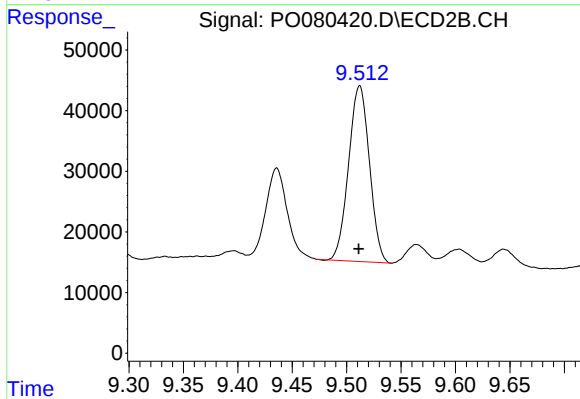

#2 Decachlorobiphenyl

R.T.: 9.512 min
Delta R.T.: 0.000 min
Response: 386367
Conc: 17.03 ng/ml