

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081321\
 Data File : P0080421.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2021 11:42
 Operator : DD\AJ
 Sample : M3384-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MAIN-BODY-(21-04881)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:54:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.003	4.122	895301	402624	12.929	16.154
2) SA Decachlor...	11.102	9.512	804786	375783	15.548	16.568

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081321\
Data File : P0080421.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2021 11:42
Operator : DD\AJ
Sample : M3384-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MAIN-BODY-(21-04881)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:54:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

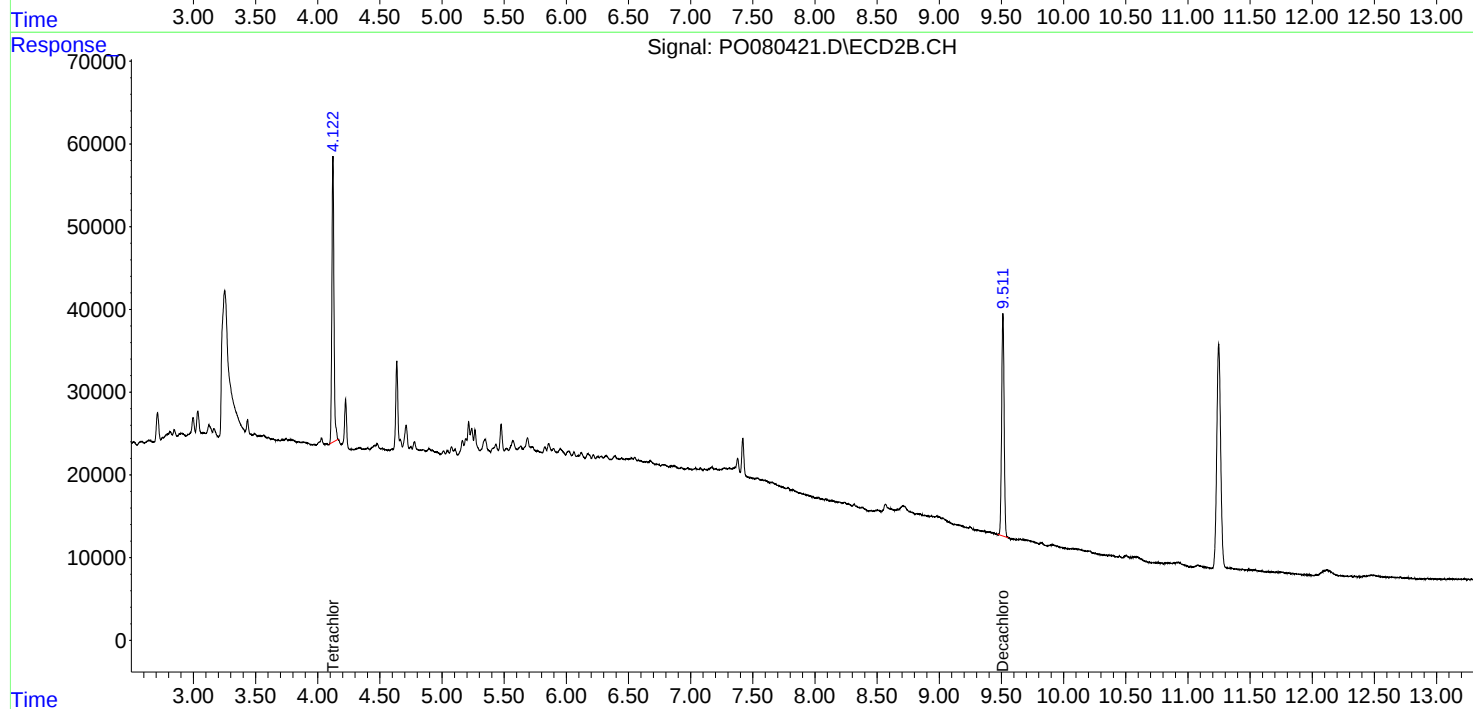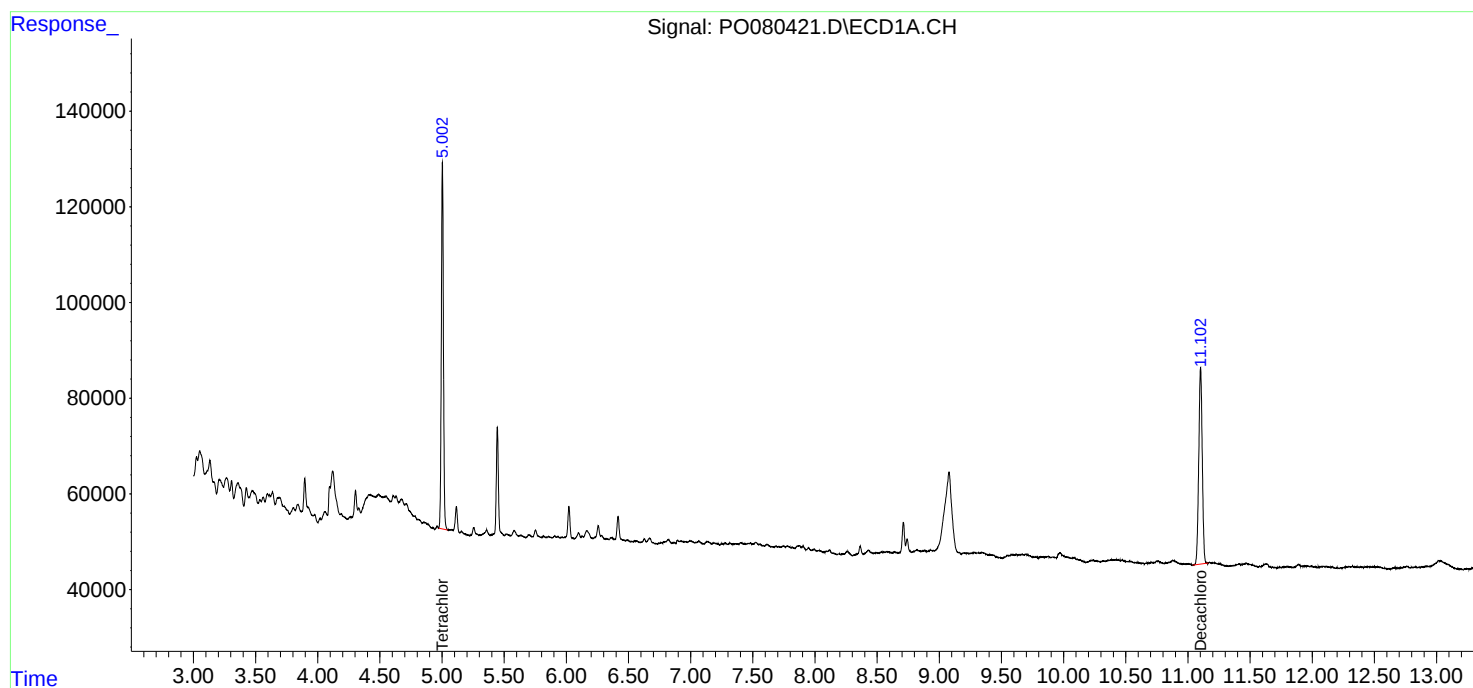


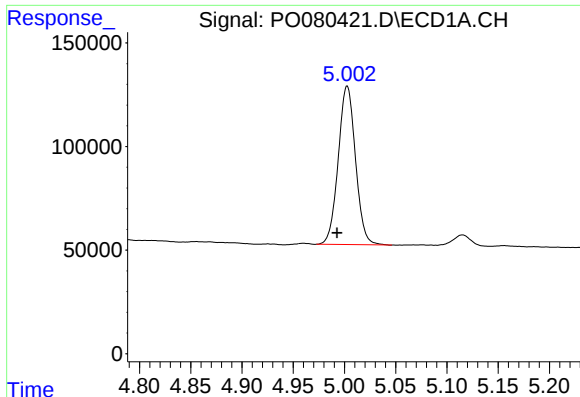

#1 Tetrachloro-m-xylene


R.T.: 5.003 min
Delta R.T.: 0.010 min
Response: 895301
Conc: 12.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MAIN-BODY-(21-04881)

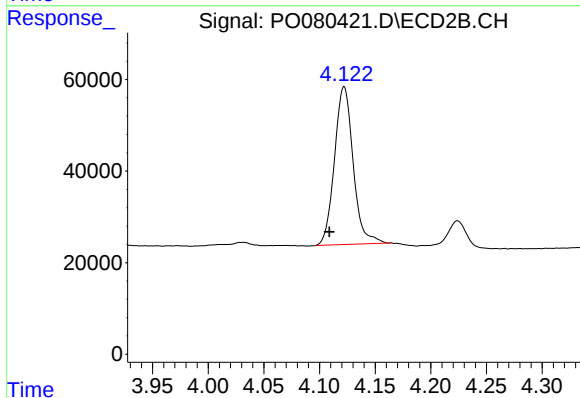


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: 0.013 min
Response: 402624
Conc: 16.15 ng/ml

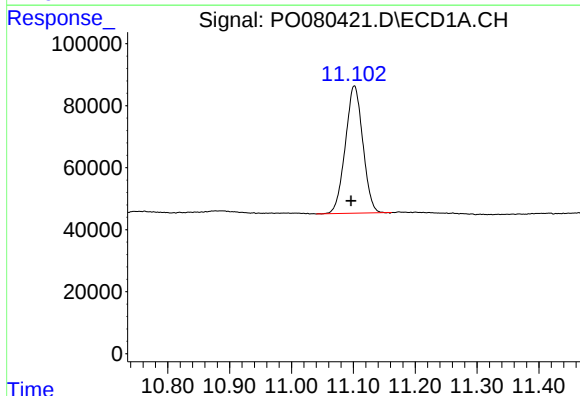

#2 Decachlorobiphenyl

R.T.: 11.102 min
Delta R.T.: 0.005 min
Response: 804786
Conc: 15.55 ng/ml

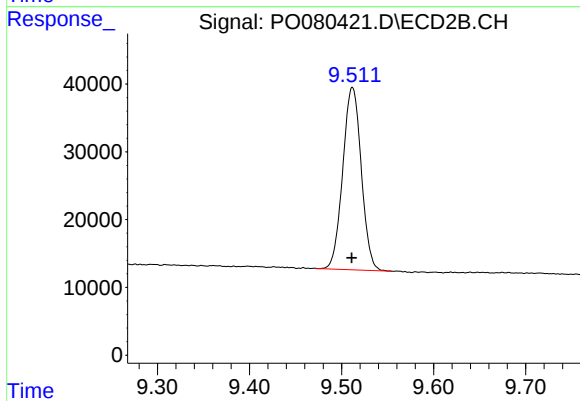

#2 Decachlorobiphenyl

R.T.: 9.512 min
Delta R.T.: 0.000 min
Response: 375783
Conc: 16.57 ng/ml