

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081321\
 Data File : P0080427.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2021 13:26
 Operator : DD\AJ
 Sample : M3386-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRANSFO-CAP-(21-04881)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:58:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.001	4.122	914228	402776	13.203	16.160
2) SA Decachlor...	11.099	9.510	916817	407257	17.712	17.956

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081321\
Data File : P0080427.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2021 13:26
Operator : DD\AJ
Sample : M3386-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TRANSFO-CAP-(21-04881)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:58:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

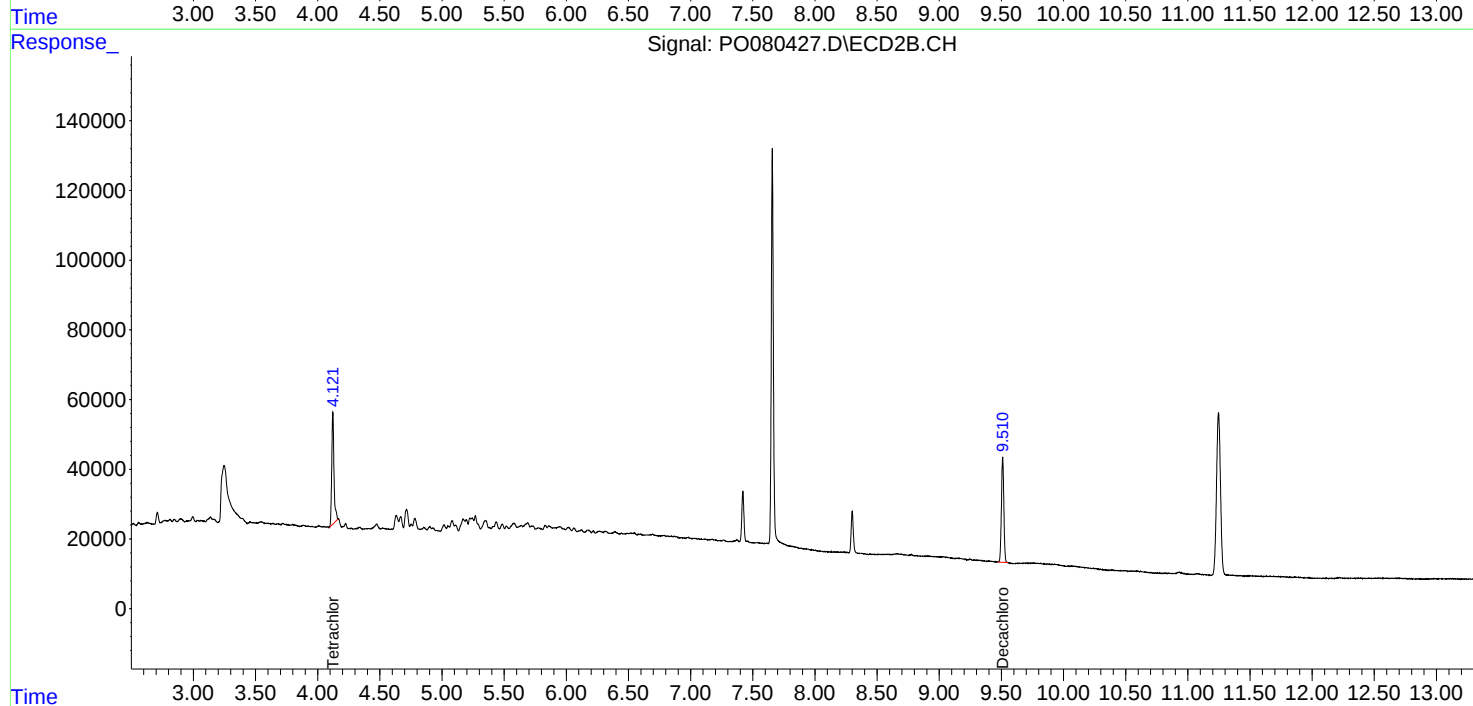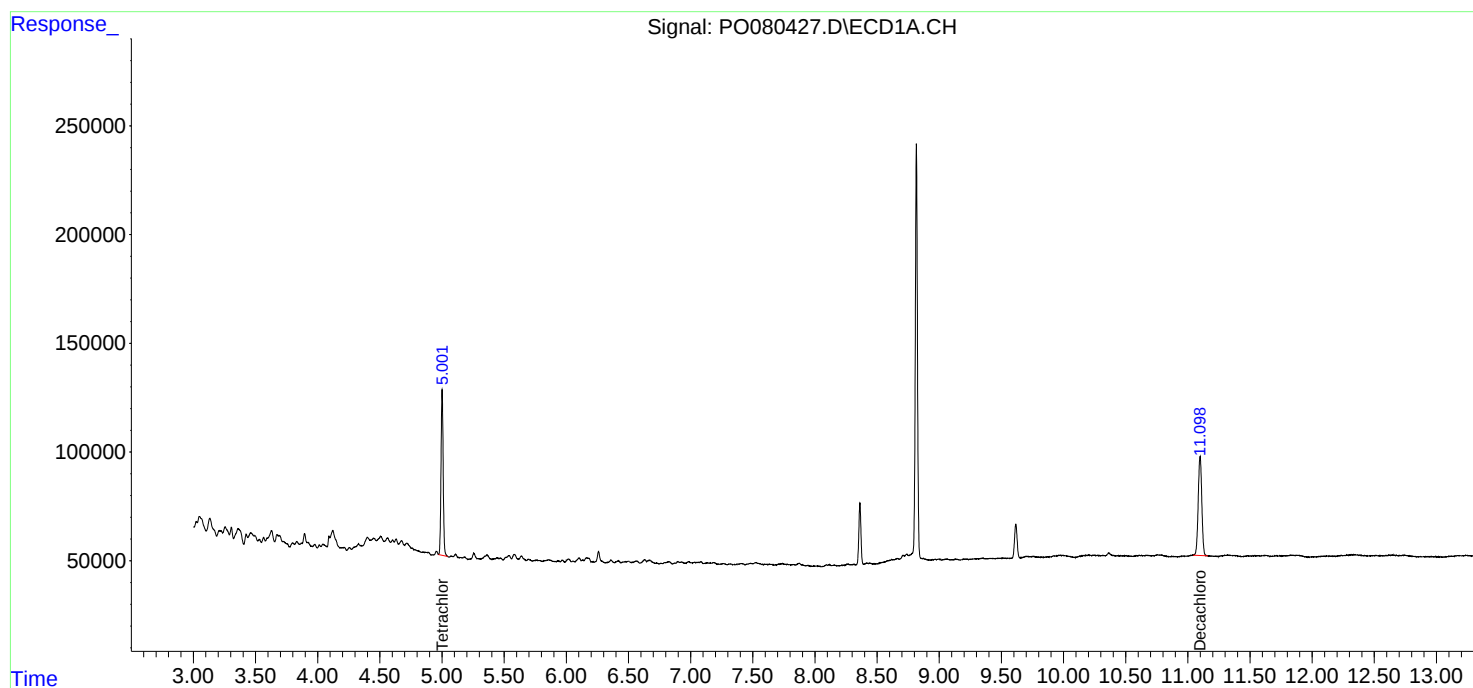


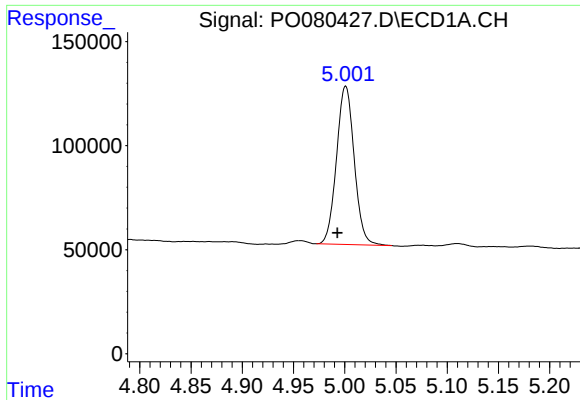

#1 Tetrachloro-m-xylene


R.T.: 5.001 min
Delta R.T.: 0.008 min
Response: 914228
Conc: 13.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRANSFO-CAP-(21-04881)

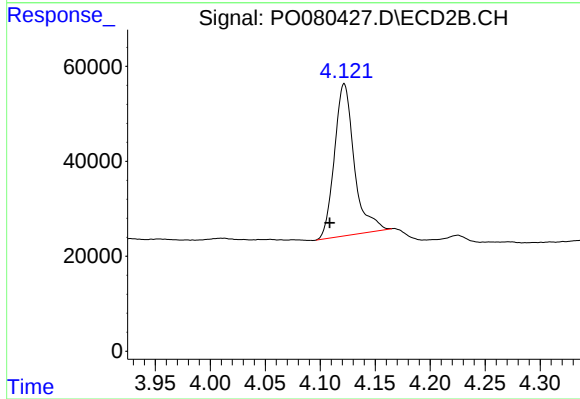


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: 0.013 min
Response: 402776
Conc: 16.16 ng/ml

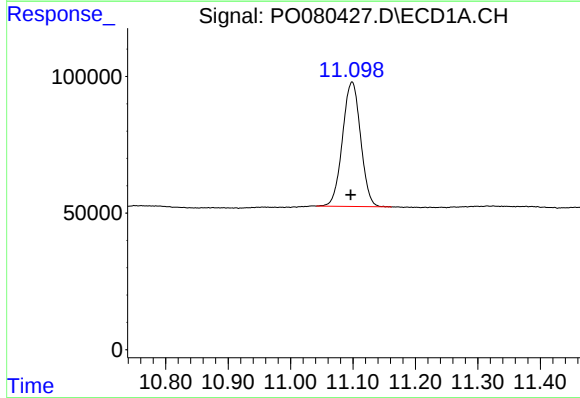

#2 Decachlorobiphenyl

R.T.: 11.099 min
Delta R.T.: 0.002 min
Response: 916817
Conc: 17.71 ng/ml

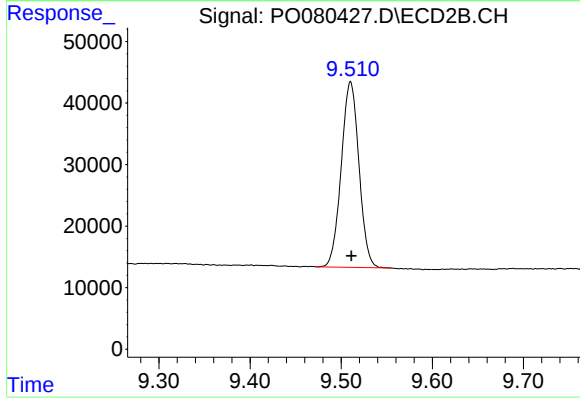

#2 Decachlorobiphenyl

R.T.: 9.510 min
Delta R.T.: 0.000 min
Response: 407257
Conc: 17.96 ng/ml