

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081324\
 Data File : P0105490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 11:58
 Operator : YP/AJ
 Sample : P3390-09
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:04:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.426	3.535	93859881	42072304	10.746	13.395
2)	SA Decachlor...	10.216	8.425	72988554	26788745	12.688	15.132
Target Compounds							
3)	L1 AR-1016-1	5.597	4.589	4641863	2177068	15.345	19.372 #
4)	L1 AR-1016-2	5.620	4.607	6743249	2902639	15.774	18.644
5)	L1 AR-1016-3	5.683	4.779	4063882	1488575	15.838	17.775
6)	L1 AR-1016-4	5.782	4.821	4707896	1284065	21.526	19.069
7)	L1 AR-1016-5	6.078	5.029	3950074	1721757	18.462	20.573
8)	L2 AR-1221-1	4.631	3.742	993976	209522	8.864	5.308 #
9)	L2 AR-1221-2	4.732	3.826	2811201	1071747	33.166	34.885
10)	L2 AR-1221-3	4.796	3.899	3414868	1235231	14.037	13.804
11)	L3 AR-1232-1	4.796	3.899	3414868	1235231	17.080	16.914
12)	L3 AR-1232-2	5.327	4.607	3393713	2902639	32.061	41.340 #
13)	L3 AR-1232-3	5.620	4.779	6743249	1488575	35.230	38.950
14)	L3 AR-1232-4	5.782	4.861	4707896	1664128	48.269	47.834
15)	L3 AR-1232-5	5.873	5.029	2671505	1721757	37.072	48.777 #
16)	L4 AR-1242-1	5.597	4.589	4641863	2177068	19.973	24.683
17)	L4 AR-1242-2	5.620	4.607	6743249	2902639	20.691	24.447
18)	L4 AR-1242-3	5.683	4.779	4063882	1488575	20.600	22.924
19)	L4 AR-1242-4	5.782	4.861	4707896	1664128	27.593	25.092
20)	L4 AR-1242-5	6.527	5.374	2553647	1833668	14.612	22.315 #
21)	L5 AR-1248-1	5.597	4.589	4641863	2177068	25.421	31.171
22)	L5 AR-1248-2	5.873	4.821	2671505	1284065	10.607	13.531 #
23)	L5 AR-1248-3	6.078	4.861	3950074	1664128	13.974	16.671
24)	L5 AR-1248-4	6.485	5.029	2150438	1721757	6.725	15.254 #
25)	L5 AR-1248-5	6.527	5.412	2553647	507244	8.256	4.505 #
26)	L6 AR-1254-1	6.459	5.374	5146284	1833668	16.411	11.263 #
27)	L6 AR-1254-2	6.678	5.519	2476044	1443819	5.487	9.870 #
28)	L6 AR-1254-3	7.051	5.931	3053164	2472564	6.436	10.961 #
29)	L6 AR-1254-4	7.334	6.141	3012147	580507	8.409	4.114 #
30)	L6 AR-1254-5	7.756	6.551	13455888	4133188	33.897	20.630 #
31)	L7 AR-1260-1	7.214	6.044	6221777	4026567	16.975	25.795 #
32)	L7 AR-1260-2	7.472	6.229	8900667	4495200	21.377	23.784
33)	L7 AR-1260-3	7.835	6.380	8959973	6405767	34.619	34.676
34)	L7 AR-1260-4	8.063	6.845	14597379	3068484	44.244	25.104 #
35)	L7 AR-1260-5	8.385	7.085	15248961	6583103	25.634	23.653
36)	L8 AR-1262-1	7.756	6.551	13455888	4133188	42.363	38.845
37)	L8 AR-1262-2	8.385	6.845	15248961	3068484	20.273	18.058
38)	L8 AR-1262-3	8.714	7.365	6856228	1949939	13.933	15.445
39)	L8 AR-1262-4	8.779	7.427	2561970	4633549	6.977	20.016 #
40)	L8 AR-1262-5	9.452	7.917	2102440	1514323	7.850	15.068 #
41)	L9 AR-1268-1	8.714	7.365	6856228	1949939	8.430	5.585 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081324\
Data File : P0105490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 11:58
Operator : YP/AJ
Sample : P3390-09
Misc : AR1660 MDL 25 PPB
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:04:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.779	7.427	2561970	4633549	3.524	14.852 #
43)	L9 AR-1268-3	9.036	7.631	200083	782331	0.310	3.095 #
44)	L9 AR-1268-4	9.452	7.917	2102440	1514323	7.551	14.080 #
45)	L9 AR-1268-5	9.871	8.189	1988550	577068	0.951	0.863


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

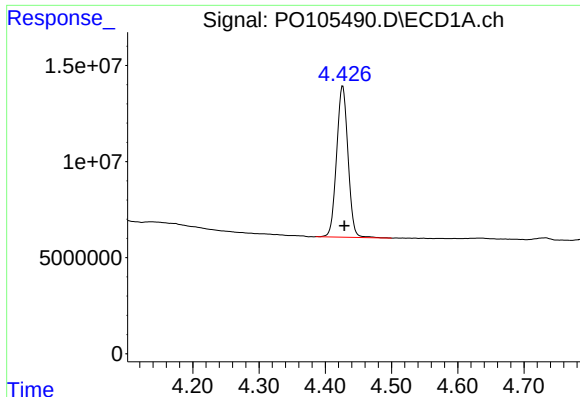

#1 Tetrachloro-m-xylene


R.T.: 4.426 min
Delta R.T.: -0.003 min
Response: 93859881
Conc: 10.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

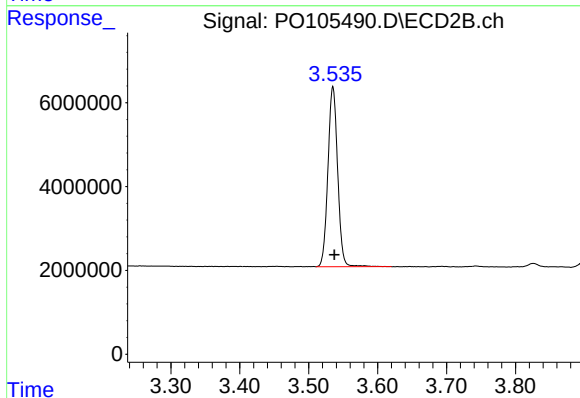


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.002 min
Response: 42072304
Conc: 13.39 ng/ml

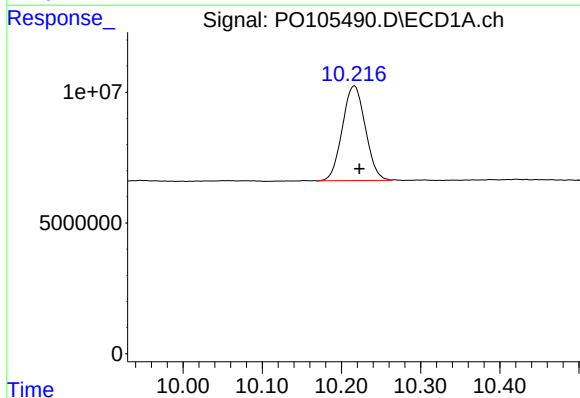


#2 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.006 min
Response: 72988554
Conc: 12.69 ng/ml

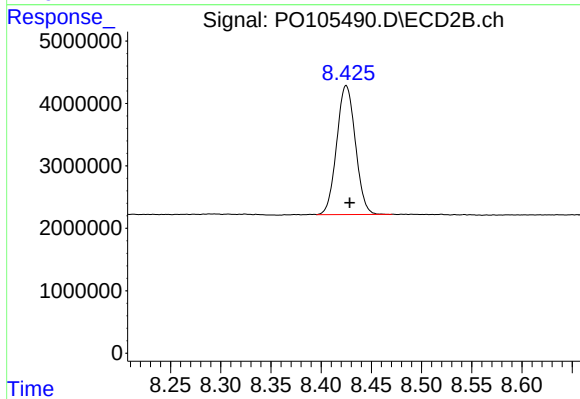

#2 Decachlorobiphenyl


R.T.: 8.425 min
Delta R.T.: -0.003 min
Response: 26788745
Conc: 15.13 ng/ml

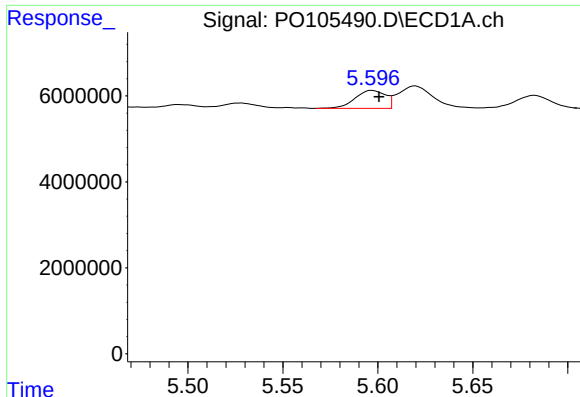

#3 AR-1016-1


R.T.: 5.597 min
Delta R.T.: -0.004 min
Response: 4641863
Conc: 15.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

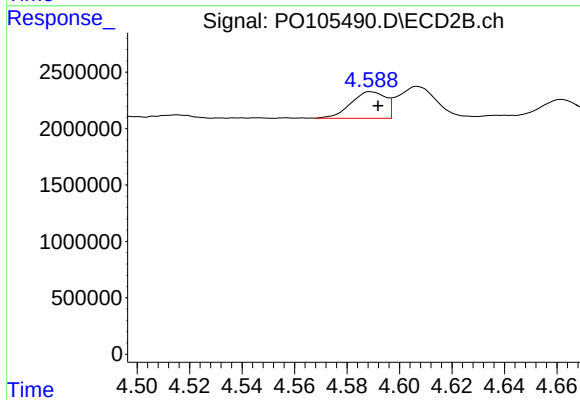


#3 AR-1016-1

R.T.: 4.589 min
Delta R.T.: -0.003 min
Response: 2177068
Conc: 19.37 ng/ml

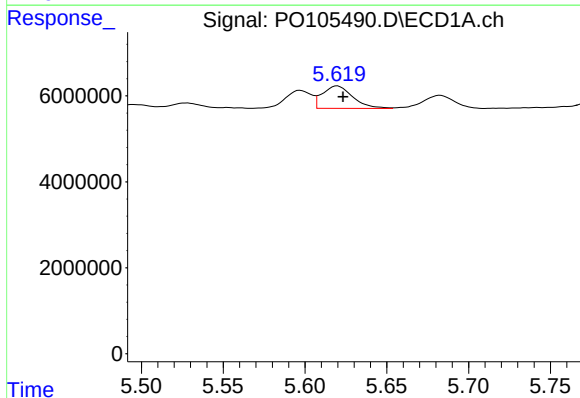


#4 AR-1016-2

R.T.: 5.620 min
Delta R.T.: -0.004 min
Response: 6743249
Conc: 15.77 ng/ml

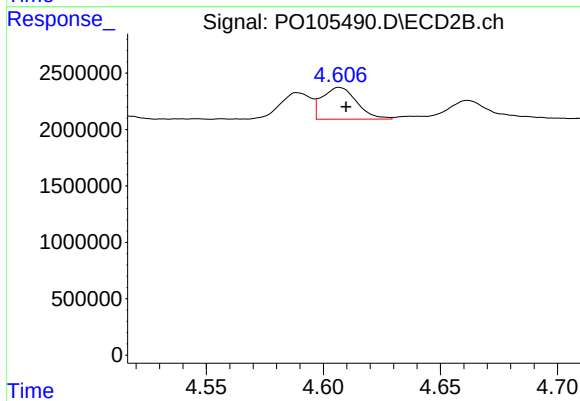

#4 AR-1016-2


R.T.: 4.607 min
Delta R.T.: -0.003 min
Response: 2902639
Conc: 18.64 ng/ml

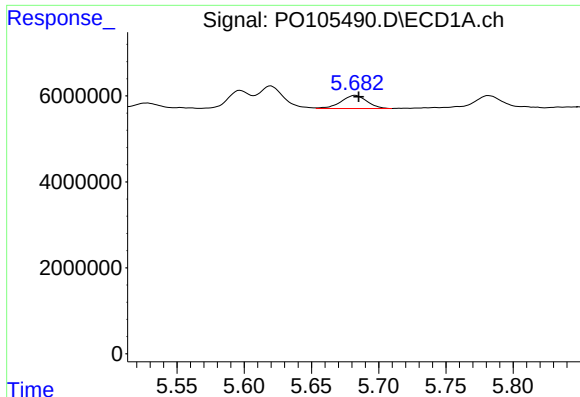

#5 AR-1016-3


R.T.: 5.683 min
Delta R.T.: -0.003 min
Response: 4063882
Conc: 15.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

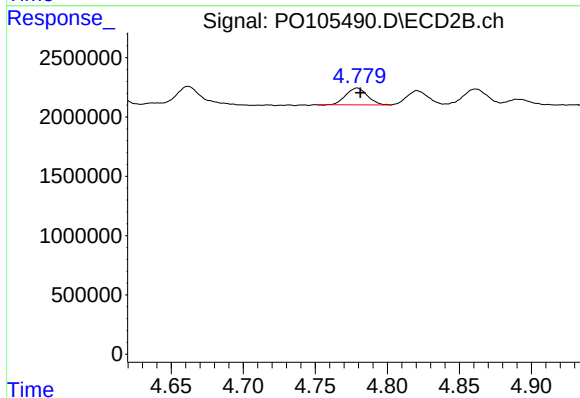


#5 AR-1016-3

R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 1488575
Conc: 17.77 ng/ml

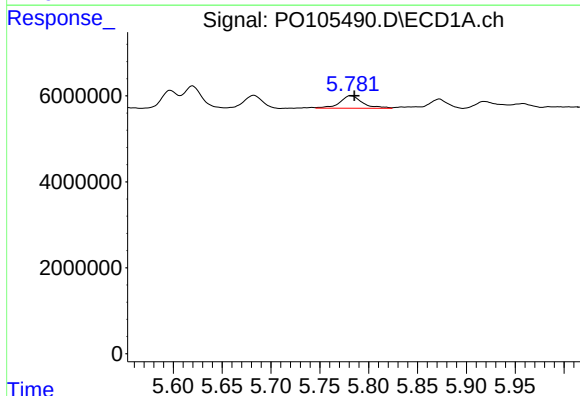


#6 AR-1016-4

R.T.: 5.782 min
Delta R.T.: -0.004 min
Response: 4707896
Conc: 21.53 ng/ml

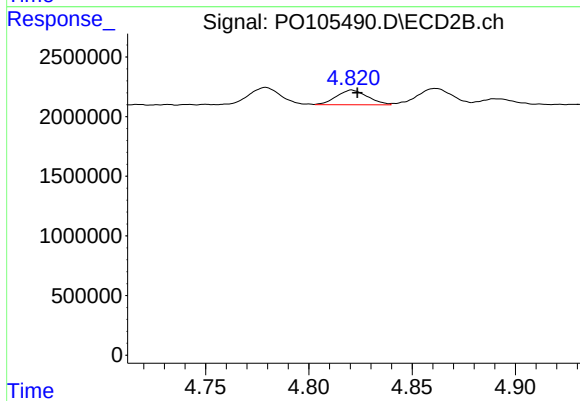

#6 AR-1016-4


R.T.: 4.821 min
Delta R.T.: -0.003 min
Response: 1284065
Conc: 19.07 ng/ml

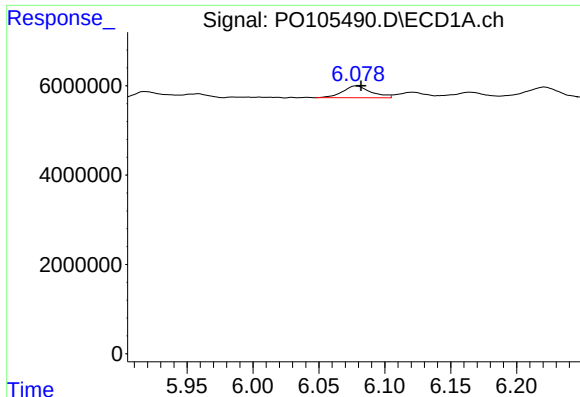

#7 AR-1016-5


R.T.: 6.078 min
Delta R.T.: -0.004 min
Response: 3950074
Conc: 18.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

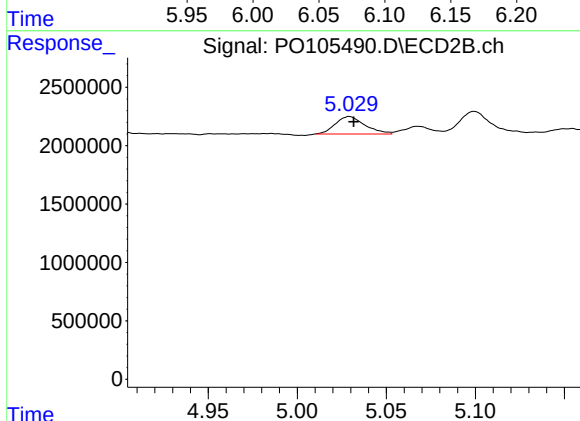


#7 AR-1016-5

R.T.: 5.029 min
Delta R.T.: -0.003 min
Response: 1721757
Conc: 20.57 ng/ml

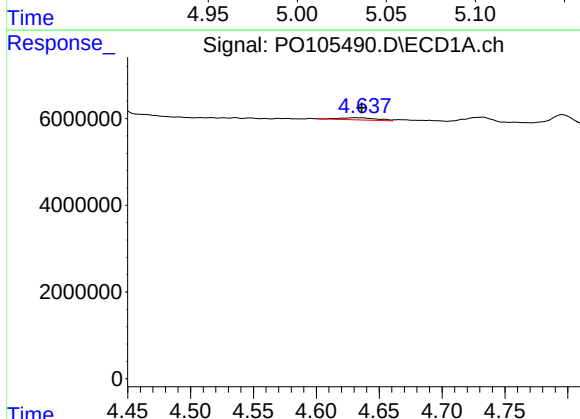


#8 AR-1221-1

R.T.: 4.631 min
Delta R.T.: -0.005 min
Response: 993976
Conc: 8.86 ng/ml

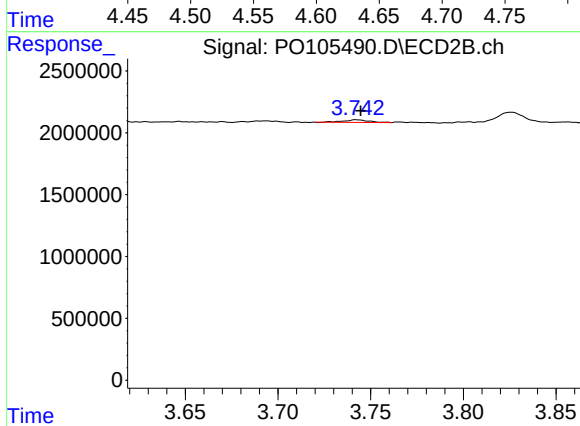

#8 AR-1221-1


R.T.: 3.742 min
Delta R.T.: -0.002 min
Response: 209522
Conc: 5.31 ng/ml

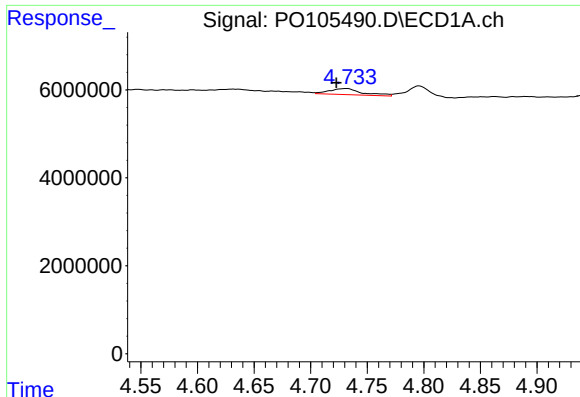

#9 AR-1221-2


R.T.: 4.732 min
Delta R.T.: 0.010 min
Response: 2811201
Conc: 33.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

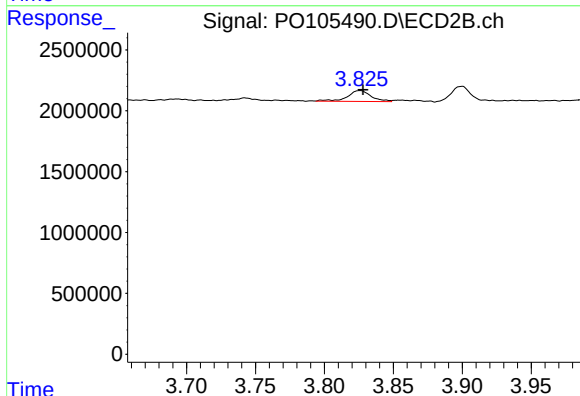


#9 AR-1221-2

R.T.: 3.826 min
Delta R.T.: -0.002 min
Response: 1071747
Conc: 34.88 ng/ml

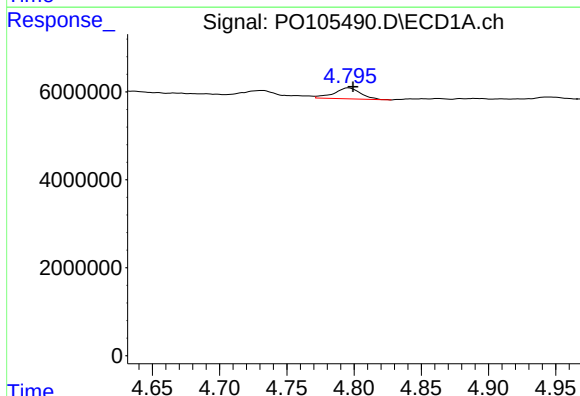


#10 AR-1221-3

R.T.: 4.796 min
Delta R.T.: -0.004 min
Response: 3414868
Conc: 14.04 ng/ml

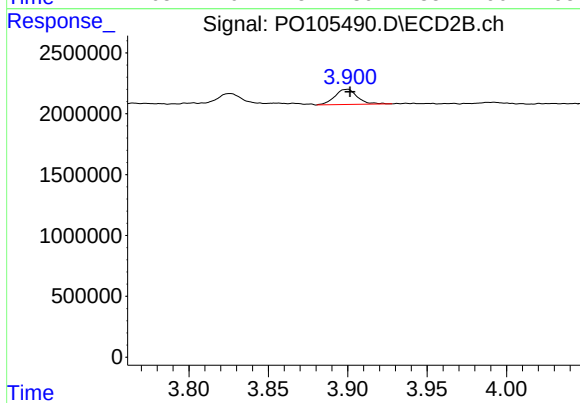

#10 AR-1221-3


R.T.: 3.899 min
Delta R.T.: -0.002 min
Response: 1235231
Conc: 13.80 ng/ml

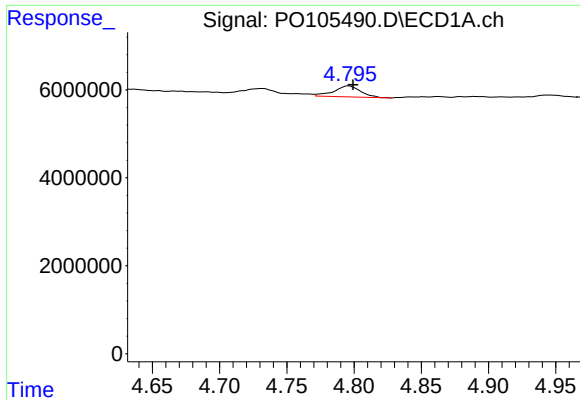

#11 AR-1232-1


R.T.: 4.796 min
Delta R.T.: -0.003 min
Response: 3414868
Conc: 17.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

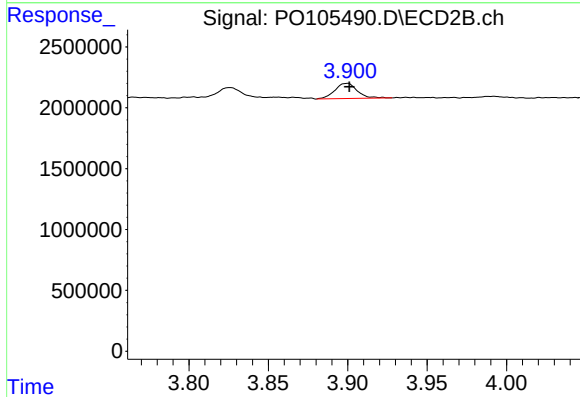


#11 AR-1232-1

R.T.: 3.899 min
Delta R.T.: -0.002 min
Response: 1235231
Conc: 16.91 ng/ml

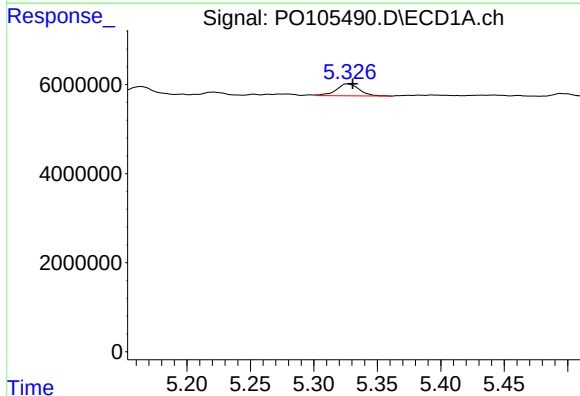


#12 AR-1232-2

R.T.: 5.327 min
Delta R.T.: -0.004 min
Response: 3393713
Conc: 32.06 ng/ml

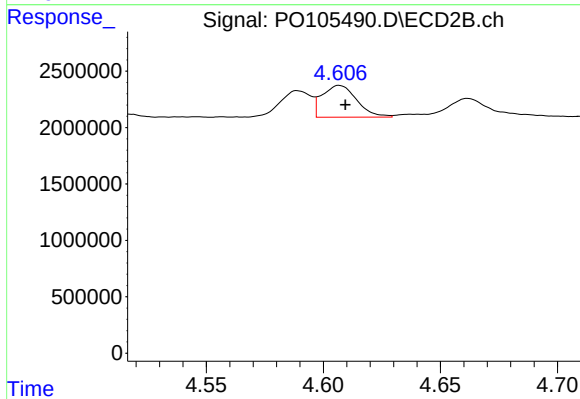

#12 AR-1232-2


R.T.: 4.607 min
Delta R.T.: -0.003 min
Response: 2902639
Conc: 41.34 ng/ml

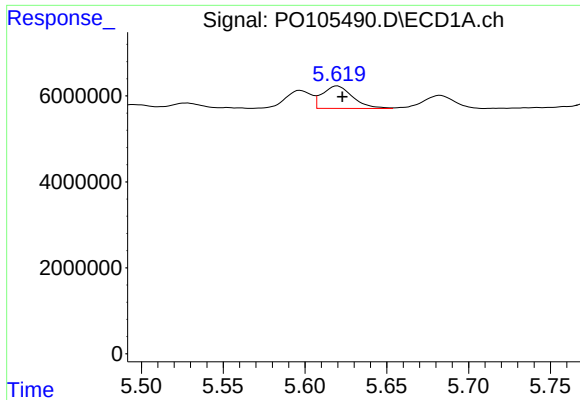

#13 AR-1232-3


R.T.: 5.620 min
Delta R.T.: -0.003 min
Response: 6743249
Conc: 35.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

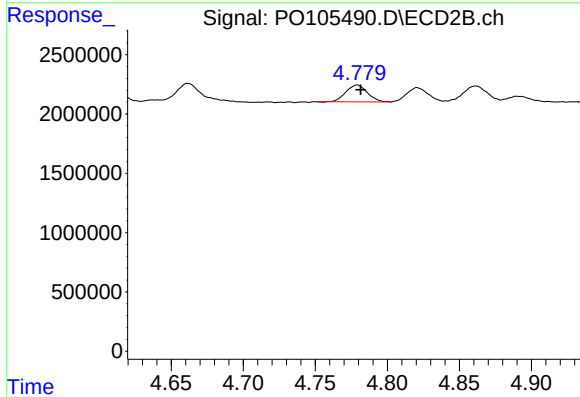


#13 AR-1232-3

R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 1488575
Conc: 38.95 ng/ml

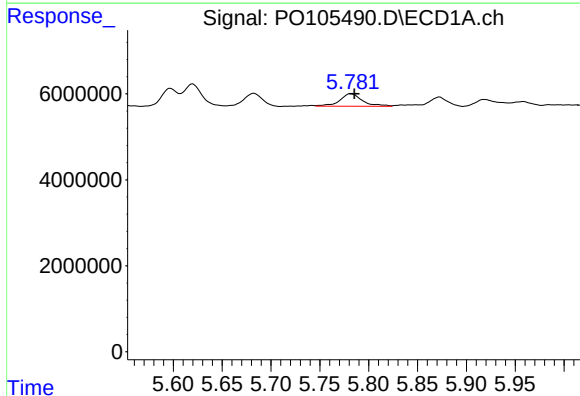


#14 AR-1232-4

R.T.: 5.782 min
Delta R.T.: -0.003 min
Response: 4707896
Conc: 48.27 ng/ml

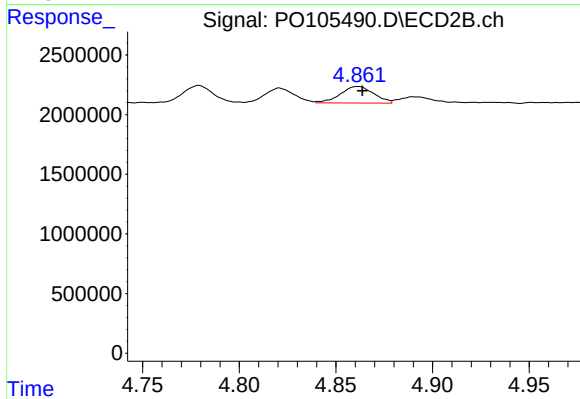

#14 AR-1232-4


R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 1664128
Conc: 47.83 ng/ml

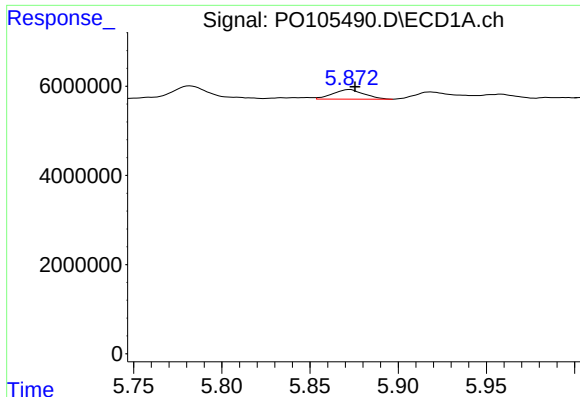

#15 AR-1232-5


R.T.: 5.873 min
Delta R.T.: -0.003 min
Response: 2671505
Conc: 37.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

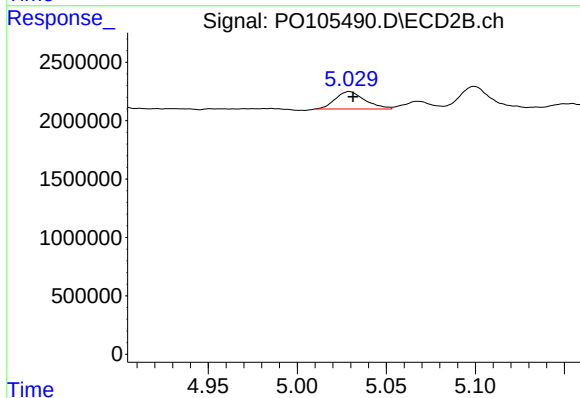


#15 AR-1232-5

R.T.: 5.029 min
Delta R.T.: -0.002 min
Response: 1721757
Conc: 48.78 ng/ml

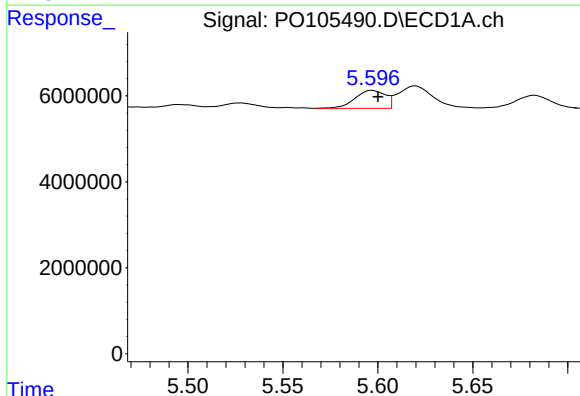


#16 AR-1242-1

R.T.: 5.597 min
Delta R.T.: -0.003 min
Response: 4641863
Conc: 19.97 ng/ml

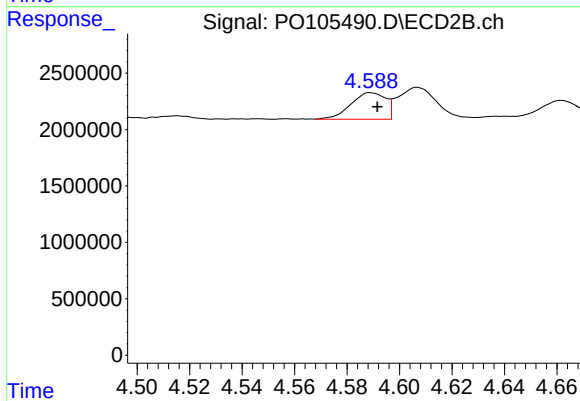

#16 AR-1242-1


R.T.: 4.589 min
Delta R.T.: -0.002 min
Response: 2177068
Conc: 24.68 ng/ml

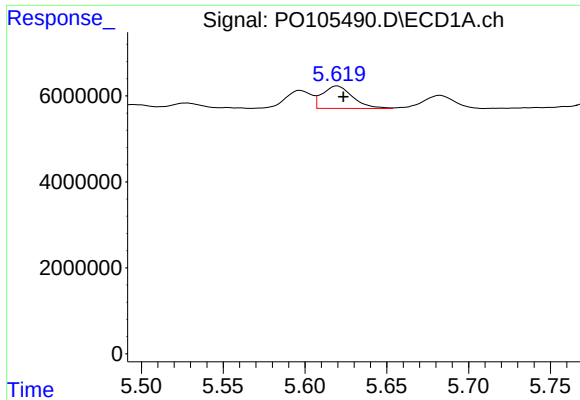

#17 AR-1242-2


R.T.: 5.620 min
Delta R.T.: -0.004 min
Response: 6743249
Conc: 20.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

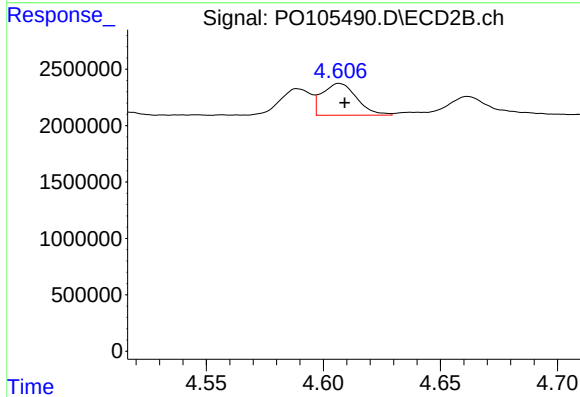


#17 AR-1242-2

R.T.: 4.607 min
Delta R.T.: -0.002 min
Response: 2902639
Conc: 24.45 ng/ml

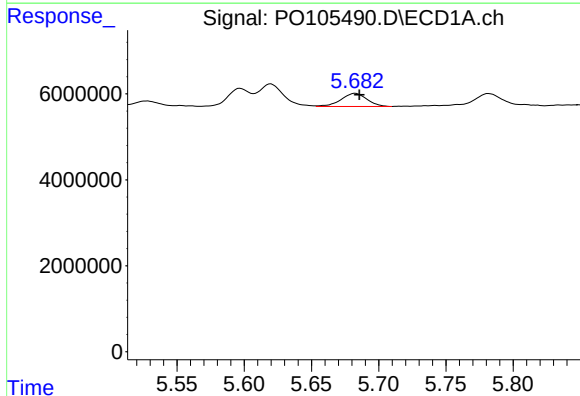


#18 AR-1242-3

R.T.: 5.683 min
Delta R.T.: -0.003 min
Response: 4063882
Conc: 20.60 ng/ml

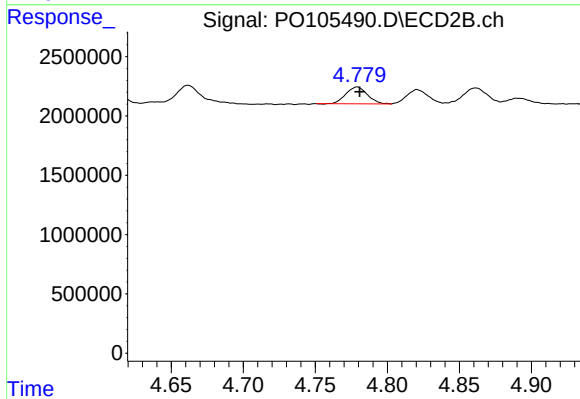

#18 AR-1242-3


R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 1488575
Conc: 22.92 ng/ml

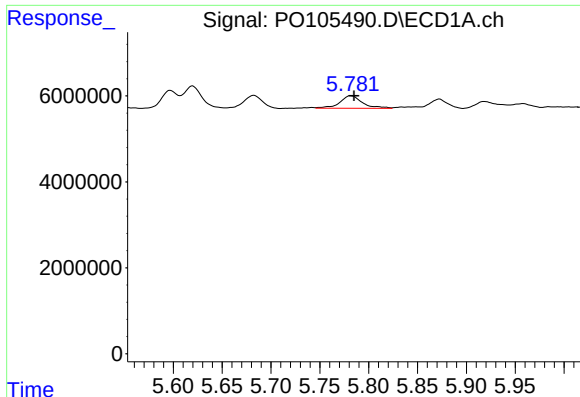

#19 AR-1242-4


R.T.: 5.782 min
Delta R.T.: -0.003 min
Response: 4707896
Conc: 27.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

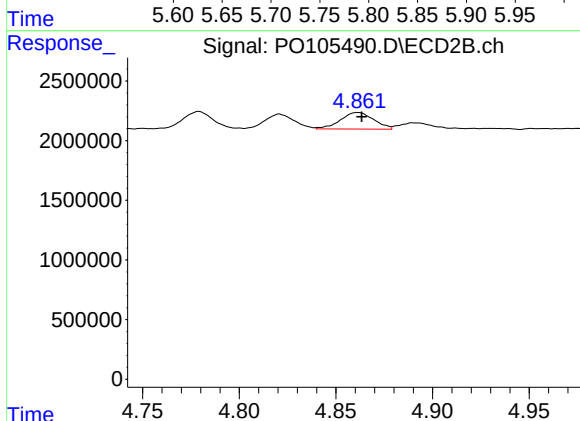


#19 AR-1242-4

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 1664128
Conc: 25.09 ng/ml

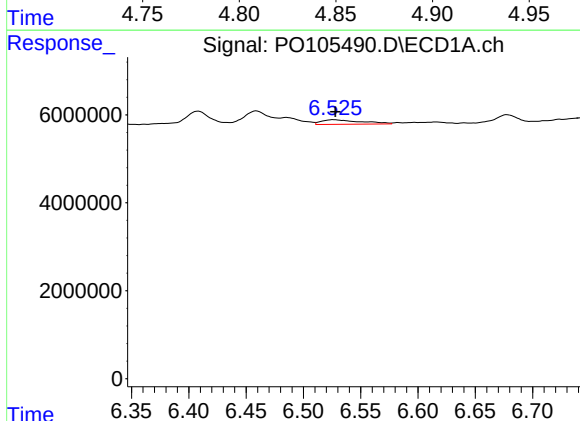


#20 AR-1242-5

R.T.: 6.527 min
Delta R.T.: -0.001 min
Response: 2553647
Conc: 14.61 ng/ml

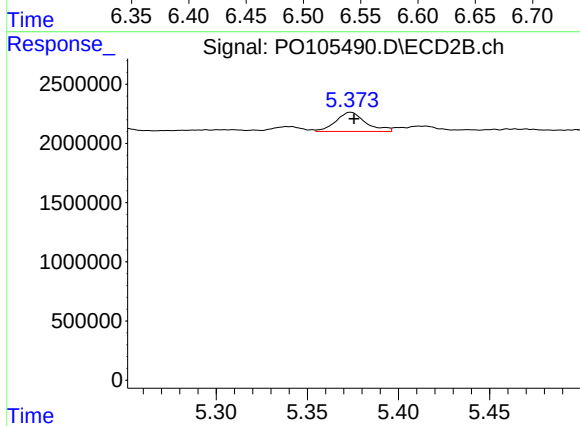

#20 AR-1242-5


R.T.: 5.374 min
Delta R.T.: -0.002 min
Response: 1833668
Conc: 22.31 ng/ml

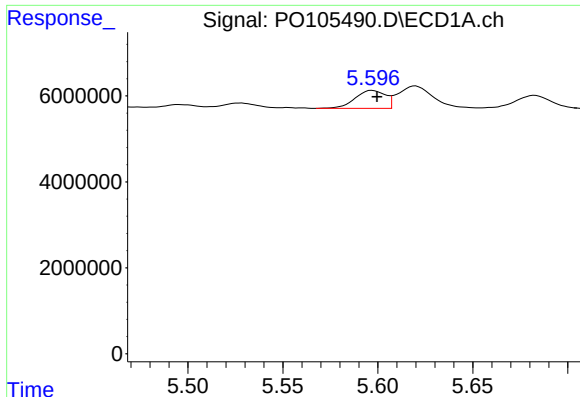

#21 AR-1248-1


R.T.: 5.597 min
Delta R.T.: -0.002 min
Response: 4641863
Conc: 25.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

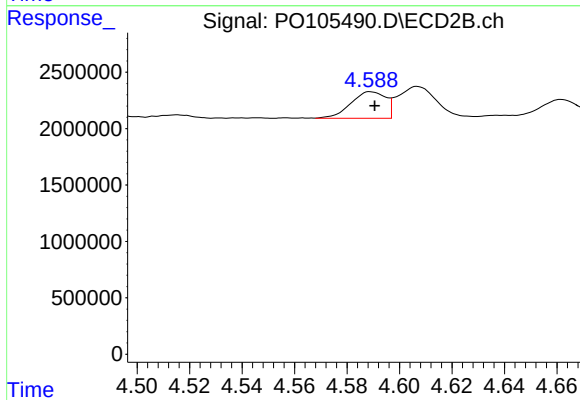


#21 AR-1248-1

R.T.: 4.589 min
Delta R.T.: -0.001 min
Response: 2177068
Conc: 31.17 ng/ml

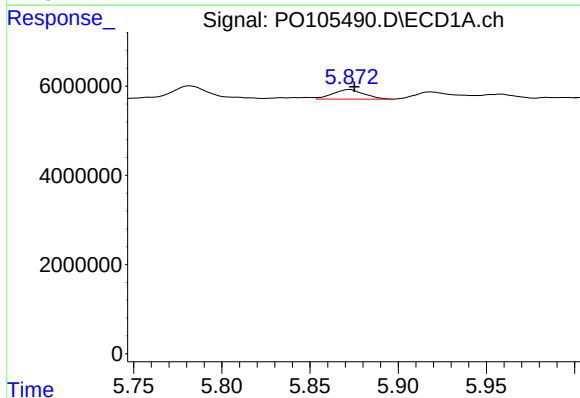


#22 AR-1248-2

R.T.: 5.873 min
Delta R.T.: -0.003 min
Response: 2671505
Conc: 10.61 ng/ml

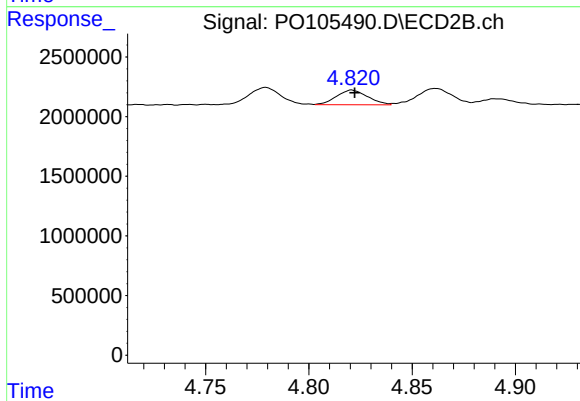

#22 AR-1248-2


R.T.: 4.821 min
Delta R.T.: -0.001 min
Response: 1284065
Conc: 13.53 ng/ml

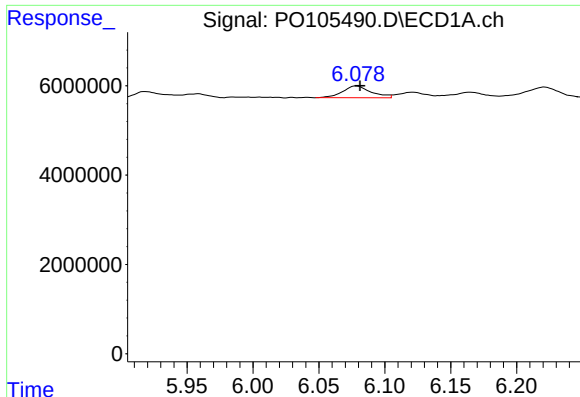

#23 AR-1248-3


R.T.: 6.078 min
Delta R.T.: -0.003 min
Response: 3950074
Conc: 13.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

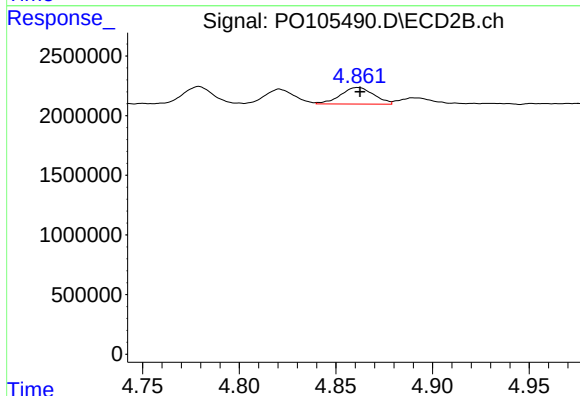


#23 AR-1248-3

R.T.: 4.861 min
Delta R.T.: -0.001 min
Response: 1664128
Conc: 16.67 ng/ml

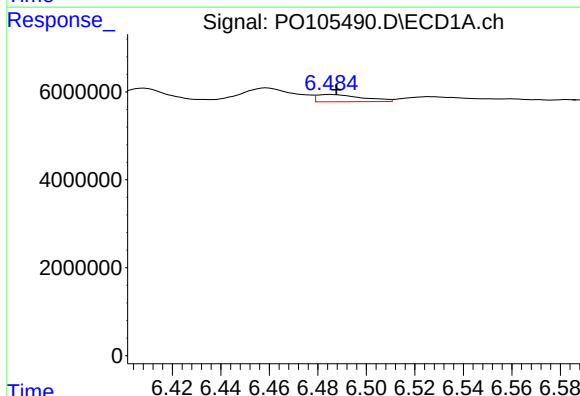


#24 AR-1248-4

R.T.: 6.485 min
Delta R.T.: -0.003 min
Response: 2150438
Conc: 6.73 ng/ml

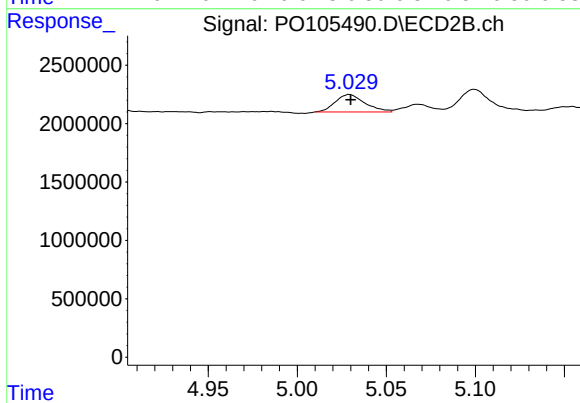

#24 AR-1248-4


R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 1721757
Conc: 15.25 ng/ml

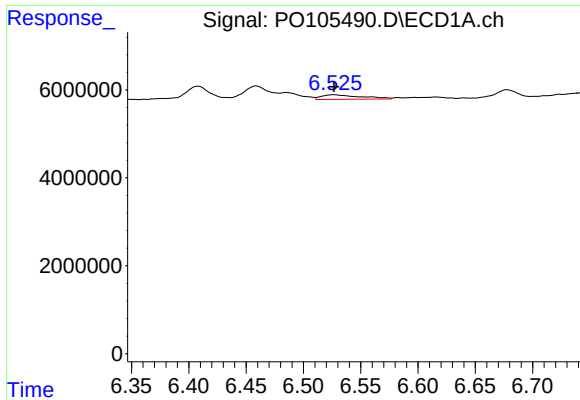

#25 AR-1248-5


R.T.: 6.527 min
Delta R.T.: 0.000 min
Response: 2553647
Conc: 8.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

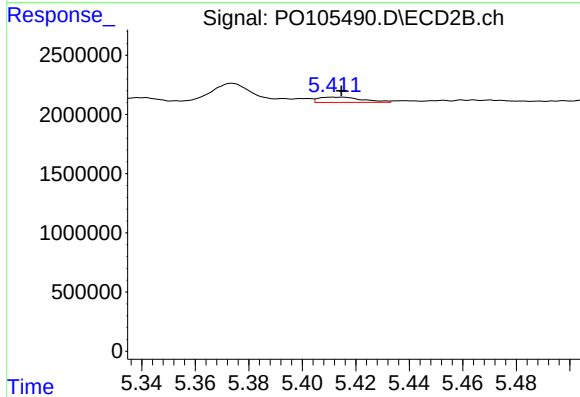


#25 AR-1248-5

R.T.: 5.412 min
Delta R.T.: -0.003 min
Response: 507244
Conc: 4.50 ng/ml

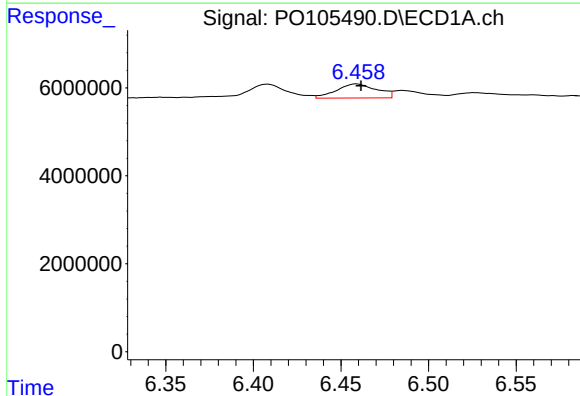


#26 AR-1254-1

R.T.: 6.459 min
Delta R.T.: -0.002 min
Response: 5146284
Conc: 16.41 ng/ml

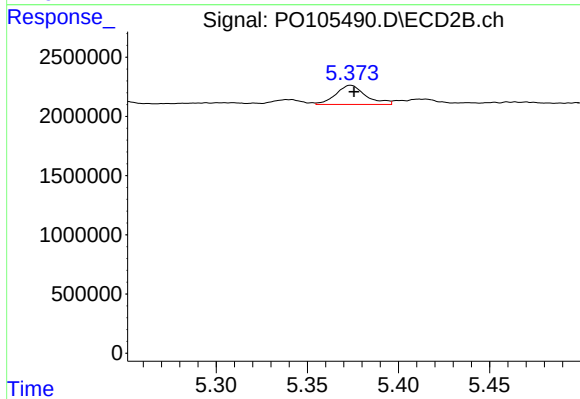

#26 AR-1254-1


R.T.: 5.374 min
Delta R.T.: -0.002 min
Response: 1833668
Conc: 11.26 ng/ml

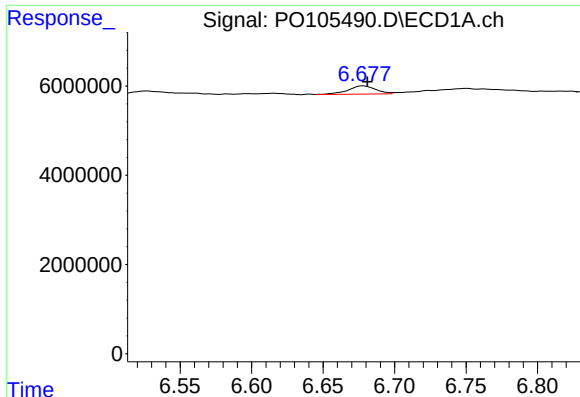

#27 AR-1254-2


R.T.: 6.678 min
Delta R.T.: -0.003 min
Response: 2476044
Conc: 5.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

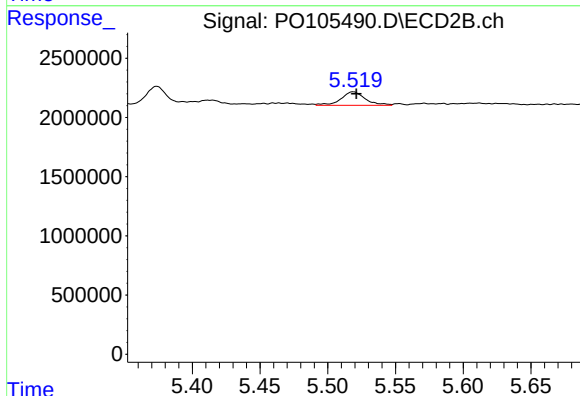


#27 AR-1254-2

R.T.: 5.519 min
Delta R.T.: -0.002 min
Response: 1443819
Conc: 9.87 ng/ml

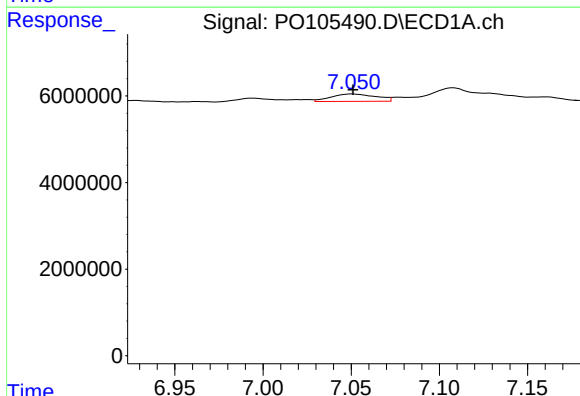


#28 AR-1254-3

R.T.: 7.051 min
Delta R.T.: 0.000 min
Response: 3053164
Conc: 6.44 ng/ml

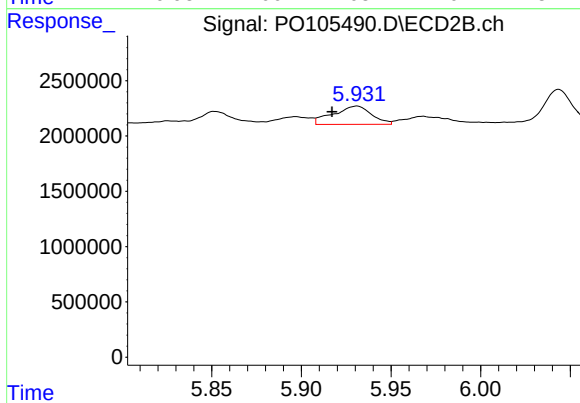

#28 AR-1254-3


R.T.: 5.931 min
Delta R.T.: 0.014 min
Response: 2472564
Conc: 10.96 ng/ml

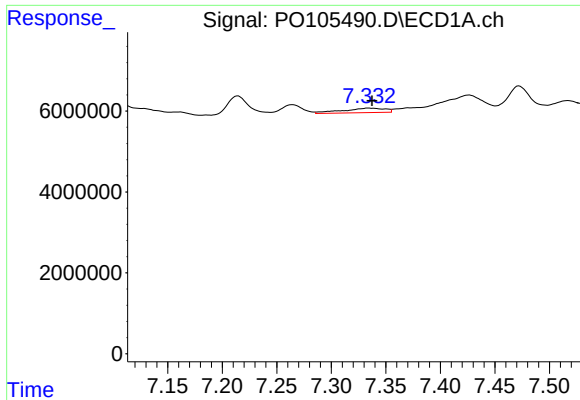

#29 AR-1254-4


R.T.: 7.334 min
Delta R.T.: -0.004 min
Response: 3012147
Conc: 8.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

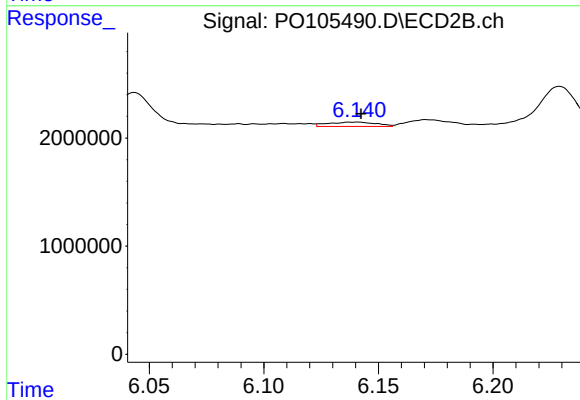


#29 AR-1254-4

R.T.: 6.141 min
Delta R.T.: -0.002 min
Response: 580507
Conc: 4.11 ng/ml

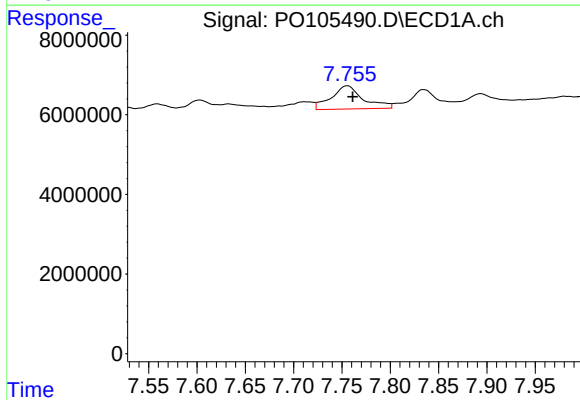


#30 AR-1254-5

R.T.: 7.756 min
Delta R.T.: -0.005 min
Response: 1345588
Conc: 33.90 ng/ml

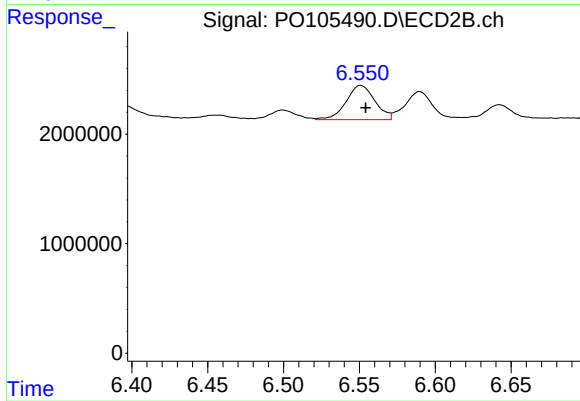

#30 AR-1254-5


R.T.: 6.551 min
Delta R.T.: -0.003 min
Response: 4133188
Conc: 20.63 ng/ml

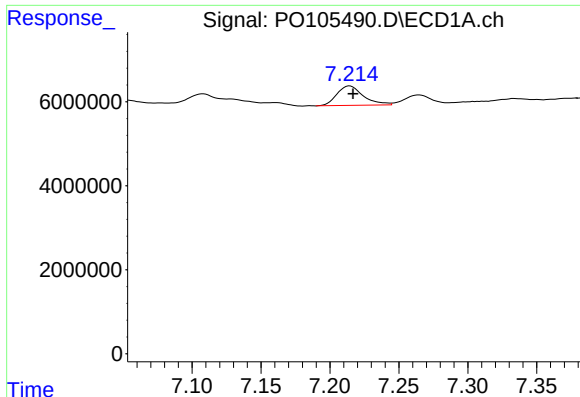

#31 AR-1260-1


R.T.: 7.214 min
Delta R.T.: -0.002 min
Response: 6221777
Conc: 16.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

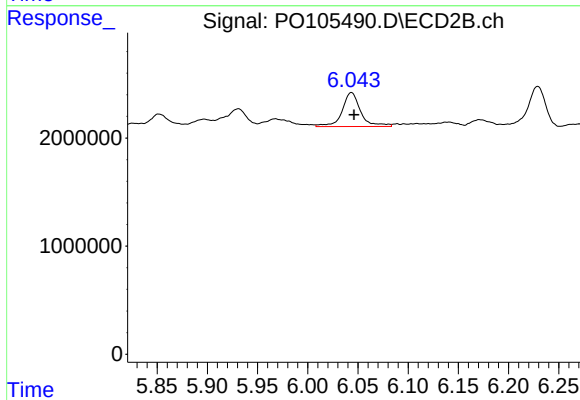


#31 AR-1260-1

R.T.: 6.044 min
Delta R.T.: -0.003 min
Response: 4026567
Conc: 25.80 ng/ml

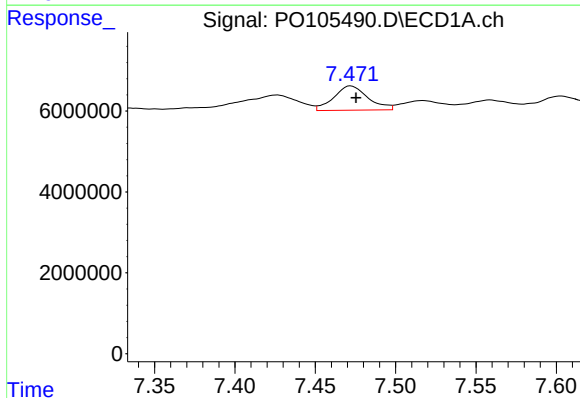


#32 AR-1260-2

R.T.: 7.472 min
Delta R.T.: -0.003 min
Response: 8900667
Conc: 21.38 ng/ml

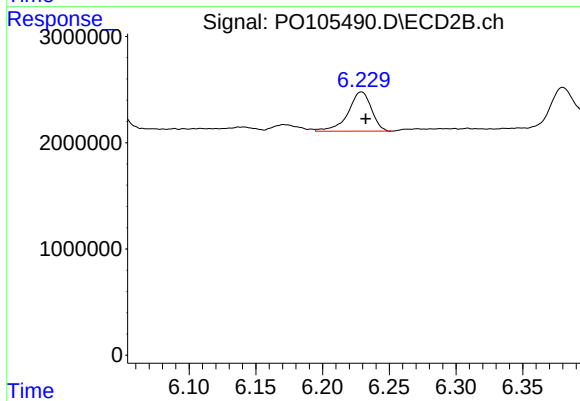

#32 AR-1260-2


R.T.: 6.229 min
Delta R.T.: -0.003 min
Response: 4495200
Conc: 23.78 ng/ml

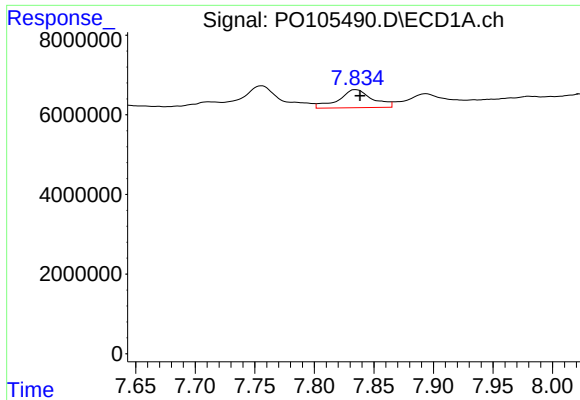

#33 AR-1260-3


R.T.: 7.835 min
Delta R.T.: -0.004 min
Response: 8959973
Conc: 34.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

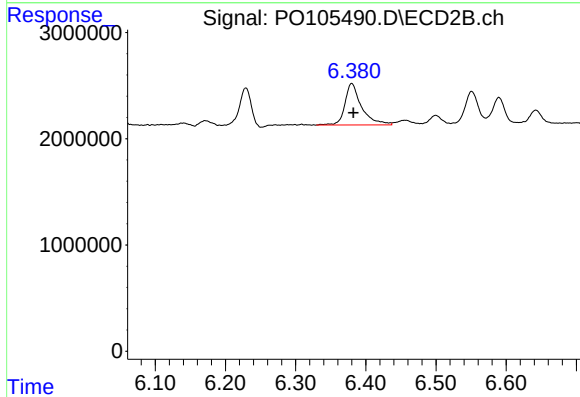


#33 AR-1260-3

R.T.: 6.380 min
Delta R.T.: -0.002 min
Response: 6405767
Conc: 34.68 ng/ml

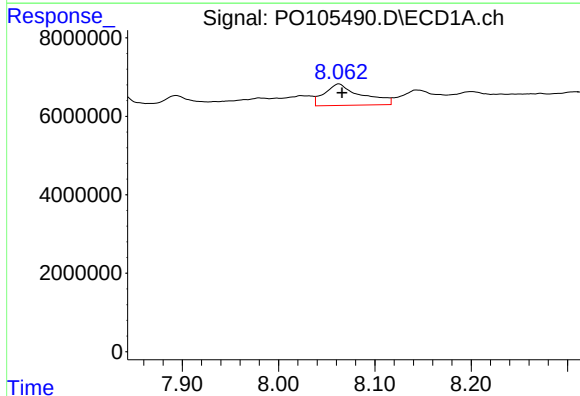


#34 AR-1260-4

R.T.: 8.063 min
Delta R.T.: -0.003 min
Response: 14597379
Conc: 44.24 ng/ml

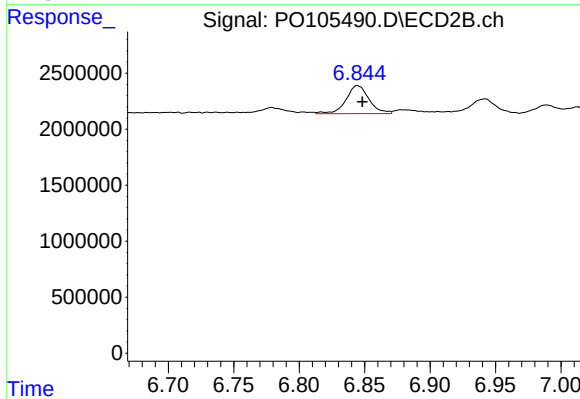

#34 AR-1260-4


R.T.: 6.845 min
Delta R.T.: -0.004 min
Response: 3068484
Conc: 25.10 ng/ml

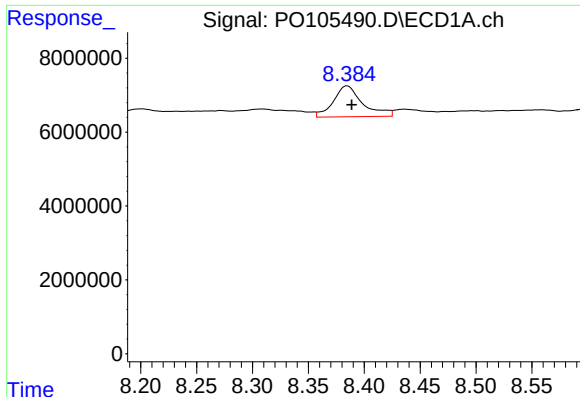

#35 AR-1260-5


R.T.: 8.385 min
Delta R.T.: -0.004 min
Response: 15248961
Conc: 25.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

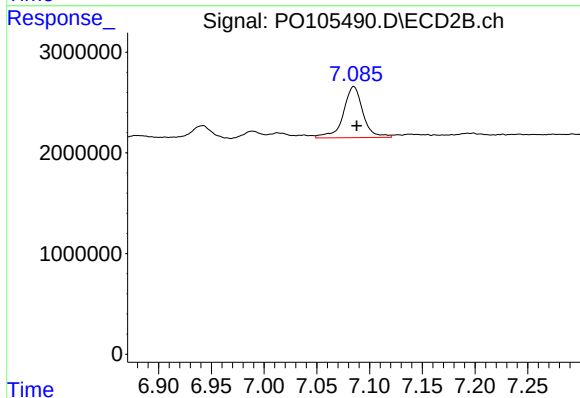


#35 AR-1260-5

R.T.: 7.085 min
Delta R.T.: -0.003 min
Response: 6583103
Conc: 23.65 ng/ml

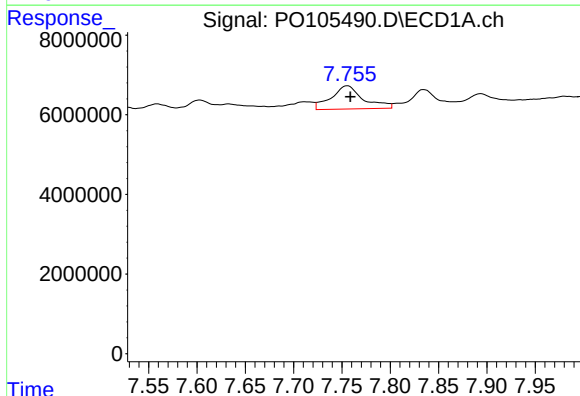


#36 AR-1262-1

R.T.: 7.756 min
Delta R.T.: -0.003 min
Response: 13455888
Conc: 42.36 ng/ml

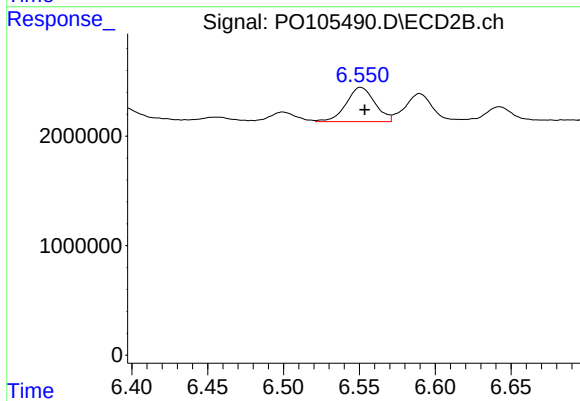

#36 AR-1262-1


R.T.: 6.551 min
Delta R.T.: -0.003 min
Response: 4133188
Conc: 38.84 ng/ml

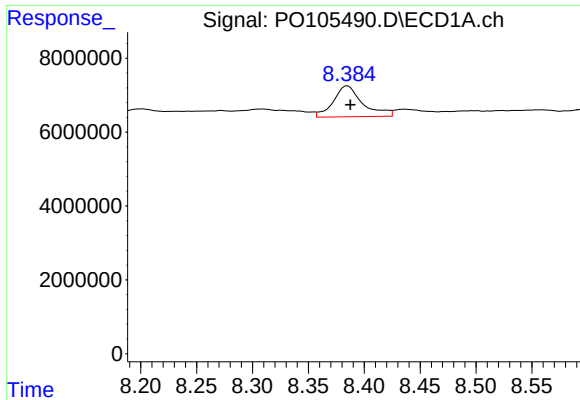

#37 AR-1262-2


R.T.: 8.385 min
Delta R.T.: -0.003 min
Response: 15248961
Conc: 20.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

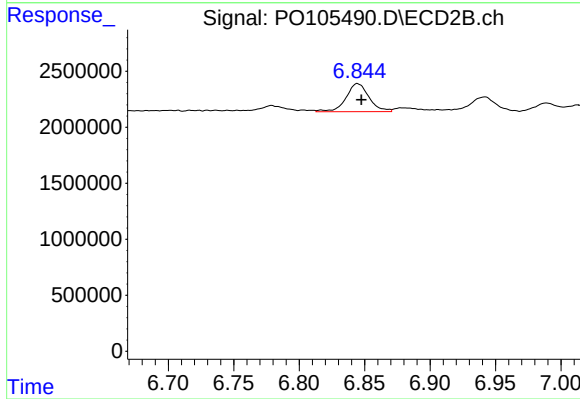


#37 AR-1262-2

R.T.: 6.845 min
Delta R.T.: -0.003 min
Response: 3068484
Conc: 18.06 ng/ml

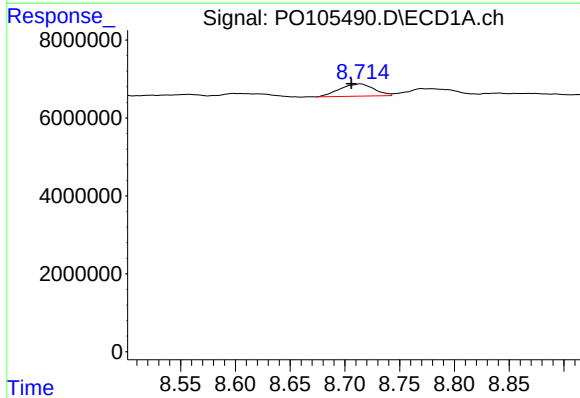


#38 AR-1262-3

R.T.: 8.714 min
Delta R.T.: 0.009 min
Response: 6856228
Conc: 13.93 ng/ml

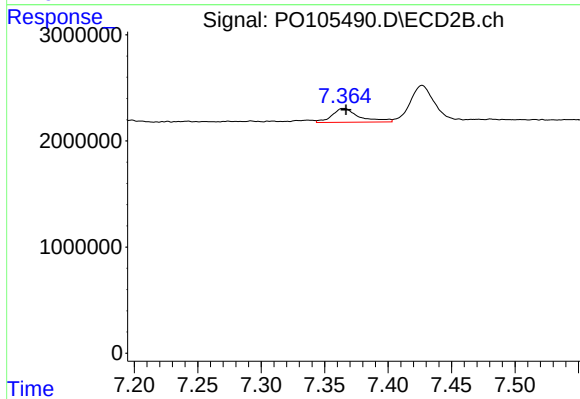

#38 AR-1262-3


R.T.: 7.365 min
Delta R.T.: -0.002 min
Response: 1949939
Conc: 15.44 ng/ml

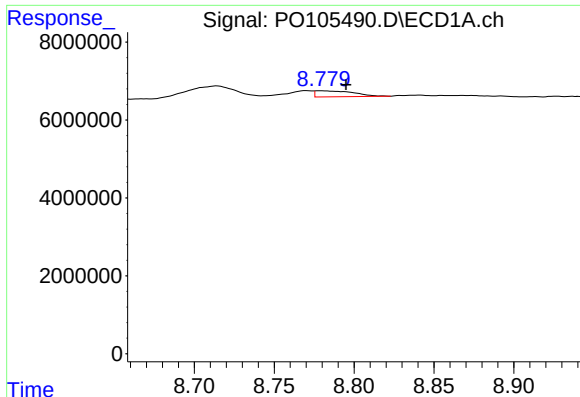

#39 AR-1262-4


R.T.: 8.779 min
Delta R.T.: -0.016 min
Response: 2561970
Conc: 6.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

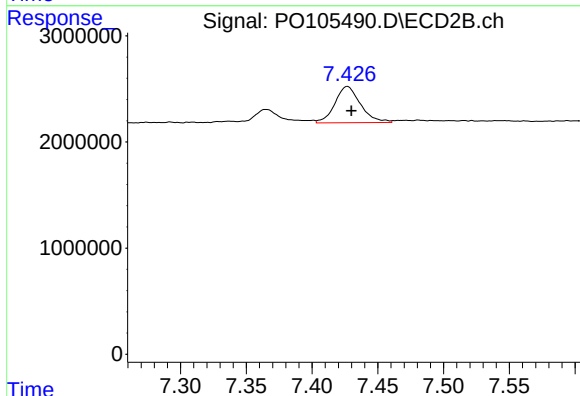


#39 AR-1262-4

R.T.: 7.427 min
Delta R.T.: -0.003 min
Response: 4633549
Conc: 20.02 ng/ml

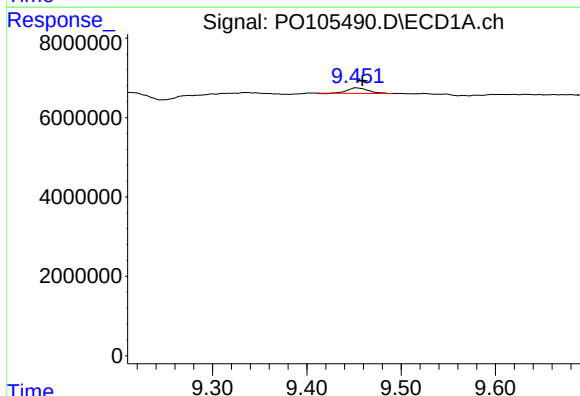


#40 AR-1262-5

R.T.: 9.452 min
Delta R.T.: -0.007 min
Response: 2102440
Conc: 7.85 ng/ml

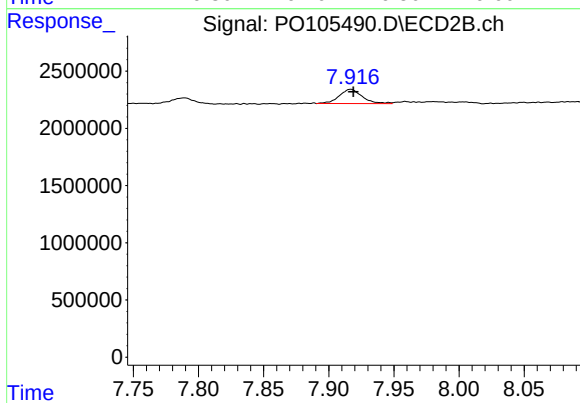

#40 AR-1262-5


R.T.: 7.917 min
Delta R.T.: -0.002 min
Response: 1514323
Conc: 15.07 ng/ml

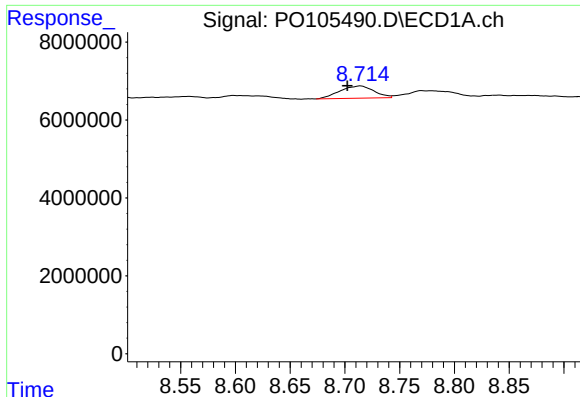

#41 AR-1268-1


R.T.: 8.714 min
Delta R.T.: 0.012 min
Response: 6856228
Conc: 8.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

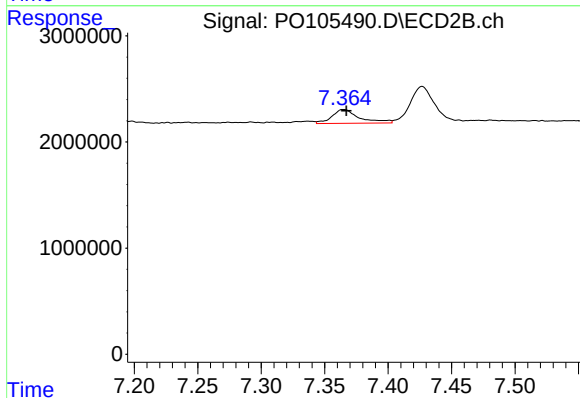


#41 AR-1268-1

R.T.: 7.365 min
Delta R.T.: -0.002 min
Response: 1949939
Conc: 5.59 ng/ml

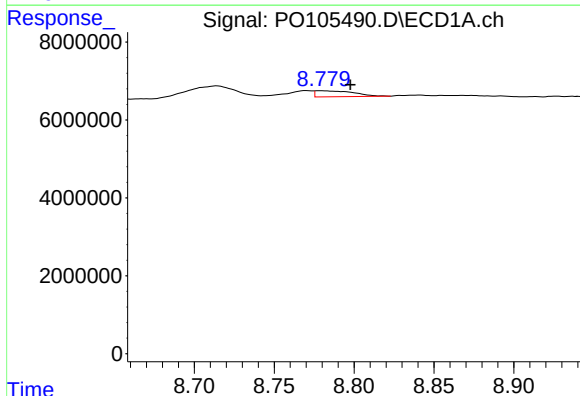


#42 AR-1268-2

R.T.: 8.779 min
Delta R.T.: -0.019 min
Response: 2561970
Conc: 3.52 ng/ml

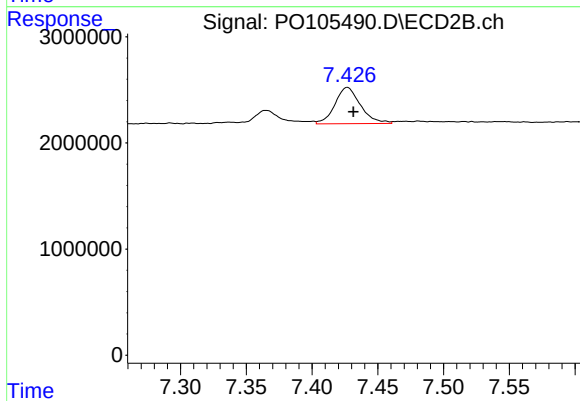

#42 AR-1268-2


R.T.: 7.427 min
Delta R.T.: -0.005 min
Response: 4633549
Conc: 14.85 ng/ml

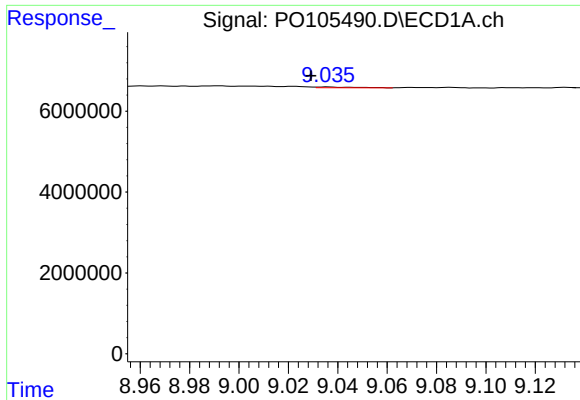

#43 AR-1268-3


R.T.: 9.036 min
Delta R.T.: 0.006 min
Response: 200083
Conc: 0.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

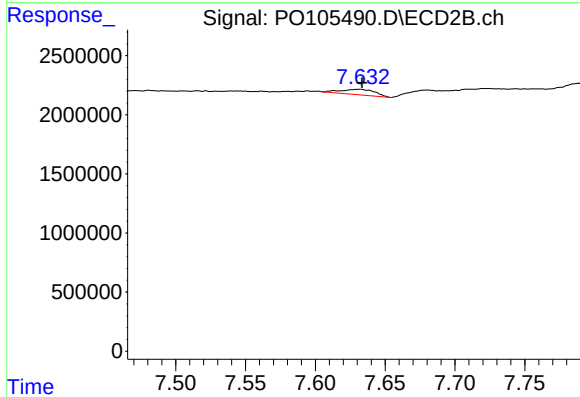


#43 AR-1268-3

R.T.: 7.631 min
Delta R.T.: -0.002 min
Response: 782331
Conc: 3.10 ng/ml

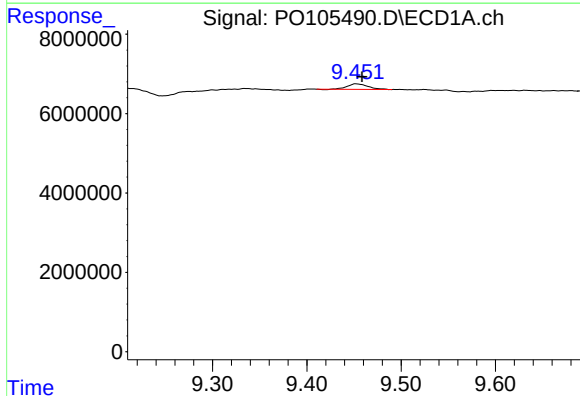


#44 AR-1268-4

R.T.: 9.452 min
Delta R.T.: -0.006 min
Response: 2102440
Conc: 7.55 ng/ml

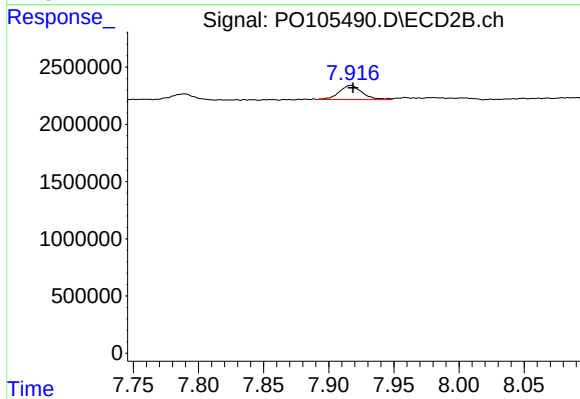

#44 AR-1268-4


R.T.: 7.917 min
Delta R.T.: -0.002 min
Response: 1514323
Conc: 14.08 ng/ml

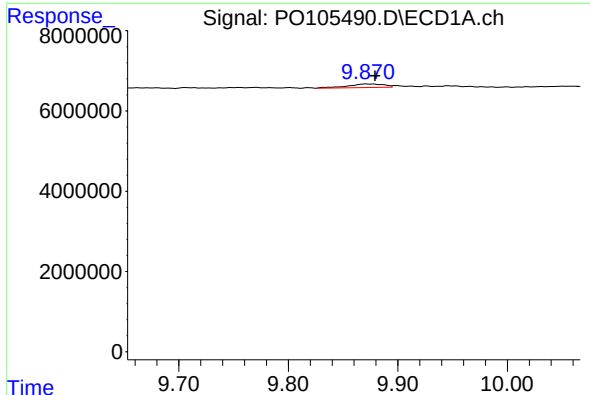

#45 AR-1268-5

R.T.: 9.871 min
Delta R.T.: -0.008 min
Response: 1988550
Conc: 0.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

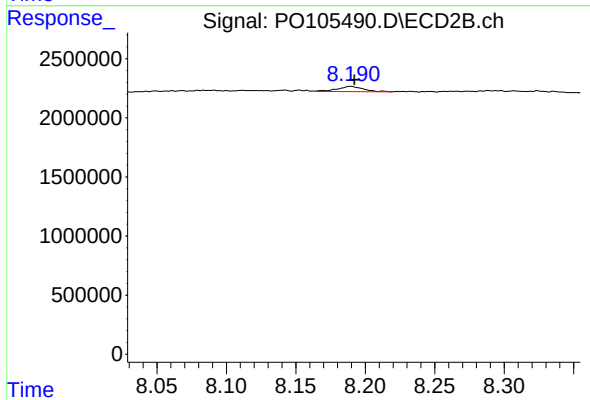

#45 AR-1268-5

R.T.: 8.189 min
Delta R.T.: -0.003 min
Response: 577068
Conc: 0.86 ng/ml