

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081324\
 Data File : P0105491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 12:15
 Operator : YP/AJ
 Sample : P3390-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:05:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.427	3.536	104.4E6	46554381	11.955	14.822
2)	SA Decachlor...	10.216	8.426	80342241	29323076	13.966	16.563
Target Compounds							
3)	L1 AR-1016-1	5.596	4.590	314888	178831	1.041	1.591 #
4)	L1 AR-1016-2	5.618	4.608	650079	353936	1.521	2.273 #
5)	L1 AR-1016-3	5.682	4.780	310309	102938	1.209	1.229
6)	L1 AR-1016-4	5.783	4.823	1466404	61934	6.705	0.920 #
7)	L1 AR-1016-5	6.081	5.034	1084081	336802	5.067	4.024
8)	L2 AR-1221-1	4.633	3.742	2736911	863944	24.406	21.887
9)	L2 AR-1221-2	4.729	3.826	3841963	1522415	45.327	49.554
10)	L2 AR-1221-3	4.796	3.900	5074140	1965587	20.857	21.966
11)	L3 AR-1232-1	4.796	3.900	5074140	1965587	25.379	26.915
12)	L3 AR-1232-2	5.335	4.608	170268	353936	1.609	5.041 #
13)	L3 AR-1232-3	5.618	4.780	650079	102938	3.396	2.693
14)	L3 AR-1232-4	5.783	4.860	1466404	154028	15.035	4.427 #
15)	L3 AR-1232-5	5.873	5.034	123184	336802	1.709	9.542 #
16)	L4 AR-1242-1	5.596	4.590	314888	178831	1.355	2.028 #
17)	L4 AR-1242-2	5.618	4.608	650079	353936	1.995	2.981 #
18)	L4 AR-1242-3	5.682	4.780	310309	102938	1.573	1.585
19)	L4 AR-1242-4	5.783	4.860	1466404	154028	8.594	2.322 #
20)	L4 AR-1242-5	6.533	5.397	799397	965640	4.574	11.751 #
21)	L5 AR-1248-1	5.596	4.590	314888	178831	1.724	2.561 #
22)	L5 AR-1248-2	5.873	4.823	123184	61934	0.489	0.653 #
23)	L5 AR-1248-3	6.081	4.860	1084081	154028	3.835	1.543 #
24)	L5 AR-1248-4	6.500	5.034	976731	336802	3.055	2.984
25)	L5 AR-1248-5	6.533	5.420	799397	198033	2.584	1.759 #
26)	L6 AR-1254-1	6.460	5.397	3557218	965640	11.343	5.931 #
27)	L6 AR-1254-2	6.688	5.516	496011	156720	1.099	1.071
28)	L6 AR-1254-3	7.055	5.908	3248801	470150	6.849	2.084 #
29)	L6 AR-1254-4	7.335	6.139	362317	537664	1.011	3.810 #
30)	L6 AR-1254-5	7.752	6.551	9136650	433639	23.016	2.164 #
31)	L7 AR-1260-1	7.231	6.043	859317	660049	2.345	4.228 #
32)	L7 AR-1260-2	7.478	6.215	1015847	764413	2.440	4.045 #
33)	L7 AR-1260-3	7.842	6.388	944211	3567376	3.648	19.311 #
34)	L7 AR-1260-4	8.076	6.848	5736532	285409	17.387	2.335 #
35)	L7 AR-1260-5	8.404	7.092	3499740	143954	5.883	0.517 #
36)	L8 AR-1262-1	7.752	6.551	9136650	433639	28.765	4.075 #
37)	L8 AR-1262-2	8.404	6.848	3499740	285409	4.653	1.680 #
38)	L8 AR-1262-3	8.717	7.373	1011522	462109	2.056	3.660 #
39)	L8 AR-1262-4	8.799	7.420	339667	390926	0.925	1.689 #
40)	L8 AR-1262-5	9.458	7.927	196927	37089	0.735	0.369 #
41)	L9 AR-1268-1	8.717	7.373	1011522	462109	1.244	1.324

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081324\
Data File : P0105491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 12:15
Operator : YP/AJ
Sample : P3390-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:05:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.799	7.420	339667	390926	0.467	1.253 #
43)	L9 AR-1268-3	9.022	7.631	390829	650233	0.605	2.573 #
44)	L9 AR-1268-4	9.458	7.927	196927	37089	0.707	0.345 #
45)	L9 AR-1268-5	9.877	8.188	1362114	298602	0.651	0.446 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081324\
Data File : PO105491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 12:15
Operator : YP/AJ
Sample : P3390-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:05:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

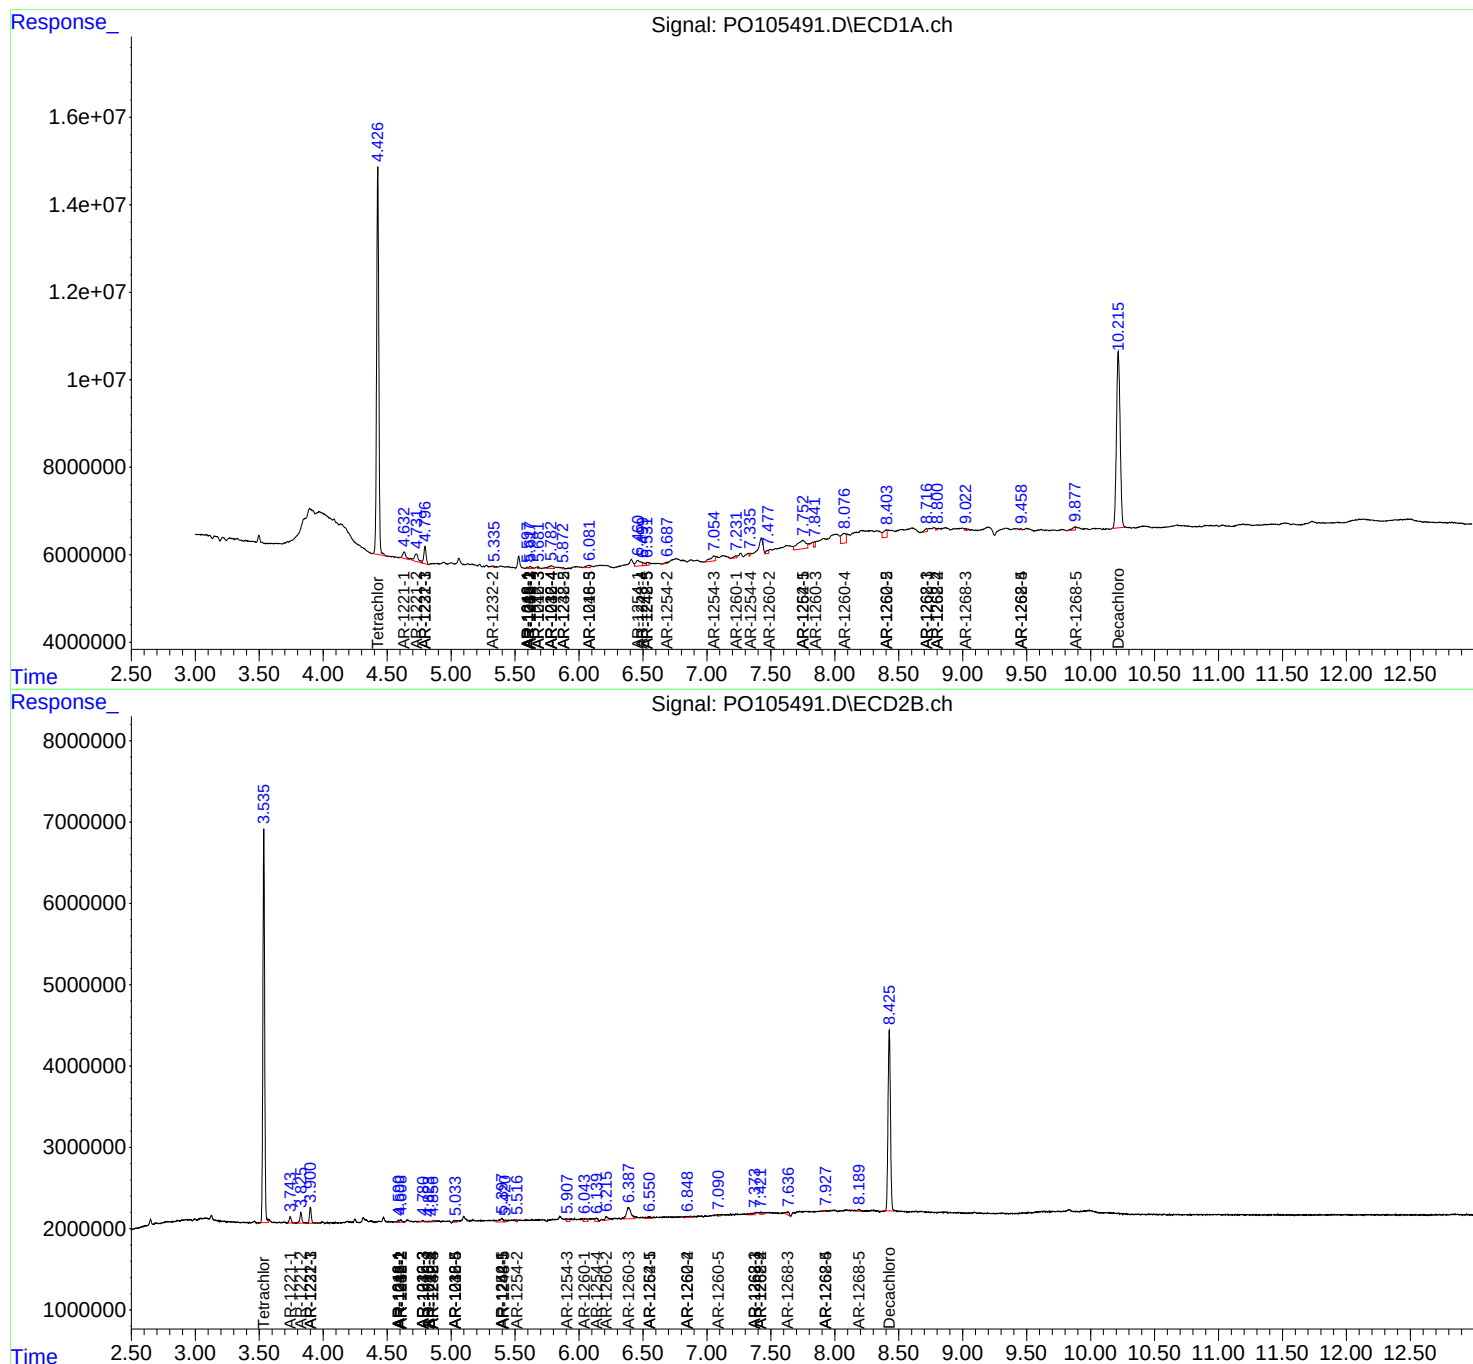


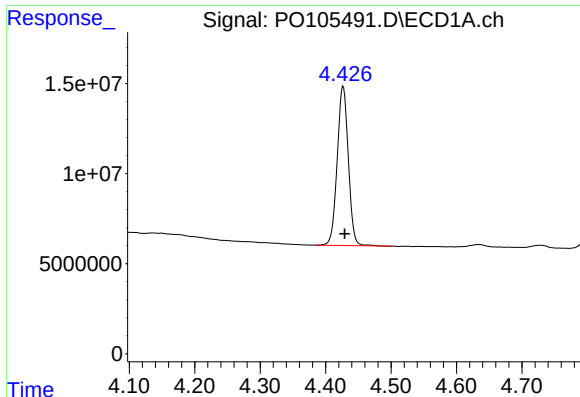

#1 Tetrachloro-m-xylene


R.T.: 4.427 min
Delta R.T.: -0.002 min
Response: 104416275
Conc: 11.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

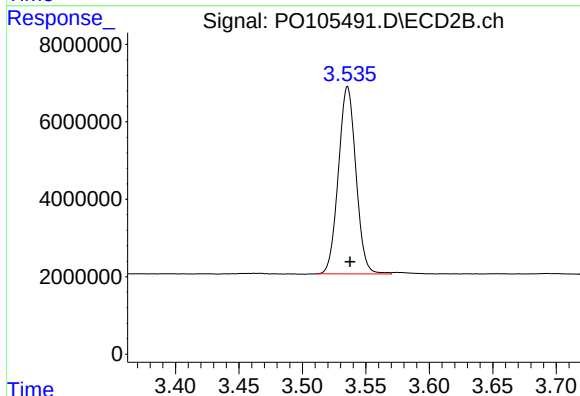


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 46554381
Conc: 14.82 ng/ml

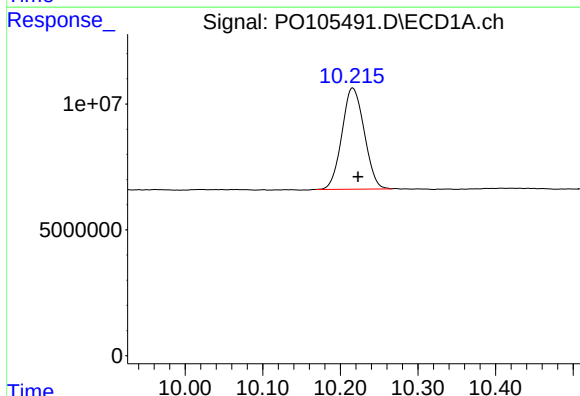


#2 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.007 min
Response: 80342241
Conc: 13.97 ng/ml

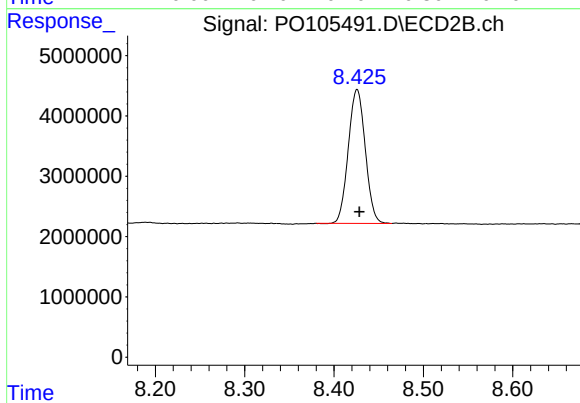

#2 Decachlorobiphenyl


R.T.: 8.426 min
Delta R.T.: -0.003 min
Response: 29323076
Conc: 16.56 ng/ml

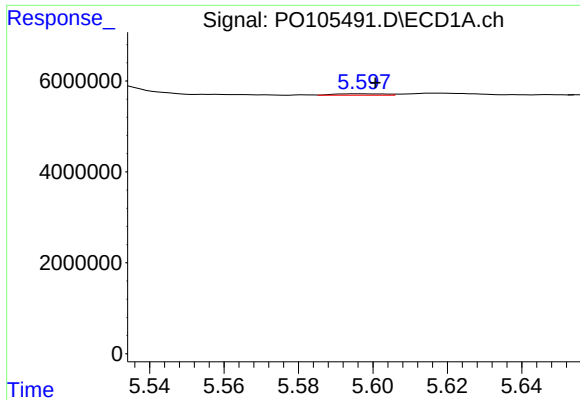

#3 AR-1016-1


R.T.: 5.596 min
Delta R.T.: -0.004 min
Response: 314888
Conc: 1.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

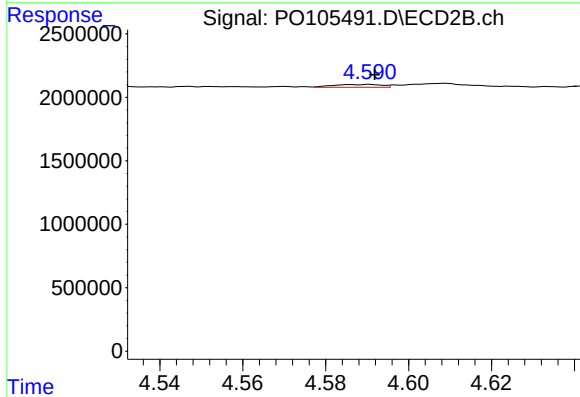


#3 AR-1016-1

R.T.: 4.590 min
Delta R.T.: -0.002 min
Response: 178831
Conc: 1.59 ng/ml

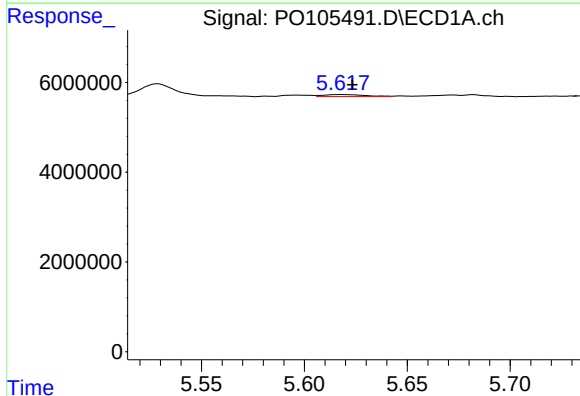


#4 AR-1016-2

R.T.: 5.618 min
Delta R.T.: -0.005 min
Response: 650079
Conc: 1.52 ng/ml

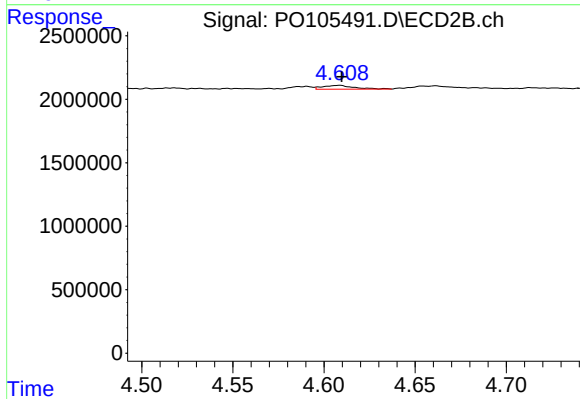

#4 AR-1016-2


R.T.: 4.608 min
Delta R.T.: -0.001 min
Response: 353936
Conc: 2.27 ng/ml

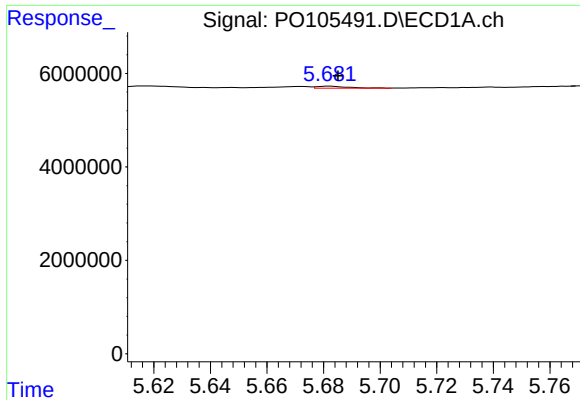

#5 AR-1016-3


R.T.: 5.682 min
Delta R.T.: -0.003 min
Response: 310309
Conc: 1.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

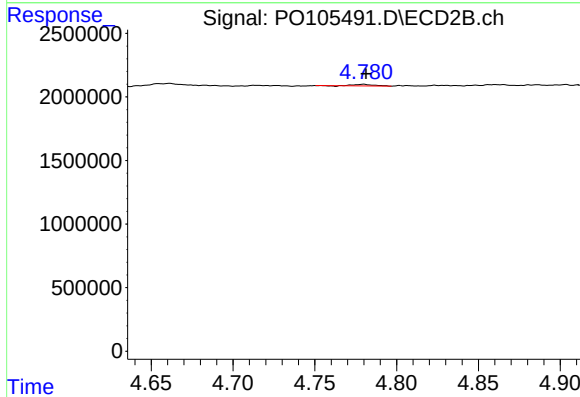


#5 AR-1016-3

R.T.: 4.780 min
Delta R.T.: -0.002 min
Response: 102938
Conc: 1.23 ng/ml

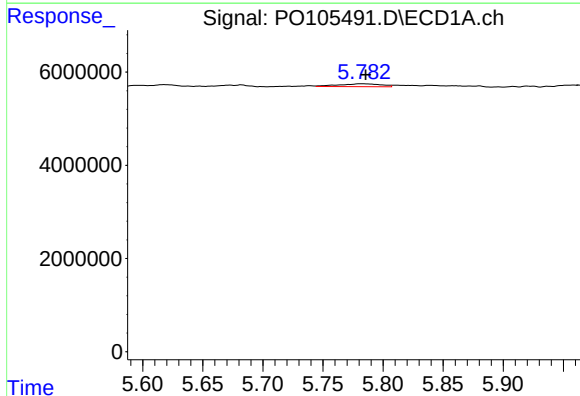


#6 AR-1016-4

R.T.: 5.783 min
Delta R.T.: -0.003 min
Response: 1466404
Conc: 6.70 ng/ml

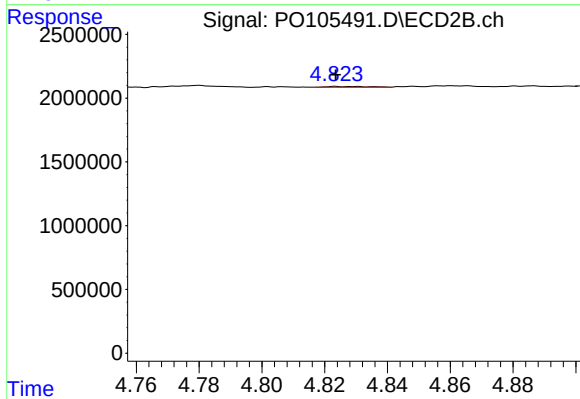

#6 AR-1016-4


R.T.: 4.823 min
Delta R.T.: 0.000 min
Response: 61934
Conc: 0.92 ng/ml

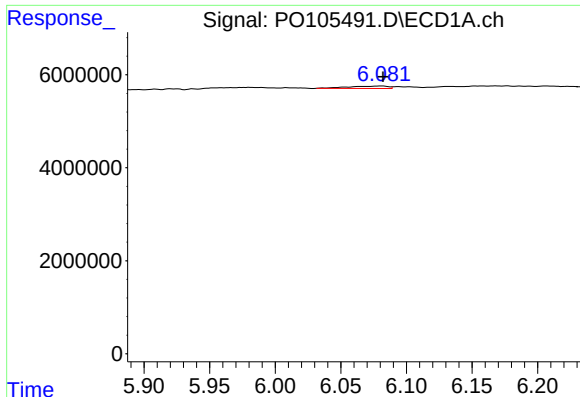

#7 AR-1016-5


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 1084081
Conc: 5.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

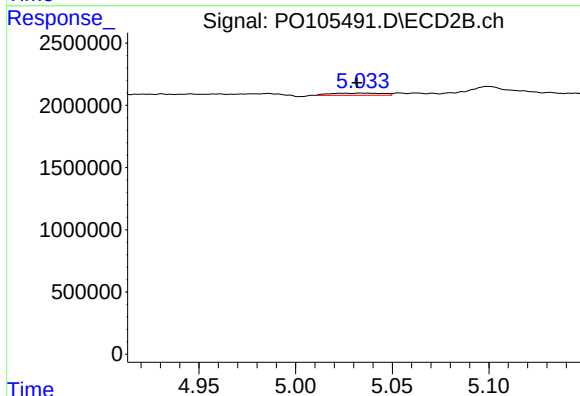


#7 AR-1016-5

R.T.: 5.034 min
Delta R.T.: 0.002 min
Response: 336802
Conc: 4.02 ng/ml

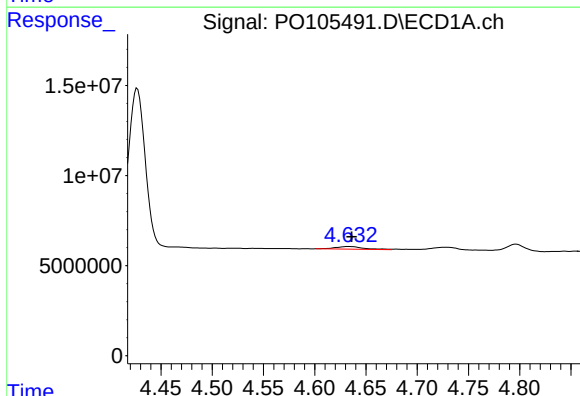


#8 AR-1221-1

R.T.: 4.633 min
Delta R.T.: -0.003 min
Response: 2736911
Conc: 24.41 ng/ml

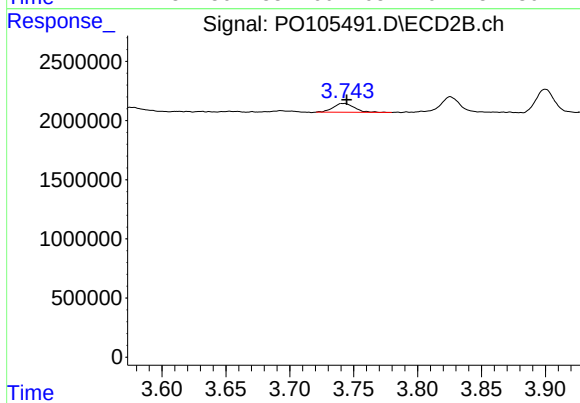

#8 AR-1221-1


R.T.: 3.742 min
Delta R.T.: -0.002 min
Response: 863944
Conc: 21.89 ng/ml

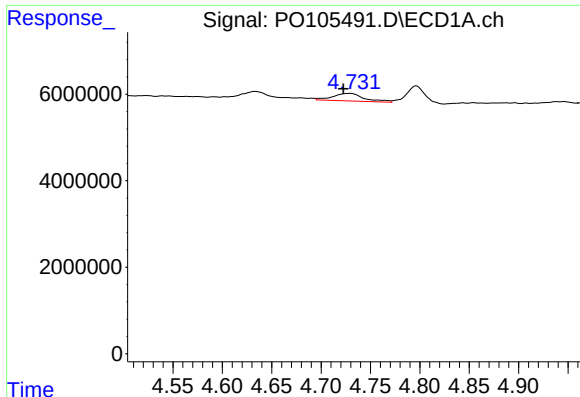

#9 AR-1221-2


R.T.: 4.729 min
Delta R.T.: 0.007 min
Response: 3841963
Conc: 45.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

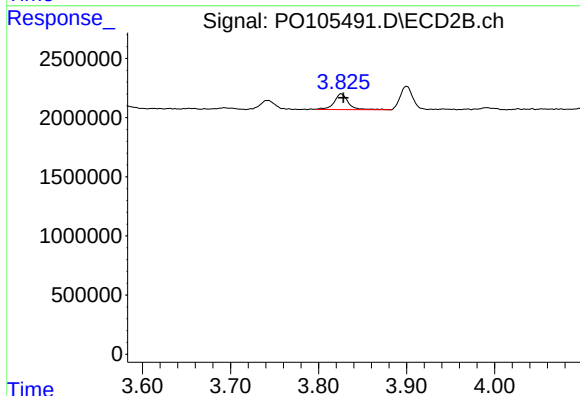


#9 AR-1221-2

R.T.: 3.826 min
Delta R.T.: -0.002 min
Response: 1522415
Conc: 49.55 ng/ml

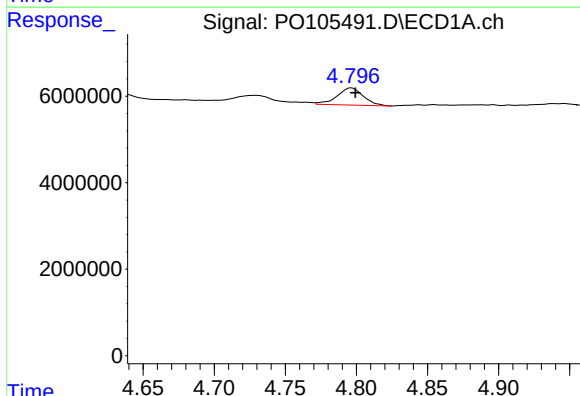


#10 AR-1221-3

R.T.: 4.796 min
Delta R.T.: -0.003 min
Response: 5074140
Conc: 20.86 ng/ml

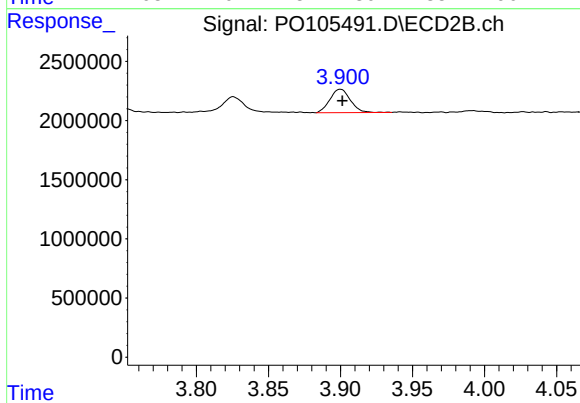

#10 AR-1221-3


R.T.: 3.900 min
Delta R.T.: -0.001 min
Response: 1965587
Conc: 21.97 ng/ml

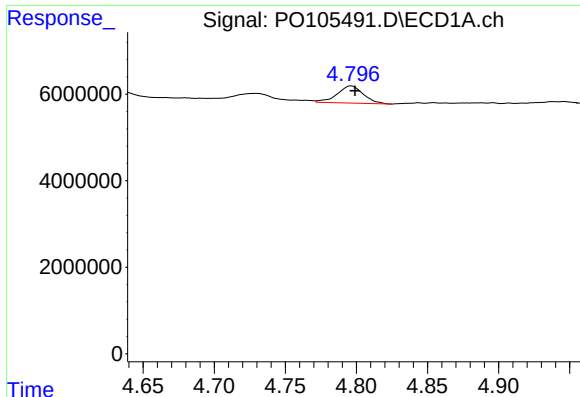

#11 AR-1232-1


R.T.: 4.796 min
Delta R.T.: -0.003 min
Response: 5074140
Conc: 25.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

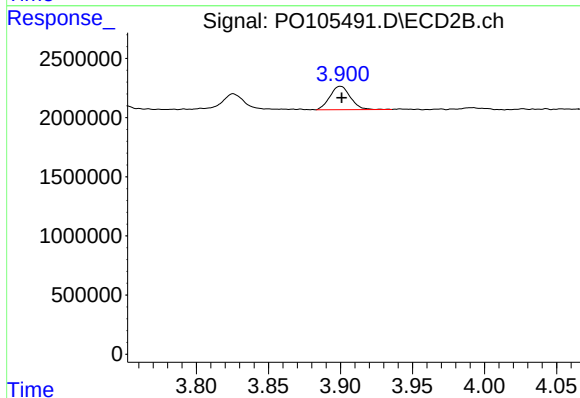


#11 AR-1232-1

R.T.: 3.900 min
Delta R.T.: -0.001 min
Response: 1965587
Conc: 26.92 ng/ml

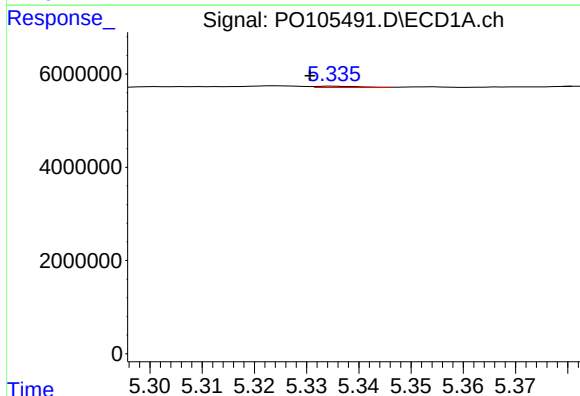


#12 AR-1232-2

R.T.: 5.335 min
Delta R.T.: 0.005 min
Response: 170268
Conc: 1.61 ng/ml

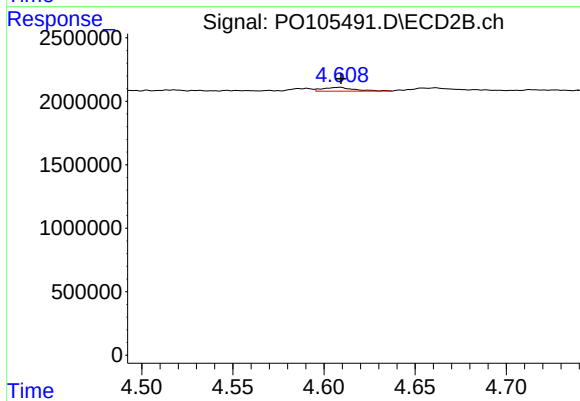

#12 AR-1232-2


R.T.: 4.608 min
Delta R.T.: -0.001 min
Response: 353936
Conc: 5.04 ng/ml

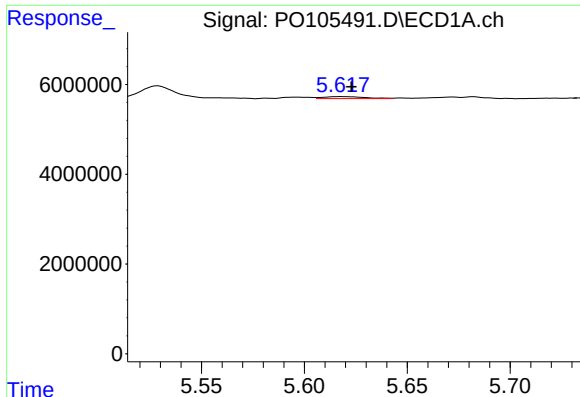

#13 AR-1232-3


R.T.: 5.618 min
Delta R.T.: -0.005 min
Response: 650079
Conc: 3.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

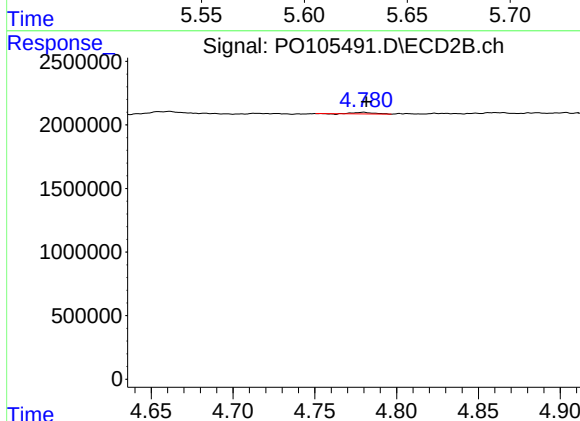


#13 AR-1232-3

R.T.: 4.780 min
Delta R.T.: -0.002 min
Response: 102938
Conc: 2.69 ng/ml

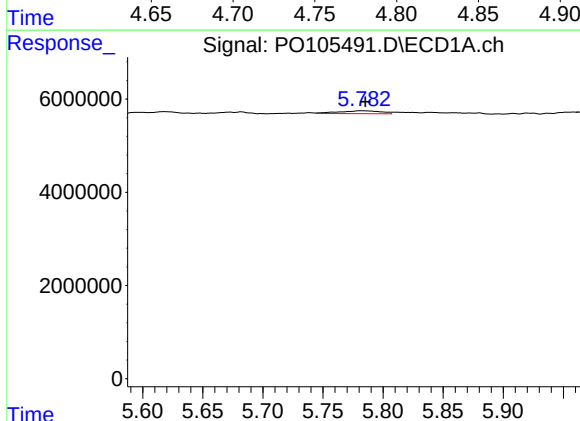


#14 AR-1232-4

R.T.: 5.783 min
Delta R.T.: -0.003 min
Response: 1466404
Conc: 15.03 ng/ml

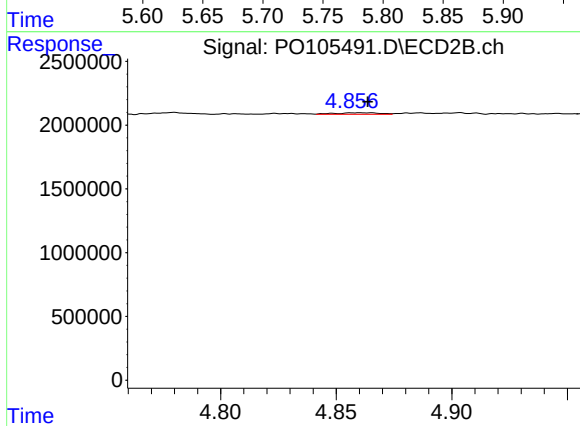

#14 AR-1232-4


R.T.: 4.860 min
Delta R.T.: -0.003 min
Response: 154028
Conc: 4.43 ng/ml

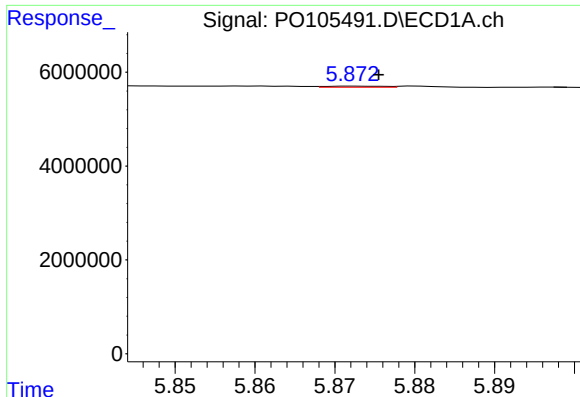

#15 AR-1232-5


R.T.: 5.873 min
Delta R.T.: -0.003 min
Response: 123184
Conc: 1.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

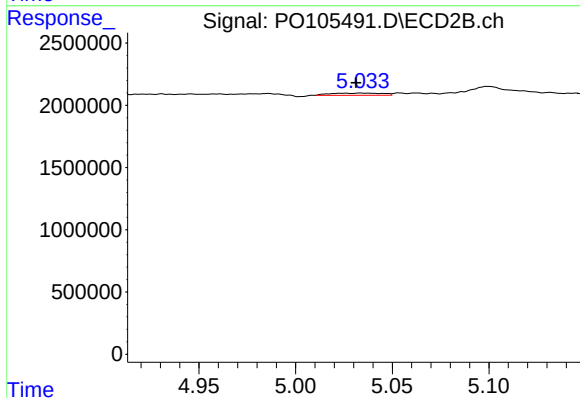


#15 AR-1232-5

R.T.: 5.034 min
Delta R.T.: 0.003 min
Response: 336802
Conc: 9.54 ng/ml

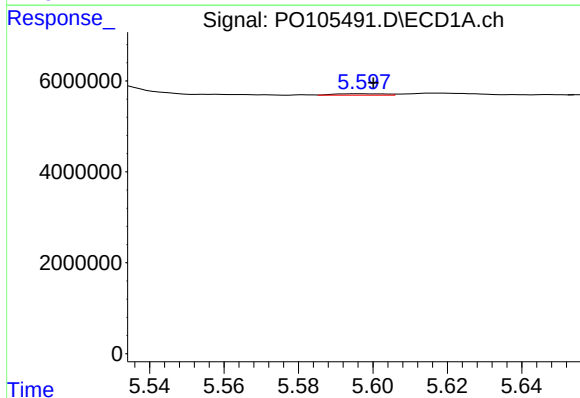


#16 AR-1242-1

R.T.: 5.596 min
Delta R.T.: -0.004 min
Response: 314888
Conc: 1.35 ng/ml

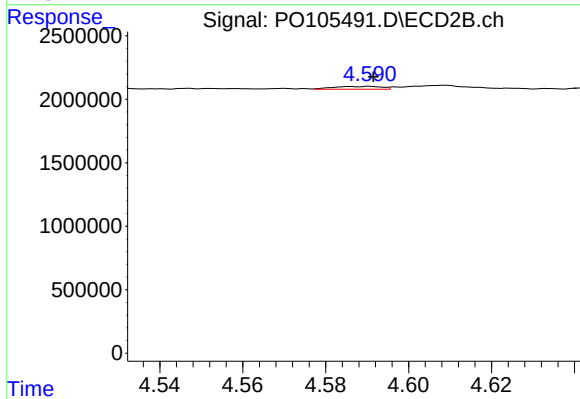

#16 AR-1242-1


R.T.: 4.590 min
Delta R.T.: -0.001 min
Response: 178831
Conc: 2.03 ng/ml

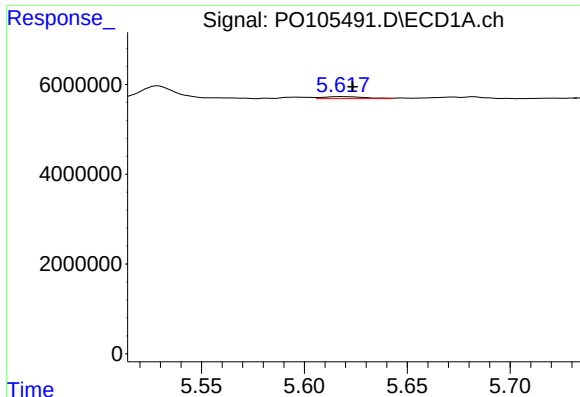

#17 AR-1242-2


R.T.: 5.618 min
Delta R.T.: -0.005 min
Response: 650079
Conc: 1.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

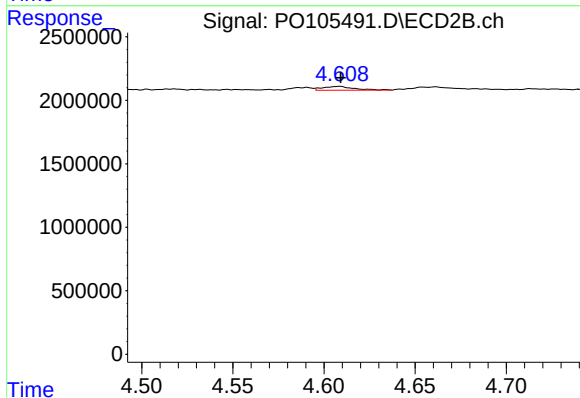


#17 AR-1242-2

R.T.: 4.608 min
Delta R.T.: 0.000 min
Response: 353936
Conc: 2.98 ng/ml

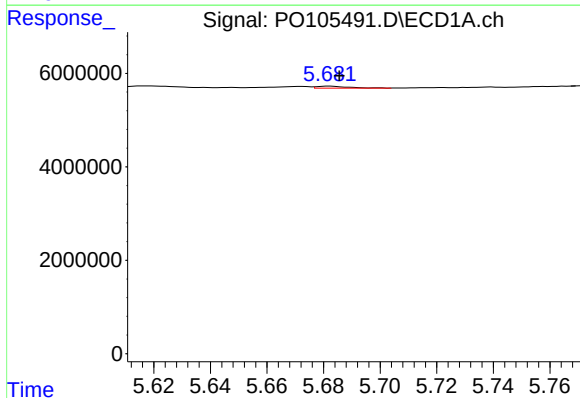


#18 AR-1242-3

R.T.: 5.682 min
Delta R.T.: -0.003 min
Response: 310309
Conc: 1.57 ng/ml

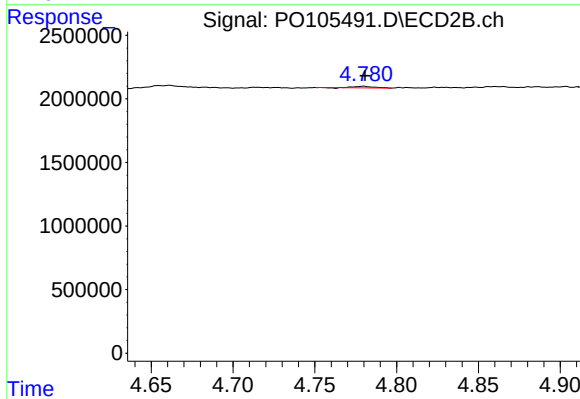

#18 AR-1242-3


R.T.: 4.780 min
Delta R.T.: -0.001 min
Response: 102938
Conc: 1.59 ng/ml

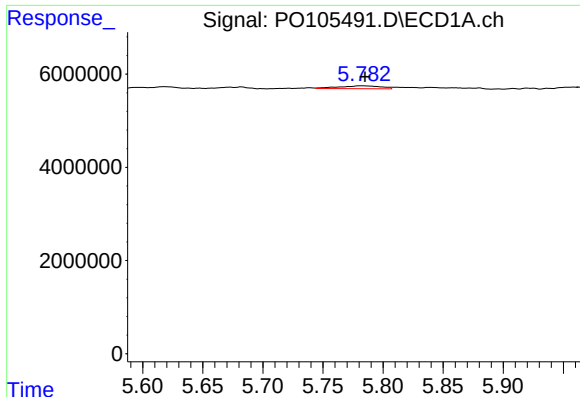

#19 AR-1242-4


R.T.: 5.783 min
Delta R.T.: -0.002 min
Response: 1466404
Conc: 8.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

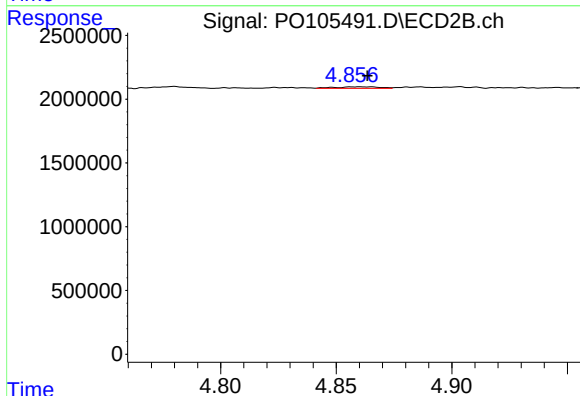


#19 AR-1242-4

R.T.: 4.860 min
Delta R.T.: -0.003 min
Response: 154028
Conc: 2.32 ng/ml

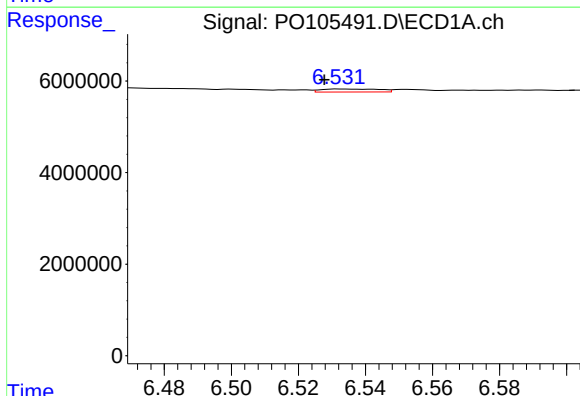


#20 AR-1242-5

R.T.: 6.533 min
Delta R.T.: 0.005 min
Response: 799397
Conc: 4.57 ng/ml

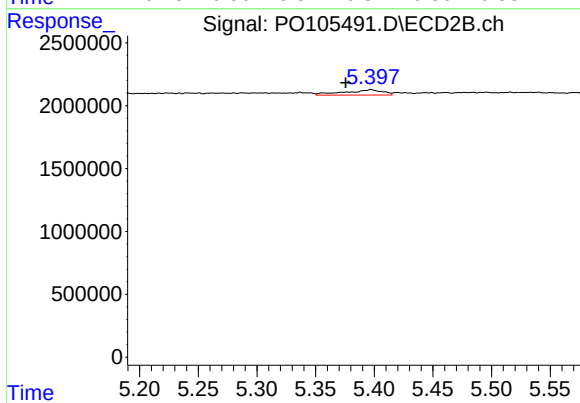

#20 AR-1242-5


R.T.: 5.397 min
Delta R.T.: 0.022 min
Response: 965640
Conc: 11.75 ng/ml

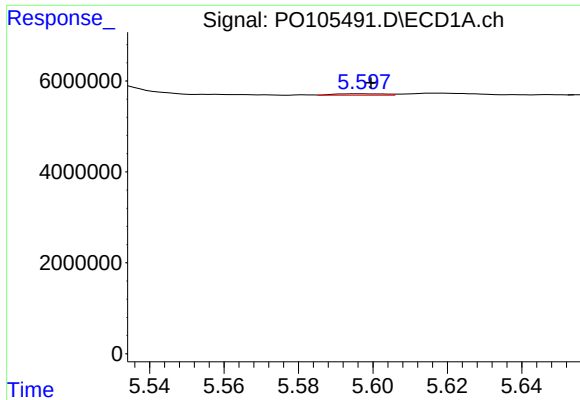

#21 AR-1248-1


R.T.: 5.596 min
Delta R.T.: -0.003 min
Response: 314888
Conc: 1.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

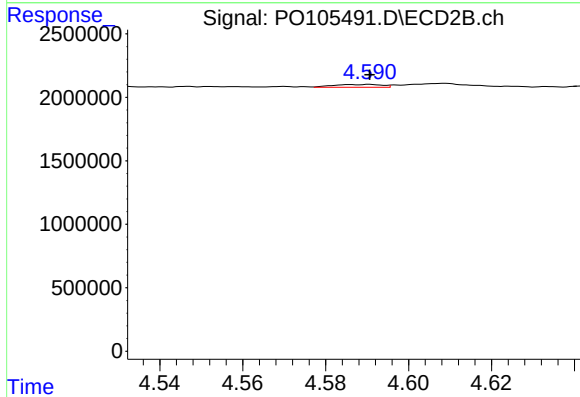


#21 AR-1248-1

R.T.: 4.590 min
Delta R.T.: 0.000 min
Response: 178831
Conc: 2.56 ng/ml

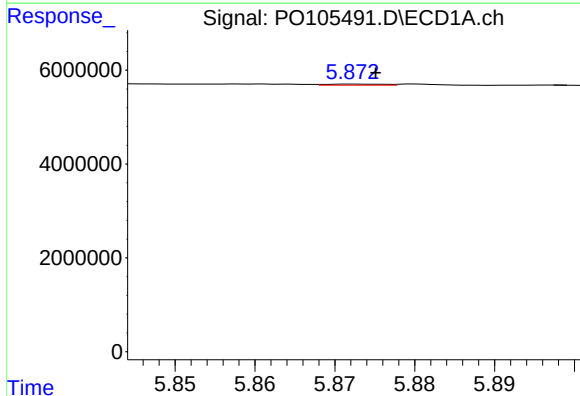


#22 AR-1248-2

R.T.: 5.873 min
Delta R.T.: -0.003 min
Response: 123184
Conc: 0.49 ng/ml

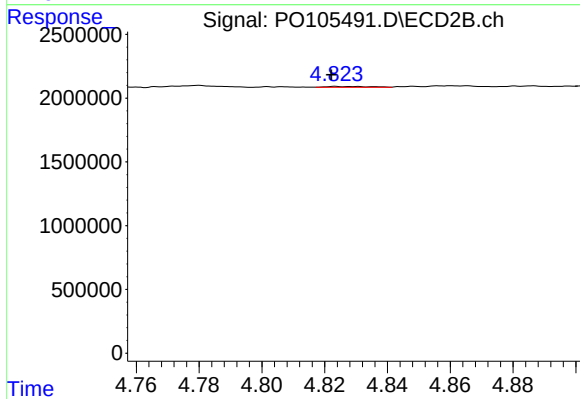

#22 AR-1248-2


R.T.: 4.823 min
Delta R.T.: 0.001 min
Response: 61934
Conc: 0.65 ng/ml

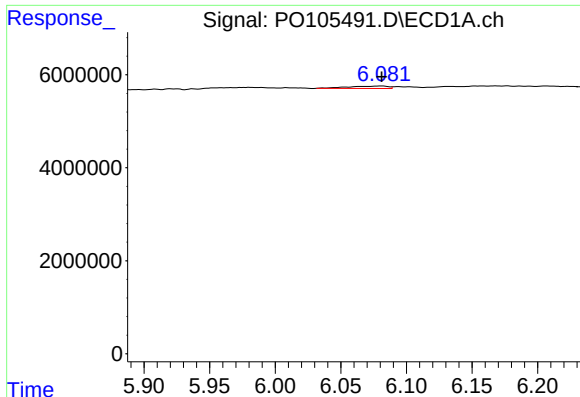

#23 AR-1248-3


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 1084081
Conc: 3.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

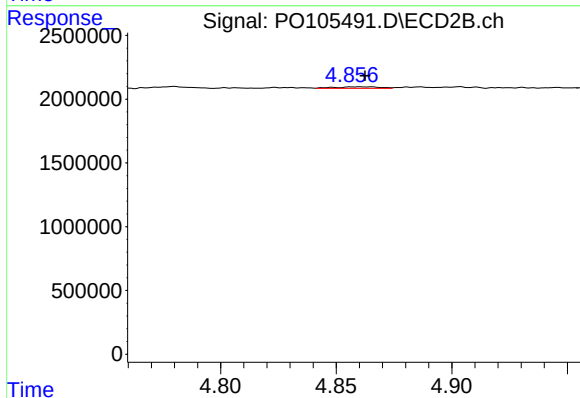


#23 AR-1248-3

R.T.: 4.860 min
Delta R.T.: -0.002 min
Response: 154028
Conc: 1.54 ng/ml

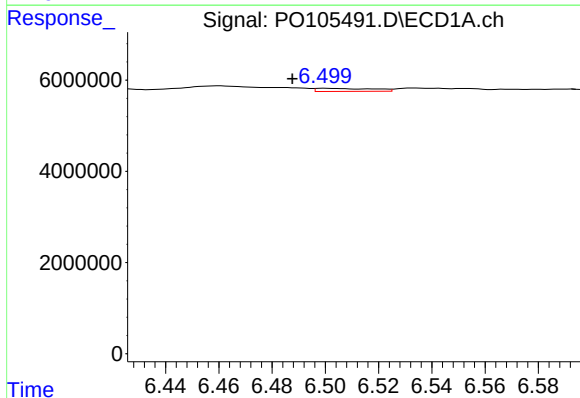


#24 AR-1248-4

R.T.: 6.500 min
Delta R.T.: 0.012 min
Response: 976731
Conc: 3.05 ng/ml

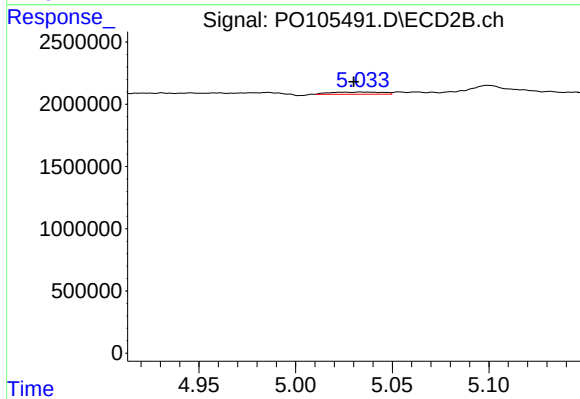

#24 AR-1248-4


R.T.: 5.034 min
Delta R.T.: 0.004 min
Response: 336802
Conc: 2.98 ng/ml

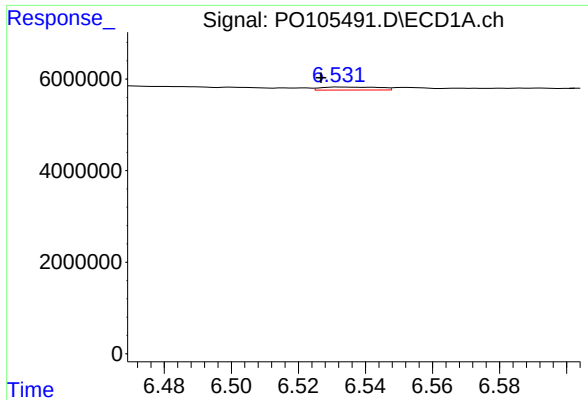

#25 AR-1248-5


R.T.: 6.533 min
Delta R.T.: 0.006 min
Response: 799397
Conc: 2.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

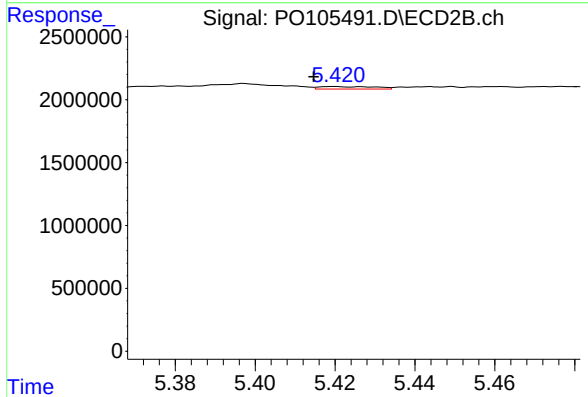


#25 AR-1248-5

R.T.: 5.420 min
Delta R.T.: 0.005 min
Response: 198033
Conc: 1.76 ng/ml

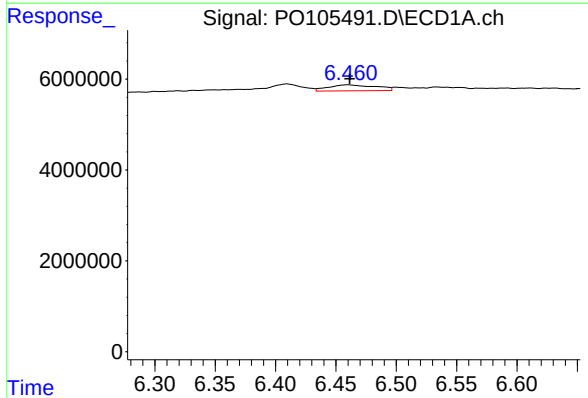


#26 AR-1254-1

R.T.: 6.460 min
Delta R.T.: -0.001 min
Response: 3557218
Conc: 11.34 ng/ml

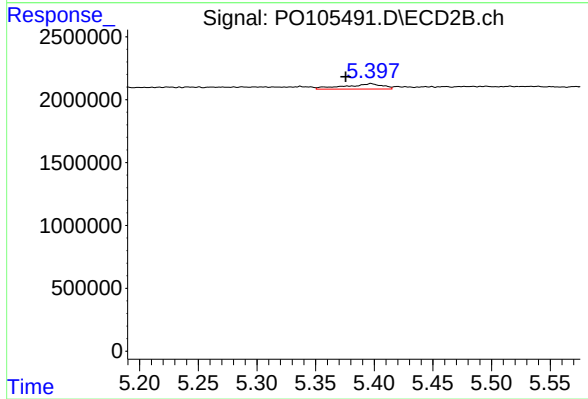

#26 AR-1254-1


R.T.: 5.397 min
Delta R.T.: 0.022 min
Response: 965640
Conc: 5.93 ng/ml

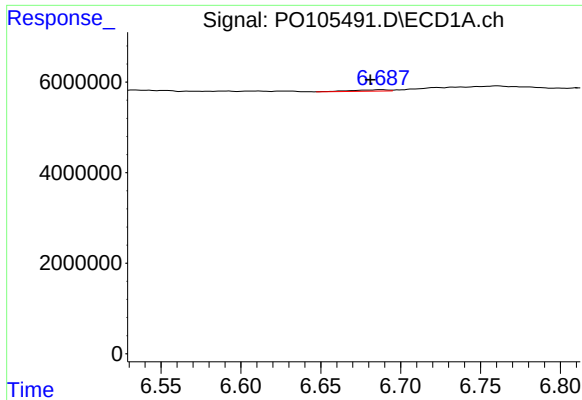

#27 AR-1254-2


R.T.: 6.688 min
Delta R.T.: 0.007 min
Response: 496011
Conc: 1.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

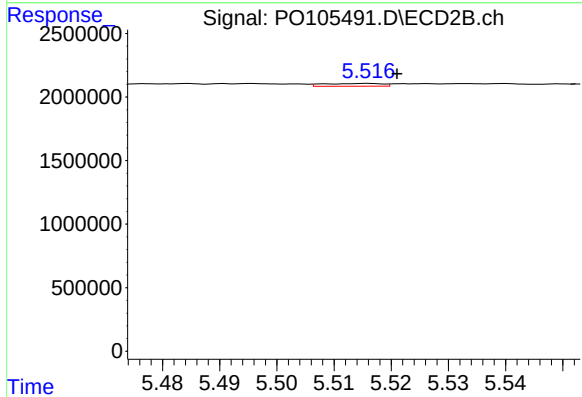


#27 AR-1254-2

R.T.: 5.516 min
Delta R.T.: -0.005 min
Response: 156720
Conc: 1.07 ng/ml

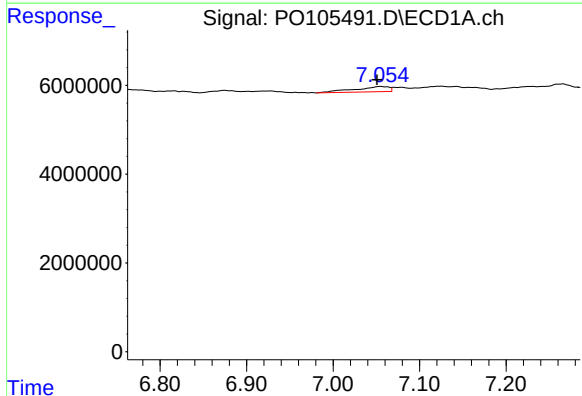


#28 AR-1254-3

R.T.: 7.055 min
Delta R.T.: 0.004 min
Response: 3248801
Conc: 6.85 ng/ml

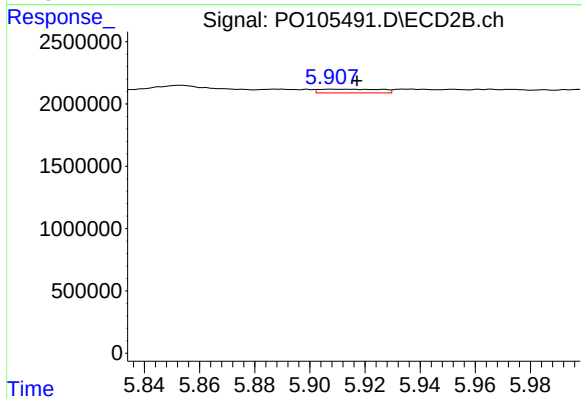

#28 AR-1254-3


R.T.: 5.908 min
Delta R.T.: -0.009 min
Response: 470150
Conc: 2.08 ng/ml

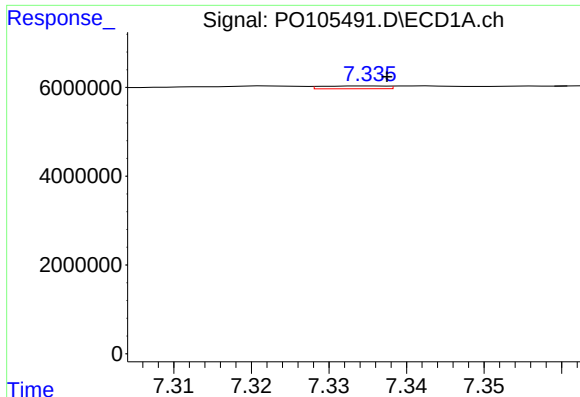

#29 AR-1254-4


R.T.: 7.335 min
Delta R.T.: -0.003 min
Response: 362317
Conc: 1.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

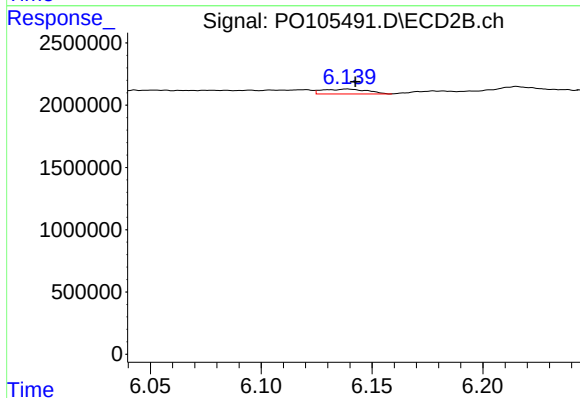


#29 AR-1254-4

R.T.: 6.139 min
Delta R.T.: -0.004 min
Response: 537664
Conc: 3.81 ng/ml

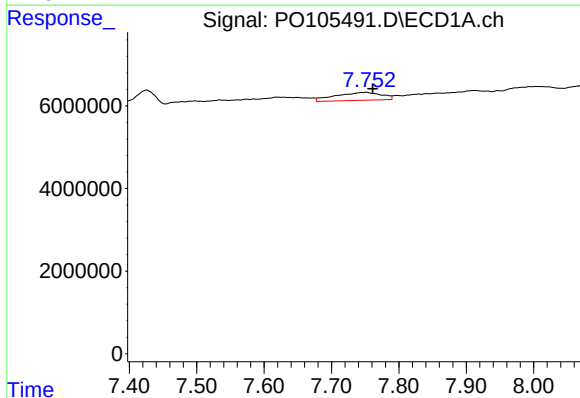


#30 AR-1254-5

R.T.: 7.752 min
Delta R.T.: -0.009 min
Response: 9136650
Conc: 23.02 ng/ml

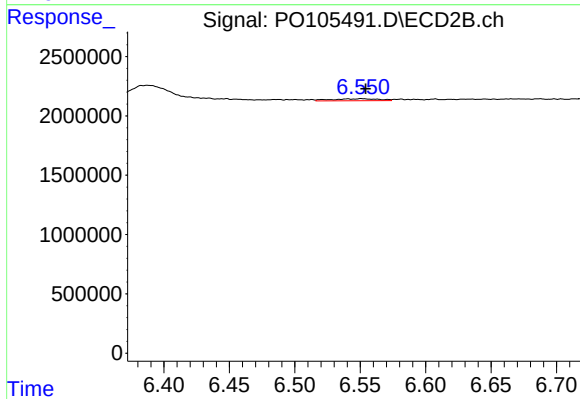

#30 AR-1254-5


R.T.: 6.551 min
Delta R.T.: -0.003 min
Response: 433639
Conc: 2.16 ng/ml

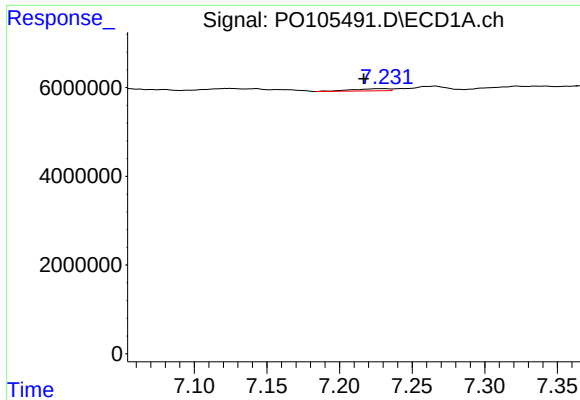

#31 AR-1260-1


R.T.: 7.231 min
Delta R.T.: 0.014 min
Response: 859317
Conc: 2.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

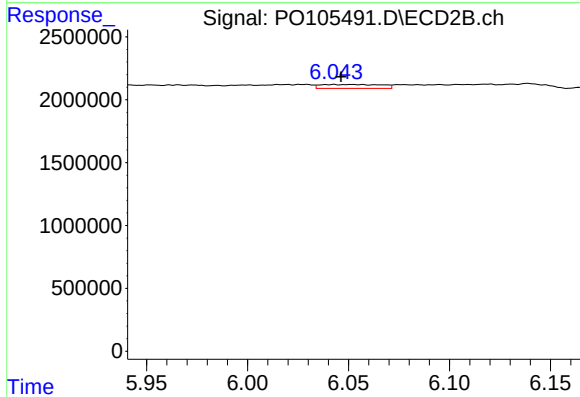


#31 AR-1260-1

R.T.: 6.043 min
Delta R.T.: -0.003 min
Response: 660049
Conc: 4.23 ng/ml

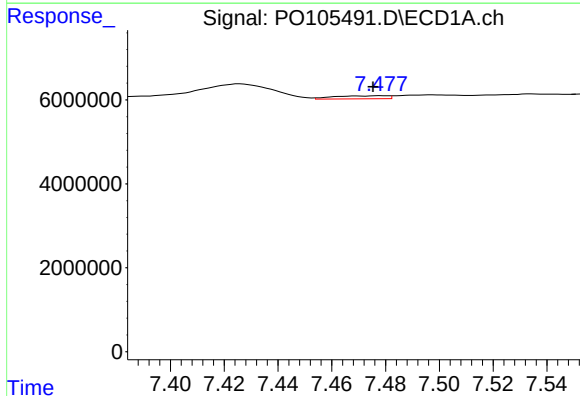


#32 AR-1260-2

R.T.: 7.478 min
Delta R.T.: 0.003 min
Response: 1015847
Conc: 2.44 ng/ml

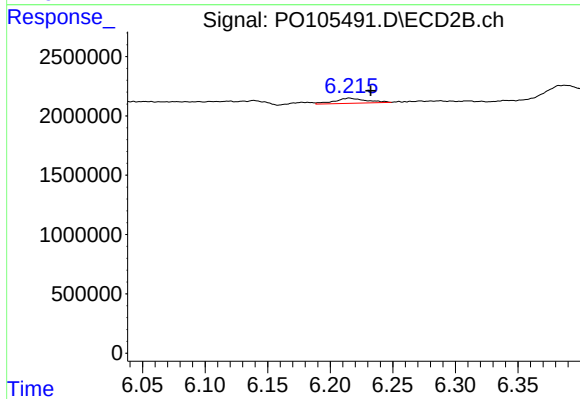

#32 AR-1260-2


R.T.: 6.215 min
Delta R.T.: -0.017 min
Response: 764413
Conc: 4.04 ng/ml

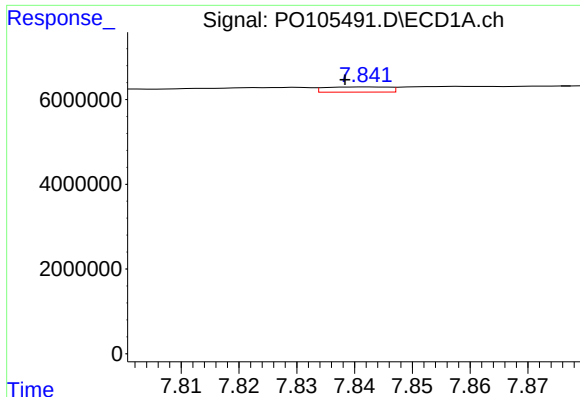

#33 AR-1260-3


R.T.: 7.842 min
Delta R.T.: 0.004 min
Response: 944211
Conc: 3.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

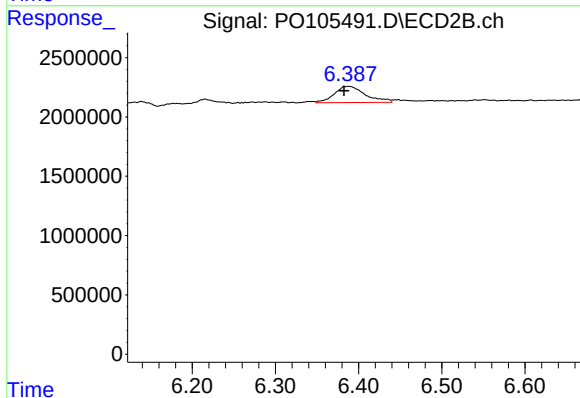


#33 AR-1260-3

R.T.: 6.388 min
Delta R.T.: 0.005 min
Response: 3567376
Conc: 19.31 ng/ml

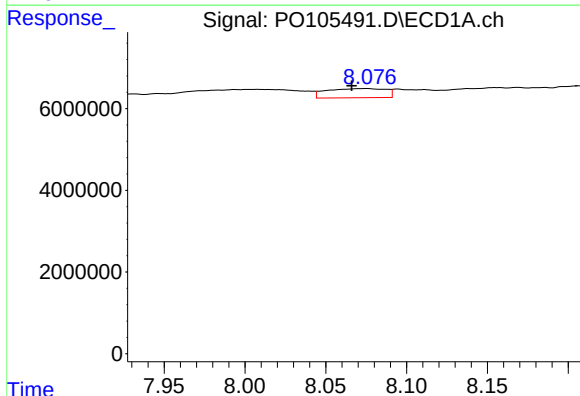


#34 AR-1260-4

R.T.: 8.076 min
Delta R.T.: 0.010 min
Response: 5736532
Conc: 17.39 ng/ml

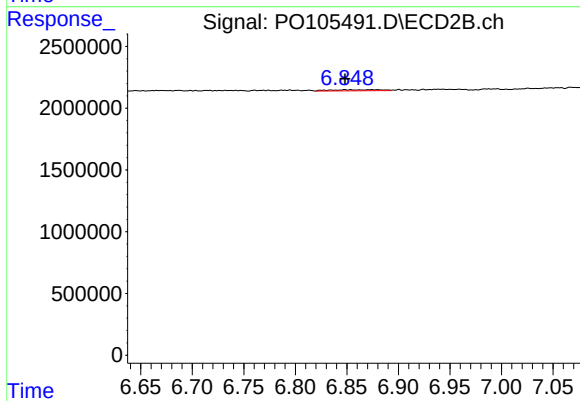

#34 AR-1260-4


R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 285409
Conc: 2.34 ng/ml

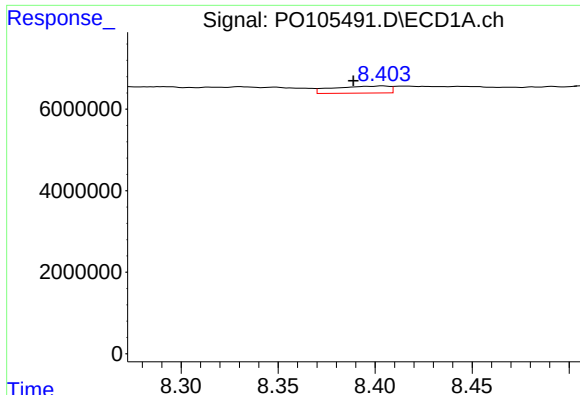

#35 AR-1260-5


R.T.: 8.404 min
Delta R.T.: 0.015 min
Response: 3499740
Conc: 5.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

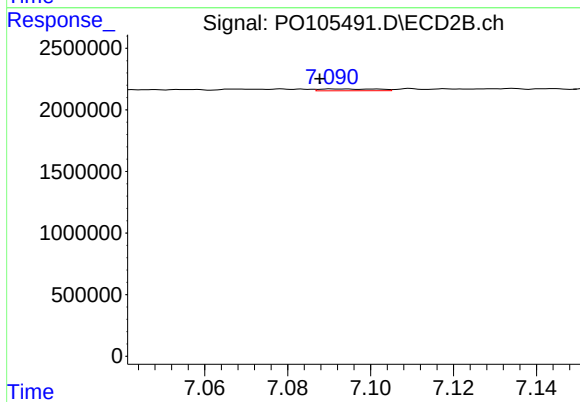


#35 AR-1260-5

R.T.: 7.092 min
Delta R.T.: 0.005 min
Response: 143954
Conc: 0.52 ng/ml

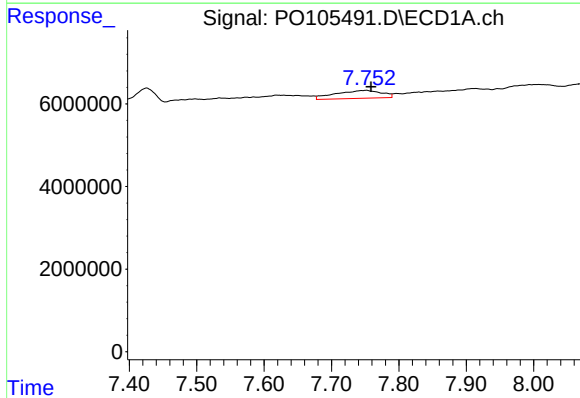


#36 AR-1262-1

R.T.: 7.752 min
Delta R.T.: -0.007 min
Response: 9136650
Conc: 28.76 ng/ml

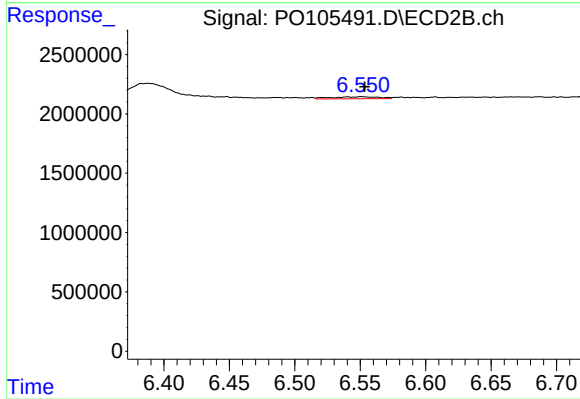

#36 AR-1262-1


R.T.: 6.551 min
Delta R.T.: -0.002 min
Response: 433639
Conc: 4.08 ng/ml

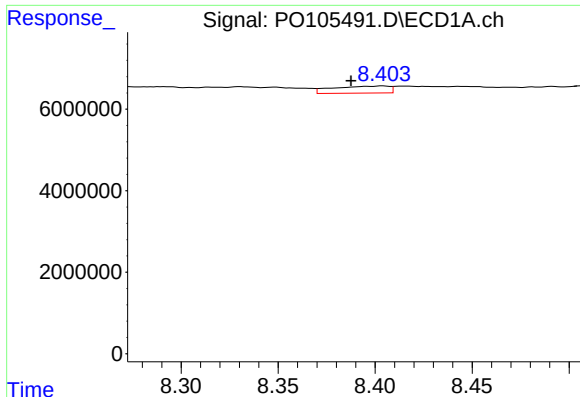

#37 AR-1262-2


R.T.: 8.404 min
Delta R.T.: 0.017 min
Response: 3499740
Conc: 4.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

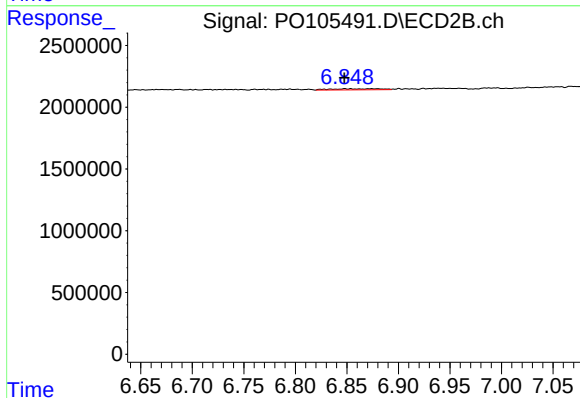


#37 AR-1262-2

R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 285409
Conc: 1.68 ng/ml

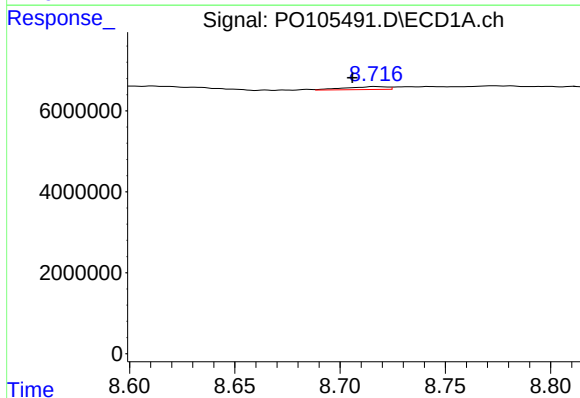


#38 AR-1262-3

R.T.: 8.717 min
Delta R.T.: 0.011 min
Response: 1011522
Conc: 2.06 ng/ml

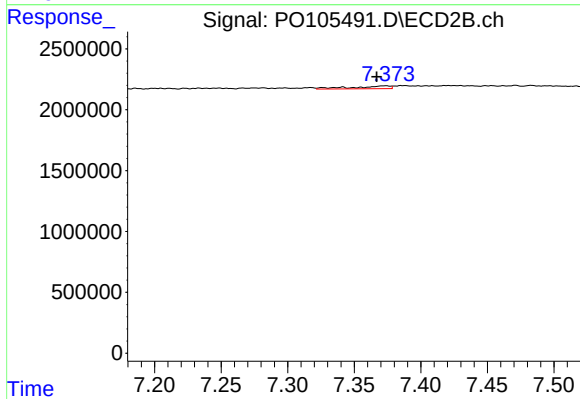

#38 AR-1262-3


R.T.: 7.373 min
Delta R.T.: 0.006 min
Response: 462109
Conc: 3.66 ng/ml

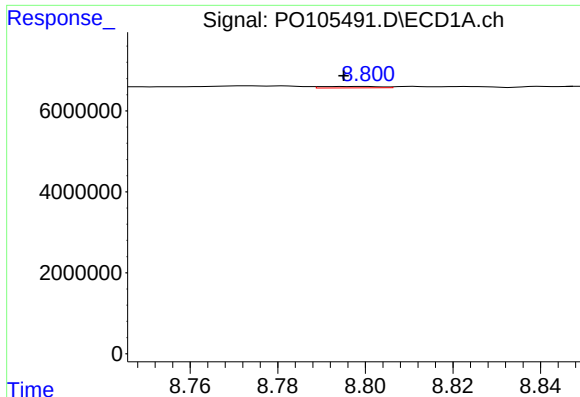

#39 AR-1262-4


R.T.: 8.799 min
Delta R.T.: 0.004 min
Response: 339667
Conc: 0.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

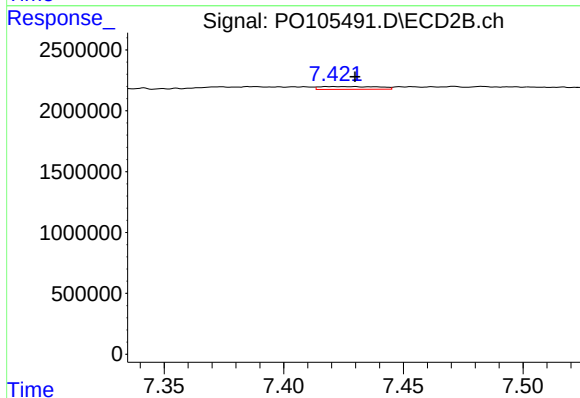


#39 AR-1262-4

R.T.: 7.420 min
Delta R.T.: -0.010 min
Response: 390926
Conc: 1.69 ng/ml

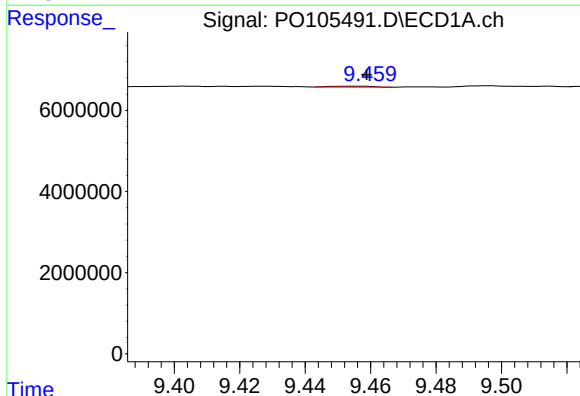


#40 AR-1262-5

R.T.: 9.458 min
Delta R.T.: 0.000 min
Response: 196927
Conc: 0.74 ng/ml

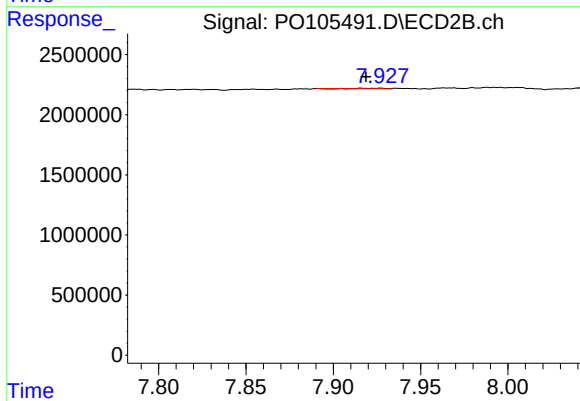

#40 AR-1262-5


R.T.: 7.927 min
Delta R.T.: 0.008 min
Response: 37089
Conc: 0.37 ng/ml

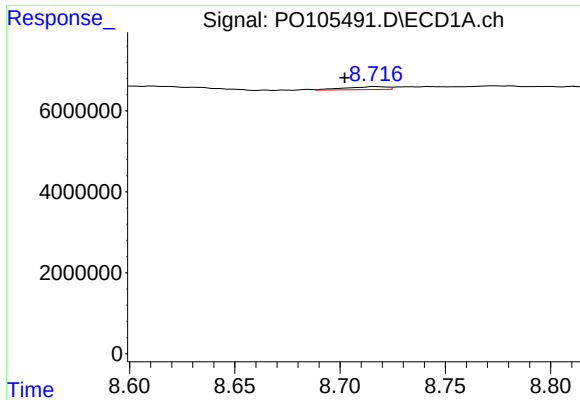

#41 AR-1268-1


R.T.: 8.717 min
Delta R.T.: 0.015 min
Response: 1011522
Conc: 1.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

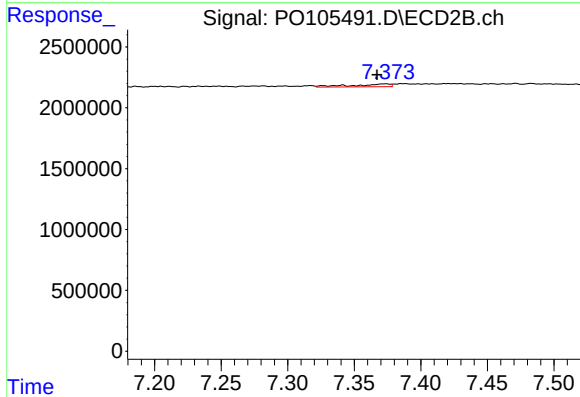


#41 AR-1268-1

R.T.: 7.373 min
Delta R.T.: 0.006 min
Response: 462109
Conc: 1.32 ng/ml

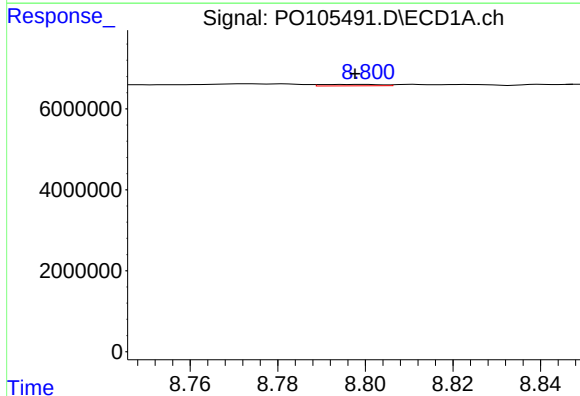


#42 AR-1268-2

R.T.: 8.799 min
Delta R.T.: 0.002 min
Response: 339667
Conc: 0.47 ng/ml

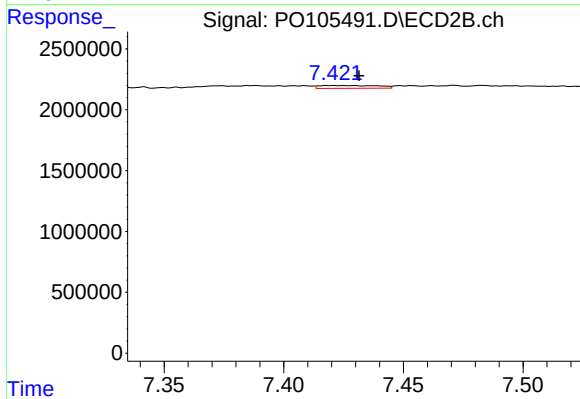

#42 AR-1268-2


R.T.: 7.420 min
Delta R.T.: -0.011 min
Response: 390926
Conc: 1.25 ng/ml

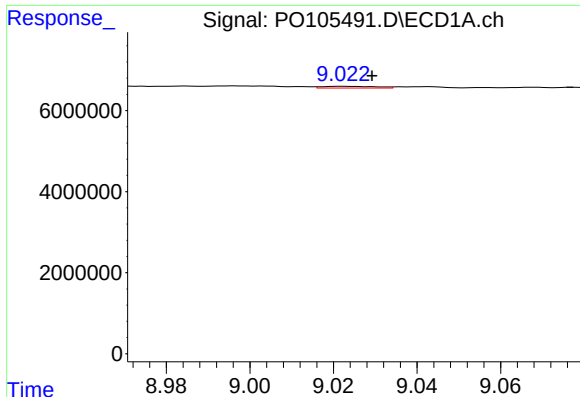

#43 AR-1268-3


R.T.: 9.022 min
Delta R.T.: -0.007 min
Response: 390829
Conc: 0.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

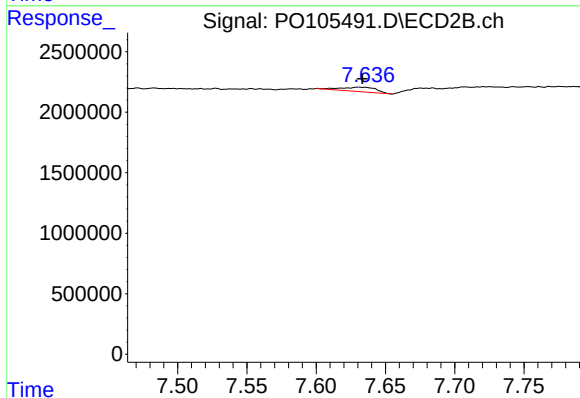


#43 AR-1268-3

R.T.: 7.631 min
Delta R.T.: -0.003 min
Response: 650233
Conc: 2.57 ng/ml

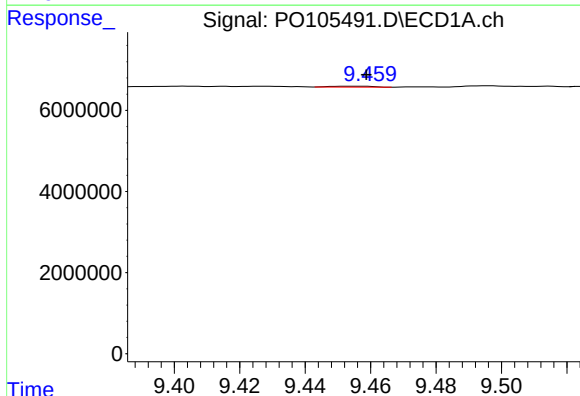


#44 AR-1268-4

R.T.: 9.458 min
Delta R.T.: 0.000 min
Response: 196927
Conc: 0.71 ng/ml

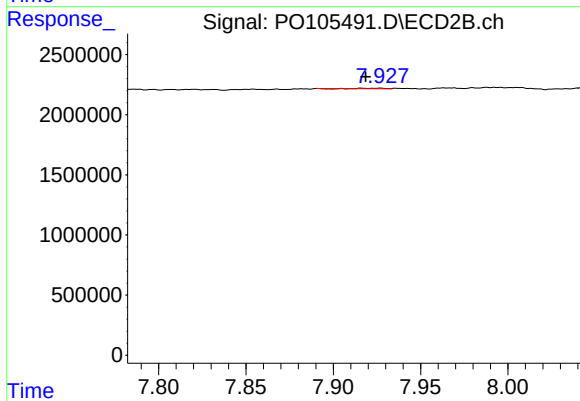

#44 AR-1268-4


R.T.: 7.927 min
Delta R.T.: 0.008 min
Response: 37089
Conc: 0.34 ng/ml

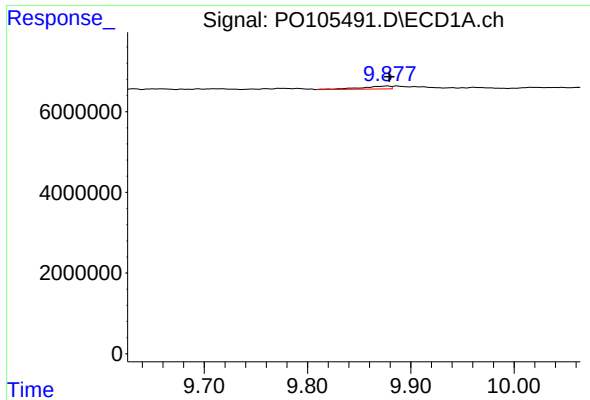

#45 AR-1268-5

R.T.: 9.877 min
Delta R.T.: -0.002 min
Response: 1362114
Conc: 0.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

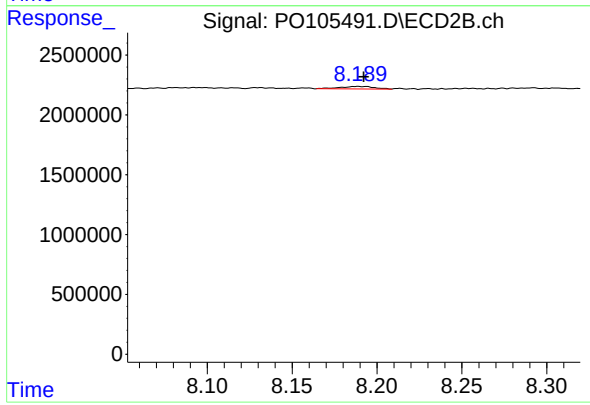

#45 AR-1268-5

R.T.: 8.188 min
Delta R.T.: -0.004 min
Response: 298602
Conc: 0.45 ng/ml