

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081324\
 Data File : P0105493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 12:50
 Operator : YP/AJ
 Sample : P3390-09
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:06:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.426	3.535	99884402	44590234	11.436	14.196
2)	SA Decachlor...	10.215	8.425	76919416	27919535	13.371	15.771
Target Compounds							
3)	L1 AR-1016-1	5.597	4.588	4018558	1914803	13.284	17.038 #
4)	L1 AR-1016-2	5.620	4.606	5707541	2442940	13.351	15.692
5)	L1 AR-1016-3	5.682	4.779	3276678	1387861	12.770	16.572 #
6)	L1 AR-1016-4	5.781	4.821	3477053	1096324	15.898	16.281
7)	L1 AR-1016-5	6.078	5.028	3475168	1562898	16.242	18.674
8)	L2 AR-1221-1	4.627	3.739	879693	269504	7.844	6.828
9)	L2 AR-1221-2	4.731	3.825	3066578	1108478	36.179	36.080
10)	L2 AR-1221-3	4.795	3.899	3243562	1061050	13.332	11.858
11)	L3 AR-1232-1	4.795	3.899	3243562	1061050	16.223	14.529
12)	L3 AR-1232-2	5.328	4.606	3066682	2442940	28.972	34.793
13)	L3 AR-1232-3	5.620	4.779	5707541	1387861	29.819	36.315
14)	L3 AR-1232-4	5.781	4.861	3477053	1478749	35.650	42.505
15)	L3 AR-1232-5	5.872	5.028	2272744	1562898	31.538	44.277 #
16)	L4 AR-1242-1	5.597	4.588	4018558	1914803	17.291	21.710 #
17)	L4 AR-1242-2	5.620	4.606	5707541	2442940	17.513	20.575
18)	L4 AR-1242-3	5.682	4.779	3276678	1387861	16.610	21.373 #
19)	L4 AR-1242-4	5.781	4.861	3477053	1478749	20.379	22.297
20)	L4 AR-1242-5	6.524	5.373	4140795	1876751	23.693	22.839
21)	L5 AR-1248-1	5.597	4.588	4018558	1914803	22.008	27.416
22)	L5 AR-1248-2	5.872	4.821	2272744	1096324	9.023	11.553 #
23)	L5 AR-1248-3	6.078	4.861	3475168	1478749	12.294	14.814
24)	L5 AR-1248-4	6.484	5.028	4045799	1562898	12.653	13.847
25)	L5 AR-1248-5	6.524	5.412	4140795	1667806	13.387	14.811
26)	L6 AR-1254-1	6.457	5.373	3607557	1876751	11.504	11.528
27)	L6 AR-1254-2	6.683	5.519	2594640	751751	5.750	5.139
28)	L6 AR-1254-3	7.050	5.915	4109459	840467	8.663	3.726 #
29)	L6 AR-1254-4	7.337	6.140	1705216	632799	4.760	4.484
30)	L6 AR-1254-5	7.747	6.557	6494714	381991	16.361	1.907 #
31)	L7 AR-1260-1	7.228	6.044	999394	147488	2.727	0.945 #
32)	L7 AR-1260-2	7.465	6.215	849814	544840	2.041	2.883 #
33)	L7 AR-1260-3	7.834	6.388	701806	3276193	2.712	17.735 #
34)	L7 AR-1260-4	8.053	6.864	2119285	146991	6.423	1.203 #
35)	L7 AR-1260-5	8.400	7.086	2661952	127419	4.475	0.458 #
36)	L8 AR-1262-1	7.747	6.557	6494714	381991	20.447	3.590 #
37)	L8 AR-1262-2	8.400	6.864	2661952	146991	3.539	0.865 #
38)	L8 AR-1262-3	8.690	7.377	238731	260413	0.485	2.063 #
39)	L8 AR-1262-4	8.800	7.422	115255	247322	0.314	1.068 #
40)	L8 AR-1262-5	9.453	7.910	78660	74627	0.294	0.743 #
41)	L9 AR-1268-1	8.690	7.377	238731	260413	0.294	0.746 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081324\
Data File : P0105493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 12:50
Operator : YP/AJ
Sample : P3390-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:06:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.800	7.422	115255	247322	0.159	0.793 #
43)	L9 AR-1268-3	9.022	7.630	821619	1295596	1.273	5.126 #
44)	L9 AR-1268-4	9.453	7.910	78660	74627	0.282	0.694 #
45)	L9 AR-1268-5	9.875	8.187	393151	247554	0.188	0.370 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081324\
Data File : PO105493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 12:50
Operator : YP/AJ
Sample : P3390-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:06:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

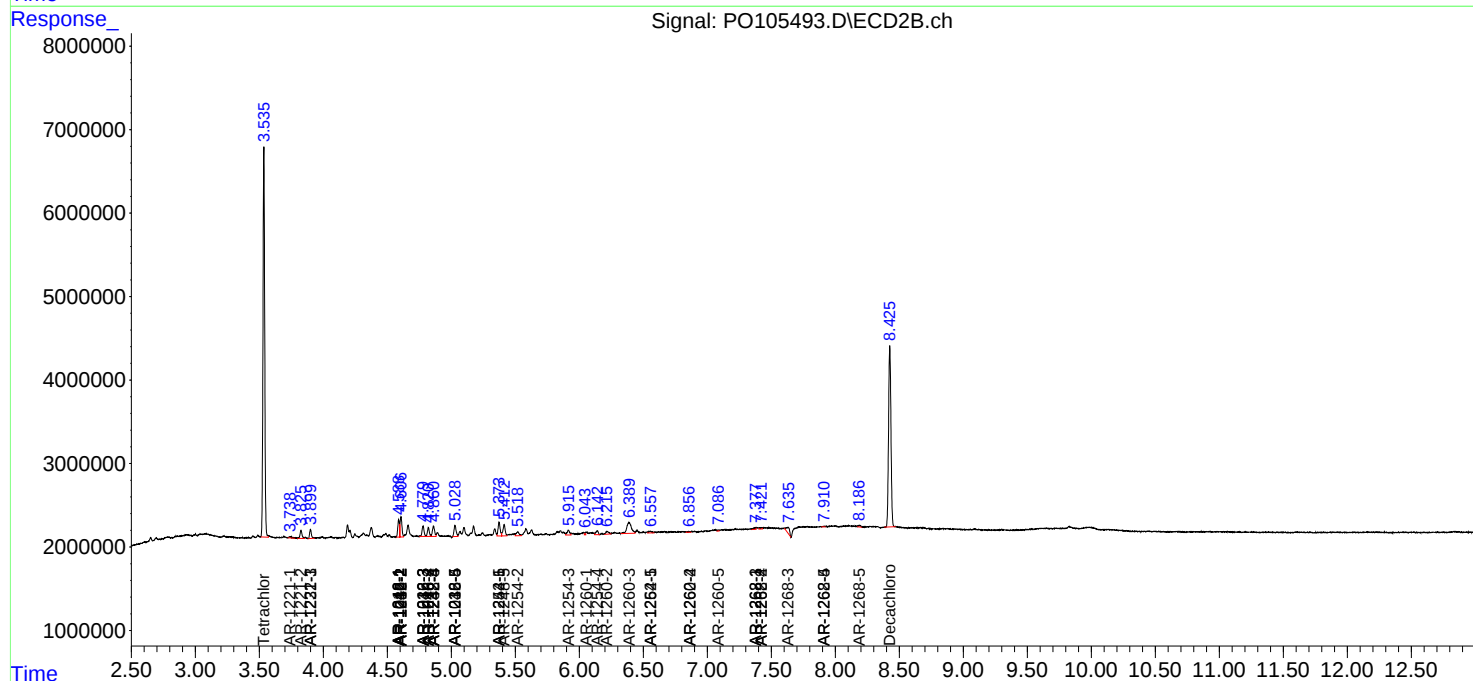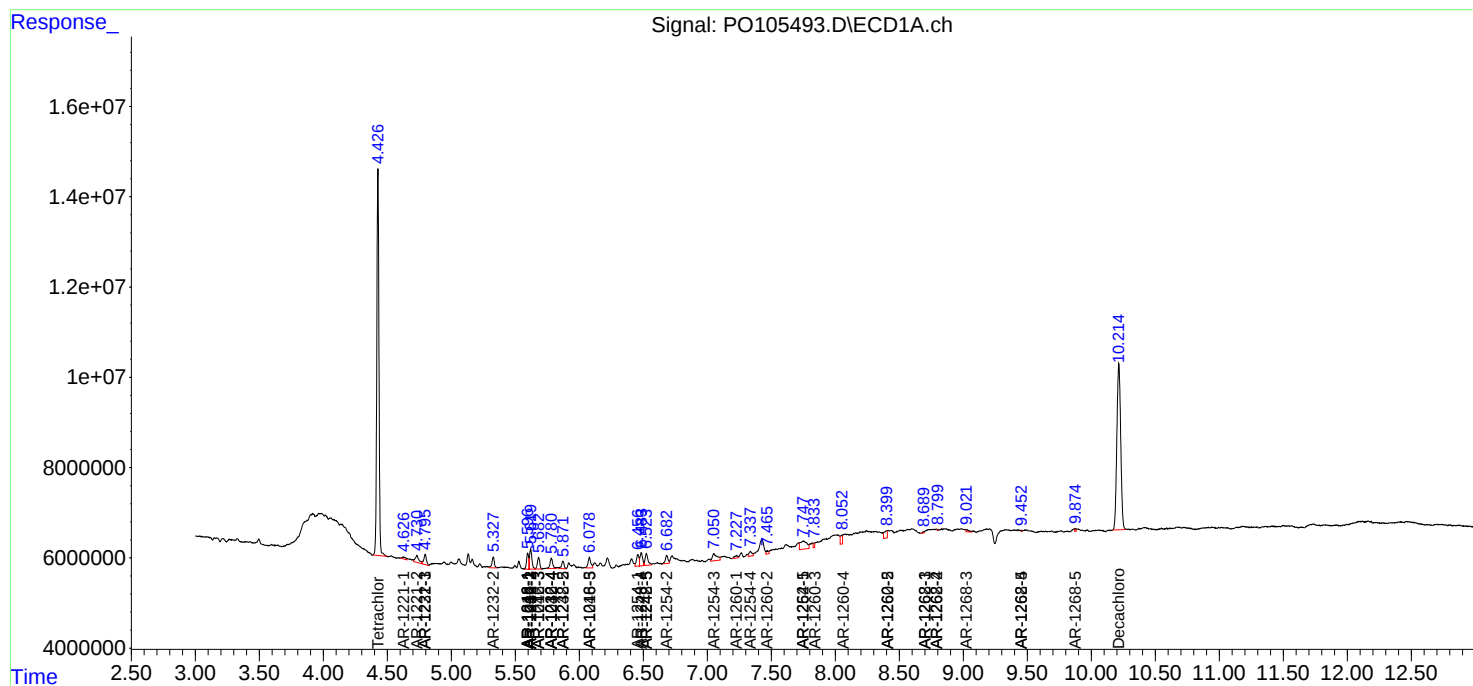


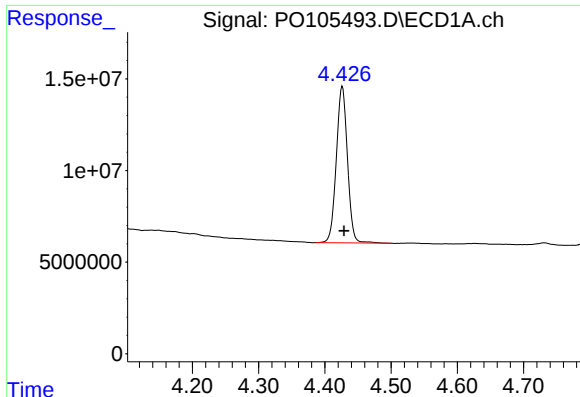

#1 Tetrachloro-m-xylene


R.T.: 4.426 min
Delta R.T.: -0.003 min
Response: 99884402
Conc: 11.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

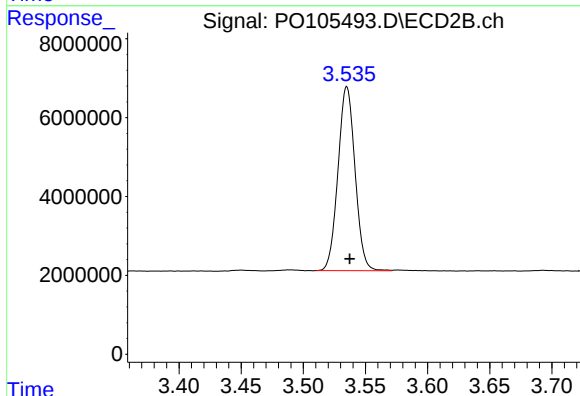


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.002 min
Response: 44590234
Conc: 14.20 ng/ml

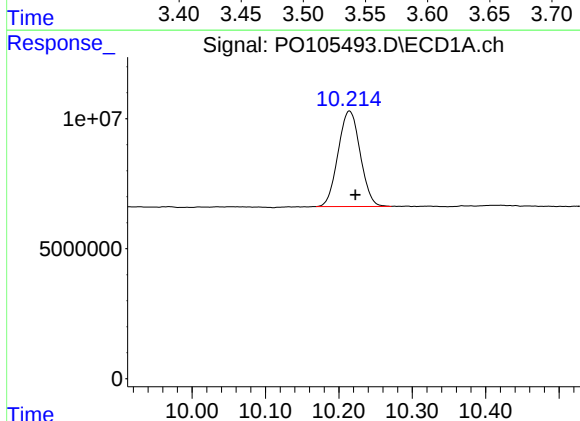


#2 Decachlorobiphenyl

R.T.: 10.215 min
Delta R.T.: -0.008 min
Response: 76919416
Conc: 13.37 ng/ml

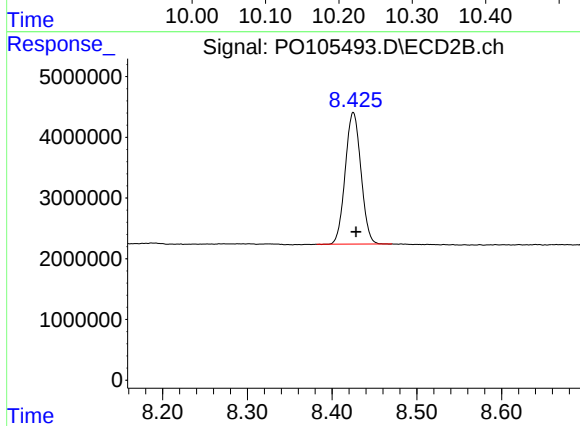

#2 Decachlorobiphenyl


R.T.: 8.425 min
Delta R.T.: -0.003 min
Response: 27919535
Conc: 15.77 ng/ml

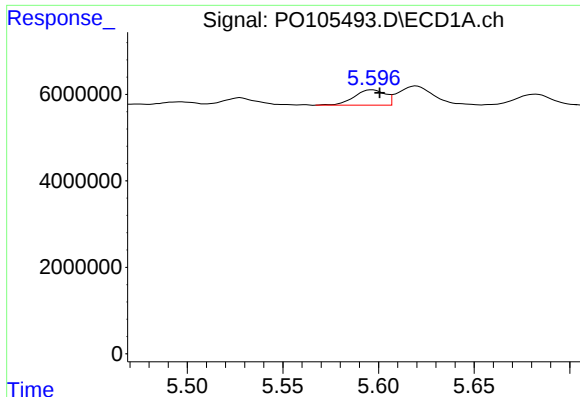

#3 AR-1016-1


R.T.: 5.597 min
Delta R.T.: -0.004 min
Response: 4018558
Conc: 13.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

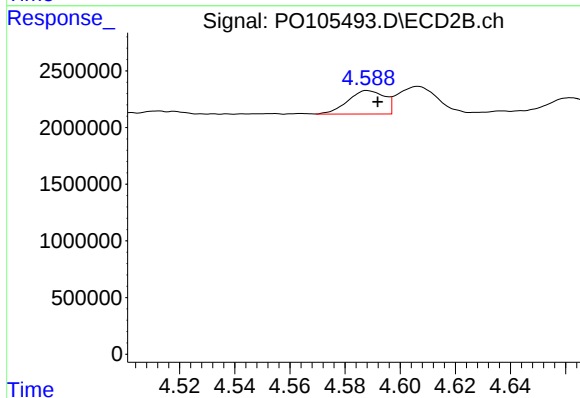


#3 AR-1016-1

R.T.: 4.588 min
Delta R.T.: -0.004 min
Response: 1914803
Conc: 17.04 ng/ml

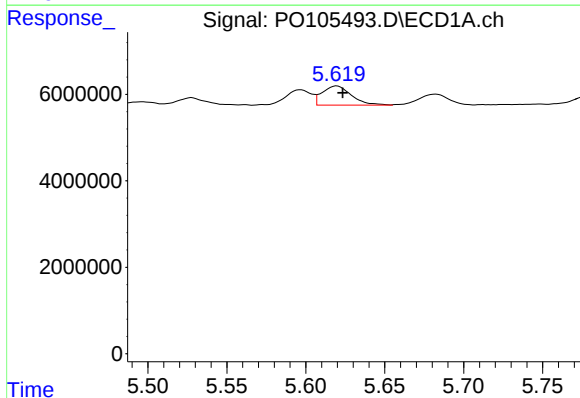


#4 AR-1016-2

R.T.: 5.620 min
Delta R.T.: -0.004 min
Response: 5707541
Conc: 13.35 ng/ml

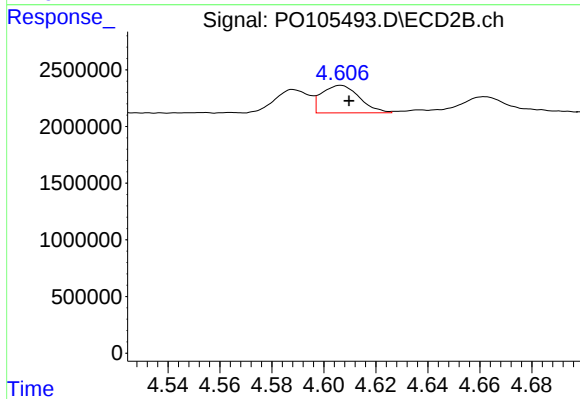

#4 AR-1016-2


R.T.: 4.606 min
Delta R.T.: -0.003 min
Response: 2442940
Conc: 15.69 ng/ml

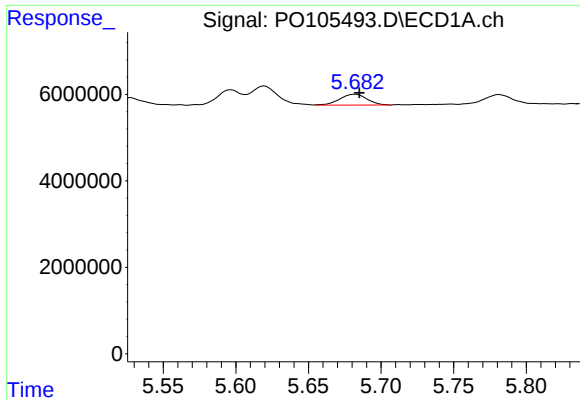

#5 AR-1016-3


R.T.: 5.682 min
Delta R.T.: -0.003 min
Response: 3276678
Conc: 12.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

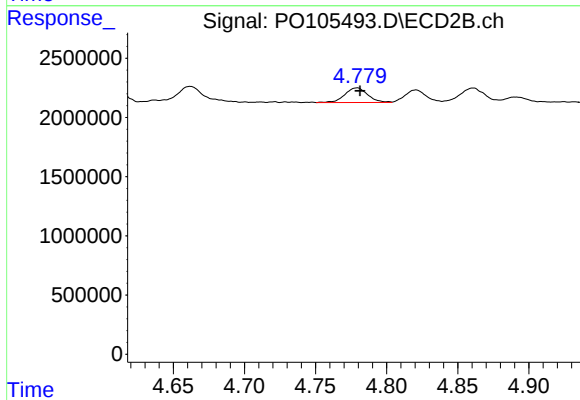


#5 AR-1016-3

R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 1387861
Conc: 16.57 ng/ml

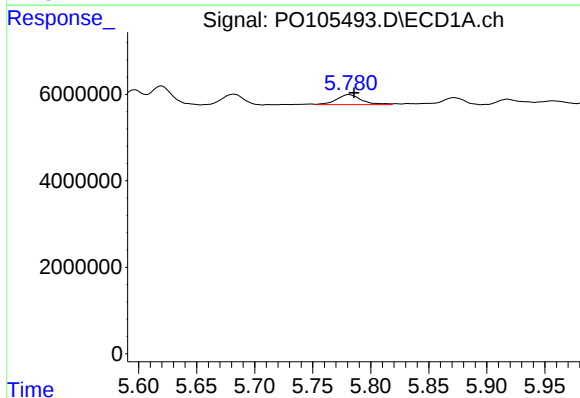


#6 AR-1016-4

R.T.: 5.781 min
Delta R.T.: -0.004 min
Response: 3477053
Conc: 15.90 ng/ml

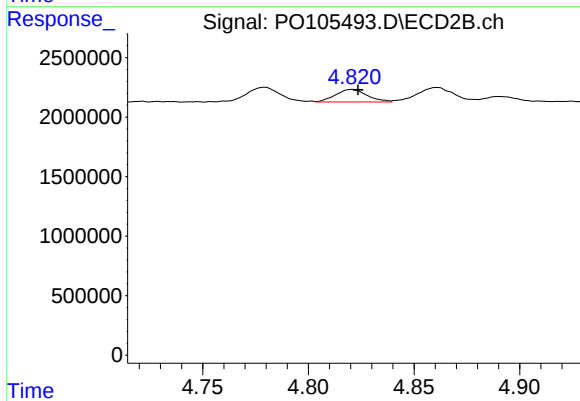

#6 AR-1016-4


R.T.: 4.821 min
Delta R.T.: -0.003 min
Response: 1096324
Conc: 16.28 ng/ml

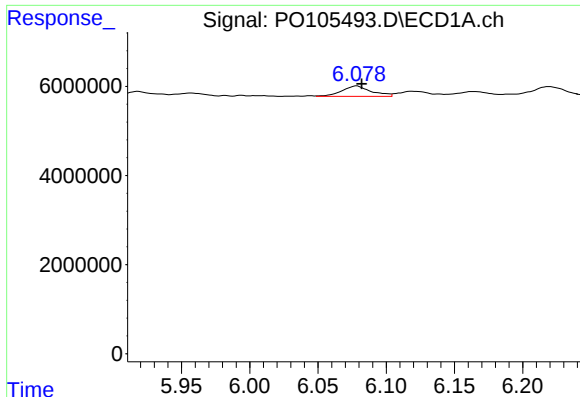

#7 AR-1016-5


R.T.: 6.078 min
Delta R.T.: -0.004 min
Response: 3475168
Conc: 16.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

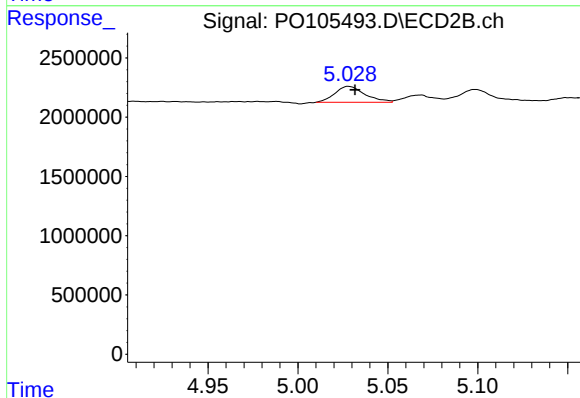


#7 AR-1016-5

R.T.: 5.028 min
Delta R.T.: -0.004 min
Response: 1562898
Conc: 18.67 ng/ml

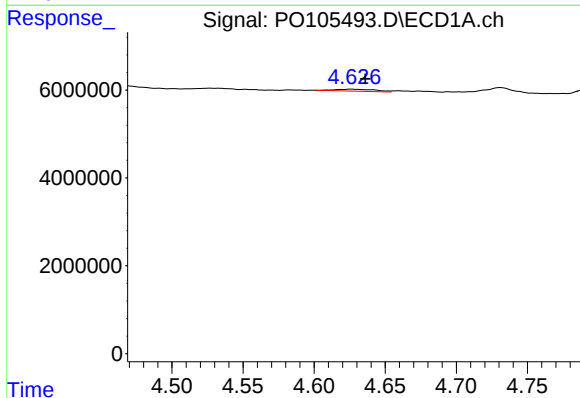


#8 AR-1221-1

R.T.: 4.627 min
Delta R.T.: -0.009 min
Response: 879693
Conc: 7.84 ng/ml

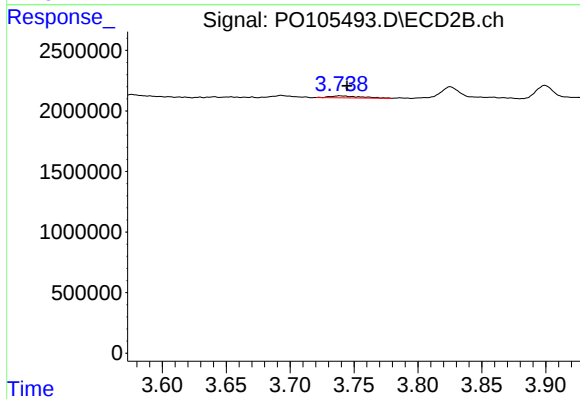

#8 AR-1221-1


R.T.: 3.739 min
Delta R.T.: -0.006 min
Response: 269504
Conc: 6.83 ng/ml

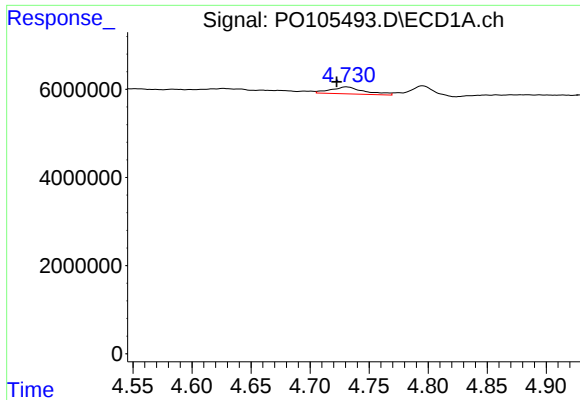

#9 AR-1221-2


R.T.: 4.731 min
Delta R.T.: 0.008 min
Response: 3066578
Conc: 36.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

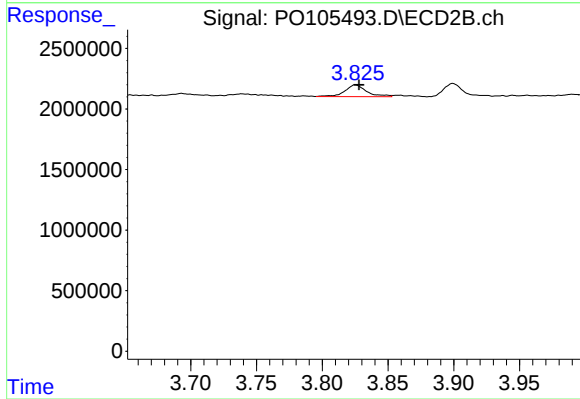


#9 AR-1221-2

R.T.: 3.825 min
Delta R.T.: -0.003 min
Response: 1108478
Conc: 36.08 ng/ml

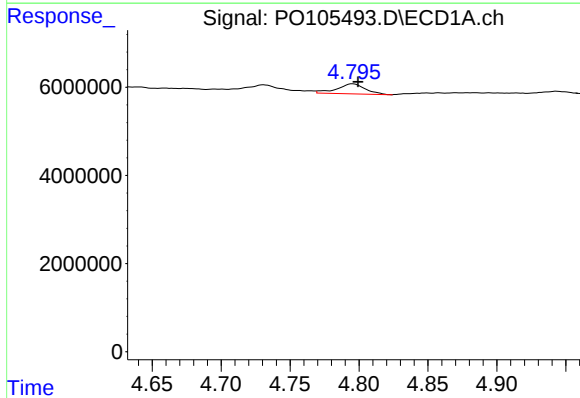


#10 AR-1221-3

R.T.: 4.795 min
Delta R.T.: -0.004 min
Response: 3243562
Conc: 13.33 ng/ml

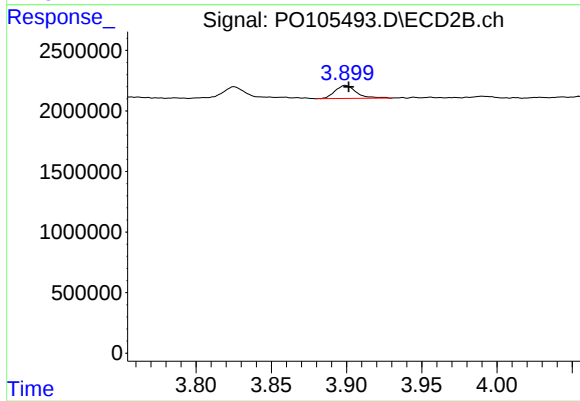

#10 AR-1221-3


R.T.: 3.899 min
Delta R.T.: -0.002 min
Response: 1061050
Conc: 11.86 ng/ml

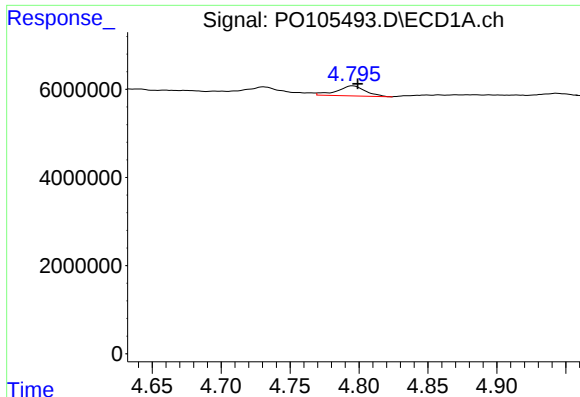

#11 AR-1232-1


R.T.: 4.795 min
Delta R.T.: -0.004 min
Response: 3243562
Conc: 16.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

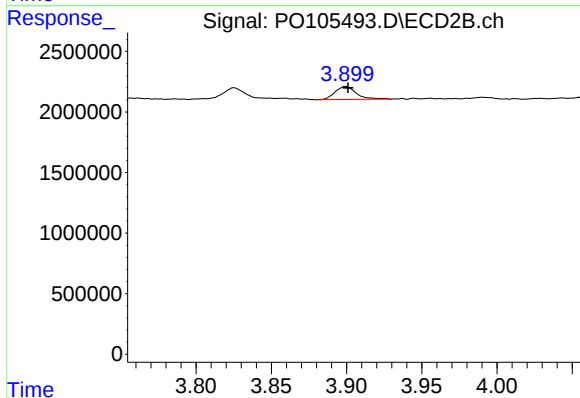


#11 AR-1232-1

R.T.: 3.899 min
Delta R.T.: -0.002 min
Response: 1061050
Conc: 14.53 ng/ml

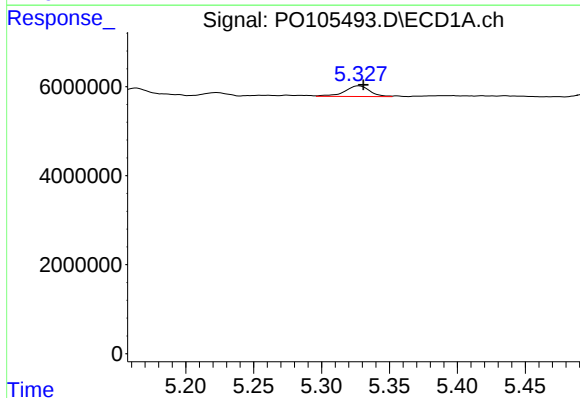


#12 AR-1232-2

R.T.: 5.328 min
Delta R.T.: -0.003 min
Response: 3066682
Conc: 28.97 ng/ml

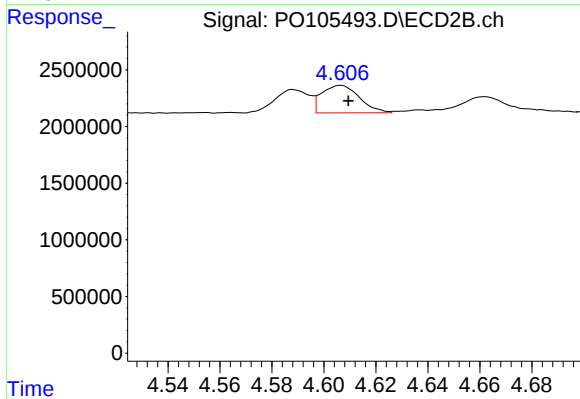

#12 AR-1232-2


R.T.: 4.606 min
Delta R.T.: -0.003 min
Response: 2442940
Conc: 34.79 ng/ml

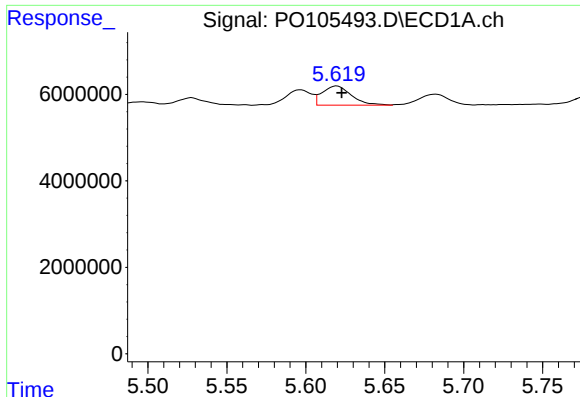

#13 AR-1232-3


R.T.: 5.620 min
Delta R.T.: -0.003 min
Response: 5707541
Conc: 29.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

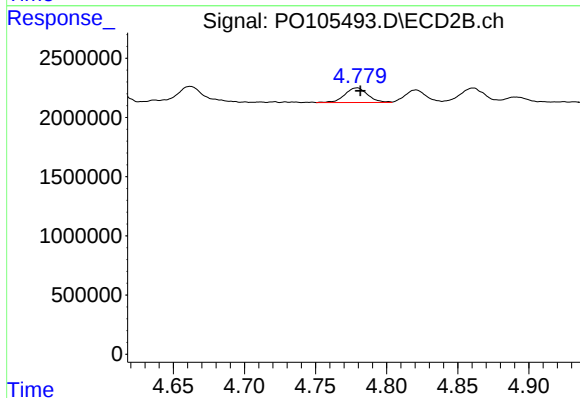


#13 AR-1232-3

R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 1387861
Conc: 36.31 ng/ml

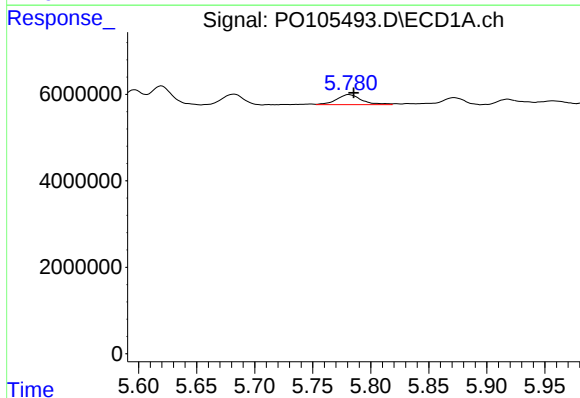


#14 AR-1232-4

R.T.: 5.781 min
Delta R.T.: -0.004 min
Response: 3477053
Conc: 35.65 ng/ml

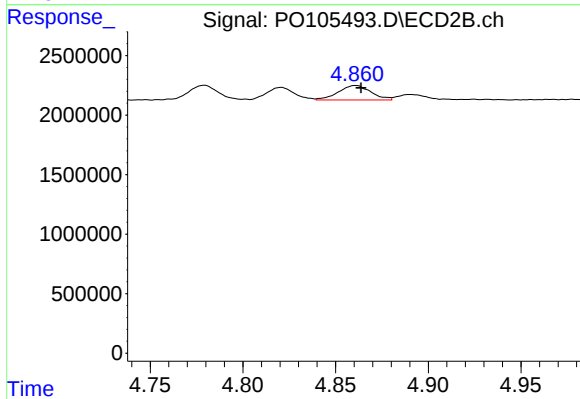

#14 AR-1232-4


R.T.: 4.861 min
Delta R.T.: -0.003 min
Response: 1478749
Conc: 42.51 ng/ml

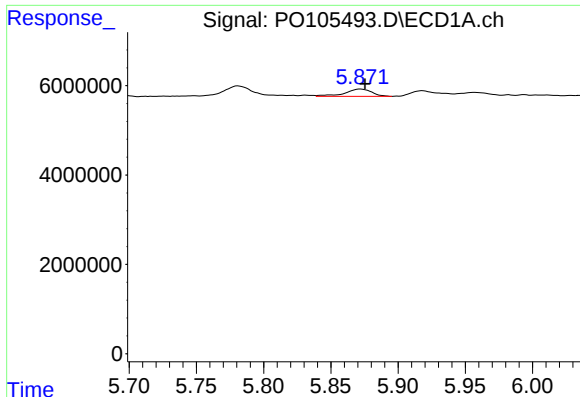

#15 AR-1232-5


R.T.: 5.872 min
Delta R.T.: -0.003 min
Response: 2272744
Conc: 31.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

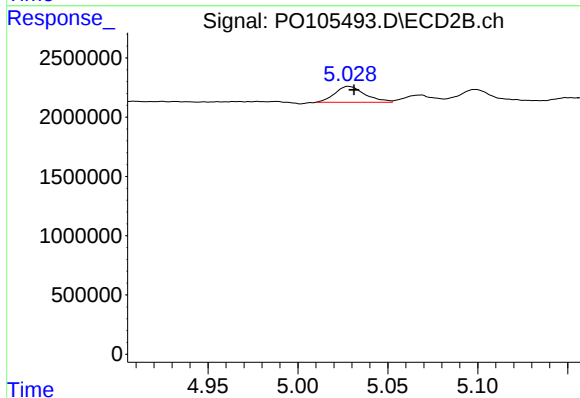


#15 AR-1232-5

R.T.: 5.028 min
Delta R.T.: -0.003 min
Response: 1562898
Conc: 44.28 ng/ml

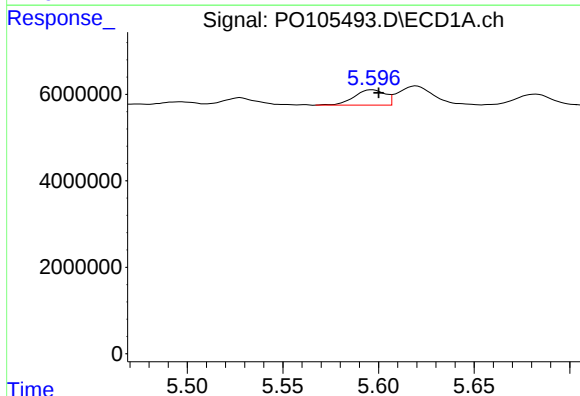


#16 AR-1242-1

R.T.: 5.597 min
Delta R.T.: -0.003 min
Response: 4018558
Conc: 17.29 ng/ml

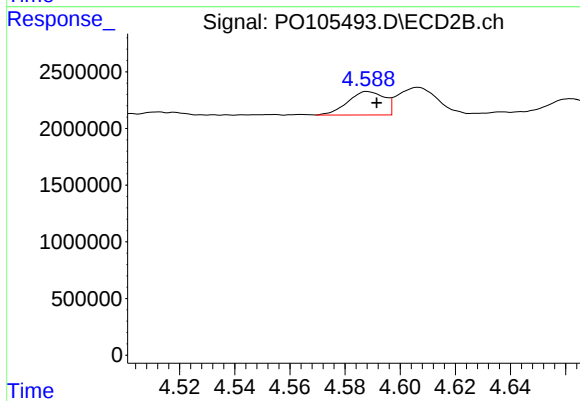

#16 AR-1242-1


R.T.: 4.588 min
Delta R.T.: -0.003 min
Response: 1914803
Conc: 21.71 ng/ml

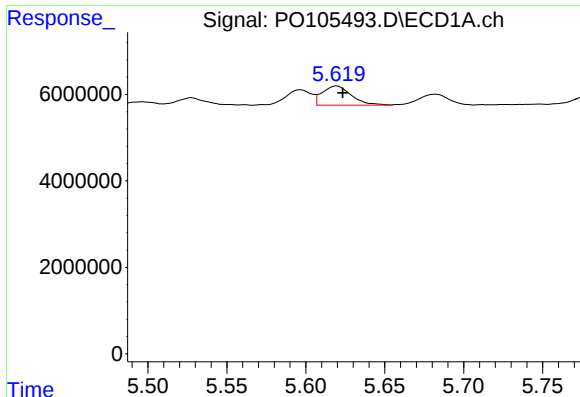

#17 AR-1242-2


R.T.: 5.620 min
Delta R.T.: -0.004 min
Response: 5707541
Conc: 17.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

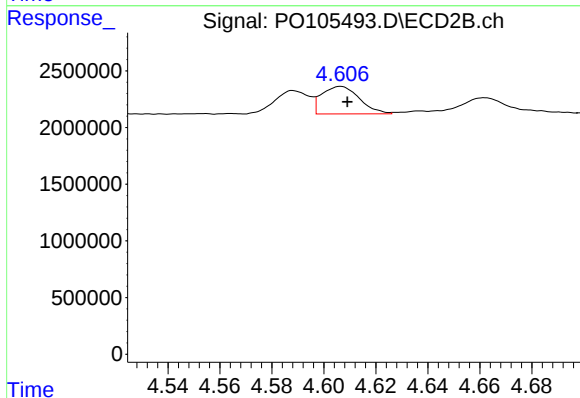


#17 AR-1242-2

R.T.: 4.606 min
Delta R.T.: -0.003 min
Response: 2442940
Conc: 20.58 ng/ml

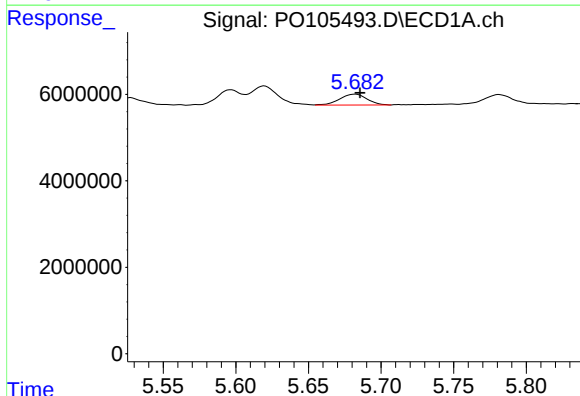


#18 AR-1242-3

R.T.: 5.682 min
Delta R.T.: -0.003 min
Response: 3276678
Conc: 16.61 ng/ml

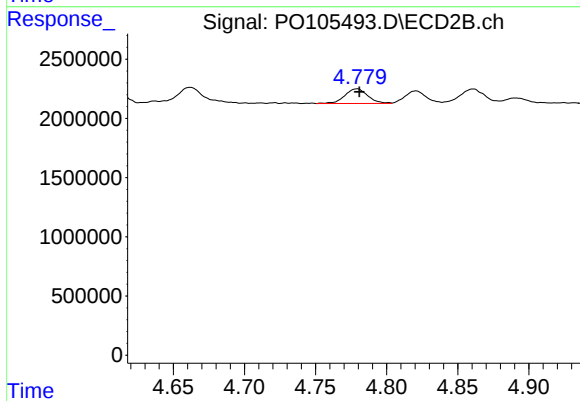

#18 AR-1242-3


R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 1387861
Conc: 21.37 ng/ml

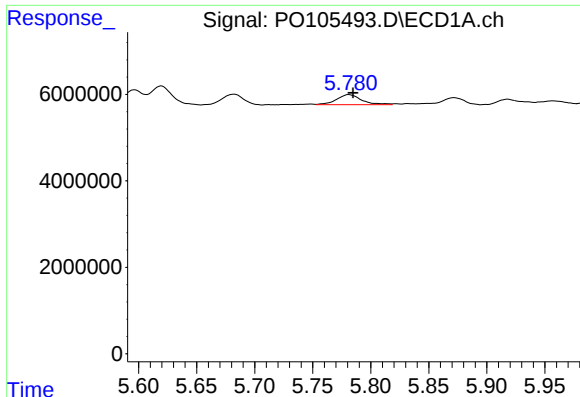

#19 AR-1242-4


R.T.: 5.781 min
Delta R.T.: -0.004 min
Response: 3477053
Conc: 20.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

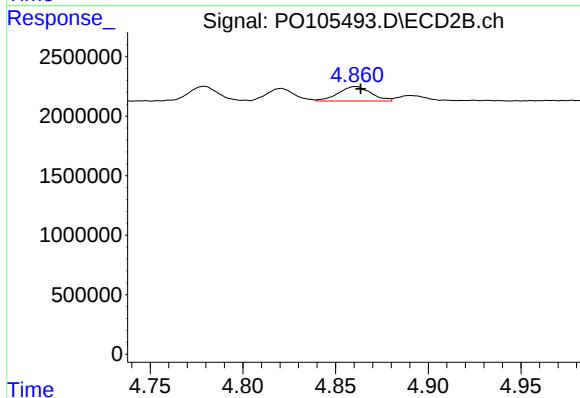


#19 AR-1242-4

R.T.: 4.861 min
Delta R.T.: -0.003 min
Response: 1478749
Conc: 22.30 ng/ml

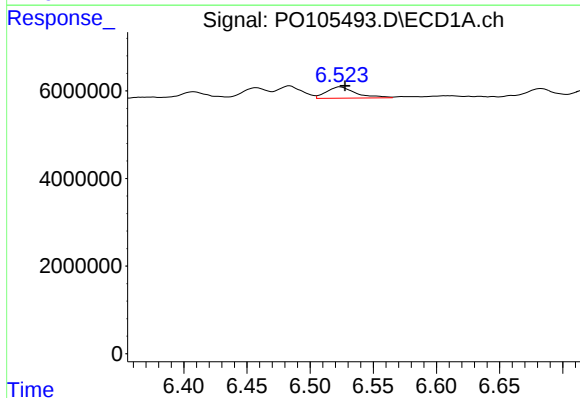


#20 AR-1242-5

R.T.: 6.524 min
Delta R.T.: -0.004 min
Response: 4140795
Conc: 23.69 ng/ml

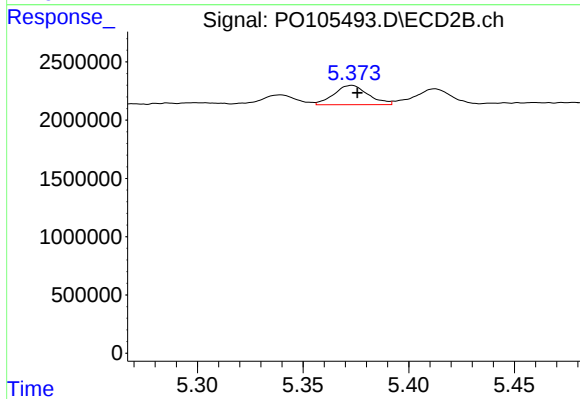

#20 AR-1242-5


R.T.: 5.373 min
Delta R.T.: -0.003 min
Response: 1876751
Conc: 22.84 ng/ml

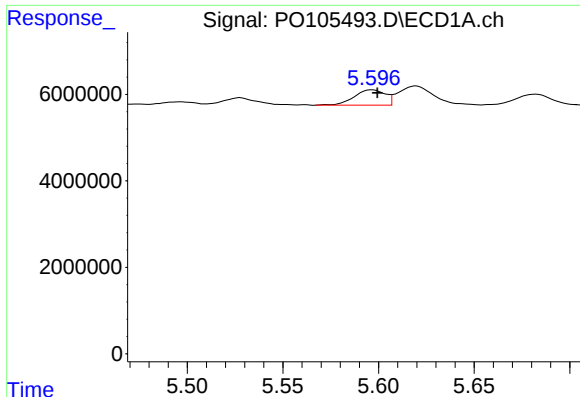

#21 AR-1248-1


R.T.: 5.597 min
Delta R.T.: -0.003 min
Response: 4018558
Conc: 22.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

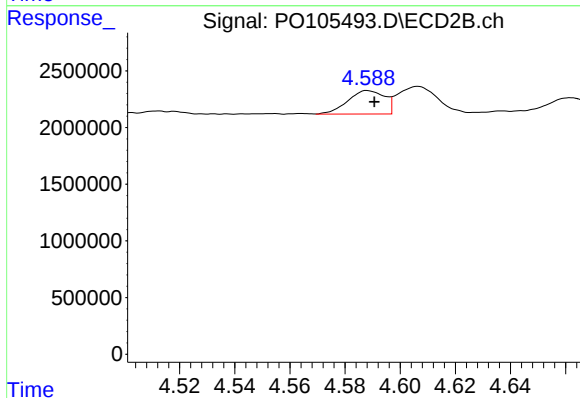


#21 AR-1248-1

R.T.: 4.588 min
Delta R.T.: -0.002 min
Response: 1914803
Conc: 27.42 ng/ml

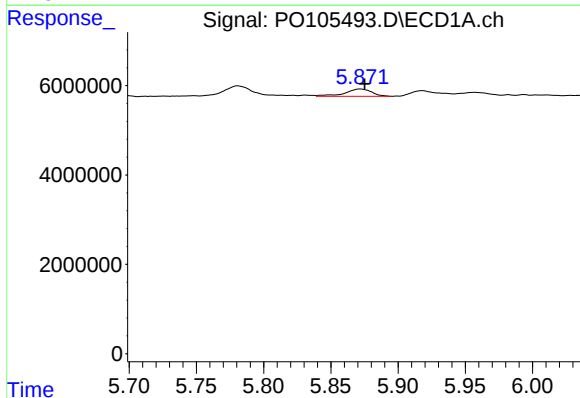


#22 AR-1248-2

R.T.: 5.872 min
Delta R.T.: -0.003 min
Response: 2272744
Conc: 9.02 ng/ml

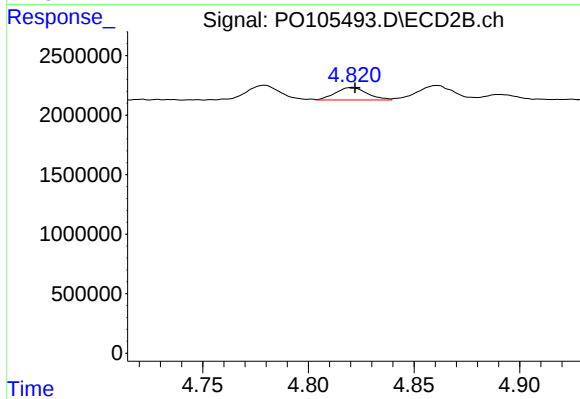

#22 AR-1248-2


R.T.: 4.821 min
Delta R.T.: -0.002 min
Response: 1096324
Conc: 11.55 ng/ml

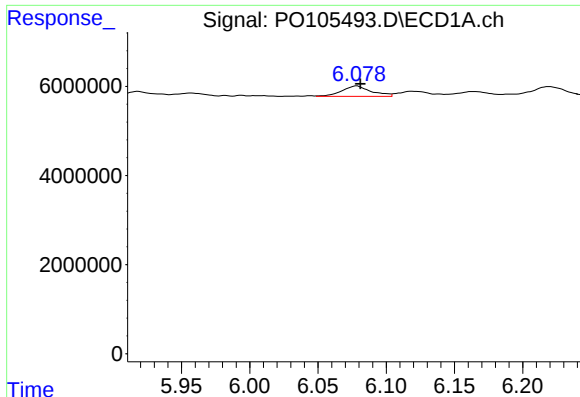

#23 AR-1248-3


R.T.: 6.078 min
Delta R.T.: -0.003 min
Response: 3475168
Conc: 12.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

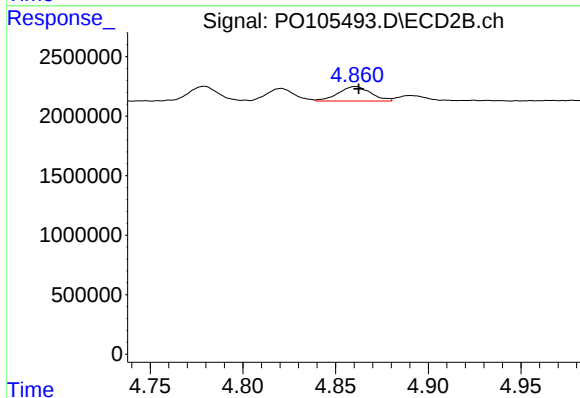


#23 AR-1248-3

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 1478749
Conc: 14.81 ng/ml

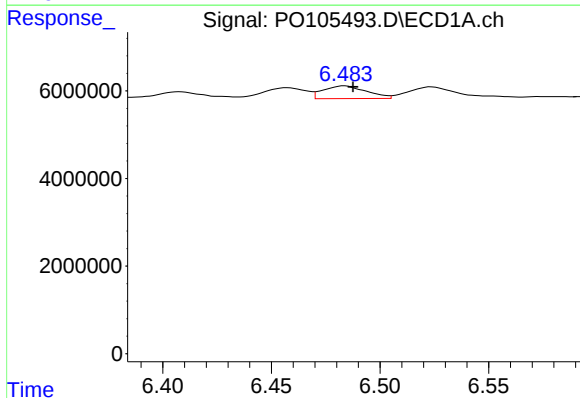


#24 AR-1248-4

R.T.: 6.484 min
Delta R.T.: -0.004 min
Response: 4045799
Conc: 12.65 ng/ml

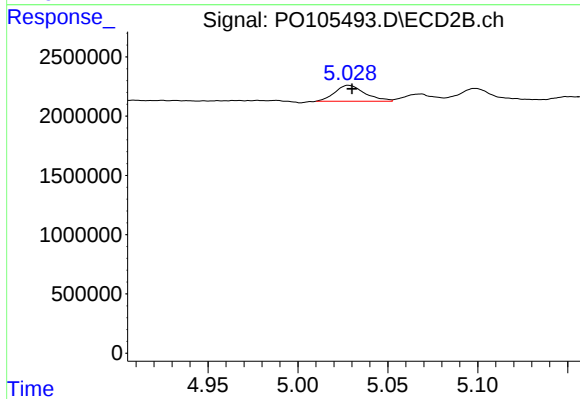

#24 AR-1248-4


R.T.: 5.028 min
Delta R.T.: -0.002 min
Response: 1562898
Conc: 13.85 ng/ml

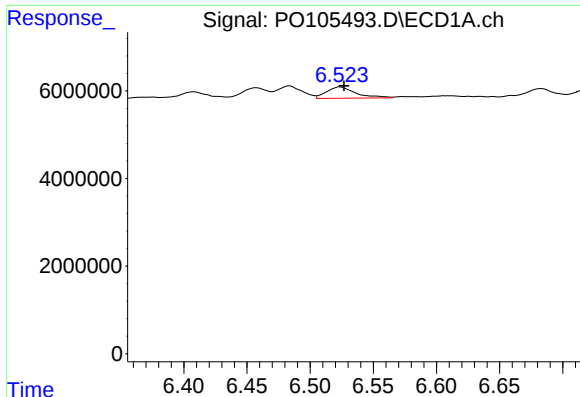

#25 AR-1248-5


R.T.: 6.524 min
Delta R.T.: -0.003 min
Response: 4140795
Conc: 13.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

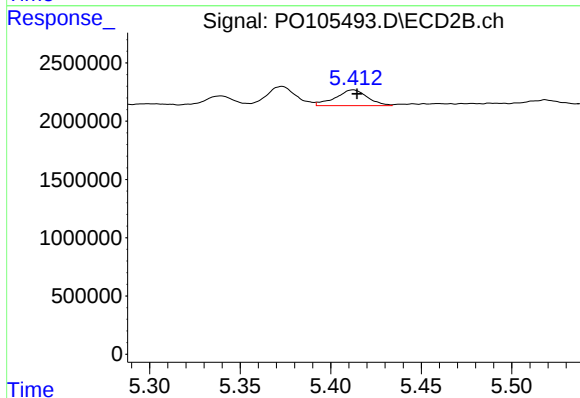


#25 AR-1248-5

R.T.: 5.412 min
Delta R.T.: -0.002 min
Response: 1667806
Conc: 14.81 ng/ml

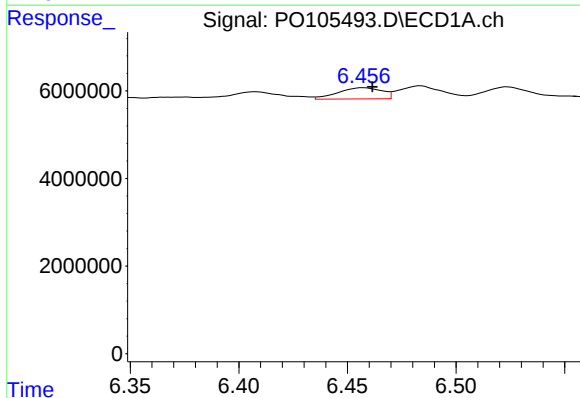


#26 AR-1254-1

R.T.: 6.457 min
Delta R.T.: -0.004 min
Response: 3607557
Conc: 11.50 ng/ml

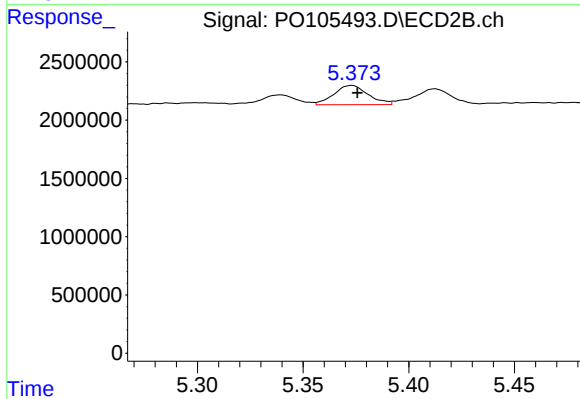

#26 AR-1254-1


R.T.: 5.373 min
Delta R.T.: -0.003 min
Response: 1876751
Conc: 11.53 ng/ml

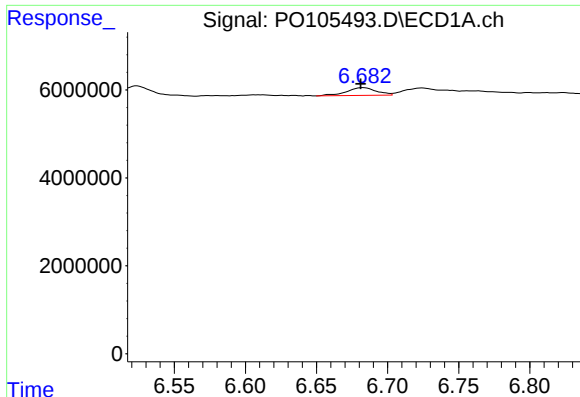

#27 AR-1254-2


R.T.: 6.683 min
Delta R.T.: 0.002 min
Response: 2594640
Conc: 5.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

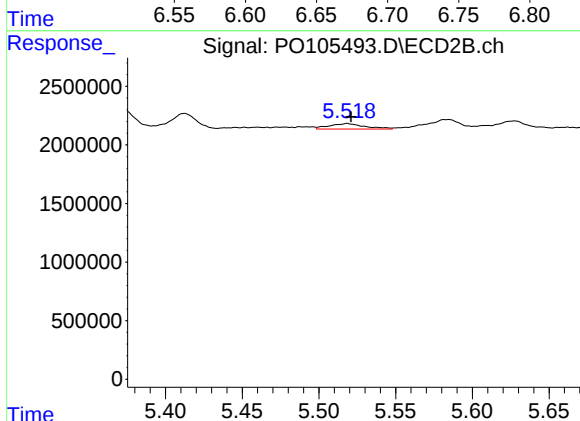


#27 AR-1254-2

R.T.: 5.519 min
Delta R.T.: -0.002 min
Response: 751751
Conc: 5.14 ng/ml

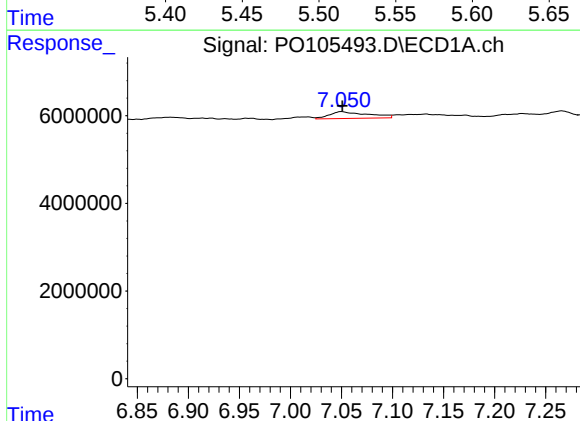


#28 AR-1254-3

R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 4109459
Conc: 8.66 ng/ml

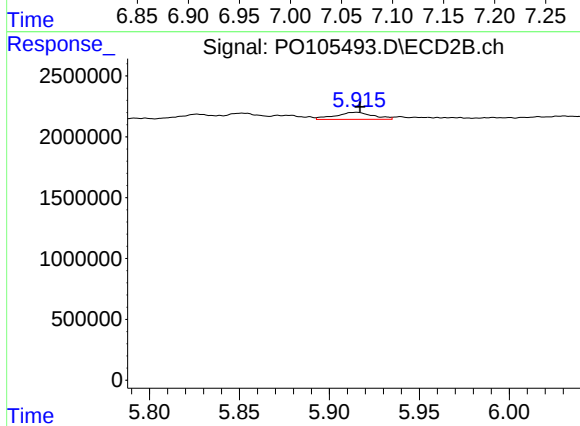

#28 AR-1254-3


R.T.: 5.915 min
Delta R.T.: -0.002 min
Response: 840467
Conc: 3.73 ng/ml

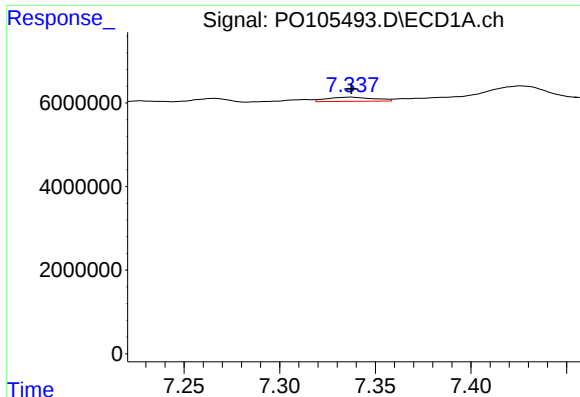

#29 AR-1254-4


R.T.: 7.337 min
Delta R.T.: 0.000 min
Response: 1705216
Conc: 4.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

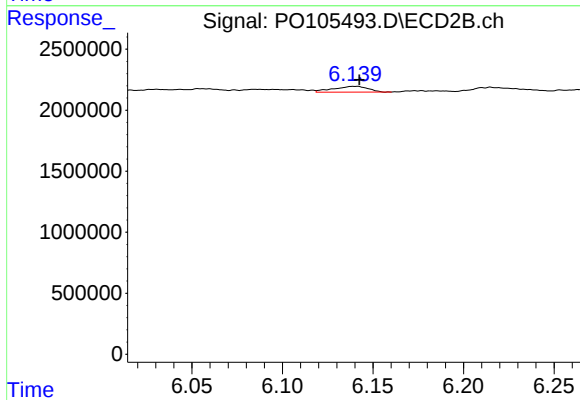


#29 AR-1254-4

R.T.: 6.140 min
Delta R.T.: -0.002 min
Response: 632799
Conc: 4.48 ng/ml

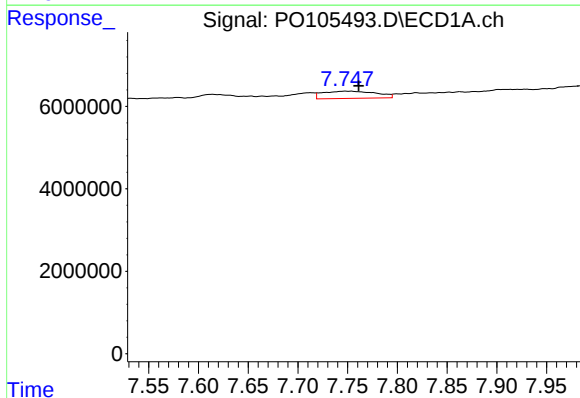


#30 AR-1254-5

R.T.: 7.747 min
Delta R.T.: -0.014 min
Response: 6494714
Conc: 16.36 ng/ml

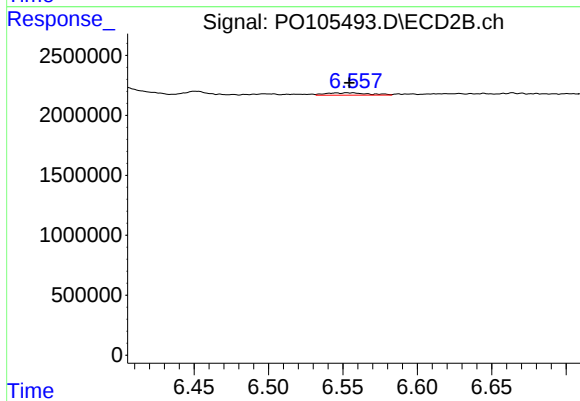

#30 AR-1254-5


R.T.: 6.557 min
Delta R.T.: 0.002 min
Response: 381991
Conc: 1.91 ng/ml

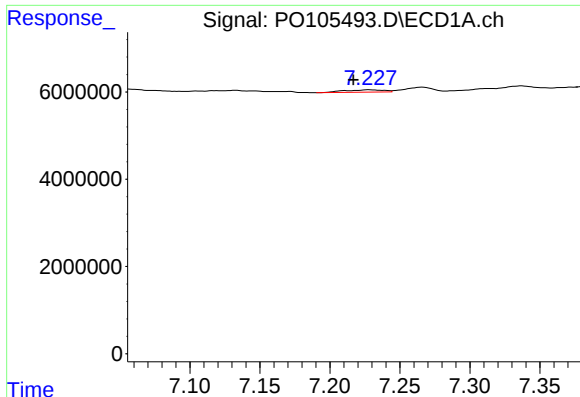

#31 AR-1260-1


R.T.: 7.228 min
Delta R.T.: 0.011 min
Response: 999394
Conc: 2.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

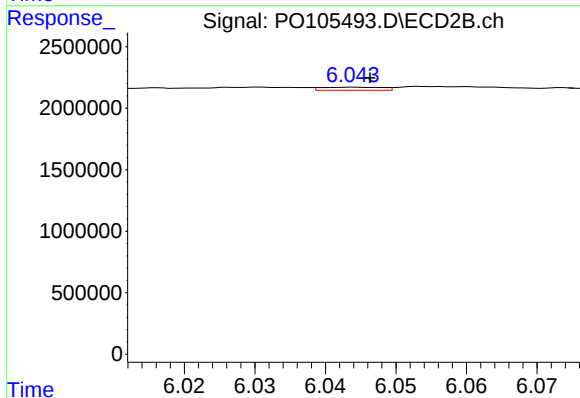


#31 AR-1260-1

R.T.: 6.044 min
Delta R.T.: -0.002 min
Response: 147488
Conc: 0.94 ng/ml

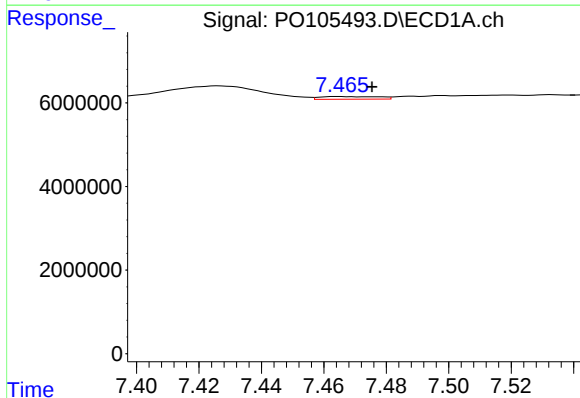


#32 AR-1260-2

R.T.: 7.465 min
Delta R.T.: -0.011 min
Response: 849814
Conc: 2.04 ng/ml

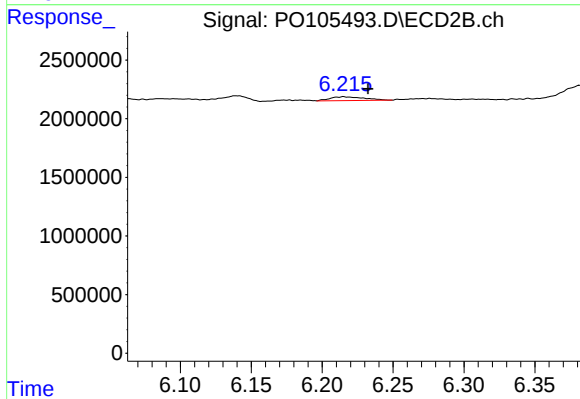

#32 AR-1260-2


R.T.: 6.215 min
Delta R.T.: -0.017 min
Response: 544840
Conc: 2.88 ng/ml

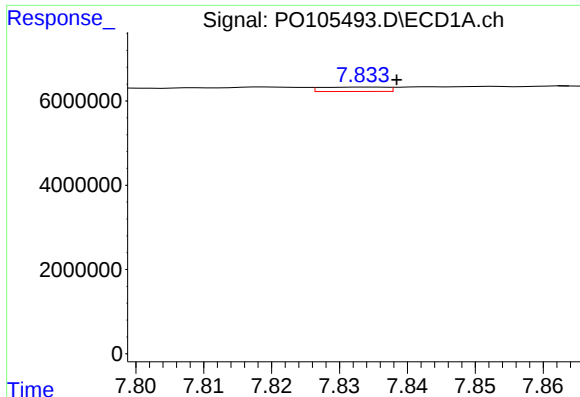

#33 AR-1260-3


R.T.: 7.834 min
Delta R.T.: -0.005 min
Response: 701806
Conc: 2.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

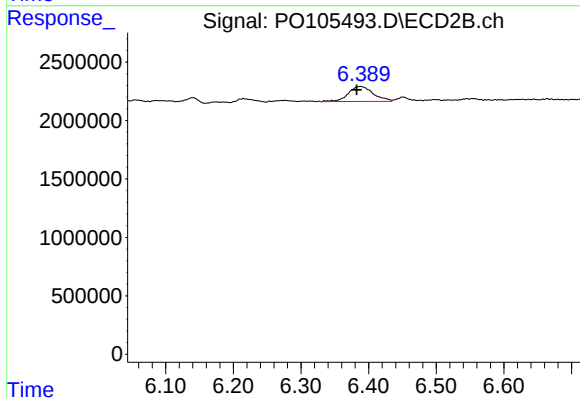


#33 AR-1260-3

R.T.: 6.388 min
Delta R.T.: 0.006 min
Response: 3276193
Conc: 17.73 ng/ml

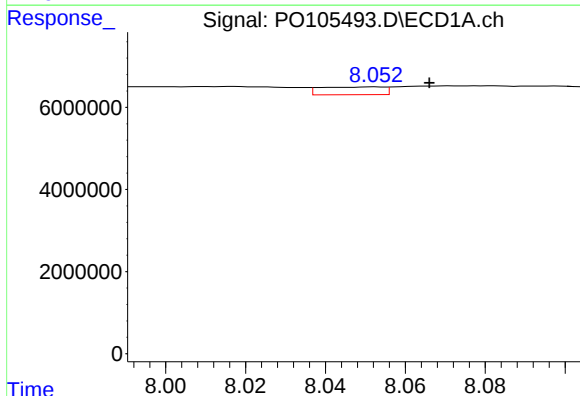


#34 AR-1260-4

R.T.: 8.053 min
Delta R.T.: -0.014 min
Response: 2119285
Conc: 6.42 ng/ml

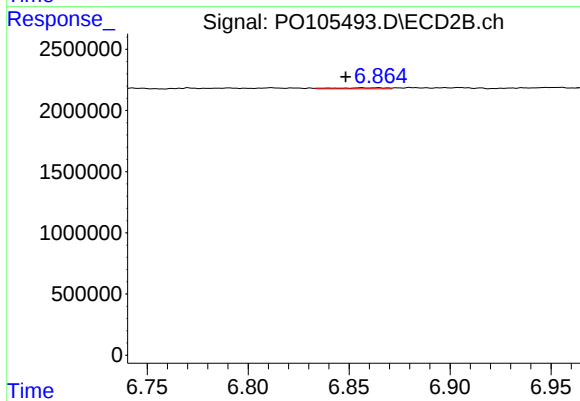

#34 AR-1260-4


R.T.: 6.864 min
Delta R.T.: 0.016 min
Response: 146991
Conc: 1.20 ng/ml

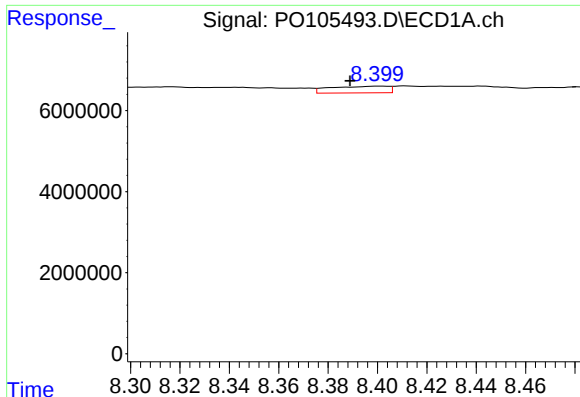

#35 AR-1260-5


R.T.: 8.400 min
Delta R.T.: 0.011 min
Response: 2661952
Conc: 4.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

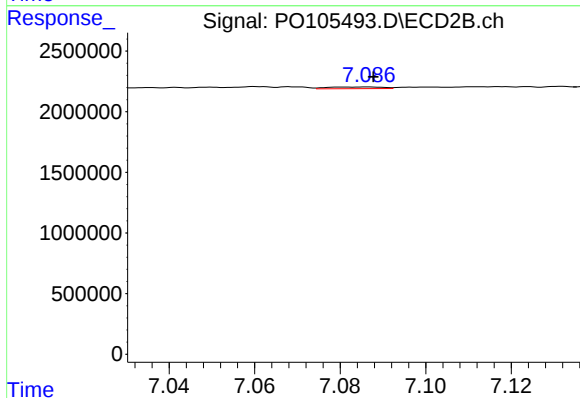


#35 AR-1260-5

R.T.: 7.086 min
Delta R.T.: -0.001 min
Response: 127419
Conc: 0.46 ng/ml

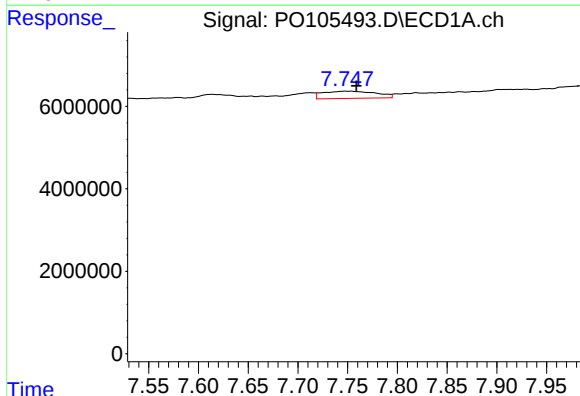


#36 AR-1262-1

R.T.: 7.747 min
Delta R.T.: -0.011 min
Response: 6494714
Conc: 20.45 ng/ml

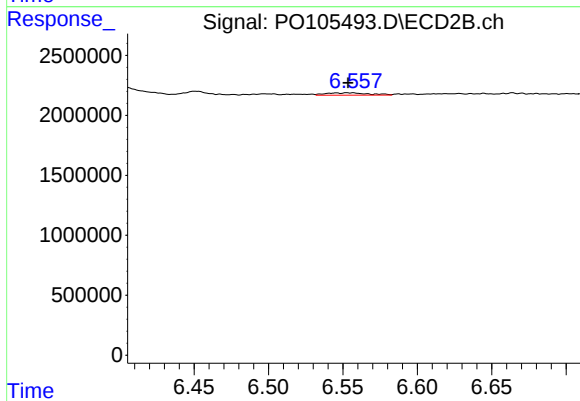

#36 AR-1262-1


R.T.: 6.557 min
Delta R.T.: 0.003 min
Response: 381991
Conc: 3.59 ng/ml

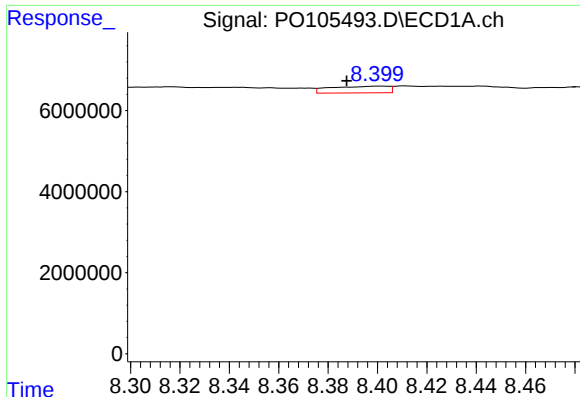

#37 AR-1262-2


R.T.: 8.400 min
Delta R.T.: 0.013 min
Response: 2661952
Conc: 3.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

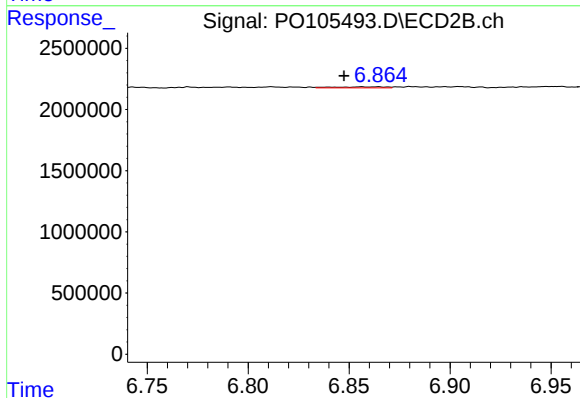


#37 AR-1262-2

R.T.: 6.864 min
Delta R.T.: 0.017 min
Response: 146991
Conc: 0.87 ng/ml

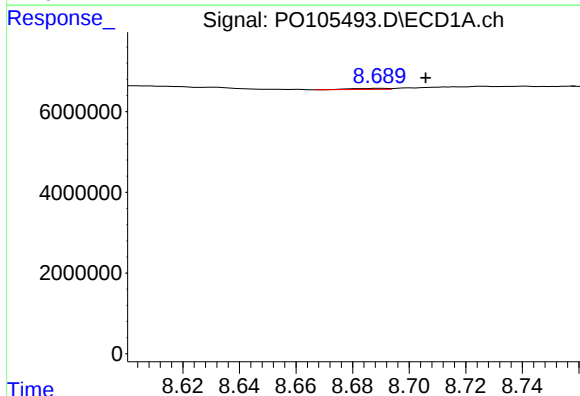


#38 AR-1262-3

R.T.: 8.690 min
Delta R.T.: -0.016 min
Response: 238731
Conc: 0.49 ng/ml

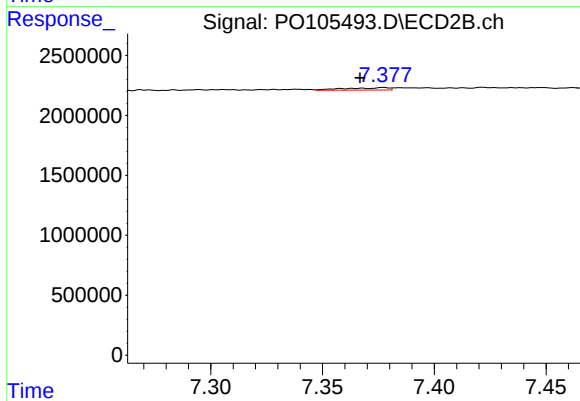

#38 AR-1262-3


R.T.: 7.377 min
Delta R.T.: 0.010 min
Response: 260413
Conc: 2.06 ng/ml

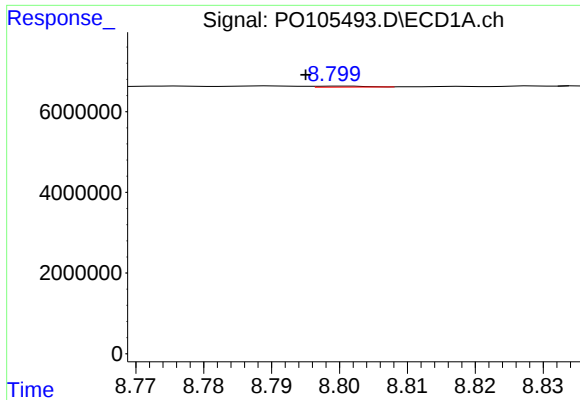

#39 AR-1262-4


R.T.: 8.800 min
Delta R.T.: 0.005 min
Response: 115255
Conc: 0.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

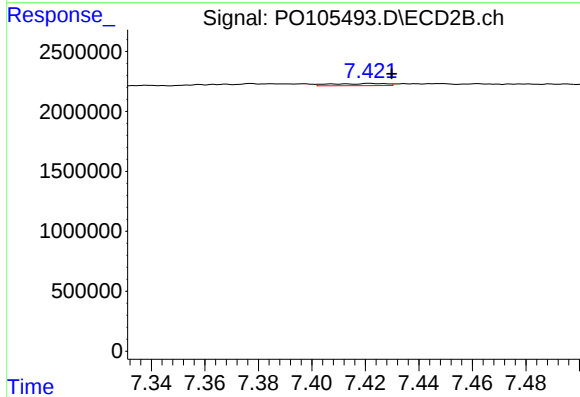


#39 AR-1262-4

R.T.: 7.422 min
Delta R.T.: -0.008 min
Response: 247322
Conc: 1.07 ng/ml

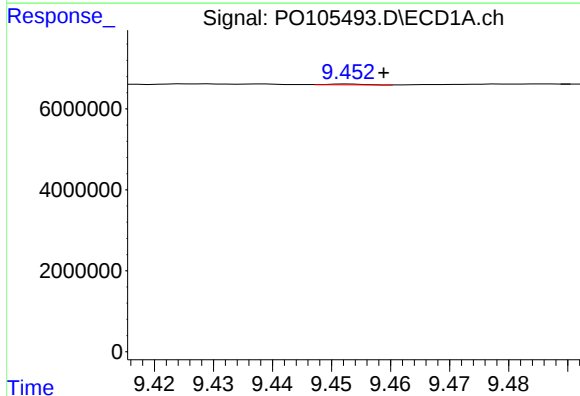


#40 AR-1262-5

R.T.: 9.453 min
Delta R.T.: -0.006 min
Response: 78660
Conc: 0.29 ng/ml

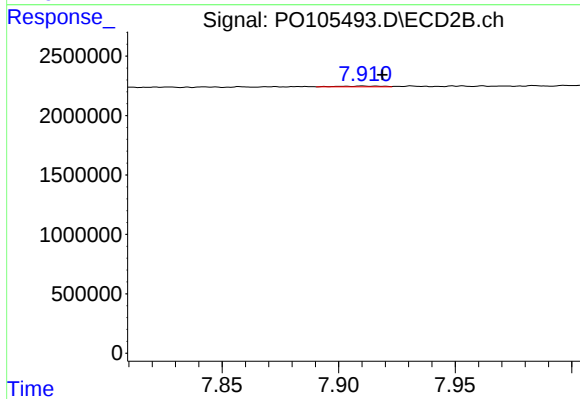

#40 AR-1262-5


R.T.: 7.910 min
Delta R.T.: -0.009 min
Response: 74627
Conc: 0.74 ng/ml

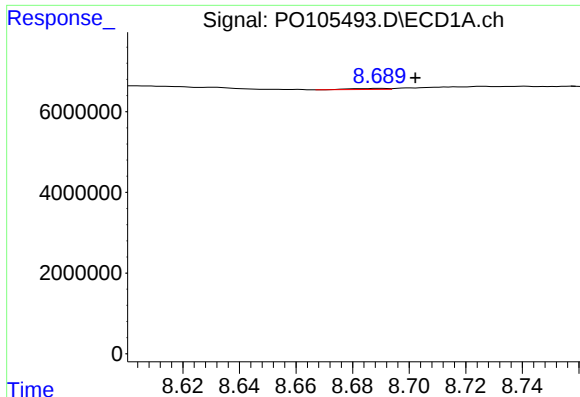

#41 AR-1268-1


R.T.: 8.690 min
Delta R.T.: -0.013 min
Response: 238731
Conc: 0.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

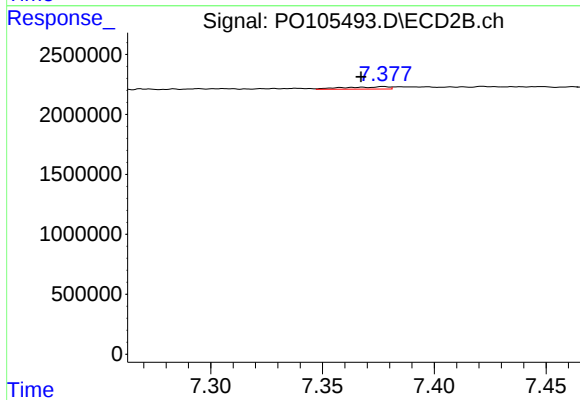


#41 AR-1268-1

R.T.: 7.377 min
Delta R.T.: 0.010 min
Response: 260413
Conc: 0.75 ng/ml

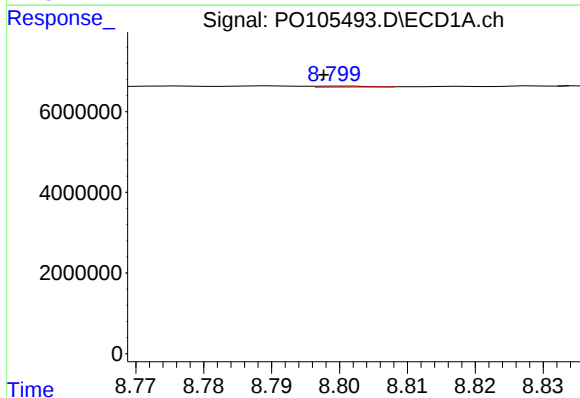


#42 AR-1268-2

R.T.: 8.800 min
Delta R.T.: 0.003 min
Response: 115255
Conc: 0.16 ng/ml

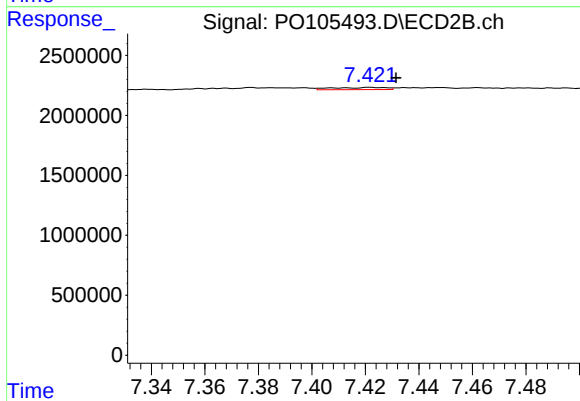

#42 AR-1268-2


R.T.: 7.422 min
Delta R.T.: -0.010 min
Response: 247322
Conc: 0.79 ng/ml

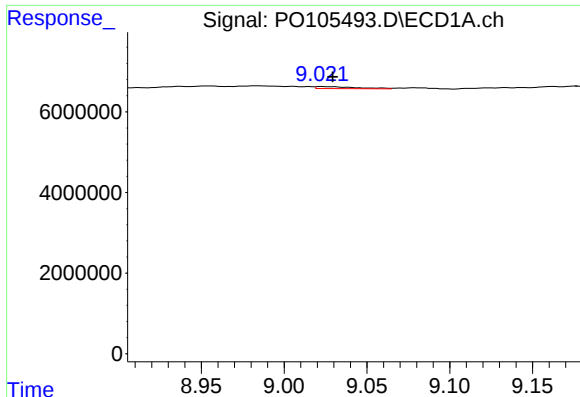

#43 AR-1268-3


R.T.: 9.022 min
Delta R.T.: -0.007 min
Response: 821619
Conc: 1.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

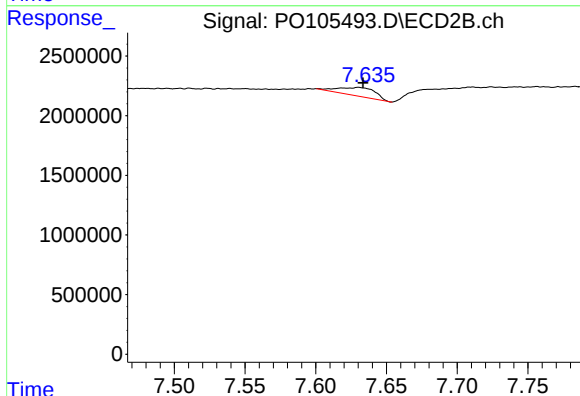


#43 AR-1268-3

R.T.: 7.630 min
Delta R.T.: -0.003 min
Response: 1295596
Conc: 5.13 ng/ml

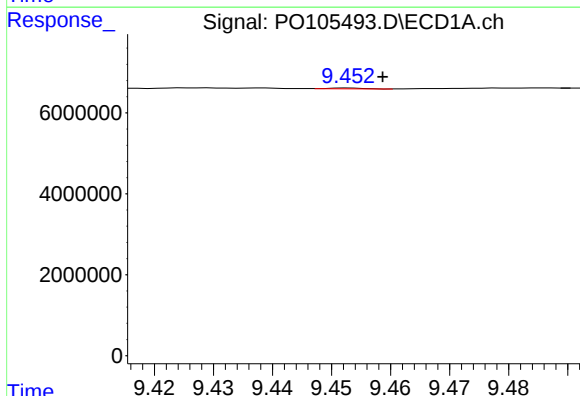


#44 AR-1268-4

R.T.: 9.453 min
Delta R.T.: -0.006 min
Response: 78660
Conc: 0.28 ng/ml

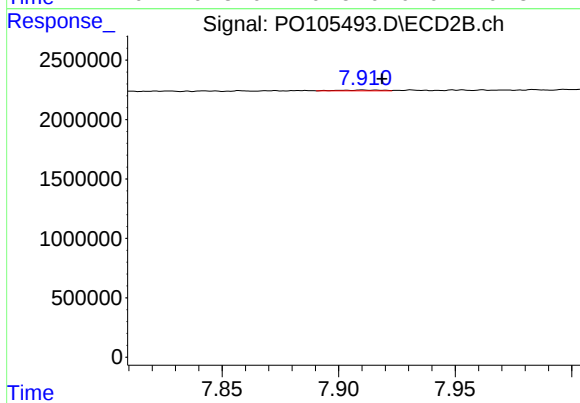

#44 AR-1268-4


R.T.: 7.910 min
Delta R.T.: -0.008 min
Response: 74627
Conc: 0.69 ng/ml

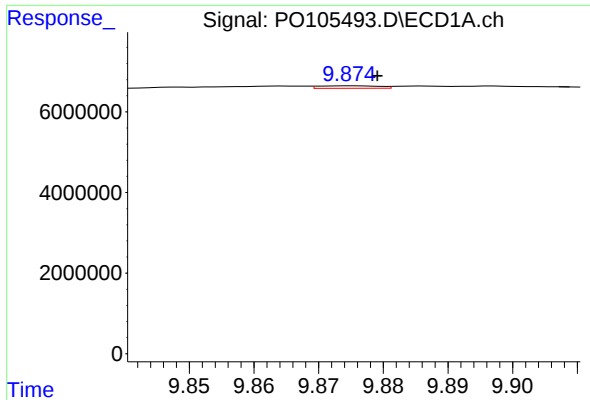

#45 AR-1268-5

R.T.: 9.875 min
Delta R.T.: -0.004 min
Response: 393151
Conc: 0.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

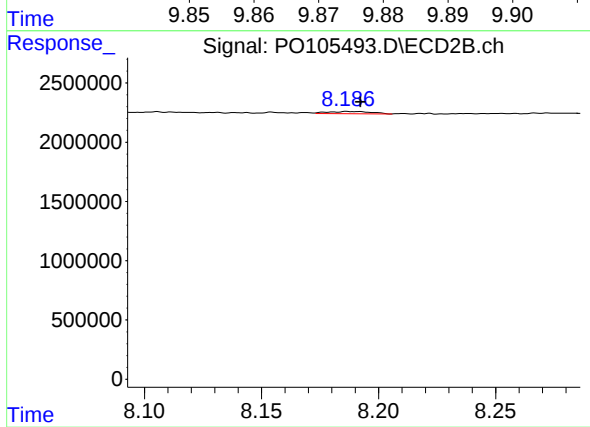

#45 AR-1268-5

R.T.: 8.187 min
Delta R.T.: -0.005 min
Response: 247554
Conc: 0.37 ng/ml