

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081324\
 Data File : P0105494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 13:07
 Operator : YP/AJ
 Sample : P3390-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:07:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.426	3.535	111.8E6	50985712	12.802	16.233 #
2)	SA Decachlor...	10.215	8.425	86724674	31637047	15.076	17.870
Target Compounds							
3)	L1 AR-1016-1	5.596	4.589	3458977	1683141	11.434	14.977 #
4)	L1 AR-1016-2	5.620	4.607	4039566	1613913	9.449	10.367
5)	L1 AR-1016-3	5.681	4.780	1729506	1101214	6.741	13.149 #
6)	L1 AR-1016-4	5.780	4.821	3056331	2354194	13.974	34.960 #
7)	L1 AR-1016-5	6.077	5.029	5838599	2841595	27.289	33.953
8)	L2 AR-1221-1	4.640	3.749	248861	46918	2.219	1.189 #
9)	L2 AR-1221-2	4.732	3.825	2027136	1078665	23.916	35.110 #
10)	L2 AR-1221-3	4.789	3.900	886656	145828	3.645	1.630 #
11)	L3 AR-1232-1	4.789	3.900	886656	145828	4.435	1.997 #
12)	L3 AR-1232-2	5.326	4.607	1874212	1613913	17.706	22.985 #
13)	L3 AR-1232-3	5.620	4.780	4039566	1101214	21.104	28.815 #
14)	L3 AR-1232-4	5.780	4.861	3056331	2492040	31.336	71.631 #
15)	L3 AR-1232-5	5.872	5.029	4913056	2841595	68.177	80.502
16)	L4 AR-1242-1	5.596	4.589	3458977	1683141	14.884	19.083 #
17)	L4 AR-1242-2	5.620	4.607	4039566	1613913	12.395	13.593
18)	L4 AR-1242-3	5.681	4.780	1729506	1101214	8.767	16.958 #
19)	L4 AR-1242-4	5.780	4.861	3056331	2492040	17.913	37.575 #
20)	L4 AR-1242-5	6.524	5.373	7752159	4264457	44.358	51.896
21)	L5 AR-1248-1	5.596	4.589	3458977	1683141	18.943	24.099 #
22)	L5 AR-1248-2	5.872	4.821	4913056	2354194	19.506	24.808 #
23)	L5 AR-1248-3	6.077	4.861	5838599	2492040	20.655	24.964
24)	L5 AR-1248-4	6.484	5.029	7572932	2841595	23.684	25.176
25)	L5 AR-1248-5	6.524	5.413	7752159	3045333	25.062	27.045
26)	L6 AR-1254-1	6.457	5.373	6391483	4264457	20.381	26.194 #
27)	L6 AR-1254-2	6.682	5.519	6622849	1962132	14.676	13.413
28)	L6 AR-1254-3	7.048	5.915	5528906	3102683	11.655	13.755
29)	L6 AR-1254-4	7.336	6.140	5136412	2177164	14.339	15.429
30)	L6 AR-1254-5	7.751	6.550	7961979	584942	20.057	2.920 #
31)	L7 AR-1260-1	7.229	6.058	1596158	2205166	4.355	14.127 #
32)	L7 AR-1260-2	7.481	6.220	1582963	1120573	3.802	5.929 #
33)	L7 AR-1260-3	7.839	6.387	1246679	3398034	4.817	18.394 #
34)	L7 AR-1260-4	8.055	6.848	3057574	110161	9.267	0.901 #
35)	L7 AR-1260-5	8.399	7.085	4022100	178508	6.761	0.641 #
36)	L8 AR-1262-1	7.751	6.550	7961979	584942	25.066	5.497 #
37)	L8 AR-1262-2	8.399	6.848	4022100	110161	5.347	0.648 #
38)	L8 AR-1262-3	8.705	7.373	566713	318457	1.152	2.522 #
39)	L8 AR-1262-4	8.789	7.421	194239	414057	0.529	1.789 #
40)	L8 AR-1262-5	9.452	7.913	59368	101883	0.222	1.014 #
41)	L9 AR-1268-1	8.705	7.373	566713	318457	0.697	0.912 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081324\
Data File : P0105494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 13:07
Operator : YP/AJ
Sample : P3390-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:07:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.789	7.421	194239	414057	0.267	1.327 #
43) L9	AR-1268-3	9.025	7.631	238364	565976	0.369	2.239 #
44) L9	AR-1268-4	9.452	7.913	59368	101883	0.213	0.947 #
45) L9	AR-1268-5	9.880	8.189	876853	284876	0.419	0.426



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081324\
Data File : PO105494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 13:07
Operator : YP/AJ
Sample : P3390-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:07:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

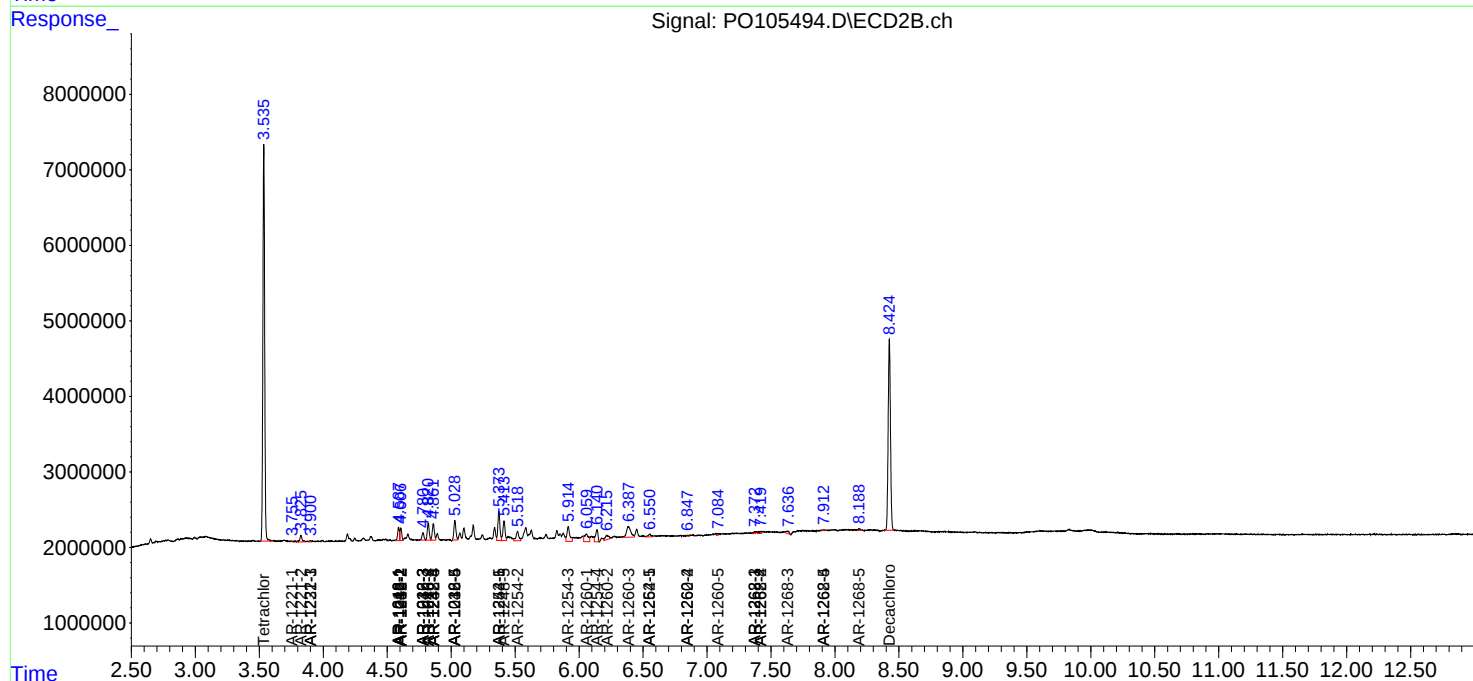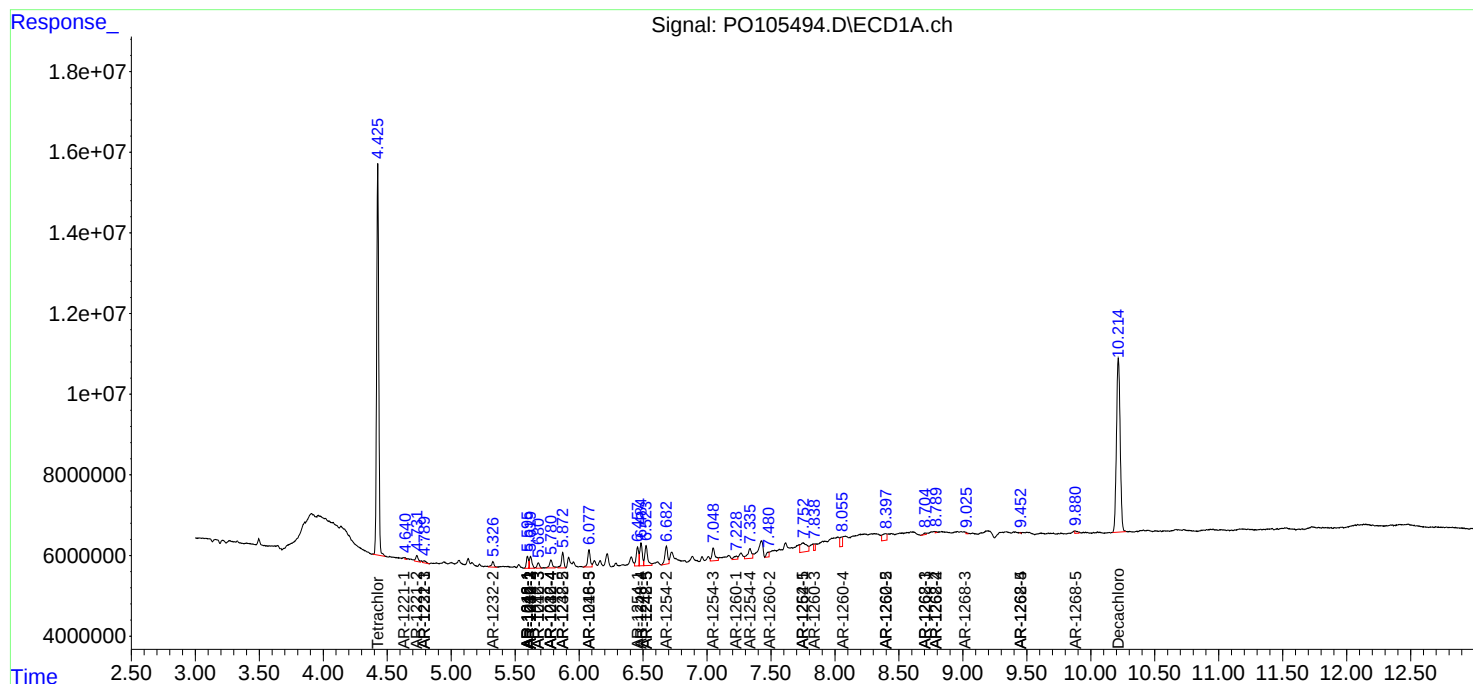


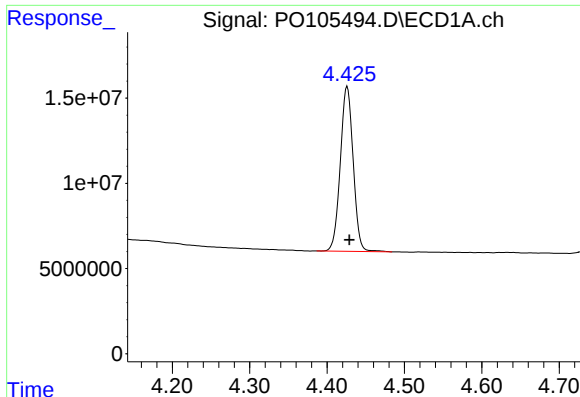

#1 Tetrachloro-m-xylene


R.T.: 4.426 min
Delta R.T.: -0.003 min
Response: 111813371
Conc: 12.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

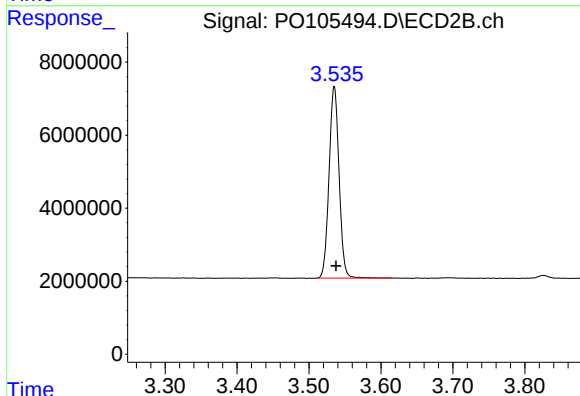


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.002 min
Response: 50985712
Conc: 16.23 ng/ml

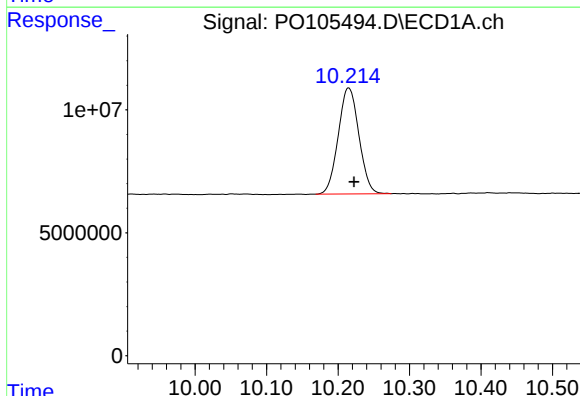


#2 Decachlorobiphenyl

R.T.: 10.215 min
Delta R.T.: -0.008 min
Response: 86724674
Conc: 15.08 ng/ml

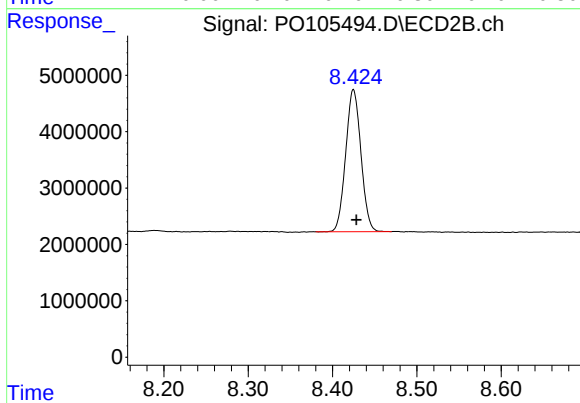

#2 Decachlorobiphenyl


R.T.: 8.425 min
Delta R.T.: -0.004 min
Response: 31637047
Conc: 17.87 ng/ml

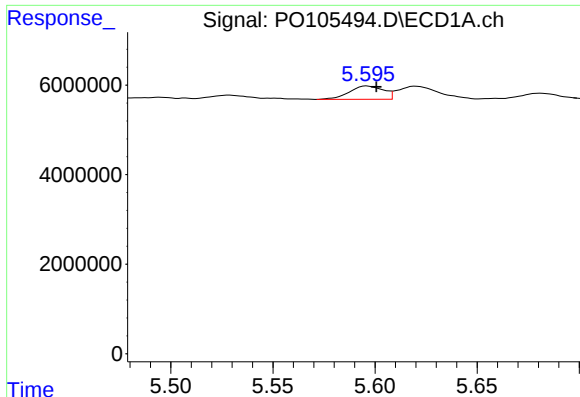

#3 AR-1016-1


R.T.: 5.596 min
Delta R.T.: -0.005 min
Response: 3458977
Conc: 11.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

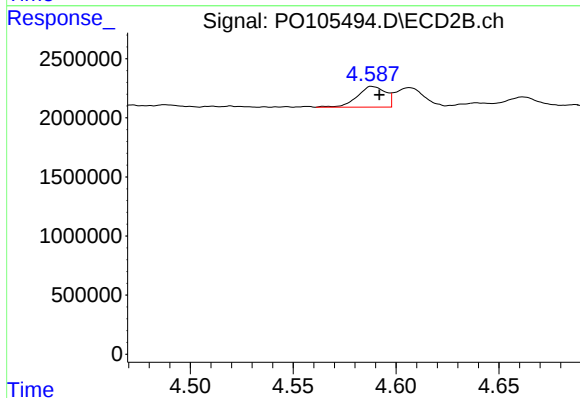


#3 AR-1016-1

R.T.: 4.589 min
Delta R.T.: -0.003 min
Response: 1683141
Conc: 14.98 ng/ml

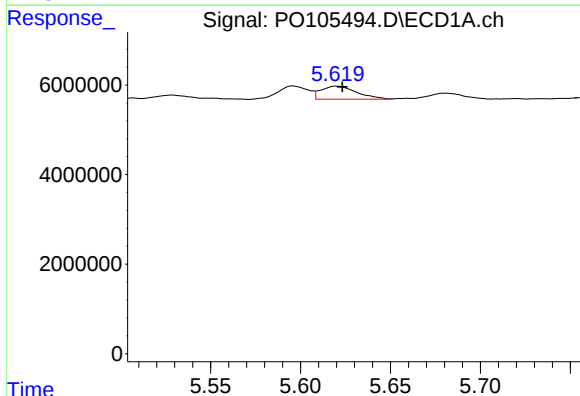


#4 AR-1016-2

R.T.: 5.620 min
Delta R.T.: -0.003 min
Response: 4039566
Conc: 9.45 ng/ml

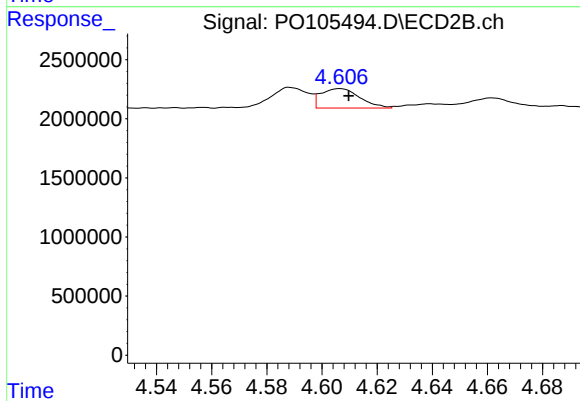

#4 AR-1016-2


R.T.: 4.607 min
Delta R.T.: -0.003 min
Response: 1613913
Conc: 10.37 ng/ml

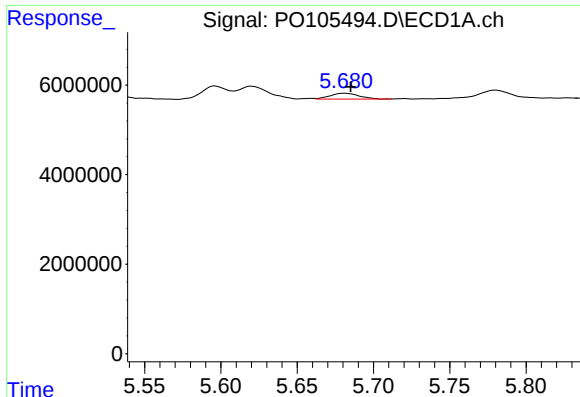

#5 AR-1016-3


R.T.: 5.681 min
Delta R.T.: -0.004 min
Response: 1729506
Conc: 6.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

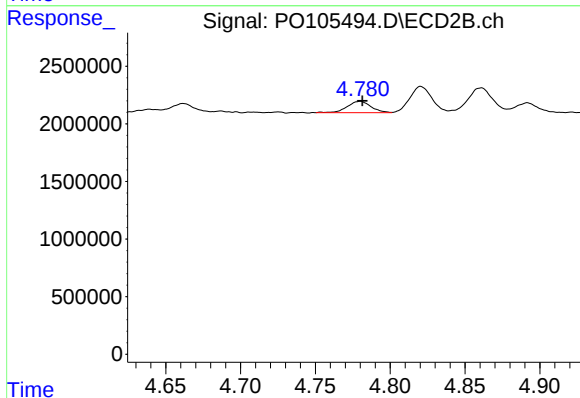


#5 AR-1016-3

R.T.: 4.780 min
Delta R.T.: -0.001 min
Response: 1101214
Conc: 13.15 ng/ml

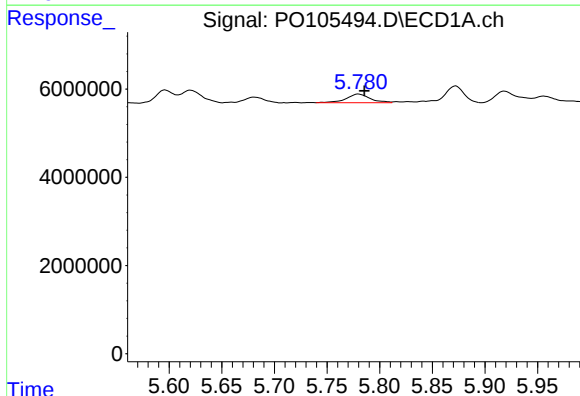


#6 AR-1016-4

R.T.: 5.780 min
Delta R.T.: -0.006 min
Response: 3056331
Conc: 13.97 ng/ml

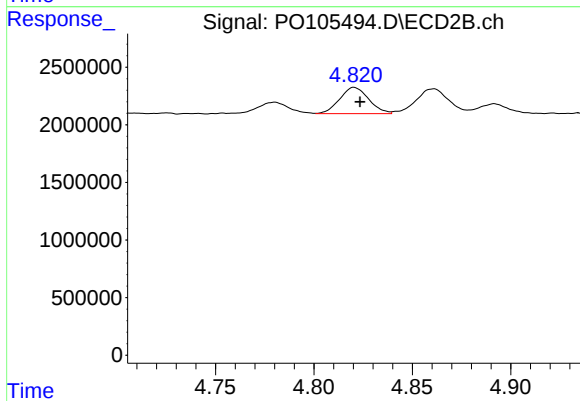

#6 AR-1016-4


R.T.: 4.821 min
Delta R.T.: -0.003 min
Response: 2354194
Conc: 34.96 ng/ml

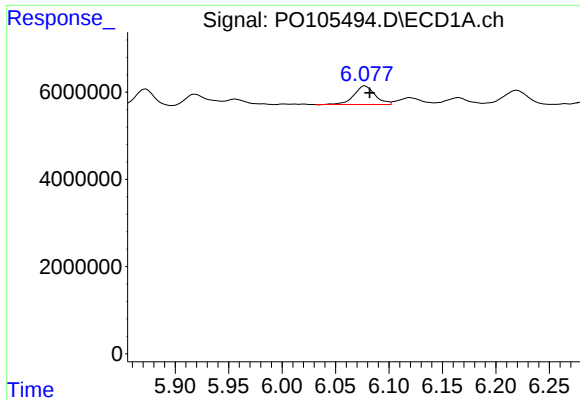

#7 AR-1016-5


R.T.: 6.077 min
Delta R.T.: -0.005 min
Response: 5838599
Conc: 27.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

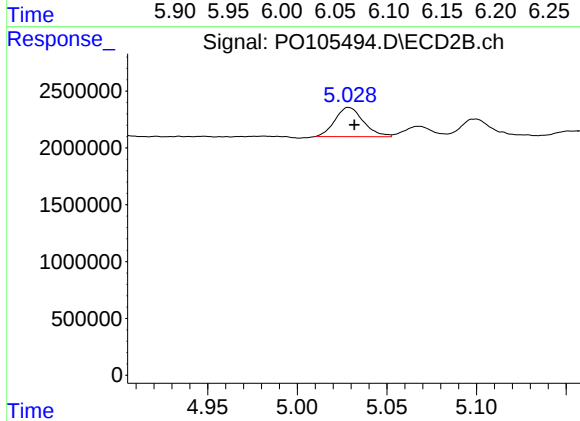


#7 AR-1016-5

R.T.: 5.029 min
Delta R.T.: -0.003 min
Response: 2841595
Conc: 33.95 ng/ml

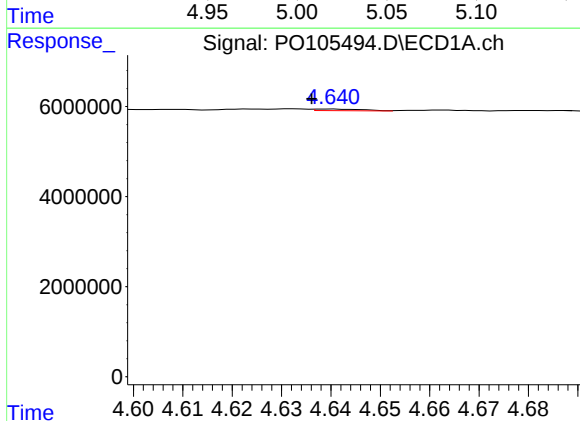


#8 AR-1221-1

R.T.: 4.640 min
Delta R.T.: 0.003 min
Response: 248861
Conc: 2.22 ng/ml

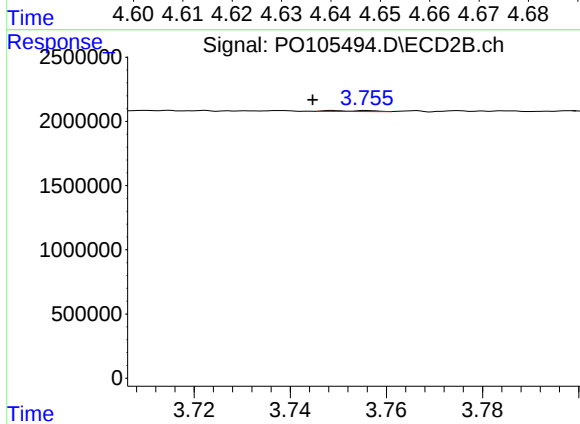

#8 AR-1221-1


R.T.: 3.749 min
Delta R.T.: 0.004 min
Response: 46918
Conc: 1.19 ng/ml

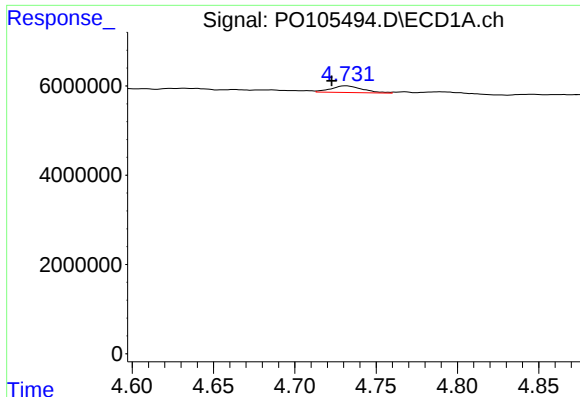

#9 AR-1221-2


R.T.: 4.732 min
Delta R.T.: 0.009 min
Response: 2027136
Conc: 23.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

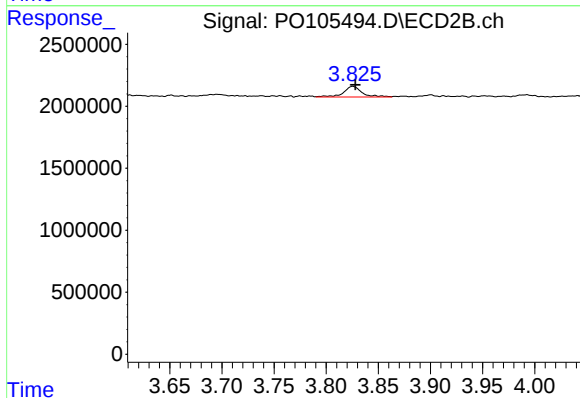


#9 AR-1221-2

R.T.: 3.825 min
Delta R.T.: -0.003 min
Response: 1078665
Conc: 35.11 ng/ml

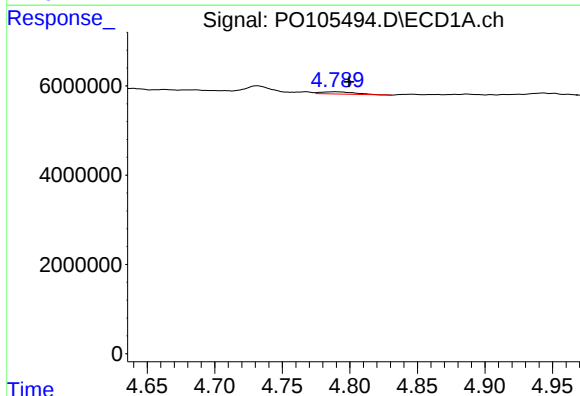


#10 AR-1221-3

R.T.: 4.789 min
Delta R.T.: -0.010 min
Response: 886656
Conc: 3.64 ng/ml

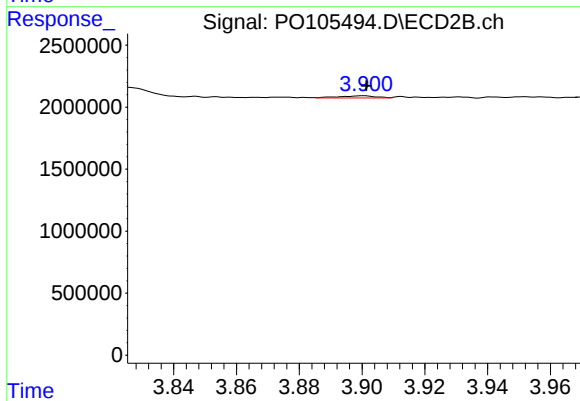

#10 AR-1221-3


R.T.: 3.900 min
Delta R.T.: -0.001 min
Response: 145828
Conc: 1.63 ng/ml

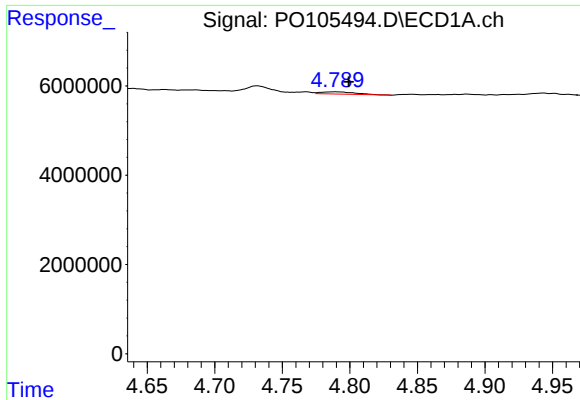

#11 AR-1232-1


R.T.: 4.789 min
Delta R.T.: -0.010 min
Response: 886656
Conc: 4.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

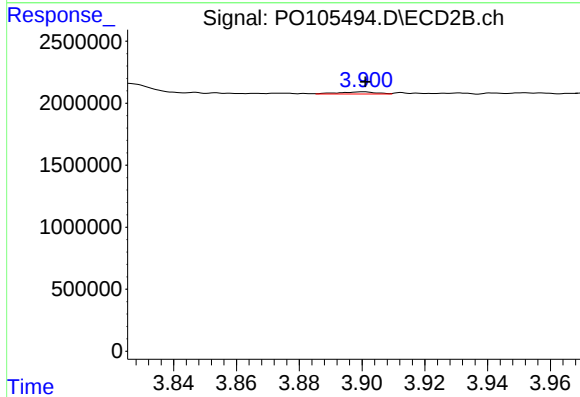


#11 AR-1232-1

R.T.: 3.900 min
Delta R.T.: 0.000 min
Response: 145828
Conc: 2.00 ng/ml

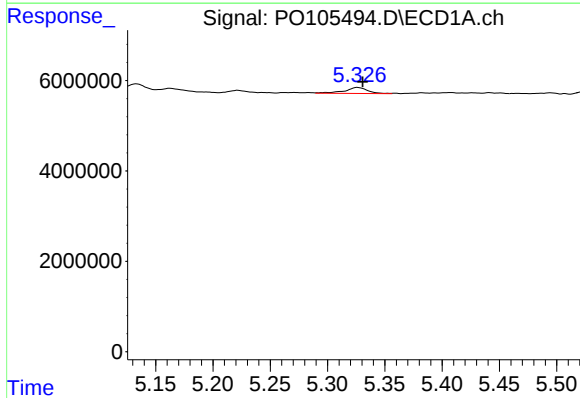


#12 AR-1232-2

R.T.: 5.326 min
Delta R.T.: -0.004 min
Response: 1874212
Conc: 17.71 ng/ml

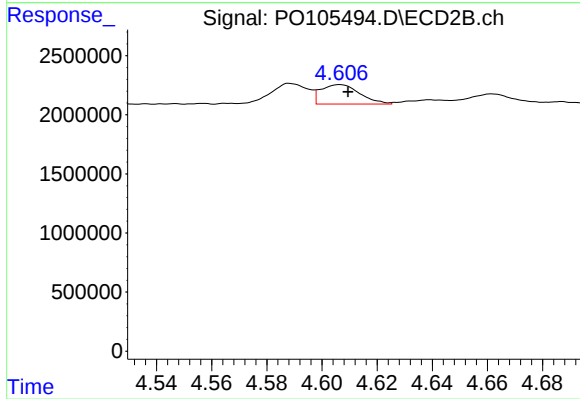

#12 AR-1232-2


R.T.: 4.607 min
Delta R.T.: -0.003 min
Response: 1613913
Conc: 22.99 ng/ml

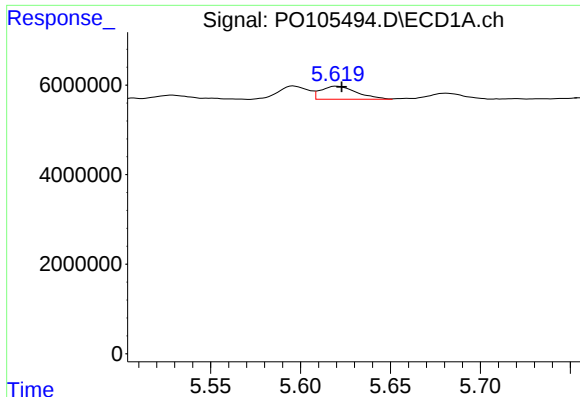

#13 AR-1232-3


R.T.: 5.620 min
Delta R.T.: -0.003 min
Response: 4039566
Conc: 21.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

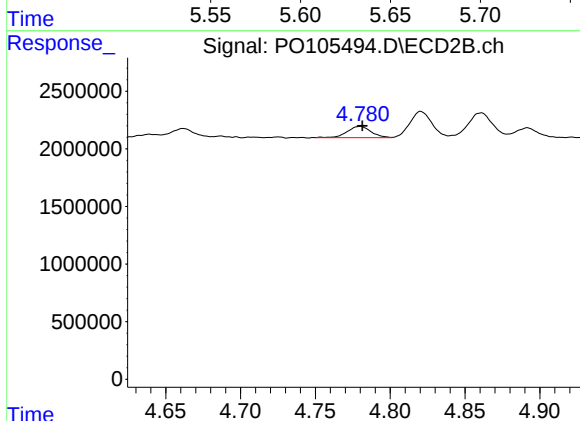


#13 AR-1232-3

R.T.: 4.780 min
Delta R.T.: -0.002 min
Response: 1101214
Conc: 28.81 ng/ml

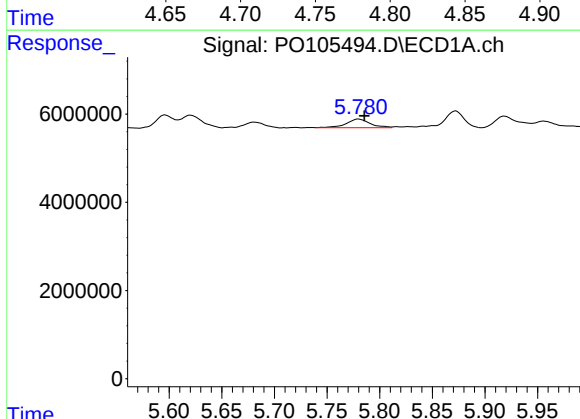


#14 AR-1232-4

R.T.: 5.780 min
Delta R.T.: -0.005 min
Response: 3056331
Conc: 31.34 ng/ml

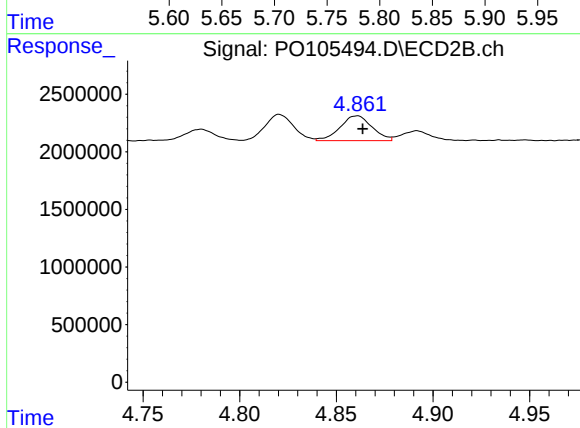

#14 AR-1232-4


R.T.: 4.861 min
Delta R.T.: -0.003 min
Response: 2492040
Conc: 71.63 ng/ml

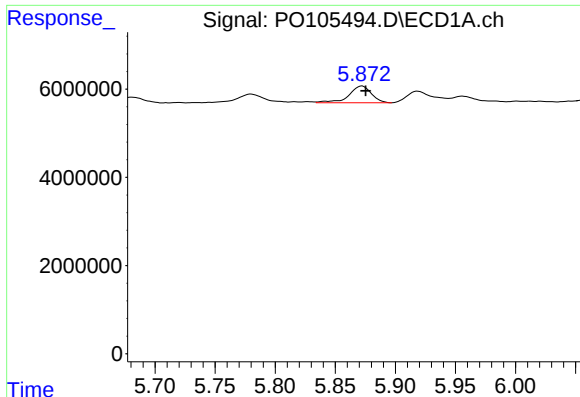

#15 AR-1232-5


R.T.: 5.872 min
Delta R.T.: -0.003 min
Response: 4913056
Conc: 68.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

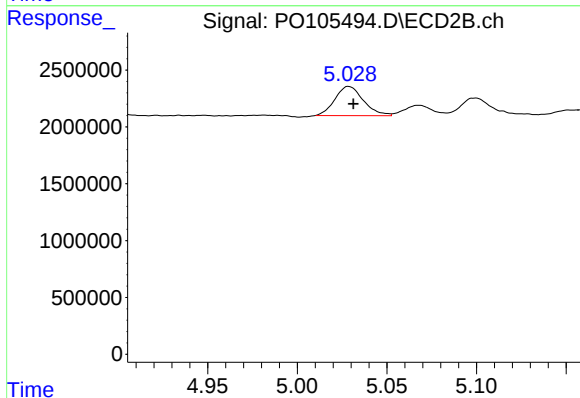


#15 AR-1232-5

R.T.: 5.029 min
Delta R.T.: -0.003 min
Response: 2841595
Conc: 80.50 ng/ml

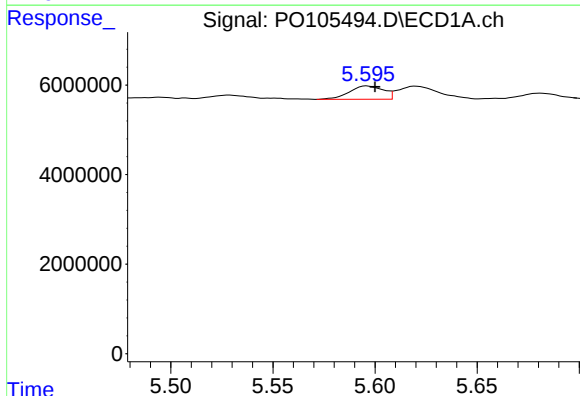


#16 AR-1242-1

R.T.: 5.596 min
Delta R.T.: -0.004 min
Response: 3458977
Conc: 14.88 ng/ml

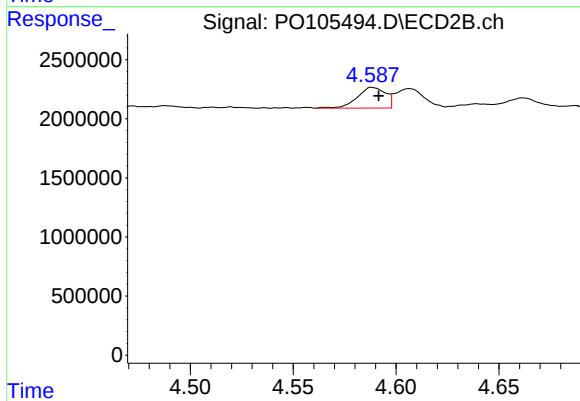

#16 AR-1242-1


R.T.: 4.589 min
Delta R.T.: -0.003 min
Response: 1683141
Conc: 19.08 ng/ml

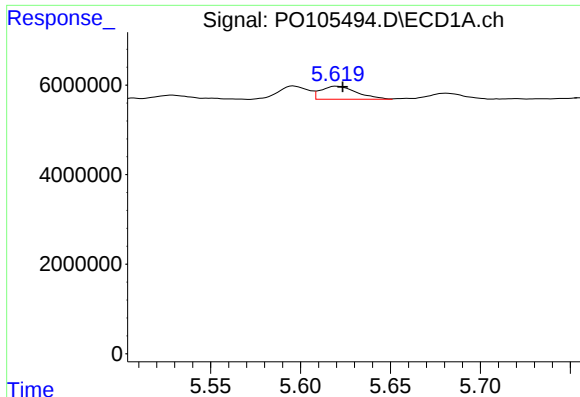

#17 AR-1242-2


R.T.: 5.620 min
Delta R.T.: -0.003 min
Response: 4039566
Conc: 12.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

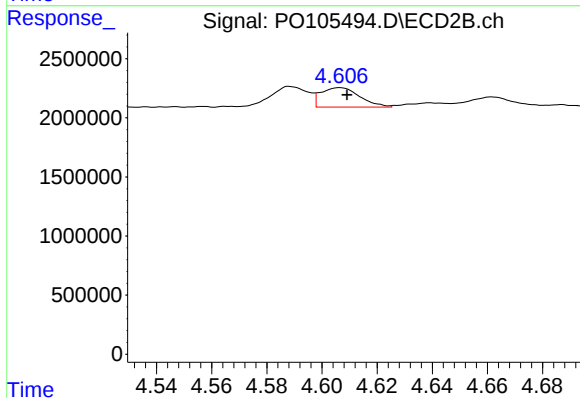


#17 AR-1242-2

R.T.: 4.607 min
Delta R.T.: -0.003 min
Response: 1613913
Conc: 13.59 ng/ml

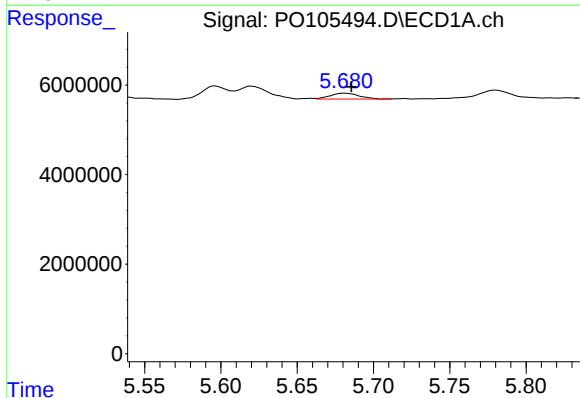


#18 AR-1242-3

R.T.: 5.681 min
Delta R.T.: -0.005 min
Response: 1729506
Conc: 8.77 ng/ml

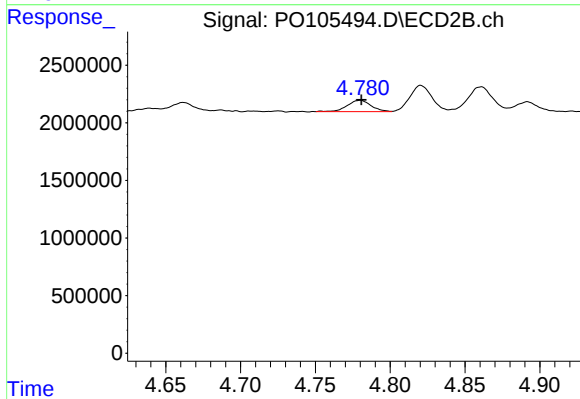

#18 AR-1242-3


R.T.: 4.780 min
Delta R.T.: 0.000 min
Response: 1101214
Conc: 16.96 ng/ml

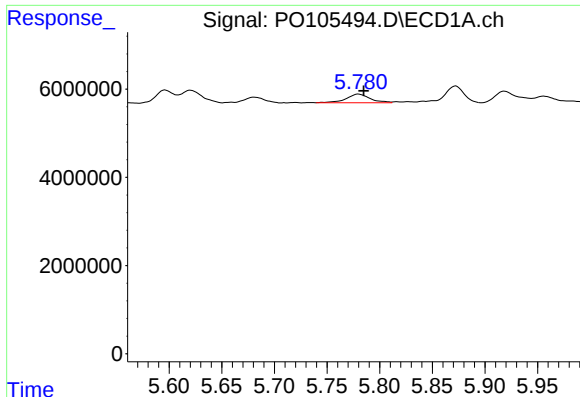

#19 AR-1242-4


R.T.: 5.780 min
Delta R.T.: -0.005 min
Response: 3056331
Conc: 17.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

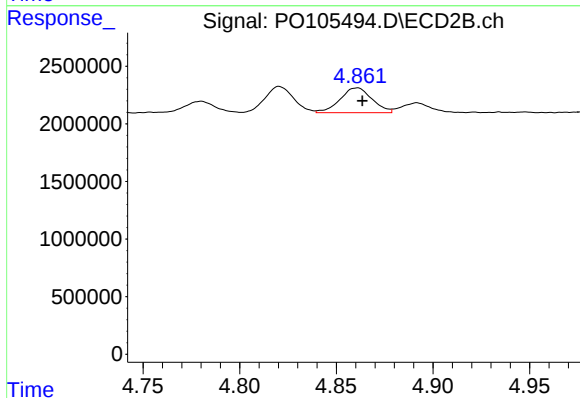


#19 AR-1242-4

R.T.: 4.861 min
Delta R.T.: -0.003 min
Response: 2492040
Conc: 37.57 ng/ml

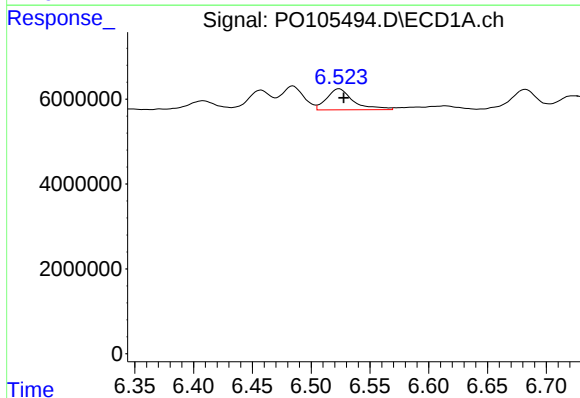


#20 AR-1242-5

R.T.: 6.524 min
Delta R.T.: -0.004 min
Response: 7752159
Conc: 44.36 ng/ml

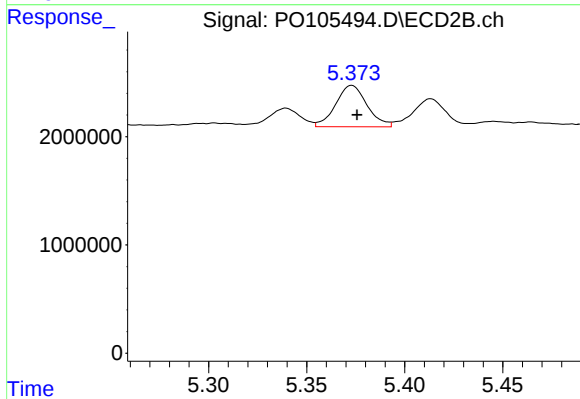

#20 AR-1242-5


R.T.: 5.373 min
Delta R.T.: -0.003 min
Response: 4264457
Conc: 51.90 ng/ml

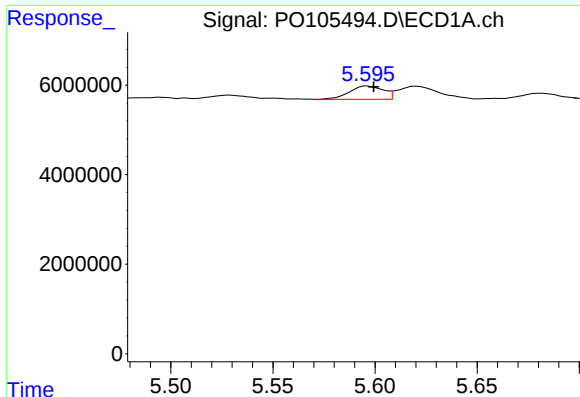

#21 AR-1248-1


R.T.: 5.596 min
Delta R.T.: -0.003 min
Response: 3458977
Conc: 18.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

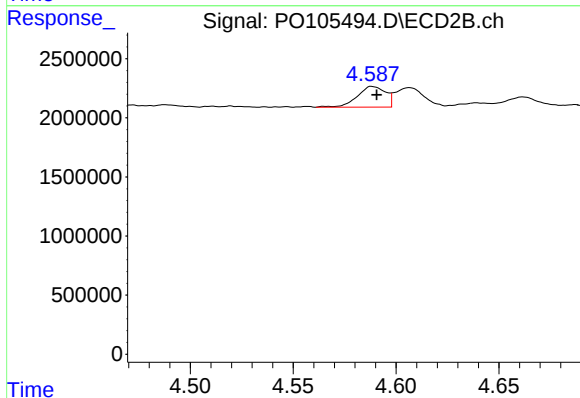


#21 AR-1248-1

R.T.: 4.589 min
Delta R.T.: -0.002 min
Response: 1683141
Conc: 24.10 ng/ml

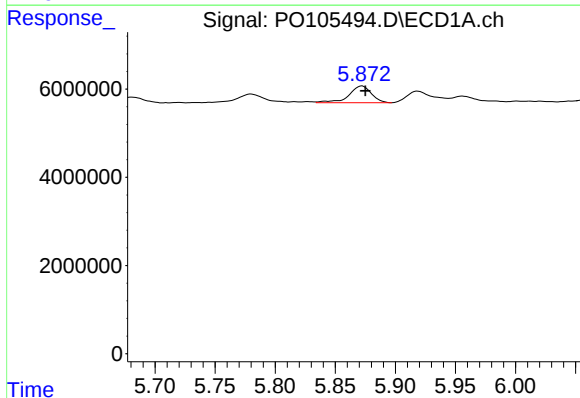


#22 AR-1248-2

R.T.: 5.872 min
Delta R.T.: -0.003 min
Response: 4913056
Conc: 19.51 ng/ml

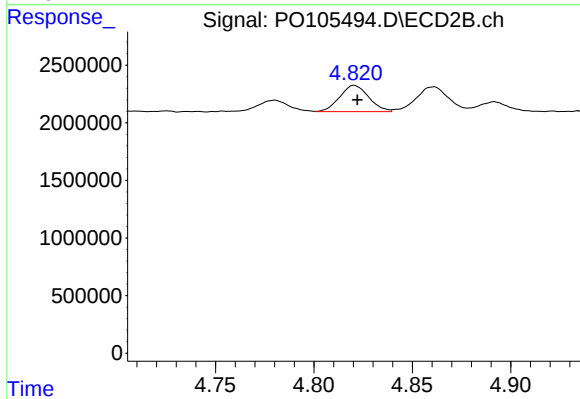

#22 AR-1248-2


R.T.: 4.821 min
Delta R.T.: -0.002 min
Response: 2354194
Conc: 24.81 ng/ml

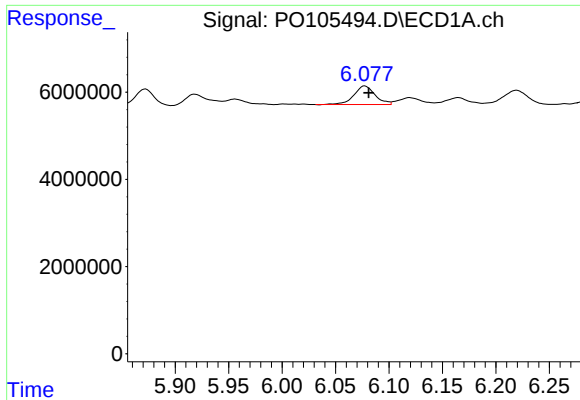

#23 AR-1248-3


R.T.: 6.077 min
Delta R.T.: -0.004 min
Response: 5838599
Conc: 20.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

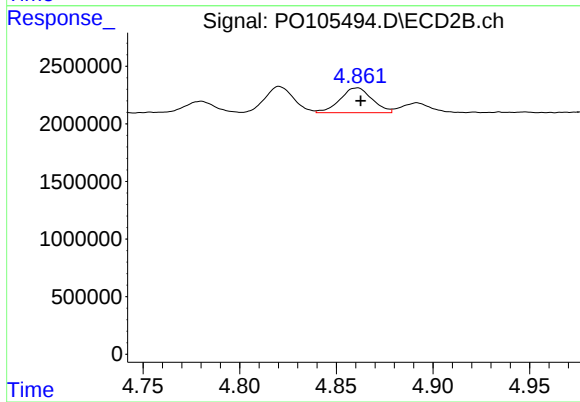


#23 AR-1248-3

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 2492040
Conc: 24.96 ng/ml

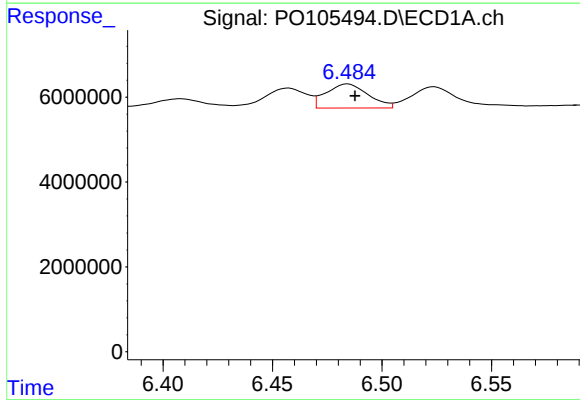


#24 AR-1248-4

R.T.: 6.484 min
Delta R.T.: -0.003 min
Response: 7572932
Conc: 23.68 ng/ml

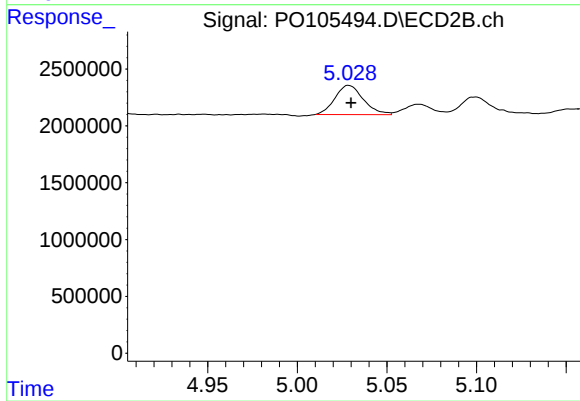

#24 AR-1248-4


R.T.: 5.029 min
Delta R.T.: -0.001 min
Response: 2841595
Conc: 25.18 ng/ml

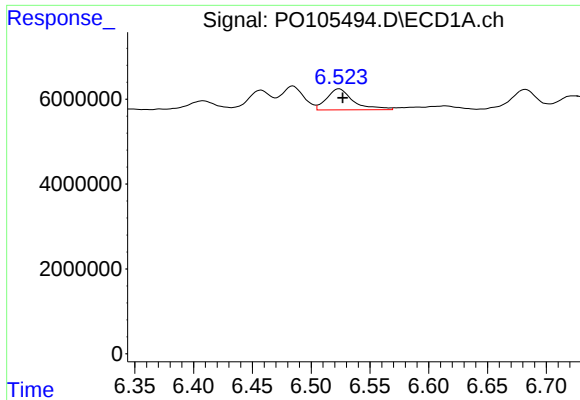

#25 AR-1248-5


R.T.: 6.524 min
Delta R.T.: -0.003 min
Response: 7752159
Conc: 25.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

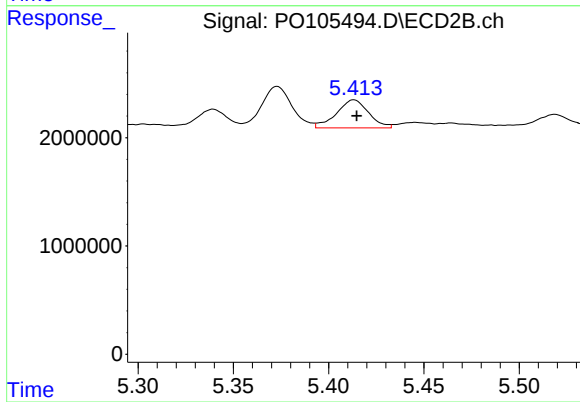


#25 AR-1248-5

R.T.: 5.413 min
Delta R.T.: -0.001 min
Response: 3045333
Conc: 27.04 ng/ml

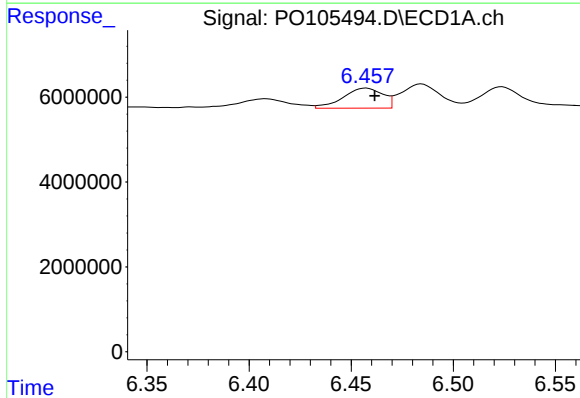


#26 AR-1254-1

R.T.: 6.457 min
Delta R.T.: -0.004 min
Response: 6391483
Conc: 20.38 ng/ml

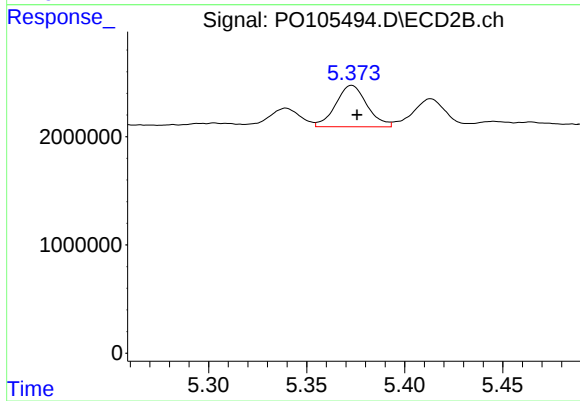

#26 AR-1254-1


R.T.: 5.373 min
Delta R.T.: -0.003 min
Response: 4264457
Conc: 26.19 ng/ml

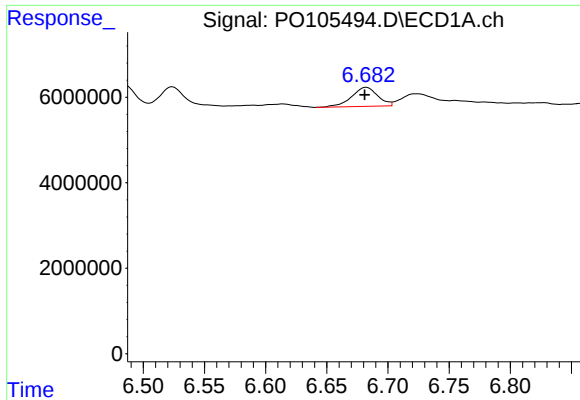

#27 AR-1254-2


R.T.: 6.682 min
Delta R.T.: 0.001 min
Response: 6622849
Conc: 14.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

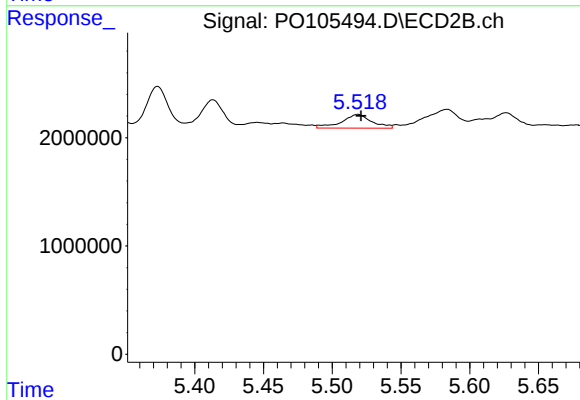


#27 AR-1254-2

R.T.: 5.519 min
Delta R.T.: -0.002 min
Response: 1962132
Conc: 13.41 ng/ml

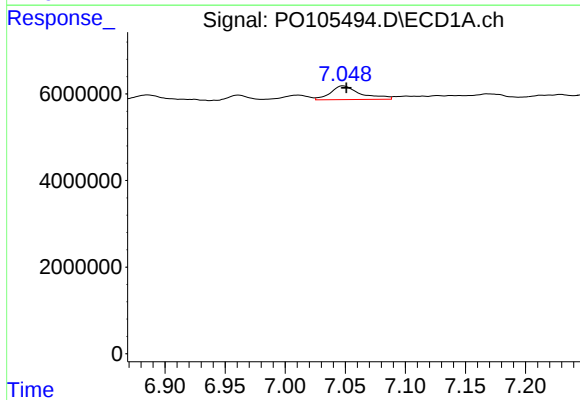


#28 AR-1254-3

R.T.: 7.048 min
Delta R.T.: -0.003 min
Response: 5528906
Conc: 11.66 ng/ml

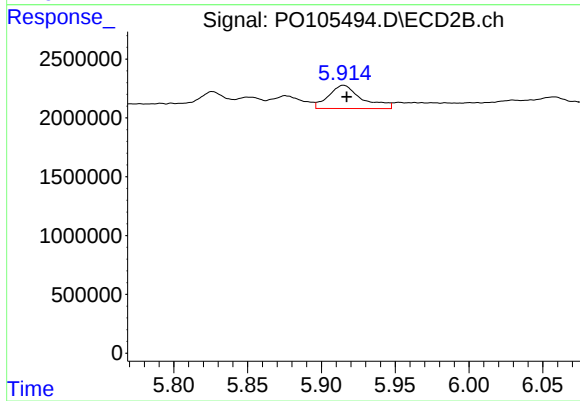

#28 AR-1254-3


R.T.: 5.915 min
Delta R.T.: -0.002 min
Response: 3102683
Conc: 13.75 ng/ml

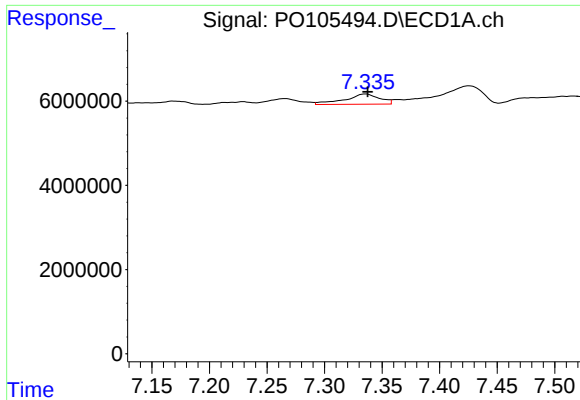

#29 AR-1254-4


R.T.: 7.336 min
Delta R.T.: -0.002 min
Response: 5136412
Conc: 14.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

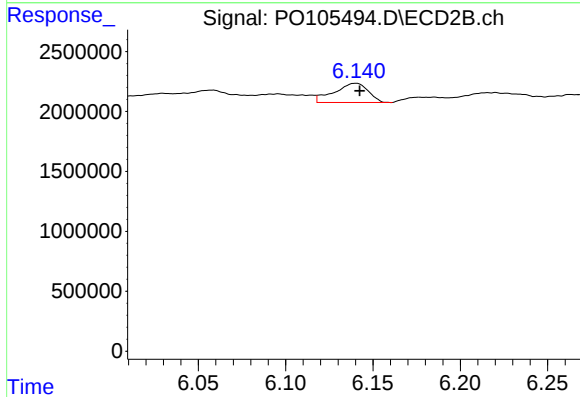


#29 AR-1254-4

R.T.: 6.140 min
Delta R.T.: -0.002 min
Response: 2177164
Conc: 15.43 ng/ml

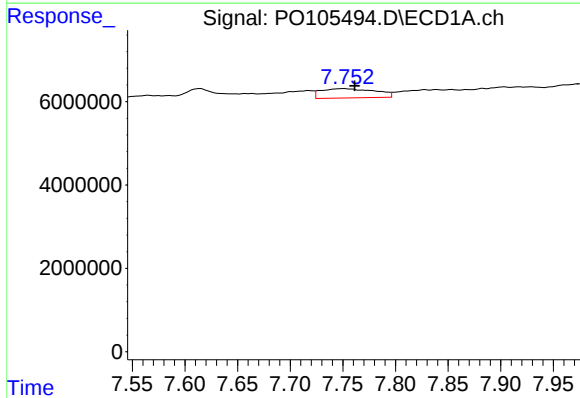


#30 AR-1254-5

R.T.: 7.751 min
Delta R.T.: -0.011 min
Response: 7961979
Conc: 20.06 ng/ml

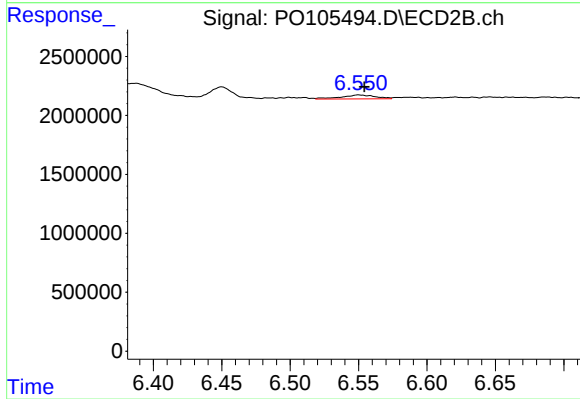

#30 AR-1254-5


R.T.: 6.550 min
Delta R.T.: -0.004 min
Response: 584942
Conc: 2.92 ng/ml

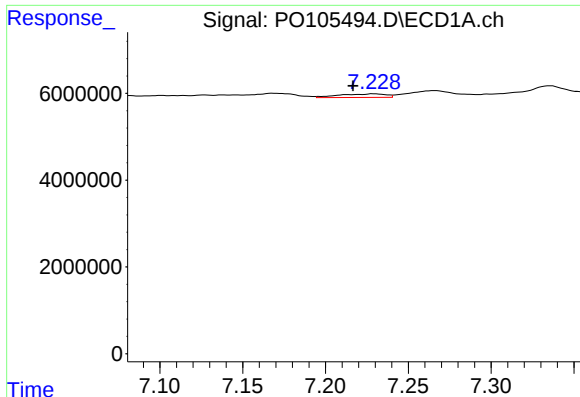

#31 AR-1260-1


R.T.: 7.229 min
Delta R.T.: 0.012 min
Response: 1596158
Conc: 4.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

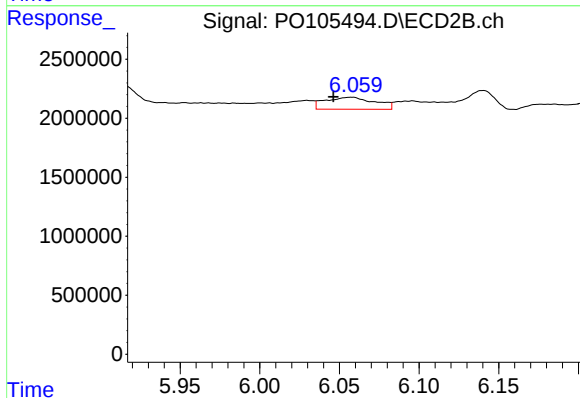


#31 AR-1260-1

R.T.: 6.058 min
Delta R.T.: 0.011 min
Response: 2205166
Conc: 14.13 ng/ml

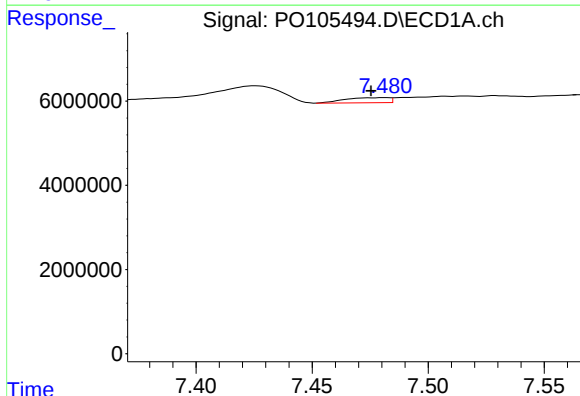


#32 AR-1260-2

R.T.: 7.481 min
Delta R.T.: 0.006 min
Response: 1582963
Conc: 3.80 ng/ml

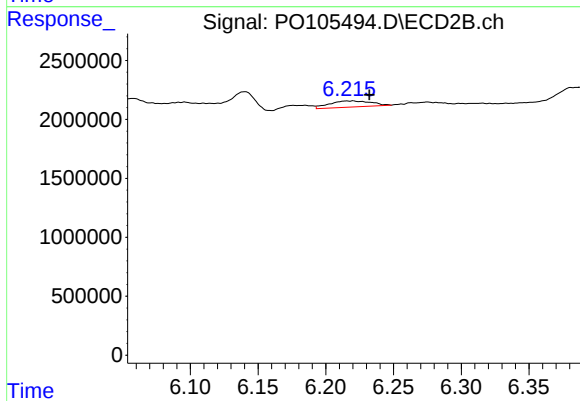

#32 AR-1260-2


R.T.: 6.220 min
Delta R.T.: -0.012 min
Response: 1120573
Conc: 5.93 ng/ml

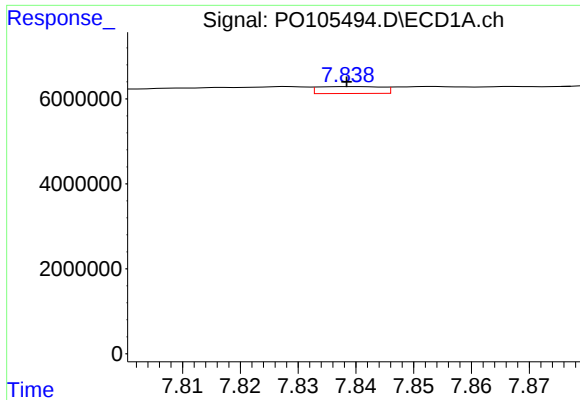

#33 AR-1260-3


R.T.: 7.839 min
Delta R.T.: 0.000 min
Response: 1246679
Conc: 4.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

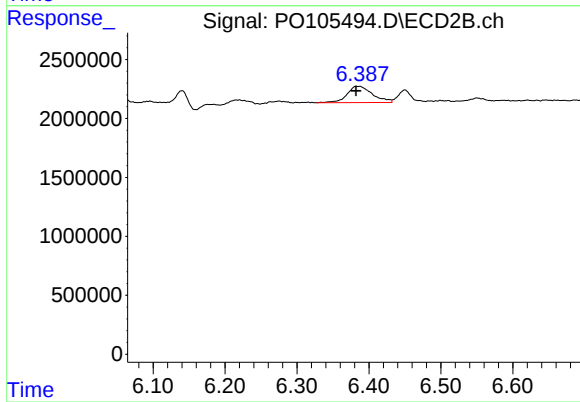


#33 AR-1260-3

R.T.: 6.387 min
Delta R.T.: 0.004 min
Response: 3398034
Conc: 18.39 ng/ml

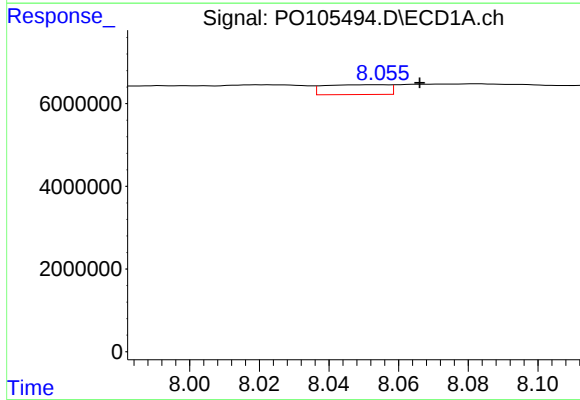


#34 AR-1260-4

R.T.: 8.055 min
Delta R.T.: -0.011 min
Response: 3057574
Conc: 9.27 ng/ml

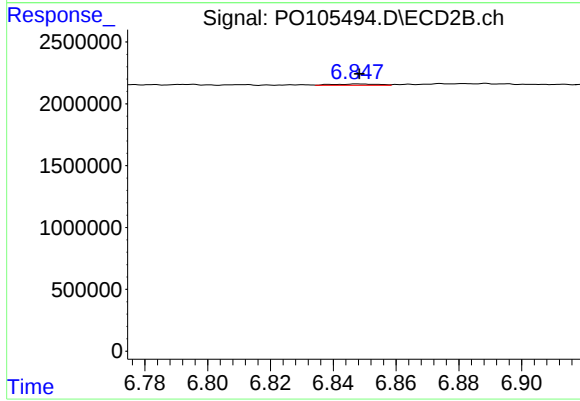

#34 AR-1260-4


R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 110161
Conc: 0.90 ng/ml

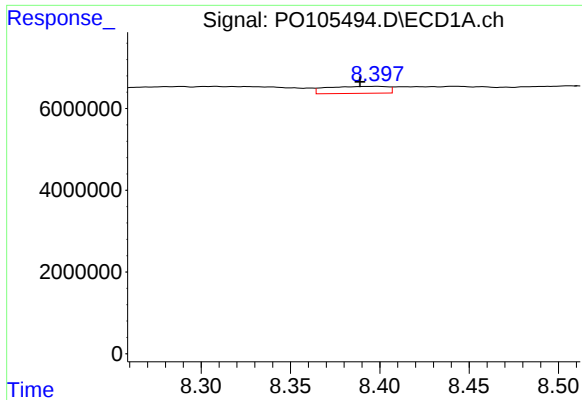

#35 AR-1260-5


R.T.: 8.399 min
Delta R.T.: 0.010 min
Response: 4022100
Conc: 6.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

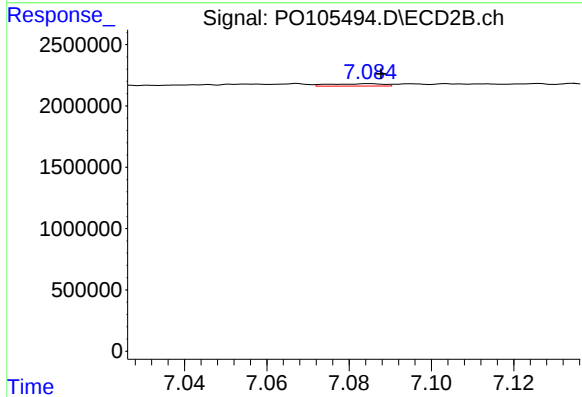


#35 AR-1260-5

R.T.: 7.085 min
Delta R.T.: -0.003 min
Response: 178508
Conc: 0.64 ng/ml

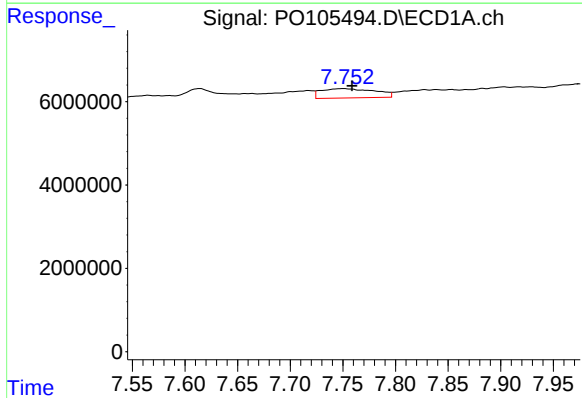


#36 AR-1262-1

R.T.: 7.751 min
Delta R.T.: -0.008 min
Response: 7961979
Conc: 25.07 ng/ml

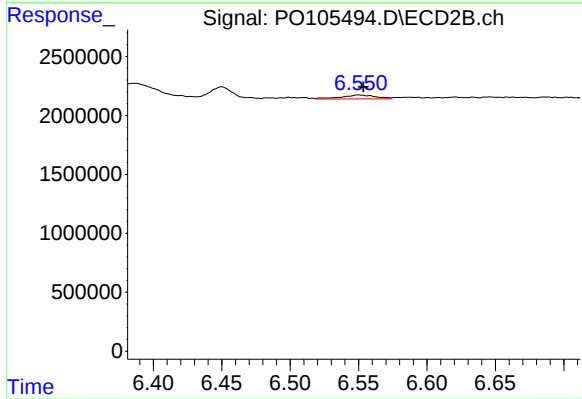

#36 AR-1262-1


R.T.: 6.550 min
Delta R.T.: -0.003 min
Response: 584942
Conc: 5.50 ng/ml

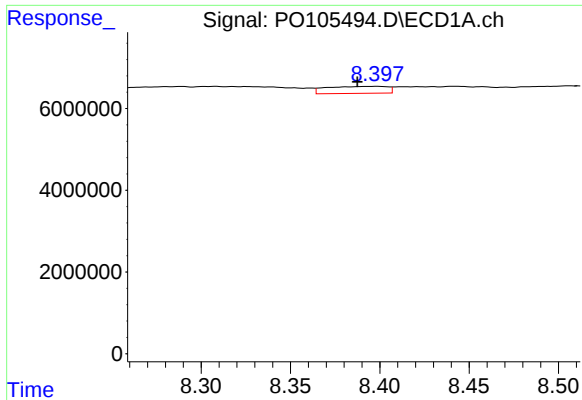

#37 AR-1262-2


R.T.: 8.399 min
Delta R.T.: 0.011 min
Response: 4022100
Conc: 5.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

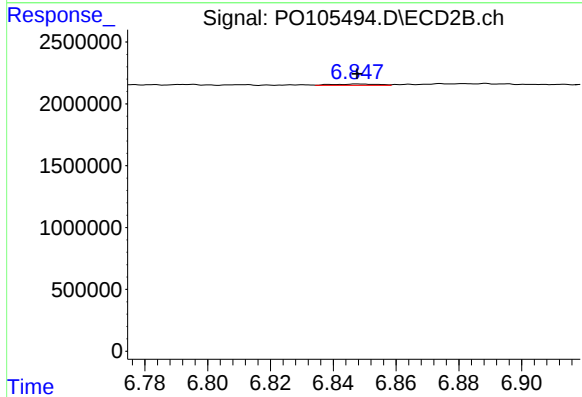


#37 AR-1262-2

R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 110161
Conc: 0.65 ng/ml

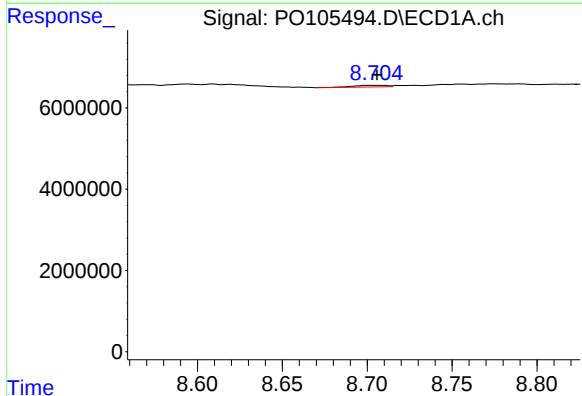


#38 AR-1262-3

R.T.: 8.705 min
Delta R.T.: 0.000 min
Response: 566713
Conc: 1.15 ng/ml

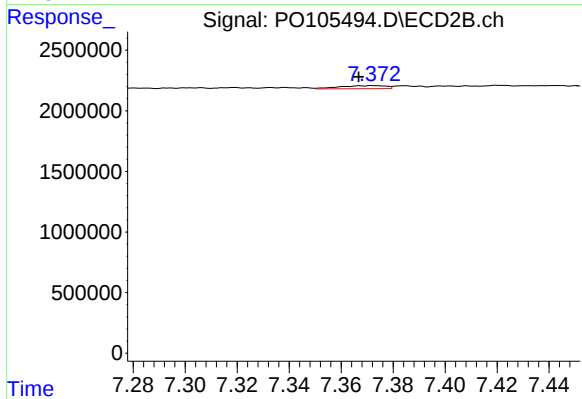

#38 AR-1262-3


R.T.: 7.373 min
Delta R.T.: 0.006 min
Response: 318457
Conc: 2.52 ng/ml

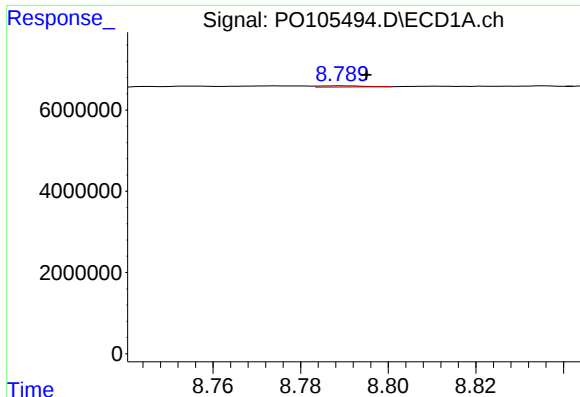

#39 AR-1262-4


R.T.: 8.789 min
Delta R.T.: -0.006 min
Response: 194239
Conc: 0.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

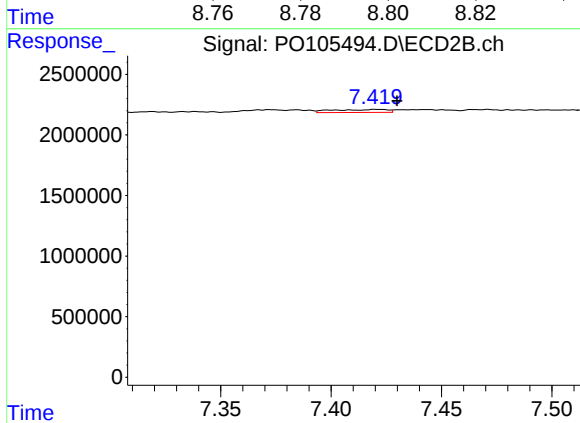


#39 AR-1262-4

R.T.: 7.421 min
Delta R.T.: -0.009 min
Response: 414057
Conc: 1.79 ng/ml

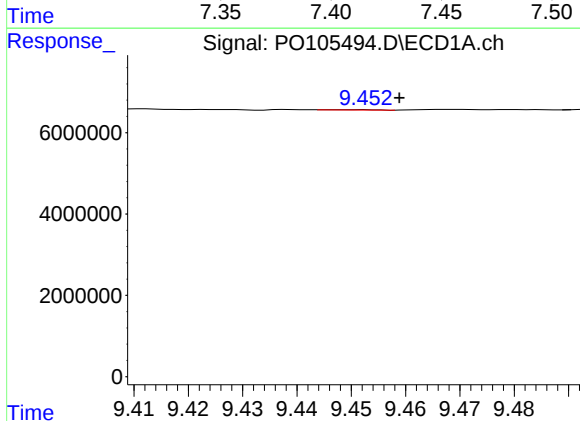


#40 AR-1262-5

R.T.: 9.452 min
Delta R.T.: -0.007 min
Response: 59368
Conc: 0.22 ng/ml

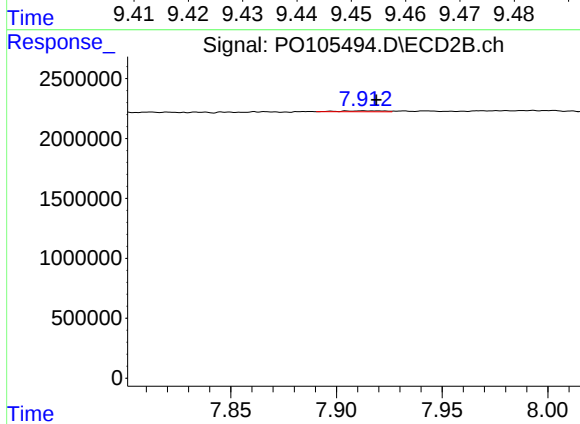

#40 AR-1262-5


R.T.: 7.913 min
Delta R.T.: -0.006 min
Response: 101883
Conc: 1.01 ng/ml

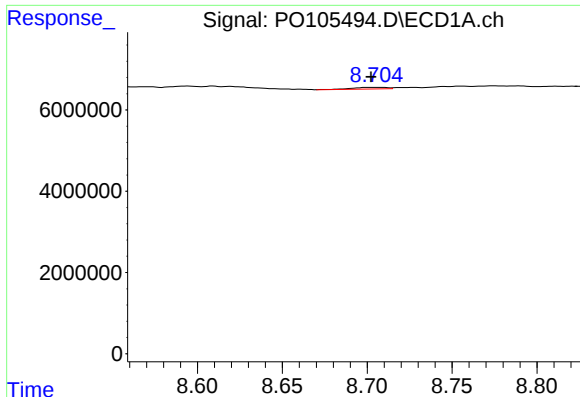

#41 AR-1268-1


R.T.: 8.705 min
Delta R.T.: 0.003 min
Response: 566713
Conc: 0.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

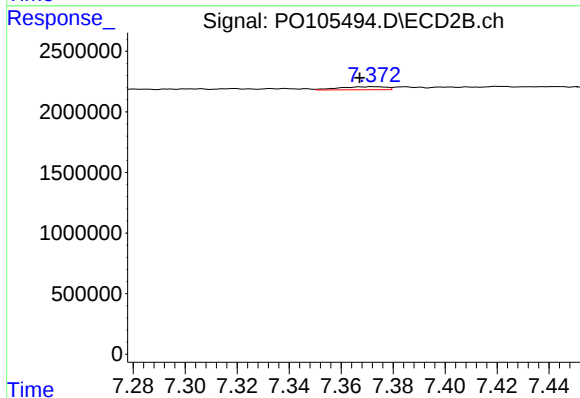


#41 AR-1268-1

R.T.: 7.373 min
Delta R.T.: 0.005 min
Response: 318457
Conc: 0.91 ng/ml

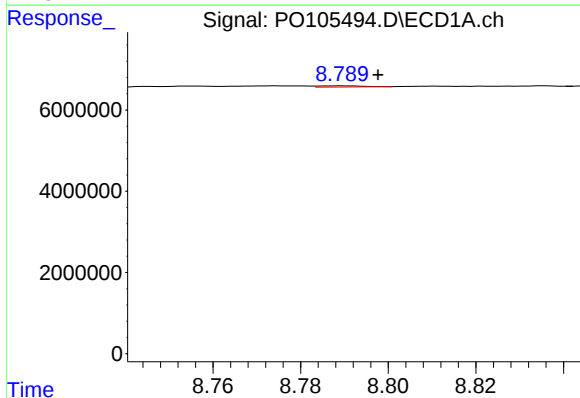


#42 AR-1268-2

R.T.: 8.789 min
Delta R.T.: -0.008 min
Response: 194239
Conc: 0.27 ng/ml

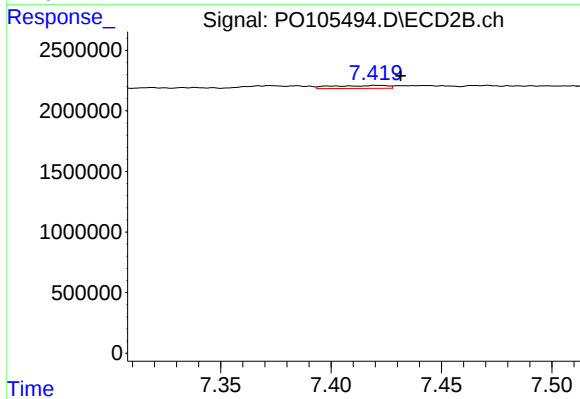

#42 AR-1268-2


R.T.: 7.421 min
Delta R.T.: -0.011 min
Response: 414057
Conc: 1.33 ng/ml

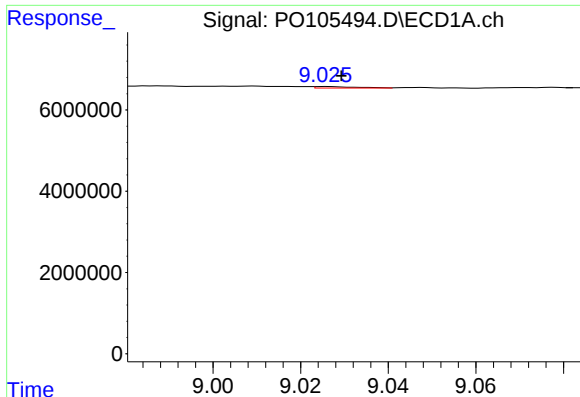

#43 AR-1268-3


R.T.: 9.025 min
Delta R.T.: -0.004 min
Response: 238364
Conc: 0.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

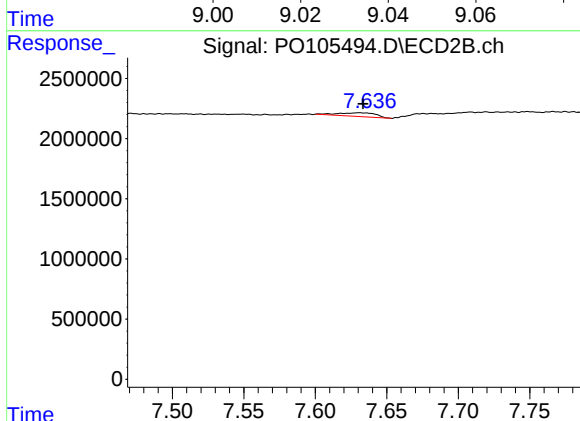


#43 AR-1268-3

R.T.: 7.631 min
Delta R.T.: -0.002 min
Response: 565976
Conc: 2.24 ng/ml

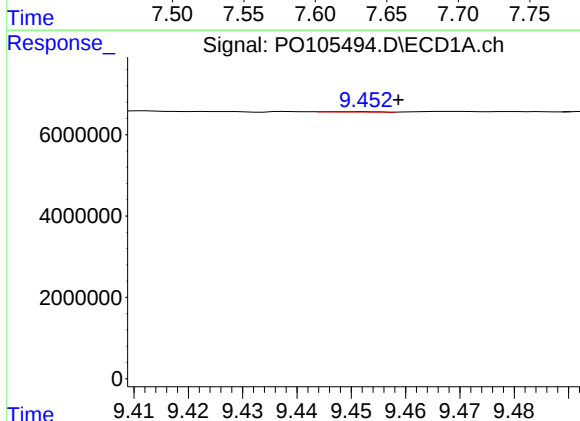


#44 AR-1268-4

R.T.: 9.452 min
Delta R.T.: -0.006 min
Response: 59368
Conc: 0.21 ng/ml

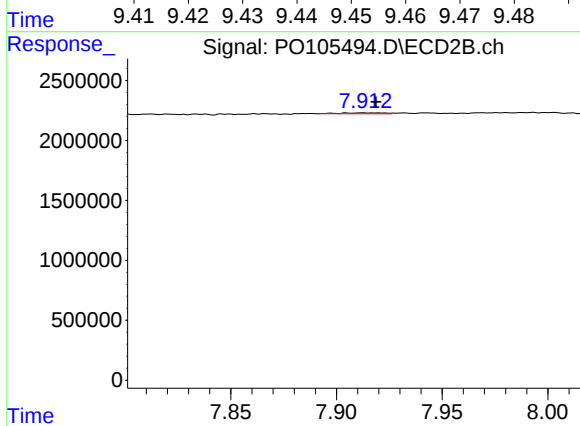

#44 AR-1268-4


R.T.: 7.913 min
Delta R.T.: -0.006 min
Response: 101883
Conc: 0.95 ng/ml

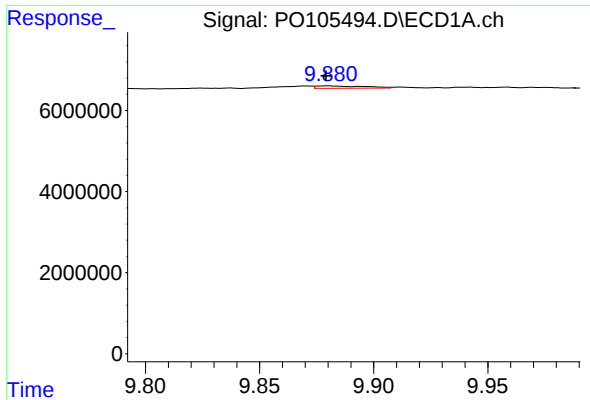

#45 AR-1268-5

R.T.: 9.880 min
Delta R.T.: 0.001 min
Response: 876853
Conc: 0.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

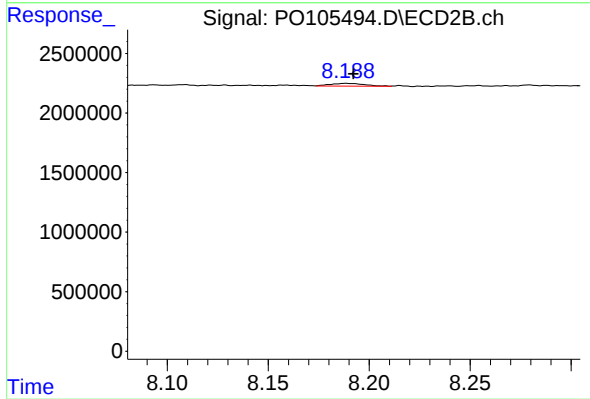

#45 AR-1268-5

R.T.: 8.189 min
Delta R.T.: -0.003 min
Response: 284876
Conc: 0.43 ng/ml