

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081324\
 Data File : P0105497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 13:59
 Operator : YP/AJ
 Sample : P3390-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:09:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.426	3.534	99317061	45712308	11.371	14.554 #
2)	SA Decachlor...	10.217	8.426	83224493	31002377	14.467	17.512
Target Compounds							
3)	L1 AR-1016-1	5.597	4.588	73338	47724	0.242	0.425 #
4)	L1 AR-1016-2	5.623	4.614	153291	45884	0.359	0.295
5)	L1 AR-1016-3	5.683	4.791	74663	57243	0.291	0.684 #
6)	L1 AR-1016-4	5.788	4.837	489344	70257	2.237	1.043 #
7)	L1 AR-1016-5	6.081	5.033	305174	106630	1.426	1.274
8)	L2 AR-1221-1	4.634	3.761	1524310	41596	13.593	1.054 #
9)	L2 AR-1221-2	4.732	3.824	1768505	1198490	20.865	39.010 #
10)	L2 AR-1221-3	4.763f	3.898	787338	37907	3.236	0.424 #
11)	L3 AR-1232-1	4.763f	3.898	787338	37907	3.938	0.519 #
12)	L3 AR-1232-2	5.320	4.614	376162	45884	3.554	0.653 #
13)	L3 AR-1232-3	5.623	4.791	153291	57243	0.801	1.498 #
14)	L3 AR-1232-4	5.788	4.857	489344	62786	5.017	1.805 #
15)	L3 AR-1232-5	5.869	5.033	208872	106630	2.898	3.021
16)	L4 AR-1242-1	5.597	4.588	73338	47724	0.316	0.541 #
17)	L4 AR-1242-2	5.623	4.605	153291	37851	0.470	0.319 #
18)	L4 AR-1242-3	5.683	4.791	74663	57243	0.378	0.882 #
19)	L4 AR-1242-4	5.788	4.857	489344	62786	2.868	0.947 #
20)	L4 AR-1242-5	6.546	5.394	1003462	756356	5.742	9.205 #
21)	L5 AR-1248-1	5.597	4.588	73338	47724	0.402	0.683 #
22)	L5 AR-1248-2	5.869	4.837	208872	70257	0.829	0.740
23)	L5 AR-1248-3	6.081	4.857	305174	62786	1.080	0.629 #
24)	L5 AR-1248-4	6.490	5.033	918320	106630	2.872	0.945 #
25)	L5 AR-1248-5	6.546	5.424	1003462	263508	3.244	2.340 #
26)	L6 AR-1254-1	6.465	5.394	856056	756356	2.730	4.646 #
27)	L6 AR-1254-2	6.683	5.508	411158	436071	0.911	2.981 #
28)	L6 AR-1254-3	7.056	5.910	2322671	587369	4.896	2.604 #
29)	L6 AR-1254-4	7.325	6.138	2048506	896048	5.719	6.350
30)	L6 AR-1254-5	7.747	6.541	10685135	298415	26.917	1.490 #
31)	L7 AR-1260-1	7.232	6.055	2076904	491818	5.667	3.151 #
32)	L7 AR-1260-2	7.506	6.215	3258356	980043	7.826	5.185 #
33)	L7 AR-1260-3	7.835	6.391	7663521	3298248	29.610	17.854 #
34)	L7 AR-1260-4	8.084	6.841	11412390	2051554	34.590	16.785 #
35)	L7 AR-1260-5	8.384	7.085	6677867	1218995	11.226	4.380 #
36)	L8 AR-1262-1	7.747	6.541	10685135	298415	33.640	2.805 #
37)	L8 AR-1262-2	8.384	6.841	6677867	2051554	8.878	12.073 #
38)	L8 AR-1262-3	8.699	7.365	14324944	7637160	29.111	60.492 #
39)	L8 AR-1262-4	8.793	7.429	13052503	6973420	35.545	30.124
40)	L8 AR-1262-5	9.455	7.917	4105264	2234737	15.329	22.236 #
41)	L9 AR-1268-1	8.699	7.365	14324944	7637160	17.613	21.875

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081324\
Data File : P0105497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 13:59
Operator : YP/AJ
Sample : P3390-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:09:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.793	7.429	13052503	6973420	17.955	22.352
43)	L9 AR-1268-3	9.025	7.631	11454747	5715396	17.743	22.613 #
44)	L9 AR-1268-4	9.455	7.917	4105264	2234737	14.743	20.778 #
45)	L9 AR-1268-5	9.874	8.190	36124569	14300611	17.278	21.379



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081324\
Data File : PO105497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 13:59
Operator : YP/AJ
Sample : P3390-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:09:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

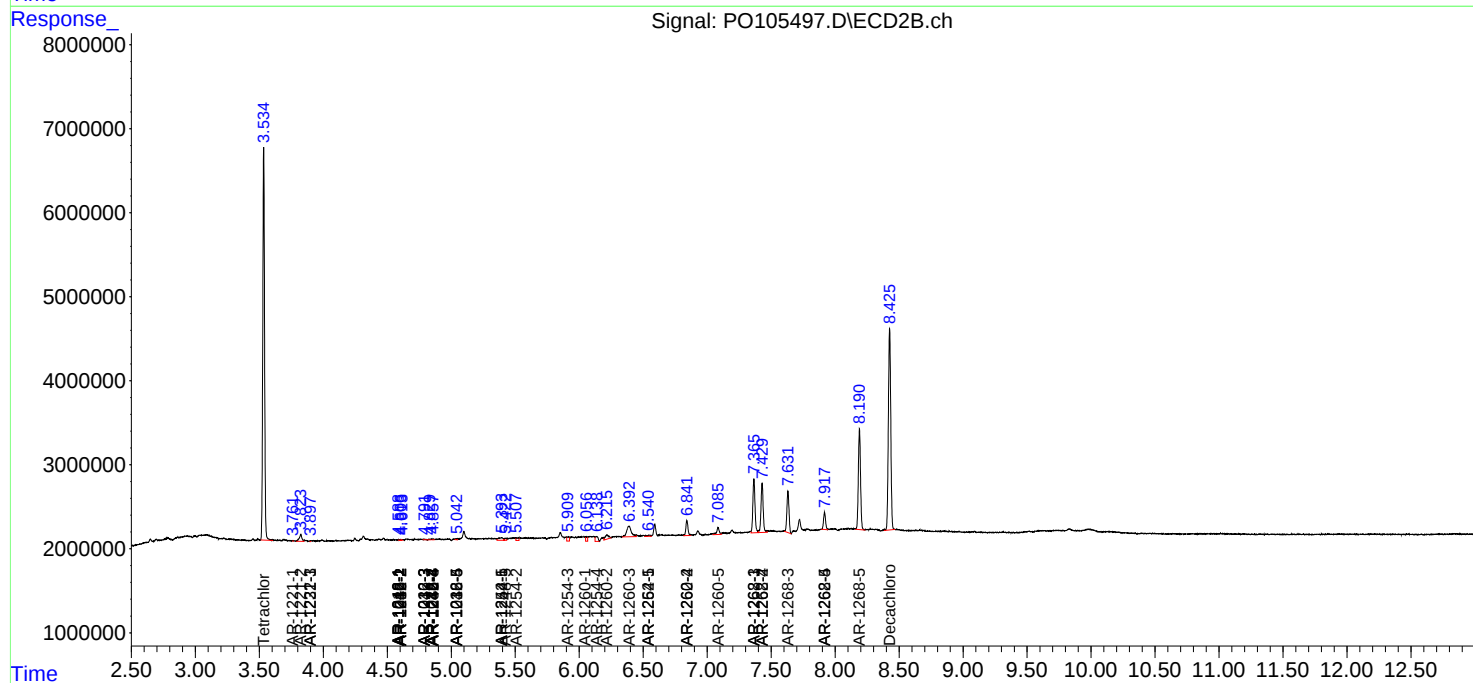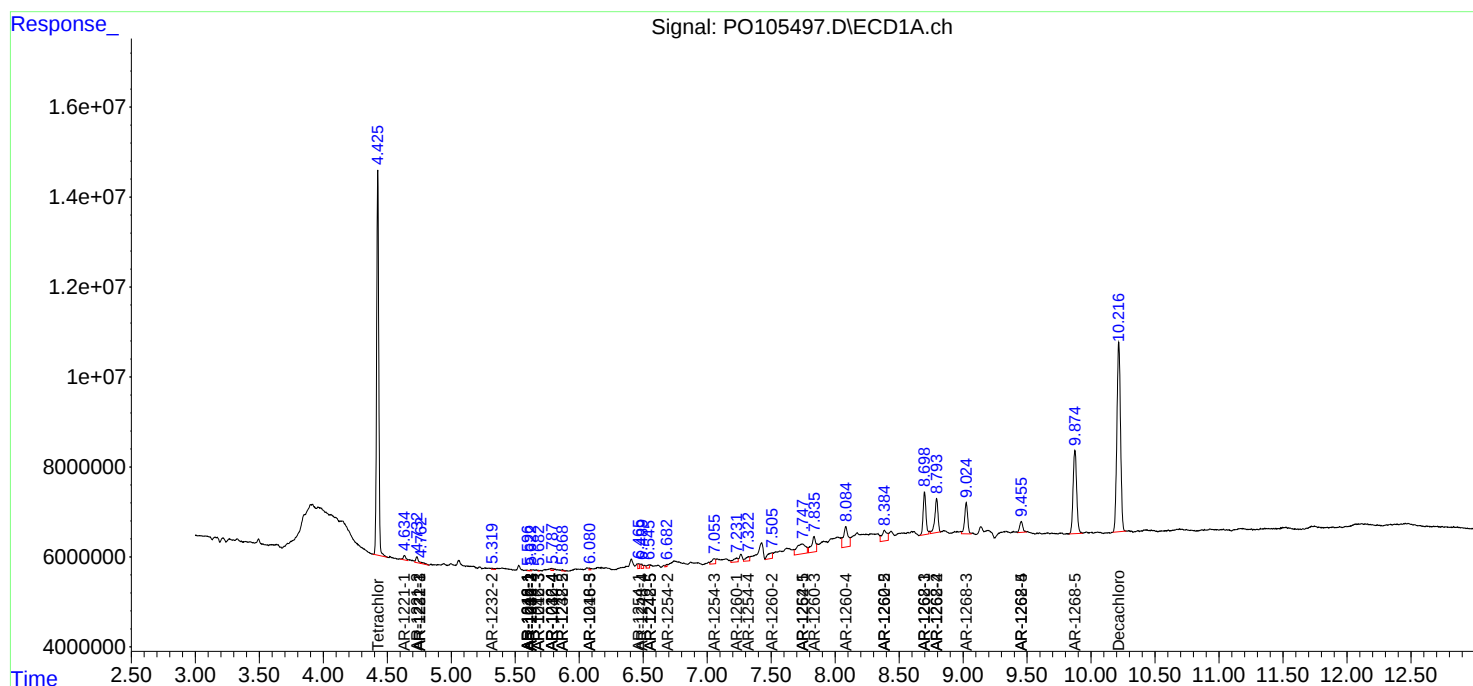


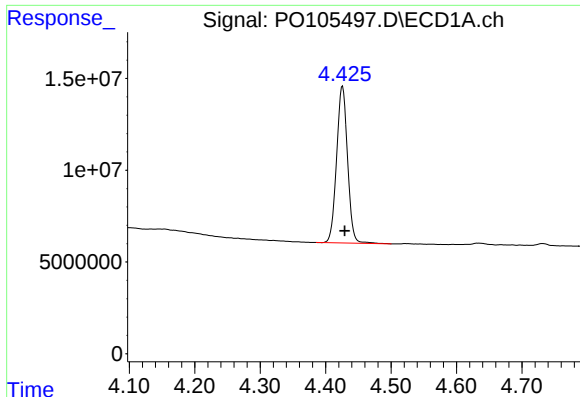

#1 Tetrachloro-m-xylene


R.T.: 4.426 min
Delta R.T.: -0.003 min
Response: 99317061
Conc: 11.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

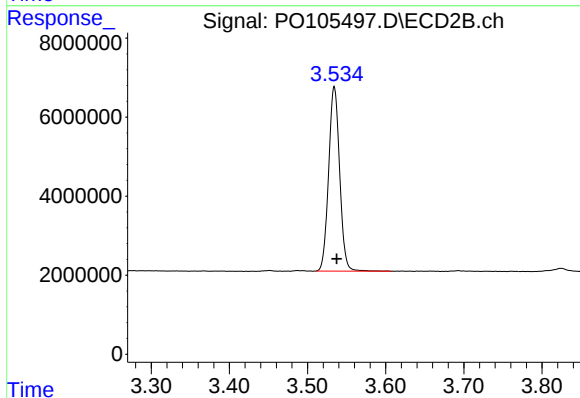


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: -0.003 min
Response: 45712308
Conc: 14.55 ng/ml

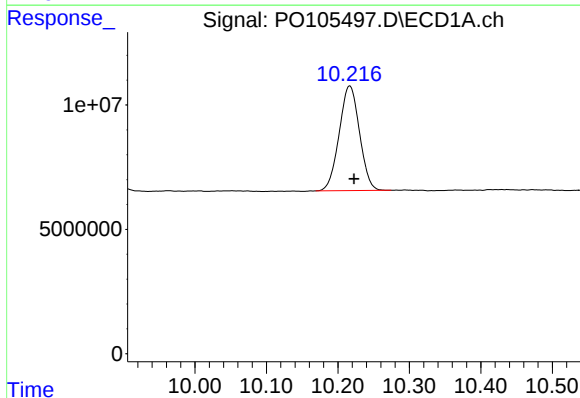


#2 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: -0.006 min
Response: 83224493
Conc: 14.47 ng/ml

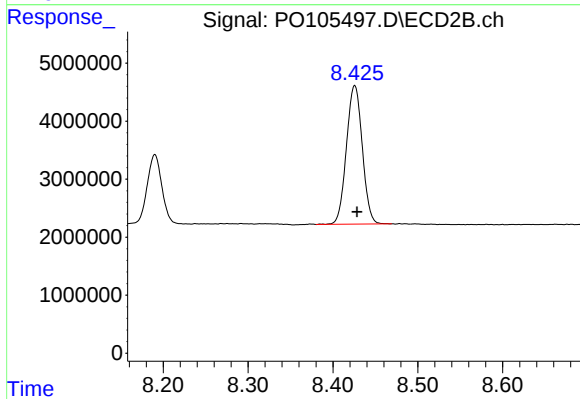

#2 Decachlorobiphenyl


R.T.: 8.426 min
Delta R.T.: -0.003 min
Response: 31002377
Conc: 17.51 ng/ml

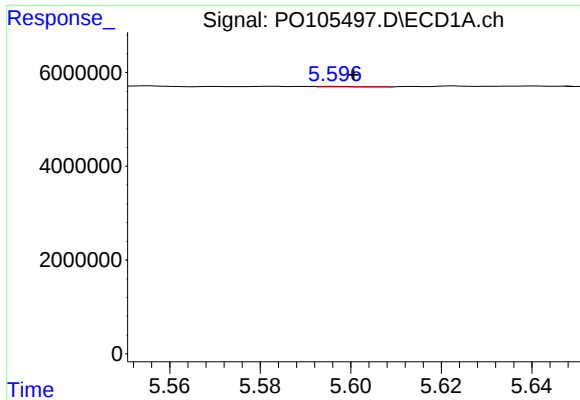

#3 AR-1016-1


R.T.: 5.597 min
Delta R.T.: -0.004 min
Response: 73338
Conc: 0.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

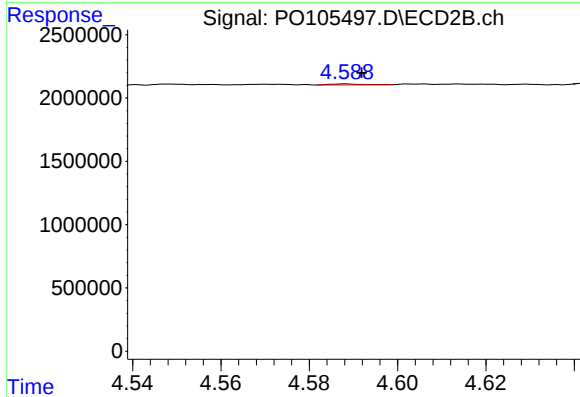


#3 AR-1016-1

R.T.: 4.588 min
Delta R.T.: -0.004 min
Response: 47724
Conc: 0.42 ng/ml

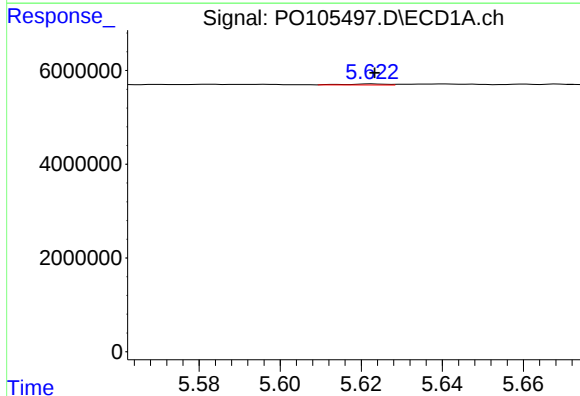


#4 AR-1016-2

R.T.: 5.623 min
Delta R.T.: 0.000 min
Response: 153291
Conc: 0.36 ng/ml

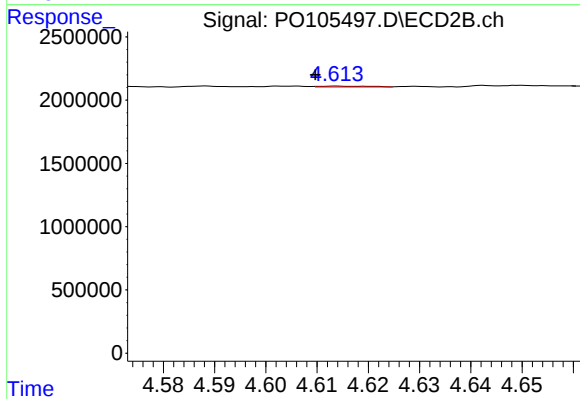

#4 AR-1016-2


R.T.: 4.614 min
Delta R.T.: 0.004 min
Response: 45884
Conc: 0.29 ng/ml

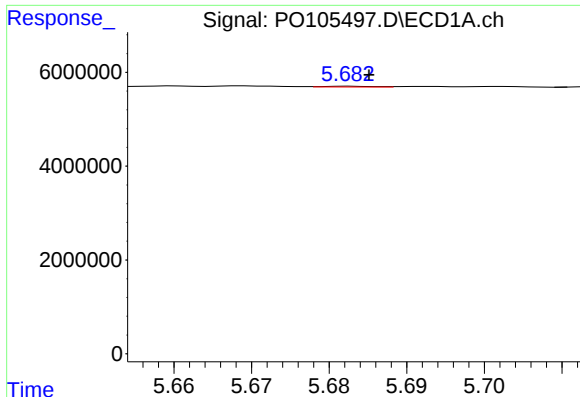

#5 AR-1016-3


R.T.: 5.683 min
Delta R.T.: -0.003 min
Response: 74663
Conc: 0.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

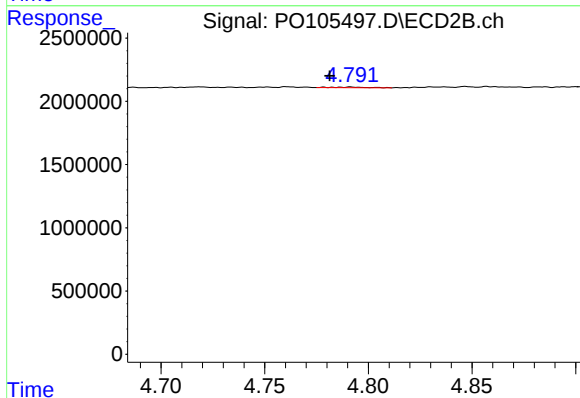


#5 AR-1016-3

R.T.: 4.791 min
Delta R.T.: 0.010 min
Response: 57243
Conc: 0.68 ng/ml

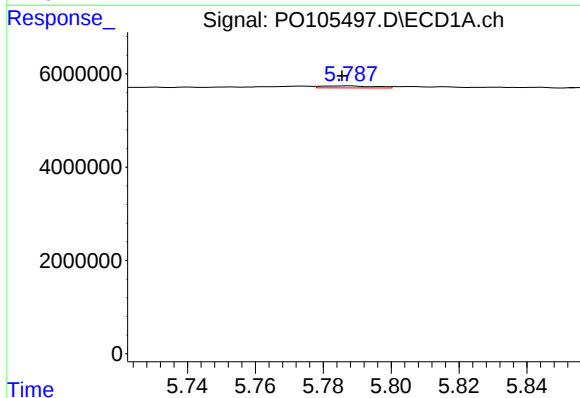


#6 AR-1016-4

R.T.: 5.788 min
Delta R.T.: 0.002 min
Response: 489344
Conc: 2.24 ng/ml

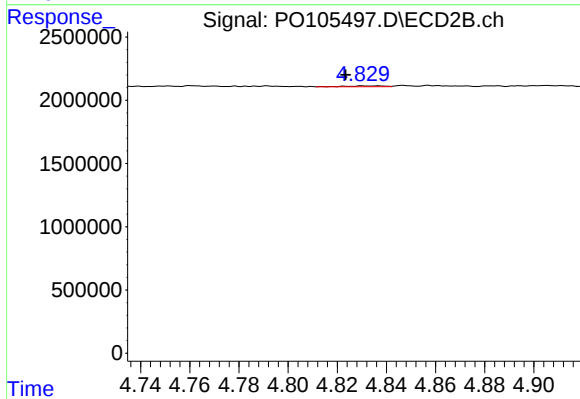

#6 AR-1016-4


R.T.: 4.837 min
Delta R.T.: 0.013 min
Response: 70257
Conc: 1.04 ng/ml

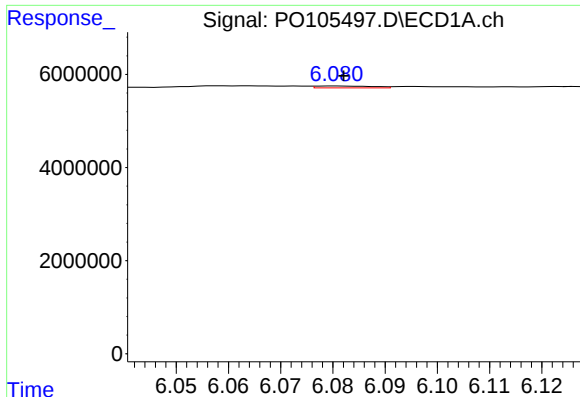

#7 AR-1016-5


R.T.: 6.081 min
Delta R.T.: -0.001 min
Response: 305174
Conc: 1.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

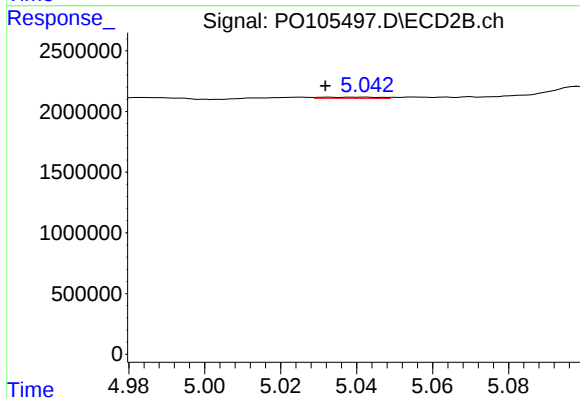


#7 AR-1016-5

R.T.: 5.033 min
Delta R.T.: 0.001 min
Response: 106630
Conc: 1.27 ng/ml

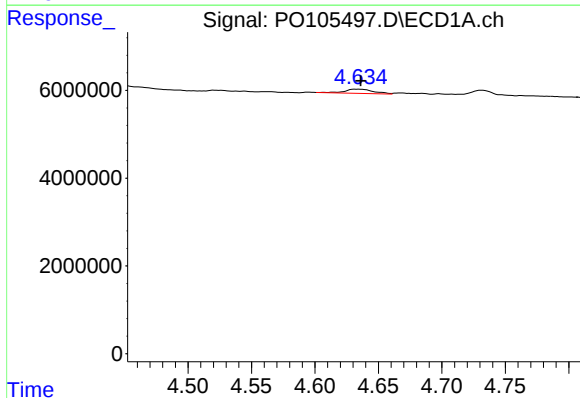


#8 AR-1221-1

R.T.: 4.634 min
Delta R.T.: -0.002 min
Response: 1524310
Conc: 13.59 ng/ml

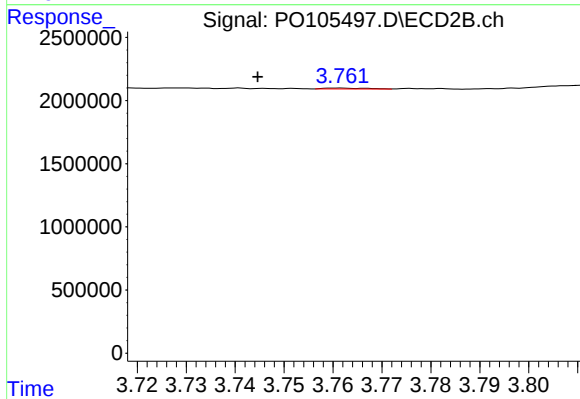

#8 AR-1221-1


R.T.: 3.761 min
Delta R.T.: 0.016 min
Response: 41596
Conc: 1.05 ng/ml

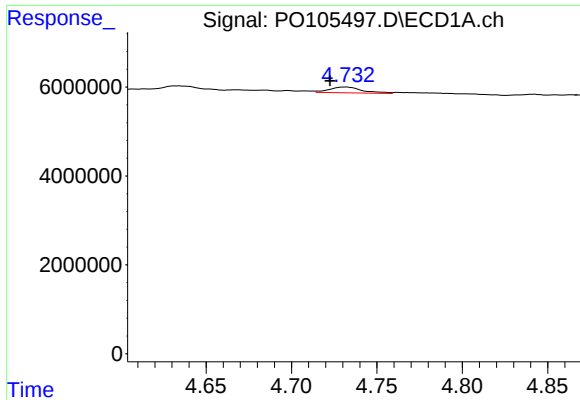

#9 AR-1221-2


R.T.: 4.732 min
Delta R.T.: 0.009 min
Response: 1768505
Conc: 20.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

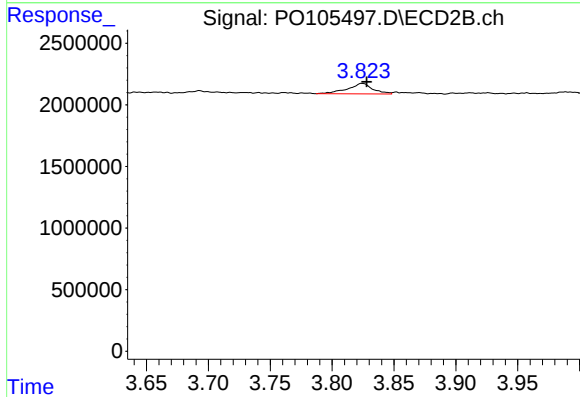


#9 AR-1221-2

R.T.: 3.824 min
Delta R.T.: -0.004 min
Response: 1198490
Conc: 39.01 ng/ml

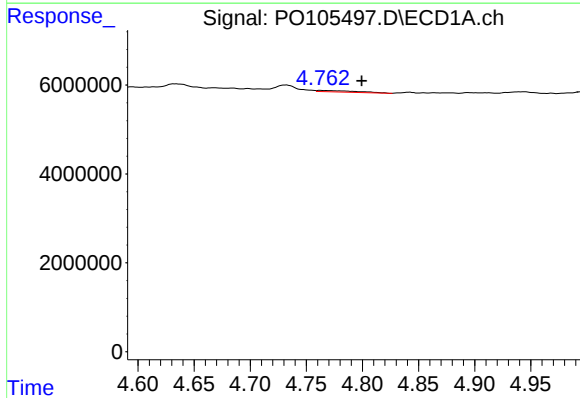


#10 AR-1221-3

R.T.: 4.763 min
Delta R.T.: -0.037 min
Response: 787338
Conc: 3.24 ng/ml

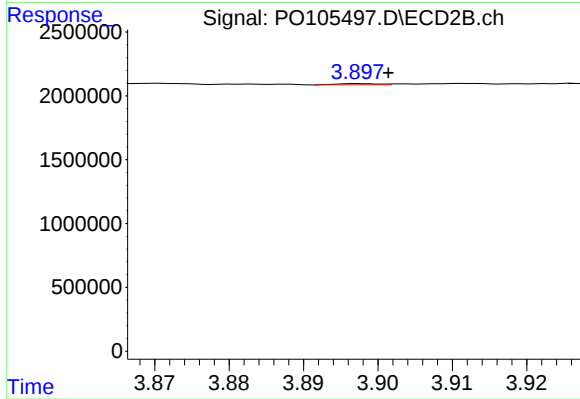

#10 AR-1221-3


R.T.: 3.898 min
Delta R.T.: -0.004 min
Response: 37907
Conc: 0.42 ng/ml

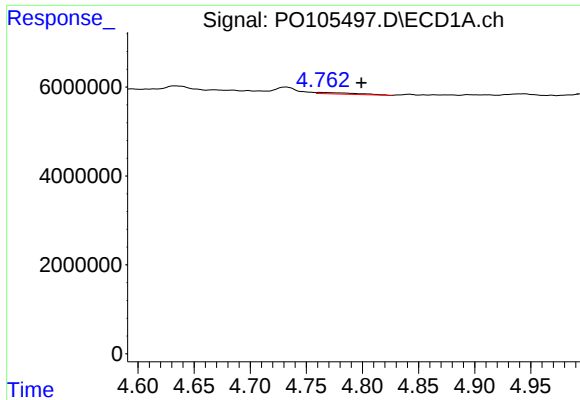

#11 AR-1232-1


R.T.: 4.763 min
Delta R.T.: -0.037 min
Response: 787338
Conc: 3.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

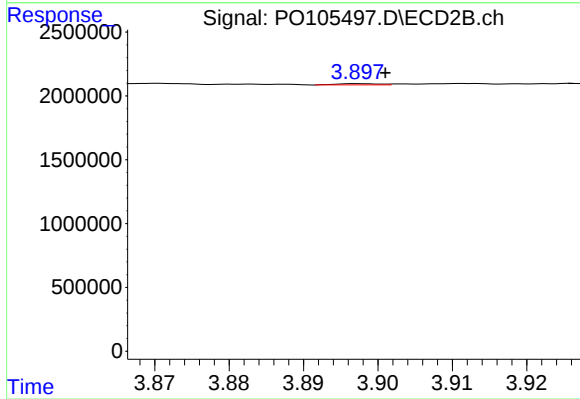


#11 AR-1232-1

R.T.: 3.898 min
Delta R.T.: -0.003 min
Response: 37907
Conc: 0.52 ng/ml

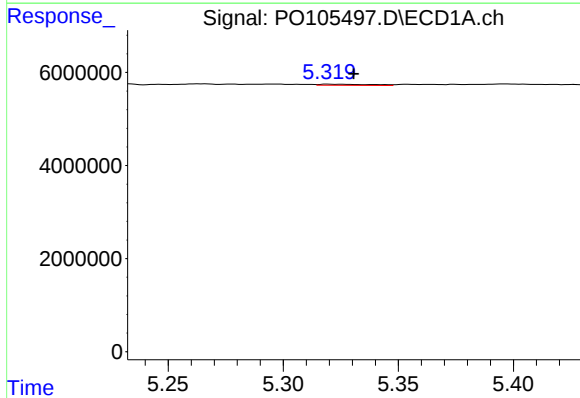


#12 AR-1232-2

R.T.: 5.320 min
Delta R.T.: -0.011 min
Response: 376162
Conc: 3.55 ng/ml

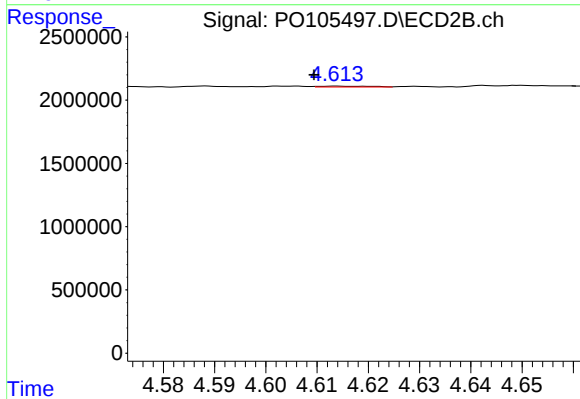

#12 AR-1232-2


R.T.: 4.614 min
Delta R.T.: 0.004 min
Response: 45884
Conc: 0.65 ng/ml

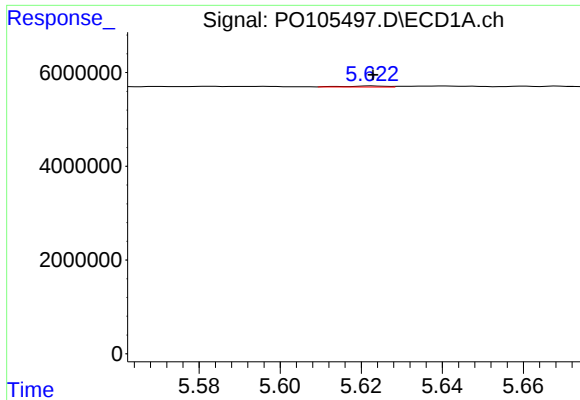

#13 AR-1232-3


R.T.: 5.623 min
Delta R.T.: 0.000 min
Response: 153291
Conc: 0.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

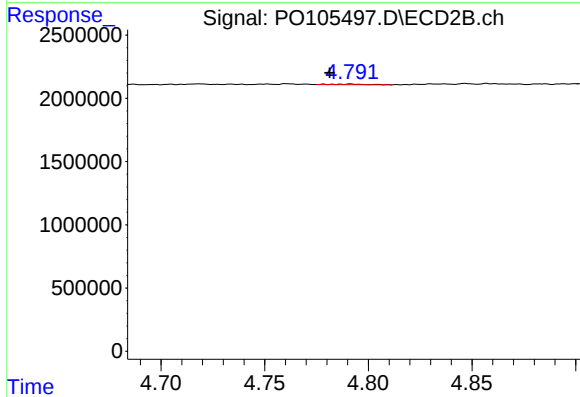


#13 AR-1232-3

R.T.: 4.791 min
Delta R.T.: 0.010 min
Response: 57243
Conc: 1.50 ng/ml

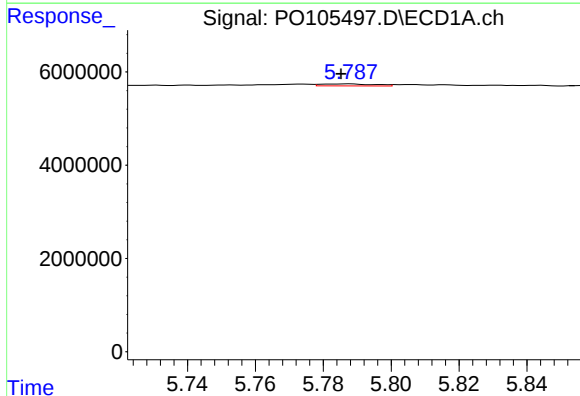


#14 AR-1232-4

R.T.: 5.788 min
Delta R.T.: 0.002 min
Response: 489344
Conc: 5.02 ng/ml

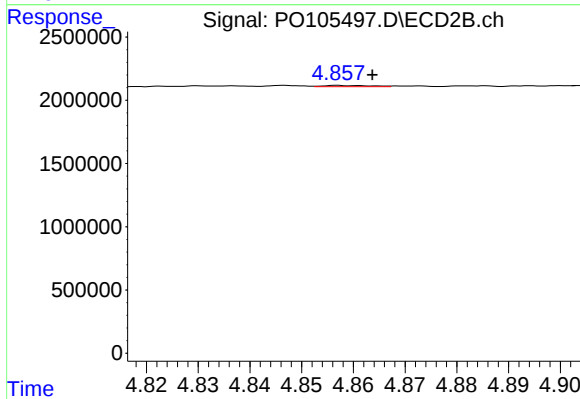

#14 AR-1232-4


R.T.: 4.857 min
Delta R.T.: -0.006 min
Response: 62786
Conc: 1.80 ng/ml

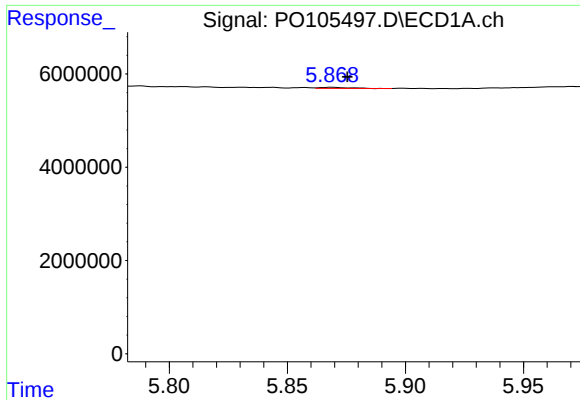

#15 AR-1232-5


R.T.: 5.869 min
Delta R.T.: -0.006 min
Response: 208872
Conc: 2.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

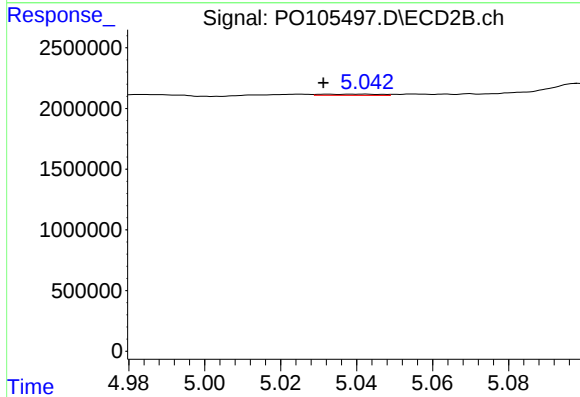


#15 AR-1232-5

R.T.: 5.033 min
Delta R.T.: 0.002 min
Response: 106630
Conc: 3.02 ng/ml

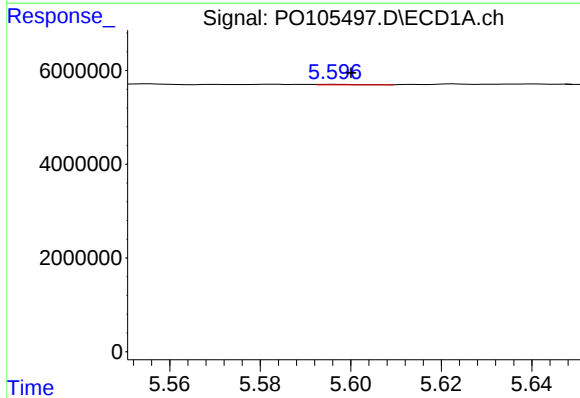


#16 AR-1242-1

R.T.: 5.597 min
Delta R.T.: -0.003 min
Response: 73338
Conc: 0.32 ng/ml

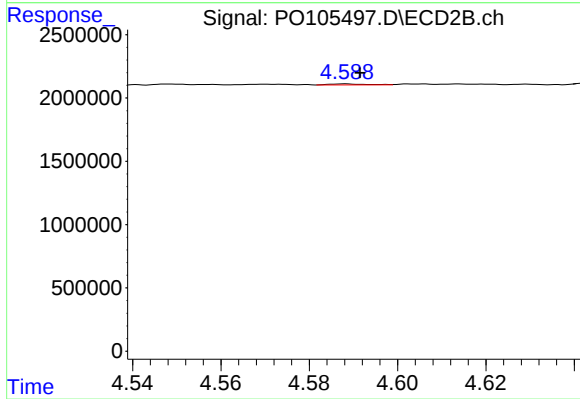

#16 AR-1242-1


R.T.: 4.588 min
Delta R.T.: -0.003 min
Response: 47724
Conc: 0.54 ng/ml

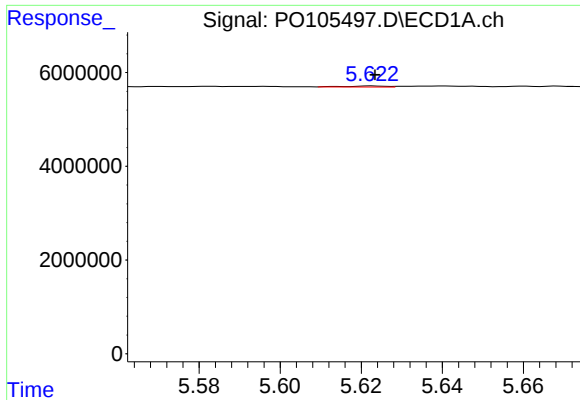

#17 AR-1242-2


R.T.: 5.623 min
Delta R.T.: 0.000 min
Response: 153291
Conc: 0.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

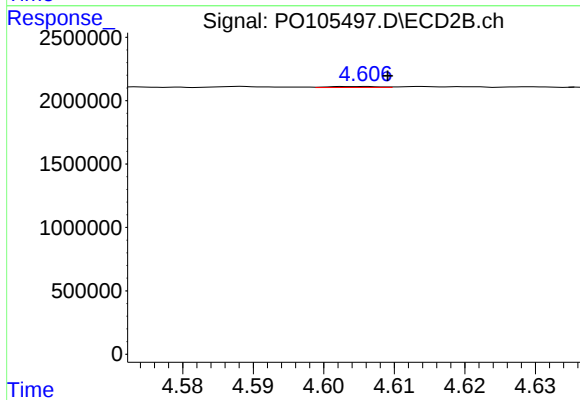


#17 AR-1242-2

R.T.: 4.605 min
Delta R.T.: -0.004 min
Response: 37851
Conc: 0.32 ng/ml

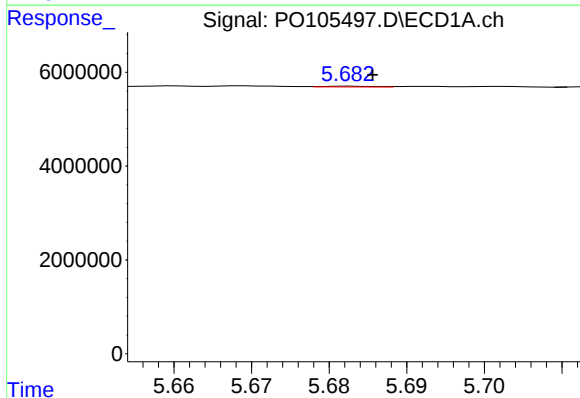


#18 AR-1242-3

R.T.: 5.683 min
Delta R.T.: -0.003 min
Response: 74663
Conc: 0.38 ng/ml

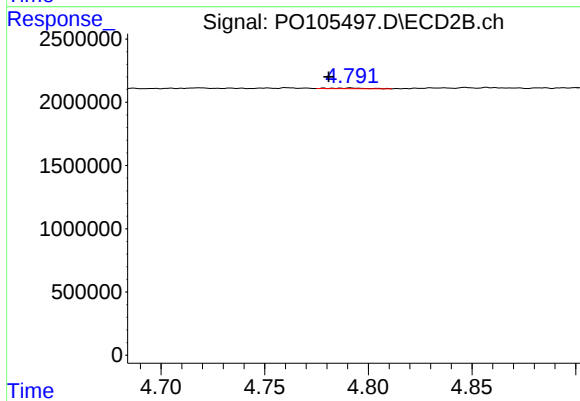

#18 AR-1242-3


R.T.: 4.791 min
Delta R.T.: 0.011 min
Response: 57243
Conc: 0.88 ng/ml

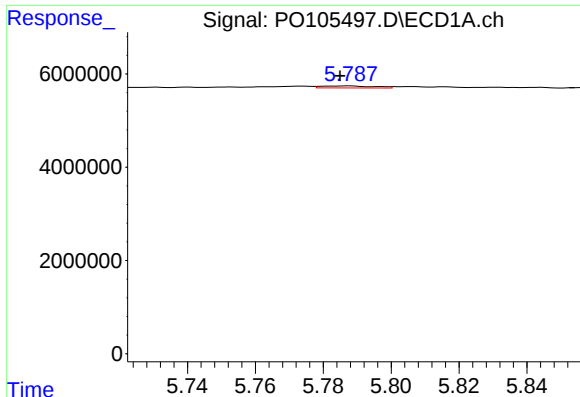

#19 AR-1242-4


R.T.: 5.788 min
Delta R.T.: 0.003 min
Response: 489344
Conc: 2.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

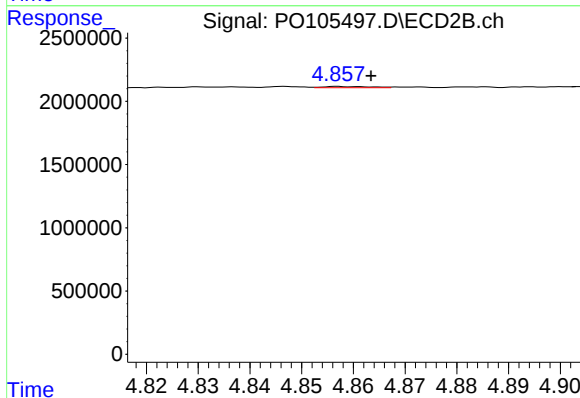


#19 AR-1242-4

R.T.: 4.857 min
Delta R.T.: -0.006 min
Response: 62786
Conc: 0.95 ng/ml

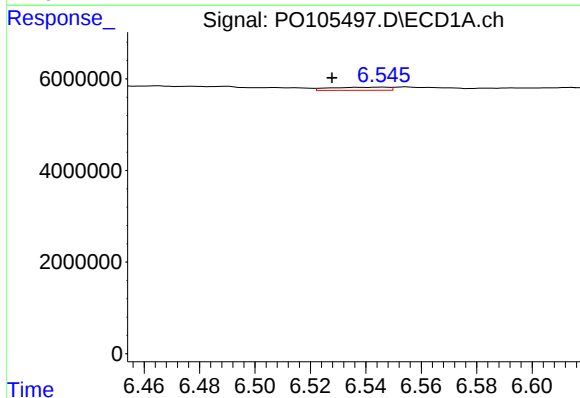


#20 AR-1242-5

R.T.: 6.546 min
Delta R.T.: 0.018 min
Response: 1003462
Conc: 5.74 ng/ml

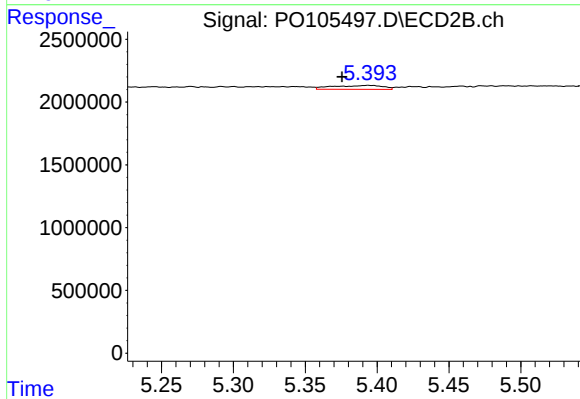

#20 AR-1242-5


R.T.: 5.394 min
Delta R.T.: 0.018 min
Response: 756356
Conc: 9.20 ng/ml

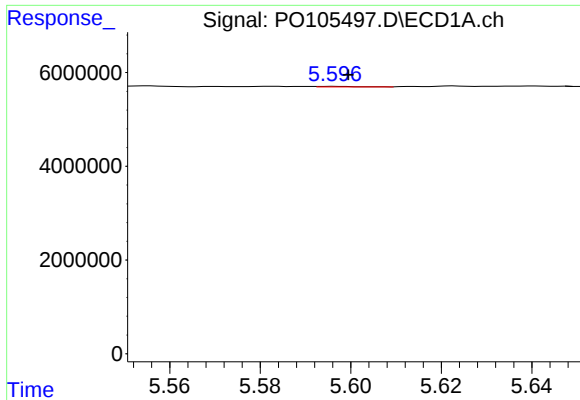

#21 AR-1248-1


R.T.: 5.597 min
Delta R.T.: -0.003 min
Response: 73338
Conc: 0.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

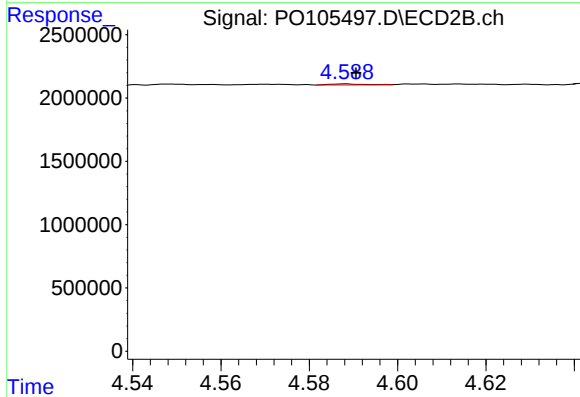


#21 AR-1248-1

R.T.: 4.588 min
Delta R.T.: -0.002 min
Response: 47724
Conc: 0.68 ng/ml

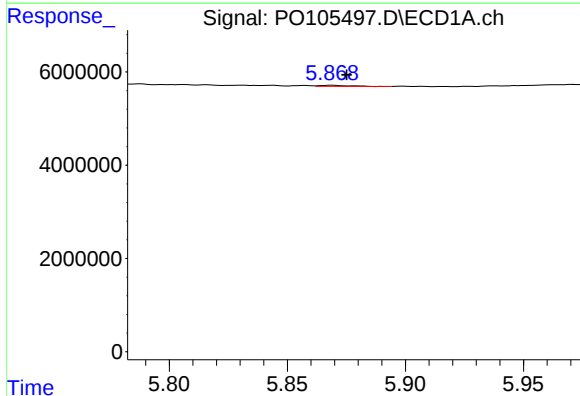


#22 AR-1248-2

R.T.: 5.869 min
Delta R.T.: -0.006 min
Response: 208872
Conc: 0.83 ng/ml

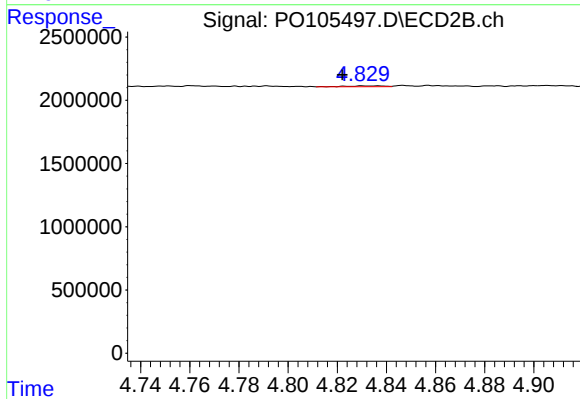

#22 AR-1248-2


R.T.: 4.837 min
Delta R.T.: 0.015 min
Response: 70257
Conc: 0.74 ng/ml

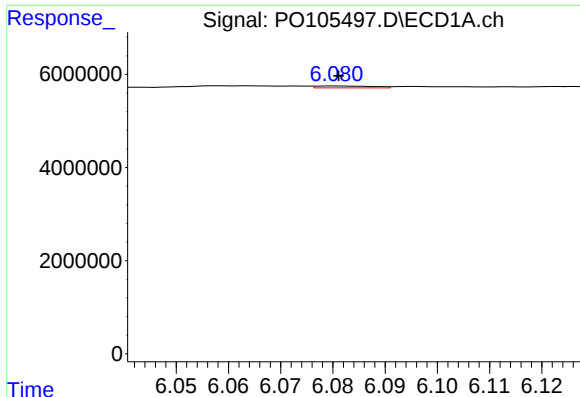

#23 AR-1248-3


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 305174
Conc: 1.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

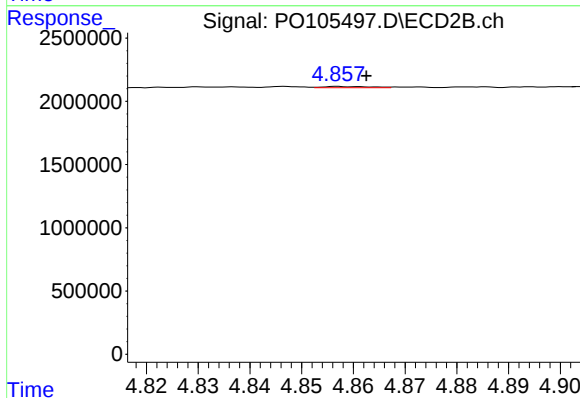


#23 AR-1248-3

R.T.: 4.857 min
Delta R.T.: -0.005 min
Response: 62786
Conc: 0.63 ng/ml

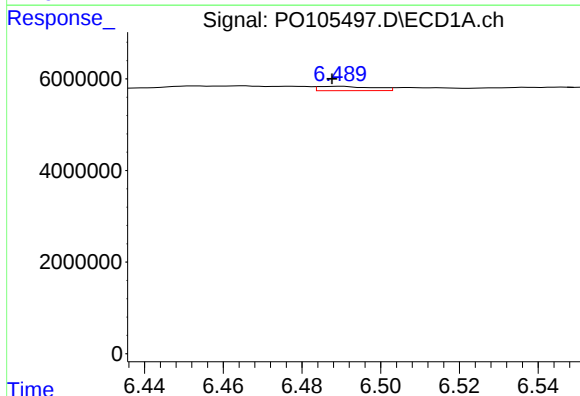


#24 AR-1248-4

R.T.: 6.490 min
Delta R.T.: 0.002 min
Response: 918320
Conc: 2.87 ng/ml

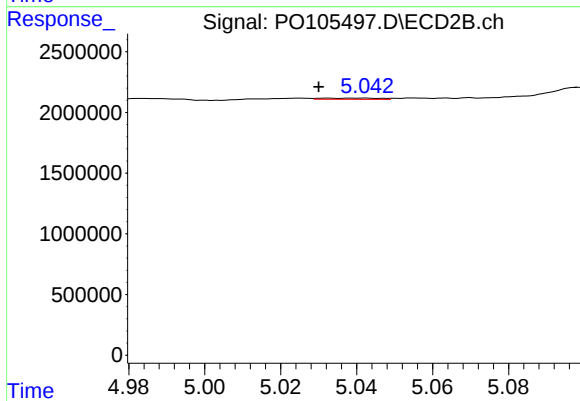

#24 AR-1248-4


R.T.: 5.033 min
Delta R.T.: 0.003 min
Response: 106630
Conc: 0.94 ng/ml

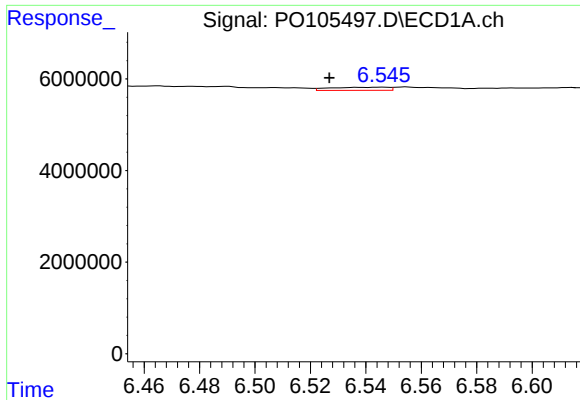

#25 AR-1248-5


R.T.: 6.546 min
Delta R.T.: 0.019 min
Response: 1003462
Conc: 3.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

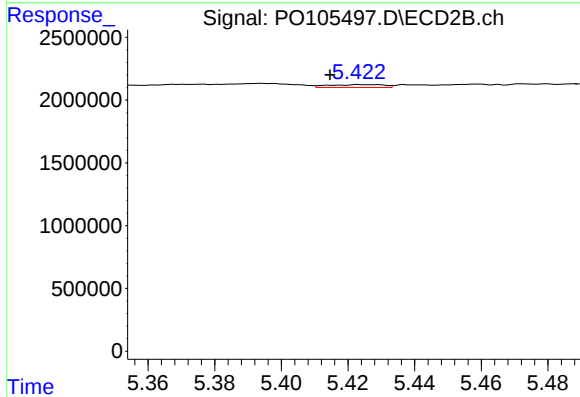


#25 AR-1248-5

R.T.: 5.424 min
Delta R.T.: 0.009 min
Response: 263508
Conc: 2.34 ng/ml

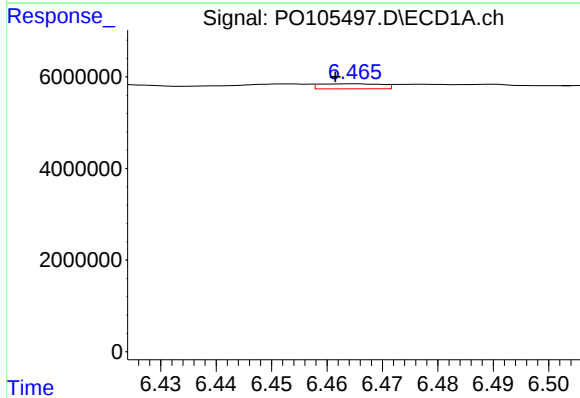


#26 AR-1254-1

R.T.: 6.465 min
Delta R.T.: 0.003 min
Response: 856056
Conc: 2.73 ng/ml

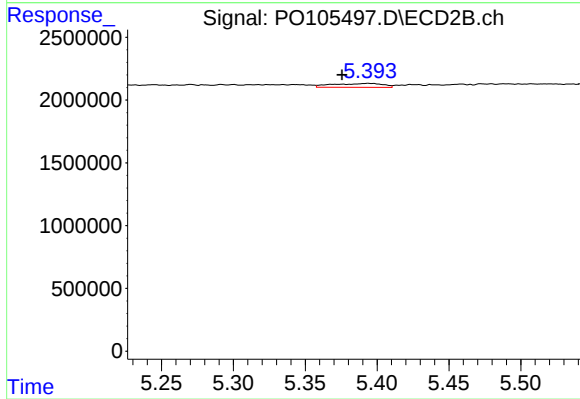

#26 AR-1254-1


R.T.: 5.394 min
Delta R.T.: 0.018 min
Response: 756356
Conc: 4.65 ng/ml

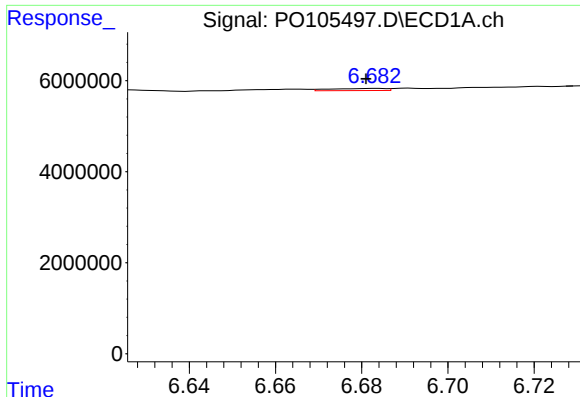

#27 AR-1254-2


R.T.: 6.683 min
Delta R.T.: 0.002 min
Response: 411158
Conc: 0.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

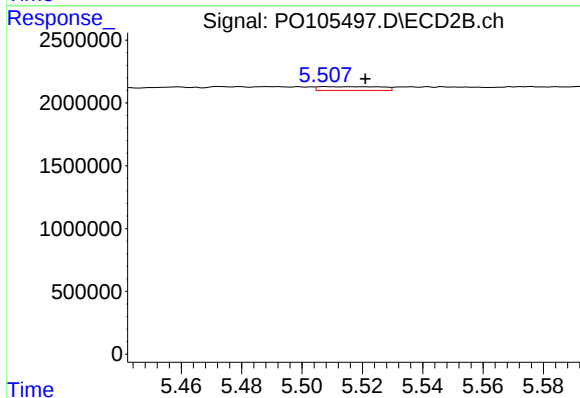


#27 AR-1254-2

R.T.: 5.508 min
Delta R.T.: -0.013 min
Response: 436071
Conc: 2.98 ng/ml

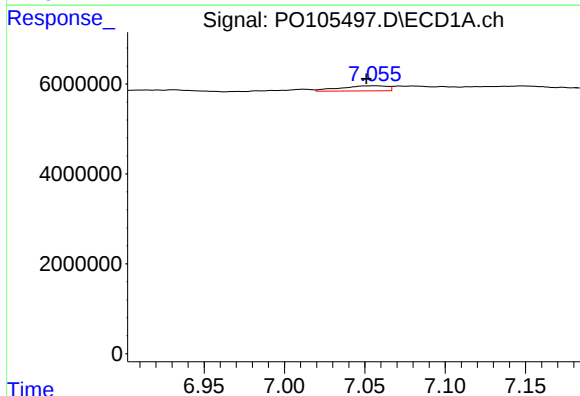


#28 AR-1254-3

R.T.: 7.056 min
Delta R.T.: 0.005 min
Response: 2322671
Conc: 4.90 ng/ml

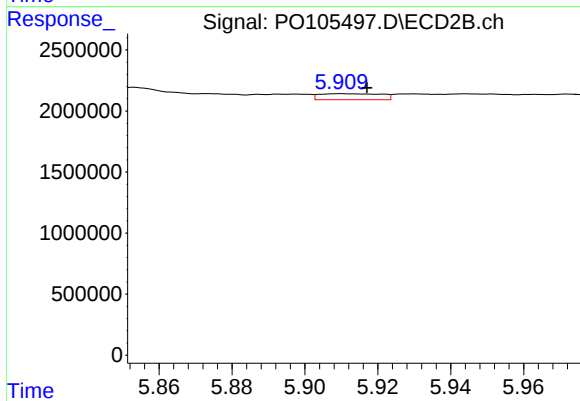

#28 AR-1254-3


R.T.: 5.910 min
Delta R.T.: -0.007 min
Response: 587369
Conc: 2.60 ng/ml

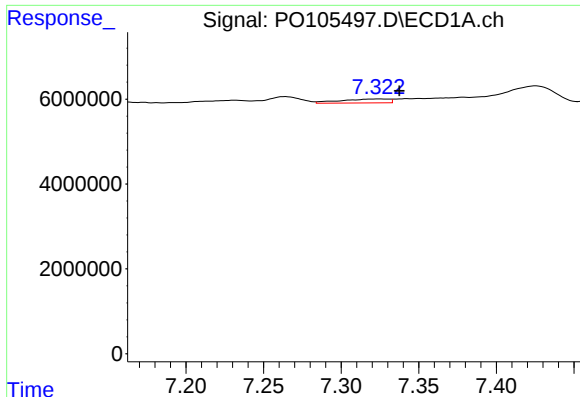

#29 AR-1254-4


R.T.: 7.325 min
Delta R.T.: -0.012 min
Response: 2048506
Conc: 5.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

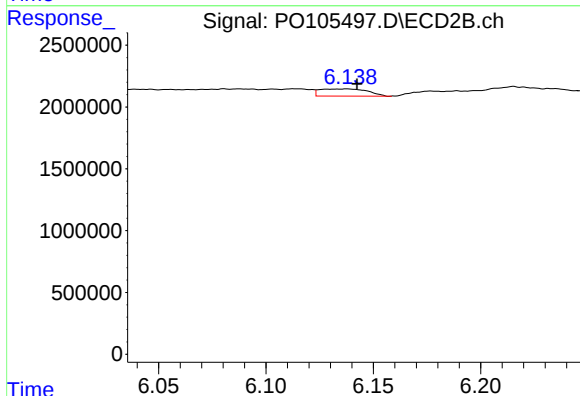


#29 AR-1254-4

R.T.: 6.138 min
Delta R.T.: -0.005 min
Response: 896048
Conc: 6.35 ng/ml

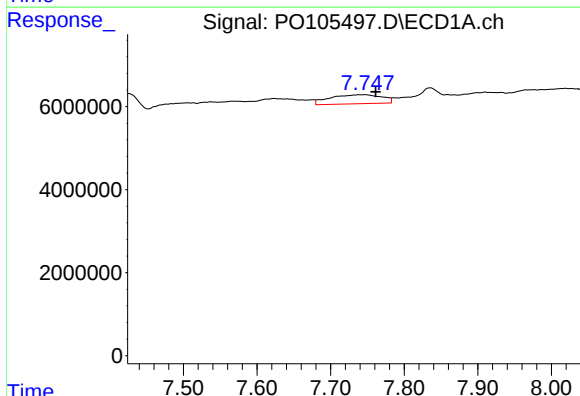


#30 AR-1254-5

R.T.: 7.747 min
Delta R.T.: -0.014 min
Response: 10685135
Conc: 26.92 ng/ml

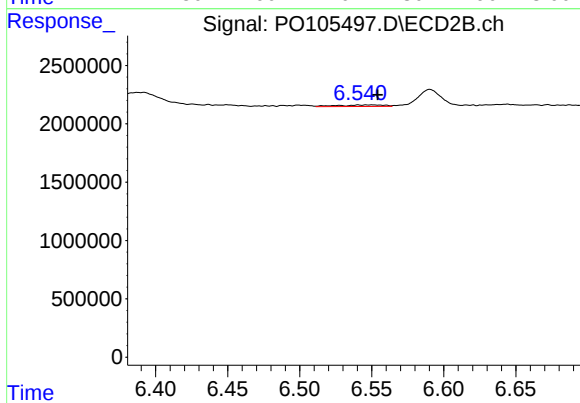

#30 AR-1254-5


R.T.: 6.541 min
Delta R.T.: -0.014 min
Response: 298415
Conc: 1.49 ng/ml

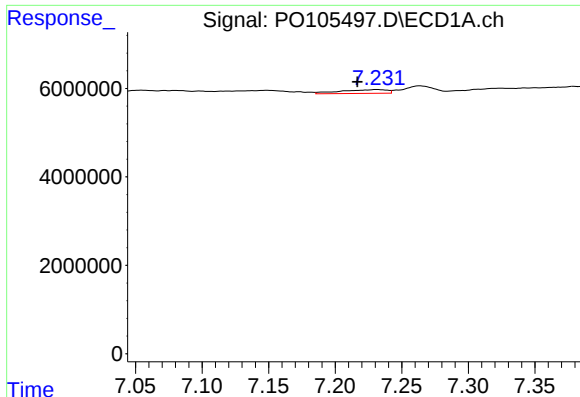

#31 AR-1260-1


R.T.: 7.232 min
Delta R.T.: 0.015 min
Response: 2076904
Conc: 5.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

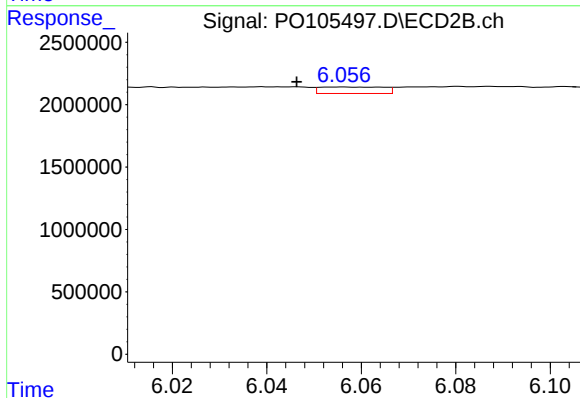


#31 AR-1260-1

R.T.: 6.055 min
Delta R.T.: 0.009 min
Response: 491818
Conc: 3.15 ng/ml

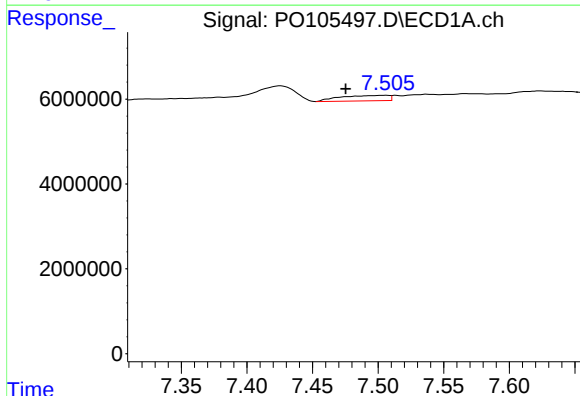


#32 AR-1260-2

R.T.: 7.506 min
Delta R.T.: 0.030 min
Response: 3258356
Conc: 7.83 ng/ml

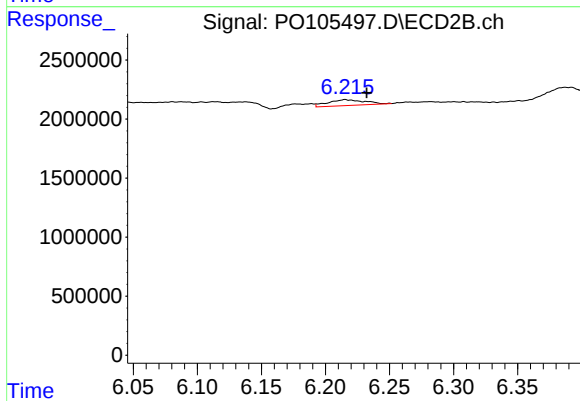

#32 AR-1260-2


R.T.: 6.215 min
Delta R.T.: -0.017 min
Response: 980043
Conc: 5.19 ng/ml

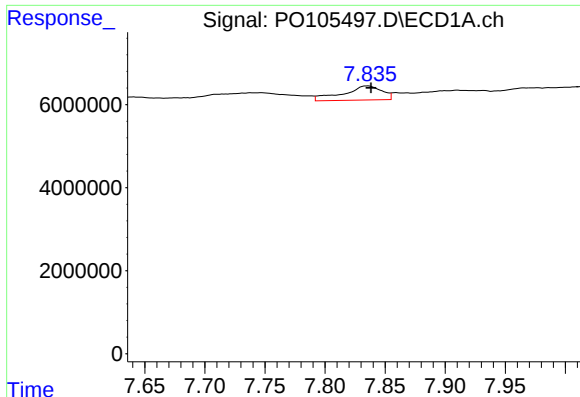

#33 AR-1260-3


R.T.: 7.835 min
Delta R.T.: -0.003 min
Response: 7663521
Conc: 29.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

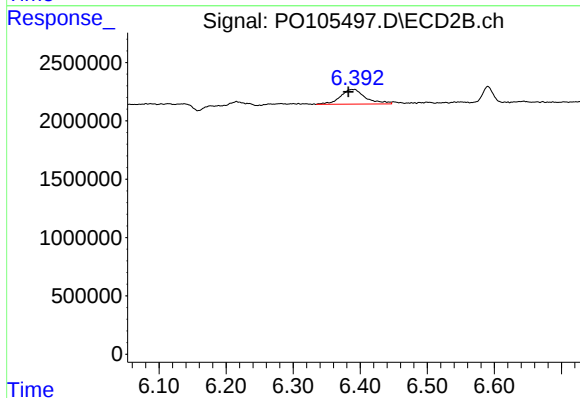


#33 AR-1260-3

R.T.: 6.391 min
Delta R.T.: 0.009 min
Response: 3298248
Conc: 17.85 ng/ml

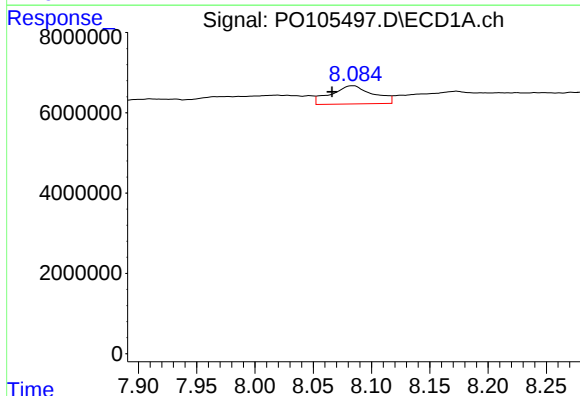


#34 AR-1260-4

R.T.: 8.084 min
Delta R.T.: 0.018 min
Response: 11412390
Conc: 34.59 ng/ml

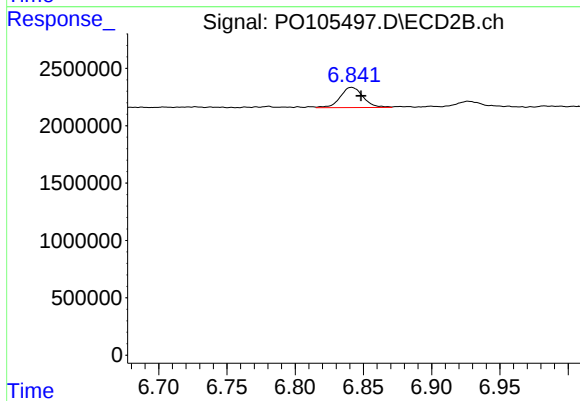

#34 AR-1260-4


R.T.: 6.841 min
Delta R.T.: -0.007 min
Response: 2051554
Conc: 16.78 ng/ml

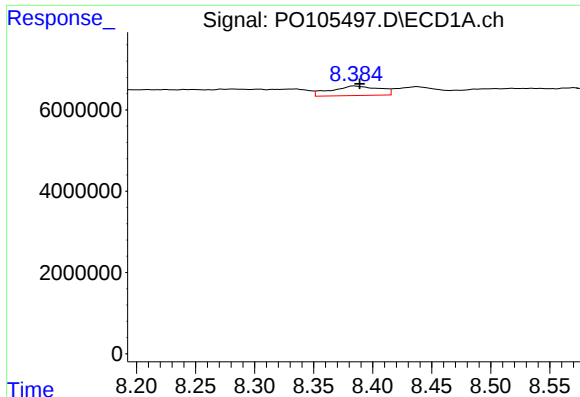

#35 AR-1260-5


R.T.: 8.384 min
Delta R.T.: -0.005 min
Response: 6677867
Conc: 11.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

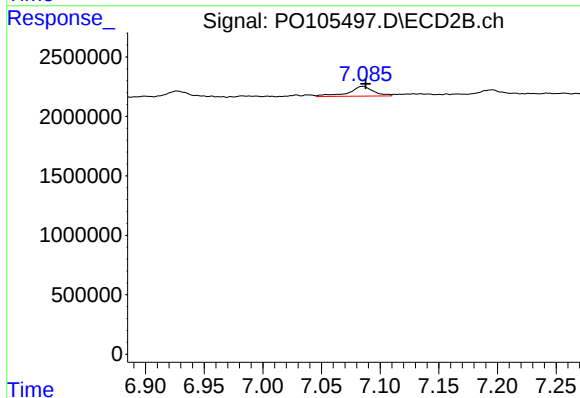


#35 AR-1260-5

R.T.: 7.085 min
Delta R.T.: -0.003 min
Response: 1218995
Conc: 4.38 ng/ml

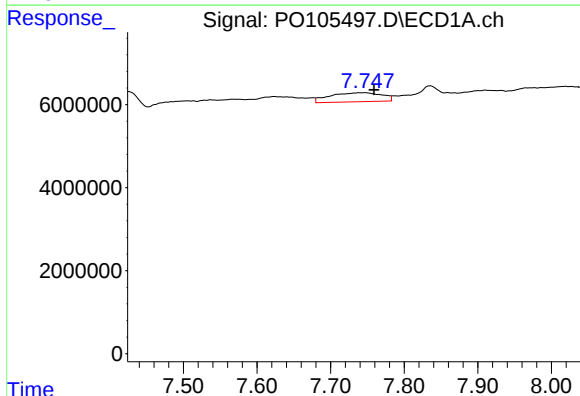


#36 AR-1262-1

R.T.: 7.747 min
Delta R.T.: -0.012 min
Response: 10685135
Conc: 33.64 ng/ml

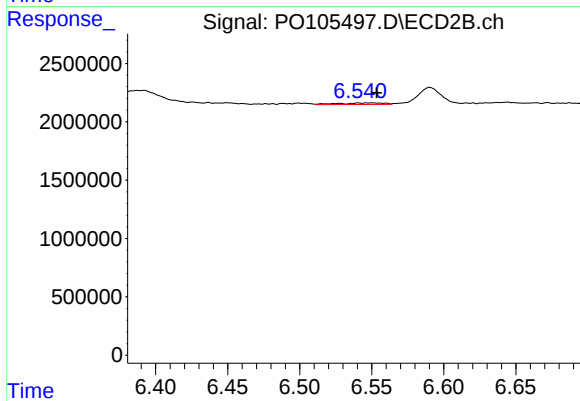

#36 AR-1262-1


R.T.: 6.541 min
Delta R.T.: -0.013 min
Response: 298415
Conc: 2.80 ng/ml

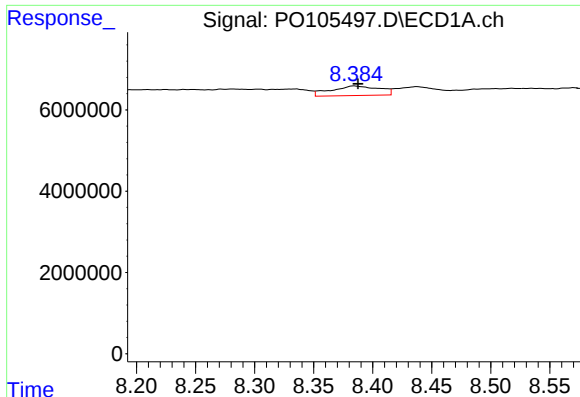

#37 AR-1262-2


R.T.: 8.384 min
Delta R.T.: -0.003 min
Response: 6677867
Conc: 8.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

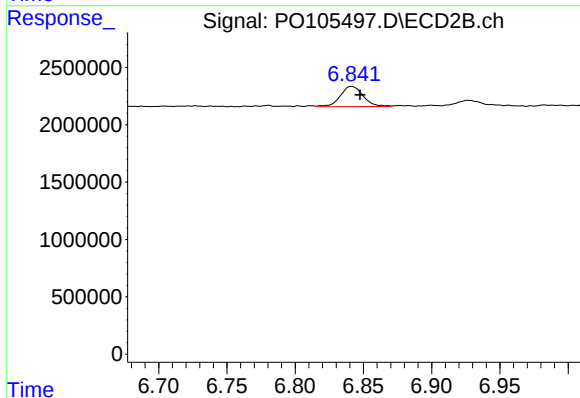


#37 AR-1262-2

R.T.: 6.841 min
Delta R.T.: -0.006 min
Response: 2051554
Conc: 12.07 ng/ml

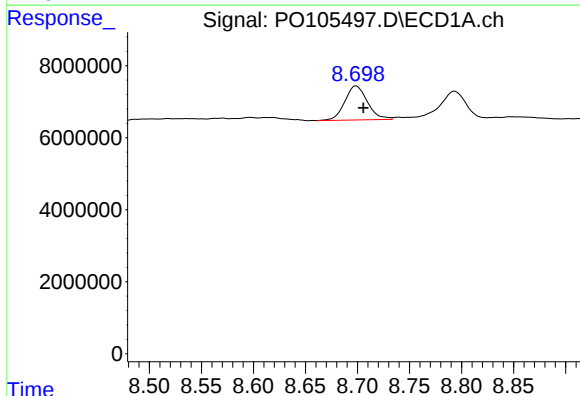


#38 AR-1262-3

R.T.: 8.699 min
Delta R.T.: -0.007 min
Response: 14324944
Conc: 29.11 ng/ml

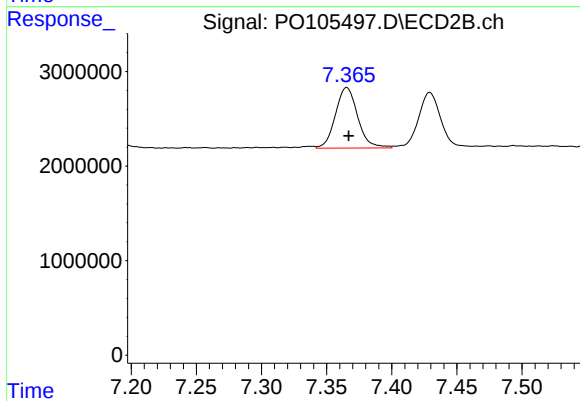

#38 AR-1262-3


R.T.: 7.365 min
Delta R.T.: -0.001 min
Response: 7637160
Conc: 60.49 ng/ml

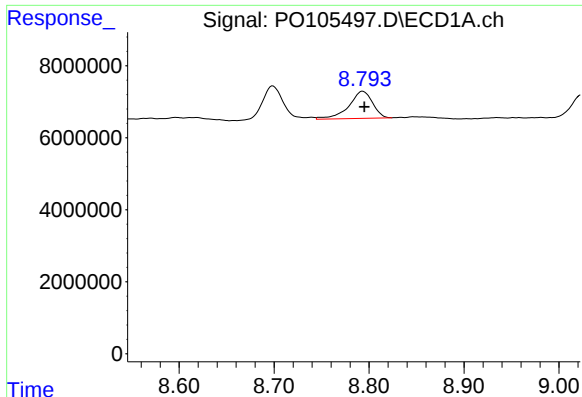

#39 AR-1262-4


R.T.: 8.793 min
Delta R.T.: -0.002 min
Response: 13052503
Conc: 35.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

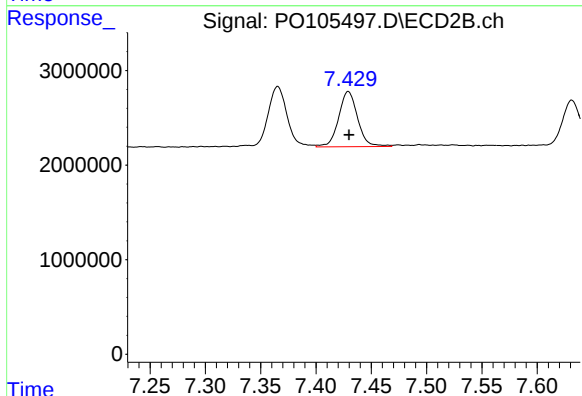


#39 AR-1262-4

R.T.: 7.429 min
Delta R.T.: 0.000 min
Response: 6973420
Conc: 30.12 ng/ml

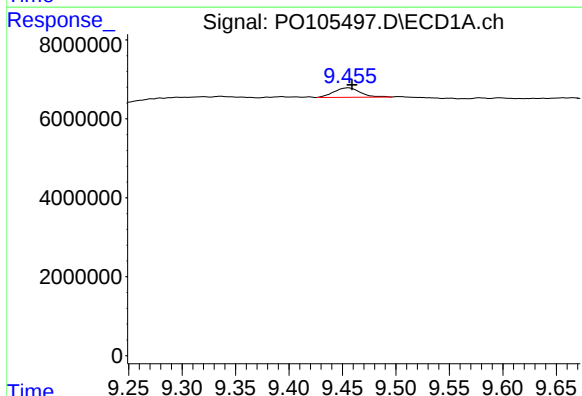


#40 AR-1262-5

R.T.: 9.455 min
Delta R.T.: -0.004 min
Response: 4105264
Conc: 15.33 ng/ml

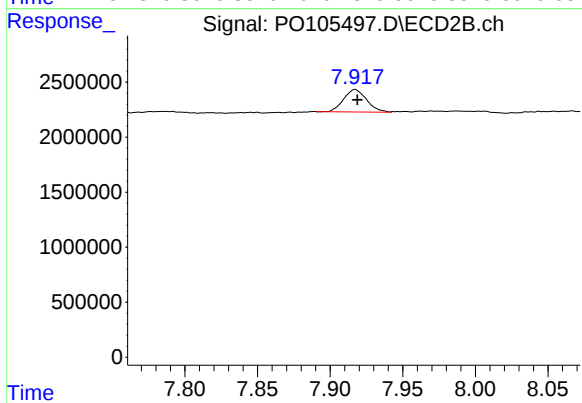

#40 AR-1262-5


R.T.: 7.917 min
Delta R.T.: -0.002 min
Response: 2234737
Conc: 22.24 ng/ml

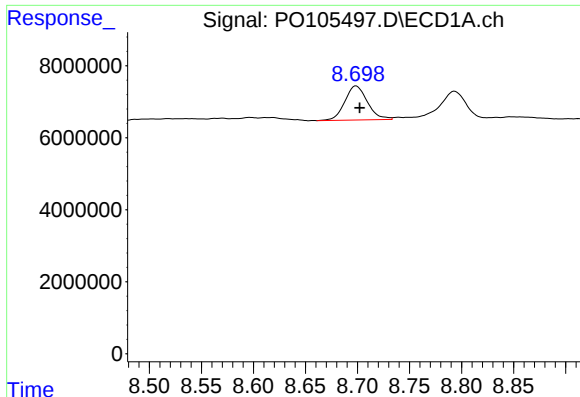

#41 AR-1268-1


R.T.: 8.699 min
Delta R.T.: -0.004 min
Response: 14324944
Conc: 17.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

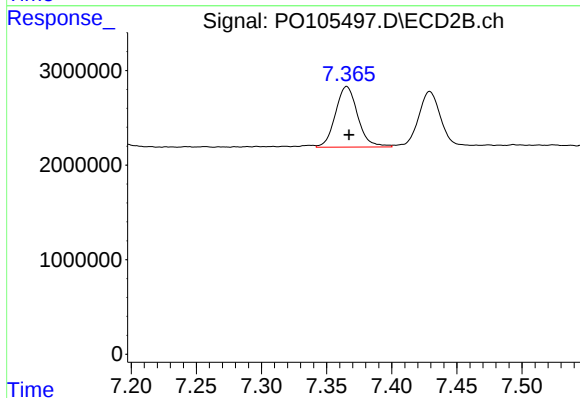


#41 AR-1268-1

R.T.: 7.365 min
Delta R.T.: -0.002 min
Response: 7637160
Conc: 21.88 ng/ml

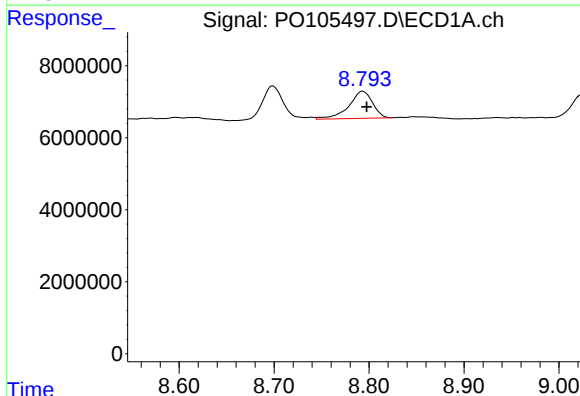


#42 AR-1268-2

R.T.: 8.793 min
Delta R.T.: -0.004 min
Response: 13052503
Conc: 17.96 ng/ml

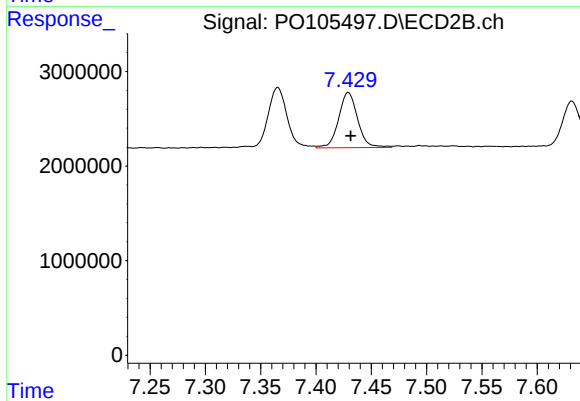

#42 AR-1268-2


R.T.: 7.429 min
Delta R.T.: -0.002 min
Response: 6973420
Conc: 22.35 ng/ml

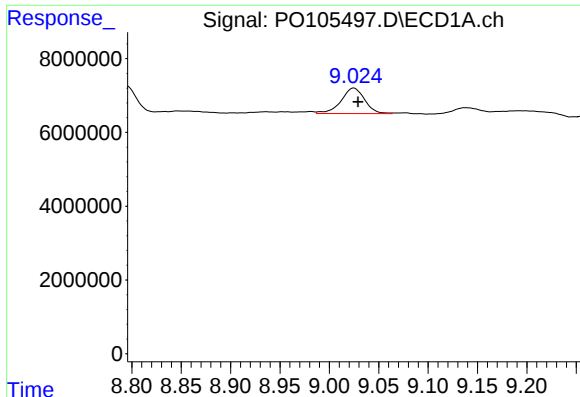

#43 AR-1268-3


R.T.: 9.025 min
Delta R.T.: -0.004 min
Response: 11454747
Conc: 17.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

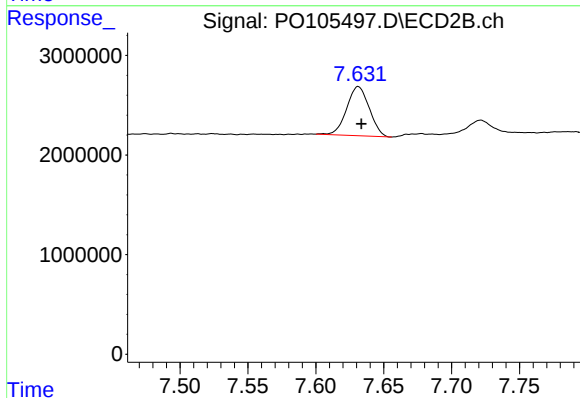


#43 AR-1268-3

R.T.: 7.631 min
Delta R.T.: -0.002 min
Response: 5715396
Conc: 22.61 ng/ml

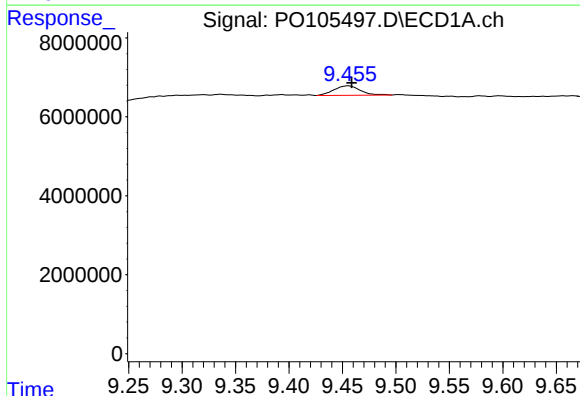


#44 AR-1268-4

R.T.: 9.455 min
Delta R.T.: -0.003 min
Response: 4105264
Conc: 14.74 ng/ml

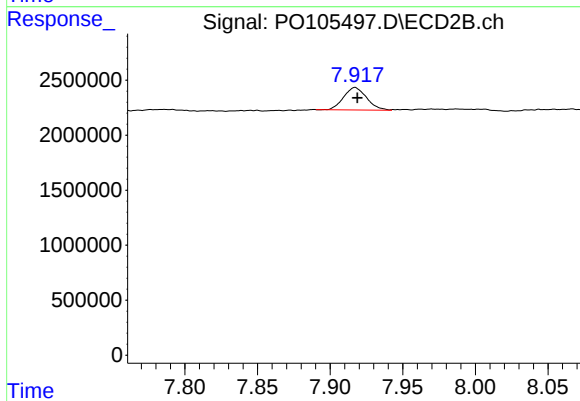

#44 AR-1268-4


R.T.: 7.917 min
Delta R.T.: -0.001 min
Response: 2234737
Conc: 20.78 ng/ml

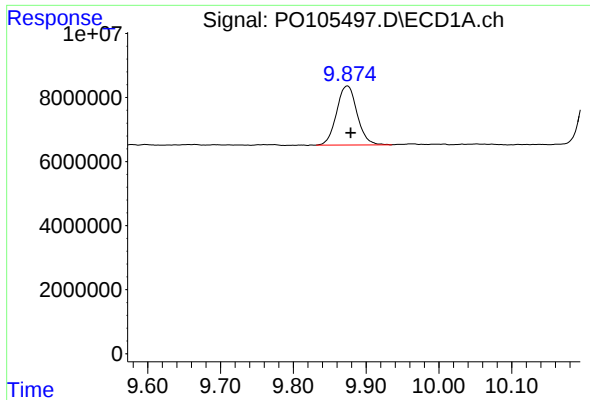

#45 AR-1268-5

R.T.: 9.874 min
Delta R.T.: -0.005 min
Response: 36124569
Conc: 17.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

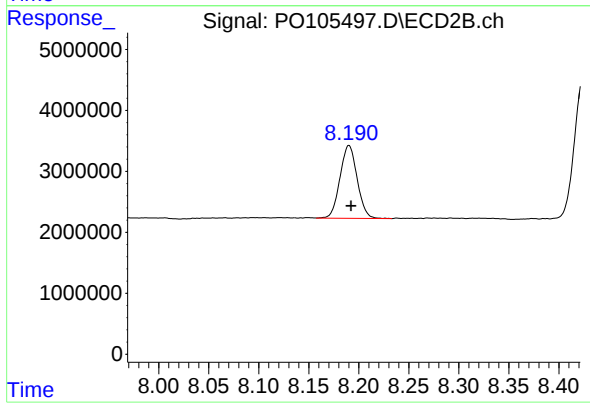

#45 AR-1268-5

R.T.: 8.190 min
Delta R.T.: -0.002 min
Response: 14300611
Conc: 21.38 ng/ml