

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081324\
 Data File : P0105494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 13:07
 Operator : YP/AJ
 Sample : P3390-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:07:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 04:08:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.426	3.535	111.8E6	50985712	12.802	16.233 #
2) SA Decachlor...	10.215	8.425	86724674	31637047	15.076	17.870
Target Compounds						
21) L5 AR-1248-1	5.596	4.589	3458977	1683141	18.943	24.099 #
22) L5 AR-1248-2	5.872	4.821	4913056	2354194	19.506	24.808 #
23) L5 AR-1248-3	6.077	4.861	5838599	2492040	20.655	24.964
24) L5 AR-1248-4	6.484	5.029	7572932	2841595	23.684	25.176
25) L5 AR-1248-5	6.524	5.413	7752159	3045333	25.062	27.045



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081324\
Data File : PO105494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 13:07
Operator : YP/AJ
Sample : P3390-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:07:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081024.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 04:08:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

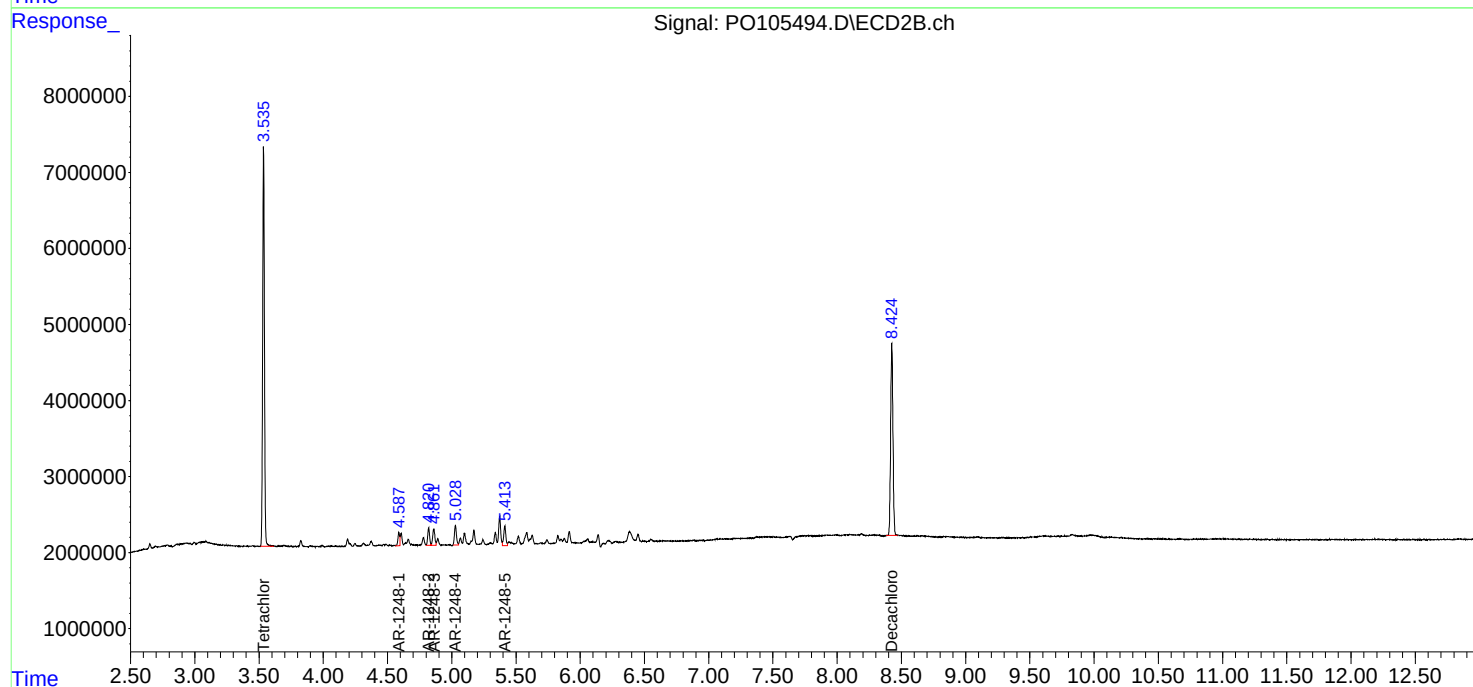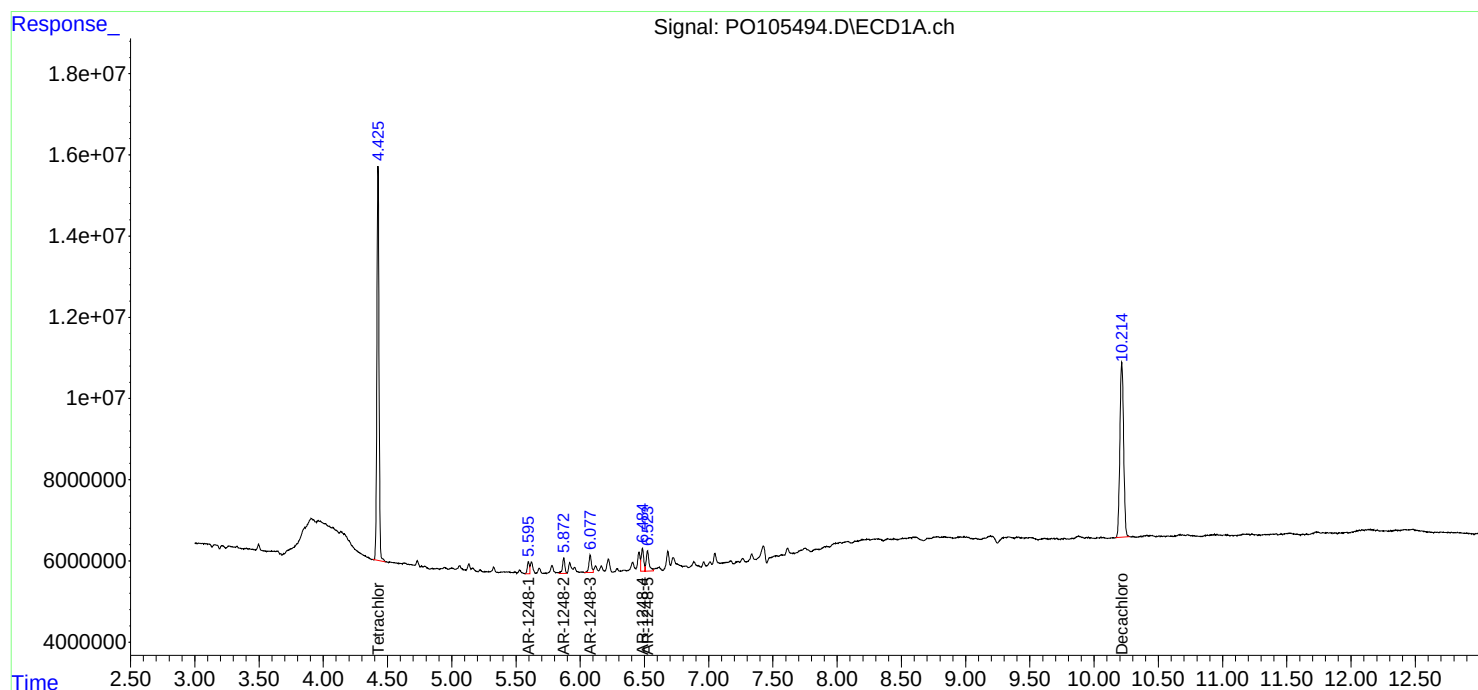


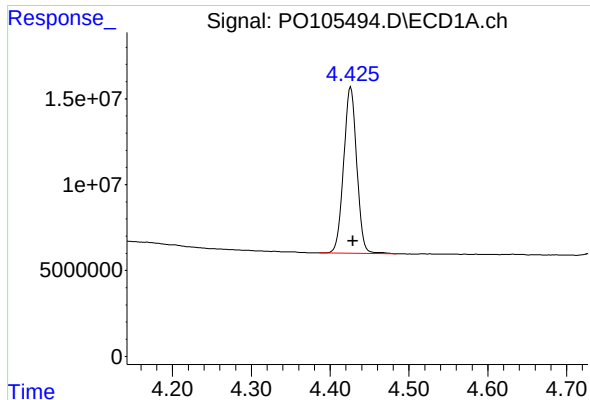

#1 Tetrachloro-m-xylene


R.T.: 4.426 min
Delta R.T.: -0.003 min
Response: 111813371
Conc: 12.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

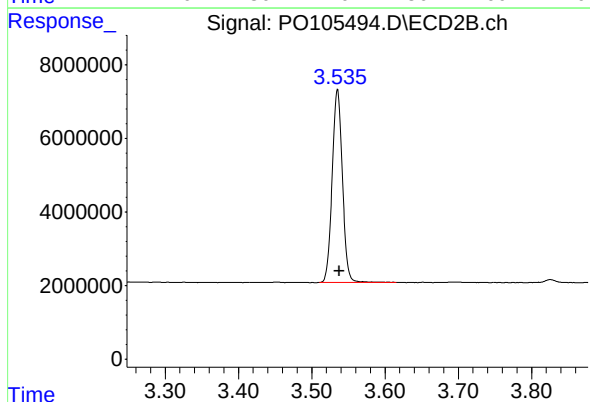


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.002 min
Response: 50985712
Conc: 16.23 ng/ml

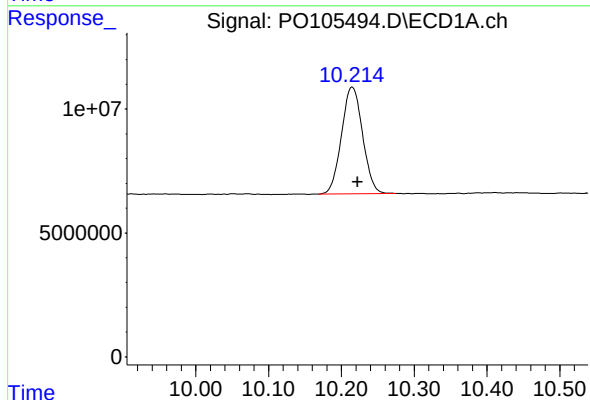


#2 Decachlorobiphenyl

R.T.: 10.215 min
Delta R.T.: -0.008 min
Response: 86724674
Conc: 15.08 ng/ml

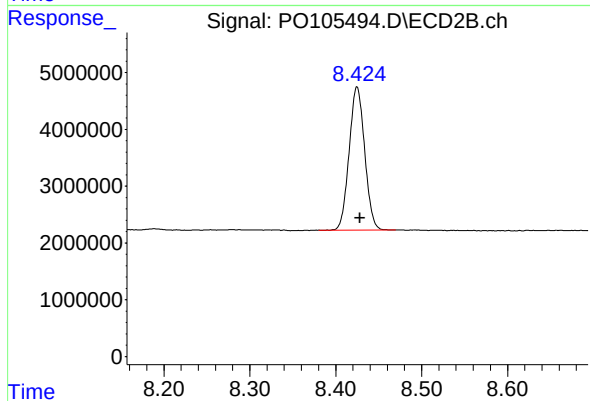

#2 Decachlorobiphenyl


R.T.: 8.425 min
Delta R.T.: -0.004 min
Response: 31637047
Conc: 17.87 ng/ml

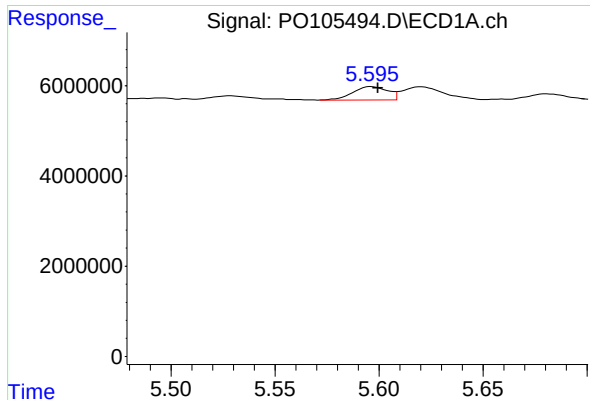

#21 AR-1248-1


R.T.: 5.596 min
Delta R.T.: -0.003 min
Response: 3458977
Conc: 18.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

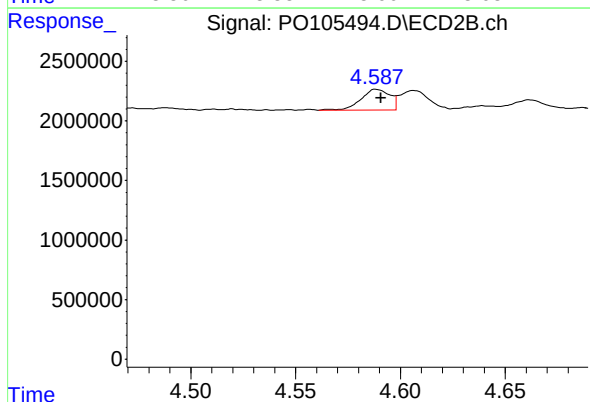


#21 AR-1248-1

R.T.: 4.589 min
Delta R.T.: -0.002 min
Response: 1683141
Conc: 24.10 ng/ml

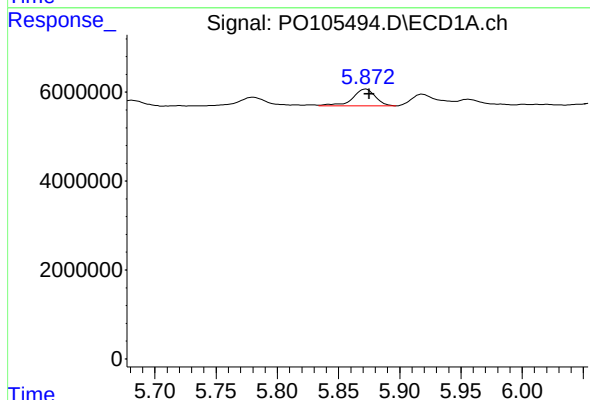


#22 AR-1248-2

R.T.: 5.872 min
Delta R.T.: -0.003 min
Response: 4913056
Conc: 19.51 ng/ml

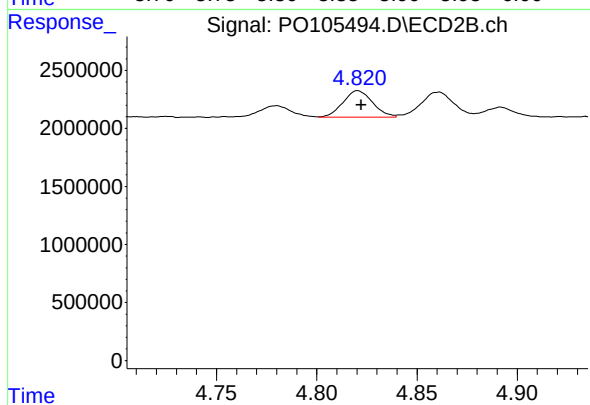

#22 AR-1248-2


R.T.: 4.821 min
Delta R.T.: -0.002 min
Response: 2354194
Conc: 24.81 ng/ml

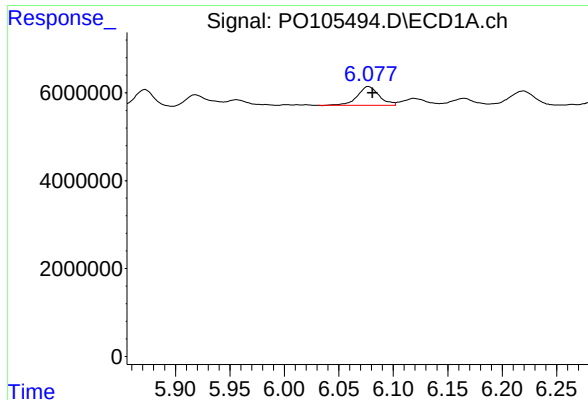

#23 AR-1248-3


R.T.: 6.077 min
Delta R.T.: -0.004 min
Response: 5838599
Conc: 20.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

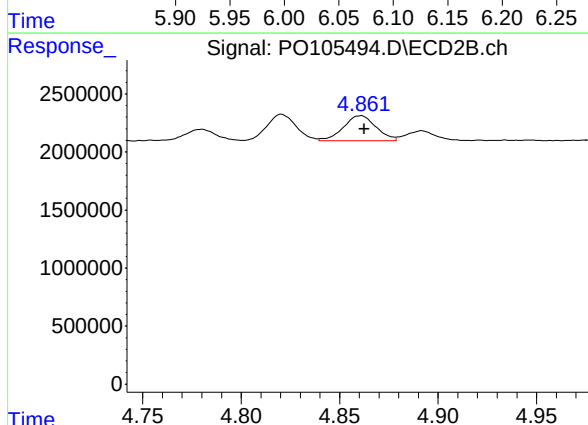


#23 AR-1248-3

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 2492040
Conc: 24.96 ng/ml

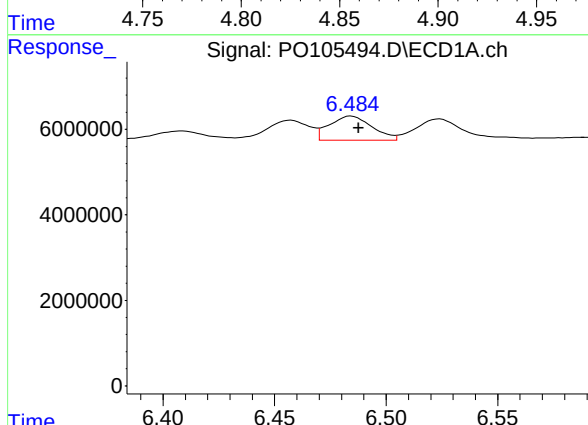


#24 AR-1248-4

R.T.: 6.484 min
Delta R.T.: -0.003 min
Response: 7572932
Conc: 23.68 ng/ml

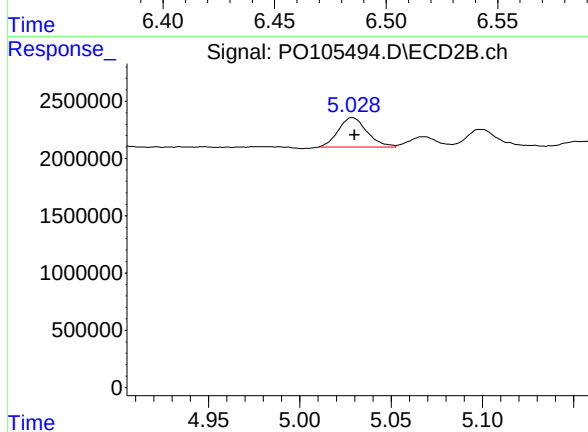

#24 AR-1248-4


R.T.: 5.029 min
Delta R.T.: -0.001 min
Response: 2841595
Conc: 25.18 ng/ml

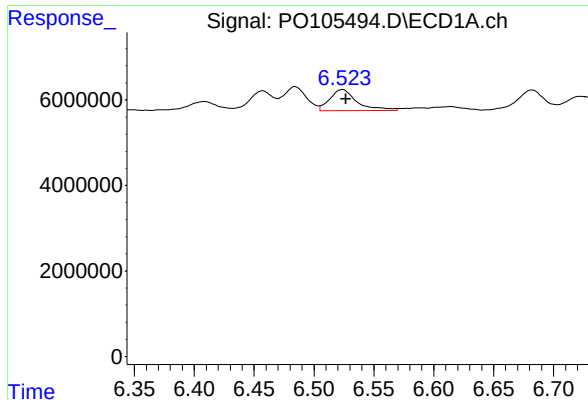

#25 AR-1248-5

R.T.: 6.524 min
Delta R.T.: -0.003 min
Response: 7752159
Conc: 25.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2024

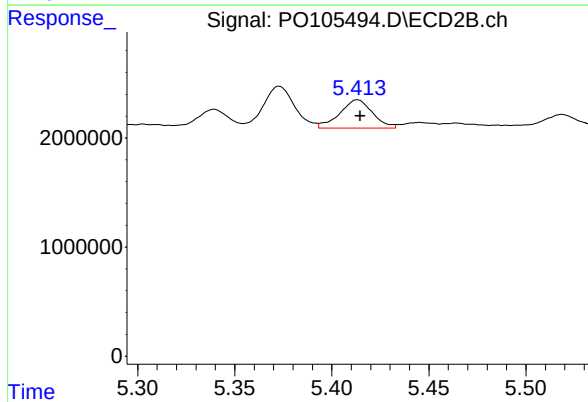

#25 AR-1248-5

R.T.: 5.413 min
Delta R.T.: -0.001 min
Response: 3045333
Conc: 27.04 ng/ml