

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081325\
 Data File : P0112901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2025 10:29
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 11:12:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.661	3.658	81345	40853	0.010	0.008
2)	SA Decachlor...	8.701	8.633	376638	173508	0.052	0.098 #
Target Compounds							
3)	L1 AR-1016-1	4.769	4.742	834040	274291	3.108	1.567 #
4)	L1 AR-1016-2	4.769	4.759	834040	63290	2.054	0.243 #
5)	L1 AR-1016-3	4.794f	4.929	864632	1700006	3.304	12.503 #
6)	L1 AR-1016-4	4.953	4.975	8271840	4505891	39.047	40.563
7)	L1 AR-1016-5	5.206	5.183	17884748	2089493	81.490	14.581 #
8)	L2 AR-1221-1	3.890	3.873	132727	166910	1.373	2.481 #
9)	L2 AR-1221-2	3.957	3.953	143579	92502	1.998	1.823
12)	L3 AR-1232-2	4.501	4.759	864766	63290	8.035	0.483 #
13)	L3 AR-1232-3	4.769	4.929	834040	1700006	4.033	25.299 #
14)	L3 AR-1232-4	4.953	5.016	8271840	554968	78.975	9.276 #
15)	L3 AR-1232-5	4.953f	5.188	8271840	520233	121.858	7.979 #
16)	L4 AR-1242-1	4.769	4.742	834040	274291	3.369	1.732 #
17)	L4 AR-1242-2	4.769	4.759	834040	63290	2.255	0.271 #
18)	L4 AR-1242-3	4.794f	4.929	864632	1700006	3.654	14.028 #
19)	L4 AR-1242-4	4.953	5.016	8271840	554968	42.577	4.522 #
20)	L4 AR-1242-5	5.577	5.520	24804141	3518217	115.953	21.856 #
21)	L5 AR-1248-1	4.769	4.742	834040	274291	4.455	2.257 #
22)	L5 AR-1248-2	4.953f	4.975	8271840	4505891	32.424	26.618
23)	L5 AR-1248-3	5.206	5.016	17884748	554968	52.036	3.124 #
24)	L5 AR-1248-4	5.577	5.188	24804141	520233	48.820	2.497 #
25)	L5 AR-1248-5	5.577	5.580	24804141	1471701	70.952	6.853 #
26)	L6 AR-1254-1	5.577	5.520	24804141	3518217	45.184	10.706 #
27)	L6 AR-1254-2	5.728	5.668	59376892	1620945	122.195	5.599 #
28)	L6 AR-1254-3	6.128	6.095	14256971	23089685	19.155	54.016 #
29)	L6 AR-1254-4	6.359	6.323	520283	1603536	0.946	5.875 #
30)	L6 AR-1254-5	6.756	6.720	3534.5E6	1670.8E6	4993.431	5002.150
31)	L7 AR-1260-1	6.246	6.217	674383	2840274	1.535	11.429 #
32)	L7 AR-1260-2	6.434	6.398	17030012	9665275	24.757	29.334
33)	L7 AR-1260-3	6.756f	6.595f	3534.5E6	197466	6010.806	0.769 #
34)	L7 AR-1260-4	7.059	7.015	2847857	243742	6.314	1.274 #
35)	L7 AR-1260-5	7.300	7.245	3124510	1862098	2.522	4.518 #
36)	L8 AR-1262-1	6.756f	6.720f	3534.5E6	1670.8E6	3803.747	4027.734
37)	L8 AR-1262-2	7.300	7.245	3124510	1862098	2.101	3.612 #
38)	L8 AR-1262-3	7.586	7.545	6888208	1961177	11.670	10.514
39)	L8 AR-1262-4	7.651	7.556f	2049574	6061894	2.062	21.041 #
40)	L8 AR-1262-5	8.156	0.000	872067	0	2.009	N.D. #
41)	L9 AR-1268-1	7.586	7.545	6888208	1961177	3.934	3.787
42)	L9 AR-1268-2	7.651	7.556f	2049574	6061894	1.391	14.261 #
43)	L9 AR-1268-3	7.834	7.830	1627087	784393	1.299	2.442 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081325\
Data File : P0112901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2025 10:29
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 11:12:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44)	L9 AR-1268-4	8.156	0.000	872067	0	1.810	N.D. #
45)	L9 AR-1268-5	8.446	8.409	291142	51358	0.087	0.070



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081325\
Data File : PO112901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2025 10:29
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 11:12:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

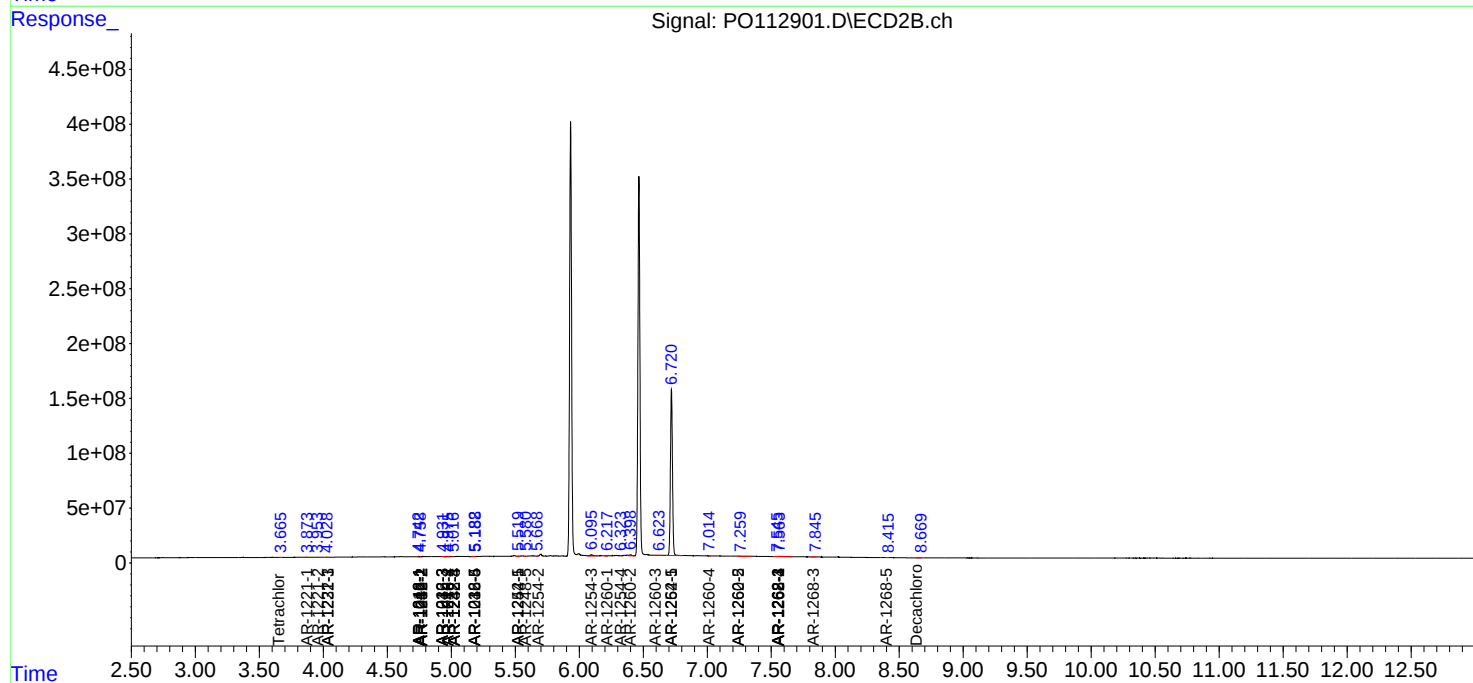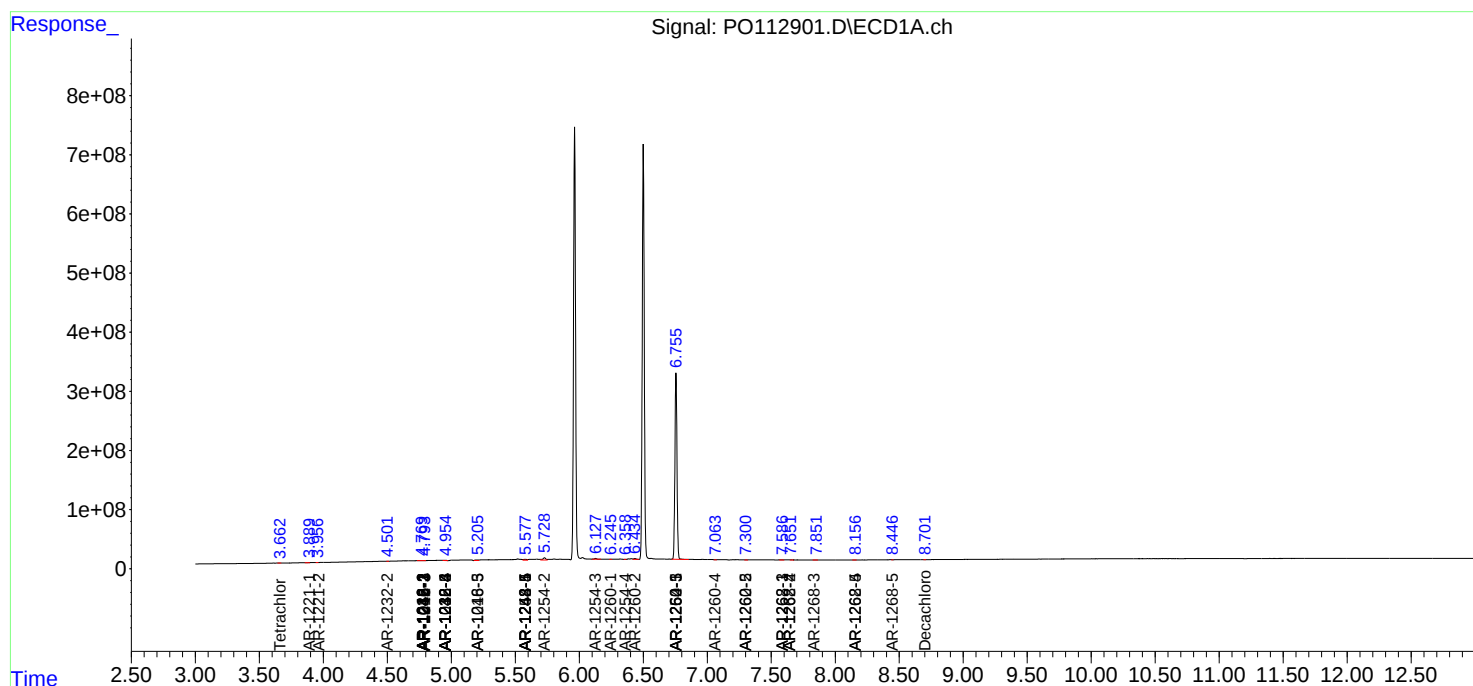


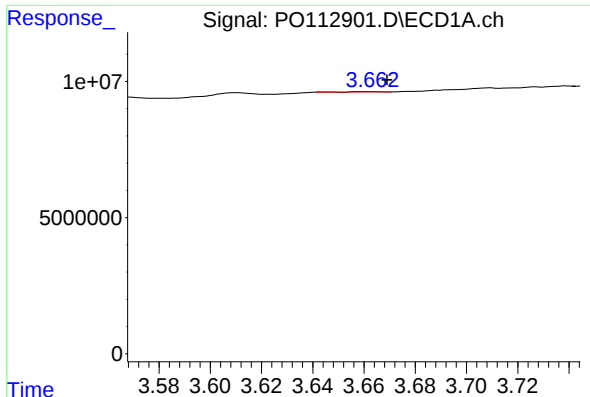

#1 Tetrachloro-m-xylene


R.T.: 3.661 min
Delta R.T.: -0.008 min
Response: 81345
Conc: 0.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

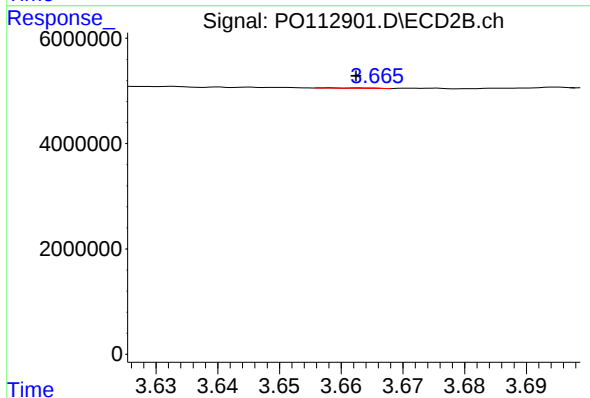


#1 Tetrachloro-m-xylene

R.T.: 3.658 min
Delta R.T.: -0.004 min
Response: 40853
Conc: 0.01 ng/ml

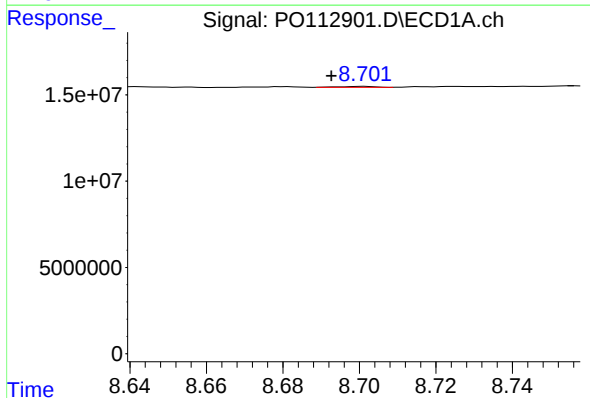


#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: 0.009 min
Response: 376638
Conc: 0.05 ng/ml

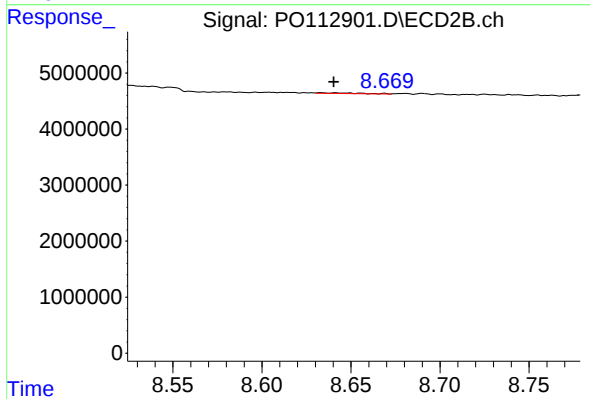

#2 Decachlorobiphenyl


R.T.: 8.633 min
Delta R.T.: -0.008 min
Response: 173508
Conc: 0.10 ng/ml

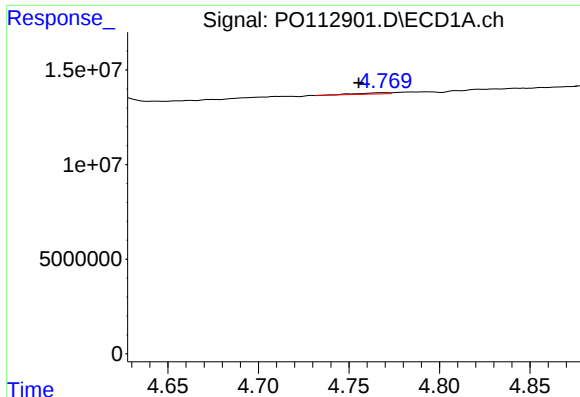

#3 AR-1016-1


R.T.: 4.769 min
Delta R.T.: 0.014 min
Response: 834040
Conc: 3.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

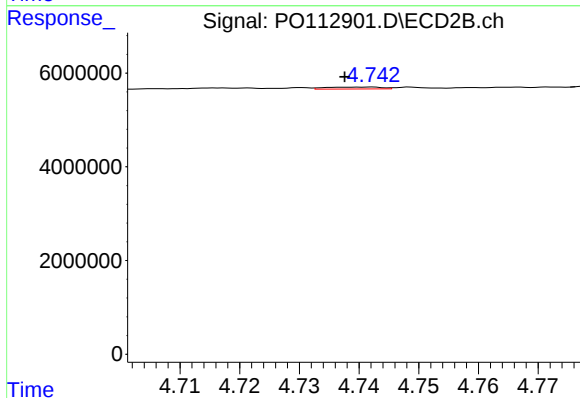


#3 AR-1016-1

R.T.: 4.742 min
Delta R.T.: 0.004 min
Response: 274291
Conc: 1.57 ng/ml

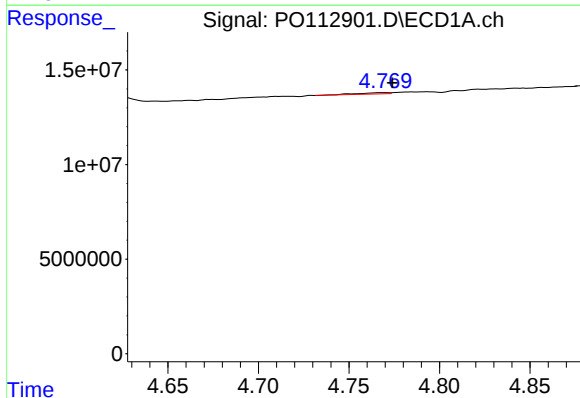


#4 AR-1016-2

R.T.: 4.769 min
Delta R.T.: -0.005 min
Response: 834040
Conc: 2.05 ng/ml

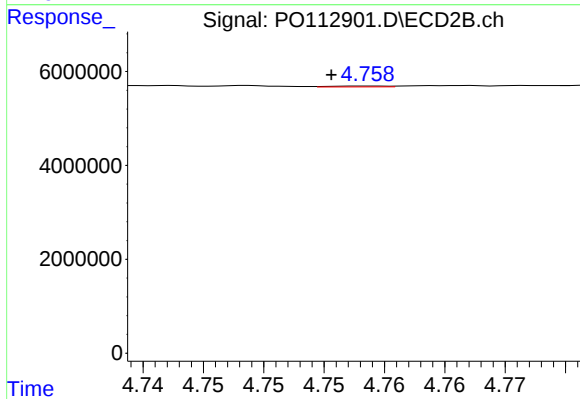

#4 AR-1016-2


R.T.: 4.759 min
Delta R.T.: 0.003 min
Response: 63290
Conc: 0.24 ng/ml

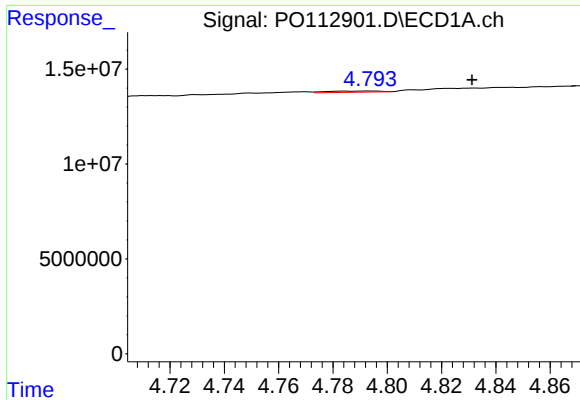

#5 AR-1016-3


R.T.: 4.794 min
Delta R.T.: -0.038 min
Response: 864632
Conc: 3.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

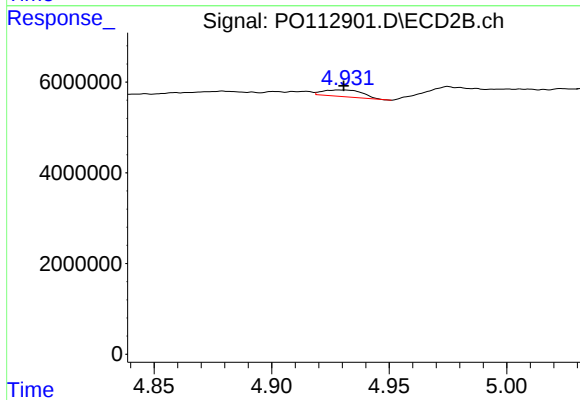


#5 AR-1016-3

R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 1700006
Conc: 12.50 ng/ml

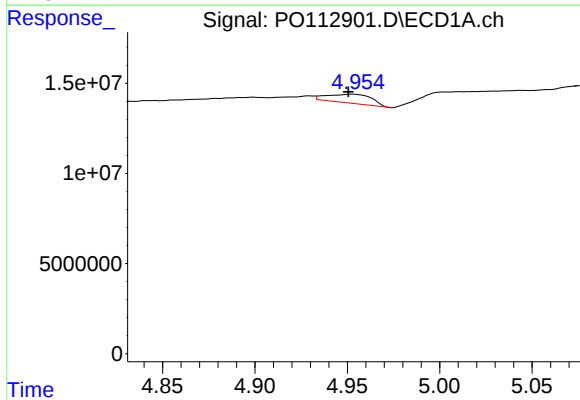


#6 AR-1016-4

R.T.: 4.953 min
Delta R.T.: 0.002 min
Response: 8271840
Conc: 39.05 ng/ml

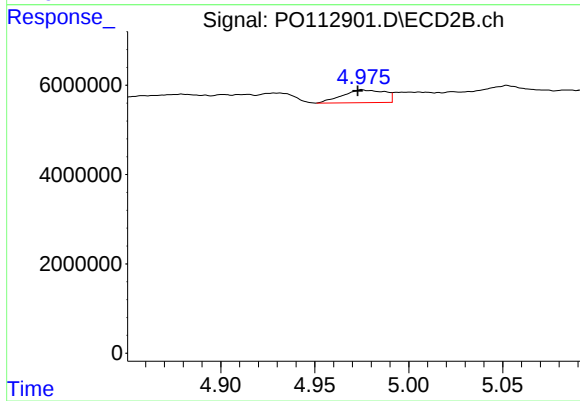

#6 AR-1016-4


R.T.: 4.975 min
Delta R.T.: 0.002 min
Response: 4505891
Conc: 40.56 ng/ml

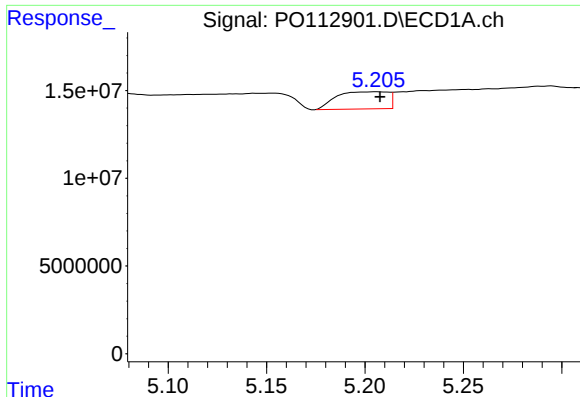

#7 AR-1016-5


R.T.: 5.206 min
Delta R.T.: -0.002 min
Response: 17884748
Conc: 81.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

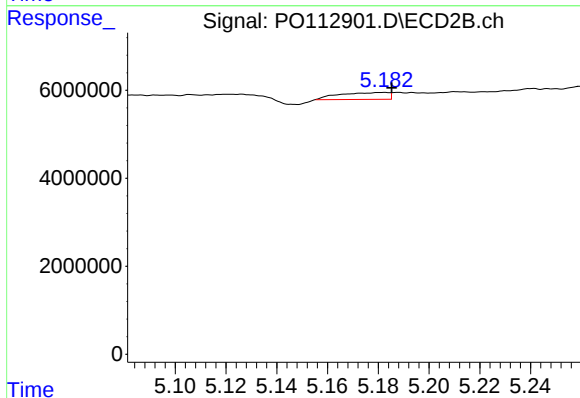


#7 AR-1016-5

R.T.: 5.183 min
Delta R.T.: -0.003 min
Response: 2089493
Conc: 14.58 ng/ml

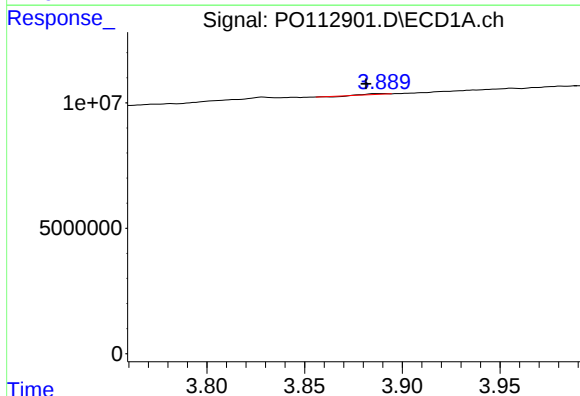


#8 AR-1221-1

R.T.: 3.890 min
Delta R.T.: 0.008 min
Response: 132727
Conc: 1.37 ng/ml

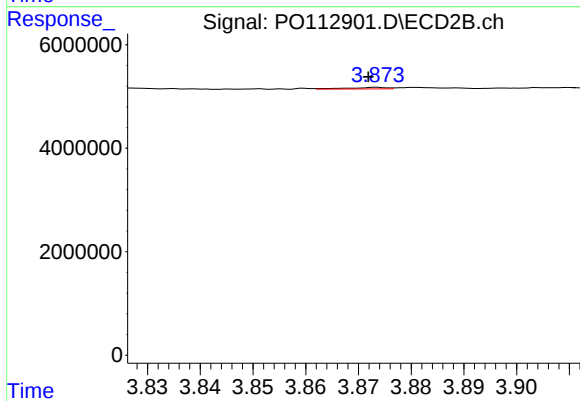

#8 AR-1221-1


R.T.: 3.873 min
Delta R.T.: 0.002 min
Response: 166910
Conc: 2.48 ng/ml

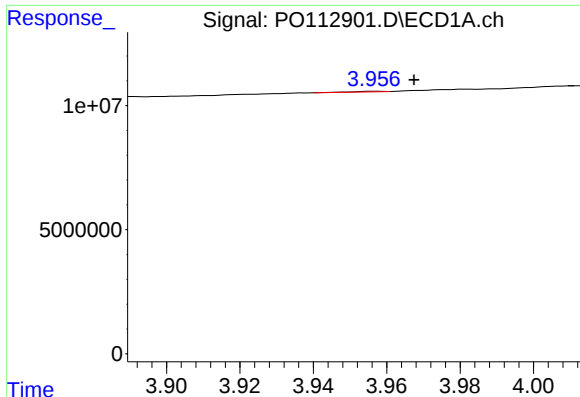

#9 AR-1221-2


R.T.: 3.957 min
Delta R.T.: -0.011 min
Response: 143579
Conc: 2.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

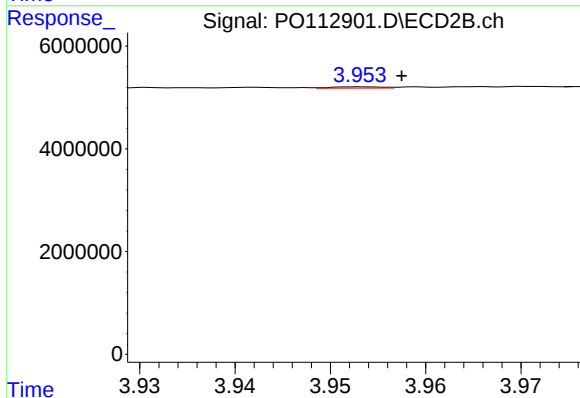


#9 AR-1221-2

R.T.: 3.953 min
Delta R.T.: -0.004 min
Response: 92502
Conc: 1.82 ng/ml

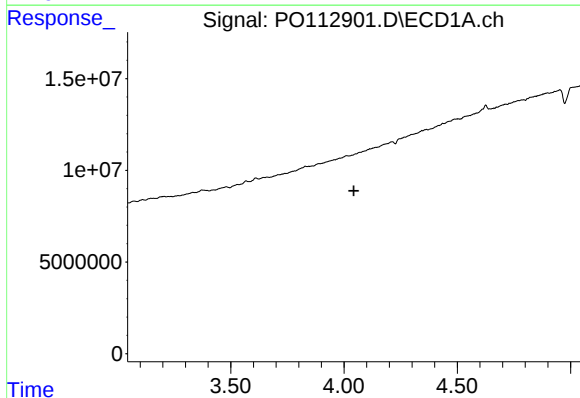


#10 AR-1221-3

R.T.: 4.070 min
Delta R.T.: 0.027 min
Response: -931639
Conc: N.D.

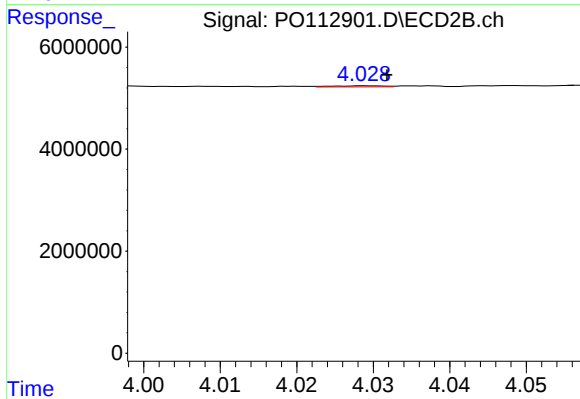

#10 AR-1221-3


R.T.: 4.029 min
Delta R.T.: -0.003 min
Response: 101783
Conc: 0.64 ng/ml

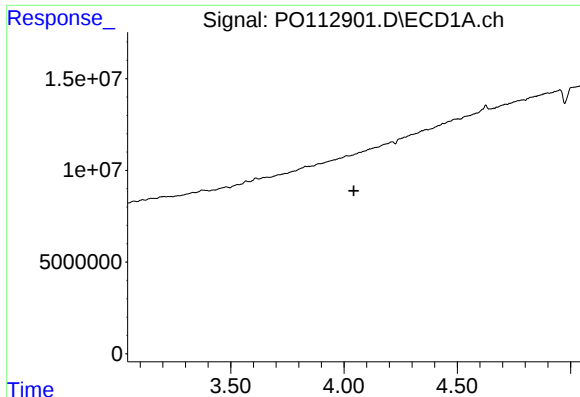

#11 AR-1232-1


R.T.: 4.070 min
Delta R.T.: 0.027 min
Response: -931639
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

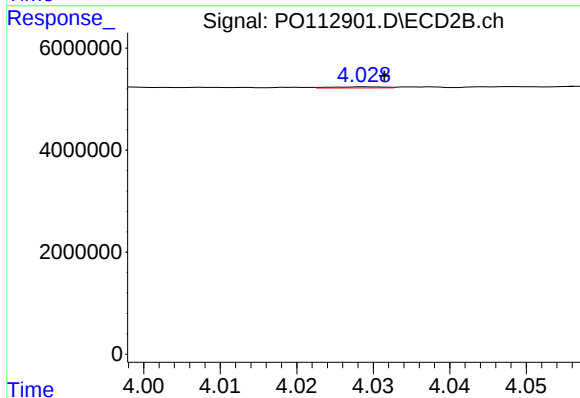


#11 AR-1232-1

R.T.: 4.029 min
Delta R.T.: -0.002 min
Response: 101783
Conc: 0.80 ng/ml

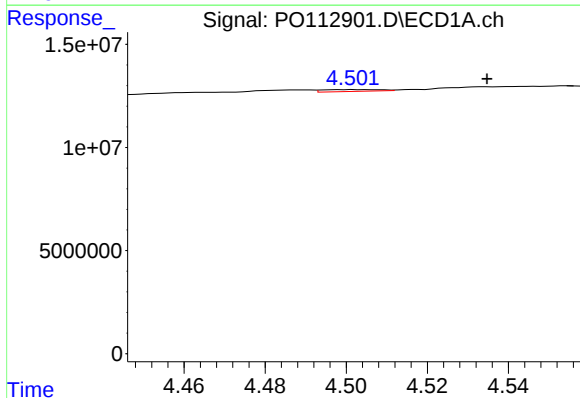


#12 AR-1232-2

R.T.: 4.501 min
Delta R.T.: -0.033 min
Response: 864766
Conc: 8.04 ng/ml

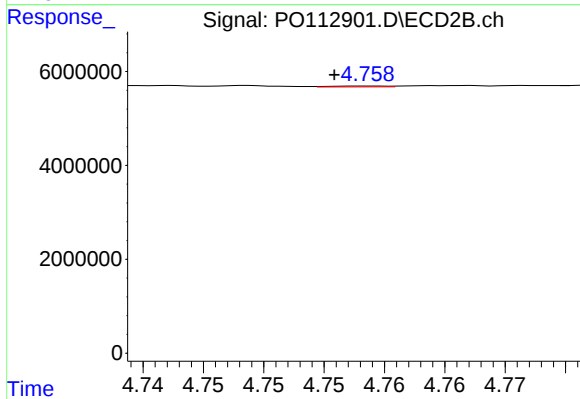

#12 AR-1232-2


R.T.: 4.759 min
Delta R.T.: 0.003 min
Response: 63290
Conc: 0.48 ng/ml

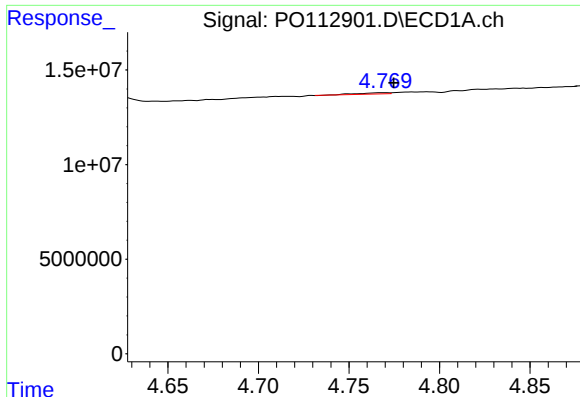

#13 AR-1232-3


R.T.: 4.769 min
Delta R.T.: -0.006 min
Response: 834040
Conc: 4.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

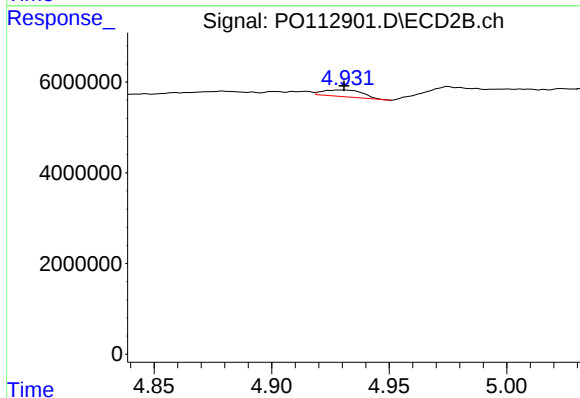


#13 AR-1232-3

R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 1700006
Conc: 25.30 ng/ml

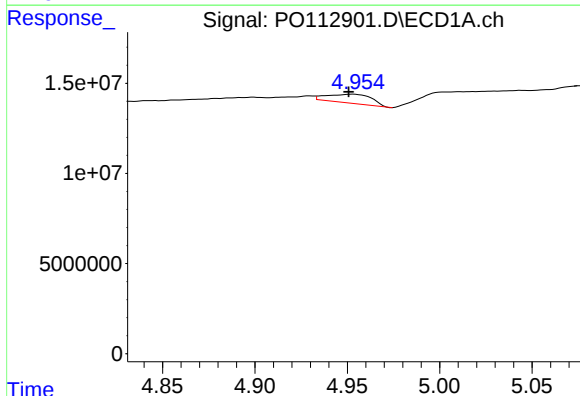


#14 AR-1232-4

R.T.: 4.953 min
Delta R.T.: 0.002 min
Response: 8271840
Conc: 78.97 ng/ml

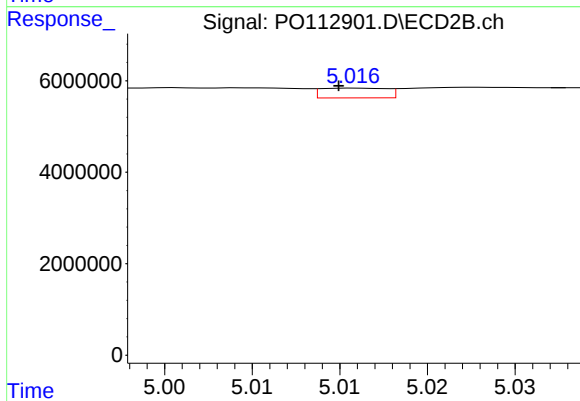

#14 AR-1232-4


R.T.: 5.016 min
Delta R.T.: 0.001 min
Response: 554968
Conc: 9.28 ng/ml

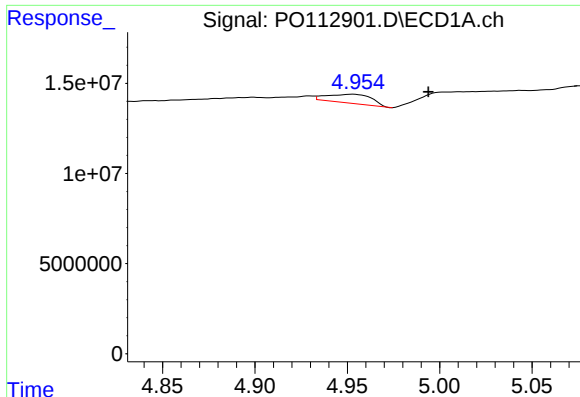

#15 AR-1232-5


R.T.: 4.953 min
Delta R.T.: -0.041 min
Response: 8271840
Conc: 121.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

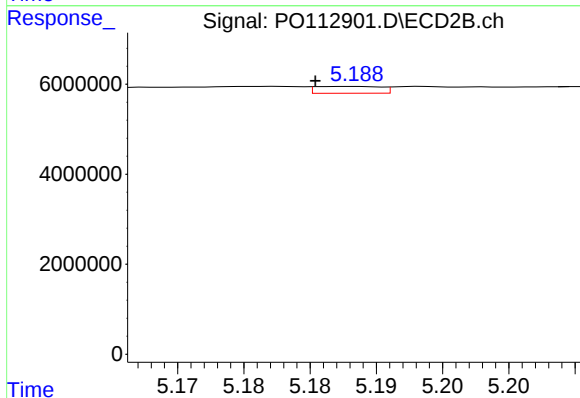


#15 AR-1232-5

R.T.: 5.188 min
Delta R.T.: 0.003 min
Response: 520233
Conc: 7.98 ng/ml

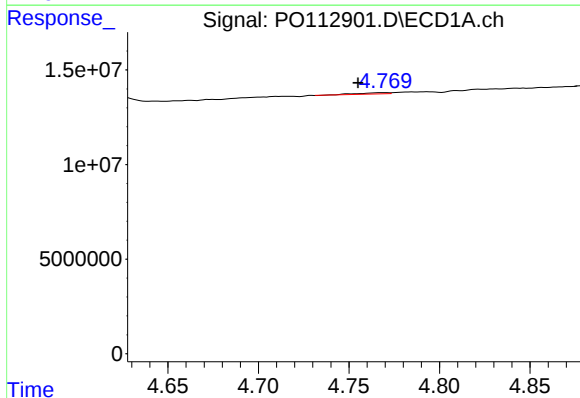


#16 AR-1242-1

R.T.: 4.769 min
Delta R.T.: 0.014 min
Response: 834040
Conc: 3.37 ng/ml

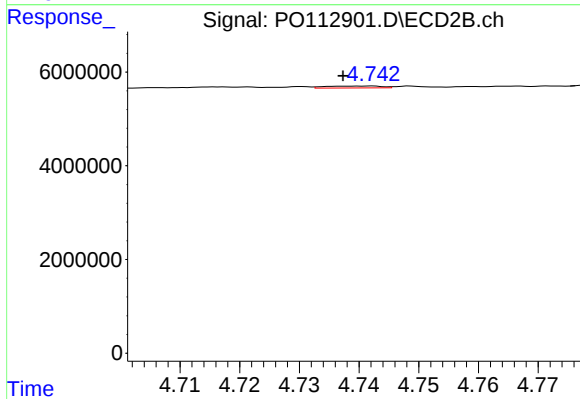

#16 AR-1242-1


R.T.: 4.742 min
Delta R.T.: 0.005 min
Response: 274291
Conc: 1.73 ng/ml

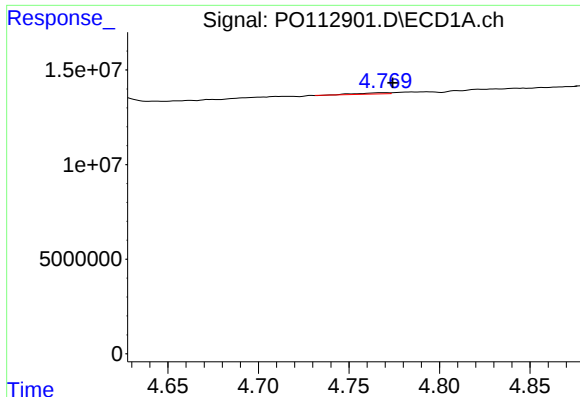

#17 AR-1242-2


R.T.: 4.769 min
Delta R.T.: -0.005 min
Response: 834040
Conc: 2.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

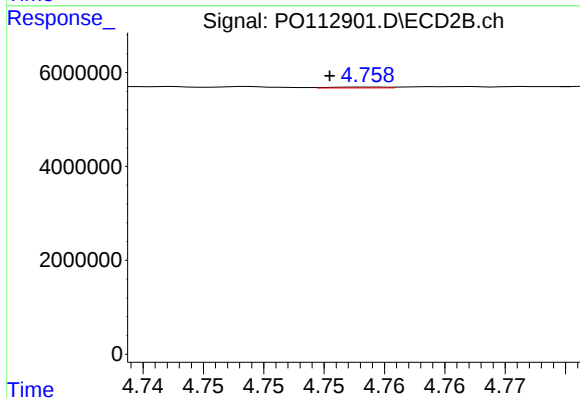


#17 AR-1242-2

R.T.: 4.759 min
Delta R.T.: 0.003 min
Response: 63290
Conc: 0.27 ng/ml

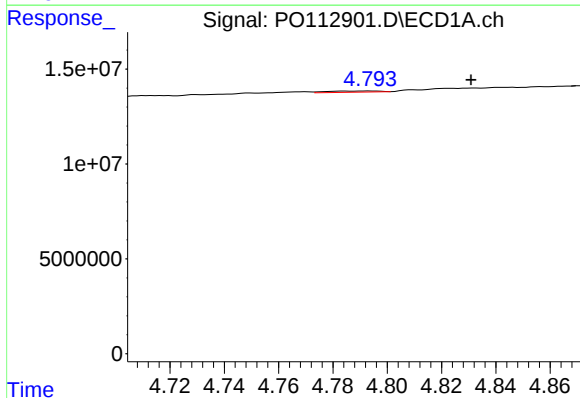


#18 AR-1242-3

R.T.: 4.794 min
Delta R.T.: -0.037 min
Response: 864632
Conc: 3.65 ng/ml

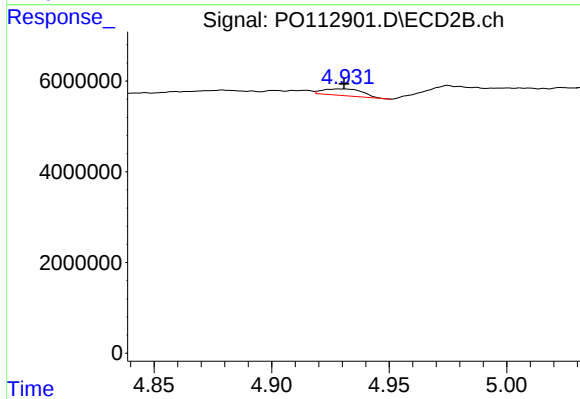

#18 AR-1242-3


R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 1700006
Conc: 14.03 ng/ml

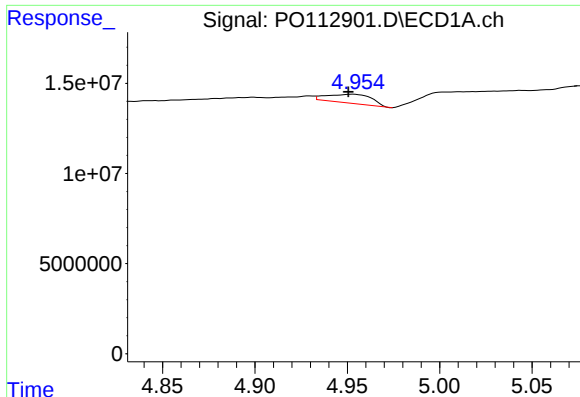

#19 AR-1242-4


R.T.: 4.953 min
Delta R.T.: 0.002 min
Response: 8271840
Conc: 42.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

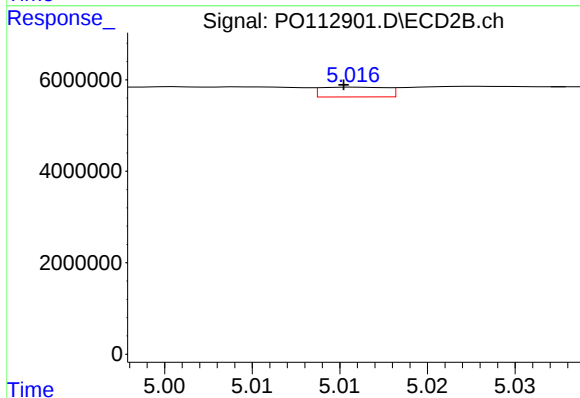


#19 AR-1242-4

R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 554968
Conc: 4.52 ng/ml

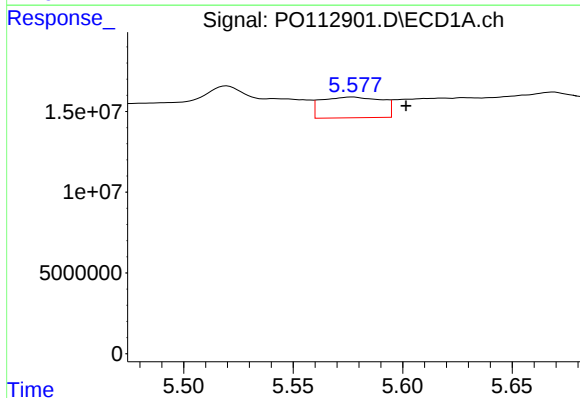


#20 AR-1242-5

R.T.: 5.577 min
Delta R.T.: -0.024 min
Response: 24804141
Conc: 115.95 ng/ml

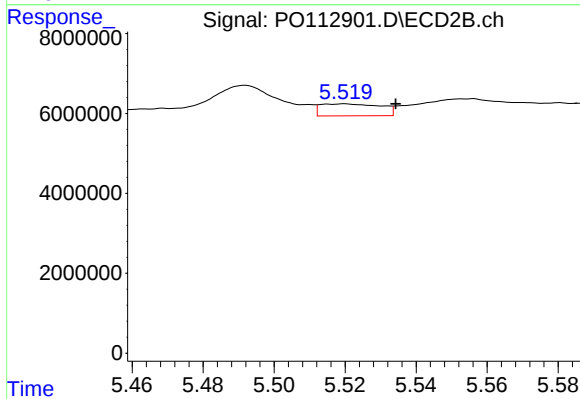

#20 AR-1242-5


R.T.: 5.520 min
Delta R.T.: -0.014 min
Response: 3518217
Conc: 21.86 ng/ml

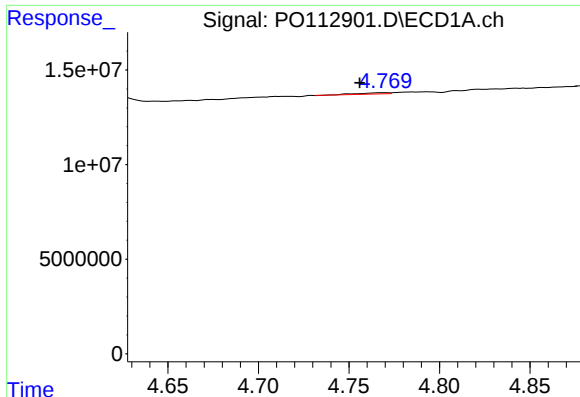

#21 AR-1248-1


R.T.: 4.769 min
Delta R.T.: 0.013 min
Response: 834040
Conc: 4.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

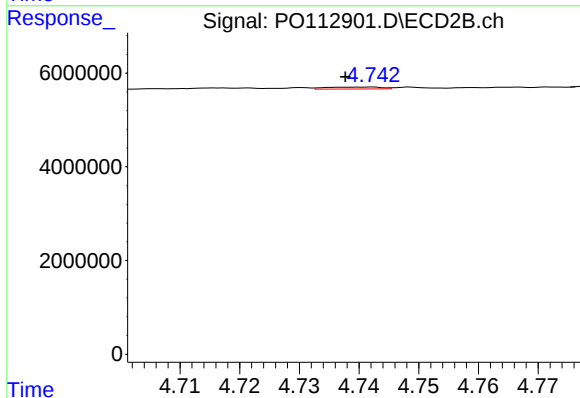


#21 AR-1248-1

R.T.: 4.742 min
Delta R.T.: 0.004 min
Response: 274291
Conc: 2.26 ng/ml

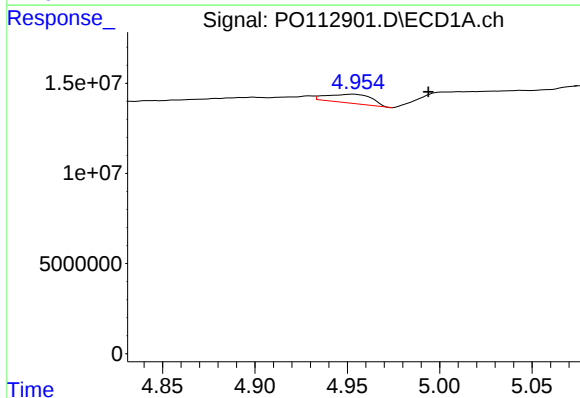


#22 AR-1248-2

R.T.: 4.953 min
Delta R.T.: -0.041 min
Response: 8271840
Conc: 32.42 ng/ml

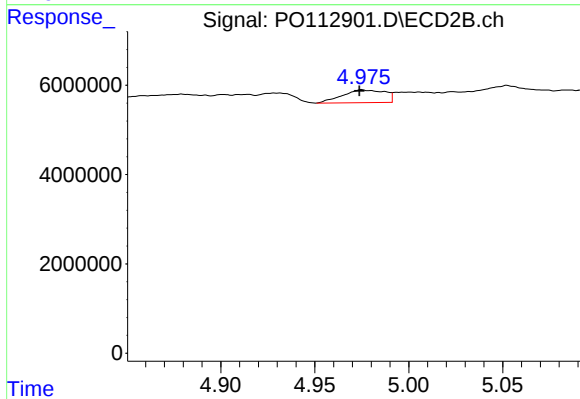

#22 AR-1248-2


R.T.: 4.975 min
Delta R.T.: 0.001 min
Response: 4505891
Conc: 26.62 ng/ml

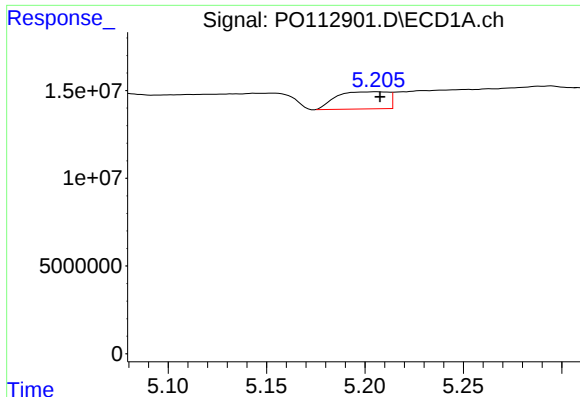

#23 AR-1248-3


R.T.: 5.206 min
Delta R.T.: -0.002 min
Response: 17884748
Conc: 52.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

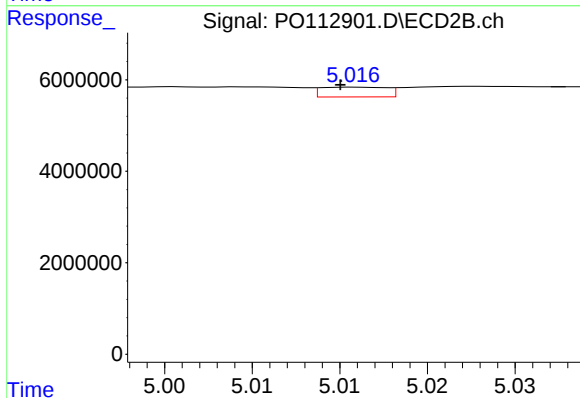


#23 AR-1248-3

R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 554968
Conc: 3.12 ng/ml

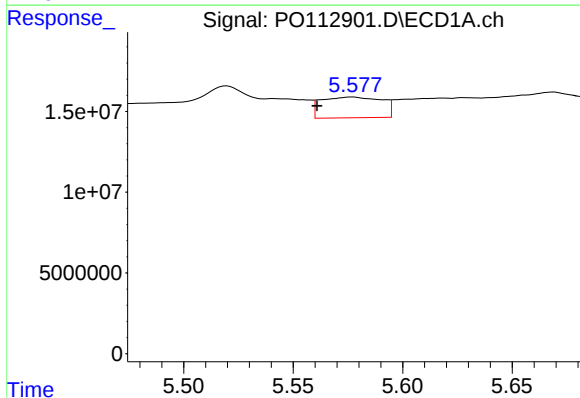


#24 AR-1248-4

R.T.: 5.577 min
Delta R.T.: 0.016 min
Response: 24804141
Conc: 48.82 ng/ml

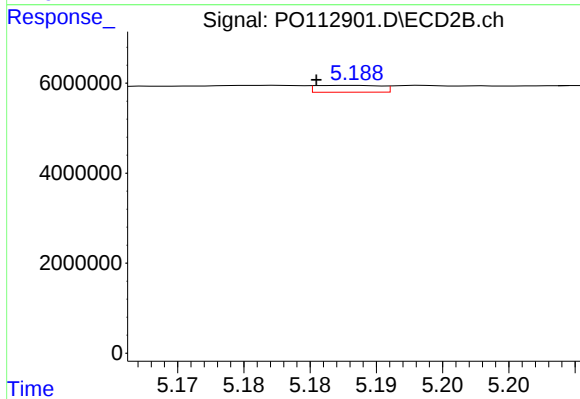

#24 AR-1248-4


R.T.: 5.188 min
Delta R.T.: 0.003 min
Response: 520233
Conc: 2.50 ng/ml

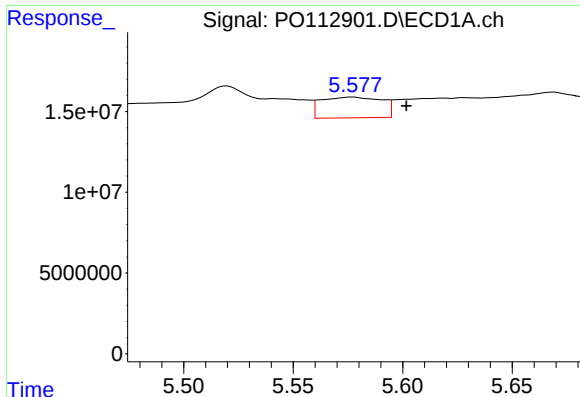

#25 AR-1248-5


R.T.: 5.577 min
Delta R.T.: -0.024 min
Response: 24804141
Conc: 70.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

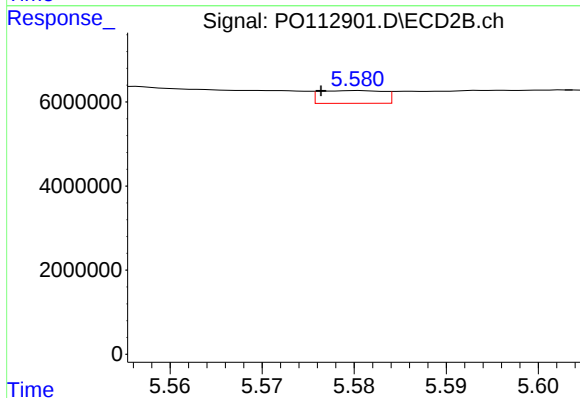


#25 AR-1248-5

R.T.: 5.580 min
Delta R.T.: 0.004 min
Response: 1471701
Conc: 6.85 ng/ml

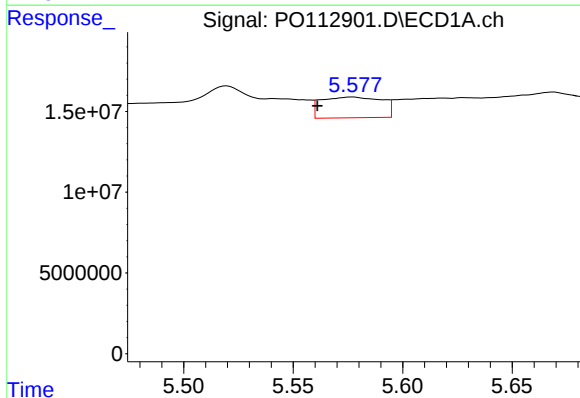


#26 AR-1254-1

R.T.: 5.577 min
Delta R.T.: 0.016 min
Response: 24804141
Conc: 45.18 ng/ml

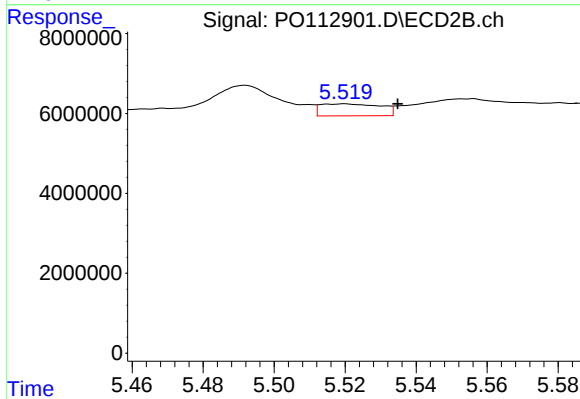

#26 AR-1254-1


R.T.: 5.520 min
Delta R.T.: -0.015 min
Response: 3518217
Conc: 10.71 ng/ml

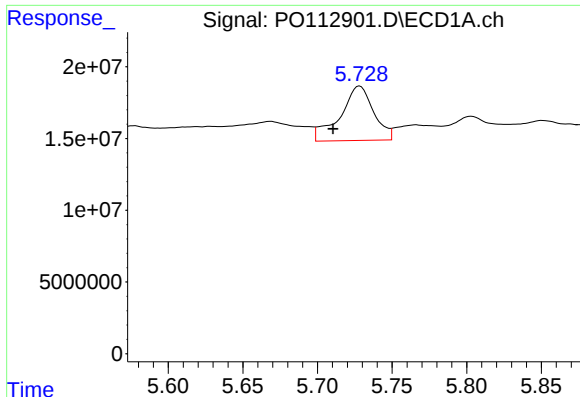

#27 AR-1254-2


R.T.: 5.728 min
Delta R.T.: 0.018 min
Response: 59376892
Conc: 122.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

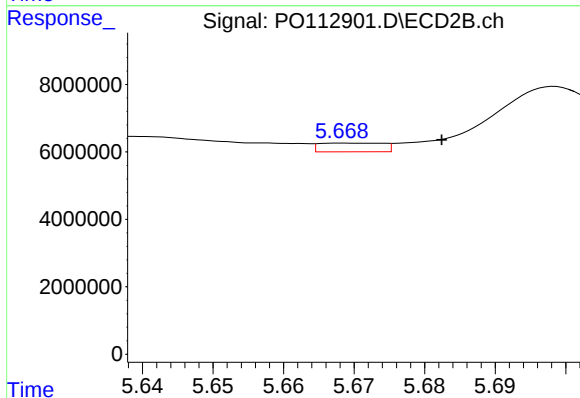


#27 AR-1254-2

R.T.: 5.668 min
Delta R.T.: -0.014 min
Response: 1620945
Conc: 5.60 ng/ml

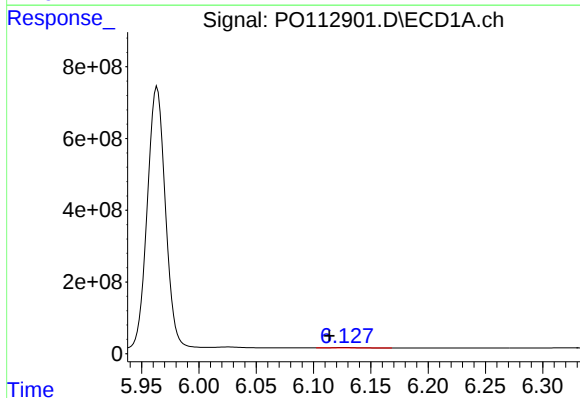


#28 AR-1254-3

R.T.: 6.128 min
Delta R.T.: 0.014 min
Response: 14256971
Conc: 19.16 ng/ml

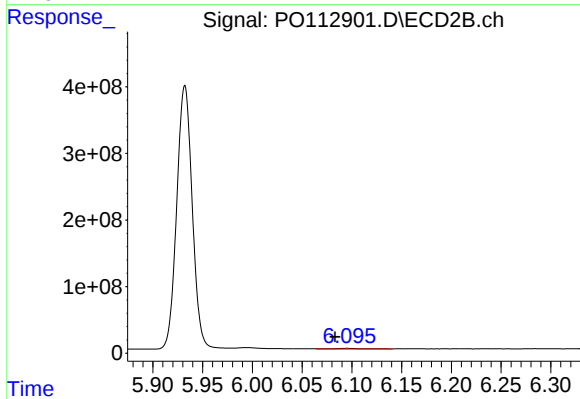

#28 AR-1254-3


R.T.: 6.095 min
Delta R.T.: 0.012 min
Response: 23089685
Conc: 54.02 ng/ml

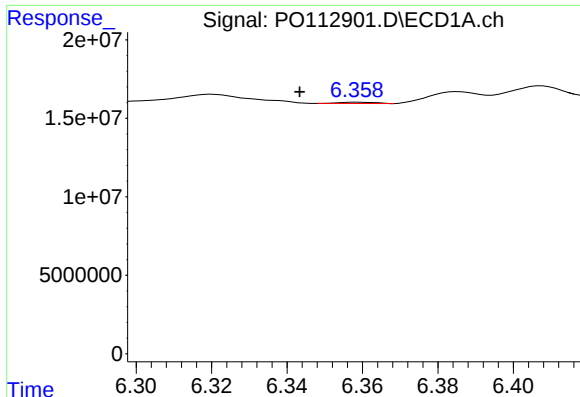

#29 AR-1254-4


R.T.: 6.359 min
Delta R.T.: 0.015 min
Response: 520283
Conc: 0.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

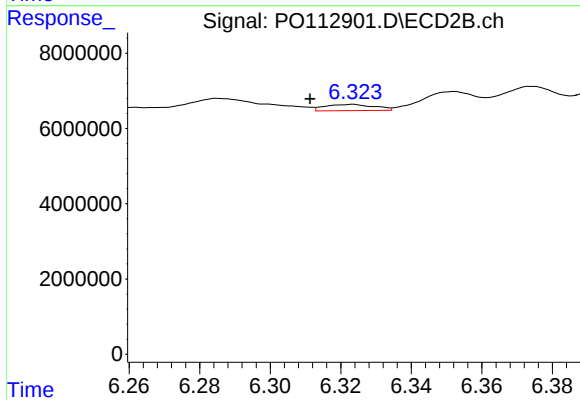


#29 AR-1254-4

R.T.: 6.323 min
Delta R.T.: 0.012 min
Response: 1603536
Conc: 5.87 ng/ml

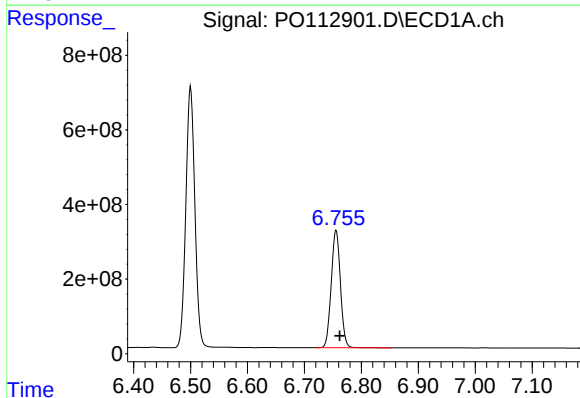


#30 AR-1254-5

R.T.: 6.756 min
Delta R.T.: -0.006 min
Response: 3534471621
Conc: 4993.43 ng/ml

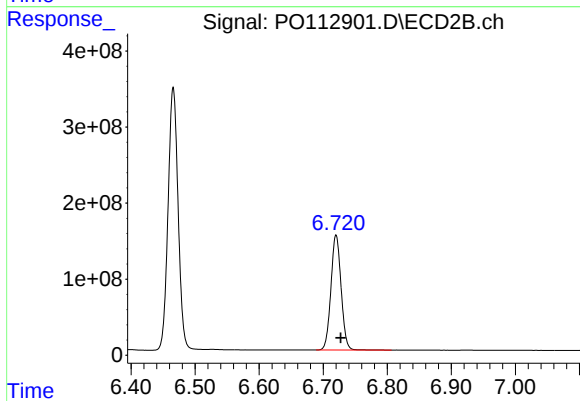

#30 AR-1254-5


R.T.: 6.720 min
Delta R.T.: -0.007 min
Response: 1670816500
Conc: 5002.15 ng/ml

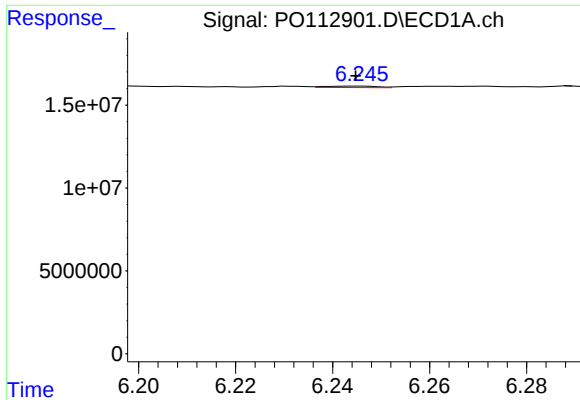

#31 AR-1260-1


R.T.: 6.246 min
Delta R.T.: 0.000 min
Response: 674383
Conc: 1.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

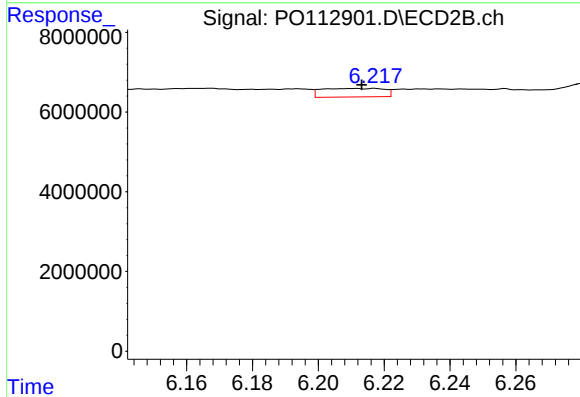


#31 AR-1260-1

R.T.: 6.217 min
Delta R.T.: 0.004 min
Response: 2840274
Conc: 11.43 ng/ml

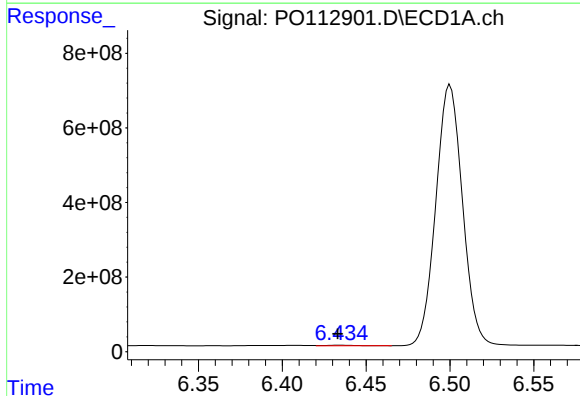


#32 AR-1260-2

R.T.: 6.434 min
Delta R.T.: 0.001 min
Response: 17030012
Conc: 24.76 ng/ml

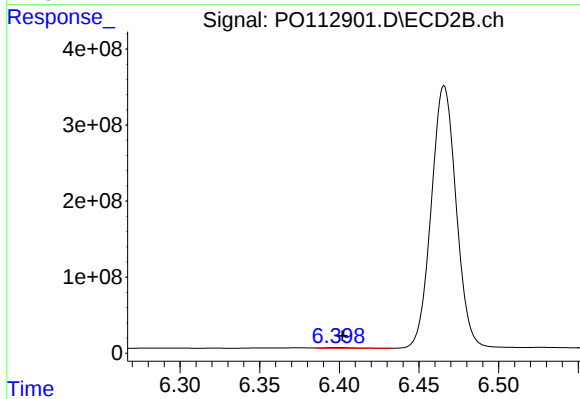

#32 AR-1260-2


R.T.: 6.398 min
Delta R.T.: -0.003 min
Response: 9665275
Conc: 29.33 ng/ml

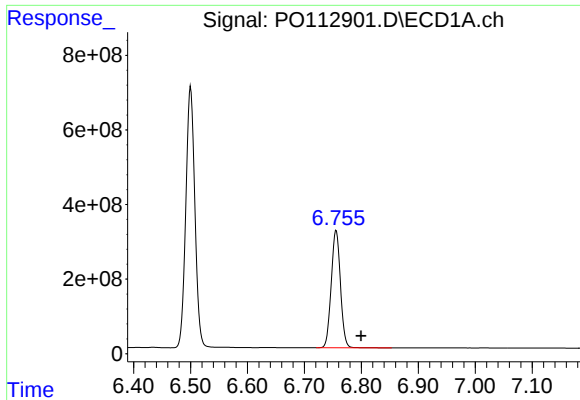

#33 AR-1260-3


R.T.: 6.756 min
Delta R.T.: -0.044 min
Response: 3534471621
Conc: 6010.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

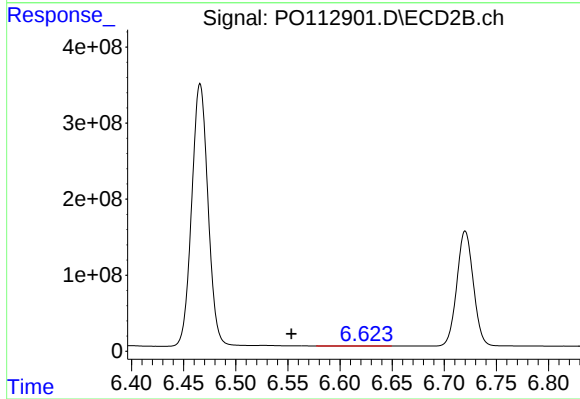


#33 AR-1260-3

R.T.: 6.595 min
Delta R.T.: 0.041 min
Response: 197466
Conc: 0.77 ng/ml

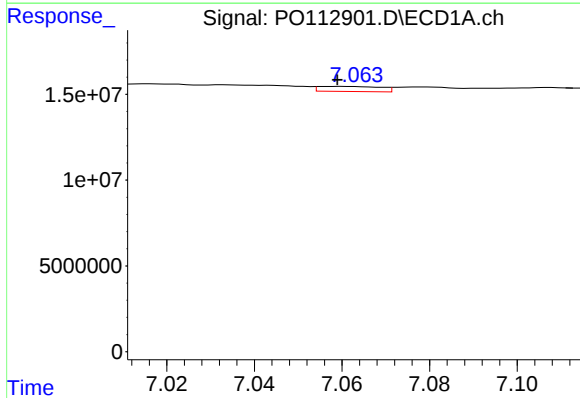


#34 AR-1260-4

R.T.: 7.059 min
Delta R.T.: 0.000 min
Response: 2847857
Conc: 6.31 ng/ml

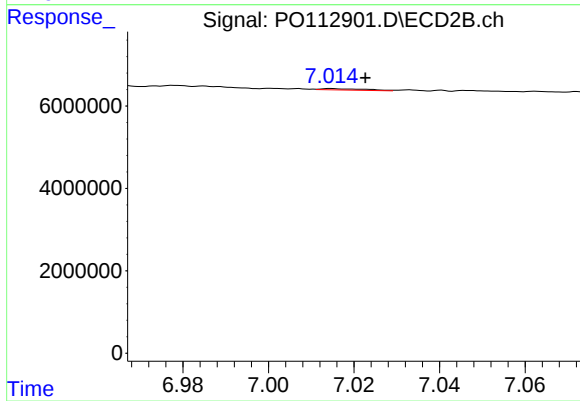

#34 AR-1260-4


R.T.: 7.015 min
Delta R.T.: -0.008 min
Response: 243742
Conc: 1.27 ng/ml

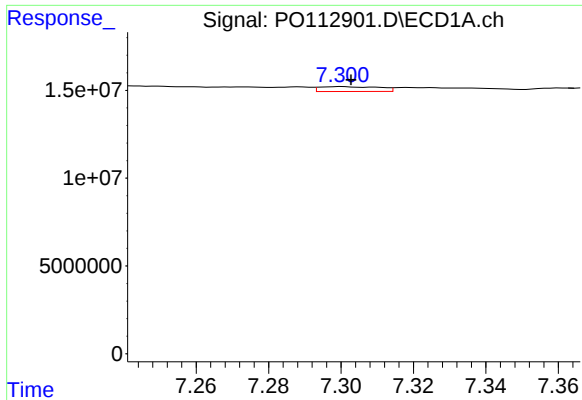

#35 AR-1260-5


R.T.: 7.300 min
Delta R.T.: -0.003 min
Response: 3124510
Conc: 2.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

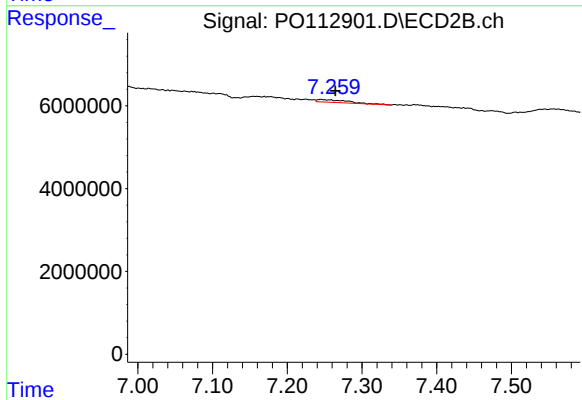


#35 AR-1260-5

R.T.: 7.245 min
Delta R.T.: -0.019 min
Response: 1862098
Conc: 4.52 ng/ml

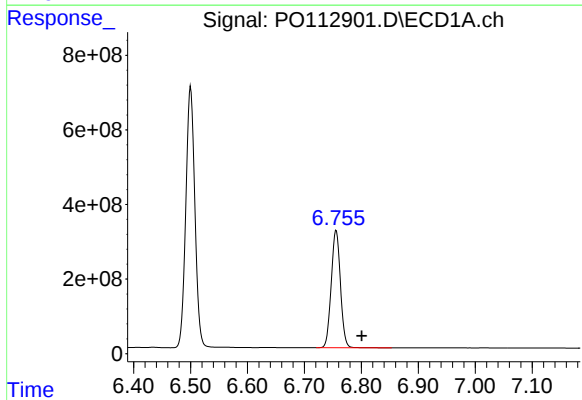


#36 AR-1262-1

R.T.: 6.756 min
Delta R.T.: -0.045 min
Response: 3534471621
Conc: 3803.75 ng/ml

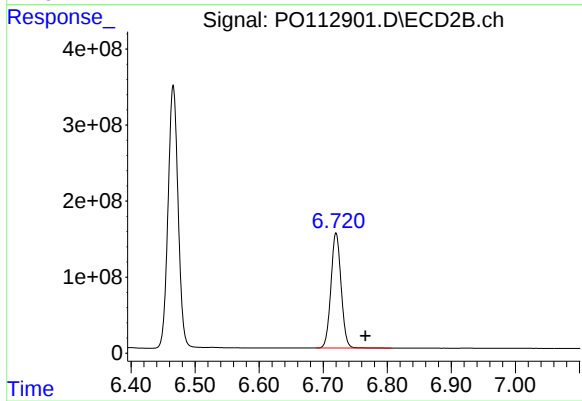

#36 AR-1262-1


R.T.: 6.720 min
Delta R.T.: -0.046 min
Response: 1670816500
Conc: 4027.73 ng/ml

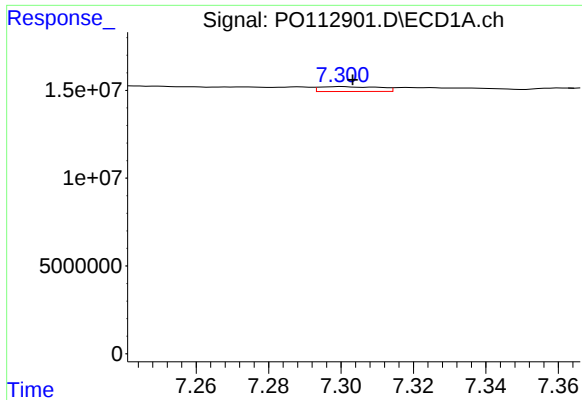

#37 AR-1262-2


R.T.: 7.300 min
Delta R.T.: -0.003 min
Response: 3124510
Conc: 2.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

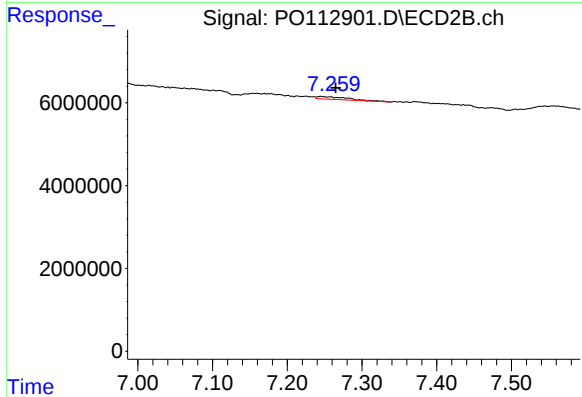


#37 AR-1262-2

R.T.: 7.245 min
Delta R.T.: -0.020 min
Response: 1862098
Conc: 3.61 ng/ml

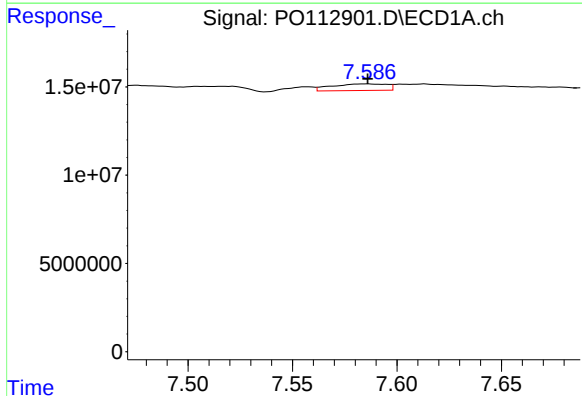


#38 AR-1262-3

R.T.: 7.586 min
Delta R.T.: 0.000 min
Response: 6888208
Conc: 11.67 ng/ml

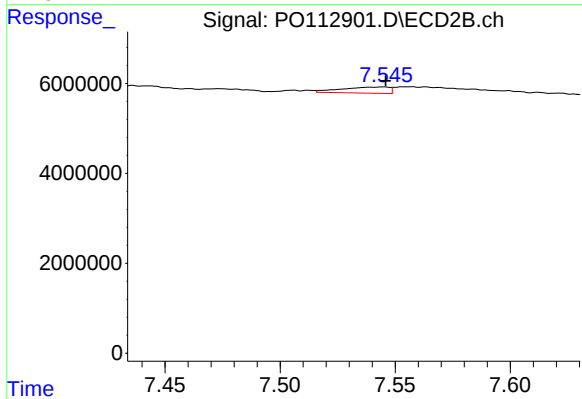

#38 AR-1262-3


R.T.: 7.545 min
Delta R.T.: 0.000 min
Response: 1961177
Conc: 10.51 ng/ml

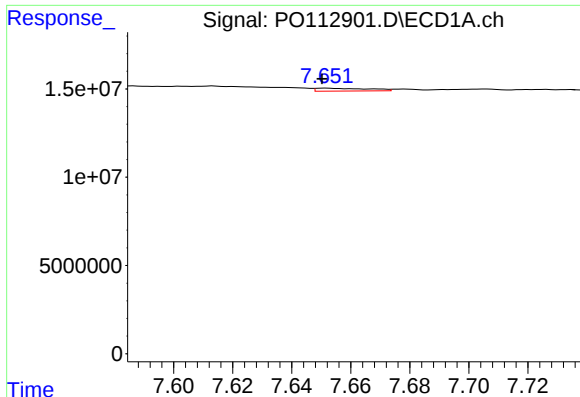

#39 AR-1262-4


R.T.: 7.651 min
Delta R.T.: 0.001 min
Response: 2049574
Conc: 2.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

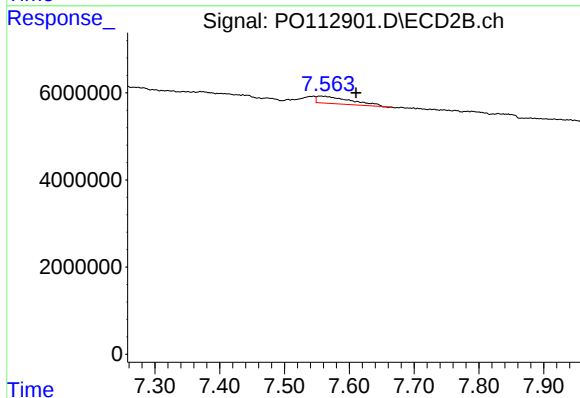


#39 AR-1262-4

R.T.: 7.556 min
Delta R.T.: -0.054 min
Response: 6061894
Conc: 21.04 ng/ml

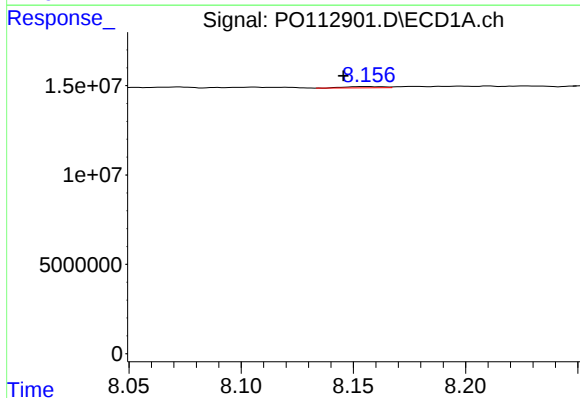


#40 AR-1262-5

R.T.: 8.156 min
Delta R.T.: 0.010 min
Response: 872067
Conc: 2.01 ng/ml

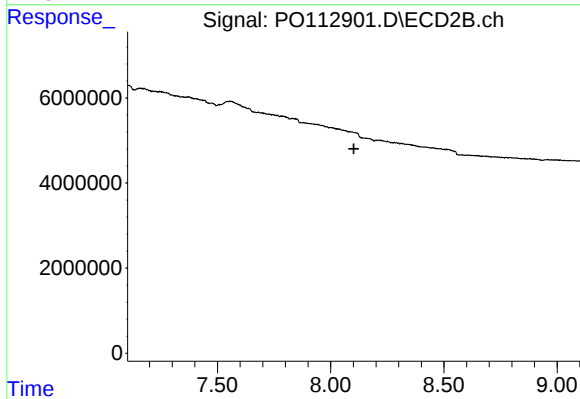

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 8.103 min
Response: 0
Conc: N.D.

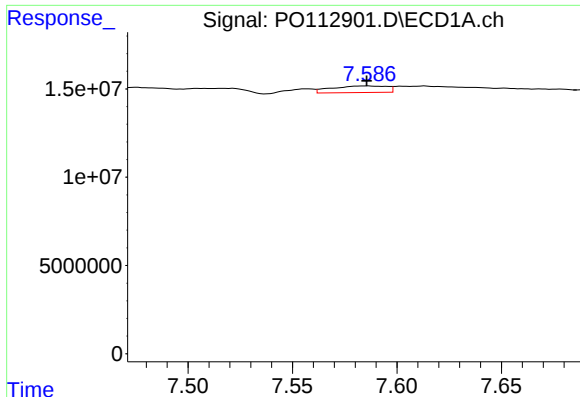

#41 AR-1268-1


R.T.: 7.586 min
Delta R.T.: 0.000 min
Response: 6888208
Conc: 3.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

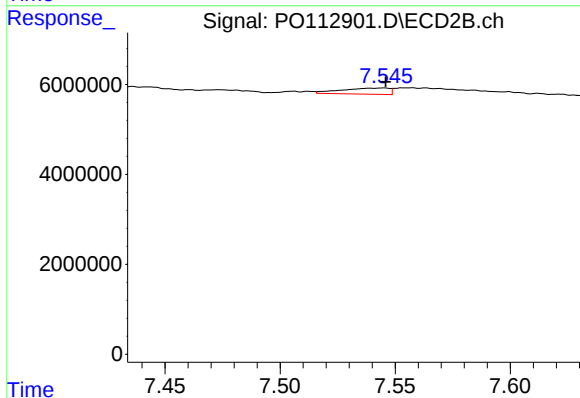


#41 AR-1268-1

R.T.: 7.545 min
Delta R.T.: -0.001 min
Response: 1961177
Conc: 3.79 ng/ml

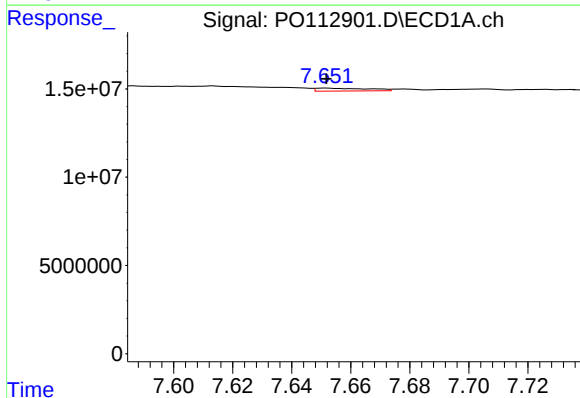


#42 AR-1268-2

R.T.: 7.651 min
Delta R.T.: 0.000 min
Response: 2049574
Conc: 1.39 ng/ml

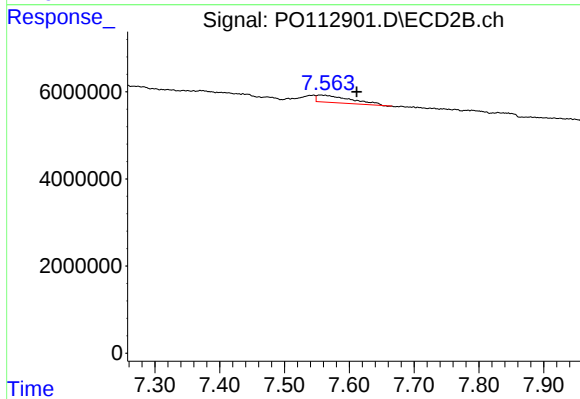

#42 AR-1268-2


R.T.: 7.556 min
Delta R.T.: -0.055 min
Response: 6061894
Conc: 14.26 ng/ml

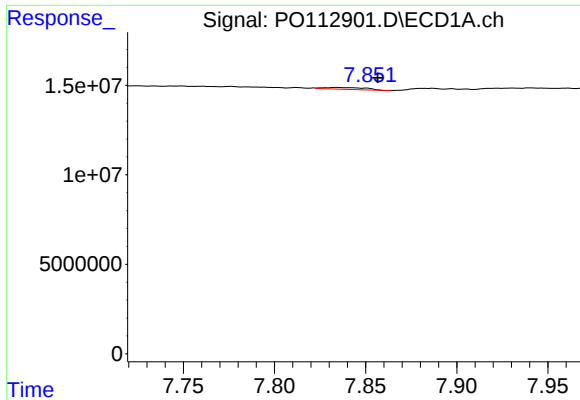

#43 AR-1268-3


R.T.: 7.834 min
Delta R.T.: -0.022 min
Response: 1627087
Conc: 1.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

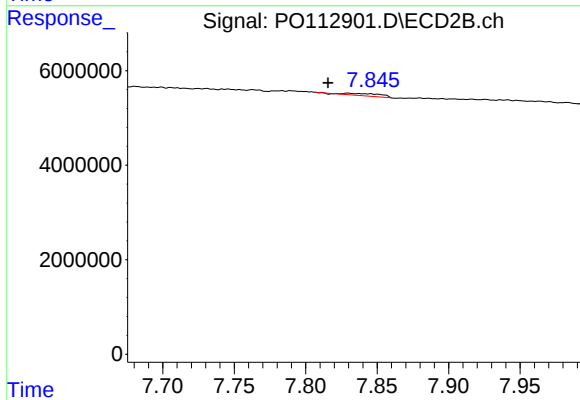


#43 AR-1268-3

R.T.: 7.830 min
Delta R.T.: 0.014 min
Response: 784393
Conc: 2.44 ng/ml

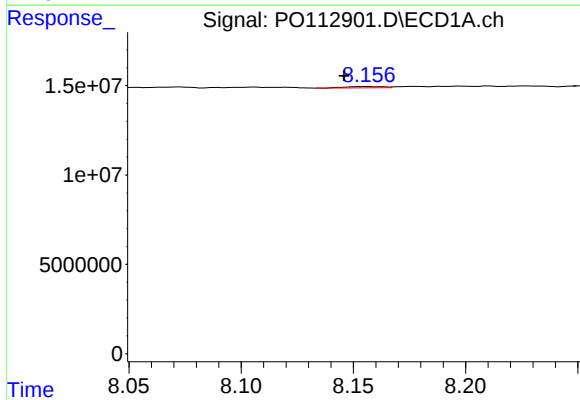


#44 AR-1268-4

R.T.: 8.156 min
Delta R.T.: 0.010 min
Response: 872067
Conc: 1.81 ng/ml

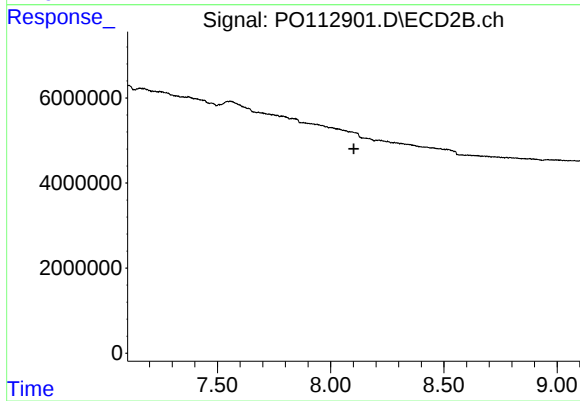

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.103 min
Response: 0
Conc: N.D.

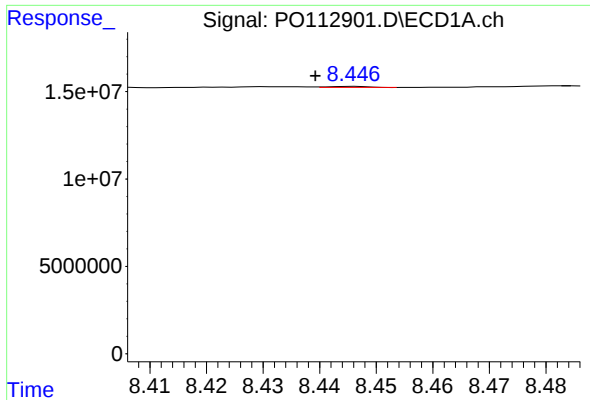

#45 AR-1268-5

R.T.: 8.446 min
Delta R.T.: 0.007 min
Response: 291142
Conc: 0.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

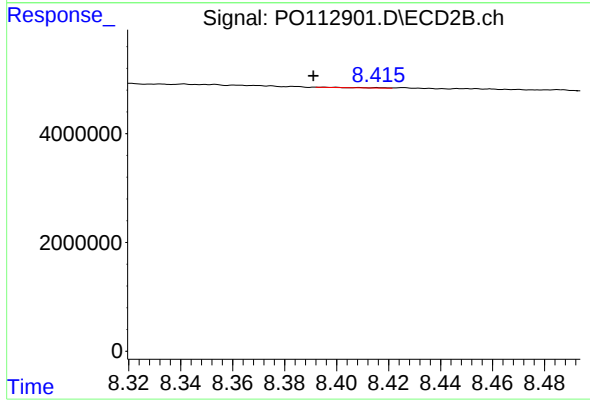

#45 AR-1268-5

R.T.: 8.409 min
Delta R.T.: 0.018 min
Response: 51358
Conc: 0.07 ng/ml