

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081325\
 Data File : P0112905.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2025 13:15
 Operator : YP/AJ
 Sample : Q2836-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-A2-15-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/14/2025
 Supervised By :mohammad ahmed 08/18/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 16:00:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.658	159.1E6	91429465	19.566m	18.399m
2) SA Decachlor...	8.684	8.633	111.1E6	31020078	15.196m	17.554

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081325\
Data File : PO112905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2025 13:15
Operator : YP/AJ
Sample : Q2836-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-A2-15-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2025
Supervised By :mohammad ahmed 08/18/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 16:00:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

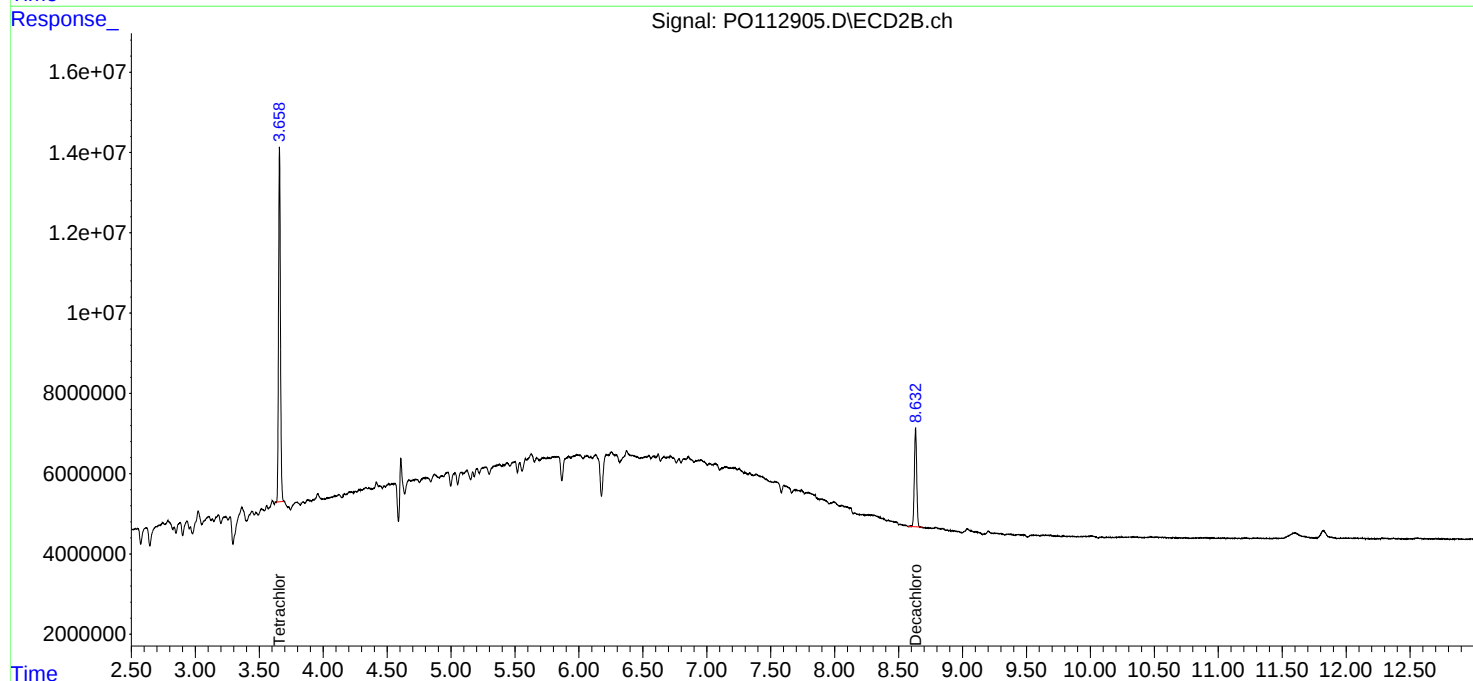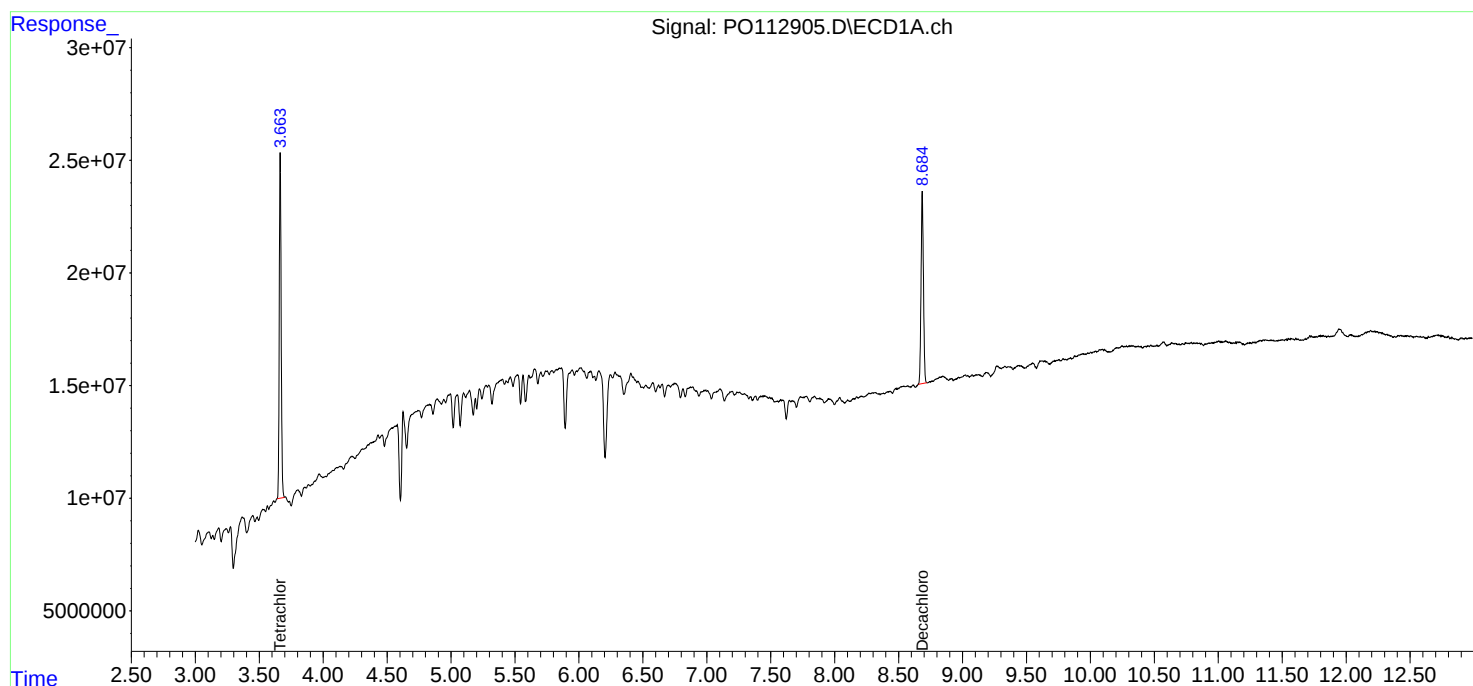

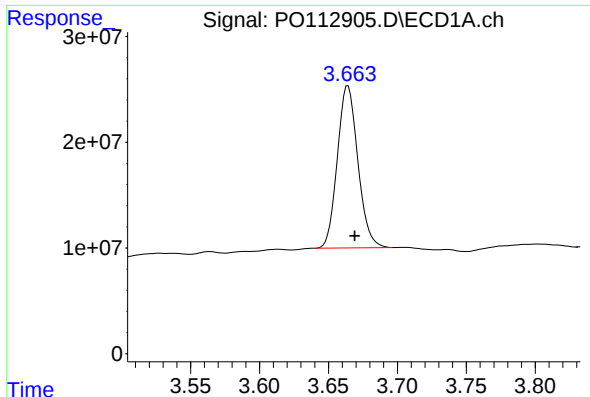


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: -0.006 min
Response: 159099306
Conc: 19.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-A2-15-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2025
Supervised By :mohammad ahmed 08/18/2025

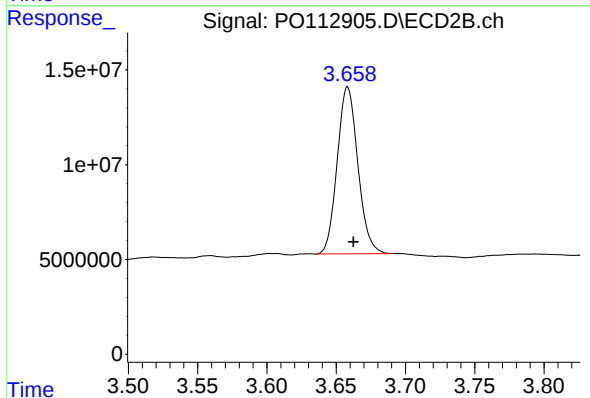


#1 Tetrachloro-m-xylene

R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 91429465
Conc: 18.40 ng/ml m

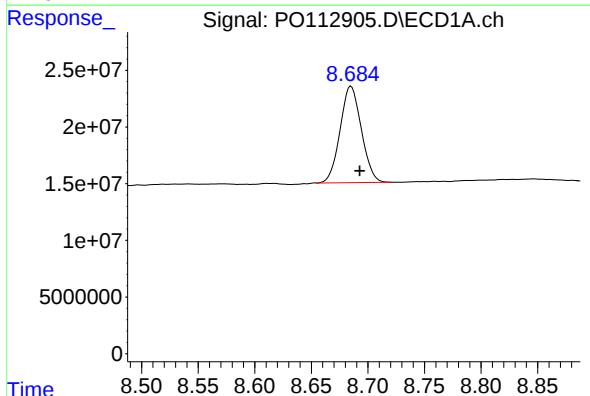

#2 Decachlorobiphenyl

R.T.: 8.684 min
Delta R.T.: -0.008 min
Response: 111112242
Conc: 15.20 ng/ml m

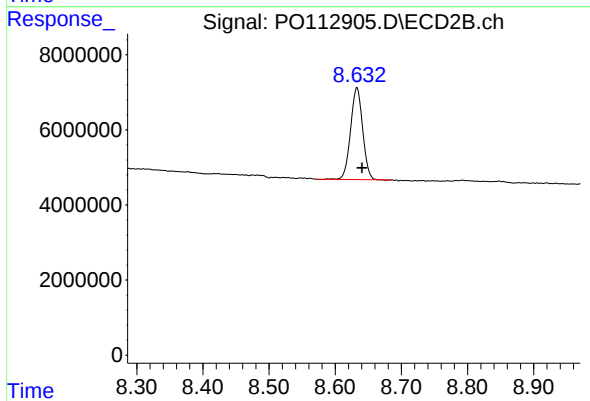

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: -0.008 min
Response: 31020078
Conc: 17.55 ng/ml