

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081419\
 Data File : P0059274.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Aug 2019 13:15
 Operator : SM/SJ
 Sample : K4341-03 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-40

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 15:56:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 14 09:07:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.149	3.509	157347	157224	3.728	3.936
2) SA Decachlor...	9.650	8.387	235325	161518	4.345	4.092

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081419\
Data File : PO059274.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2019 13:15
Operator : SM/SJ
Sample : K4341-03 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HA-40

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 15:56:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 14 09:07:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

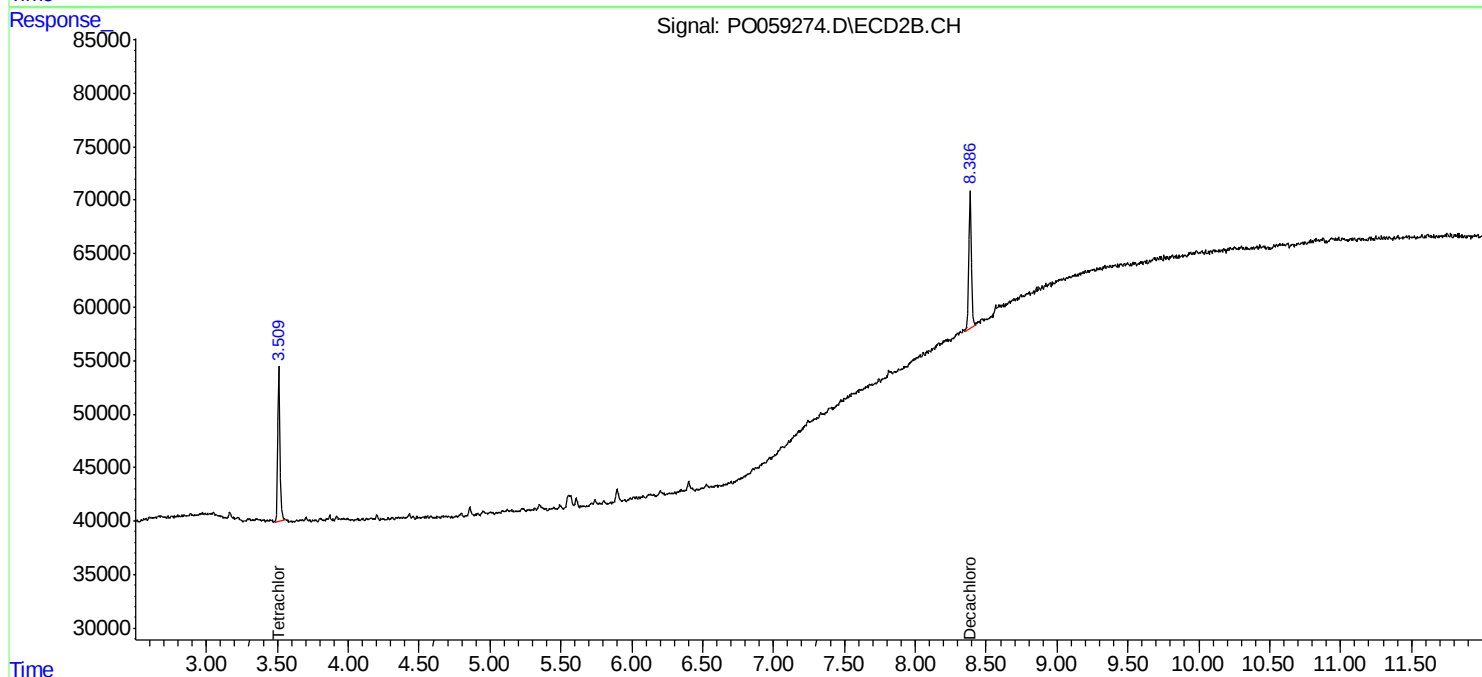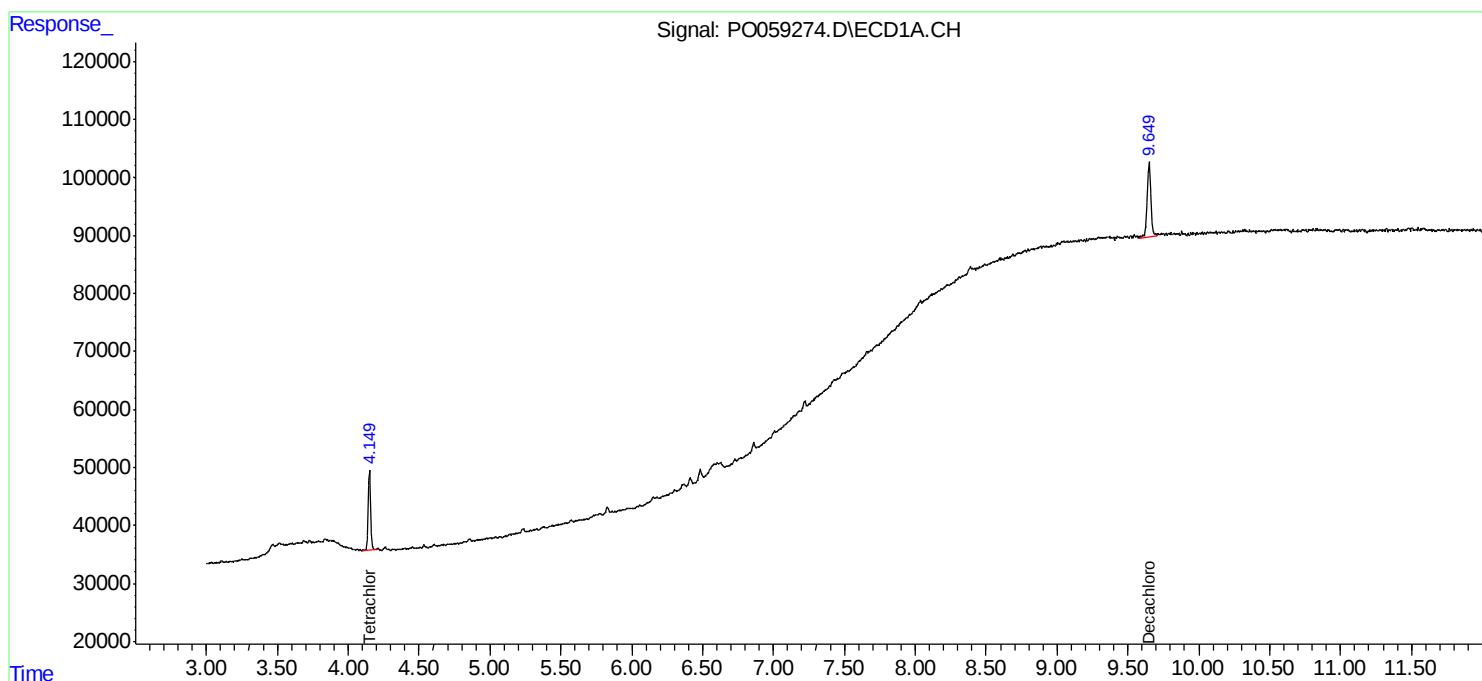


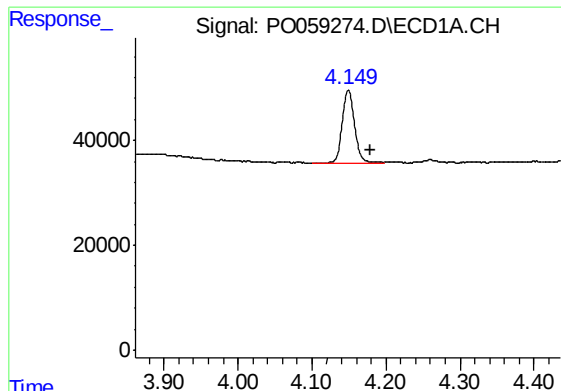

#1 Tetrachloro-m-xylene


R.T.: 4.149 min
Delta R.T.: -0.030 min
Response: 157347
Conc: 3.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-40

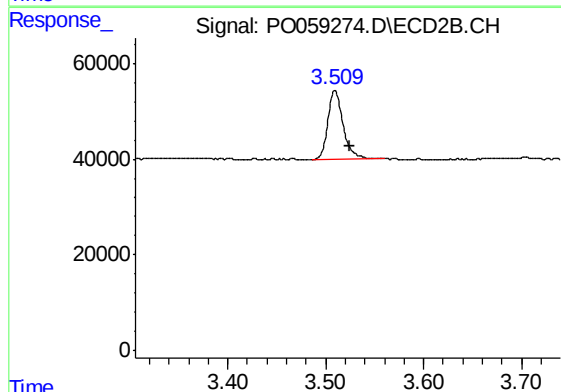


#1 Tetrachloro-m-xylene

R.T.: 3.509 min
Delta R.T.: -0.015 min
Response: 157224
Conc: 3.94 ng/ml

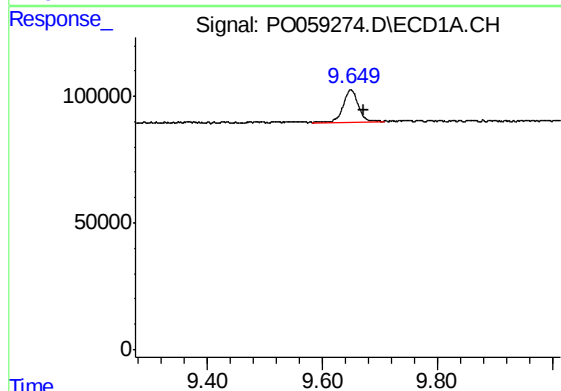

#2 Decachlorobiphenyl

R.T.: 9.650 min
Delta R.T.: -0.023 min
Response: 235325
Conc: 4.35 ng/ml

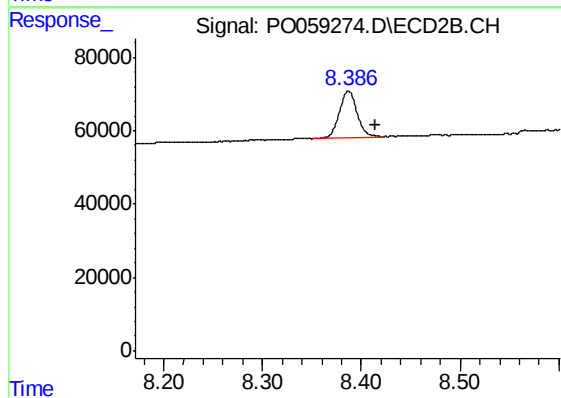

#2 Decachlorobiphenyl

R.T.: 8.387 min
Delta R.T.: -0.027 min
Response: 161518
Conc: 4.09 ng/ml