

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081419\
 Data File : P0059282.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Aug 2019 15:48
 Operator : SM/SJ
 Sample : K4341-07 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-44

Manual Integrations
 APPROVED

Ankita
 8/16/2019 2:37:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 18:42:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 14 09:07:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.150	3.511	151781	156589	3.596	3.920
2) SA Decachlor...	9.646	8.387	237600	159055	4.387	4.029
Target Compounds						
26) L6 AR-1254-1	6.144	5.349	2067950	2669951	875.771m	1030.655
27) L6 AR-1254-2	6.359	5.494	3568120	2231322	925.834m	974.620
28) L6 AR-1254-3	6.726	5.890	3647842	3267213	900.783m	887.983
29) L6 AR-1254-4	7.010	6.116	2979933	2102432	827.611	904.189m
30) L6 AR-1254-5	7.425	6.526	1516445	1487493	418.357m	431.213m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081419\
Data File : PO059282.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2019 15:48
Operator : SM/SJ
Sample : K4341-07 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HA-44


Manual Integrations
APPROVED

Ankita
8/16/2019 2:37:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 18:42:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 14 09:07:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

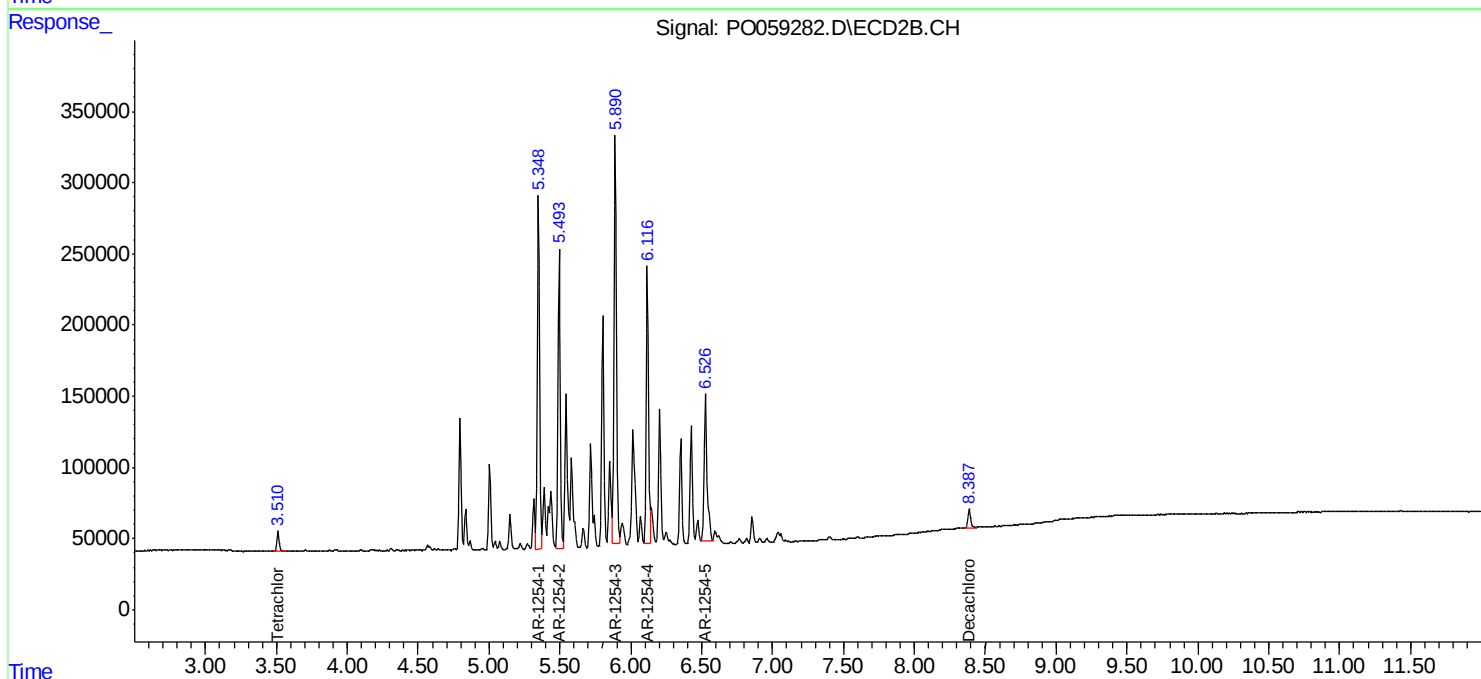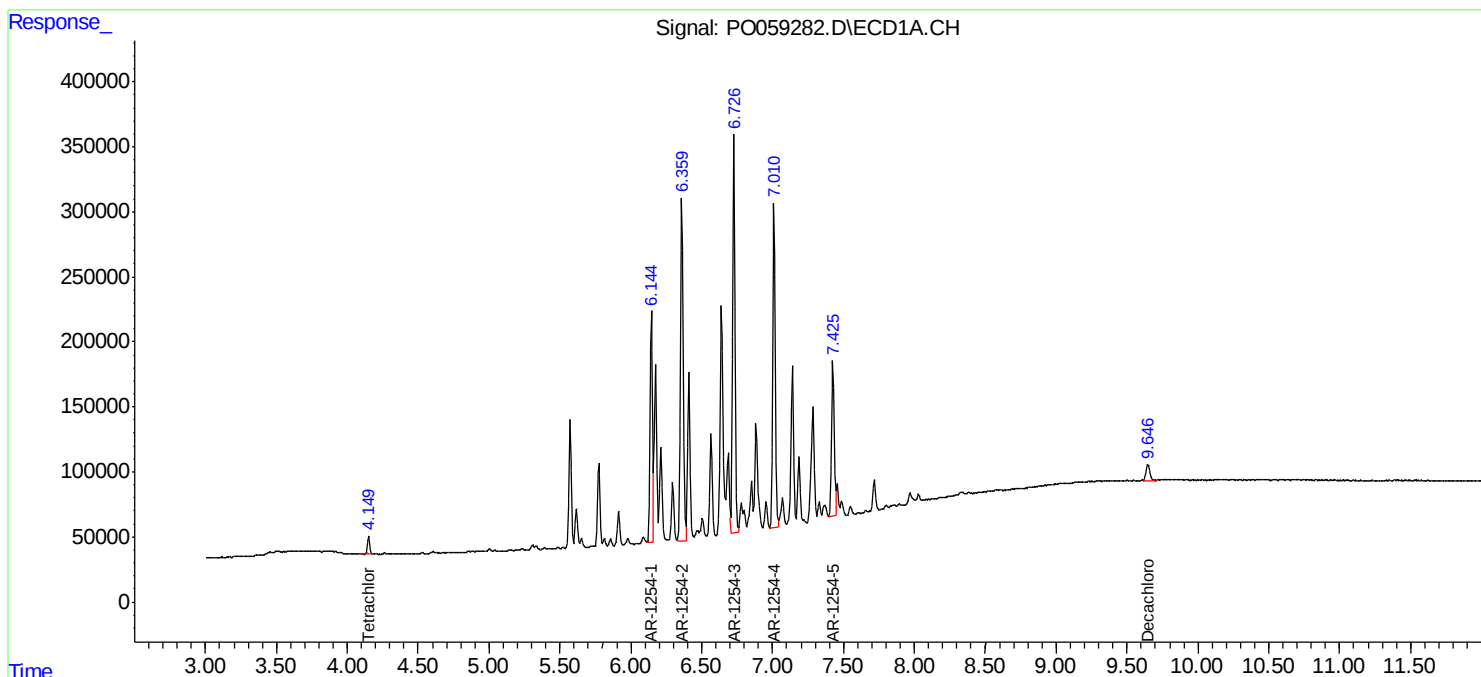

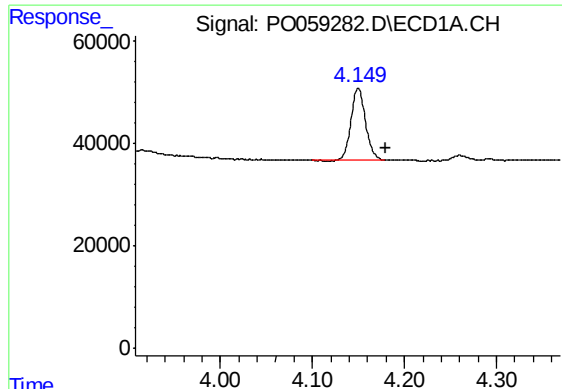


#1 Tetrachloro-m-xylene

R.T.: 4.150 min
Delta R.T.: -0.029 min
Response: 151781
Conc: 3.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-44


Manual Integrations
APPROVED

Ankita
8/16/2019 2:37:38 PM

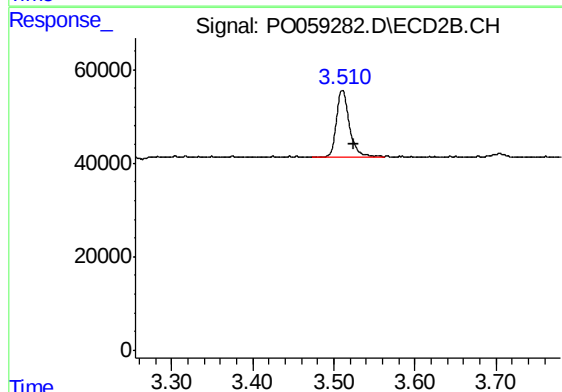


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: -0.014 min
Response: 156589
Conc: 3.92 ng/ml

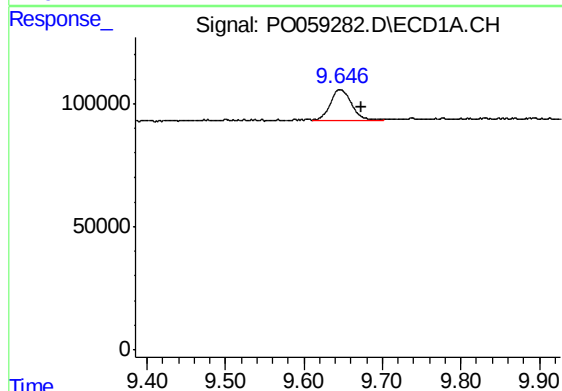


#2 Decachlorobiphenyl

R.T.: 9.646 min
Delta R.T.: -0.027 min
Response: 237600
Conc: 4.39 ng/ml

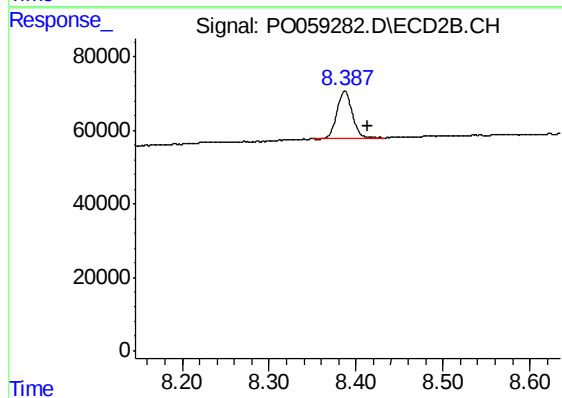

#2 Decachlorobiphenyl

R.T.: 8.387 min
Delta R.T.: -0.027 min
Response: 159055
Conc: 4.03 ng/ml

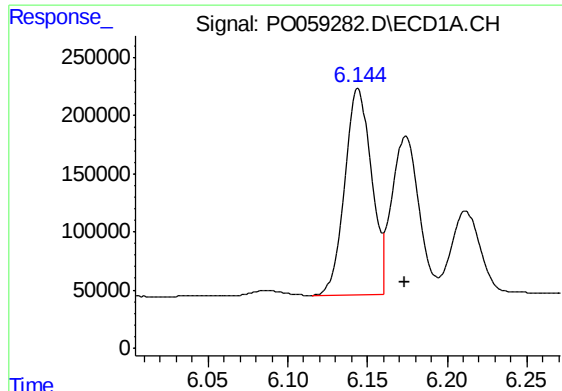


#26 AR-1254-1

R.T.: 6.144 min
Delta R.T.: -0.030 min
Response: 2067950
Conc: 875.77 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-44


Manual Integrations
APPROVED

Ankita
8/16/2019 2:37:38 PM

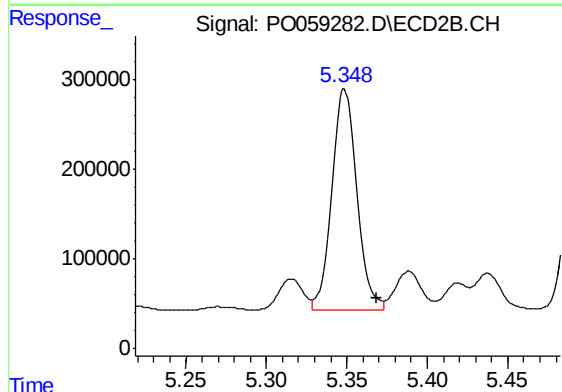


#26 AR-1254-1

R.T.: 5.349 min
Delta R.T.: -0.020 min
Response: 2669951
Conc: 1030.65 ng/ml

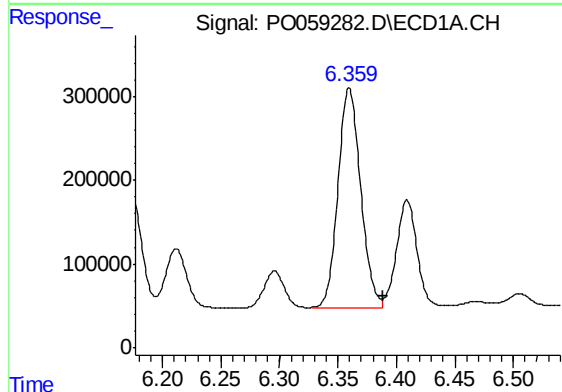


#27 AR-1254-2

R.T.: 6.359 min
Delta R.T.: -0.030 min
Response: 3568120
Conc: 925.83 ng/ml m

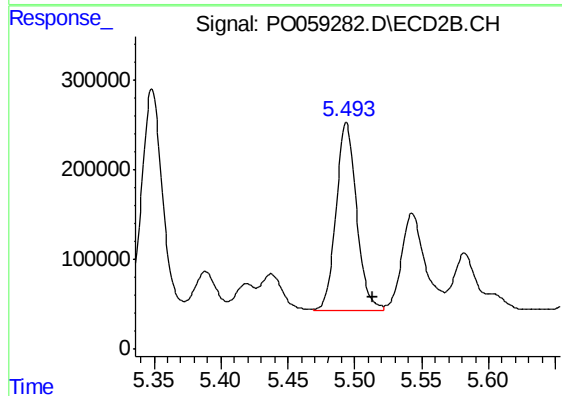

#27 AR-1254-2

R.T.: 5.494 min
Delta R.T.: -0.020 min
Response: 2231322
Conc: 974.62 ng/ml

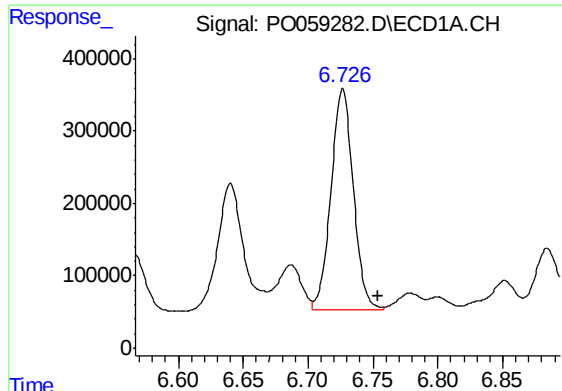


#28 AR-1254-3

R.T.: 6.726 min
Delta R.T.: -0.027 min
Response: 3647842
Conc: 900.78 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-44


Manual Integrations
APPROVED

Ankita
8/16/2019 2:37:38 PM

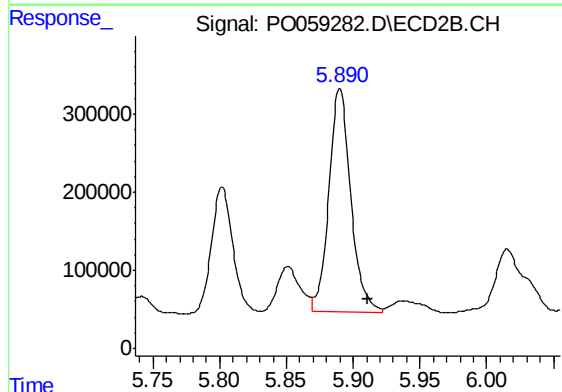


#28 AR-1254-3

R.T.: 5.890 min
Delta R.T.: -0.021 min
Response: 3267213
Conc: 887.98 ng/ml

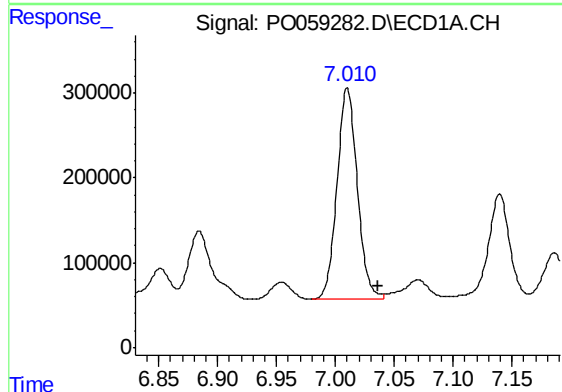


#29 AR-1254-4

R.T.: 7.010 min
Delta R.T.: -0.026 min
Response: 2979933
Conc: 827.61 ng/ml

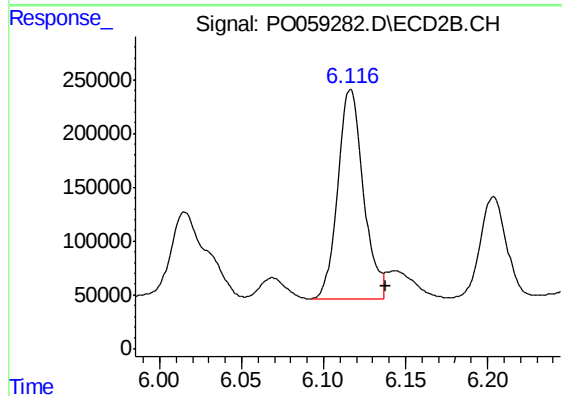

#29 AR-1254-4

R.T.: 6.116 min
Delta R.T.: -0.022 min
Response: 2102432
Conc: 904.19 ng/ml m

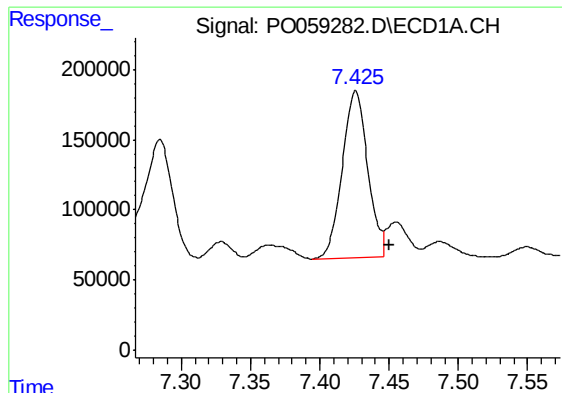


#30 AR-1254-5

R.T.: 7.425 min
Delta R.T.: -0.025 min
Response: 1516445
Conc: 418.36 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-44

Manual Integrations
APPROVED

Ankita
8/16/2019 2:37:38 PM

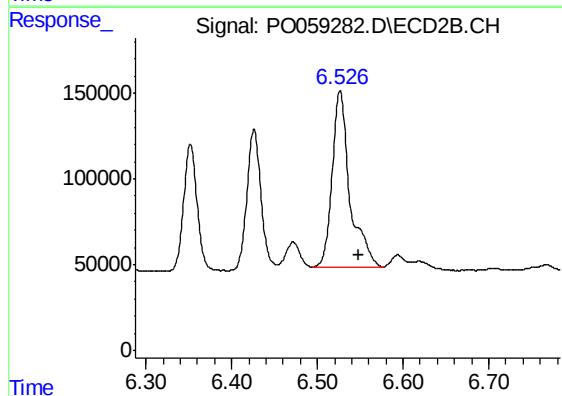

#30 AR-1254-5

R.T.: 6.526 min
Delta R.T.: -0.022 min
Response: 1487493
Conc: 431.21 ng/ml m