

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081419\
 Data File : P0059283.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Aug 2019 16:04
 Operator : SM/SJ
 Sample : K4341-08 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-45

Manual Integrations
 APPROVED

Ankita
 8/16/2019 2:37:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 18:43:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 14 09:07:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.146	3.510	200673	143517	4.755m	3.592m
2)	SA Decachlor...	9.641	8.385	225583	168433	4.165m	4.267
Target Compounds							
26)	L6 AR-1254-1	6.140	5.348	59197	68289	25.070m	26.361
27)	L6 AR-1254-2	6.356	5.492	144688	63120	37.543m	27.570m#
28)	L6 AR-1254-3	6.722	5.889	121575	120739	30.021m	32.815
29)	L6 AR-1254-4	7.006	6.115	115732	87800	32.142	37.760
30)	L6 AR-1254-5	7.423	6.524	102512	79917	28.281m	23.167m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081419\
Data File : PO059283.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2019 16:04
Operator : SM/SJ
Sample : K4341-08 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HA-45


Manual Integrations
APPROVED

Ankita
8/16/2019 2:37:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 18:43:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 14 09:07:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

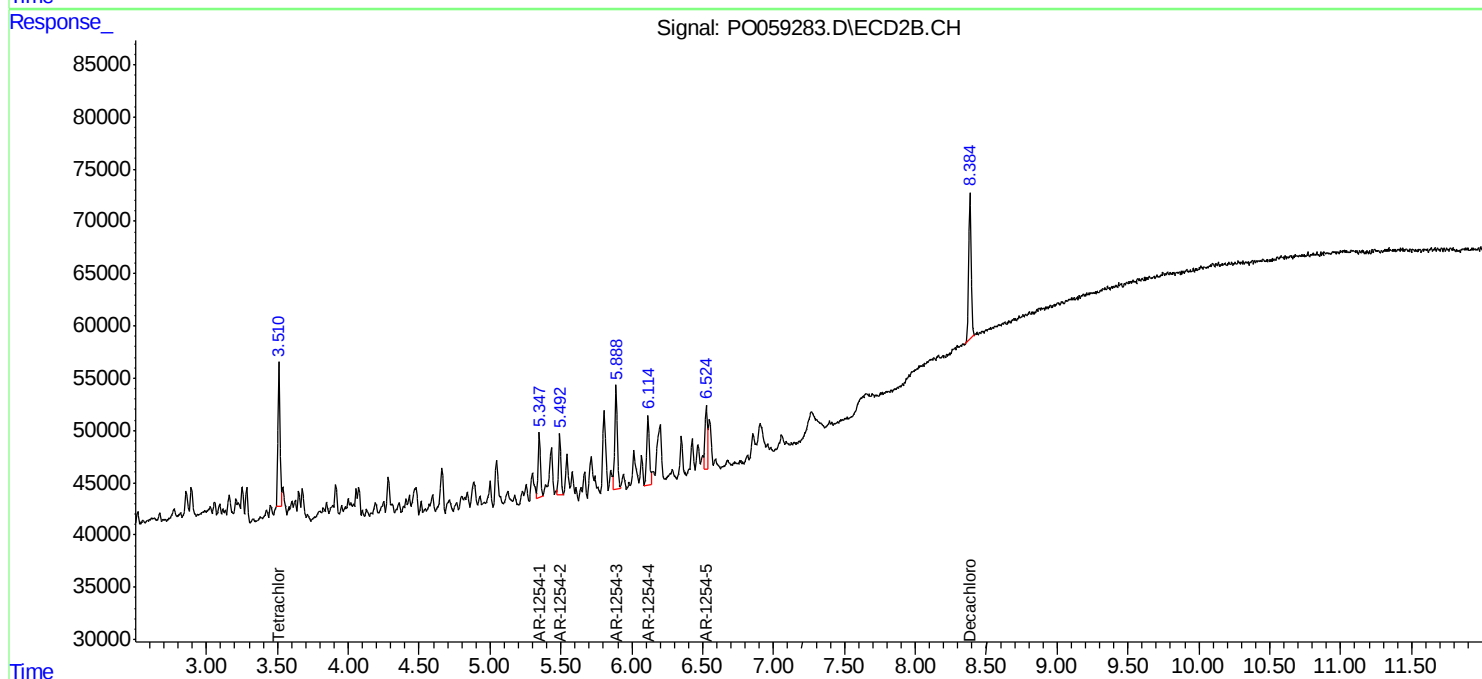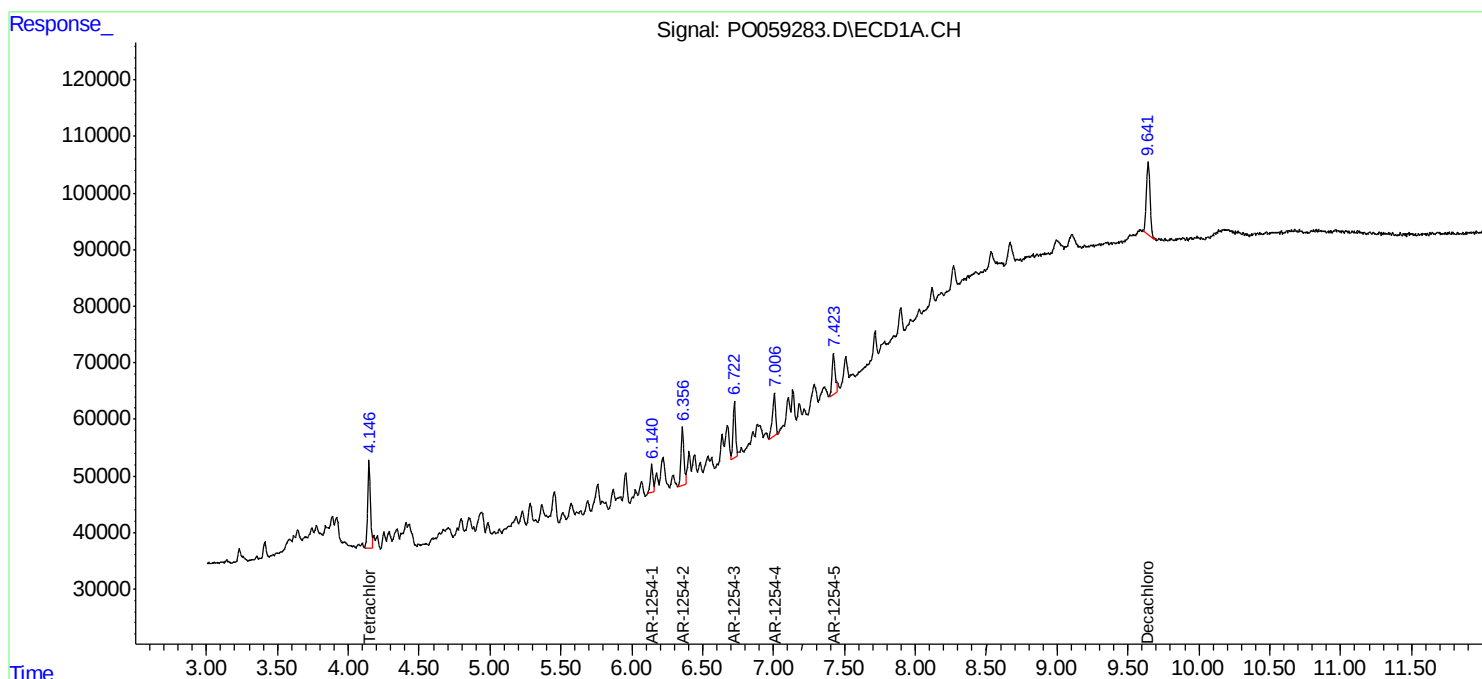

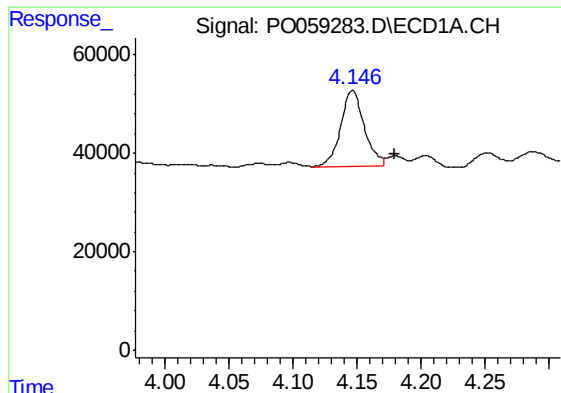


#1 Tetrachloro-m-xylene

R.T.: 4.146 min
Delta R.T.: -0.033 min
Response: 200673
Conc: 4.75 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-45


Manual Integrations
APPROVED

Ankita
8/16/2019 2:37:40 PM

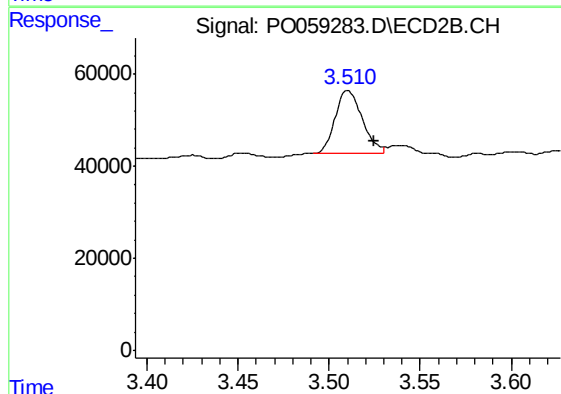


#1 Tetrachloro-m-xylene

R.T.: 3.510 min
Delta R.T.: -0.015 min
Response: 143517
Conc: 3.59 ng/ml m

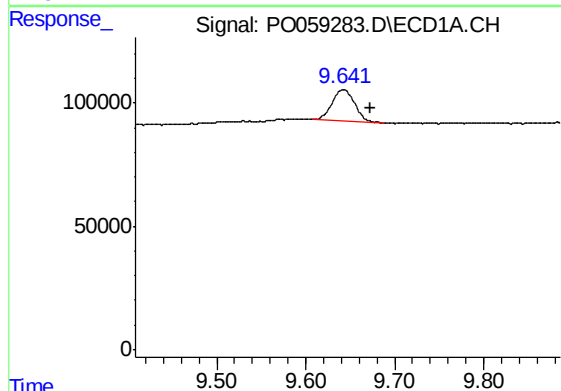


#2 Decachlorobiphenyl

R.T.: 9.641 min
Delta R.T.: -0.031 min
Response: 225583
Conc: 4.17 ng/ml m

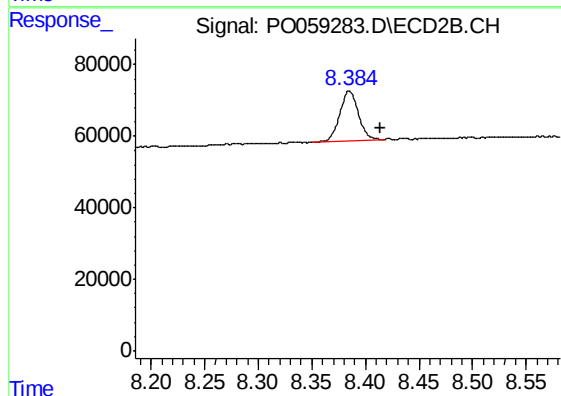

#2 Decachlorobiphenyl

R.T.: 8.385 min
Delta R.T.: -0.029 min
Response: 168433
Conc: 4.27 ng/ml

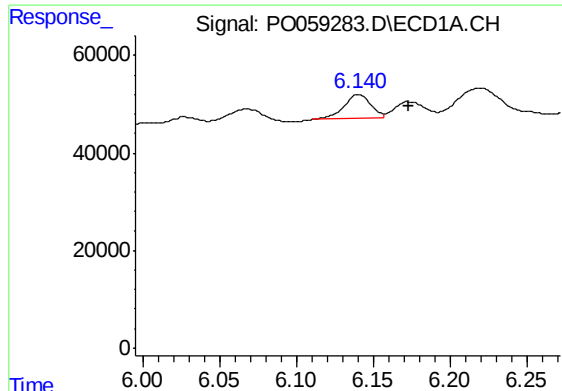


#26 AR-1254-1

R.T.: 6.140 min
Delta R.T.: -0.034 min
Response: 59197
Conc: 25.07 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-45


Manual Integrations
APPROVED

Ankita
8/16/2019 2:37:40 PM

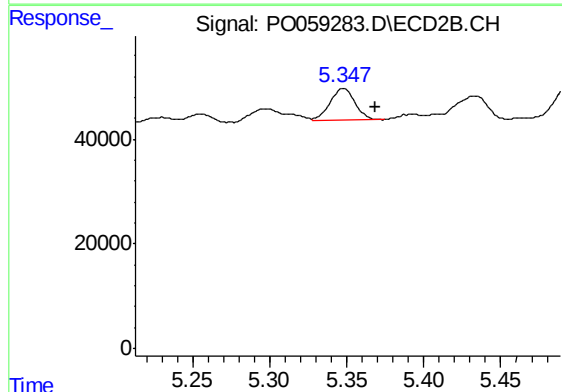


#26 AR-1254-1

R.T.: 5.348 min
Delta R.T.: -0.021 min
Response: 68289
Conc: 26.36 ng/ml

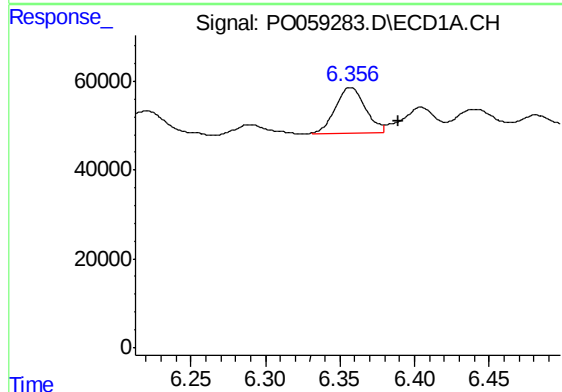


#27 AR-1254-2

R.T.: 6.356 min
Delta R.T.: -0.032 min
Response: 144688
Conc: 37.54 ng/ml m

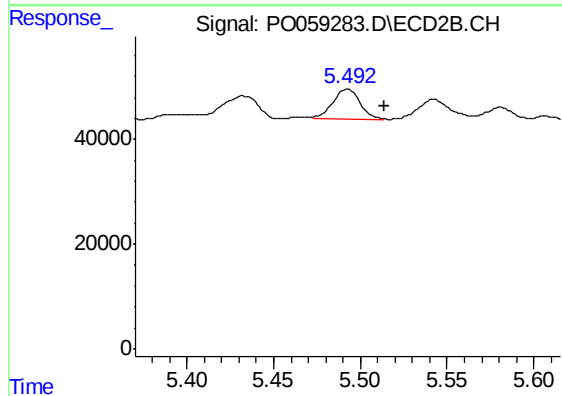

#27 AR-1254-2

R.T.: 5.492 min
Delta R.T.: -0.021 min
Response: 63120
Conc: 27.57 ng/ml m

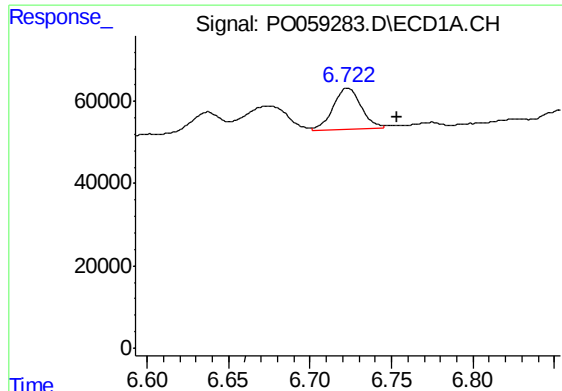


#28 AR-1254-3

R.T.: 6.722 min
Delta R.T.: -0.031 min
Response: 121575
Conc: 30.02 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-45


Manual Integrations
APPROVED

Ankita
8/16/2019 2:37:40 PM

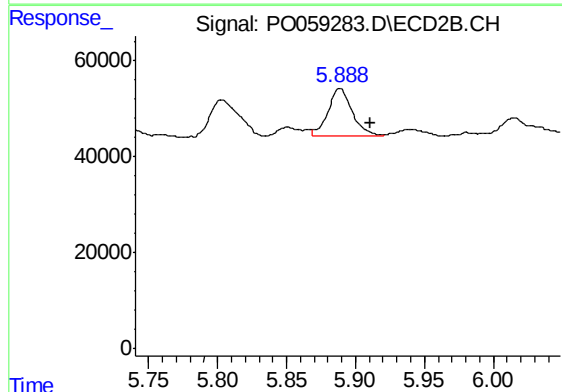


#28 AR-1254-3

R.T.: 5.889 min
Delta R.T.: -0.022 min
Response: 120739
Conc: 32.82 ng/ml

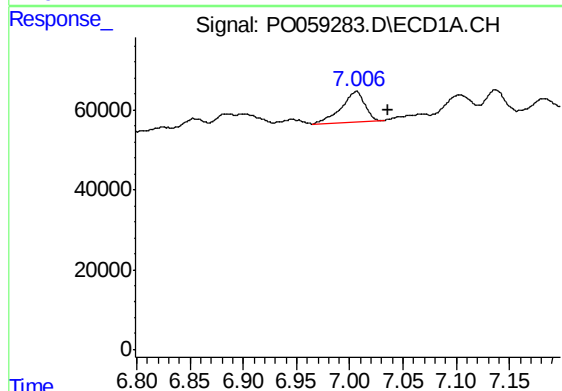


#29 AR-1254-4

R.T.: 7.006 min
Delta R.T.: -0.030 min
Response: 115732
Conc: 32.14 ng/ml

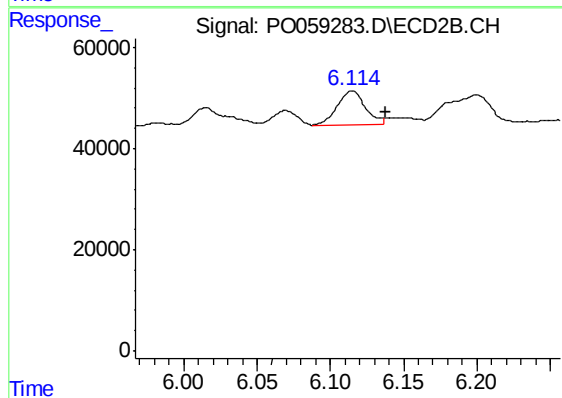

#29 AR-1254-4

R.T.: 6.115 min
Delta R.T.: -0.023 min
Response: 87800
Conc: 37.76 ng/ml

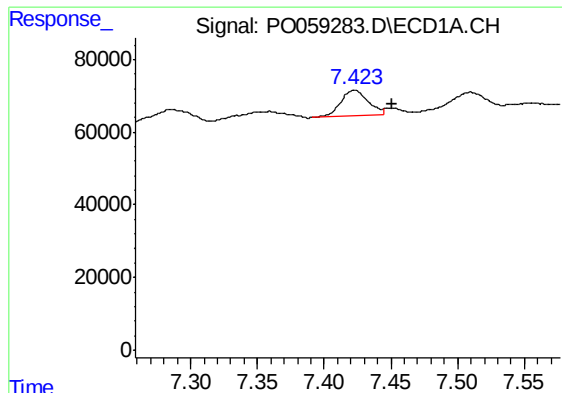


#30 AR-1254-5

R.T.: 7.423 min
Delta R.T.: -0.028 min
Response: 102512
Conc: 28.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-45

Manual Integrations
APPROVED

Ankita
8/16/2019 2:37:40 PM

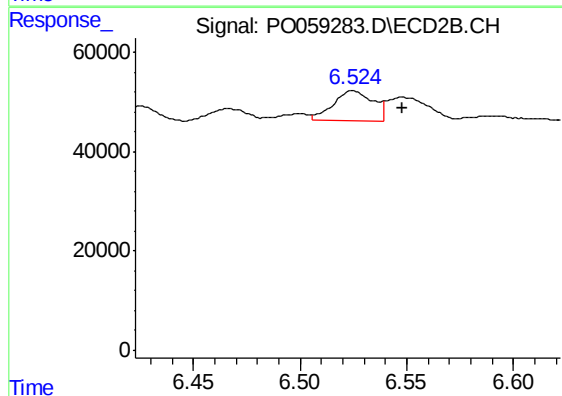

#30 AR-1254-5

R.T.: 6.524 min
Delta R.T.: -0.024 min
Response: 79917
Conc: 23.17 ng/ml m