

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081419\
 Data File : P0059297.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Aug 2019 19:51
 Operator : SM/SJ
 Sample : K4264-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 REACTOR-3-G1-G4-(0-2)

Manual Integrations
 APPROVED

Ankita
 8/16/2019 2:38:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 09:23:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 14 09:07:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.144	3.511	987050	661990	23.388m	16.570 #
2) SA Decachlor...	9.643	8.385	889735	654653	16.429	16.585

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081419\
Data File : PO059297.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2019 19:51
Operator : SM/SJ
Sample : K4264-11
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
REACTOR-3-G1-G4-(0-2)


Manual Integrations
APPROVED

Ankita
8/16/2019 2:38:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 09:23:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 14 09:07:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

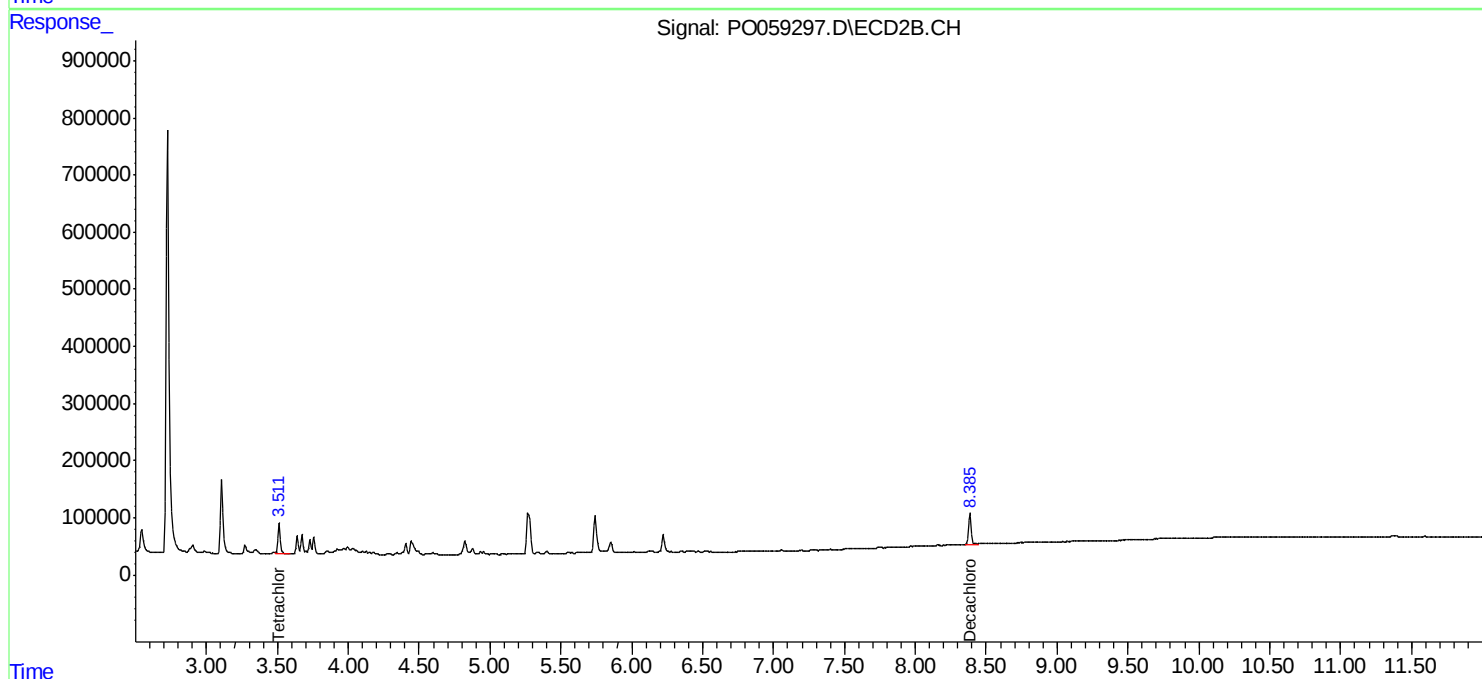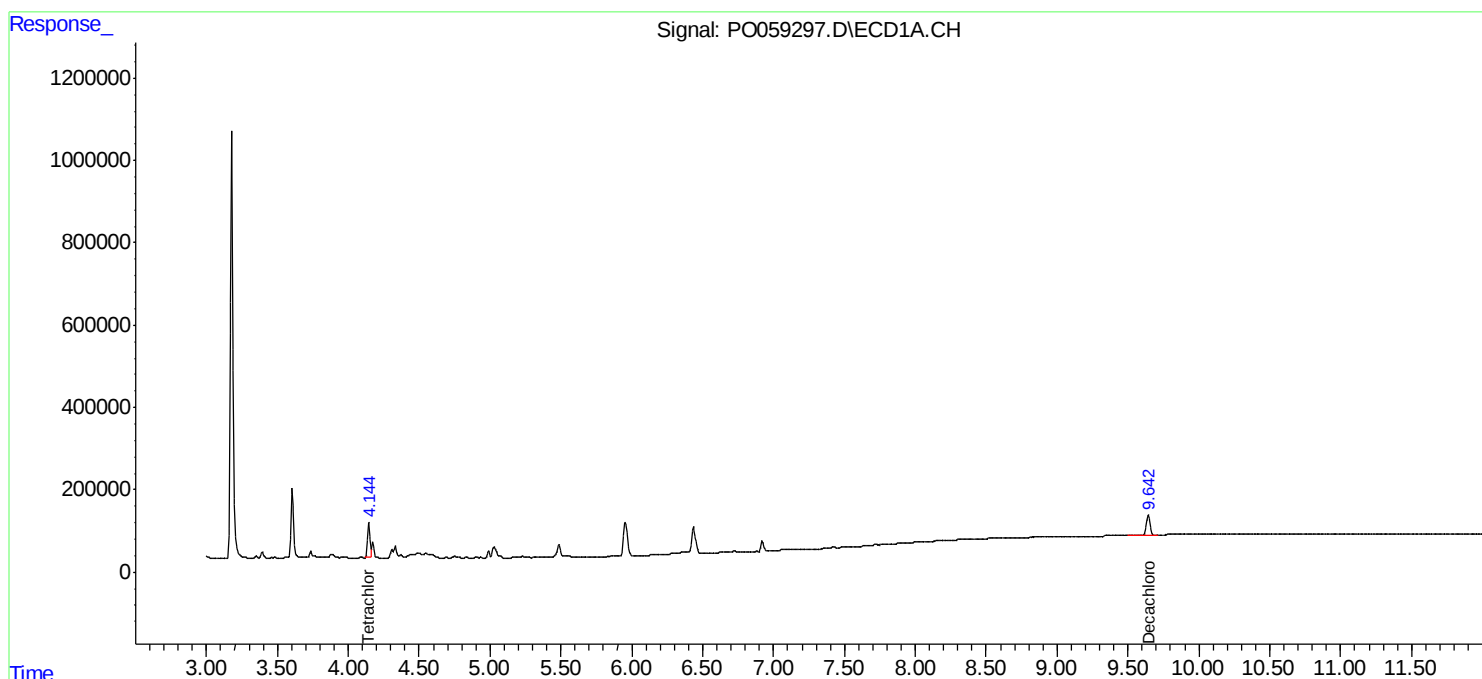

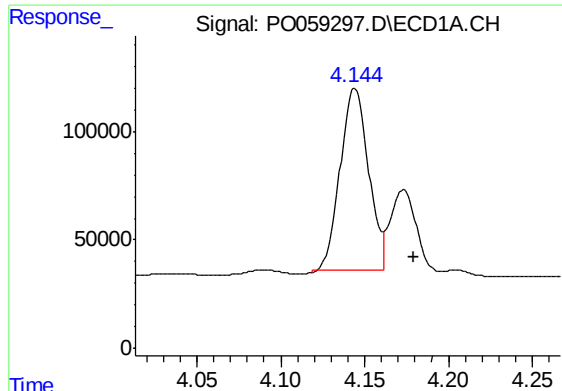


#1 Tetrachloro-m-xylene

R.T.: 4.144 min
Delta R.T.: -0.035 min
Response: 987050
Conc: 23.39 ng/ml m

Instrument :
ECD_O
ClientSampleId :
REACTOR-3-G1-G4-(0-2)


Manual Integrations
APPROVED

Ankita
8/16/2019 2:38:06 PM

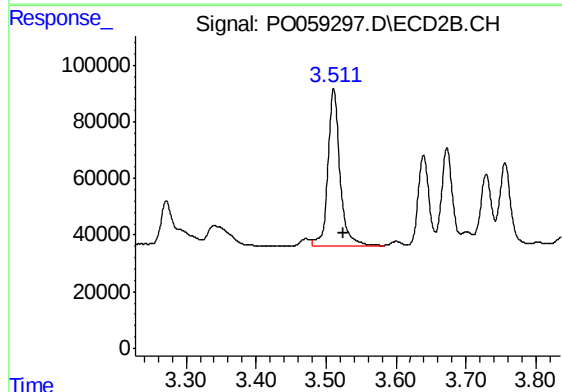


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: -0.014 min
Response: 661990
Conc: 16.57 ng/ml

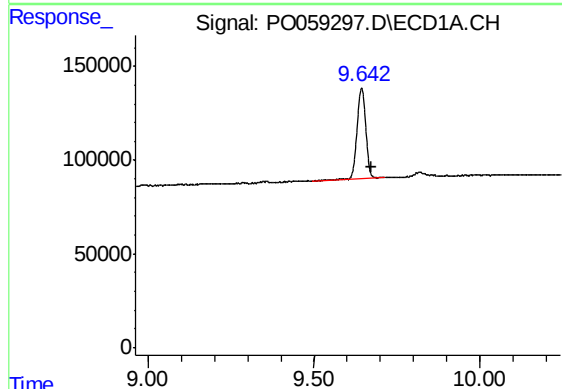

#2 Decachlorobiphenyl

R.T.: 9.643 min
Delta R.T.: -0.029 min
Response: 889735
Conc: 16.43 ng/ml

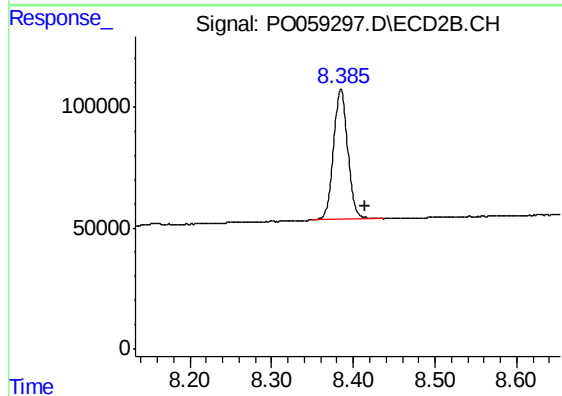

#2 Decachlorobiphenyl

R.T.: 8.385 min
Delta R.T.: -0.029 min
Response: 654653
Conc: 16.58 ng/ml