

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081419\
 Data File : P0059301.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Aug 2019 20:56
 Operator : SM/SJ
 Sample : K4265-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 REACTOR-4-B-(0-3.4)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 09:25:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 14 09:07:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.146	3.511	856215	772996	20.288	19.349
2) SA Decachlor...	9.643	8.384	772649	547370	14.267	13.867

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081419\
Data File : P0059301.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2019 20:56
Operator : SM/SJ
Sample : K4265-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
REACTOR-4-B-(0-3.4)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 09:25:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 14 09:07:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

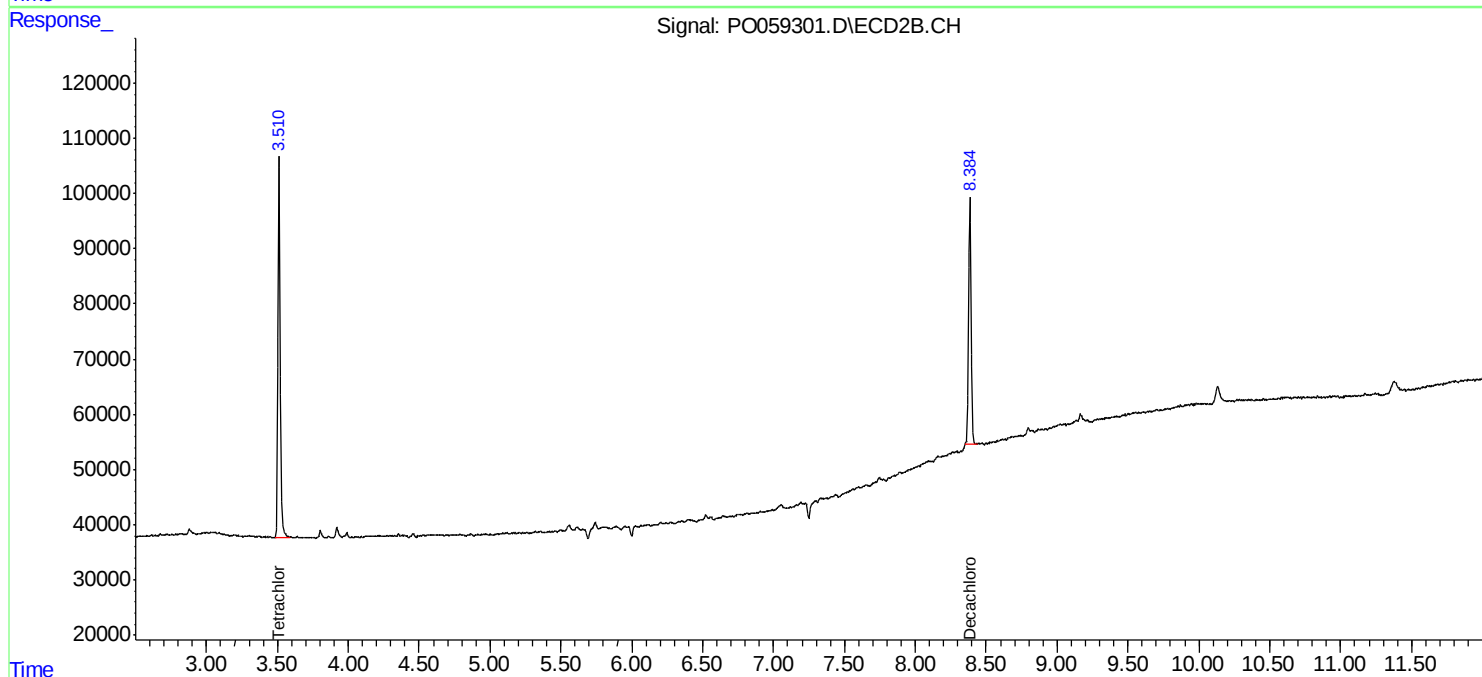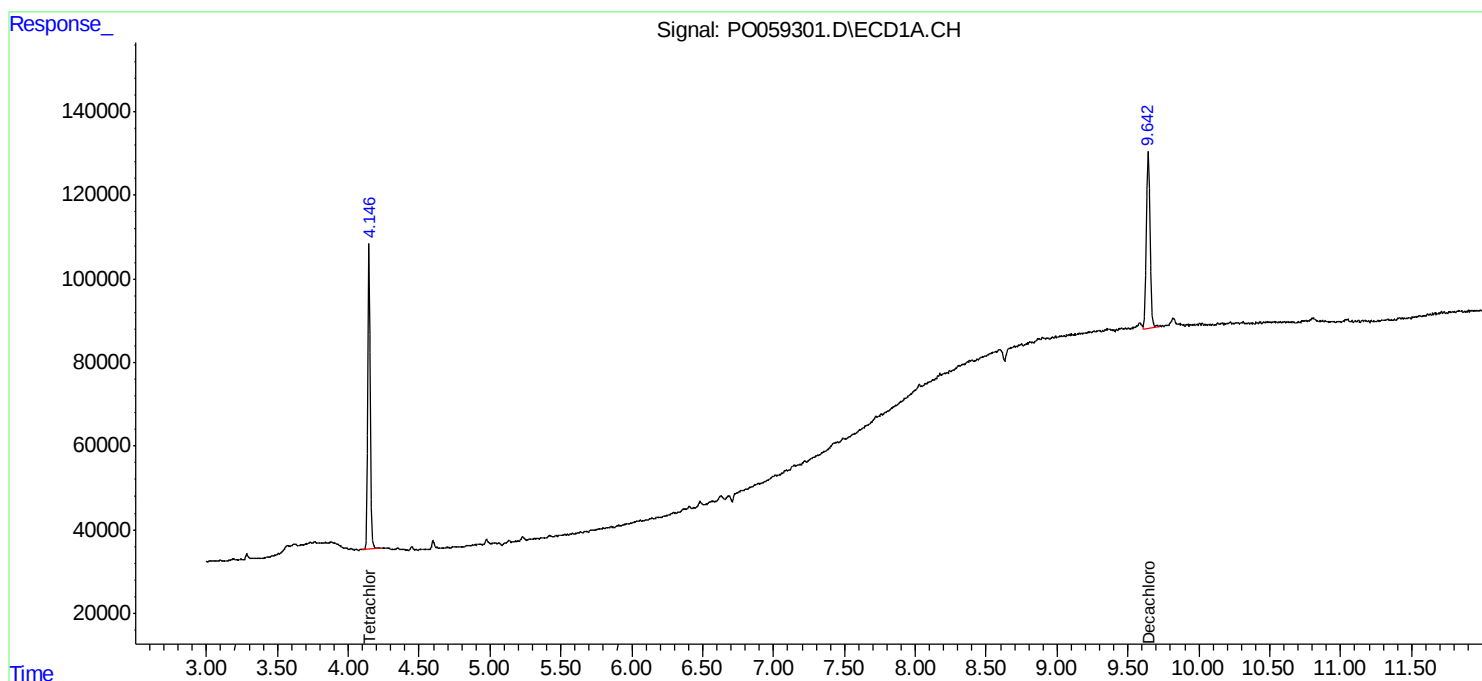


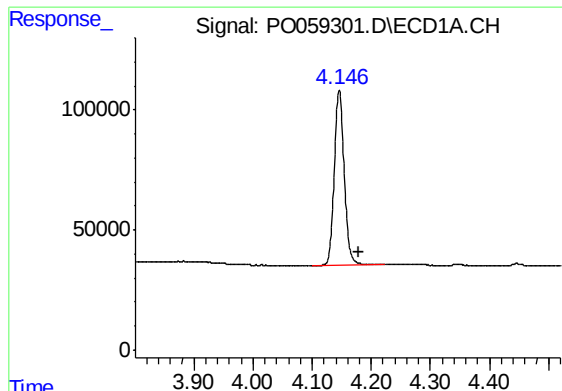

#1 Tetrachloro-m-xylene


R.T.: 4.146 min
Delta R.T.: -0.033 min
Response: 856215
Conc: 20.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
REACTOR-4-B-(0-3.4)

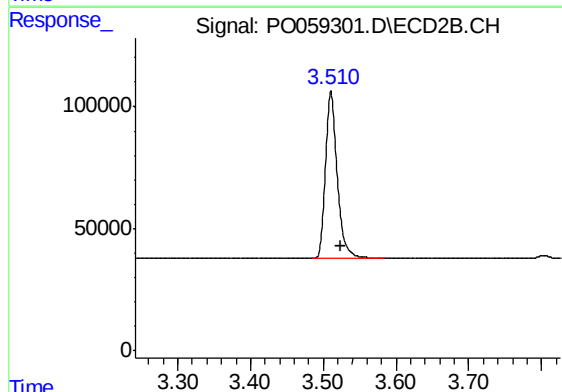


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: -0.014 min
Response: 772996
Conc: 19.35 ng/ml

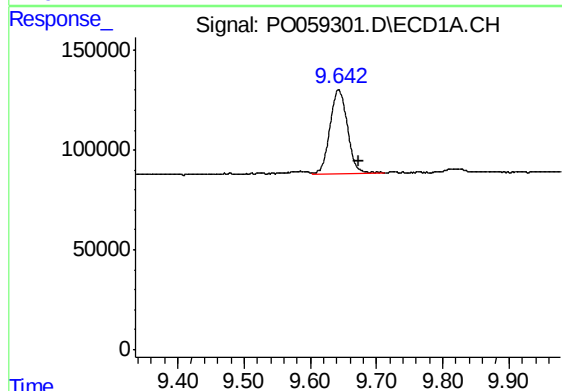

#2 Decachlorobiphenyl

R.T.: 9.643 min
Delta R.T.: -0.030 min
Response: 772649
Conc: 14.27 ng/ml

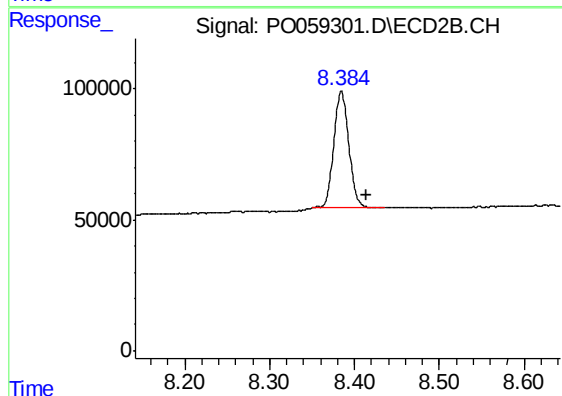

#2 Decachlorobiphenyl

R.T.: 8.384 min
Delta R.T.: -0.030 min
Response: 547370
Conc: 13.87 ng/ml