

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081419\
 Data File : P0059304.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Aug 2019 21:44
 Operator : SM/SJ
 Sample : K4265-20
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 REACTOR-4-A1-A4-(0-1)

Manual Integrations
 APPROVED

Ankita
 8/16/2019 2:38:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 09:27:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 14 09:07:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.145	3.510	939895	882267	22.271	22.084
2) SA Decachlor...	9.641	8.384	1000625	715462	18.477m	18.125

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081419\
Data File : PO059304.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2019 21:44
Operator : SM/SJ
Sample : K4265-20
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
REACTOR-4-A1-A4-(0-1)


Manual Integrations
APPROVED

Ankita
8/16/2019 2:38:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 09:27:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 14 09:07:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

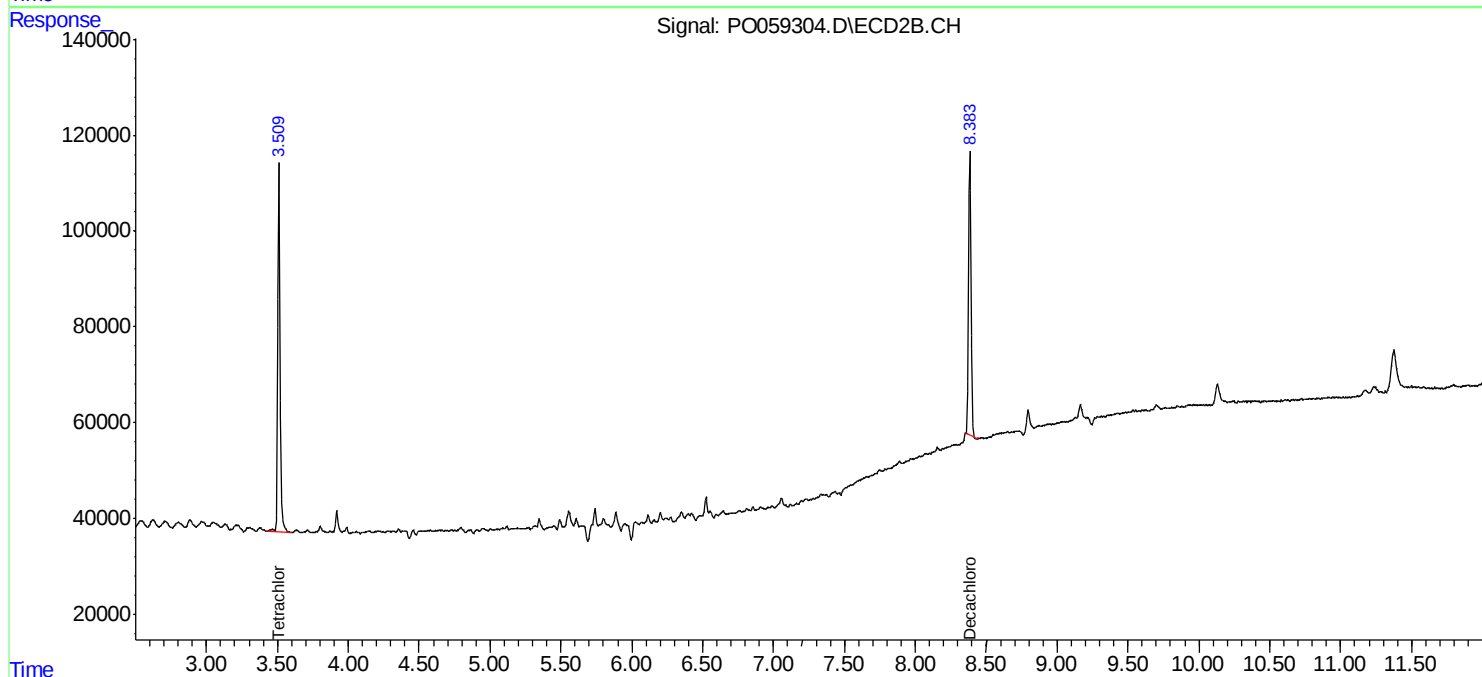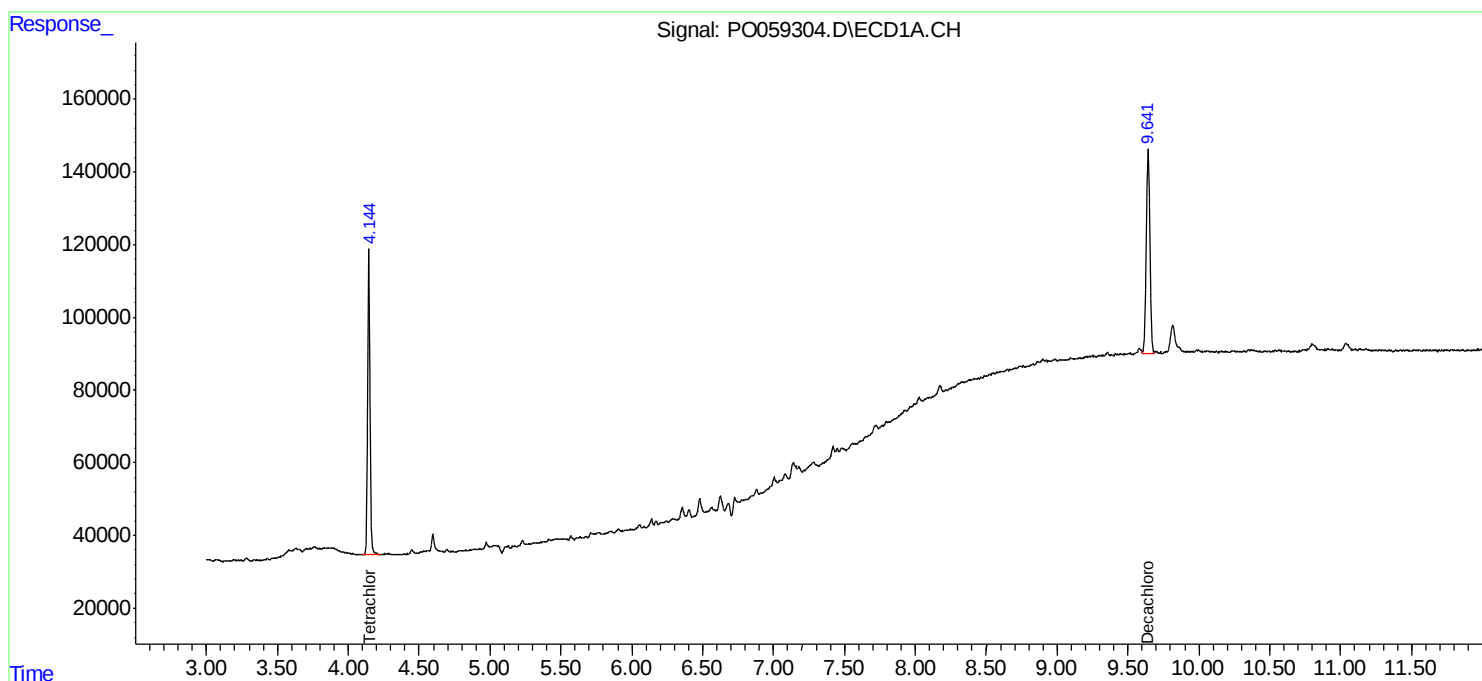

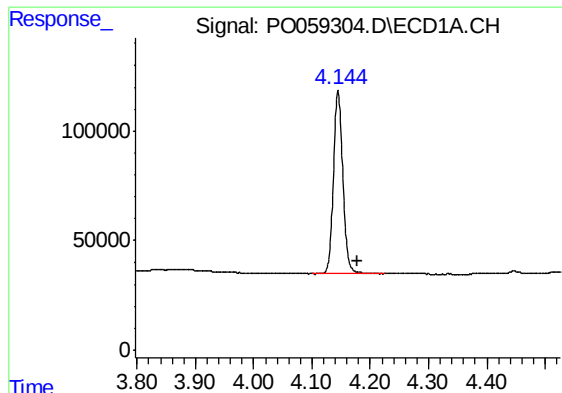


#1 Tetrachloro-m-xylene

R.T.: 4.145 min
Delta R.T.: -0.034 min
Response: 939895
Conc: 22.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
REACTOR-4-A1-A4-(0-1)


Manual Integrations
APPROVED

Ankita
8/16/2019 2:38:22 PM

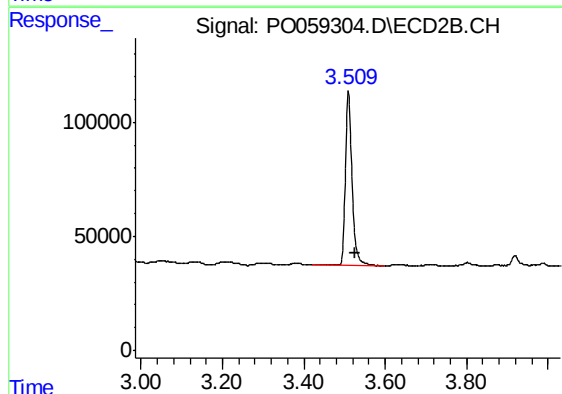


#1 Tetrachloro-m-xylene

R.T.: 3.510 min
Delta R.T.: -0.015 min
Response: 882267
Conc: 22.08 ng/ml

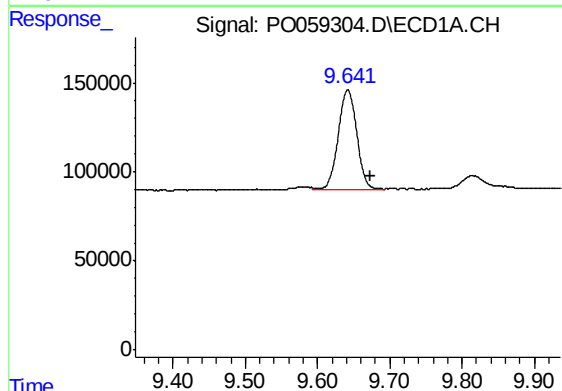

#2 Decachlorobiphenyl

R.T.: 9.641 min
Delta R.T.: -0.031 min
Response: 1000625
Conc: 18.48 ng/ml m

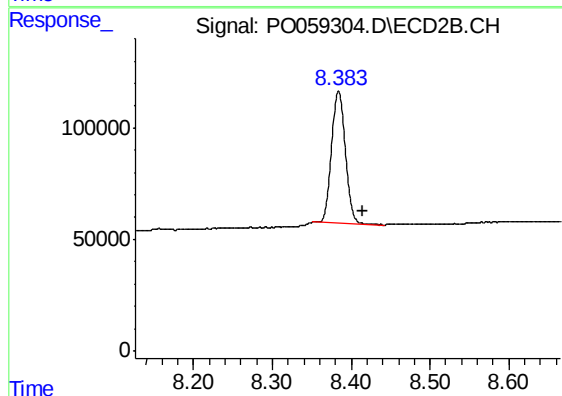

#2 Decachlorobiphenyl

R.T.: 8.384 min
Delta R.T.: -0.030 min
Response: 715462
Conc: 18.13 ng/ml