

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081420\
 Data File : P0070569.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Aug 2020 12:49
 Operator : DD\AJ
 Sample : L3502-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-01-081320

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 15:43:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.367	3.552	1968433	1185709	29.768	26.912
2) SA Decachlor...	9.994	8.743	2046540	1184210	23.901	21.334

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081420\
Data File : P0070569.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2020 12:49
Operator : DD\AJ
Sample : L3502-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-01-081320

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 15:43:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

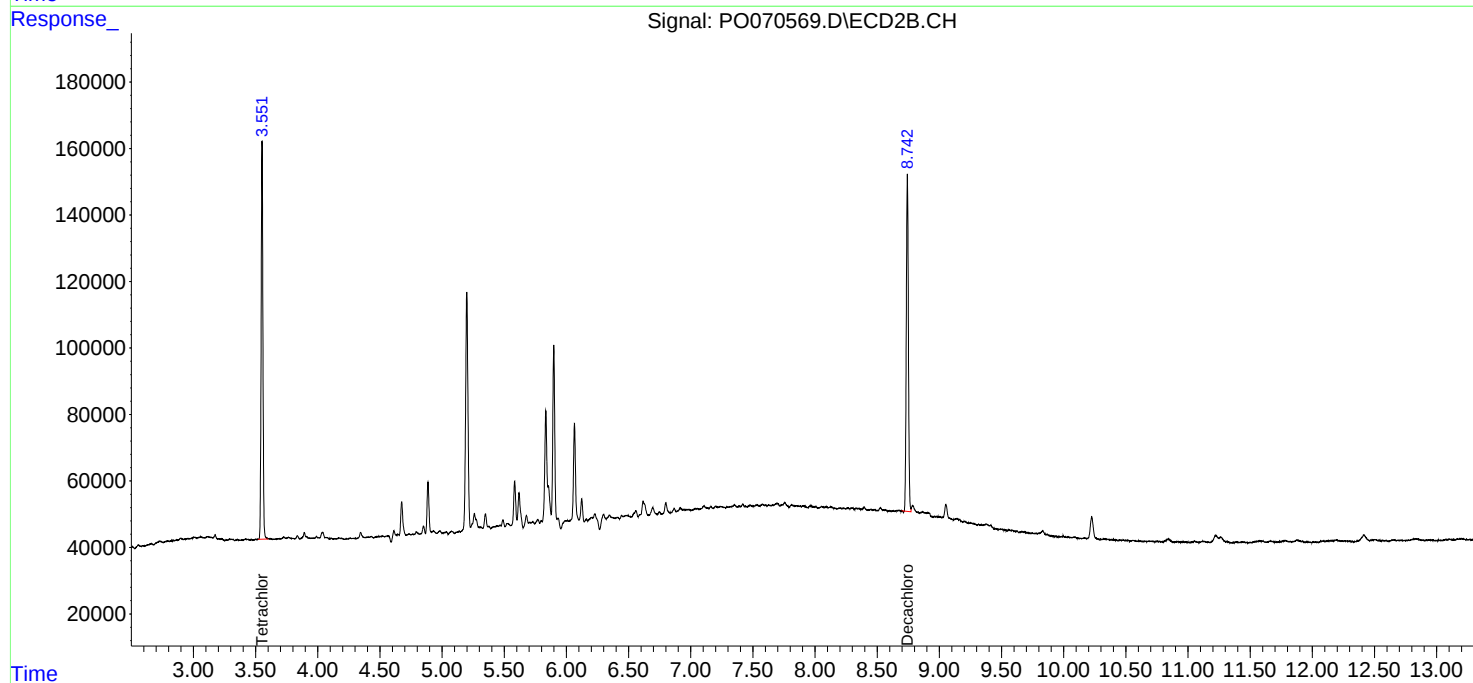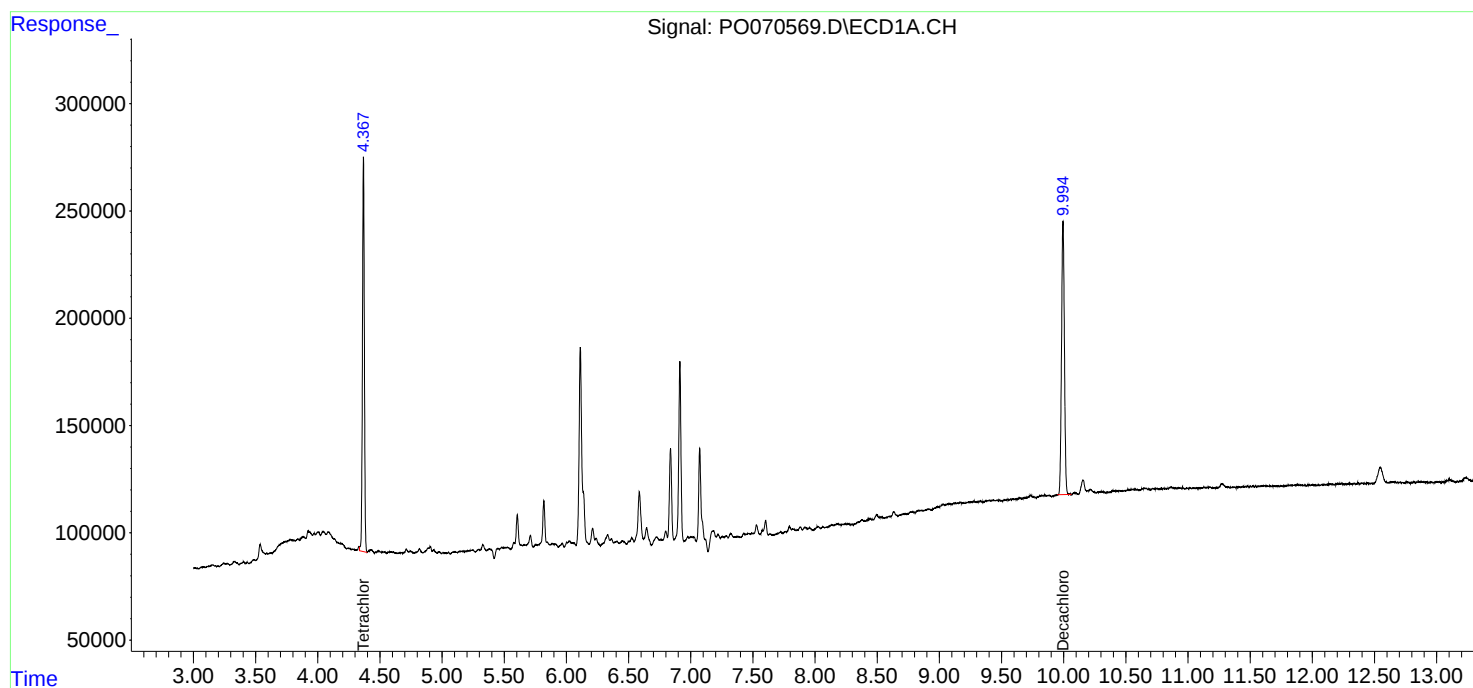


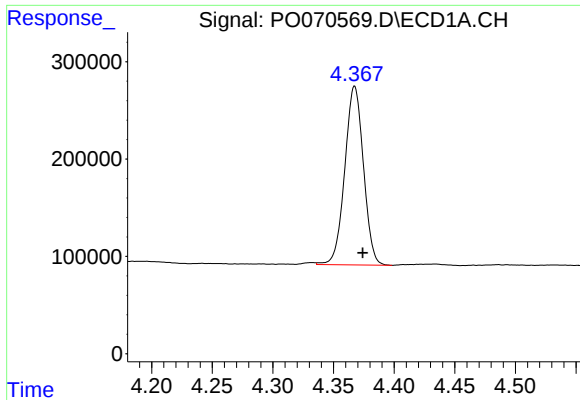

#1 Tetrachloro-m-xylene


R.T.: 4.367 min
Delta R.T.: -0.007 min
Response: 1968433
Conc: 29.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-01-081320

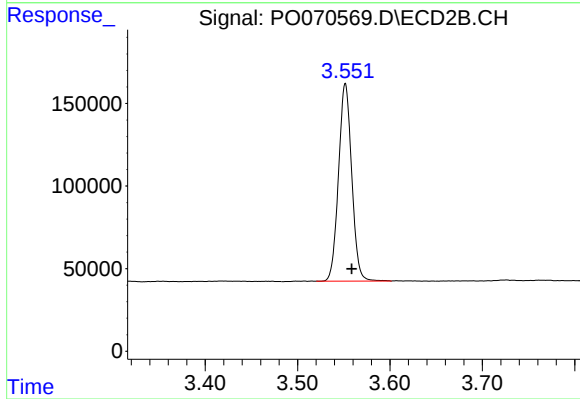


#1 Tetrachloro-m-xylene

R.T.: 3.552 min
Delta R.T.: -0.007 min
Response: 1185709
Conc: 26.91 ng/ml

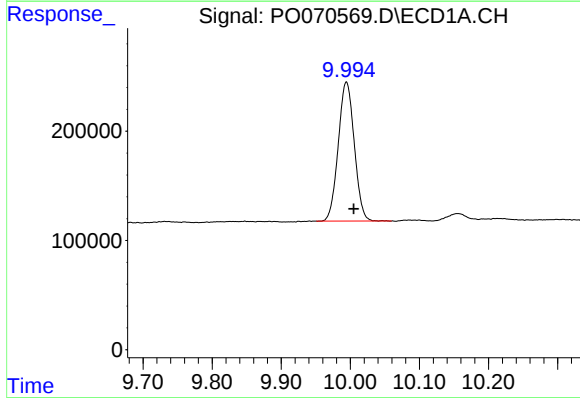

#2 Decachlorobiphenyl

R.T.: 9.994 min
Delta R.T.: -0.011 min
Response: 2046540
Conc: 23.90 ng/ml

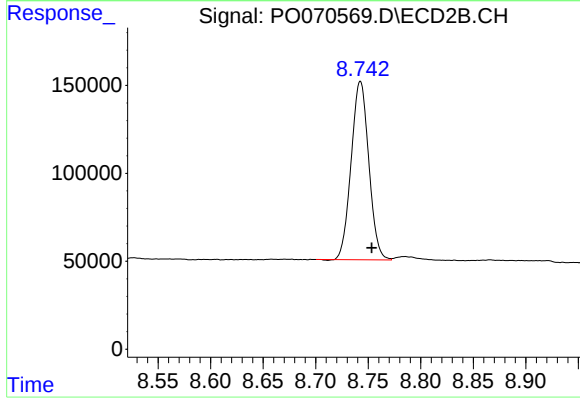

#2 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: -0.011 min
Response: 1184210
Conc: 21.33 ng/ml