

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0081518\
Data File : P0048119.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Aug 2018 15:03
Operator : SM/SJ
Sample : J4471-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Sohil
8/16/2018 5:17:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:24:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.391	3.634	4942113	6820557	24.478	27.758
2) SA Decachlor...	10.078	8.617	3678200	3739244	22.552	23.788m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0081518\
Data File : P0048119.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Aug 2018 15:03
Operator : SM/SJ
Sample : J4471-05
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Sohil
8/16/2018 5:17:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:24:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

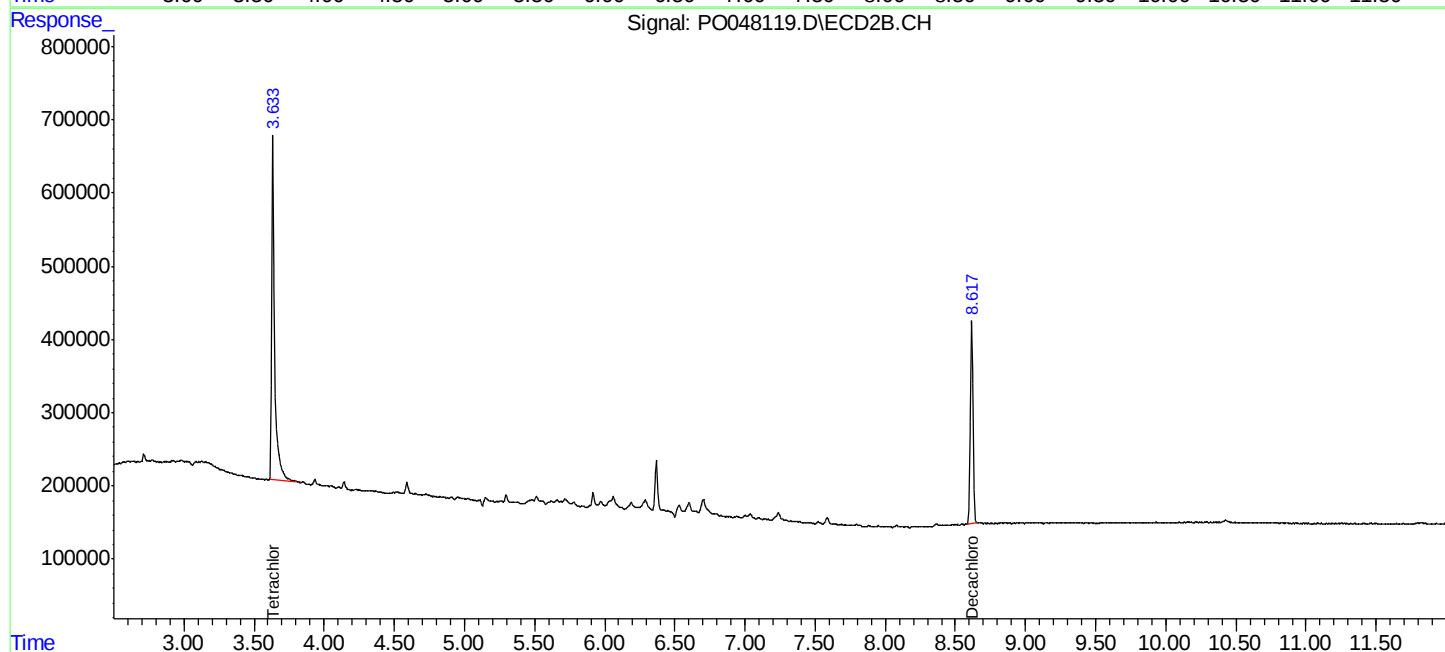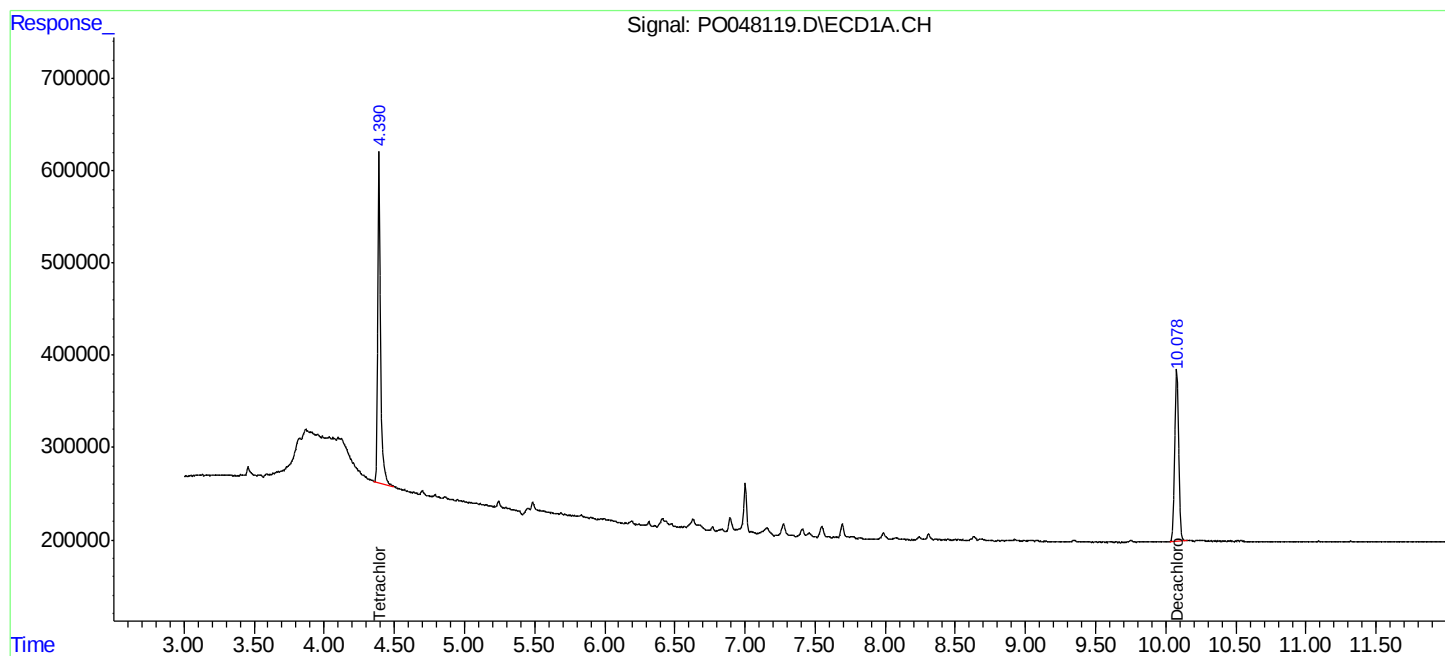

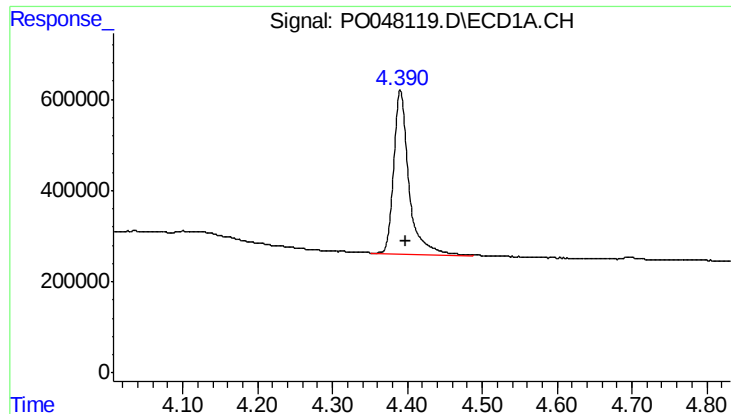


#1 Tetrachloro-m-xylene

R.T.: 4.391 min
Delta R.T.: -0.007 min
Response: 4942113
Conc: 24.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Sohil
8/16/2018 5:17:37 PM

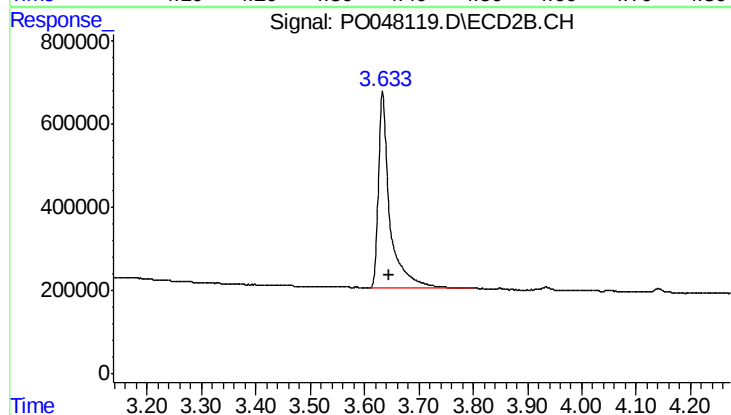


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.012 min
Response: 6820557
Conc: 27.76 ng/ml

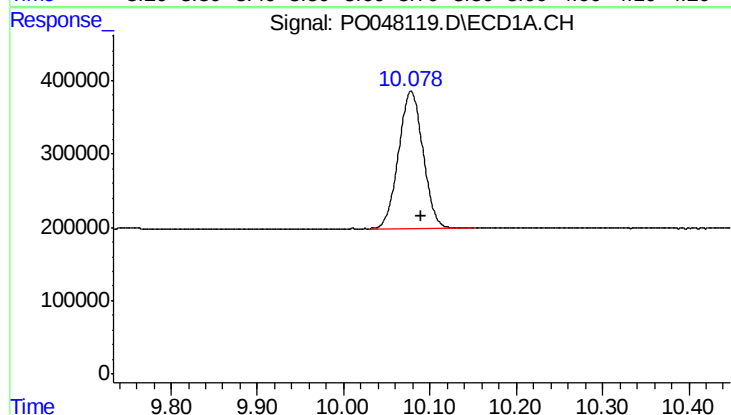

#2 Decachlorobiphenyl

R.T.: 10.078 min
Delta R.T.: -0.011 min
Response: 3678200
Conc: 22.55 ng/ml

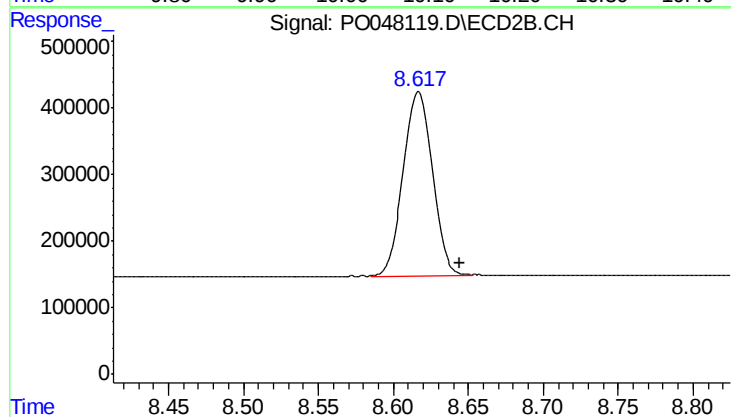

#2 Decachlorobiphenyl

R.T.: 8.617 min
Delta R.T.: -0.028 min
Response: 3739244
Conc: 23.79 ng/ml m