

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0081518\
 Data File : P0048120.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Aug 2018 15:19
 Operator : SM/SJ
 Sample : J4471-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Sohil
 8/16/2018 5:17:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:25:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.391	3.634	4502986	6314057	22.303	25.697
2) SA Decachlor...	10.079	8.617	3625254	3731171	22.227	23.736m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0081518\
Data File : P0048120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Aug 2018 15:19
Operator : SM/SJ
Sample : J4471-09
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Sohil
8/16/2018 5:17:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:25:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

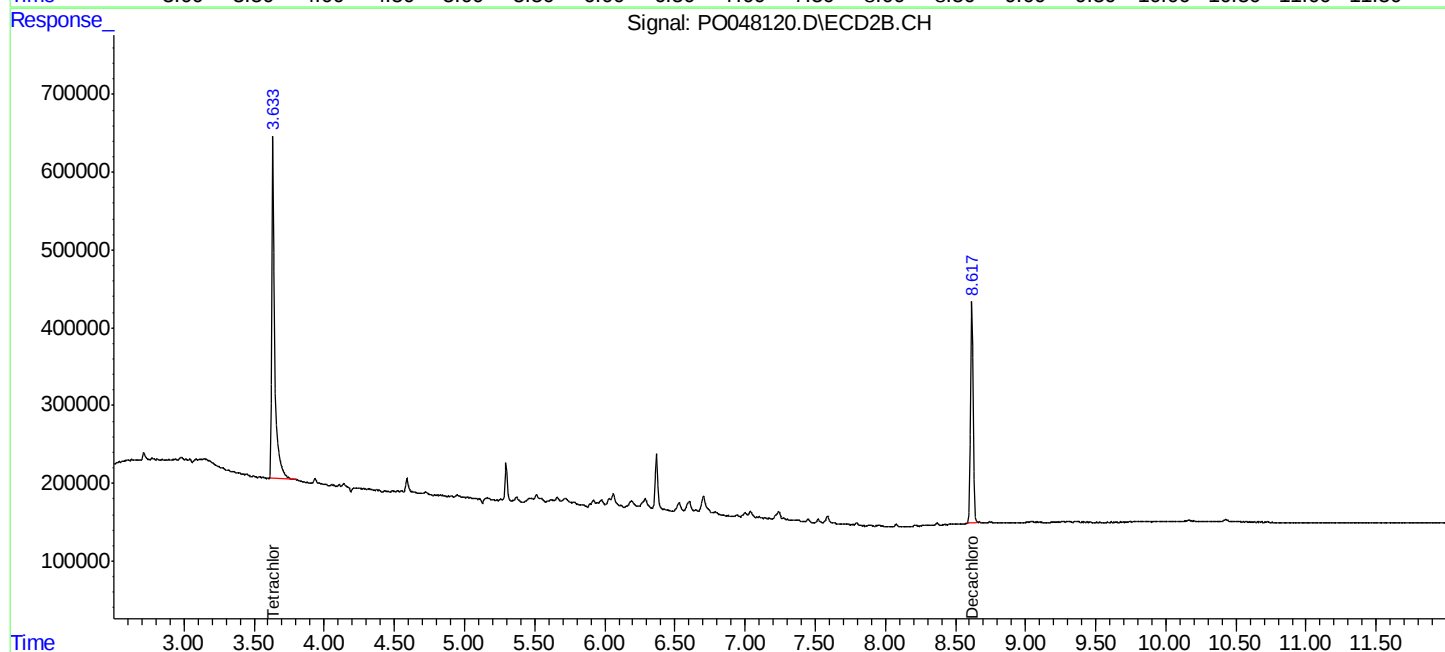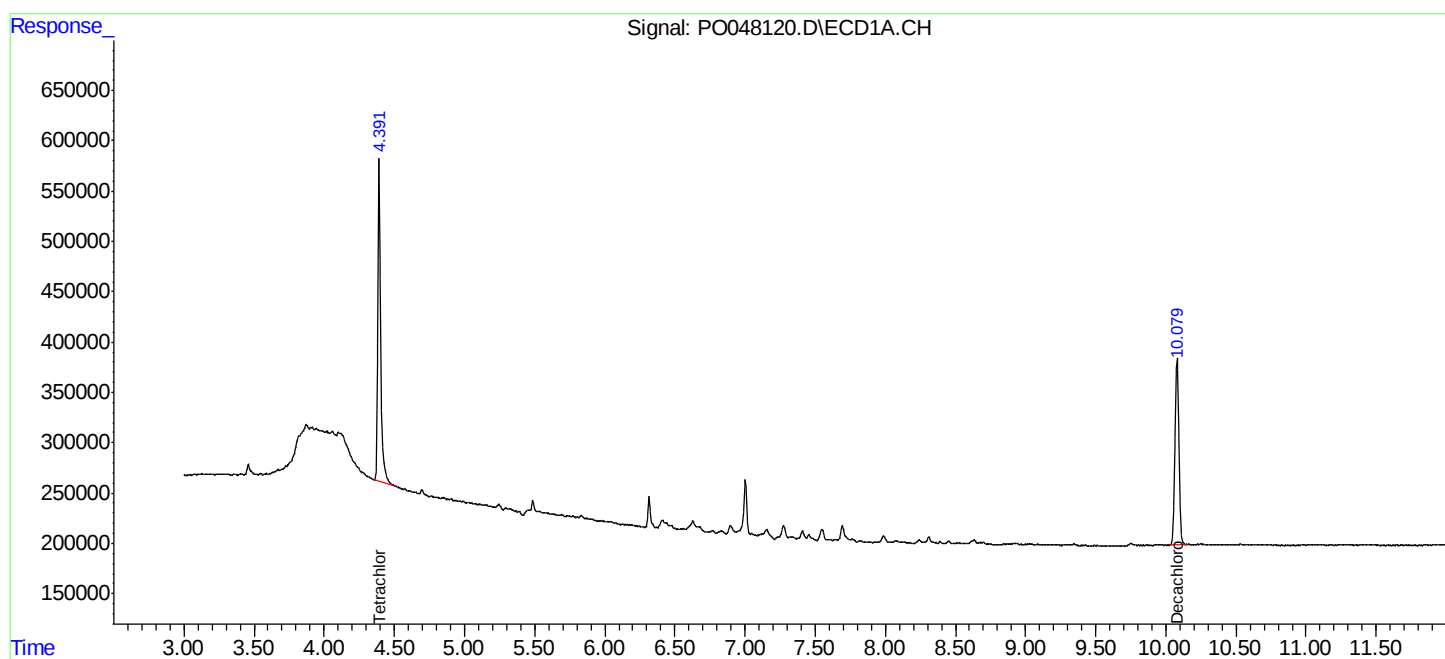

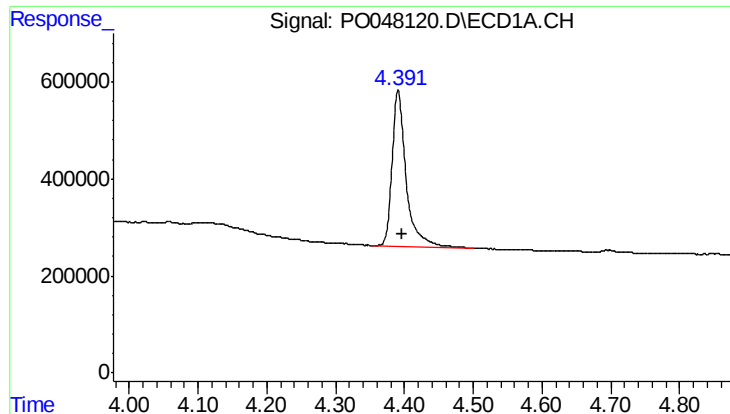


#1 Tetrachloro-m-xylene

R.T.: 4.391 min
Delta R.T.: -0.006 min
Response: 4502986
Conc: 22.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Sohil
8/16/2018 5:17:37 PM

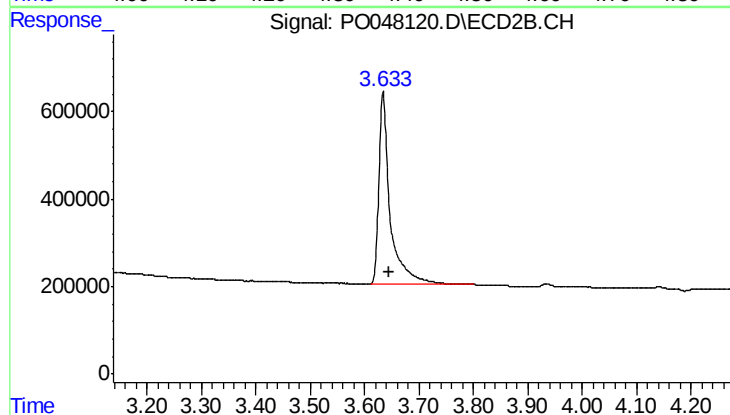


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.011 min
Response: 6314057
Conc: 25.70 ng/ml

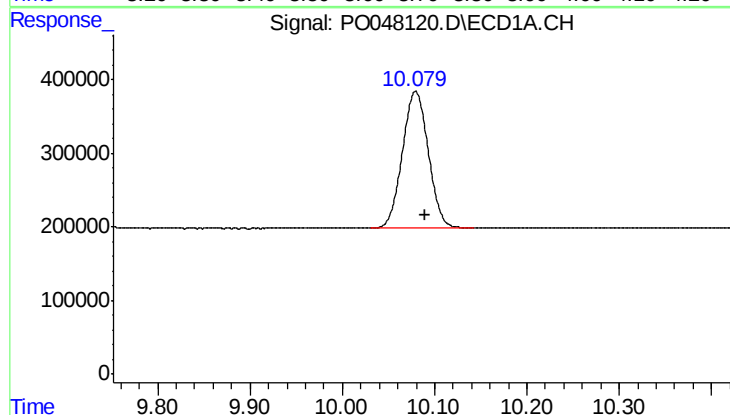

#2 Decachlorobiphenyl

R.T.: 10.079 min
Delta R.T.: -0.010 min
Response: 3625254
Conc: 22.23 ng/ml

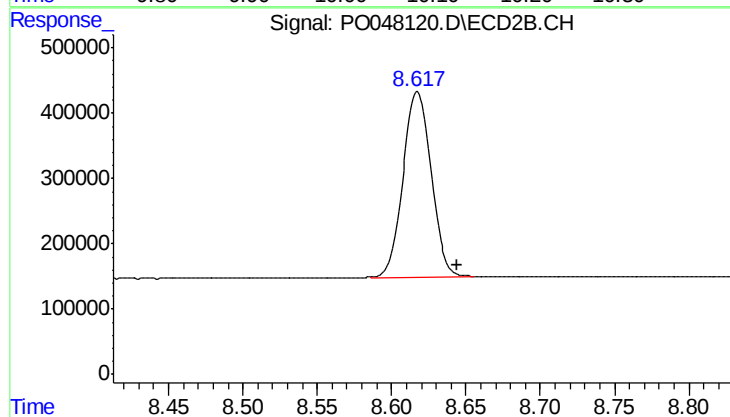

#2 Decachlorobiphenyl

R.T.: 8.617 min
Delta R.T.: -0.028 min
Response: 3731171
Conc: 23.74 ng/ml m