

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081519\
 Data File : P0059351.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Aug 2019 17:14
 Operator : SM/SJ
 Sample : K4356-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:31:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 14 09:07:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.148	3.509	598007	526356	14.170	13.175
2) SA Decachlor...	9.642	8.384	268110	245141	4.951	6.210 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081519\
Data File : P0059351.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Aug 2019 17:14
Operator : SM/SJ
Sample : K4356-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:31:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 14 09:07:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

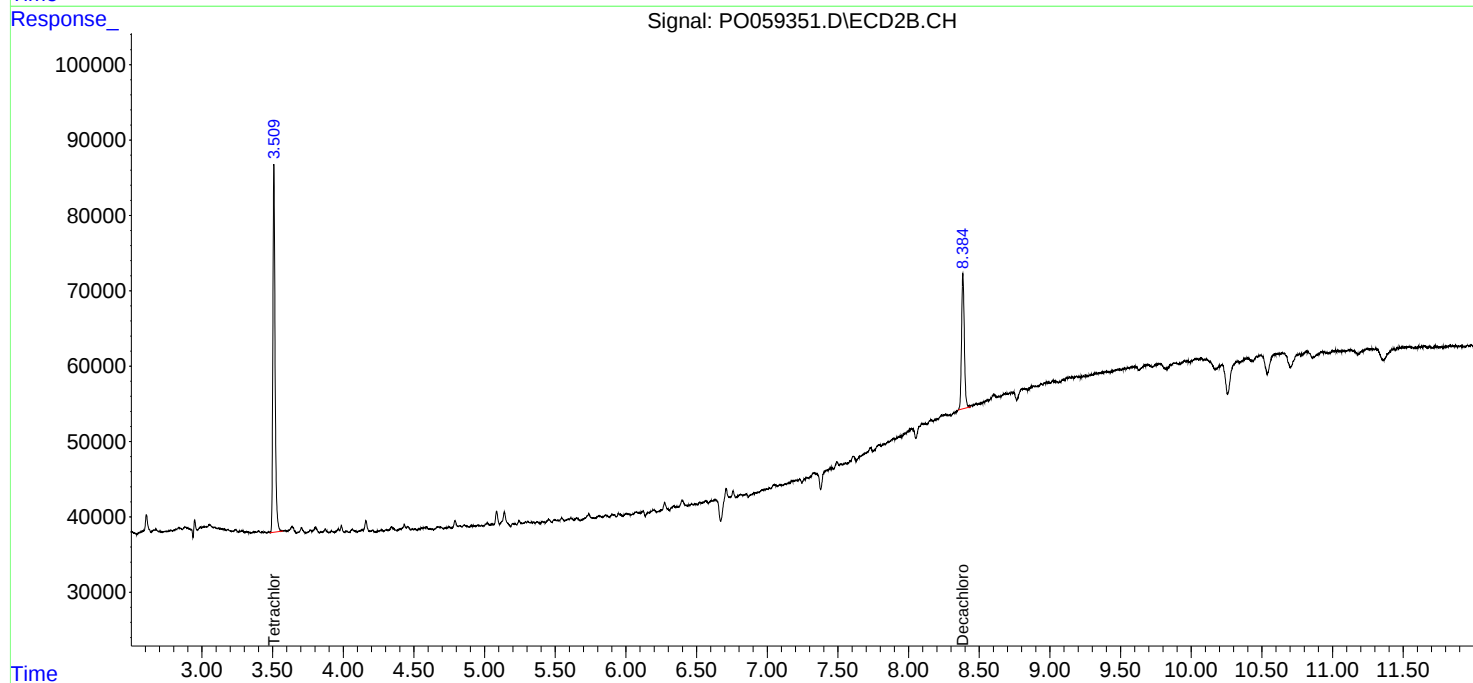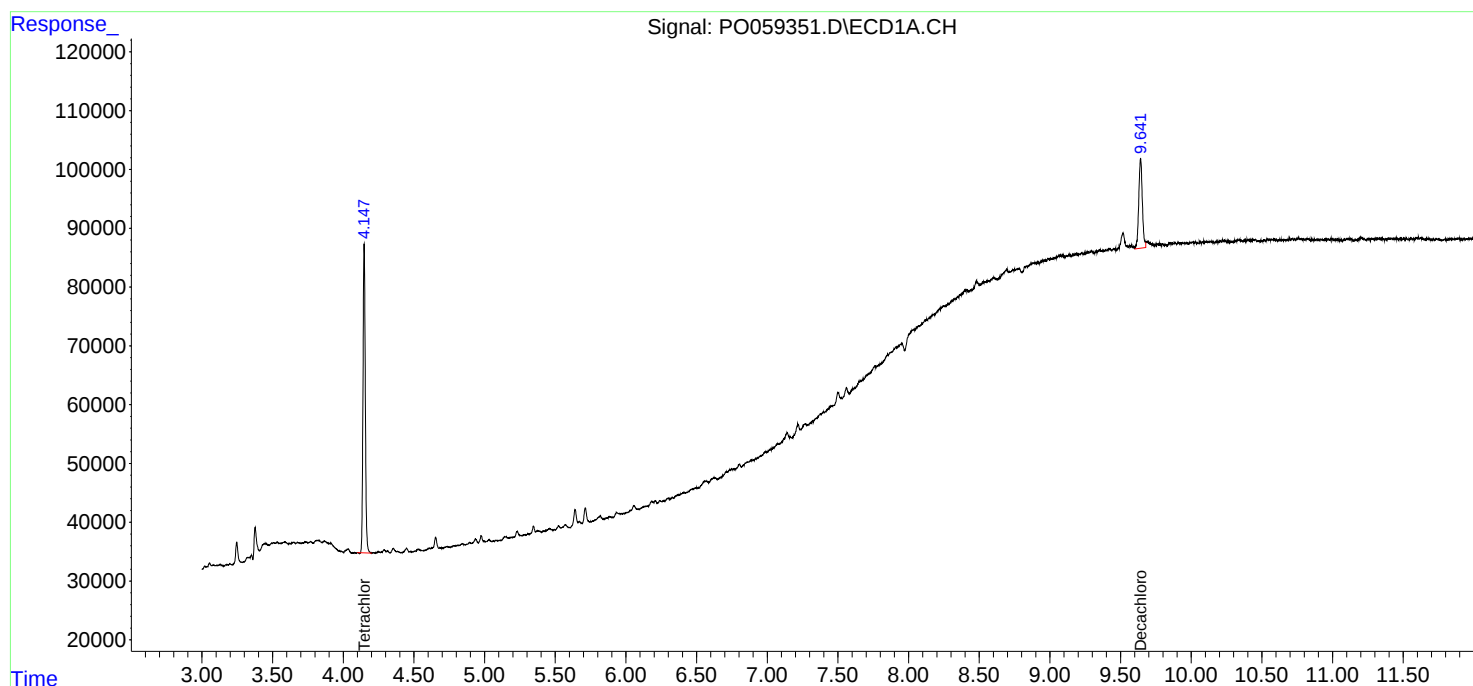


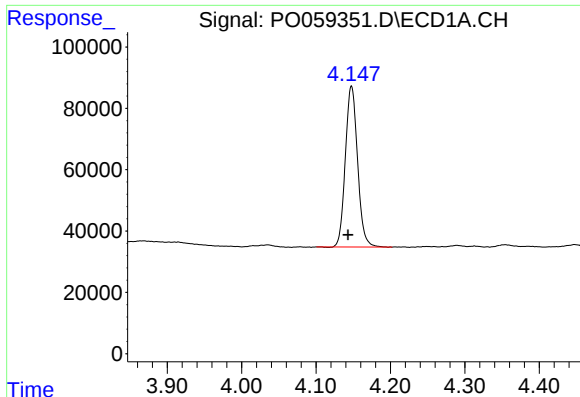

#1 Tetrachloro-m-xylene


R.T.: 4.148 min
Delta R.T.: 0.005 min
Response: 598007
Conc: 14.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4

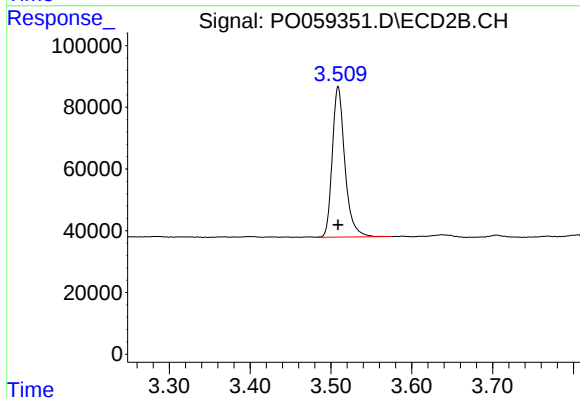


#1 Tetrachloro-m-xylene

R.T.: 3.509 min
Delta R.T.: 0.000 min
Response: 526356
Conc: 13.18 ng/ml

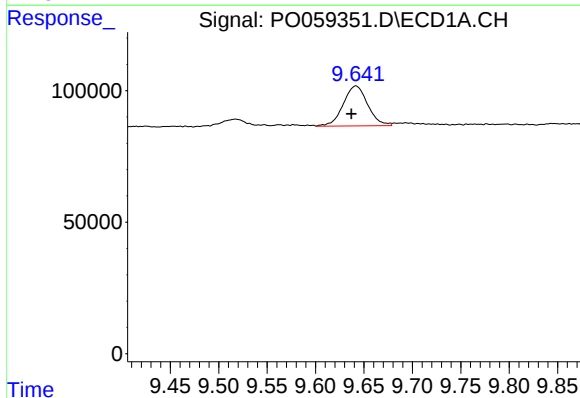

#2 Decachlorobiphenyl

R.T.: 9.642 min
Delta R.T.: 0.005 min
Response: 268110
Conc: 4.95 ng/ml

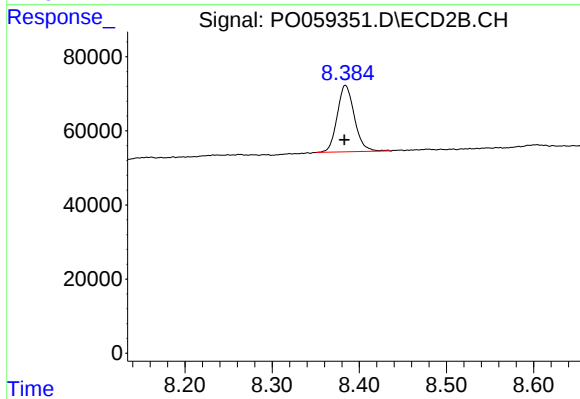

#2 Decachlorobiphenyl

R.T.: 8.384 min
Delta R.T.: 0.001 min
Response: 245141
Conc: 6.21 ng/ml