

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081522\
 Data File : P0088960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2022 11:23
 Operator : YP/AJ
 Sample : N4140-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LINDEN-MR-B1B-SP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 22:53:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.432	3.591	46196291	14284144	17.127	13.198
2) SA Decachlor...	10.269	8.581	28141188	13056620	14.583	10.774 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081522\
Data File : P0088960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2022 11:23
Operator : YP/AJ
Sample : N4140-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LINDEN-MR-B1B-SP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 22:53:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

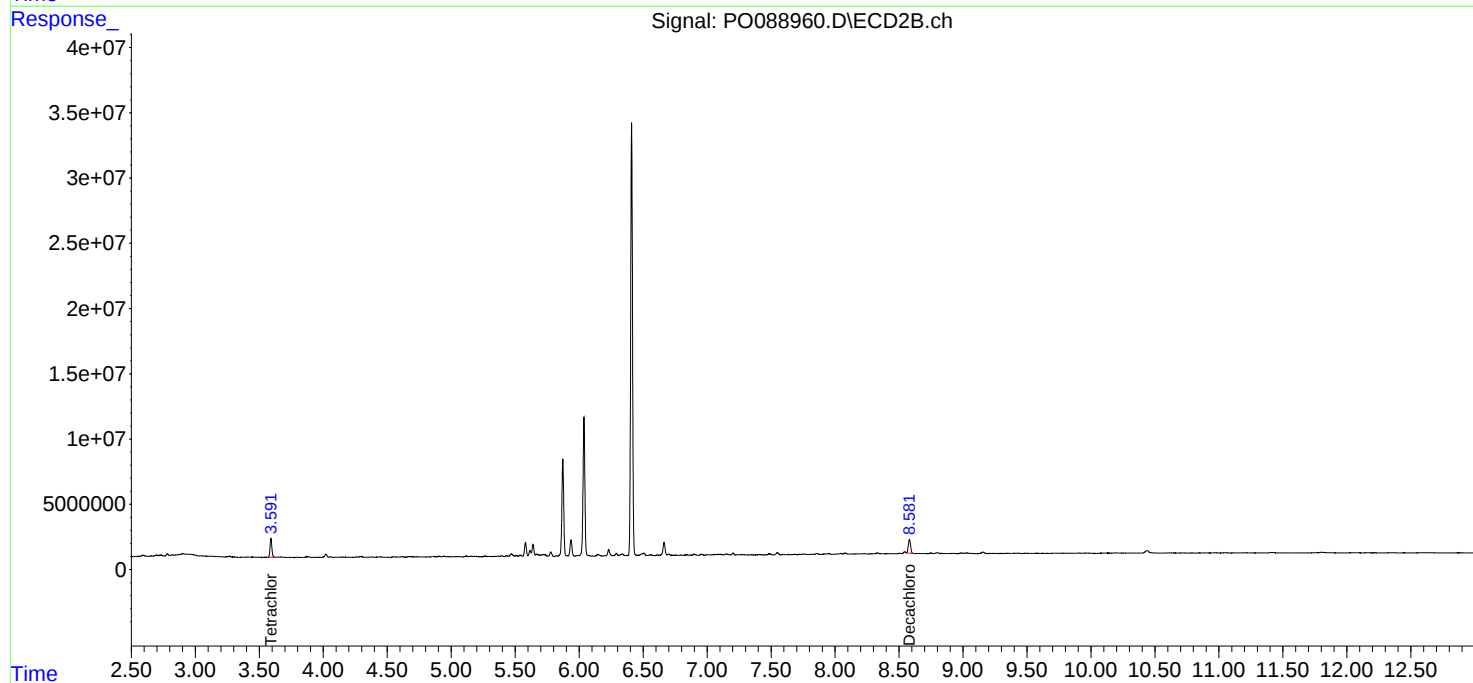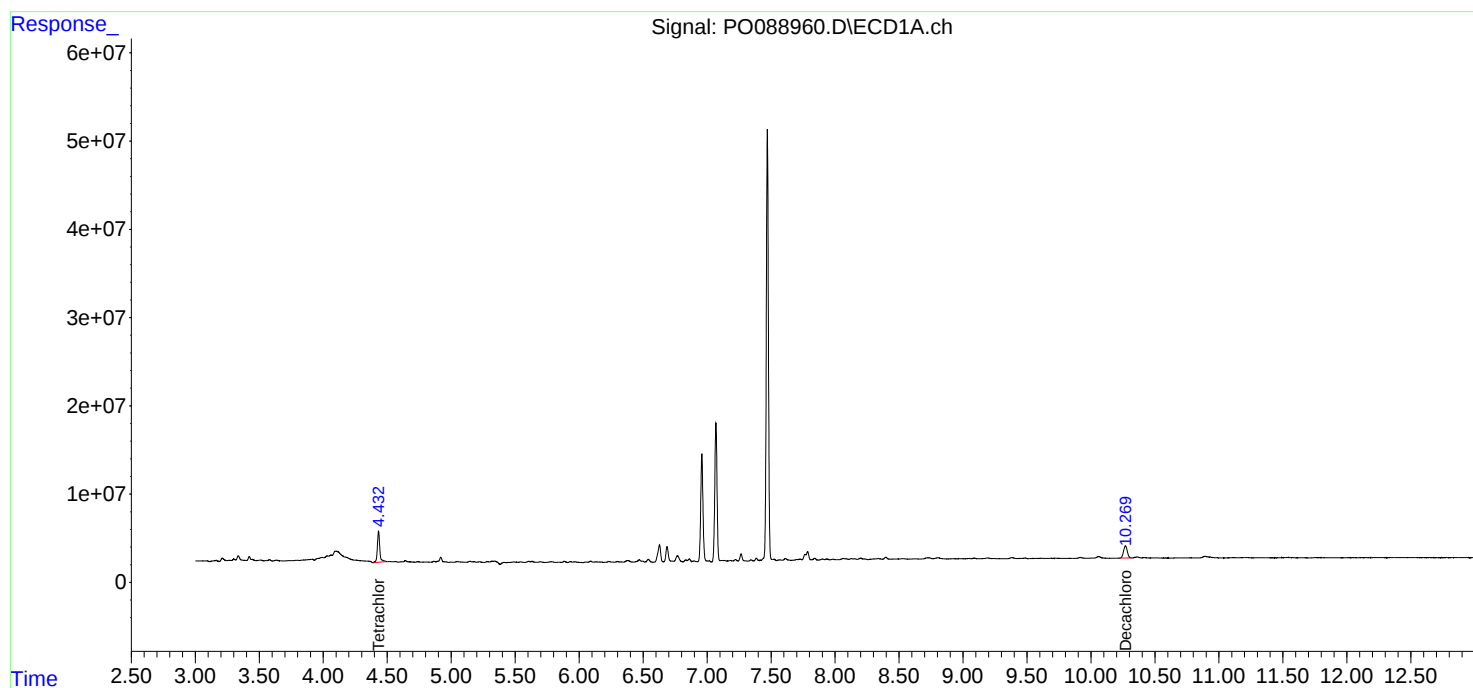


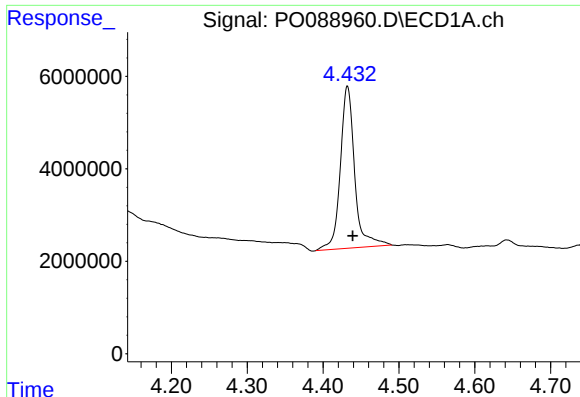

#1 Tetrachloro-m-xylene


R.T.: 4.432 min
Delta R.T.: -0.007 min
Response: 46196291
Conc: 17.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
LINDEN-MR-B1B-SP

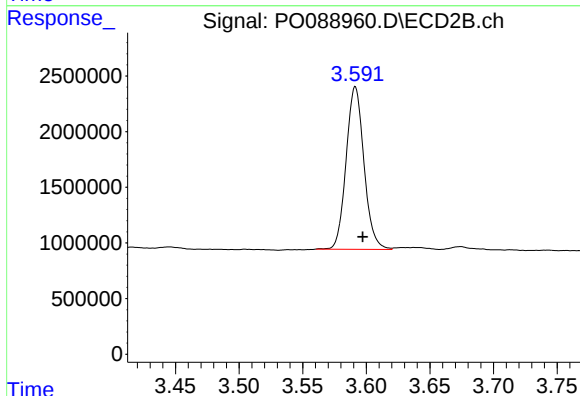


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: -0.006 min
Response: 14284144
Conc: 13.20 ng/ml

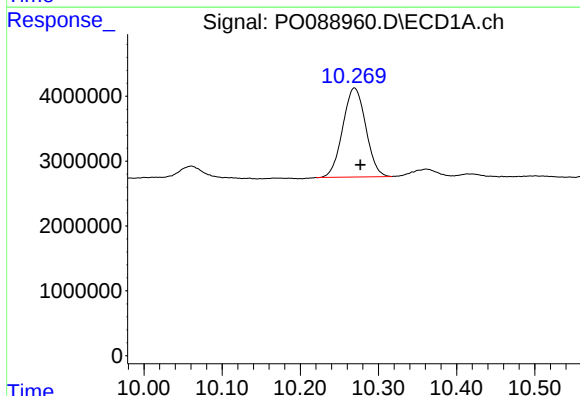

#2 Decachlorobiphenyl

R.T.: 10.269 min
Delta R.T.: -0.008 min
Response: 28141188
Conc: 14.58 ng/ml

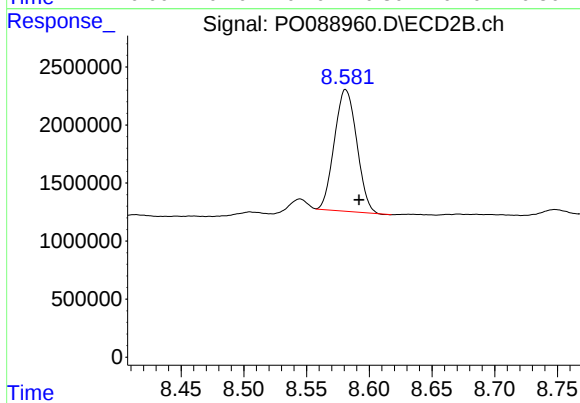

#2 Decachlorobiphenyl

R.T.: 8.581 min
Delta R.T.: -0.011 min
Response: 13056620
Conc: 10.77 ng/ml