

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081522\
 Data File : P0088991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2022 21:21
 Operator : YP/AJ
 Sample : N4189-19
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB11

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/16/2022
 Supervised By :Ankita Jodhani 08/16/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 23:16:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.432	3.591	64711921	23269400	23.991	21.500
2) SA Decachlor...	10.267	8.579	51703747	26454347	26.794	21.829

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081522\
Data File : PO088991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2022 21:21
Operator : YP/AJ
Sample : N4189-19
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB11


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2022
Supervised By :Ankita Jodhani 08/16/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 23:16:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

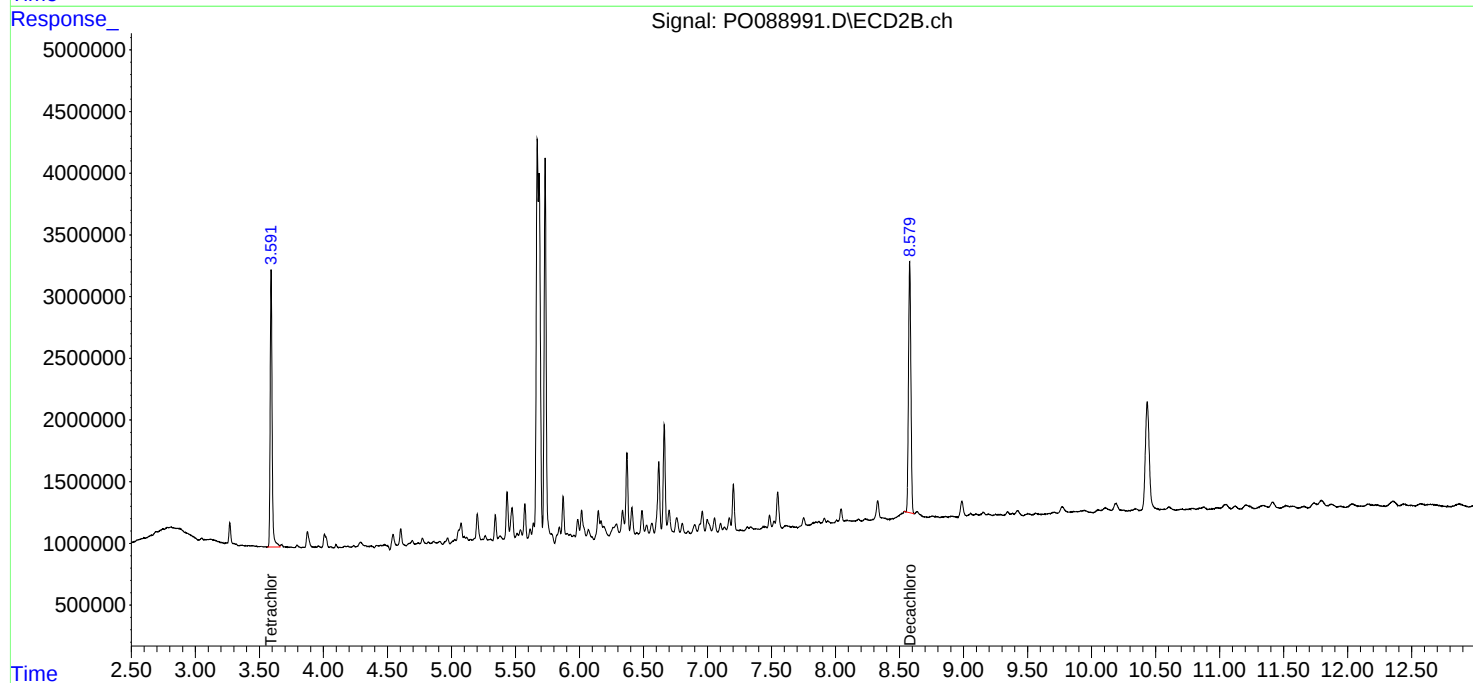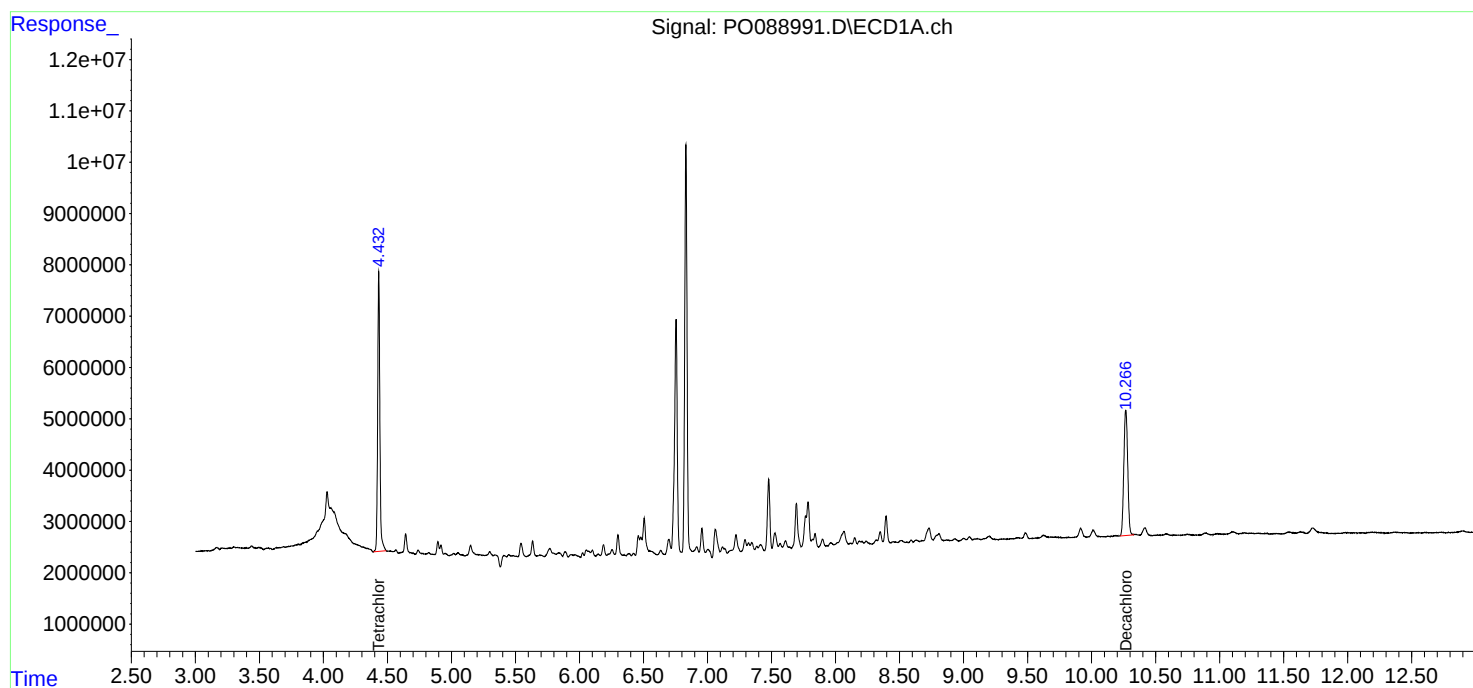

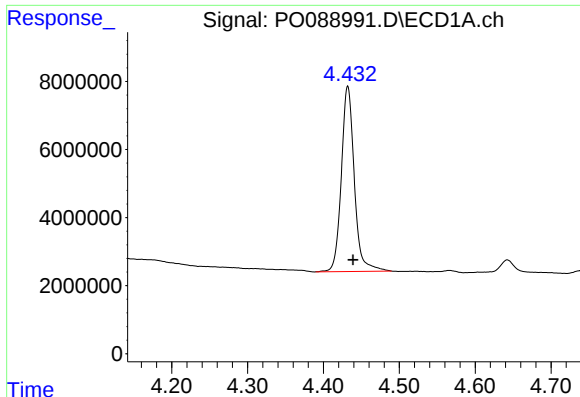


#1 Tetrachloro-m-xylene

R.T.: 4.432 min
Delta R.T.: -0.007 min
Response: 64711921
Conc: 23.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB11


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2022
Supervised By :Ankita Jodhani 08/16/2022

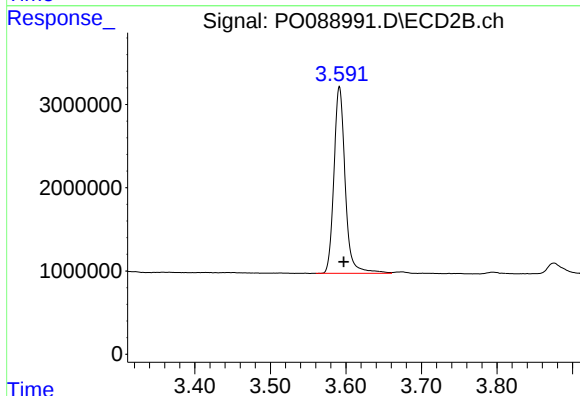


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: -0.006 min
Response: 23269400
Conc: 21.50 ng/ml

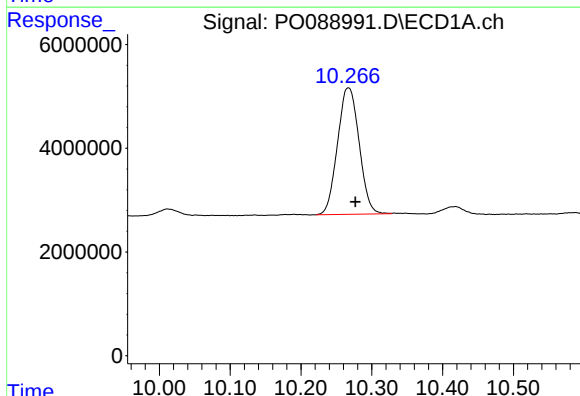

#2 Decachlorobiphenyl

R.T.: 10.267 min
Delta R.T.: -0.010 min
Response: 51703747
Conc: 26.79 ng/ml

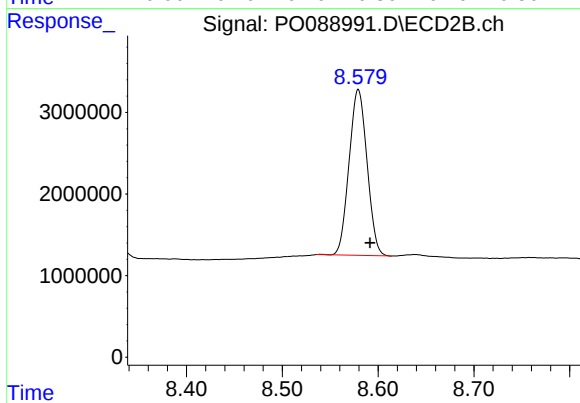

#2 Decachlorobiphenyl

R.T.: 8.579 min
Delta R.T.: -0.012 min
Response: 26454347
Conc: 21.83 ng/ml