

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081523\
 Data File : P0097131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2023 05:29
 Operator : YP/AJ
 Sample : 04001-04 10X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMH4876-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/16/2023
 Supervised By :Ankita Jodhani 08/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 06:18:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 08 04:34:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.407	3.613	4918957	2007987	1.486m	1.517m
2) SA Decachlor...	10.348	8.629	5070018	1982264	2.317m	1.713m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081523\
Data File : PO097131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2023 05:29
Operator : YP/AJ
Sample : 04001-04 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMH4876-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2023
Supervised By :Ankita Jodhani 08/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 06:18:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 08 04:34:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

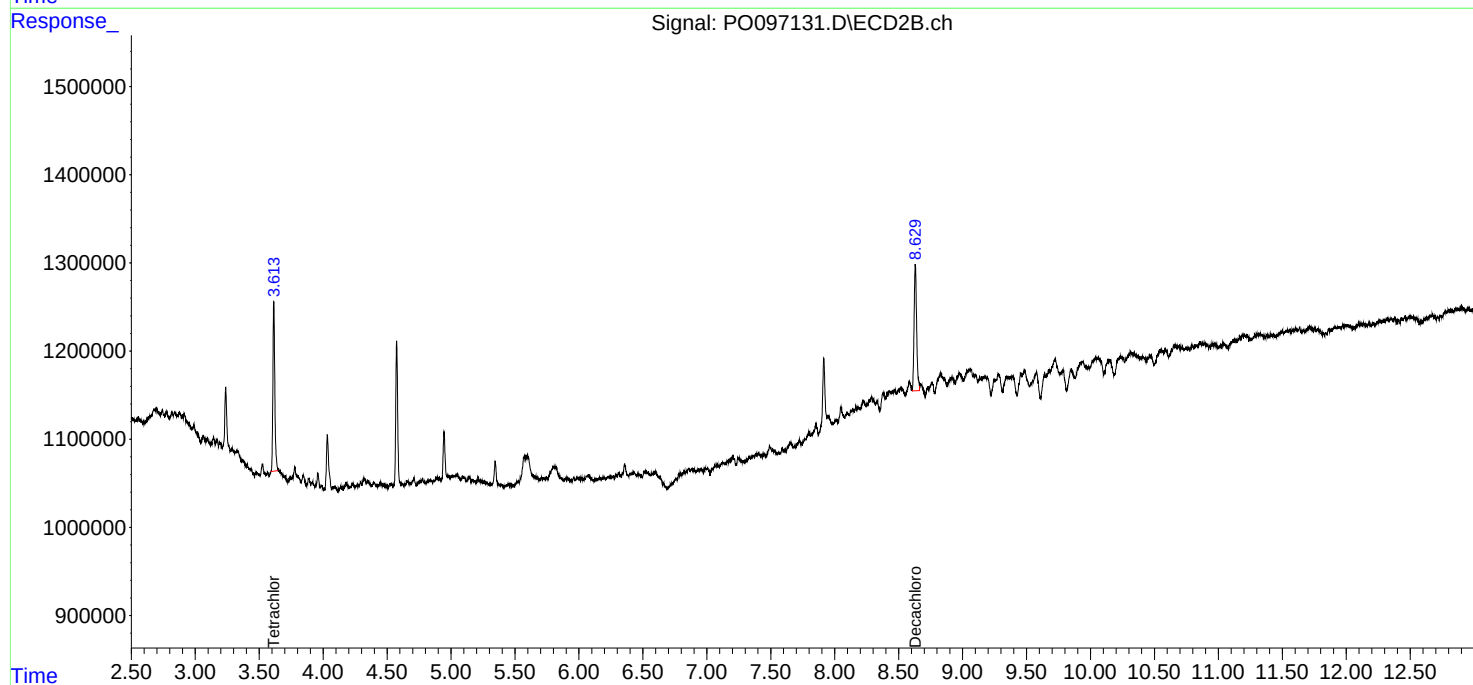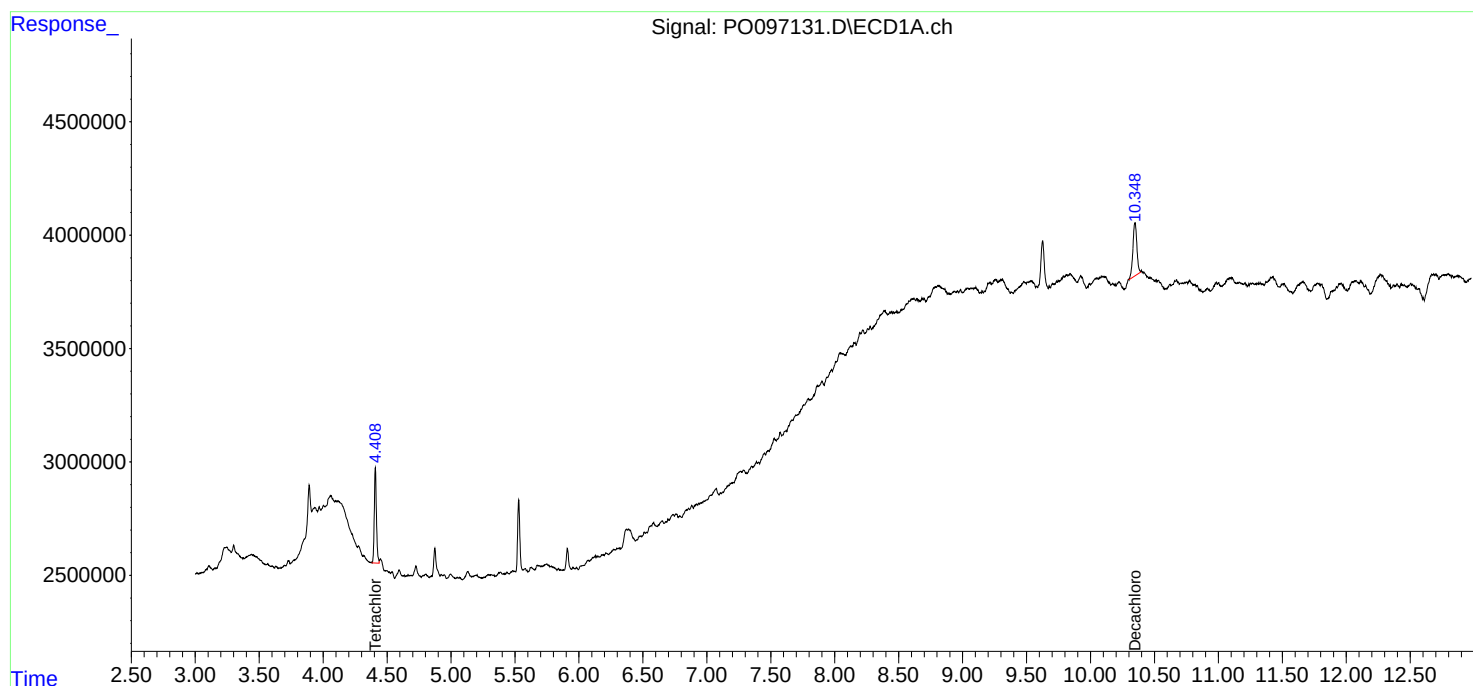

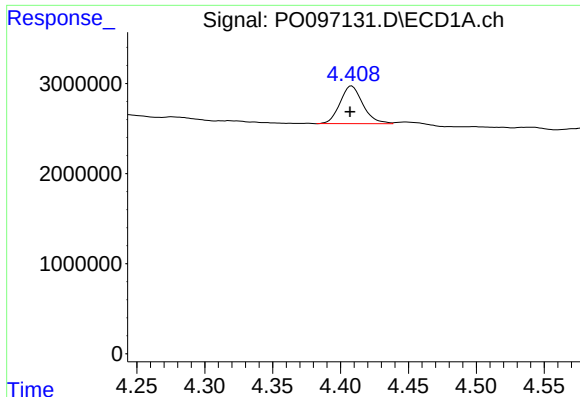


#1 Tetrachloro-m-xylene

R.T.: 4.407 min
Delta R.T.: 0.000 min
Response: 4918957
Conc: 1.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMH4876-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2023
Supervised By :Ankita Jodhani 08/16/2023

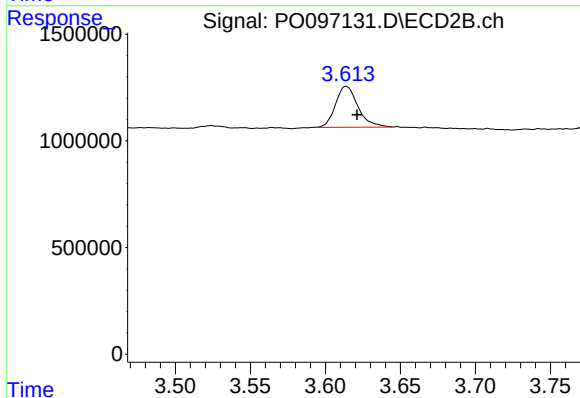


#1 Tetrachloro-m-xylene

R.T.: 3.613 min
Delta R.T.: -0.008 min
Response: 2007987
Conc: 1.52 ng/ml m

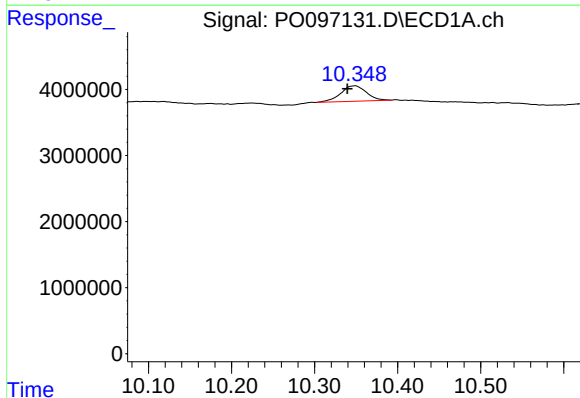

#2 Decachlorobiphenyl

R.T.: 10.348 min
Delta R.T.: 0.008 min
Response: 5070018
Conc: 2.32 ng/ml m

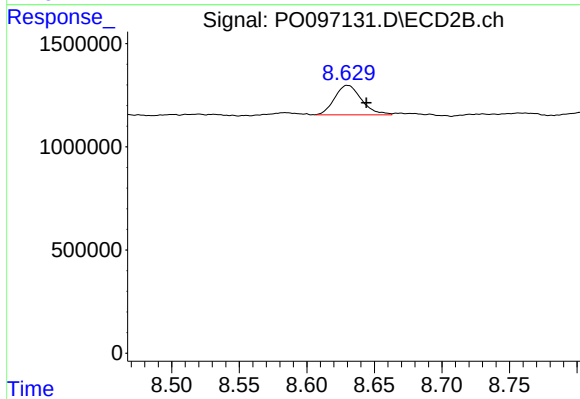

#2 Decachlorobiphenyl

R.T.: 8.629 min
Delta R.T.: -0.015 min
Response: 1982264
Conc: 1.71 ng/ml m