

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081524\
 Data File : P0105568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2024 19:42
 Operator : YP/AJ
 Sample : P3614-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-01-081424

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/16/2024
 Supervised By :Ankita Jodhani 08/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 04:55:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 11:44:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.453	3.726	173.7E6	57037600	18.578m	22.363
2) SA Decachlor...	10.197	8.777	92050233	27574168	15.858	13.972

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081524\
Data File : PO105568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2024 19:42
Operator : YP/AJ
Sample : P3614-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-01-081424


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2024
Supervised By :Ankita Jodhani 08/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 04:55:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 11:44:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

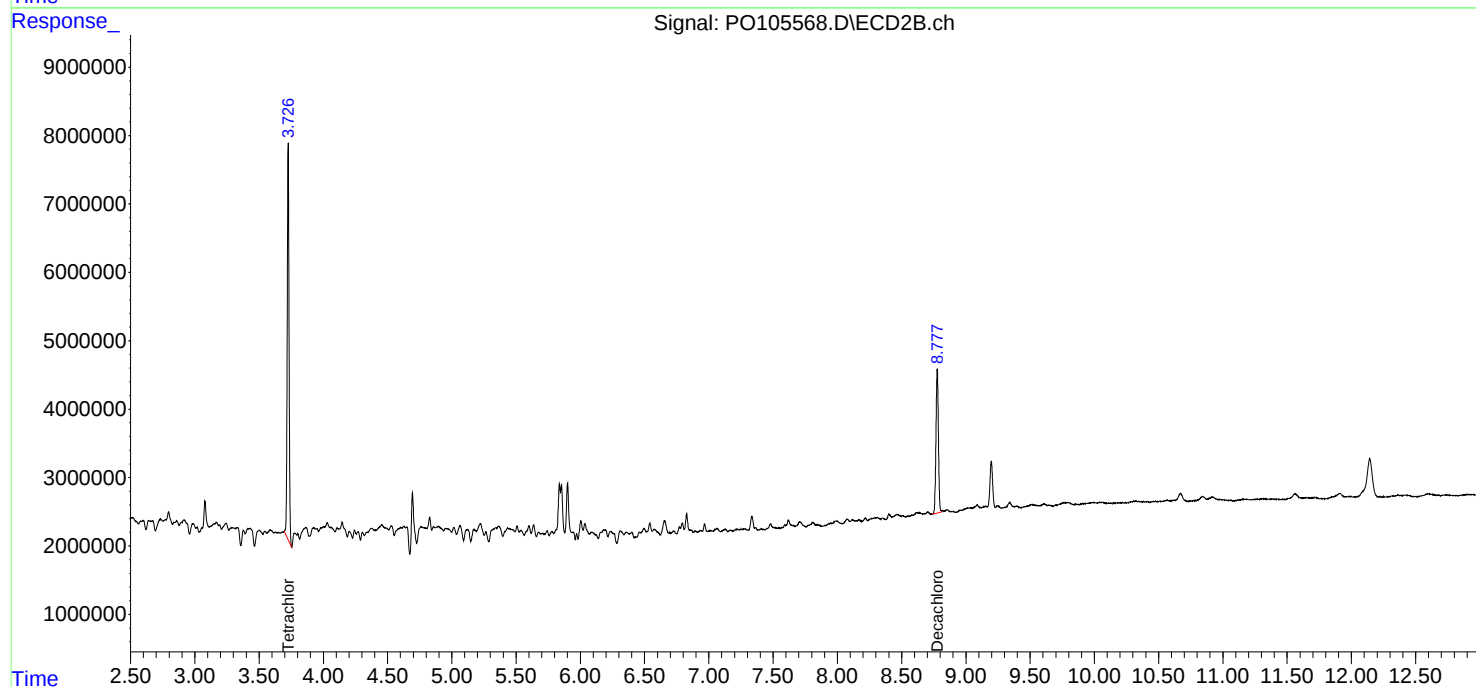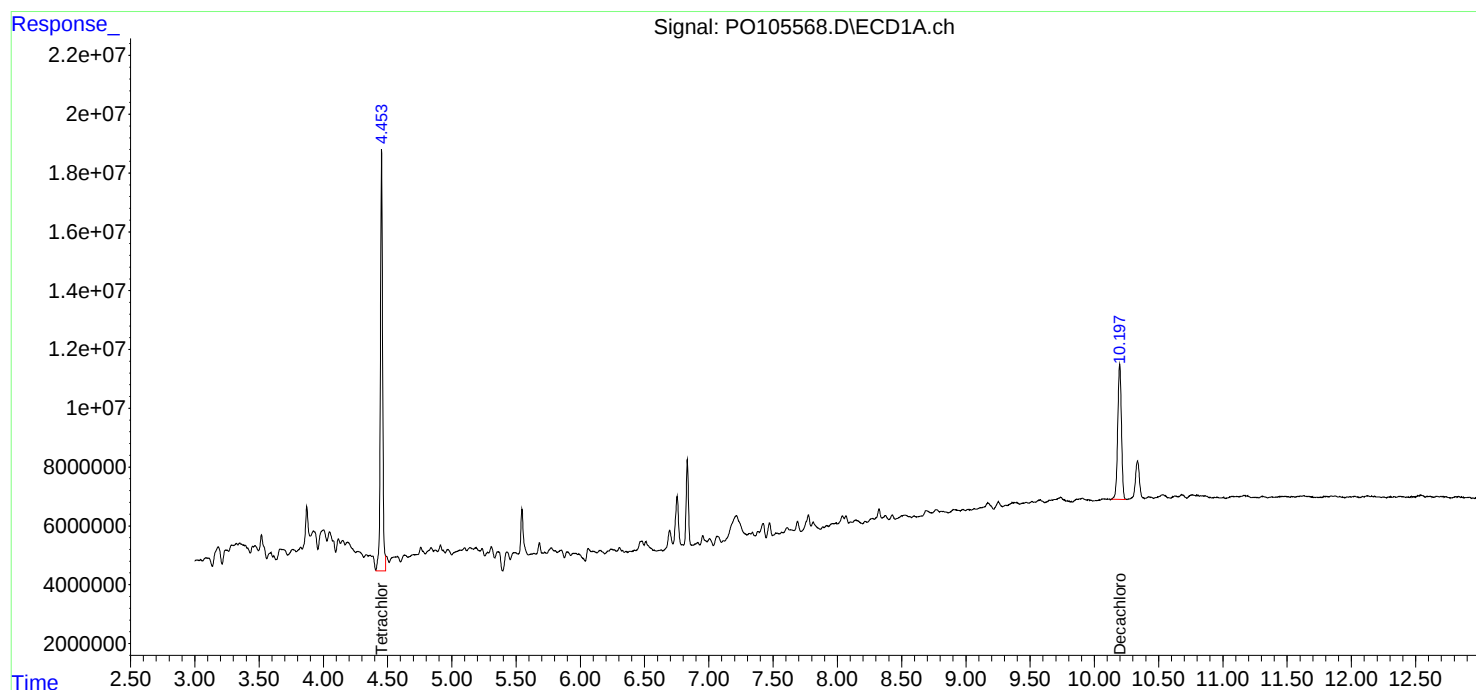

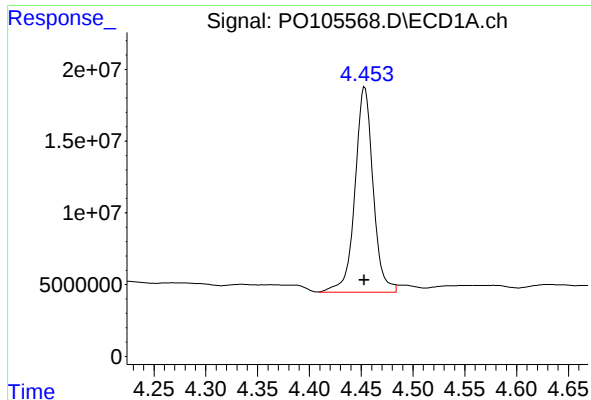


#1 Tetrachloro-m-xylene

R.T.: 4.453 min
Delta R.T.: 0.000 min
Response: 173684436
Conc: 18.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-01-081424


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2024
Supervised By :Ankita Jodhani 08/16/2024

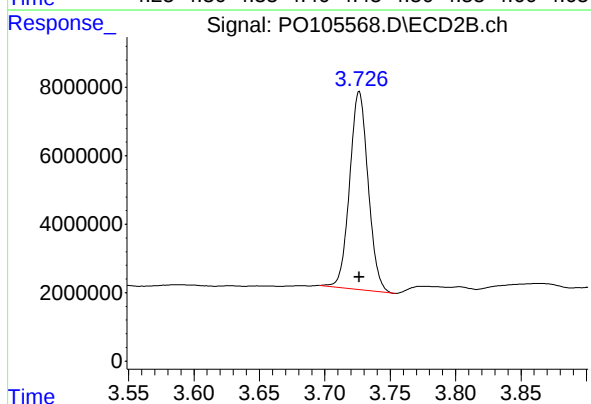


#1 Tetrachloro-m-xylene

R.T.: 3.726 min
Delta R.T.: 0.000 min
Response: 57037600
Conc: 22.36 ng/ml

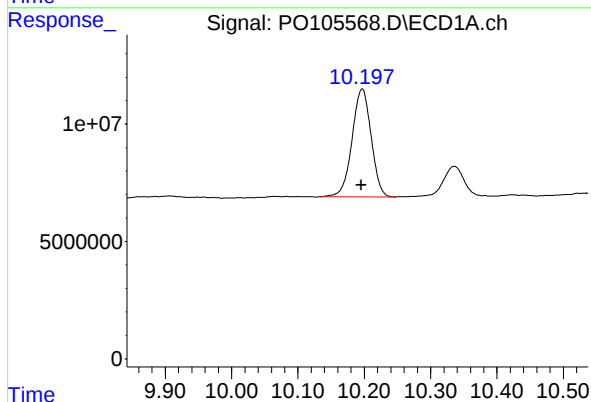

#2 Decachlorobiphenyl

R.T.: 10.197 min
Delta R.T.: 0.002 min
Response: 92050233
Conc: 15.86 ng/ml

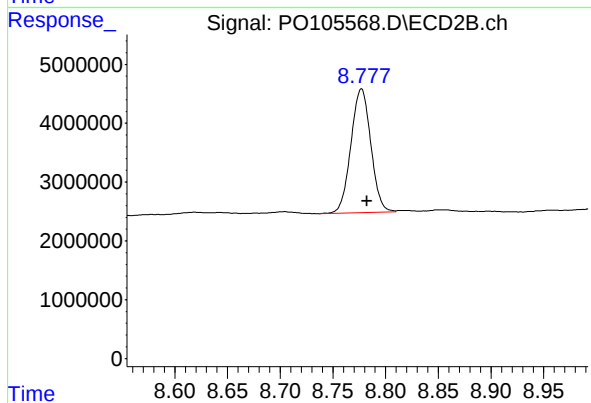

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: -0.005 min
Response: 27574168
Conc: 13.97 ng/ml