

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081524\
 Data File : P0105580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2024 05:56
 Operator : YP/AJ
 Sample : P3616-06 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JEH685X-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/16/2024
 Supervised By :Ankita Jodhani 08/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 06:53:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 11:44:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.454	3.727	14350129	3107915	1.535	1.219m
2) SA Decachlor...	10.198	8.774	10677832	3494228	1.840	1.771m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081524\
Data File : PO105580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2024 05:56
Operator : YP/AJ
Sample : P3616-06 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JEH685X-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2024
Supervised By :Ankita Jodhani 08/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 06:53:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 11:44:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

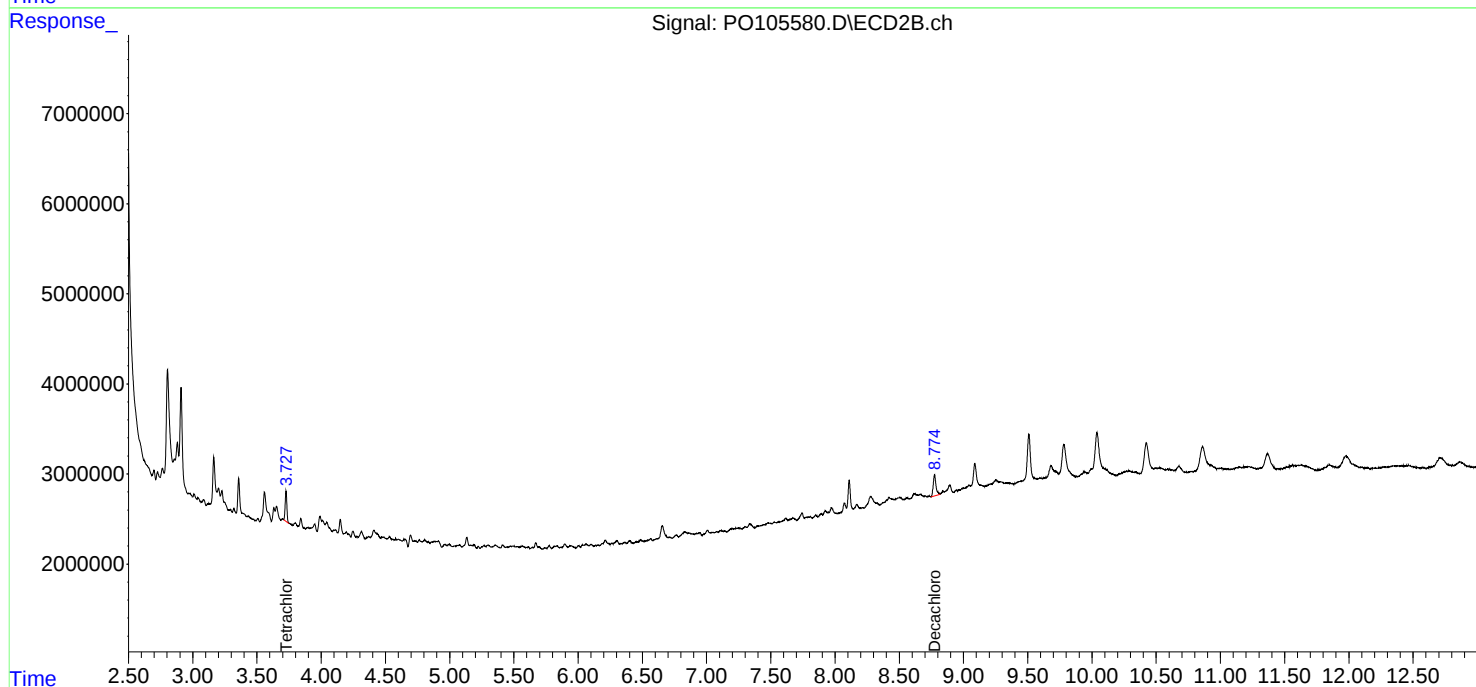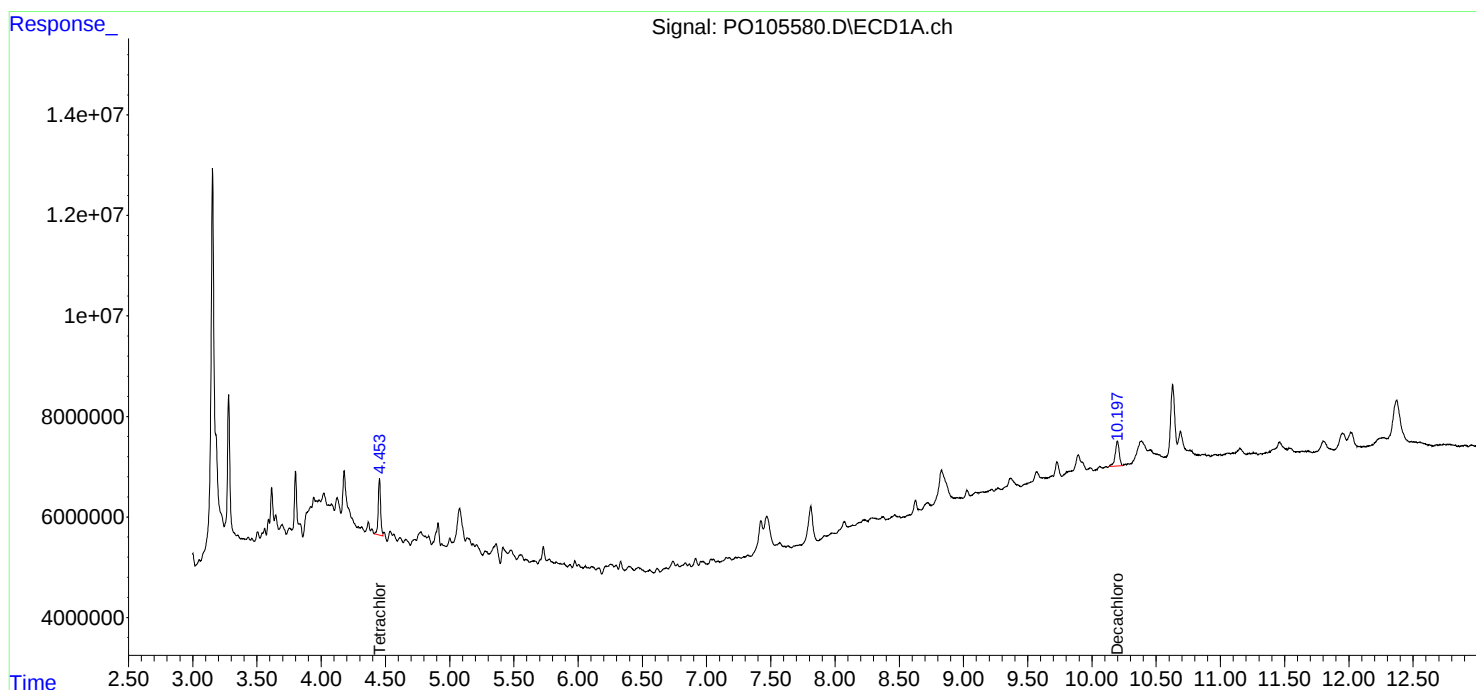

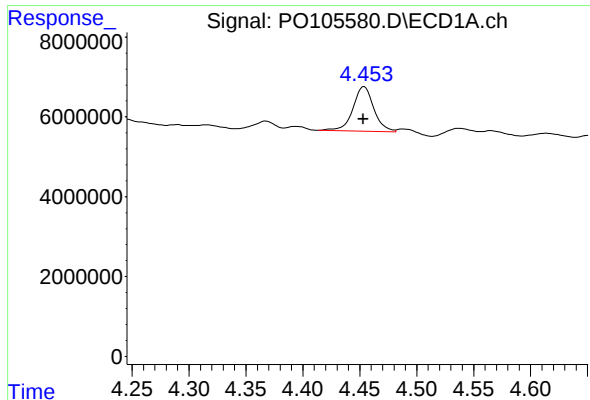


#1 Tetrachloro-m-xylene

R.T.: 4.454 min
Delta R.T.: 0.000 min
Response: 14350129
Conc: 1.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
JEH685X-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2024
Supervised By :Ankita Jodhani 08/16/2024

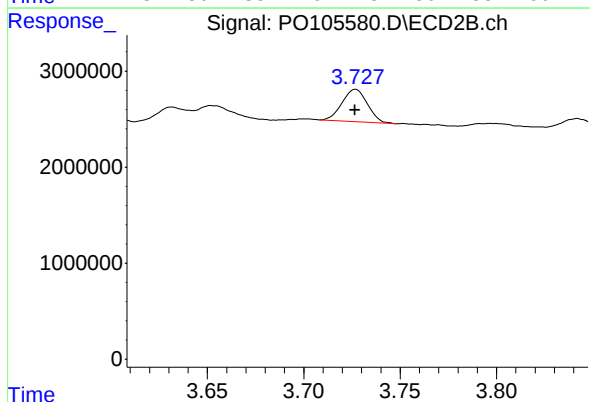


#1 Tetrachloro-m-xylene

R.T.: 3.727 min
Delta R.T.: 0.000 min
Response: 3107915
Conc: 1.22 ng/ml m

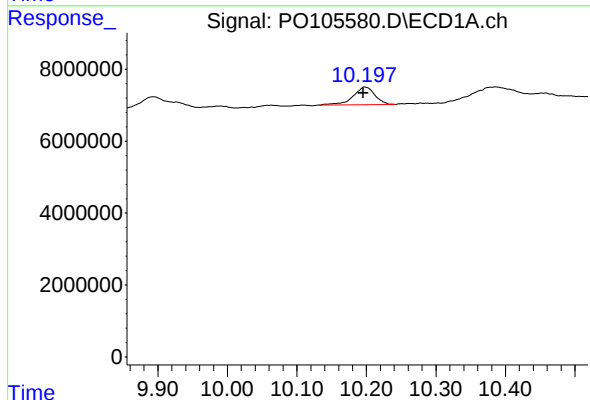

#2 Decachlorobiphenyl

R.T.: 10.198 min
Delta R.T.: 0.002 min
Response: 10677832
Conc: 1.84 ng/ml

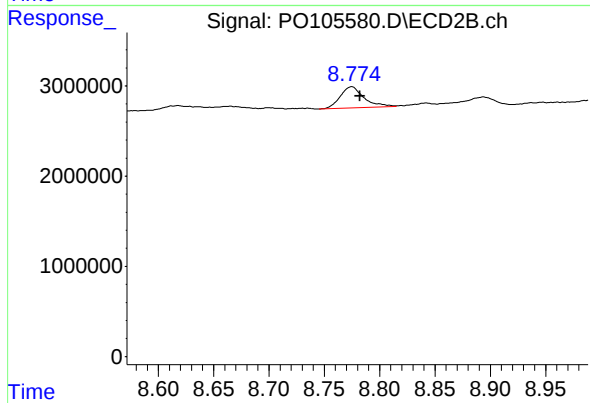

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: -0.008 min
Response: 3494228
Conc: 1.77 ng/ml m