

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081524\
 Data File : P0105583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2024 06:47
 Operator : YP/AJ
 Sample : P3616-01 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC247601-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/16/2024
 Supervised By :Ankita Jodhani 08/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 07:04:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 11:44:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.454	3.728	12416957	3898108	1.328	1.528
2) SA Decachlor...	10.197	8.775	8752294	2220281	1.508m	1.125m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081524\
Data File : PO105583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2024 06:47
Operator : YP/AJ
Sample : P3616-01 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC247601-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2024
Supervised By :Ankita Jodhani 08/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 07:04:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 11:44:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

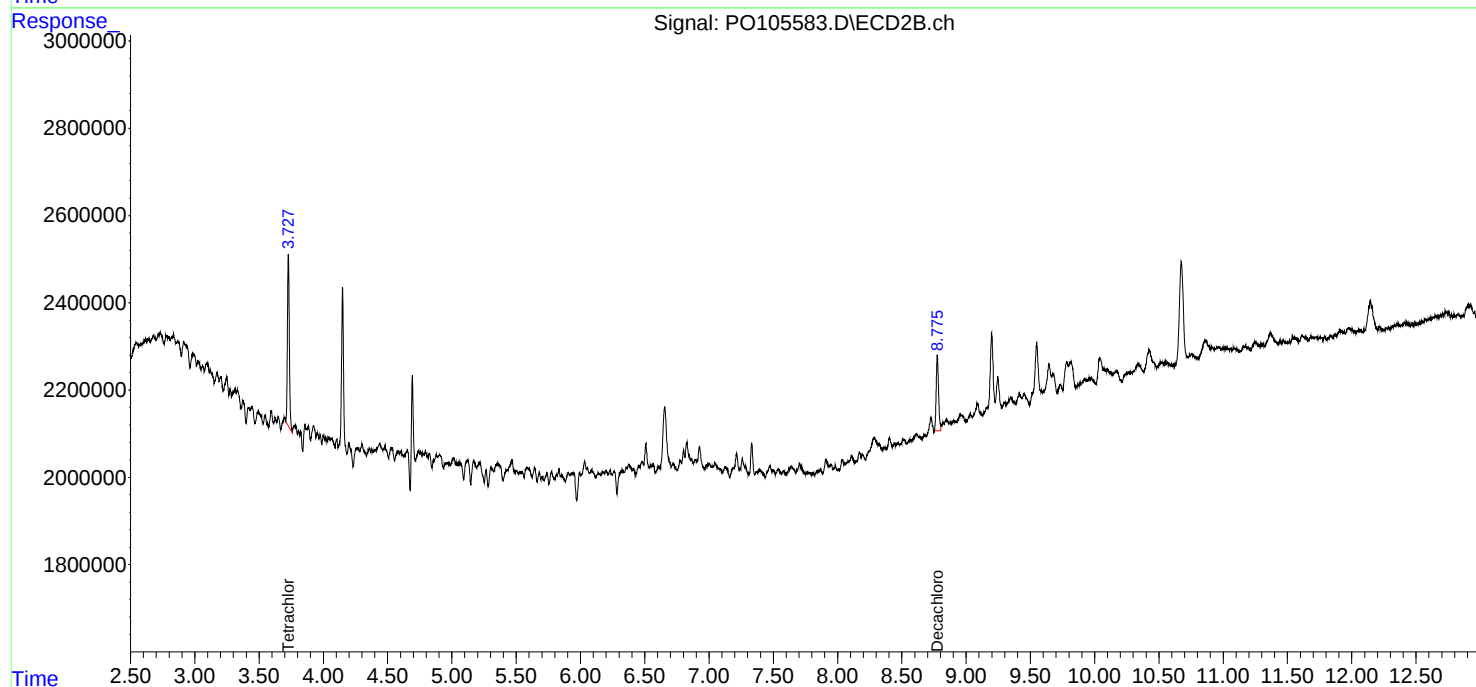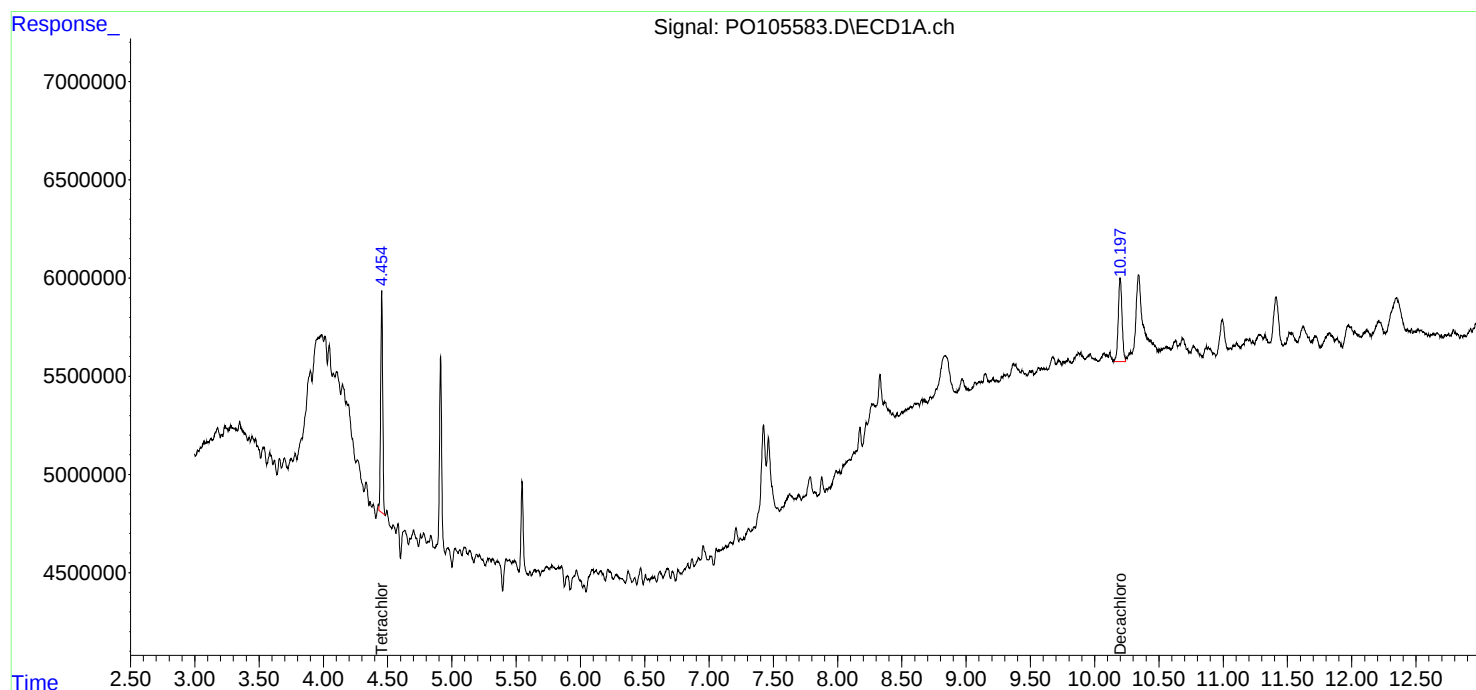

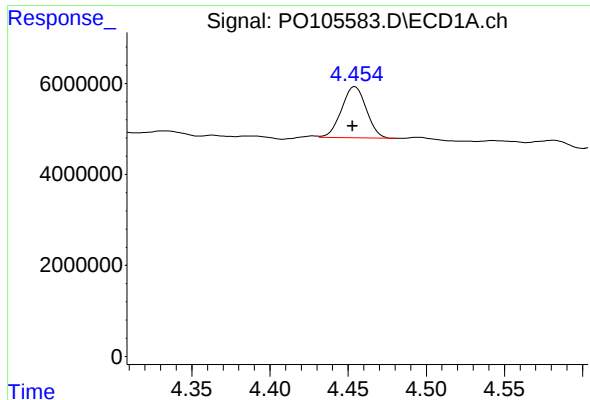


#1 Tetrachloro-m-xylene

R.T.: 4.454 min
Delta R.T.: 0.001 min
Response: 12416957
Conc: 1.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC247601-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2024
Supervised By :Ankita Jodhani 08/16/2024

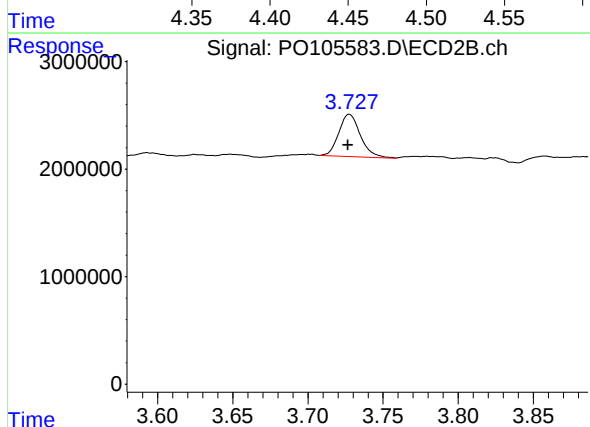


#1 Tetrachloro-m-xylene

R.T.: 3.728 min
Delta R.T.: 0.001 min
Response: 3898108
Conc: 1.53 ng/ml

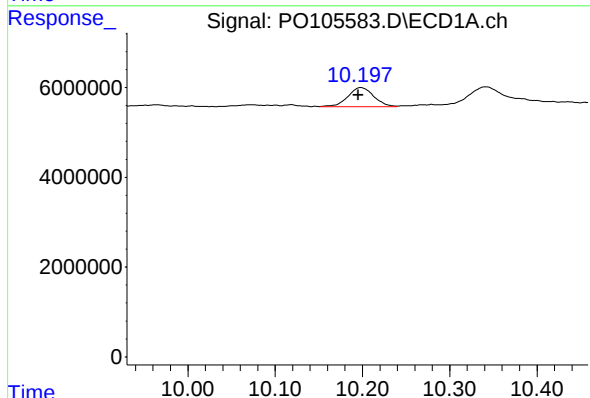

#2 Decachlorobiphenyl

R.T.: 10.197 min
Delta R.T.: 0.002 min
Response: 8752294
Conc: 1.51 ng/ml m

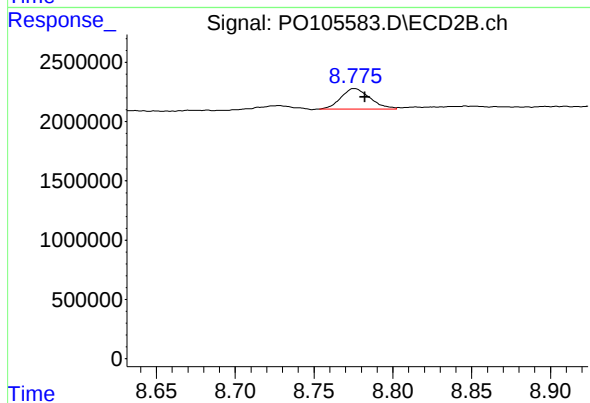

#2 Decachlorobiphenyl

R.T.: 8.775 min
Delta R.T.: -0.008 min
Response: 2220281
Conc: 1.13 ng/ml m