

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081618\
Data File : P0048156.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Aug 2018 17:15
Operator : SM/SJ
Sample : J4269-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AU-06-081518-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 04:17:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.390	3.632	5344763	6284192	26.473	25.575
2) SA Decachlor...	10.077	8.614	3207829	3058242	19.668	19.455

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081618\
Data File : P0048156.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Aug 2018 17:15
Operator : SM/SJ
Sample : J4269-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AU-06-081518-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 04:17:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

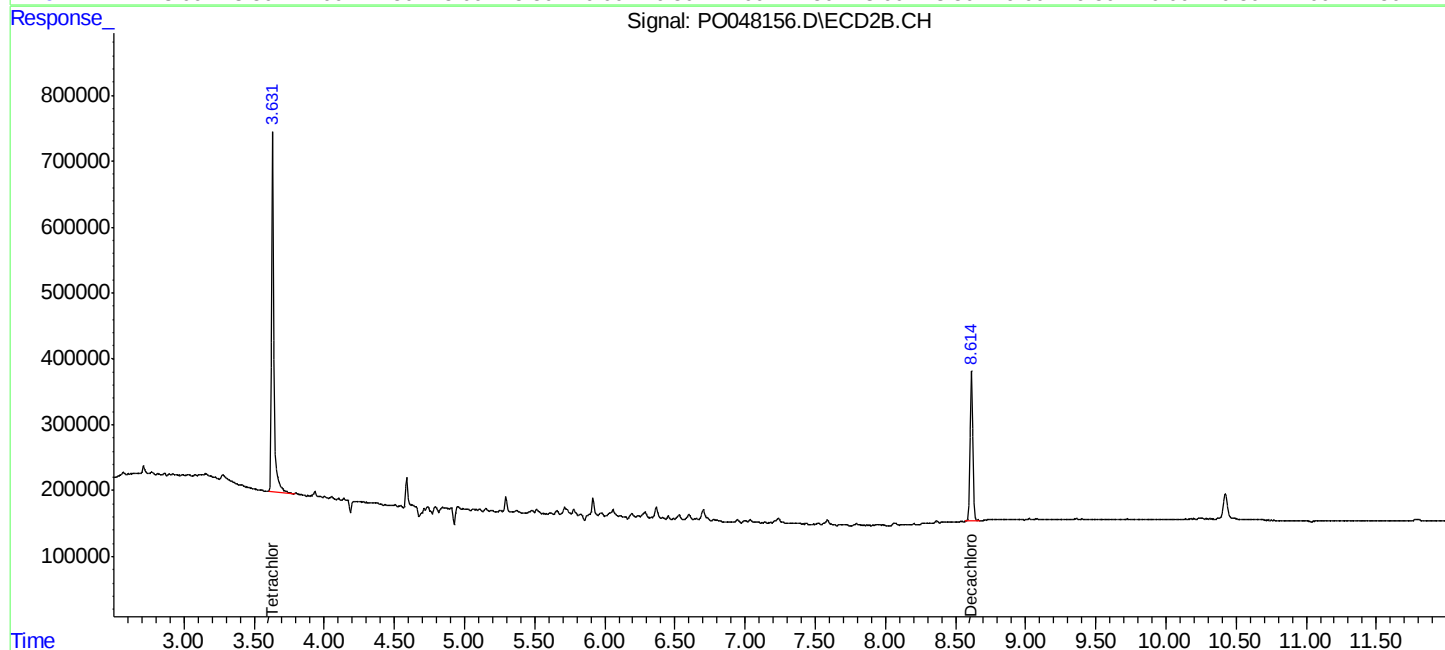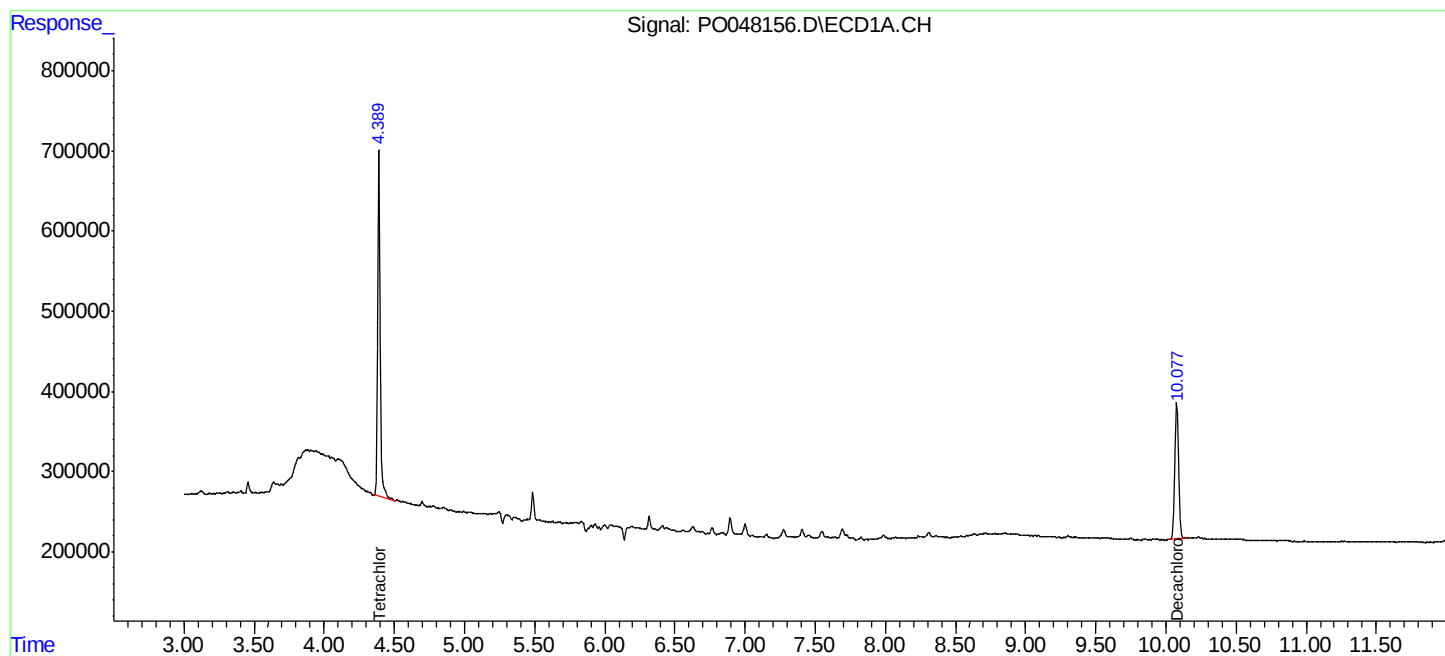


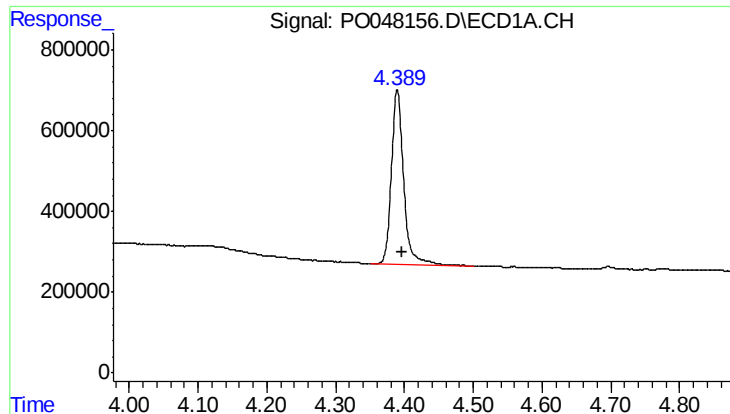

#1 Tetrachloro-m-xylene


R.T.: 4.390 min
Delta R.T.: -0.008 min
Response: 5344763
Conc: 26.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-06-081518-A

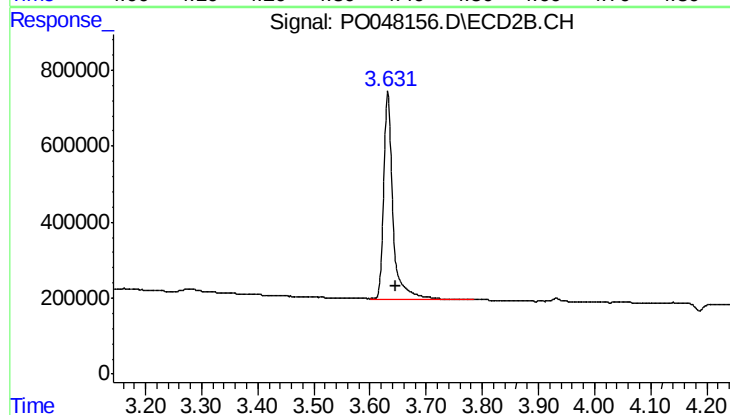


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: -0.014 min
Response: 6284192
Conc: 25.58 ng/ml

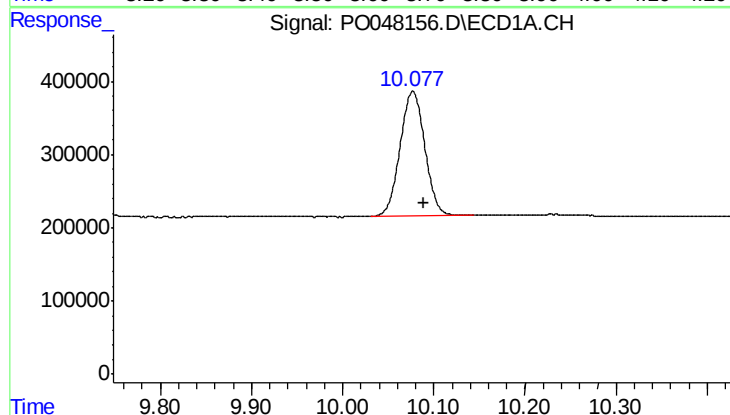

#2 Decachlorobiphenyl

R.T.: 10.077 min
Delta R.T.: -0.013 min
Response: 3207829
Conc: 19.67 ng/ml

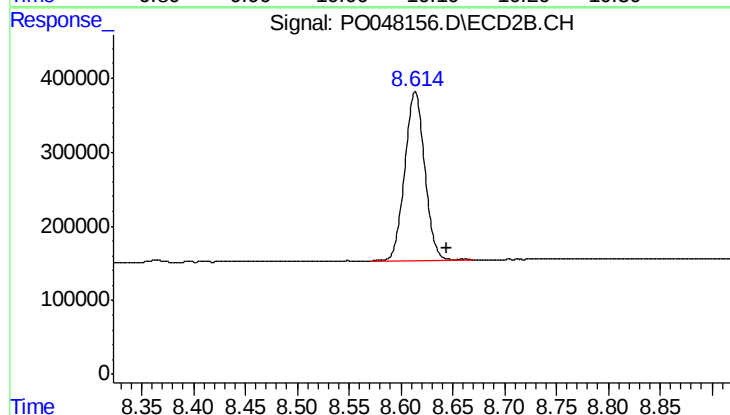

#2 Decachlorobiphenyl

R.T.: 8.614 min
Delta R.T.: -0.031 min
Response: 3058242
Conc: 19.46 ng/ml