

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081618\
Data File : P0048162.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Aug 2018 18:50
Operator : SM/SJ
Sample : J4500-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 04:25:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.390	3.633	4546157	5850070	22.517	23.808
2)	SA Decachlor...	10.077	8.615	2757411	2602542	16.906	16.556

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081618\
Data File : P0048162.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Aug 2018 18:50
Operator : SM/SJ
Sample : J4500-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 04:25:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

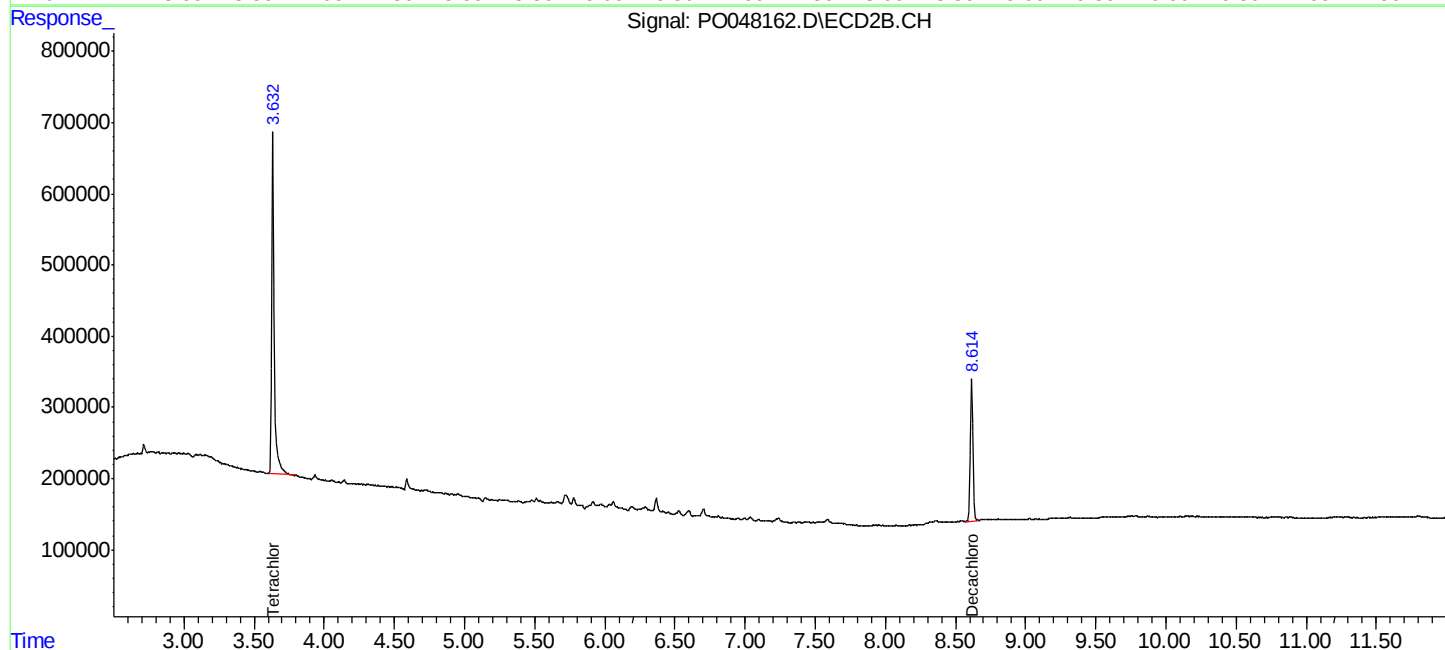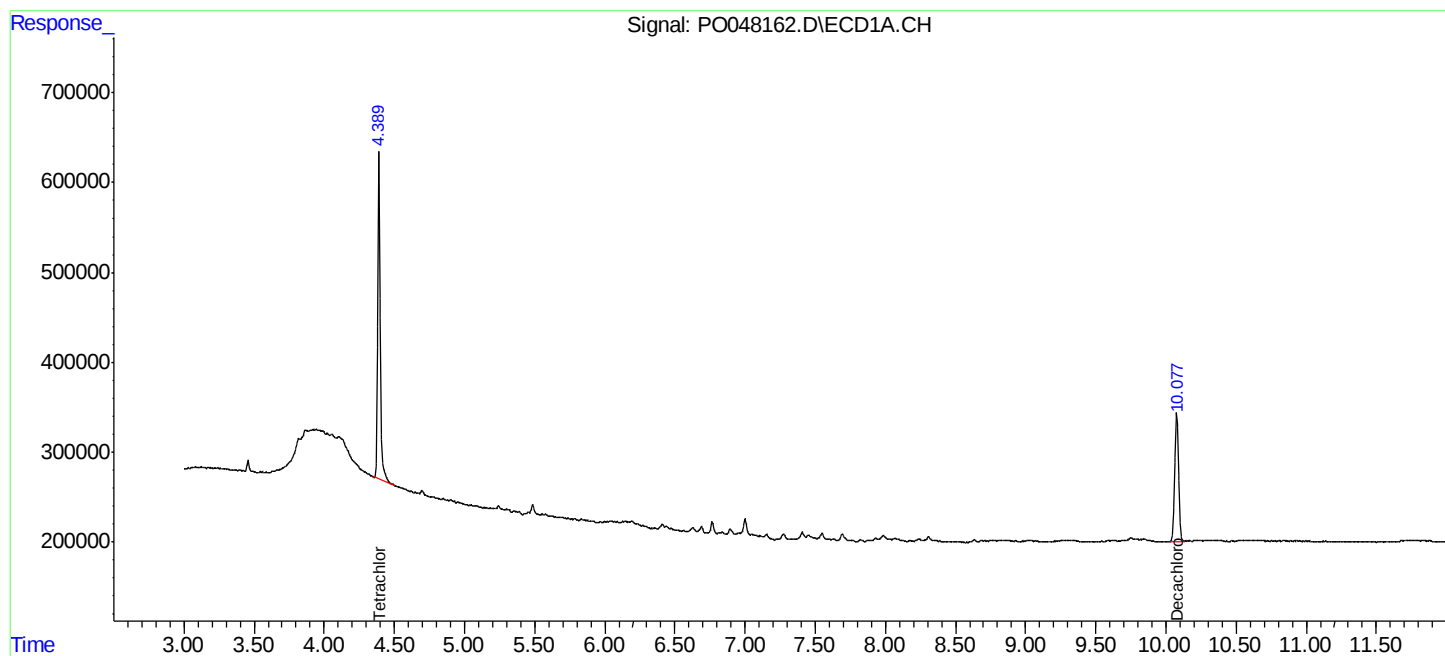


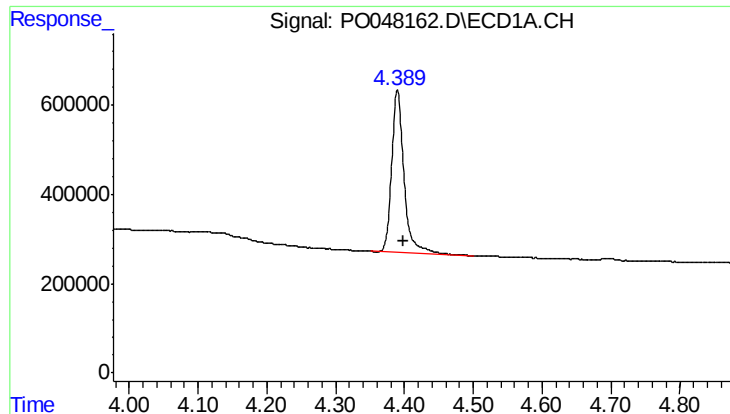

#1 Tetrachloro-m-xylene


R.T.: 4.390 min
Delta R.T.: -0.008 min
Response: 4546157
Conc: 22.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-6

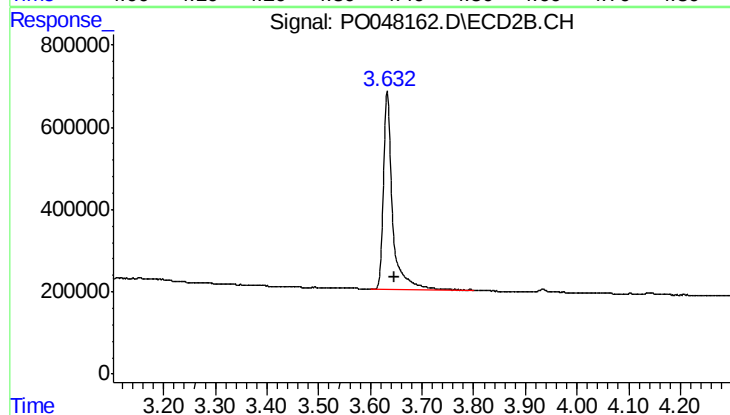


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: -0.012 min
Response: 5850070
Conc: 23.81 ng/ml

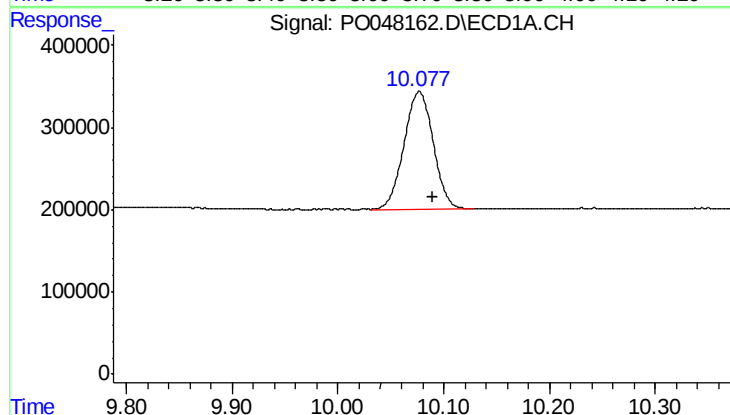

#2 Decachlorobiphenyl

R.T.: 10.077 min
Delta R.T.: -0.013 min
Response: 2757411
Conc: 16.91 ng/ml

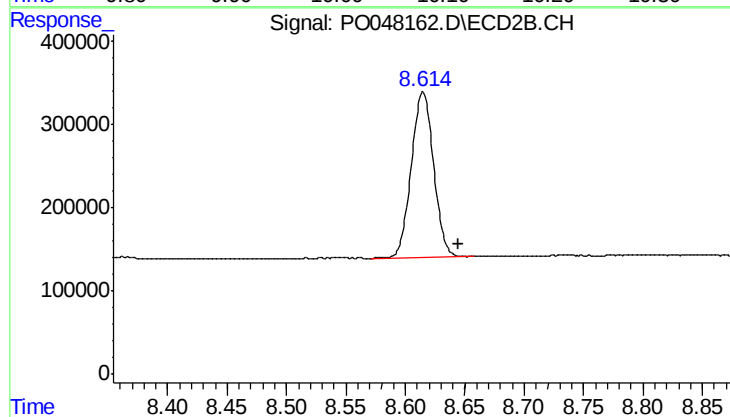

#2 Decachlorobiphenyl

R.T.: 8.615 min
Delta R.T.: -0.030 min
Response: 2602542
Conc: 16.56 ng/ml