

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081621\
 Data File : P0080516.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Aug 2021 4:14
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 05:24:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.991	4.106	1713725	558355	24.749	22.403
2)	SA Decachlor...	11.091	9.505	1243976	508223	24.032	22.407
Target Compounds							
8)	L2 AR-1221-1	5.228f	0.000	6598	0	8.296	N.D. #
9)	L2 AR-1221-2	5.345	0.000	22381	0	40.885	N.D. #
20)	L4 AR-1242-5	0.000	6.293f	0	14117	N.D.	20.259 #
24)	L5 AR-1248-4	7.269	0.000	3617	0	1.330	N.D. #
25)	L5 AR-1248-5	0.000	6.293f	0	14117	N.D.	13.617 #
26)	L6 AR-1254-1	7.242	6.293f	80415	14117	31.021	9.622 #
28)	L6 AR-1254-3	7.867	0.000	34889	0	8.548	N.D. #
32)	L7 AR-1260-2	0.000	7.170f	0	14083	N.D.	8.473 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081621\
Data File : PO080516.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2021 4:14
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 05:24:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

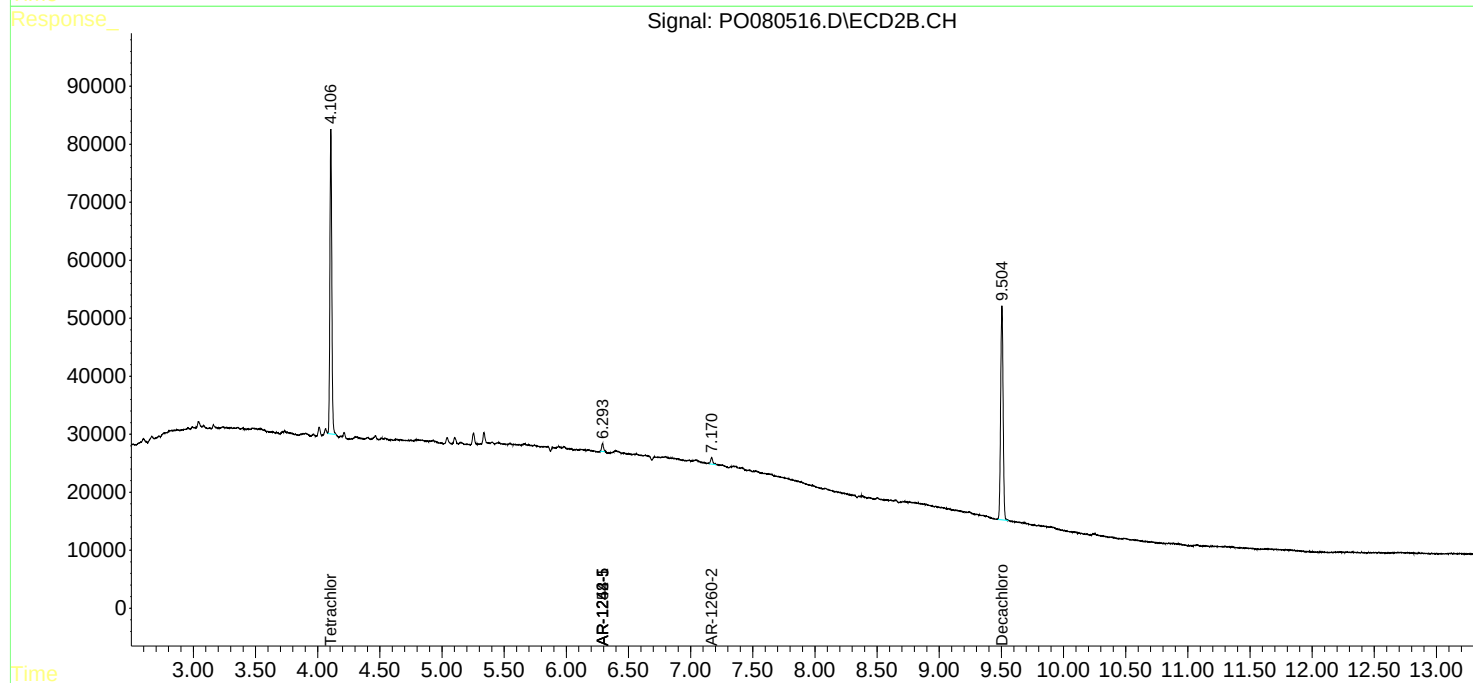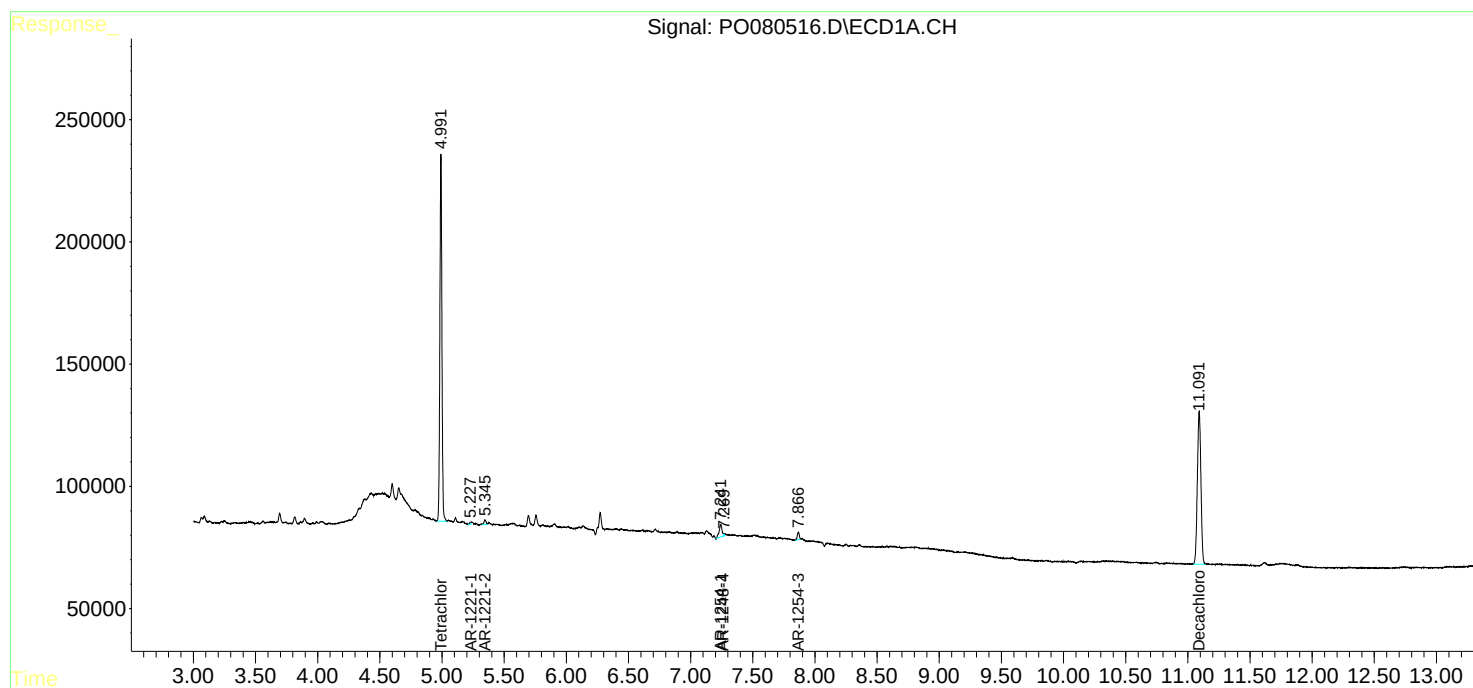


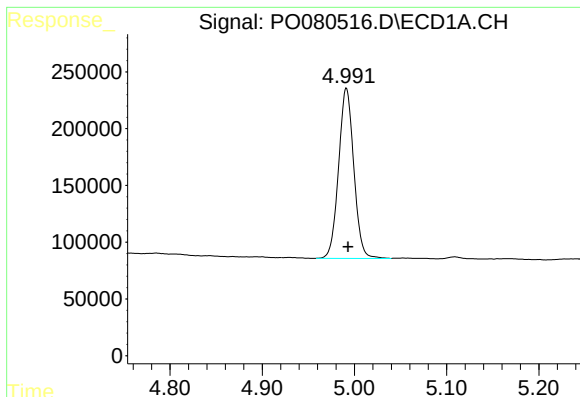

#1 Tetrachloro-m-xylene


R.T.: 4.991 min
Delta R.T.: -0.002 min
Response: 1713725
Conc: 24.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

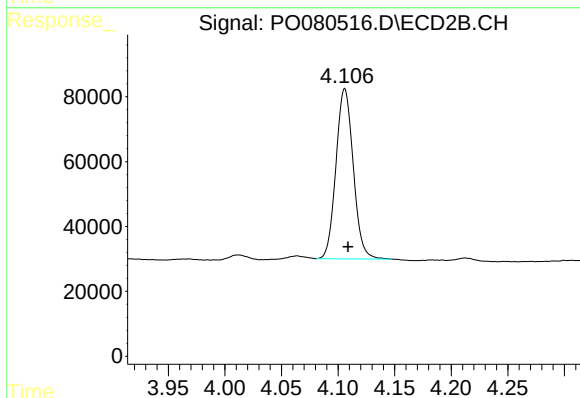


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: -0.003 min
Response: 558355
Conc: 22.40 ng/ml

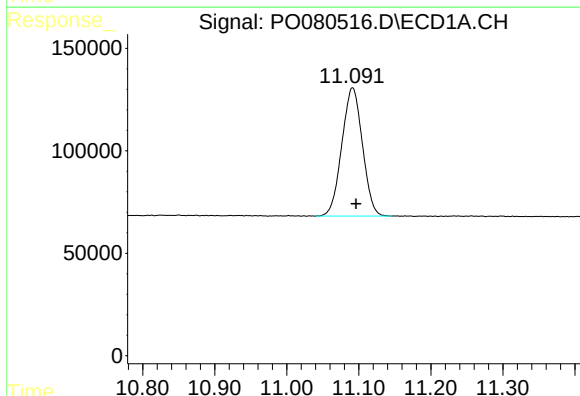


#2 Decachlorobiphenyl

R.T.: 11.091 min
Delta R.T.: -0.005 min
Response: 1243976
Conc: 24.03 ng/ml

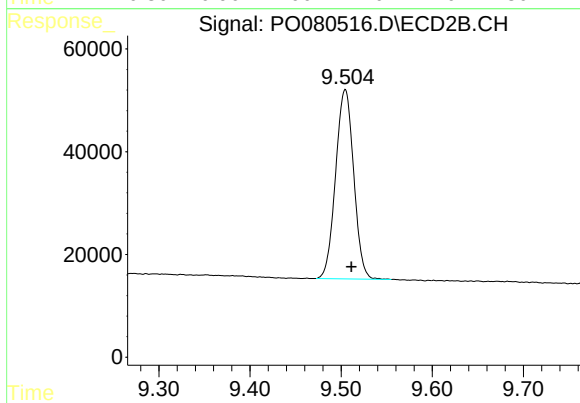

#2 Decachlorobiphenyl


R.T.: 9.505 min
Delta R.T.: -0.007 min
Response: 508223
Conc: 22.41 ng/ml

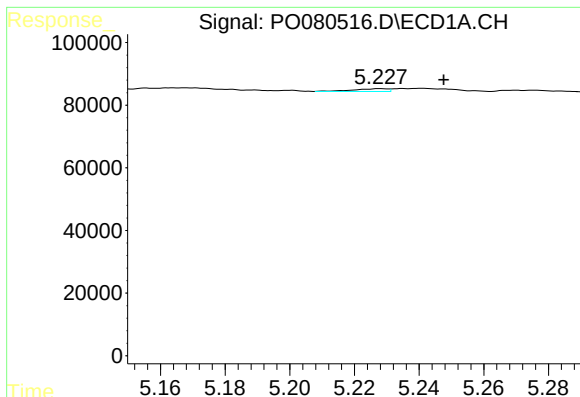

#8 AR-1221-1


R.T.: 5.228 min
Delta R.T.: -0.020 min
Response: 6598
Conc: 8.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

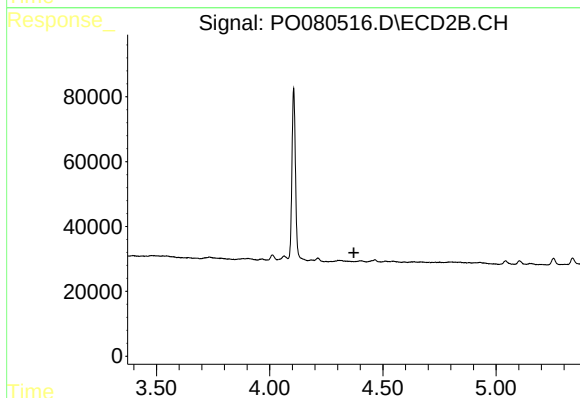


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.372 min
Response: 0
Conc: N.D.

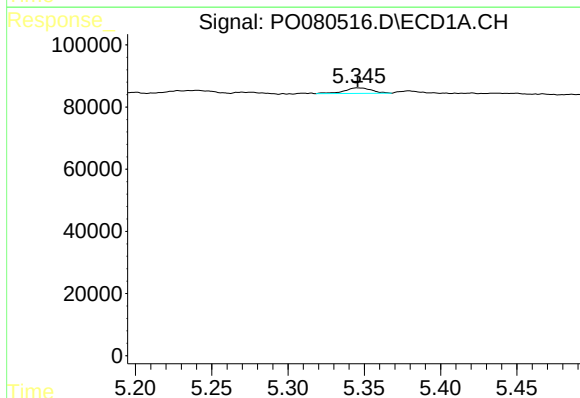


#9 AR-1221-2

R.T.: 5.345 min
Delta R.T.: 0.000 min
Response: 22381
Conc: 40.89 ng/ml

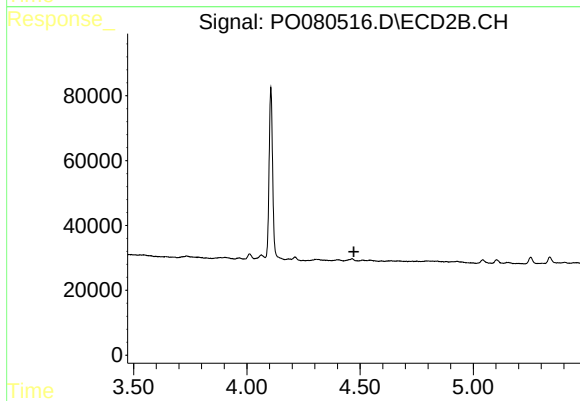

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.473 min
Response: 0
Conc: N.D.

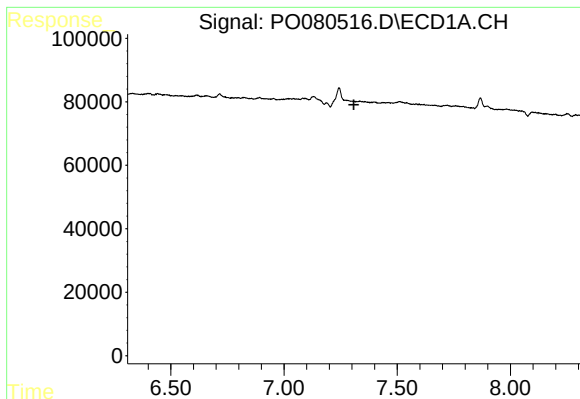

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.308 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

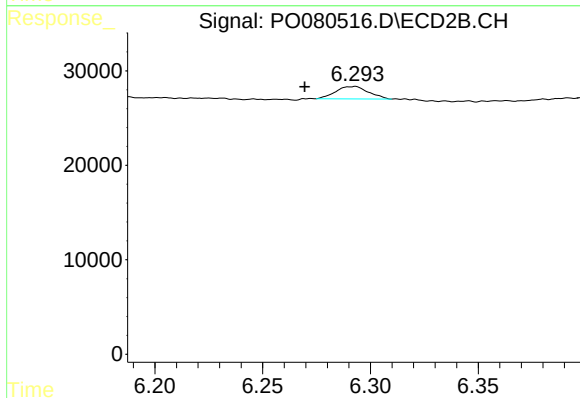


#20 AR-1242-5

R.T.: 6.293 min
Delta R.T.: 0.024 min
Response: 14117
Conc: 20.26 ng/ml

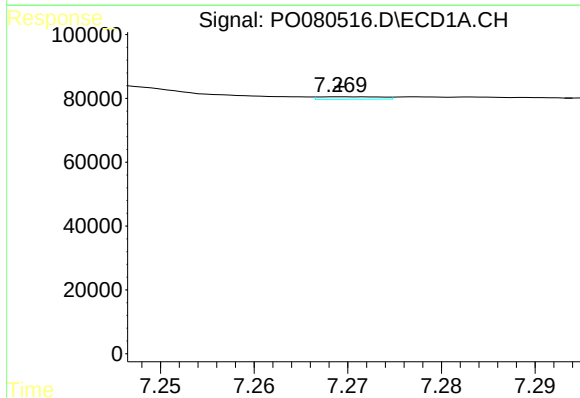


#24 AR-1248-4

R.T.: 7.269 min
Delta R.T.: 0.000 min
Response: 3617
Conc: 1.33 ng/ml

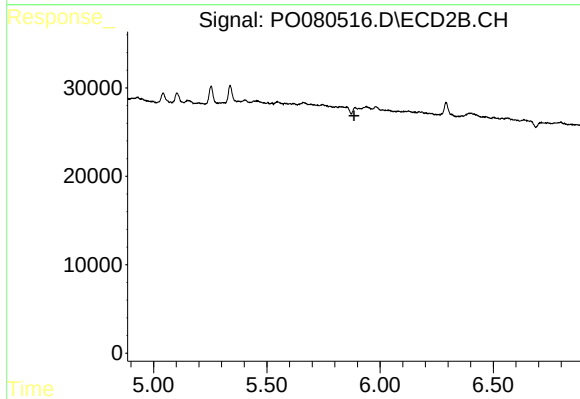

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.885 min
Response: 0
Conc: N.D.

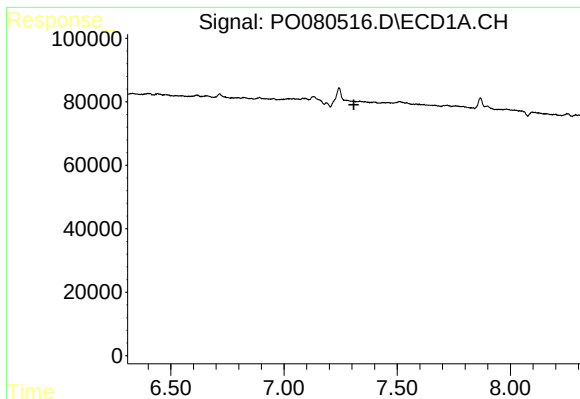

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.309 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

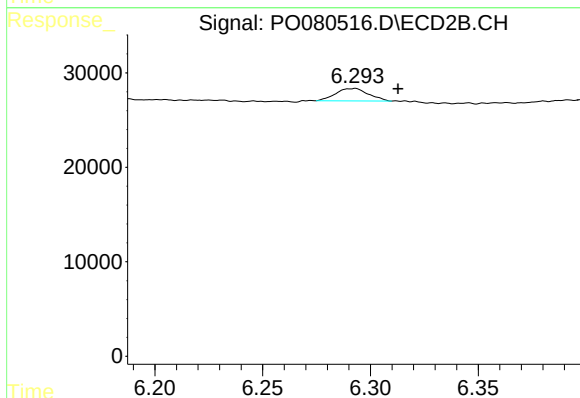


#25 AR-1248-5

R.T.: 6.293 min
Delta R.T.: -0.020 min
Response: 14117
Conc: 13.62 ng/ml

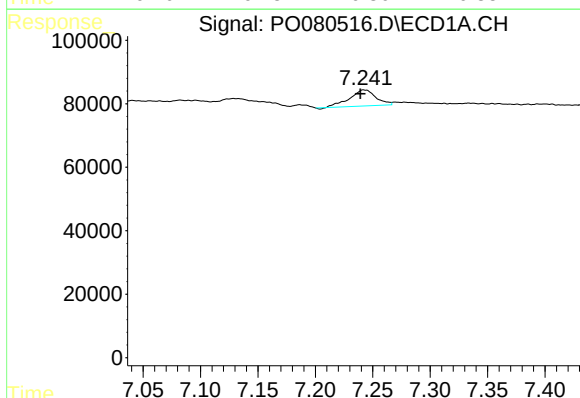


#26 AR-1254-1

R.T.: 7.242 min
Delta R.T.: 0.003 min
Response: 80415
Conc: 31.02 ng/ml

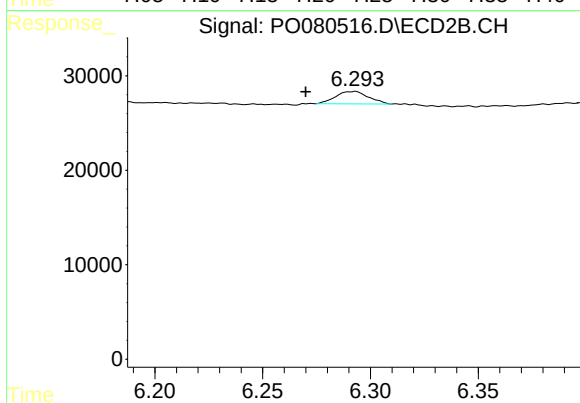

#26 AR-1254-1


R.T.: 6.293 min
Delta R.T.: 0.023 min
Response: 14117
Conc: 9.62 ng/ml

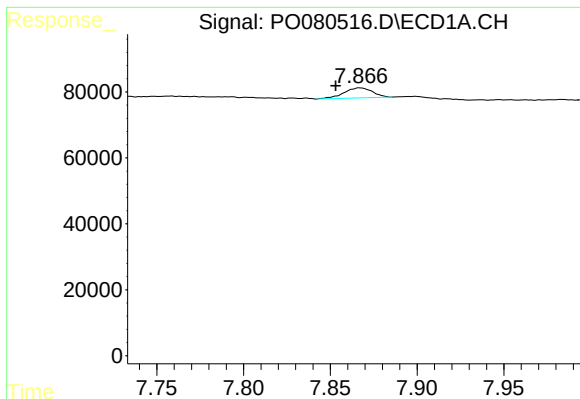

#28 AR-1254-3


R.T.: 7.867 min
Delta R.T.: 0.014 min
Response: 34889
Conc: 8.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

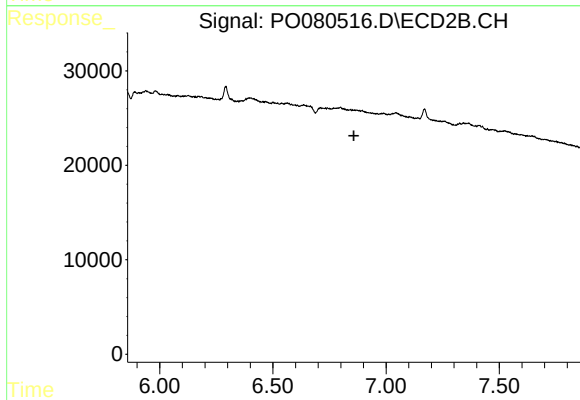


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.858 min
Response: 0
Conc: N.D.

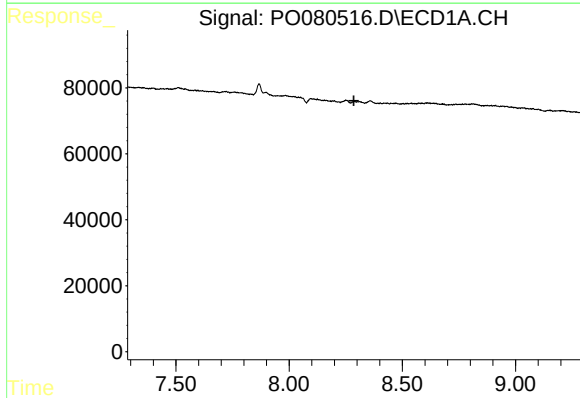

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

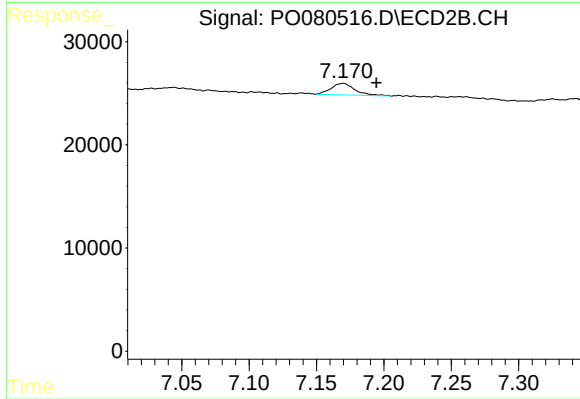

#32 AR-1260-2

R.T.: 7.170 min
Delta R.T.: -0.024 min
Response: 14083
Conc: 8.47 ng/ml