

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081621\
 Data File : PP038466.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Aug 2021 3:17
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 06:18:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.887	3.872	912433	536867	20.531	20.845
2) SA Decachlor...	10.873	9.133f	528589	563338	23.236	21.773
Target Compounds						
26) L6 AR-1254-1	7.121	0.000	34168	0	26.222	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081621\
Data File : PP038466.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2021 3:17
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 06:18:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

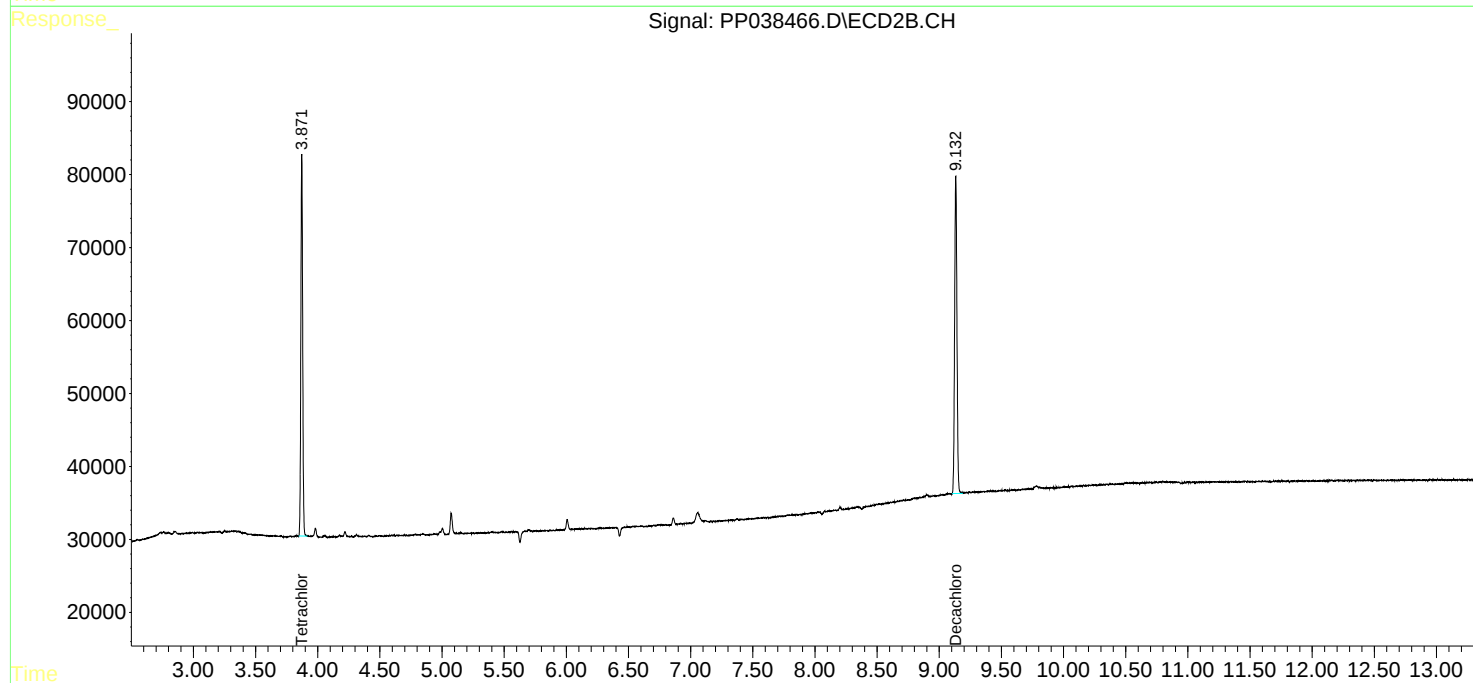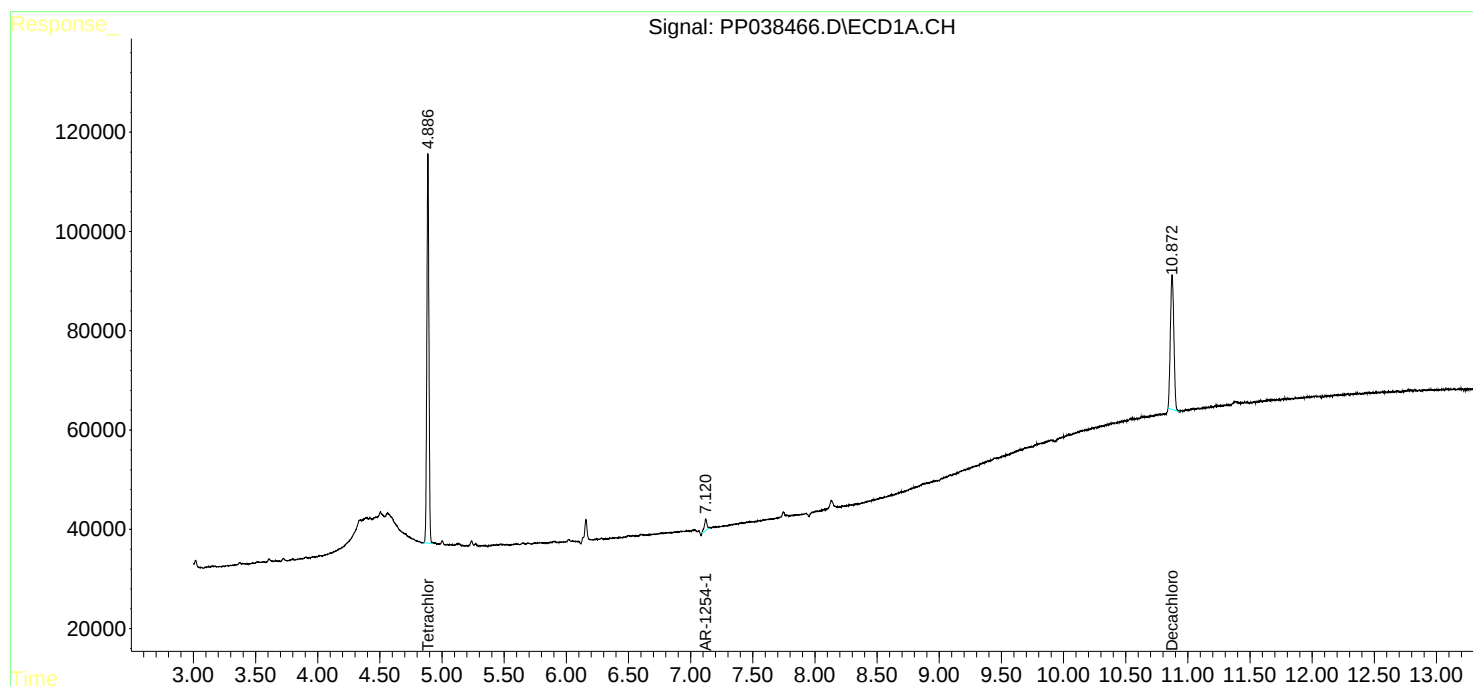


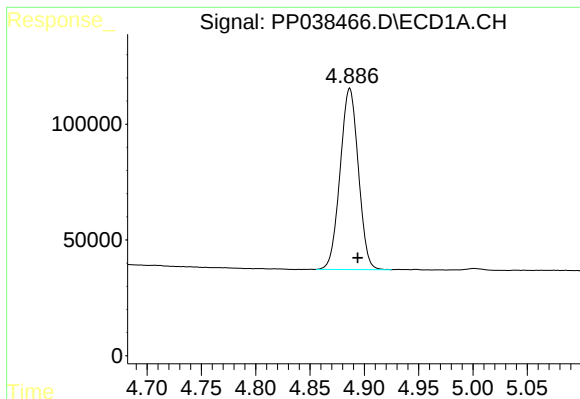

#1 Tetrachloro-m-xylene


R.T.: 4.887 min
Delta R.T.: -0.007 min
Response: 912433
Conc: 20.53 ng/ml

Instrument :
ECD_O
ClientSampleId :

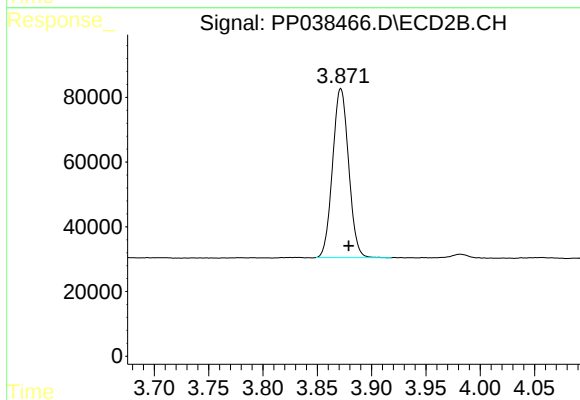


#1 Tetrachloro-m-xylene

R.T.: 3.872 min
Delta R.T.: -0.007 min
Response: 536867
Conc: 20.84 ng/ml

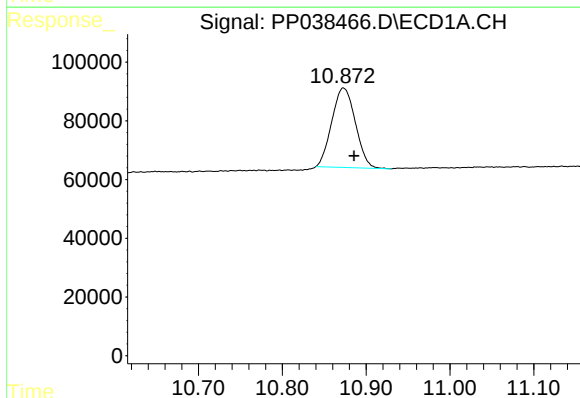


#2 Decachlorobiphenyl

R.T.: 10.873 min
Delta R.T.: -0.013 min
Response: 528589
Conc: 23.24 ng/ml

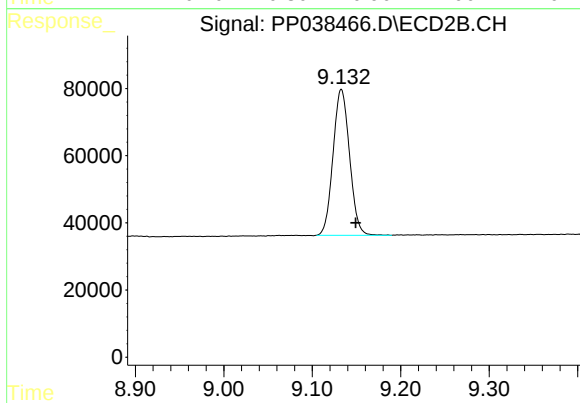

#2 Decachlorobiphenyl


R.T.: 9.133 min
Delta R.T.: -0.016 min
Response: 563338
Conc: 21.77 ng/ml

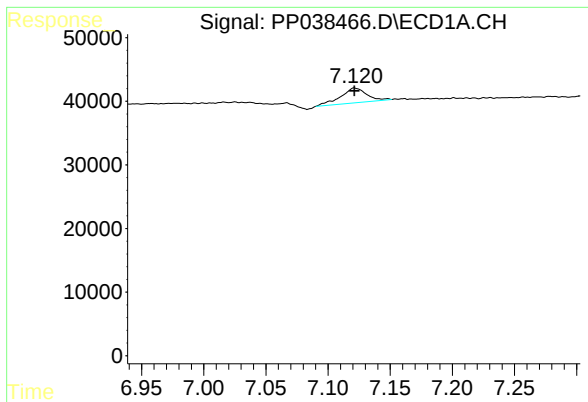

#26 AR-1254-1

R.T.: 7.121 min
Delta R.T.: 0.000 min
Response: 34168
Conc: 26.22 ng/ml

Instrument :
ECD_O
ClientSampleId :

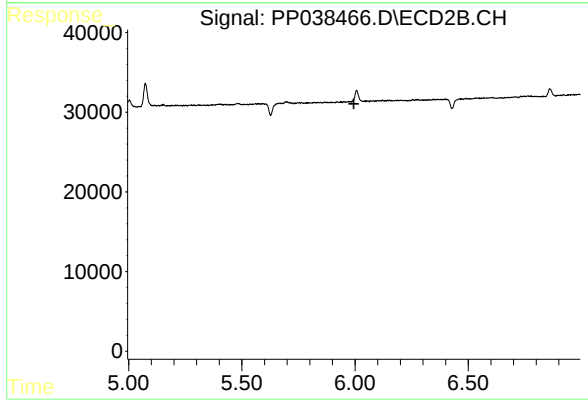

#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.995 min
Response: 0
Conc: N.D.