

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081621\
 Data File : P0080454.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Aug 2021 10:22
 Operator : DD\AJ
 Sample : M3407-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 25S

Manual Integrations
 APPROVED

mohammad
 8/17/2021 12:43:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 01:44:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.991	4.107	1236537	396005	17.857m	15.889
2) SA Decachlor...	11.092	9.505	379369	154833	7.329	6.826

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081621\
Data File : PO080454.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Aug 2021 10:22
Operator : DD\AJ
Sample : M3407-05
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
25S


Manual Integrations
APPROVED

mohammad
8/17/2021 12:43:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 01:44:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

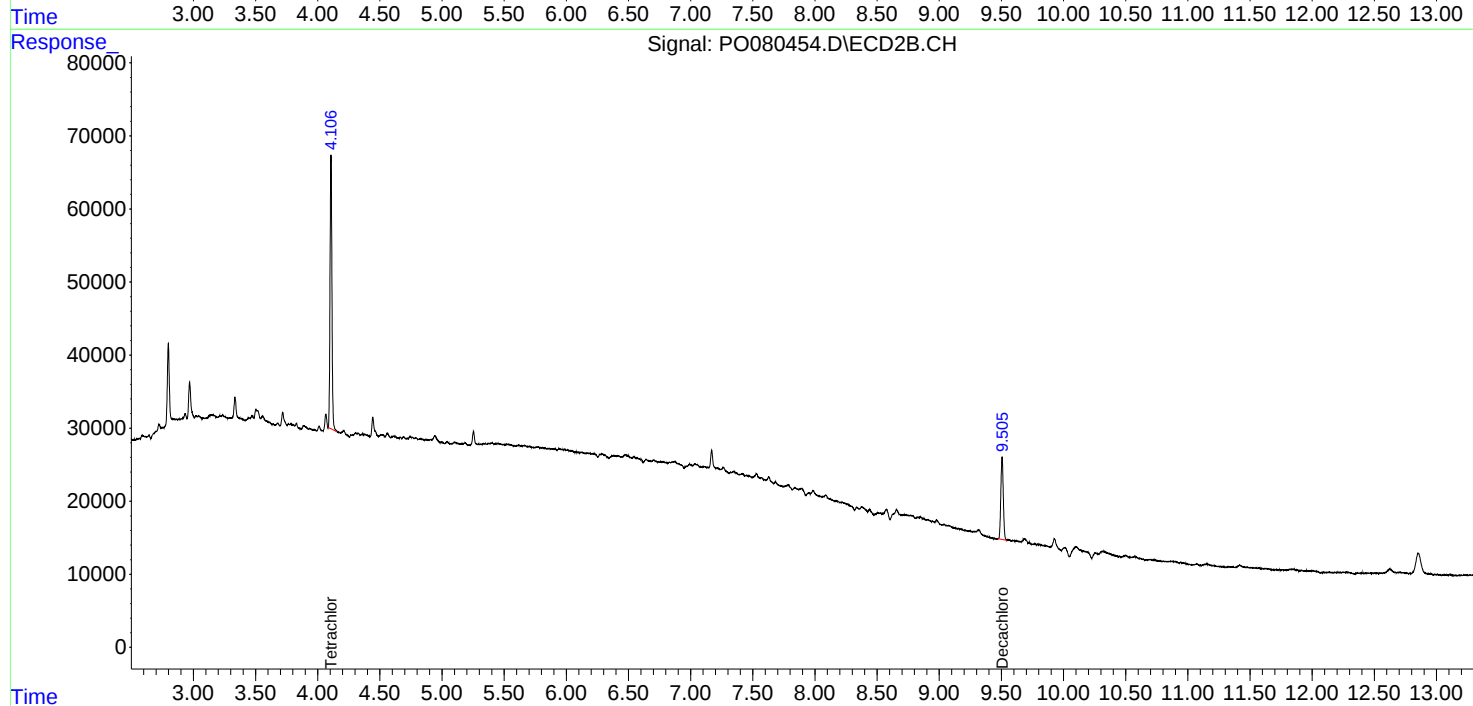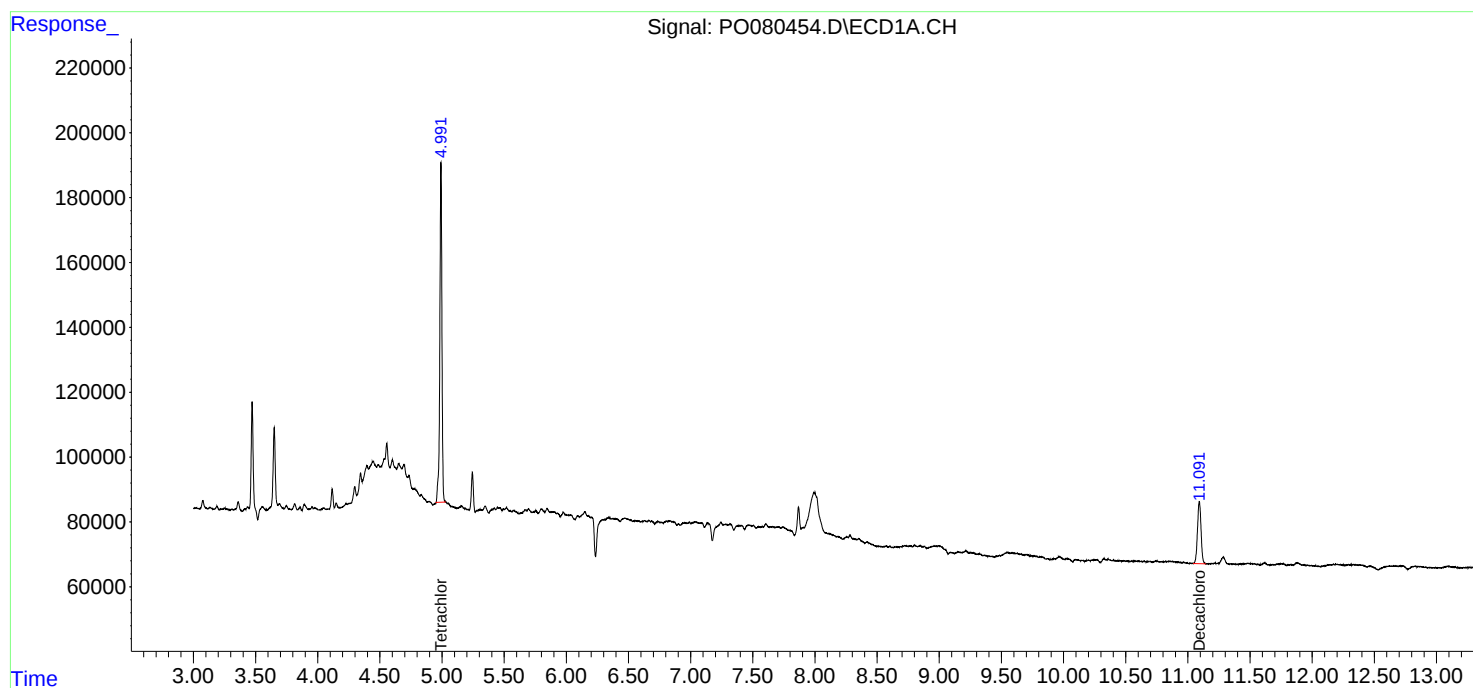

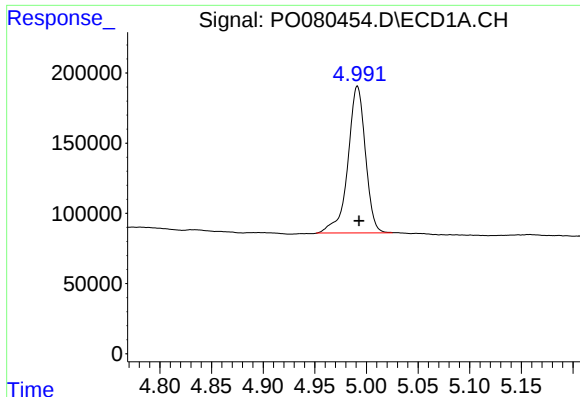


#1 Tetrachloro-m-xylene

R.T.: 4.991 min
Delta R.T.: -0.002 min
Response: 1236537
Conc: 17.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
25S


Manual Integrations
APPROVED

mohammad
8/17/2021 12:43:44 PM

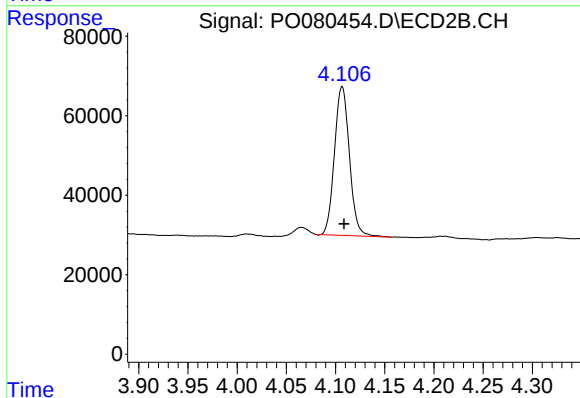


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: -0.002 min
Response: 396005
Conc: 15.89 ng/ml

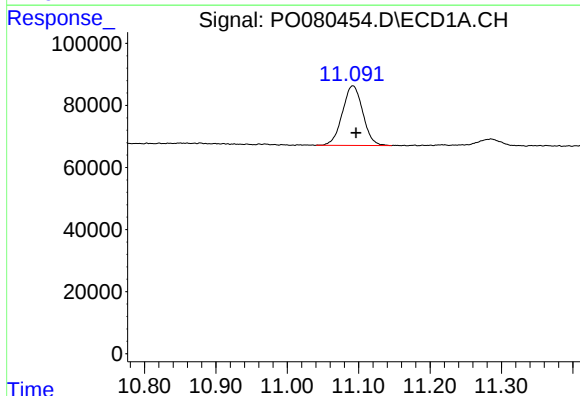

#2 Decachlorobiphenyl

R.T.: 11.092 min
Delta R.T.: -0.005 min
Response: 379369
Conc: 7.33 ng/ml

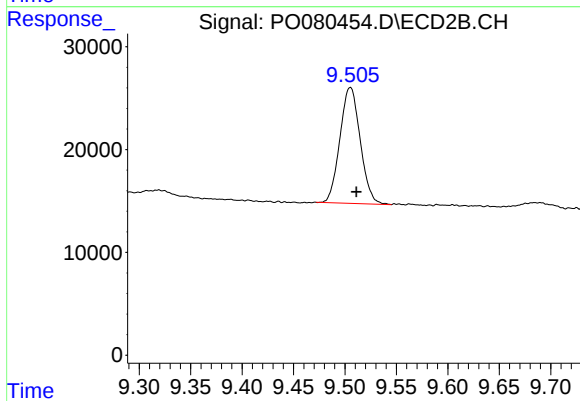

#2 Decachlorobiphenyl

R.T.: 9.505 min
Delta R.T.: -0.006 min
Response: 154833
Conc: 6.83 ng/ml