

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081622\
 Data File : P0089040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2022 19:23
 Operator : YP/AJ
 Sample : N4198-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GFD-TOTES

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/17/2022
 Supervised By :Ankita Jodhani 08/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 00:11:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.434	3.595	51346444	24989041	19.036m	23.089
2) SA Decachlor...	10.270	8.580	37531292	19255396	19.449	15.888

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081622\
Data File : PO089040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2022 19:23
Operator : YP/AJ
Sample : N4198-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
GFD-TOTES


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/17/2022
Supervised By :Ankita Jodhani 08/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 00:11:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

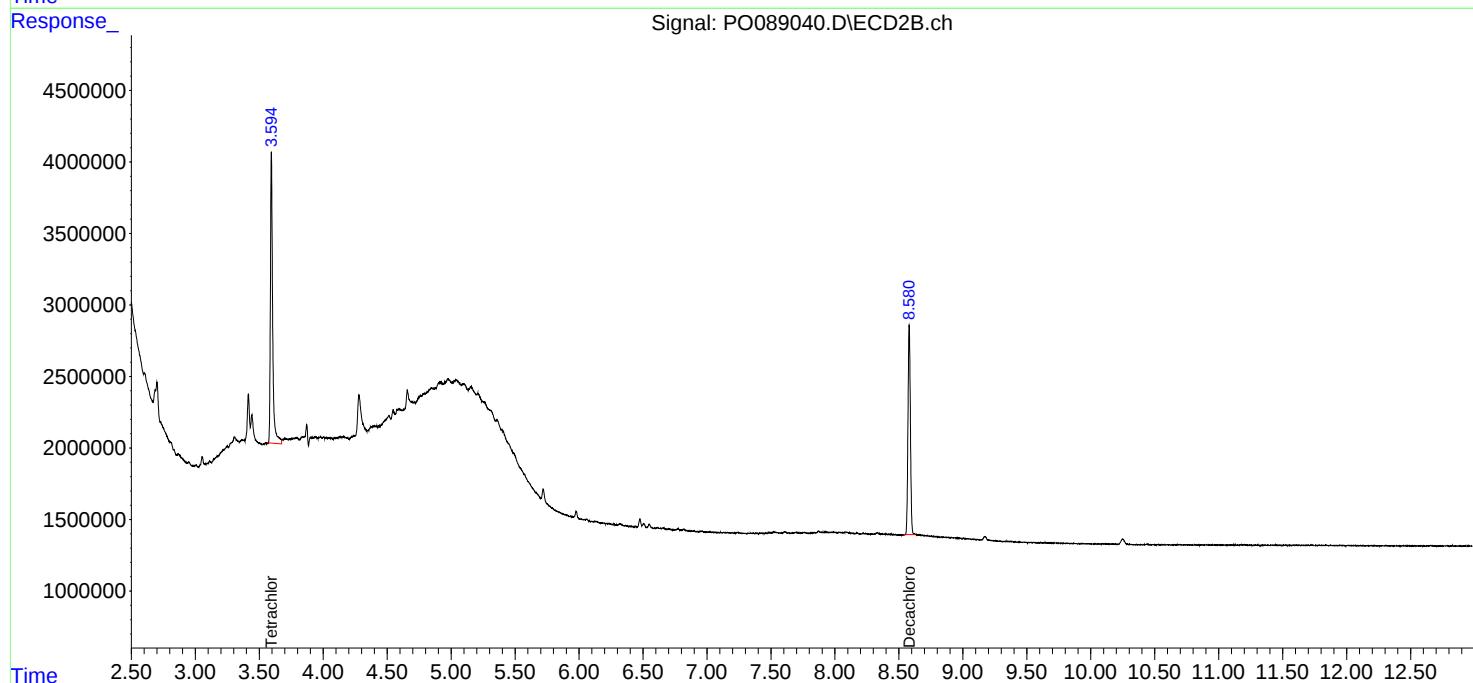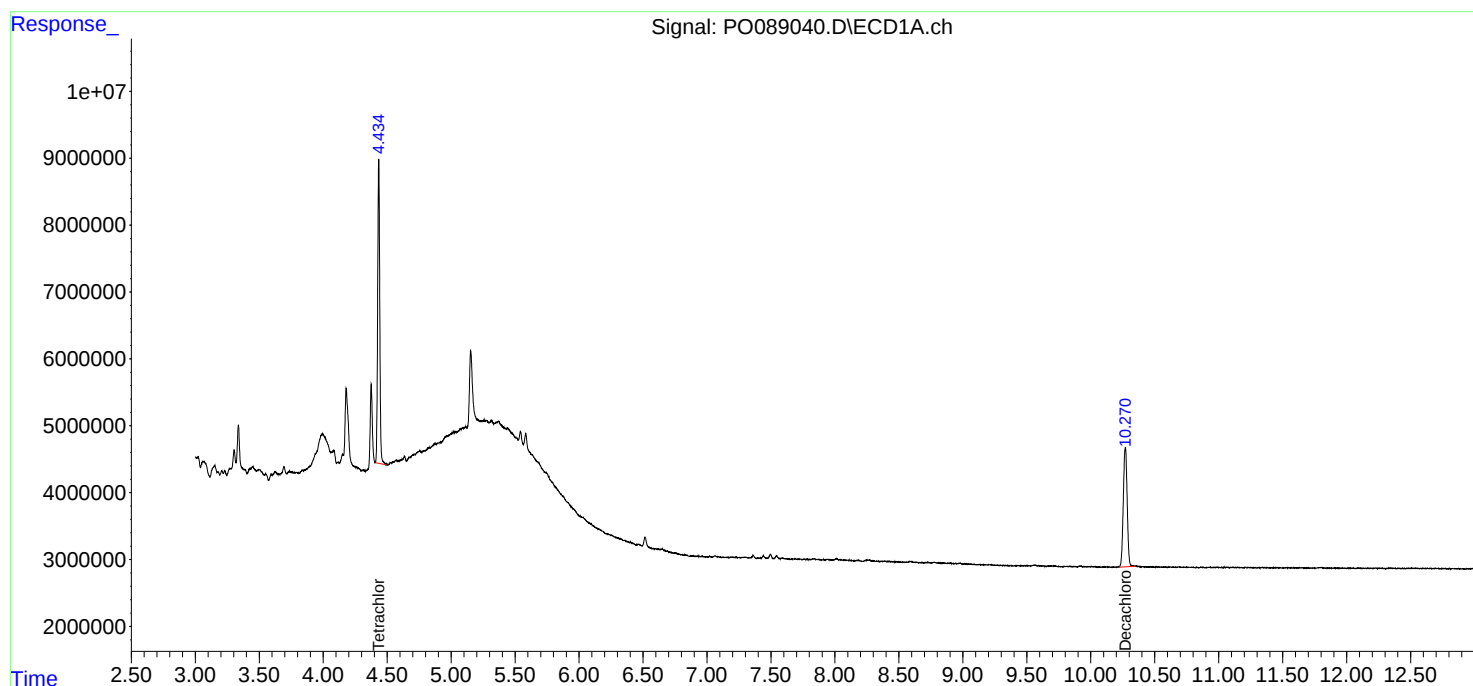

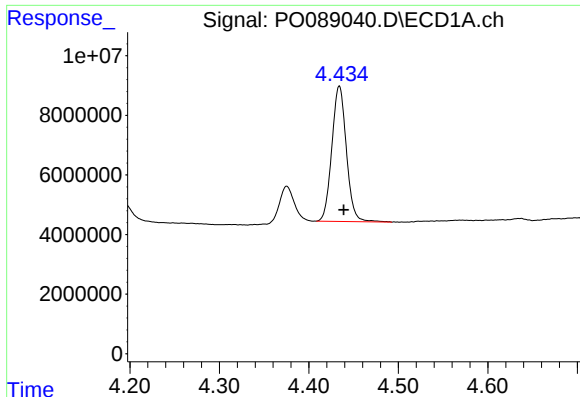


#1 Tetrachloro-m-xylene

R.T.: 4.434 min
Delta R.T.: -0.005 min
Response: 51346444
Conc: 19.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
GFD-TOTES


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/17/2022
Supervised By :Ankita Jodhani 08/17/2022

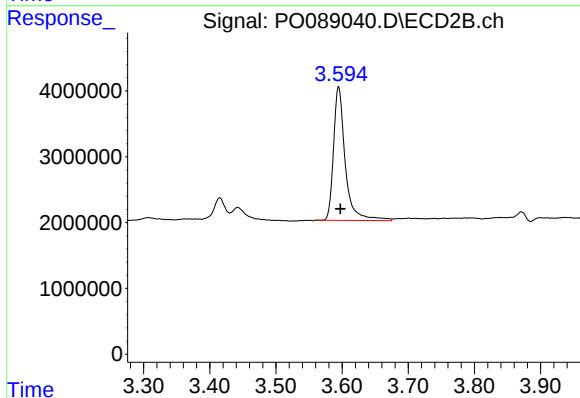


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: -0.002 min
Response: 24989041
Conc: 23.09 ng/ml

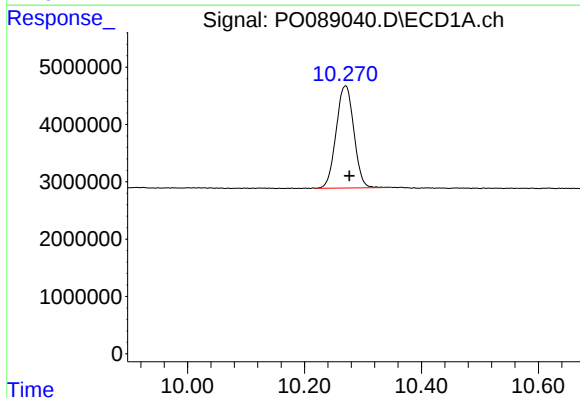

#2 Decachlorobiphenyl

R.T.: 10.270 min
Delta R.T.: -0.007 min
Response: 37531292
Conc: 19.45 ng/ml

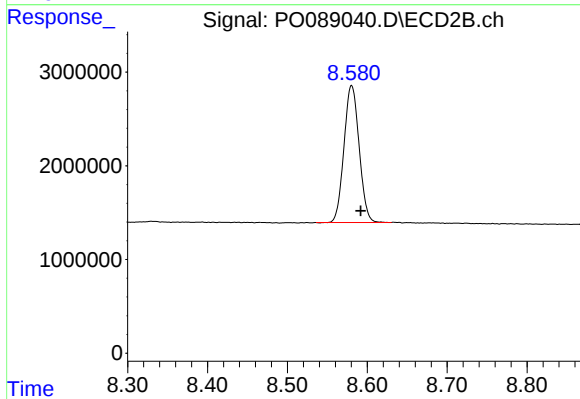

#2 Decachlorobiphenyl

R.T.: 8.580 min
Delta R.T.: -0.011 min
Response: 19255396
Conc: 15.89 ng/ml