

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081624\
 Data File : P0105603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2024 15:16
 Operator : YP/AJ
 Sample : P3617-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VCPS-B5-081424-0-10

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2024
 Supervised By :Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 05:45:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 11:44:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.454	3.727	172.7E6	44206648	18.474m	17.332
2) SA Decachlor...	10.199	8.774	77679147	28828344	13.382	14.608

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081624\
Data File : PO105603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2024 15:16
Operator : YP/AJ
Sample : P3617-12
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VCPS-B5-081424-0-10


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2024
Supervised By :Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 05:45:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 11:44:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

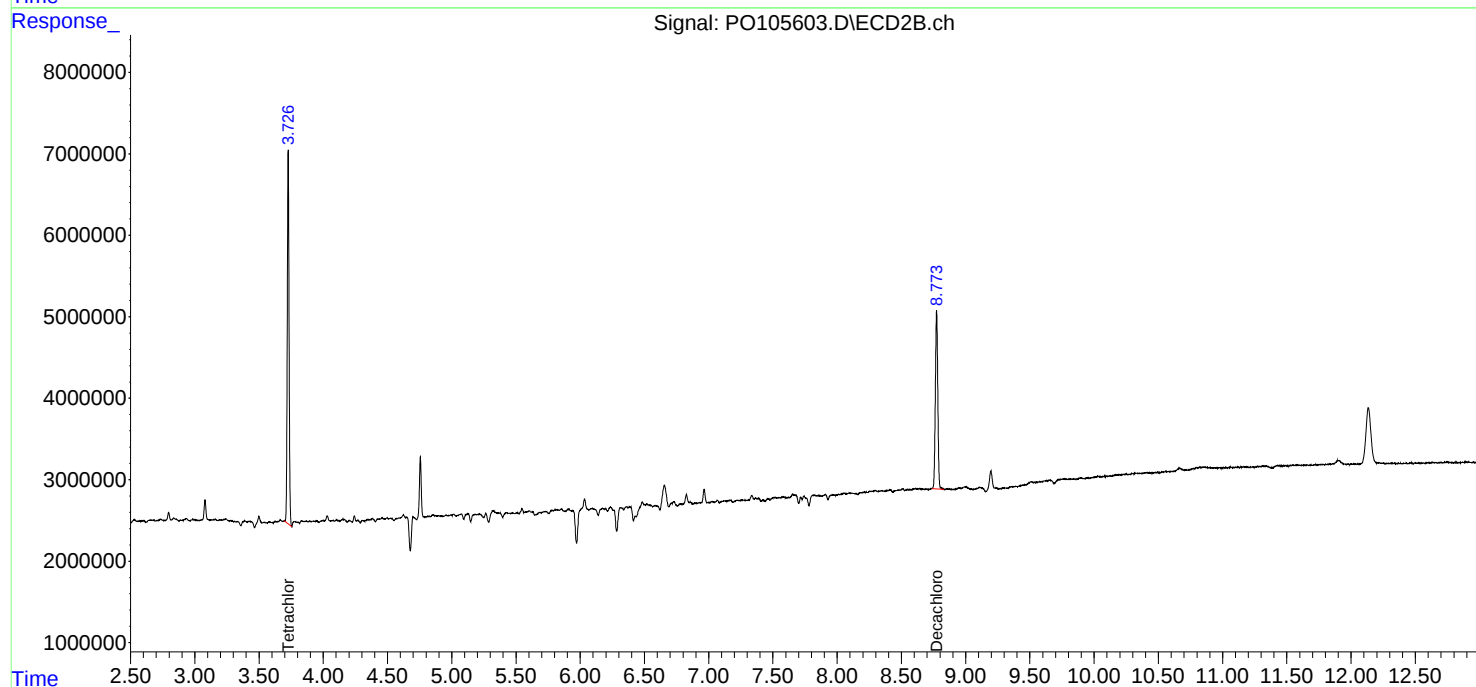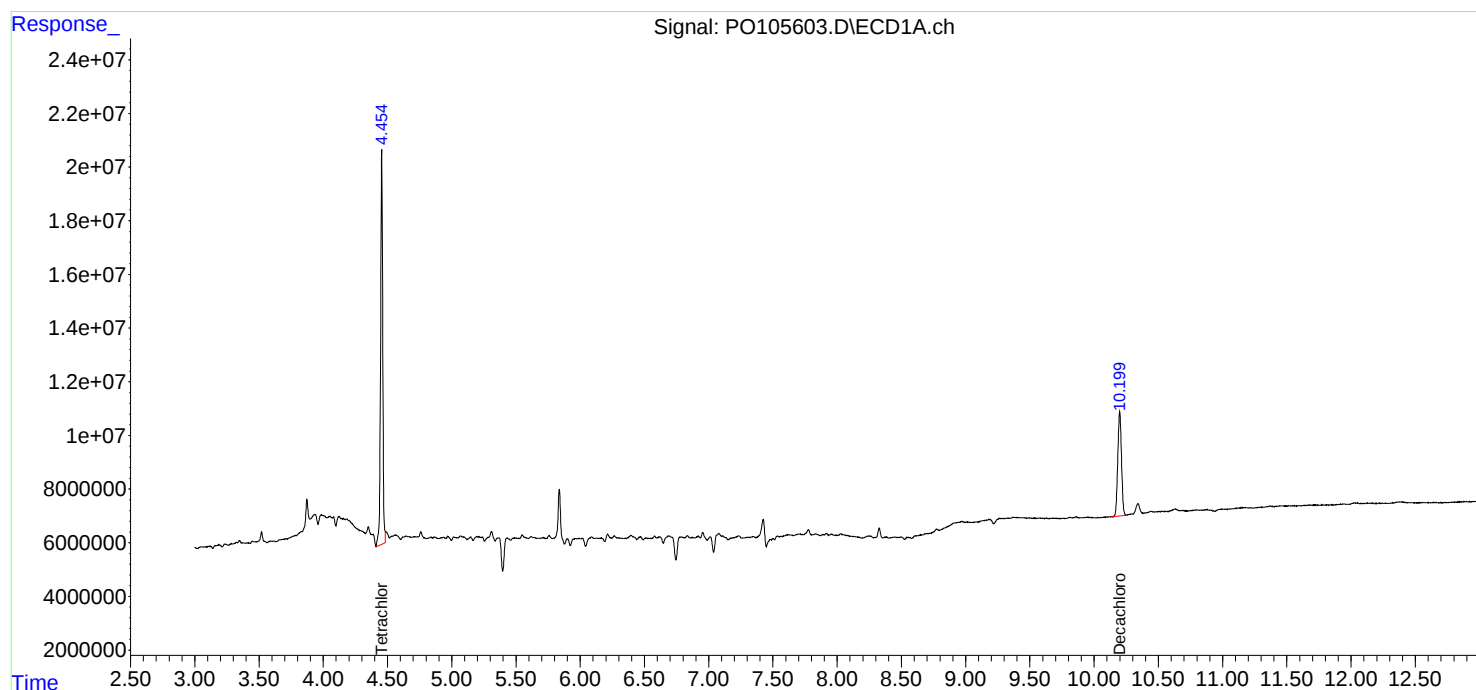

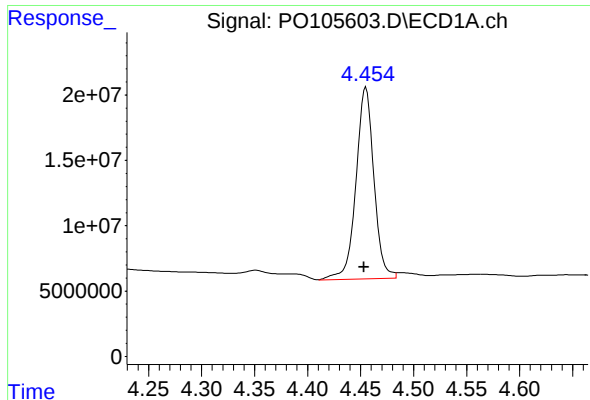


#1 Tetrachloro-m-xylene

R.T.: 4.454 min
Delta R.T.: 0.001 min
Response: 172717627
Conc: 18.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
VCPS-B5-081424-0-10


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2024
Supervised By :Ankita Jodhani 08/19/2024

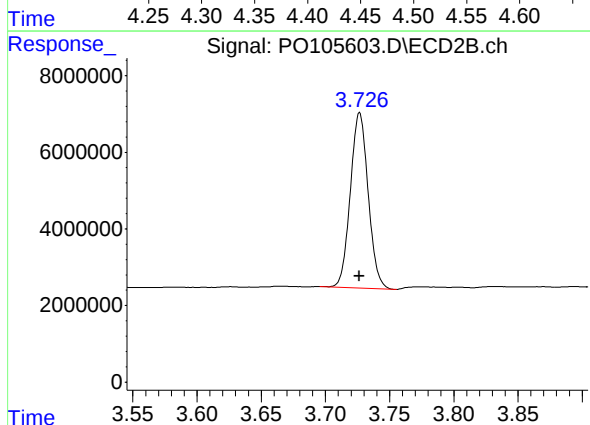


#1 Tetrachloro-m-xylene

R.T.: 3.727 min
Delta R.T.: 0.000 min
Response: 44206648
Conc: 17.33 ng/ml

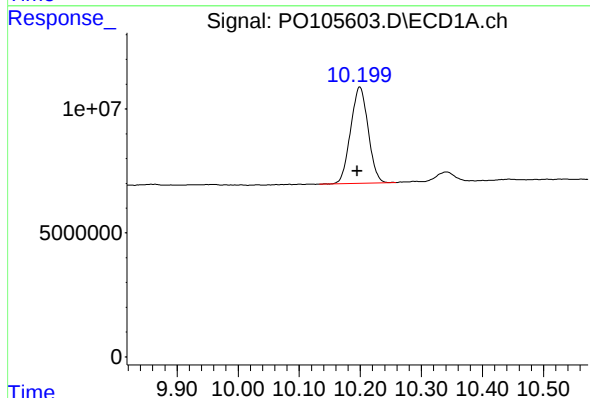

#2 Decachlorobiphenyl

R.T.: 10.199 min
Delta R.T.: 0.004 min
Response: 77679147
Conc: 13.38 ng/ml

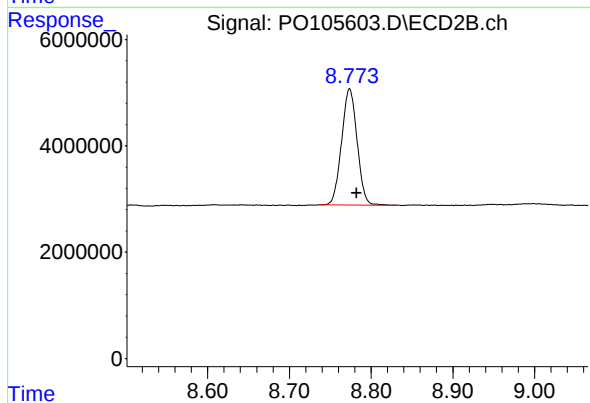

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: -0.009 min
Response: 28828344
Conc: 14.61 ng/ml