

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081624\
 Data File : P0105616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2024 20:18
 Operator : YP/AJ
 Sample : P3634-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-06-08152024

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2024
 Supervised By :Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 05:52:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 11:44:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.454	3.726	160.7E6	47371928	17.187m	18.573
2) SA Decachlor...	10.199	8.772	91037476	30326989	15.683	15.367

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081624\
Data File : PO105616.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2024 20:18
Operator : YP/AJ
Sample : P3634-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-06-08152024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2024
Supervised By :Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 05:52:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 11:44:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

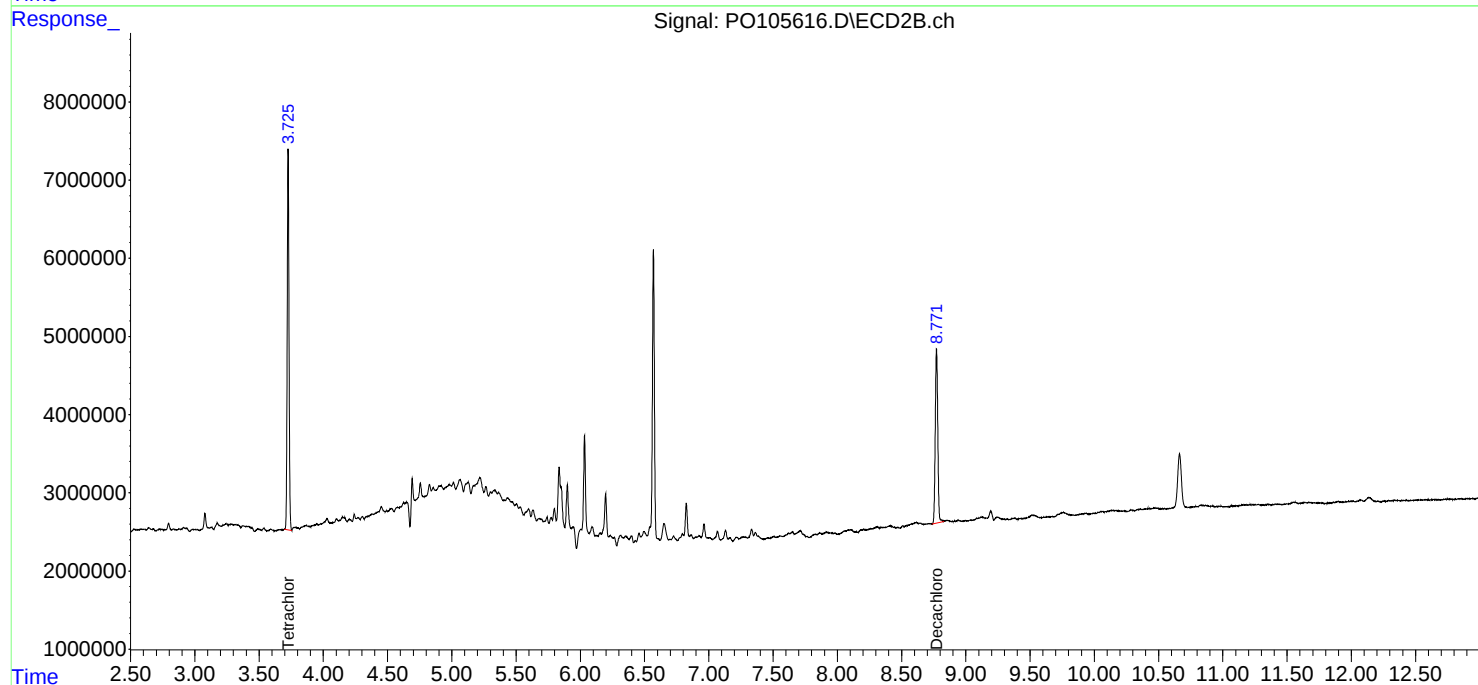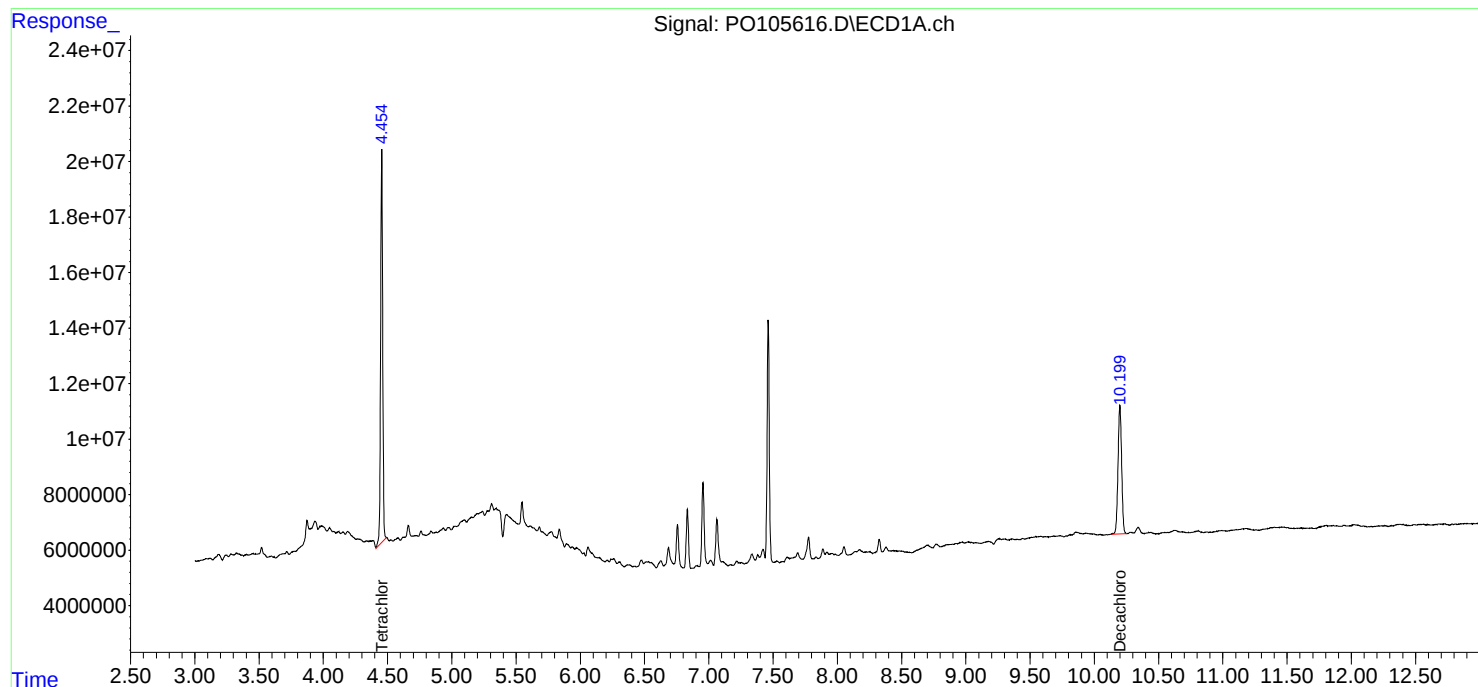

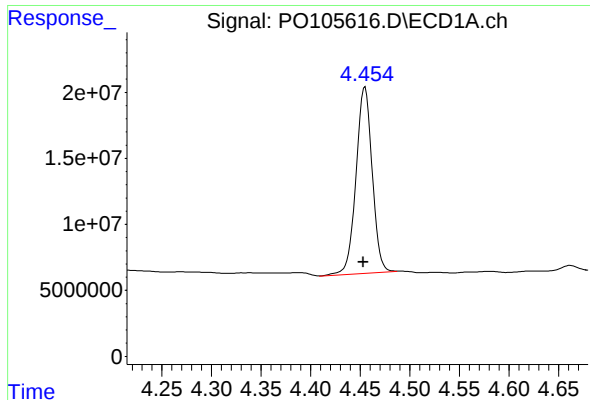


#1 Tetrachloro-m-xylene

R.T.: 4.454 min
Delta R.T.: 0.001 min
Response: 160682067
Conc: 17.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-06-08152024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2024
Supervised By :Ankita Jodhani 08/19/2024

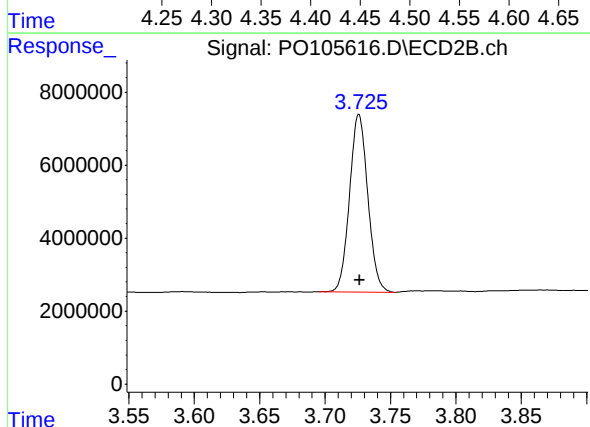


#1 Tetrachloro-m-xylene

R.T.: 3.726 min
Delta R.T.: 0.000 min
Response: 47371928
Conc: 18.57 ng/ml

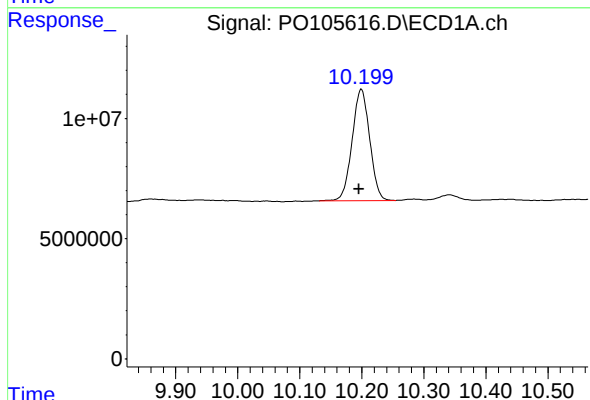

#2 Decachlorobiphenyl

R.T.: 10.199 min
Delta R.T.: 0.004 min
Response: 91037476
Conc: 15.68 ng/ml

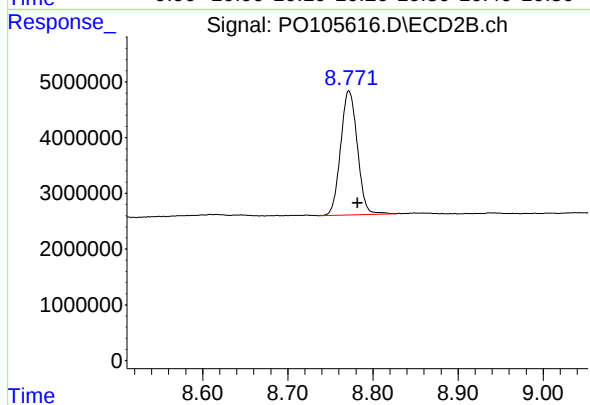

#2 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: -0.010 min
Response: 30326989
Conc: 15.37 ng/ml