

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0081718\
Data File : P0048233.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2018 18:34
Operator : SM/SJ
Sample : J4516-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ND-BASELINE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 02:57:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.389	3.633	3470958	4814740	17.192	19.595
2) SA Decachlor...	10.075	8.614	2666200	2600445	16.347	16.543

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0081718\
Data File : P0048233.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2018 18:34
Operator : SM/SJ
Sample : J4516-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ND-BASELINE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 02:57:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

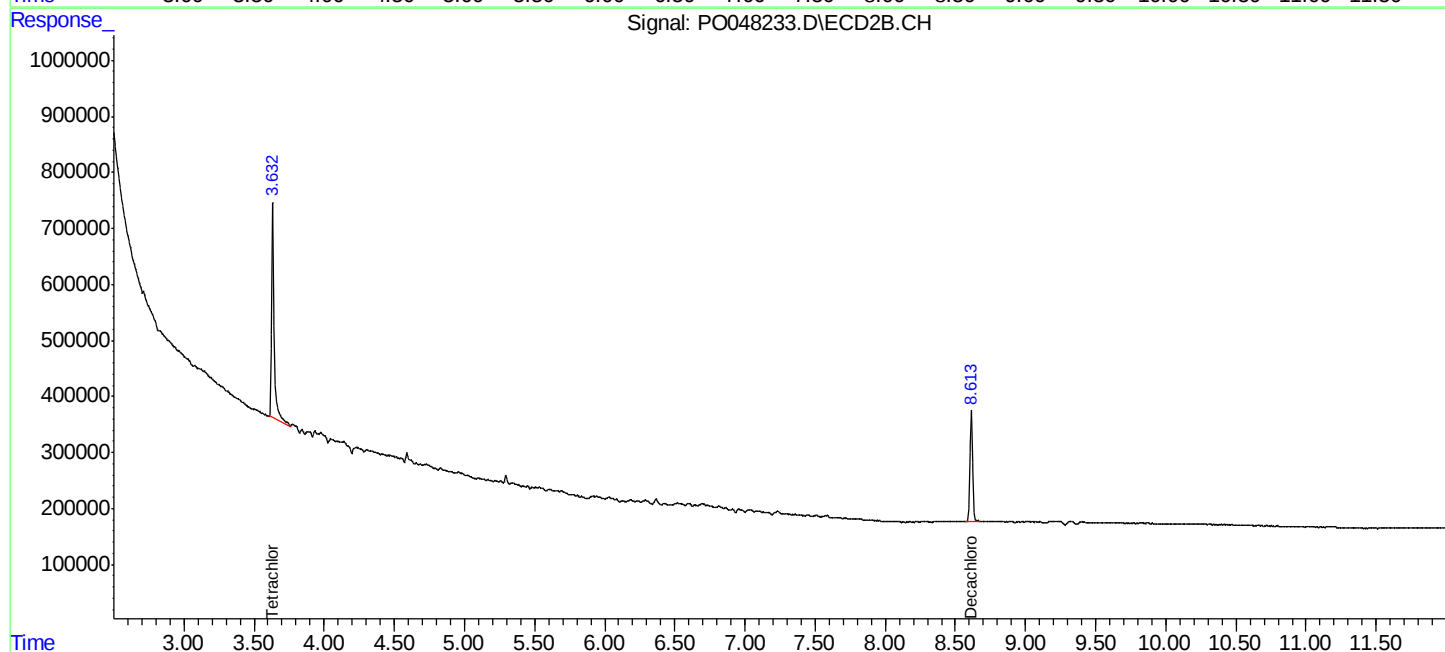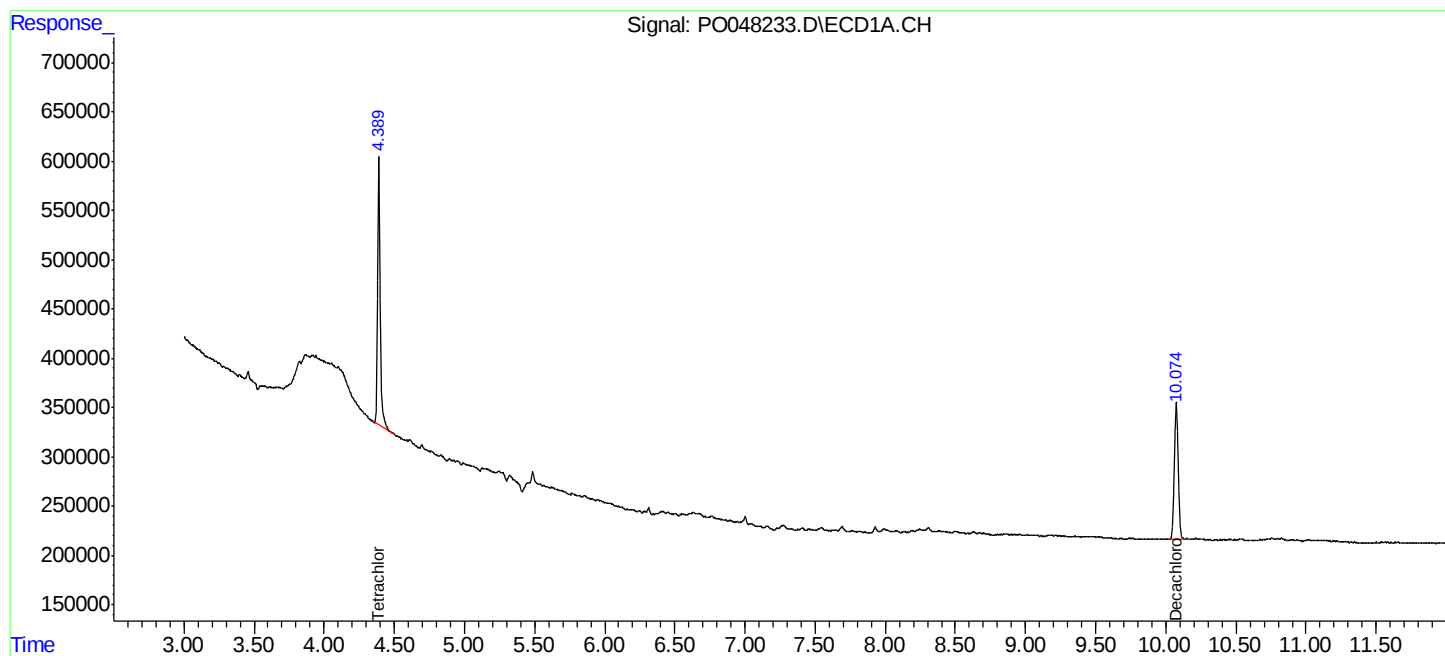


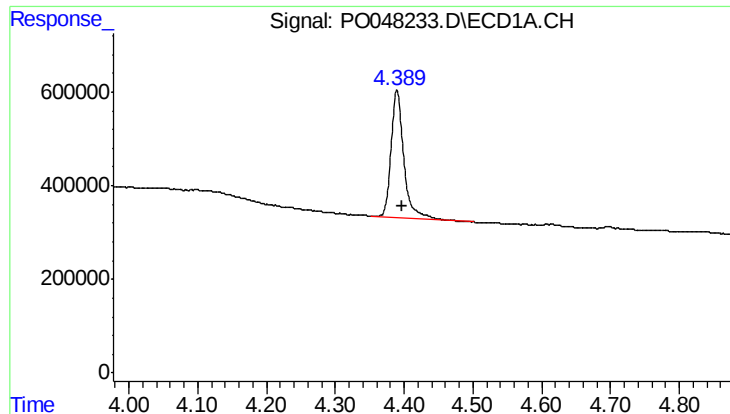

#1 Tetrachloro-m-xylene


R.T.: 4.389 min
Delta R.T.: -0.008 min
Response: 3470958
Conc: 17.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
ND-BASELINE-WATER

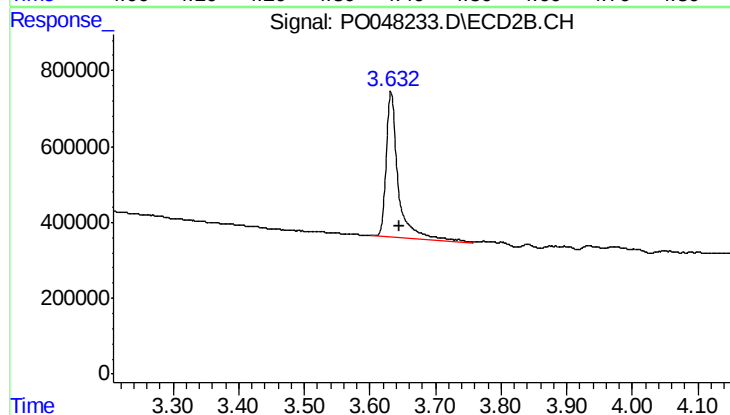


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: -0.013 min
Response: 4814740
Conc: 19.59 ng/ml

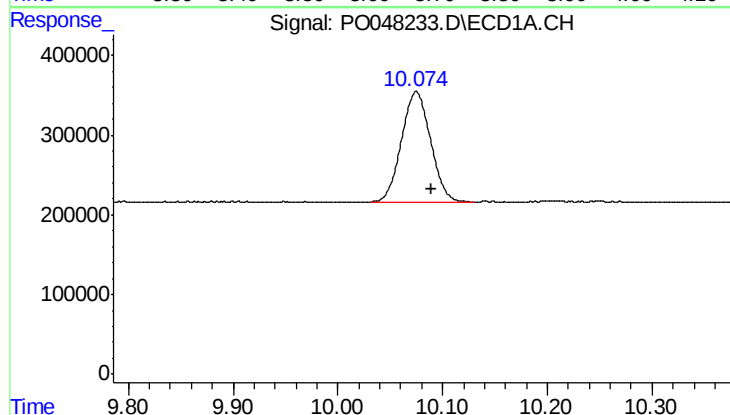

#2 Decachlorobiphenyl

R.T.: 10.075 min
Delta R.T.: -0.015 min
Response: 2666200
Conc: 16.35 ng/ml

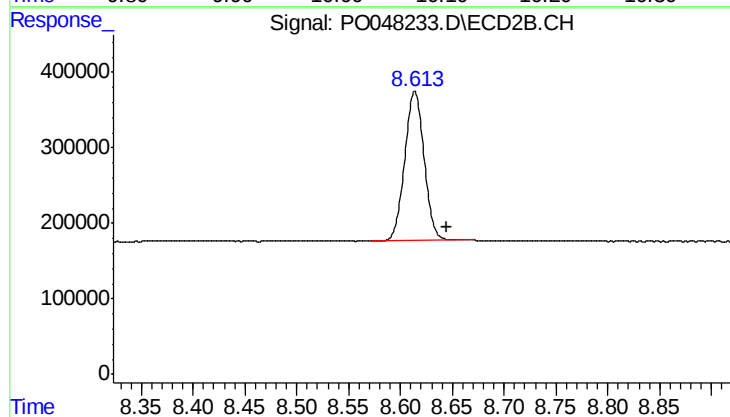

#2 Decachlorobiphenyl

R.T.: 8.614 min
Delta R.T.: -0.031 min
Response: 2600445
Conc: 16.54 ng/ml