

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081719\
Data File : P0059446.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2019 10:26
Operator : SM/SJ
Sample : K4277-13
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-22

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 23:36:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.146	3.509	936798	846367	26.756	23.513
2) SA Decachlor...	9.633	8.381	1033927	806640	19.435	20.005

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081719\
Data File : P0059446.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2019 10:26
Operator : SM/SJ
Sample : K4277-13
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-22

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 23:36:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

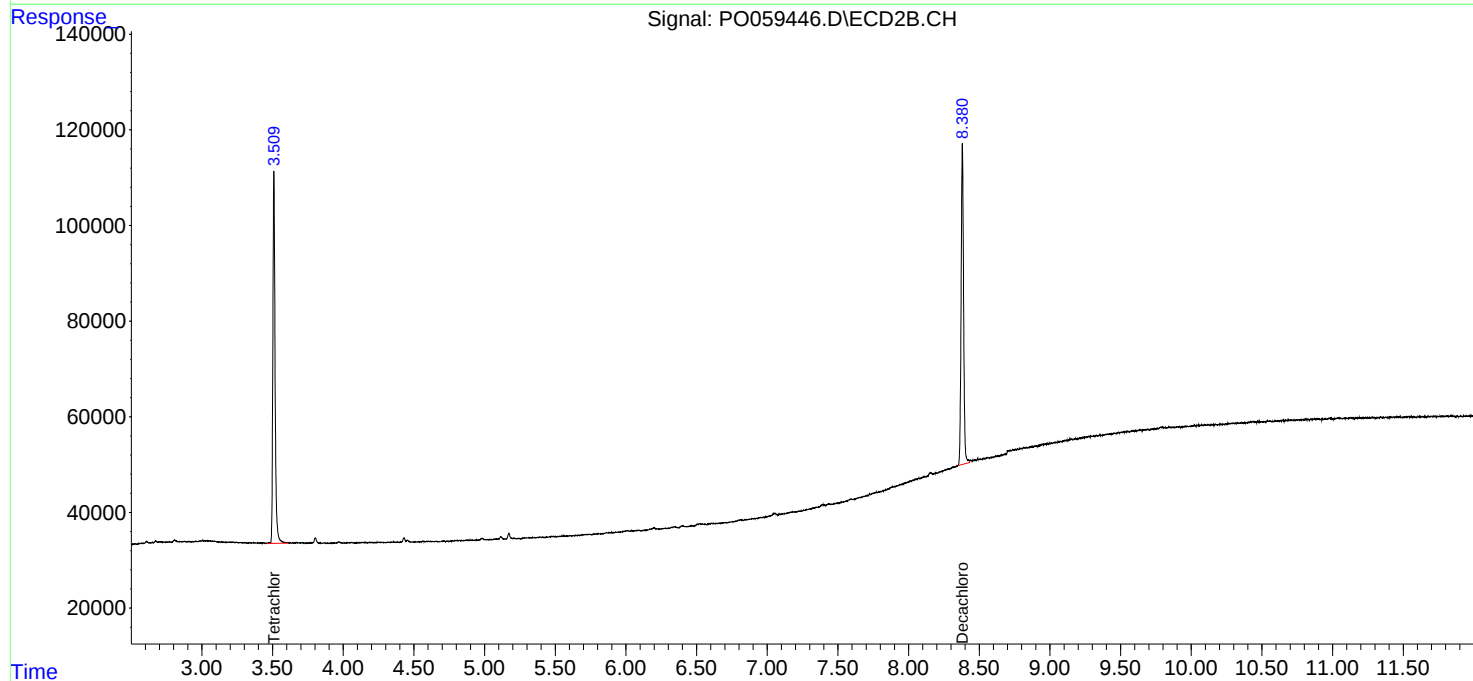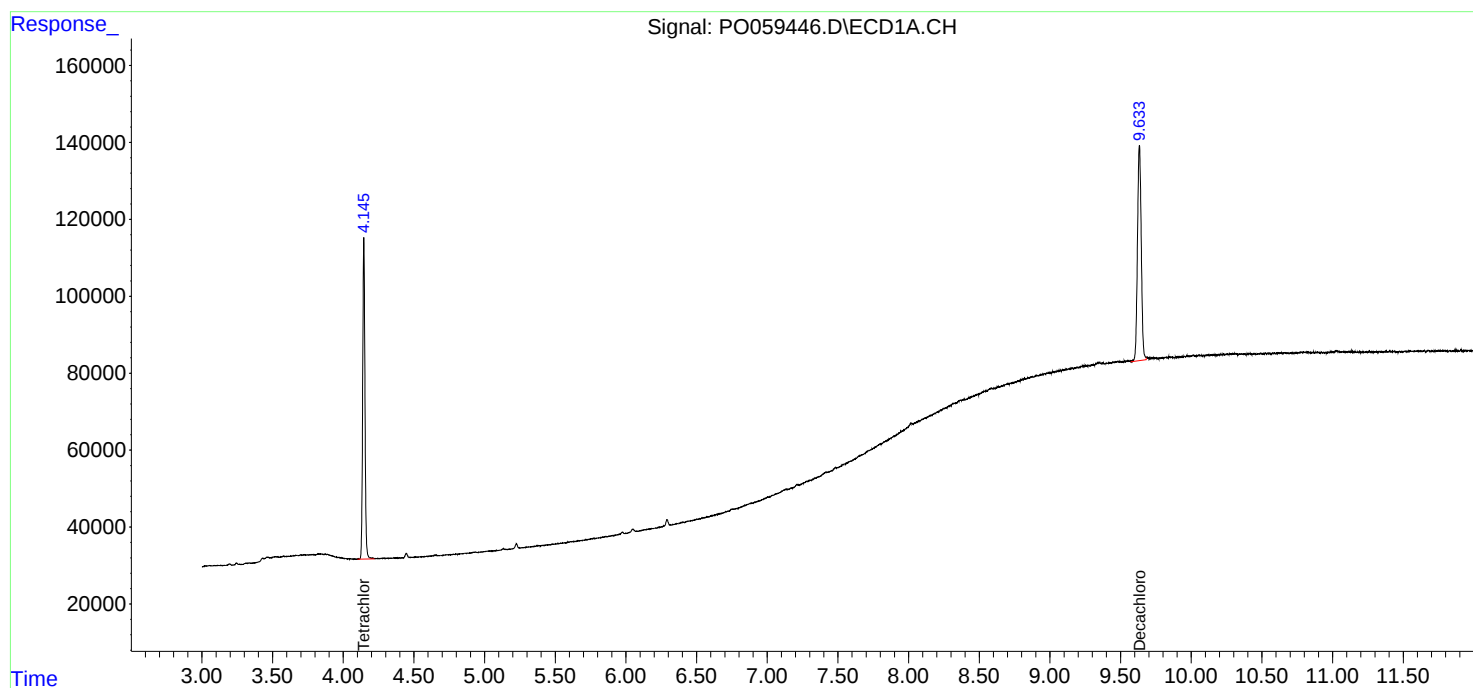


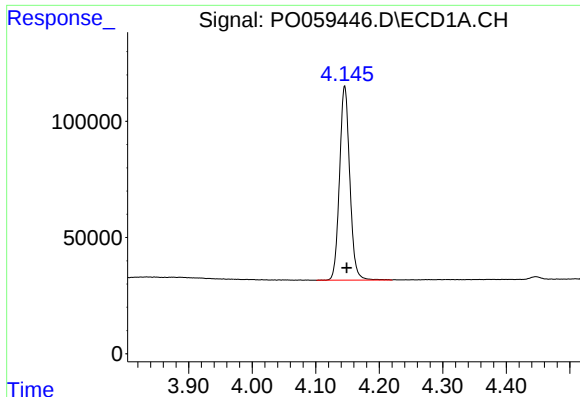

#1 Tetrachloro-m-xylene


R.T.: 4.146 min
Delta R.T.: -0.003 min
Response: 936798
Conc: 26.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-22

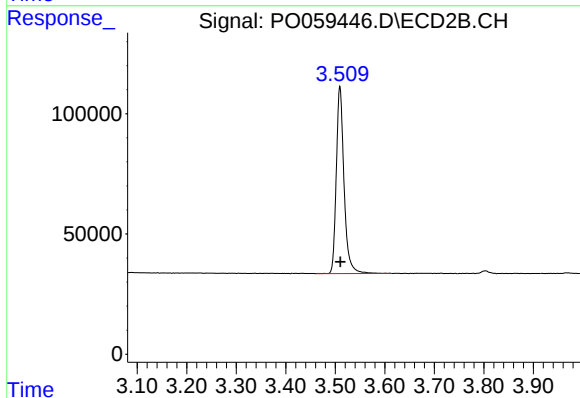


#1 Tetrachloro-m-xylene

R.T.: 3.509 min
Delta R.T.: 0.000 min
Response: 846367
Conc: 23.51 ng/ml

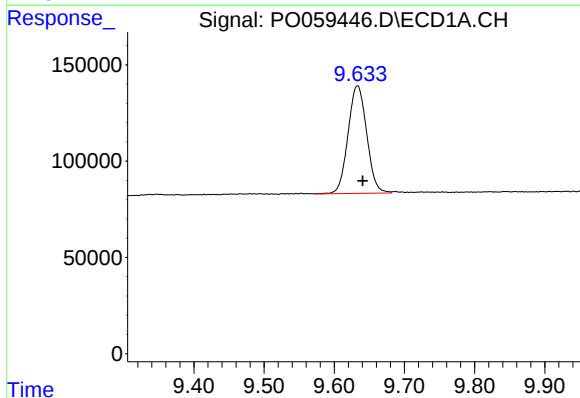

#2 Decachlorobiphenyl

R.T.: 9.633 min
Delta R.T.: -0.008 min
Response: 1033927
Conc: 19.43 ng/ml

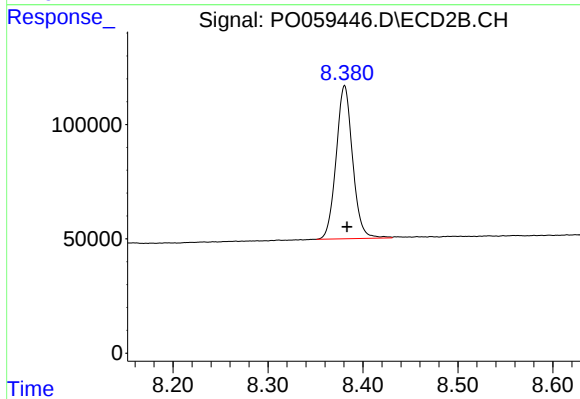

#2 Decachlorobiphenyl

R.T.: 8.381 min
Delta R.T.: -0.003 min
Response: 806640
Conc: 20.01 ng/ml