

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081720\
 Data File : P0070603.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Aug 2020 13:56
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 14:15:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.367	3.552	1559738	953665	23.587	21.645
2)	SA Decachlor...	9.994	8.742	1533516	855012	17.910	15.403
Target Compounds							
9)	L2 AR-1221-2	4.711f	0.000	18949	0	30.121	N.D. #
24)	L5 AR-1248-4	6.574f	0.000	32527	0	9.560	N.D. #
26)	L6 AR-1254-1	6.574	0.000	32527	0	9.141	N.D. #
35)	L7 AR-1260-5	8.509	0.000	8842	0	0.793	N.D. #
37)	L8 AR-1262-2	8.509	0.000	8842	0	0.702	N.D. #
39)	L8 AR-1262-4	8.839	0.000	2576	0	0.815	N.D. #
42)	L9 AR-1268-2	8.839	0.000	2576	0	0.189	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081720\
Data File : PO070603.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2020 13:56
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 14:15:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

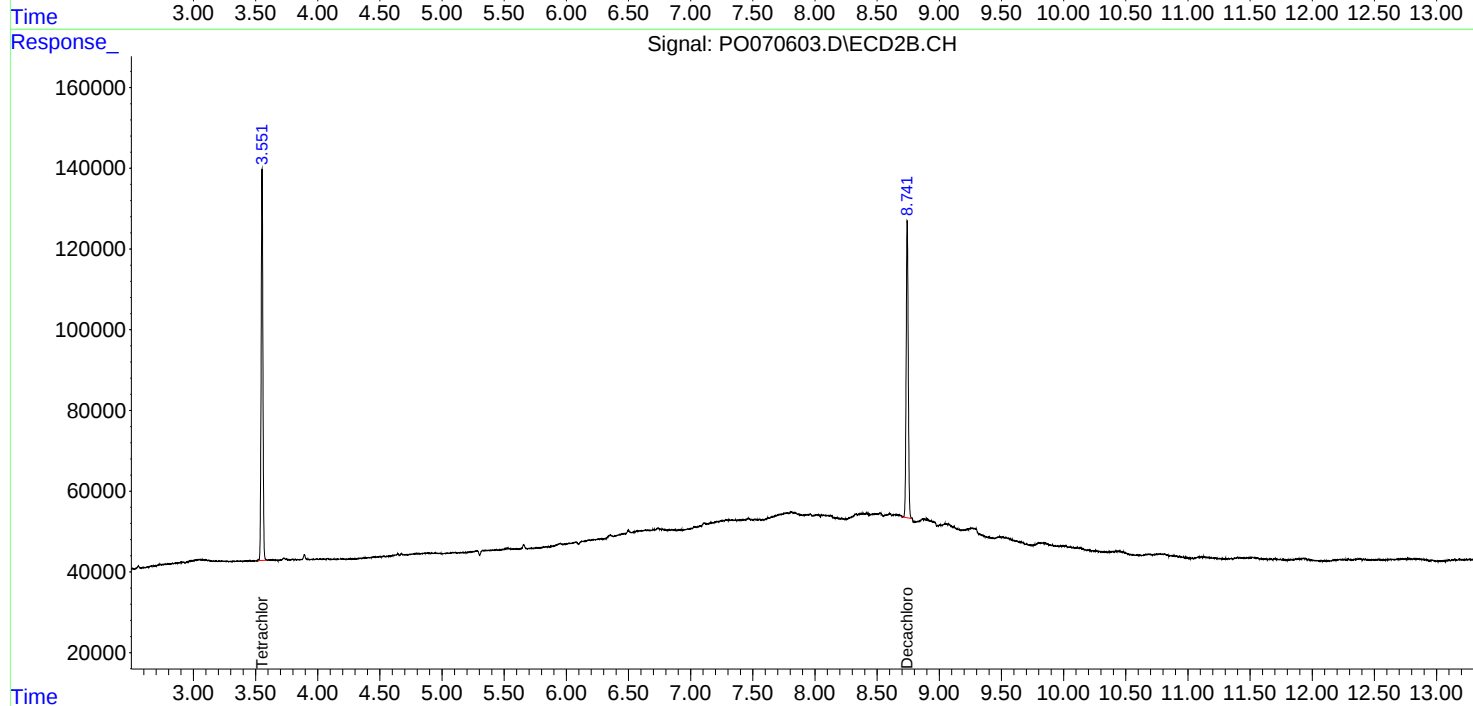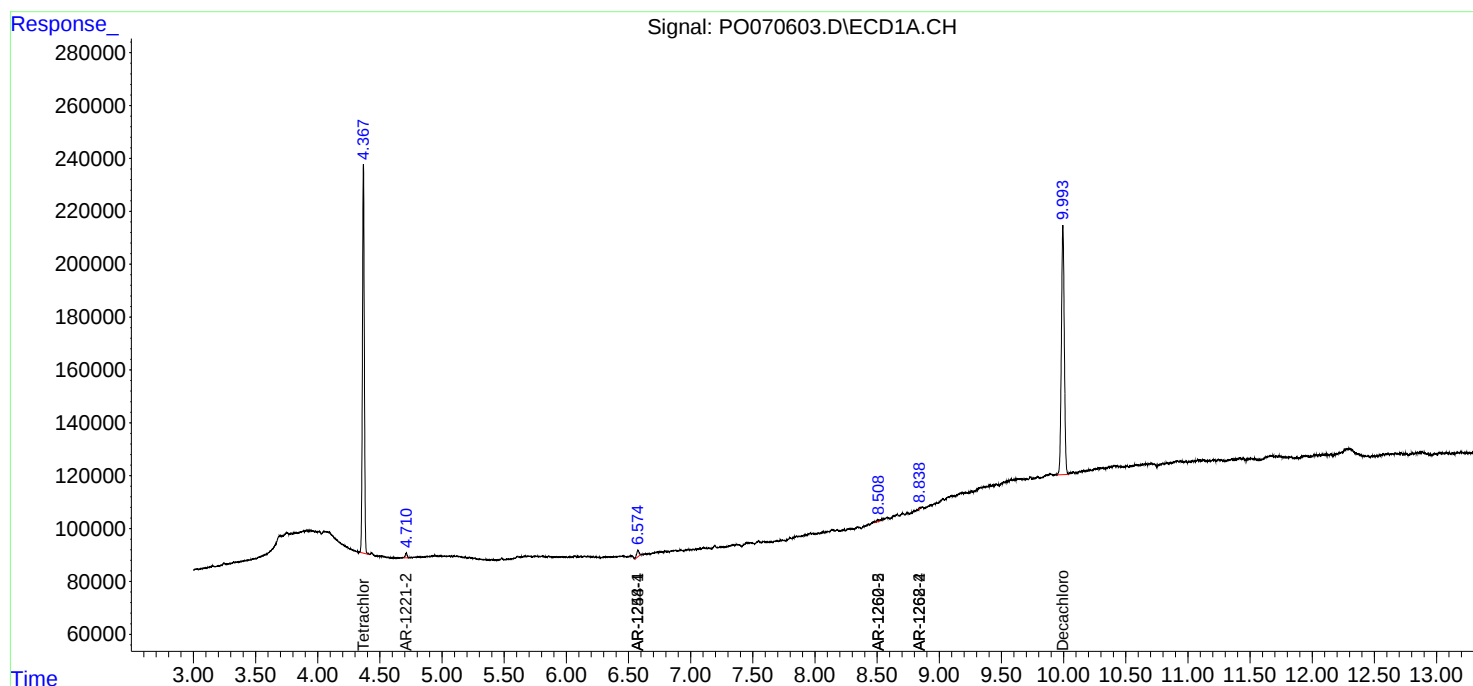


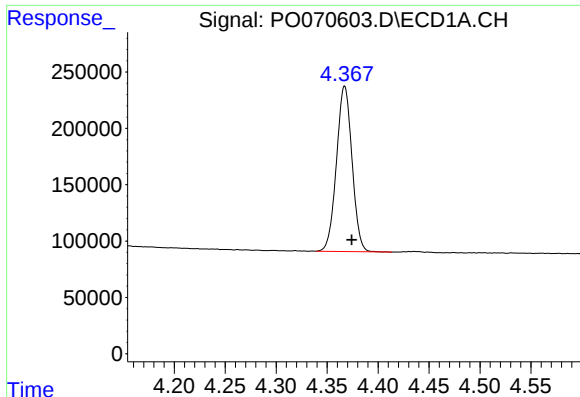

#1 Tetrachloro-m-xylene


R.T.: 4.367 min
Delta R.T.: -0.007 min
Response: 1559738
Conc: 23.59 ng/ml

Instrument :
ECD_O
ClientSampleId :

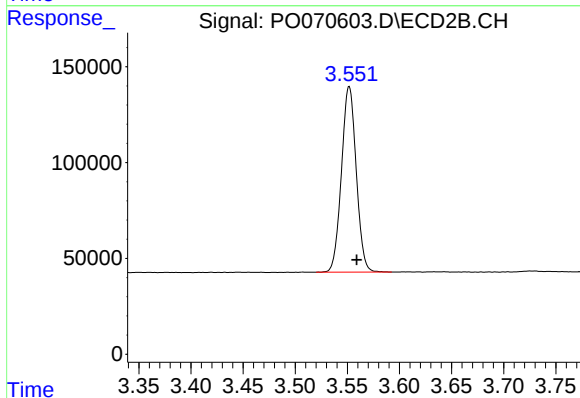


#1 Tetrachloro-m-xylene

R.T.: 3.552 min
Delta R.T.: -0.007 min
Response: 953665
Conc: 21.64 ng/ml

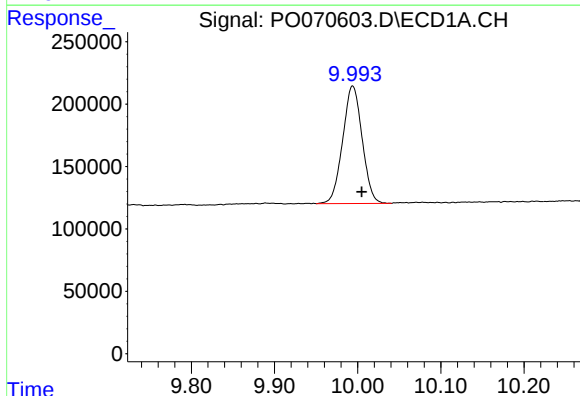


#2 Decachlorobiphenyl

R.T.: 9.994 min
Delta R.T.: -0.011 min
Response: 1533516
Conc: 17.91 ng/ml

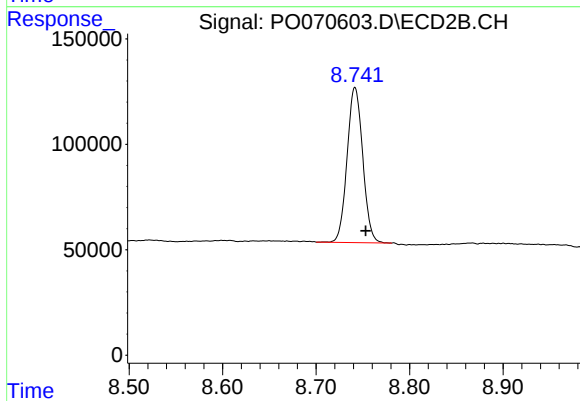

#2 Decachlorobiphenyl


R.T.: 8.742 min
Delta R.T.: -0.012 min
Response: 855012
Conc: 15.40 ng/ml

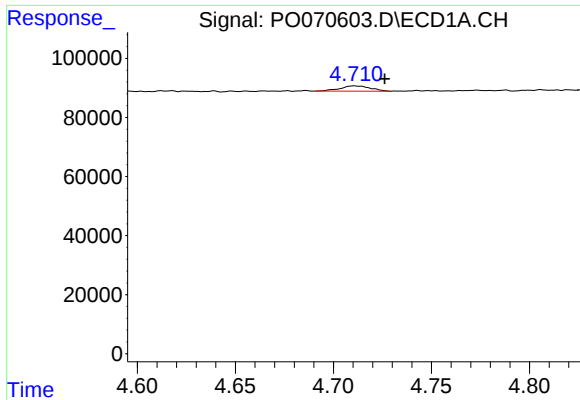

#9 AR-1221-2


R.T.: 4.711 min
Delta R.T.: -0.016 min
Response: 18949
Conc: 30.12 ng/ml

Instrument :
ECD_O
ClientSampleId :

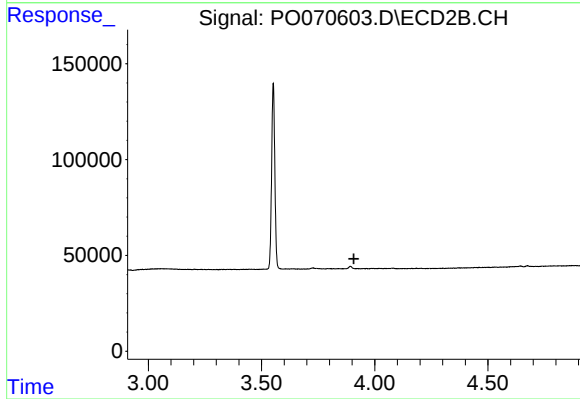


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.908 min
Response: 0
Conc: N.D.

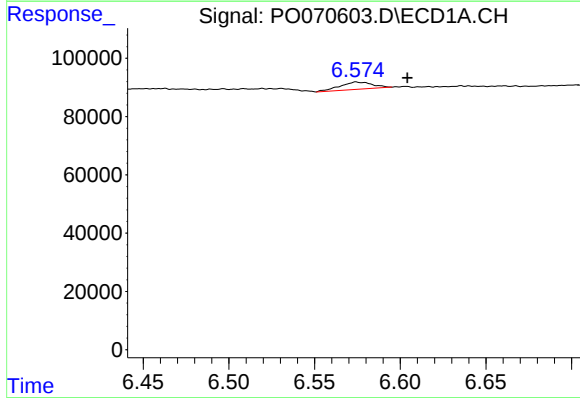


#24 AR-1248-4

R.T.: 6.574 min
Delta R.T.: -0.030 min
Response: 32527
Conc: 9.56 ng/ml

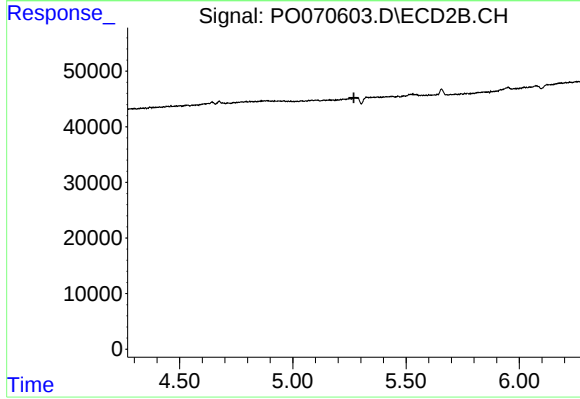

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.269 min
Response: 0
Conc: N.D.

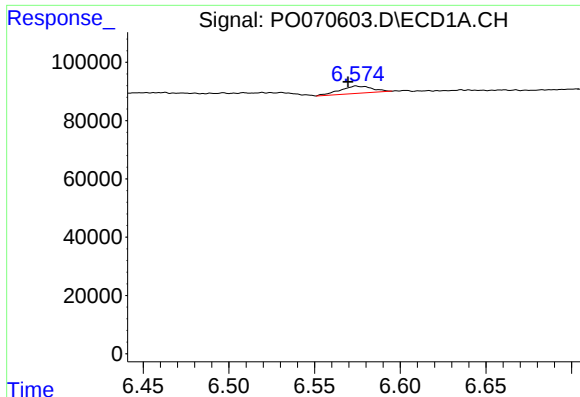

#26 AR-1254-1


R.T.: 6.574 min
Delta R.T.: 0.005 min
Response: 32527
Conc: 9.14 ng/ml

Instrument :
ECD_O
ClientSampleId :

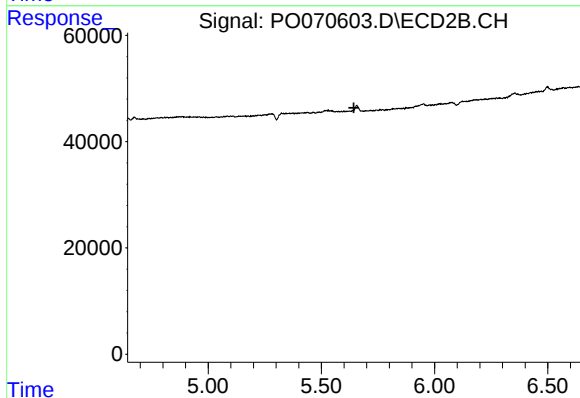


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.644 min
Response: 0
Conc: N.D.

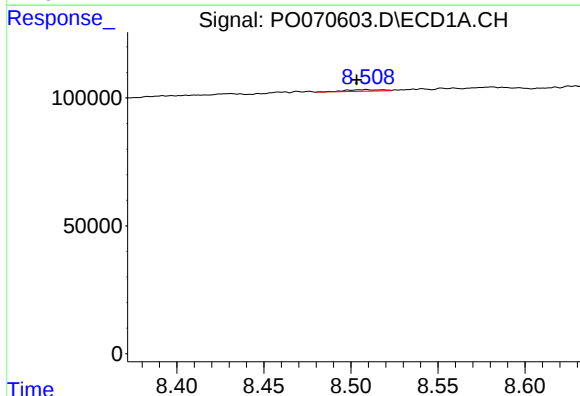


#35 AR-1260-5

R.T.: 8.509 min
Delta R.T.: 0.006 min
Response: 8842
Conc: 0.79 ng/ml

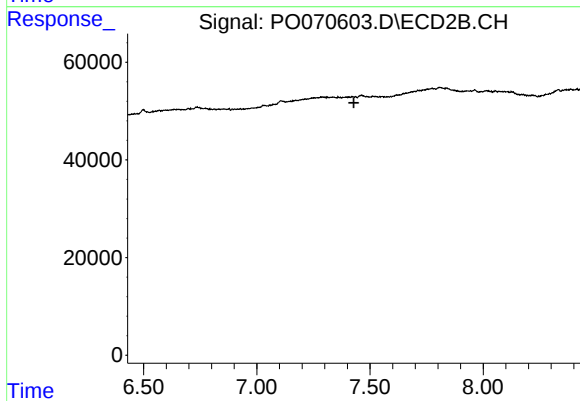

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.429 min
Response: 0
Conc: N.D.

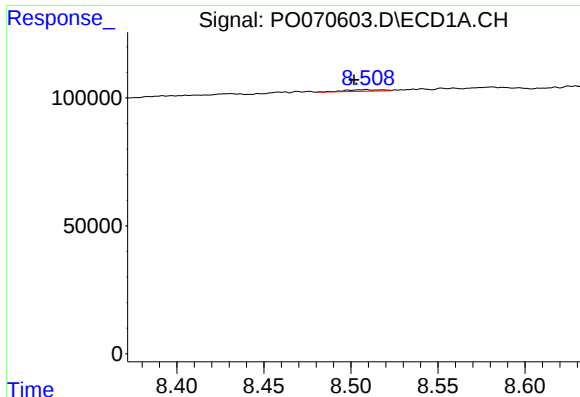

#37 AR-1262-2


R.T.: 8.509 min
Delta R.T.: 0.007 min
Response: 8842
Conc: 0.70 ng/ml

Instrument :
ECD_O
ClientSampleId :

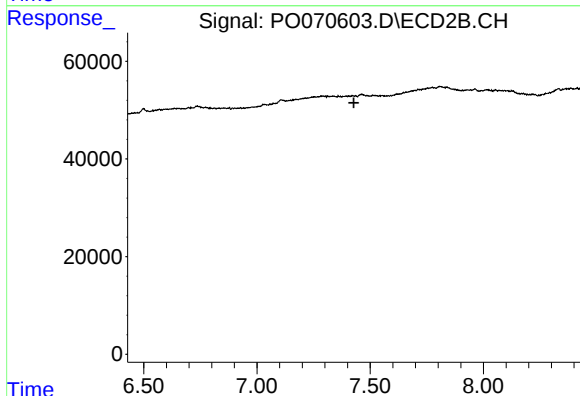


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.428 min
Response: 0
Conc: N.D.

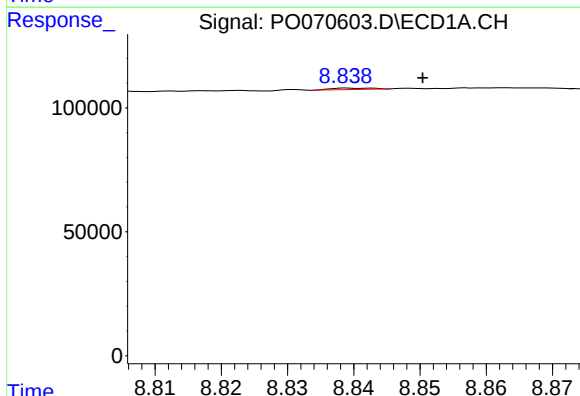


#39 AR-1262-4

R.T.: 8.839 min
Delta R.T.: -0.011 min
Response: 2576
Conc: 0.82 ng/ml

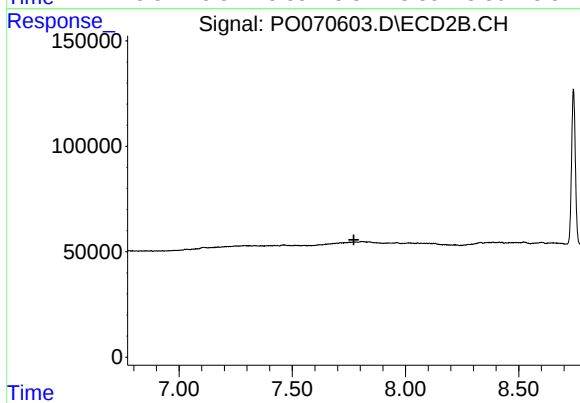

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 7.772 min
Response: 0
Conc: N.D.

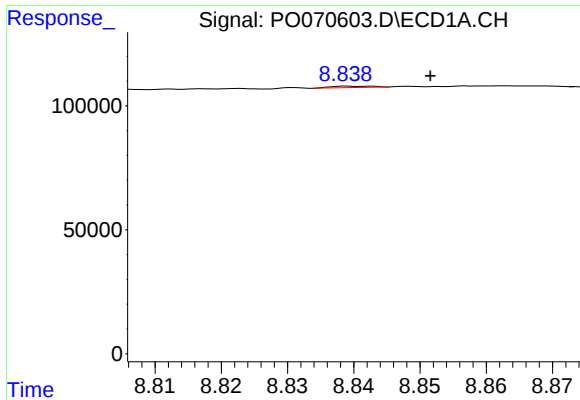

#42 AR-1268-2

R.T.: 8.839 min
Delta R.T.: -0.012 min
Response: 2576
Conc: 0.19 ng/ml

Instrument :
ECD_O
ClientSampleId :

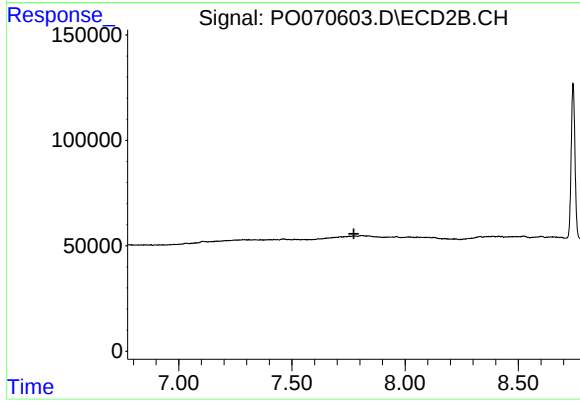

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.774 min
Response: 0
Conc: N.D.