

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081720\
 Data File : P0070601.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Aug 2020 13:22
 Operator : DD\AJ
 Sample : L3508-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-08-081420

Manual Integrations
 APPROVED

Ankita
 8/18/2020 3:40:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 14:08:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.367	3.552	1875781	1145010	28.367	25.988
2) SA Decachlor...	9.995	8.742	1893514	1094323	22.114	19.715

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081720\
Data File : P0070601.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2020 13:22
Operator : DD\AJ
Sample : L3508-19
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-08-081420


Manual Integrations
APPROVED

Ankita
8/18/2020 3:40:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 14:08:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

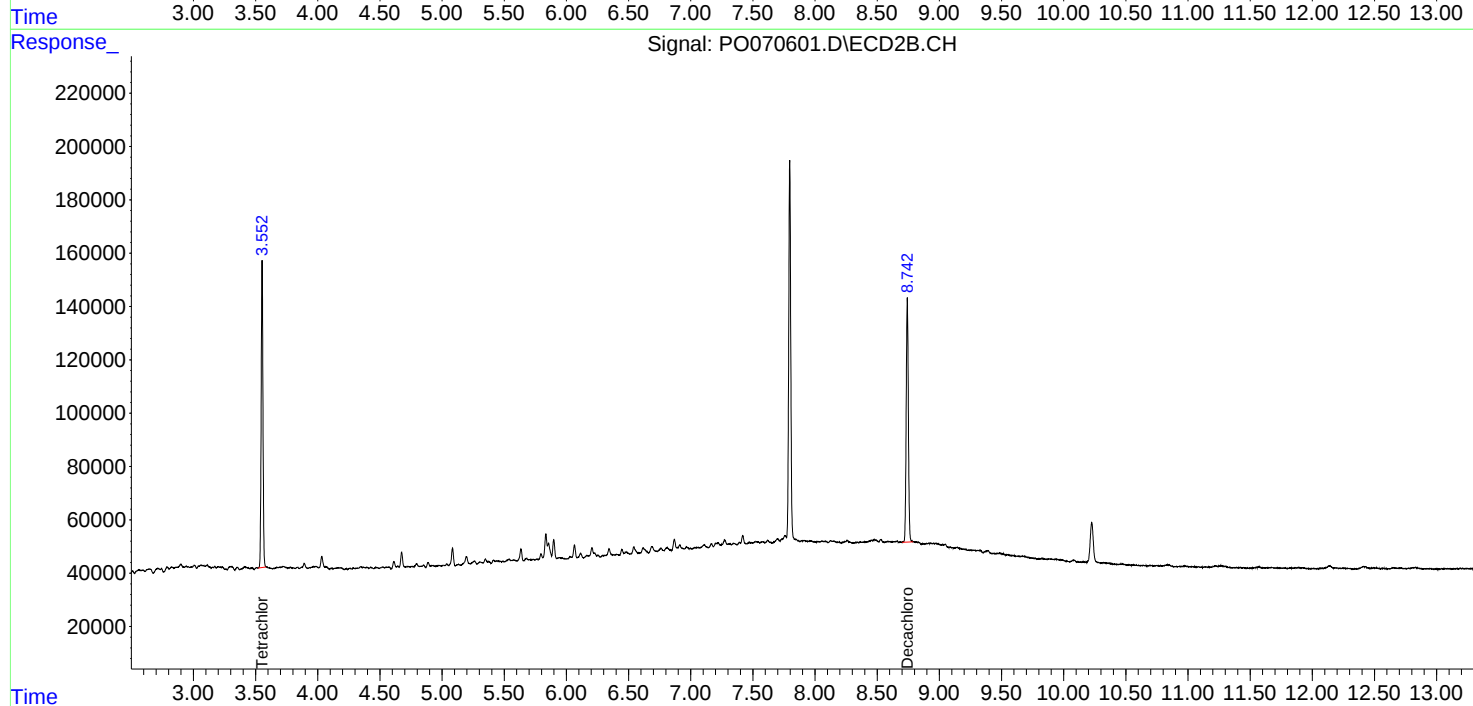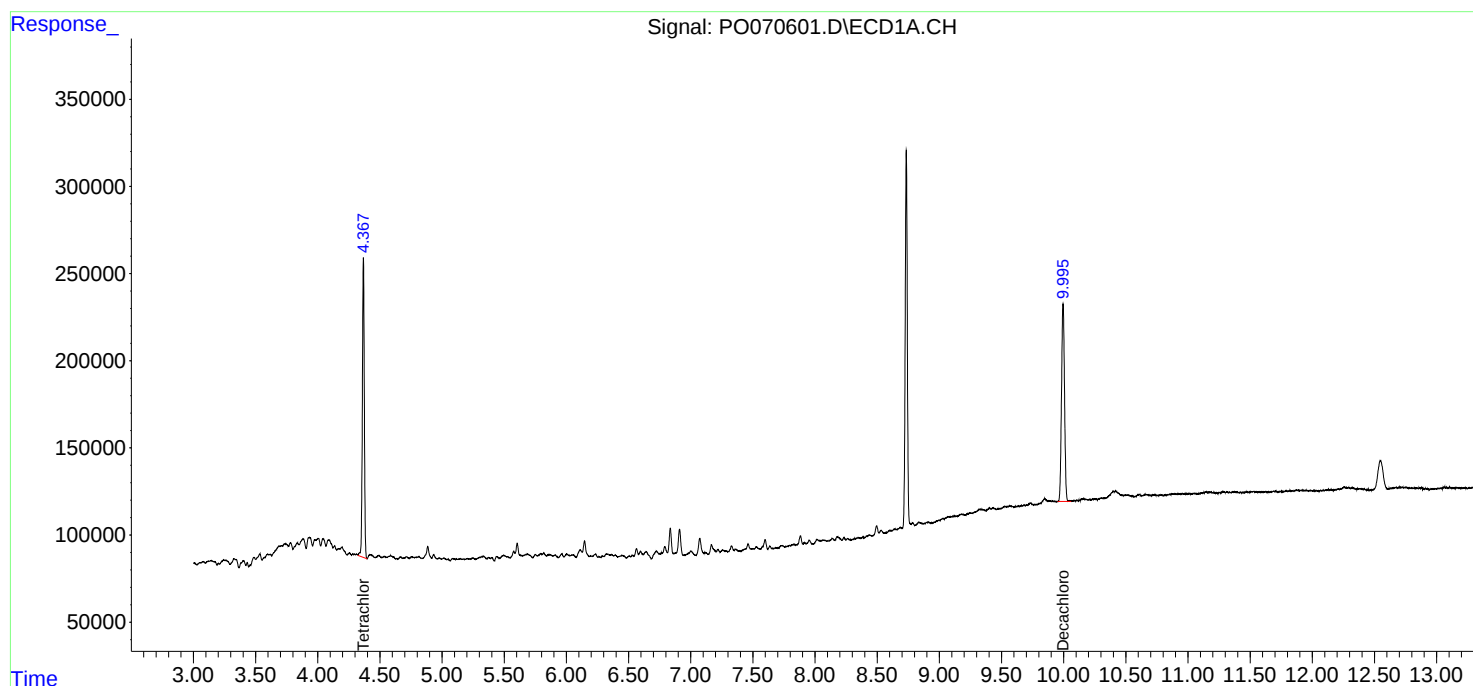

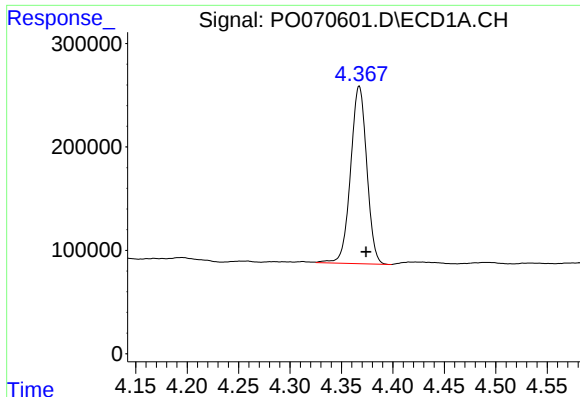


#1 Tetrachloro-m-xylene

R.T.: 4.367 min
Delta R.T.: -0.007 min
Response: 1875781
Conc: 28.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-08-081420


Manual Integrations
APPROVED

Ankita
8/18/2020 3:40:19 PM

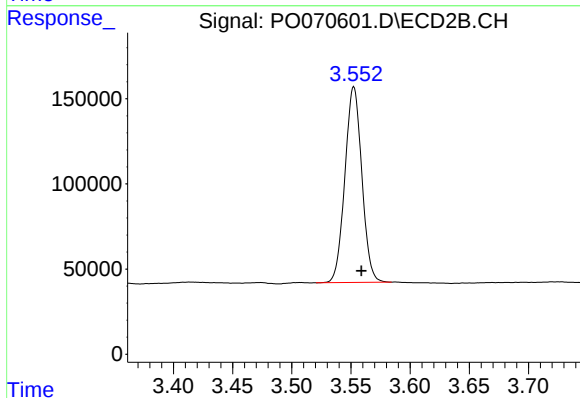


#1 Tetrachloro-m-xylene

R.T.: 3.552 min
Delta R.T.: -0.006 min
Response: 1145010
Conc: 25.99 ng/ml

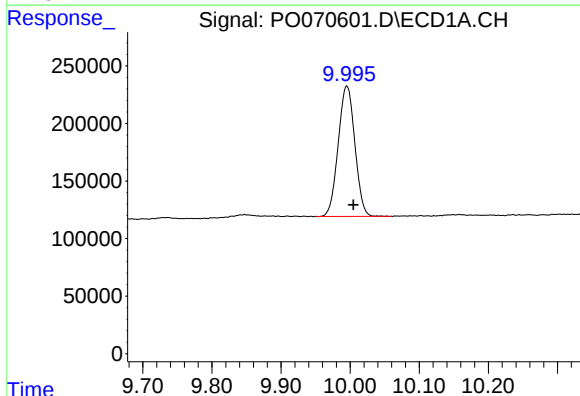

#2 Decachlorobiphenyl

R.T.: 9.995 min
Delta R.T.: -0.010 min
Response: 1893514
Conc: 22.11 ng/ml

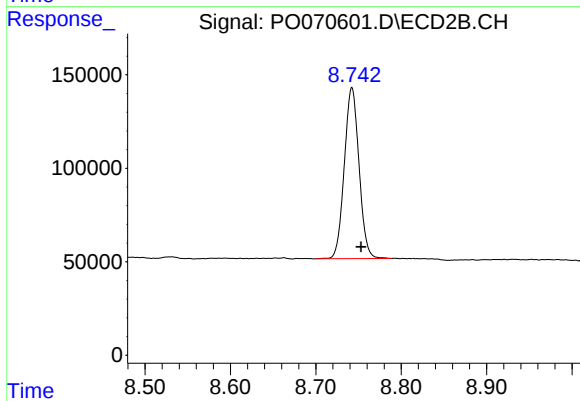

#2 Decachlorobiphenyl

R.T.: 8.742 min
Delta R.T.: -0.011 min
Response: 1094323
Conc: 19.71 ng/ml