

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081721\
 Data File : P0080566.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Aug 2021 23:30
 Operator : DD\AJ
 Sample : M3428-17
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-06-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:41:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.991	4.106	1869877	620474	27.004	24.895
2)	SA Decachlor...	11.091	9.503	1287846	509538	24.880	22.465
Target Compounds							
8)	L2 AR-1221-1	5.244	0.000	156674	0	196.994	N.D. #
9)	L2 AR-1221-2	5.346	4.443f	22854	39915	41.749	171.586 #
28)	L6 AR-1254-3	7.869f	0.000	33822	0	8.287	N.D. #
30)	L6 AR-1254-5	8.601f	7.528	39292	21850	12.699	12.454
32)	L7 AR-1260-2	8.282	0.000	22273	0	6.702	N.D. #
36)	L8 AR-1262-1	0.000	7.528	0	21850	N.D.	21.768 #
45)	L9 AR-1268-5	10.749	0.000	6708	0	0.334	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081721\
Data File : P0080566.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2021 23:30
Operator : DD\AJ
Sample : M3428-17
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-06-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:41:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

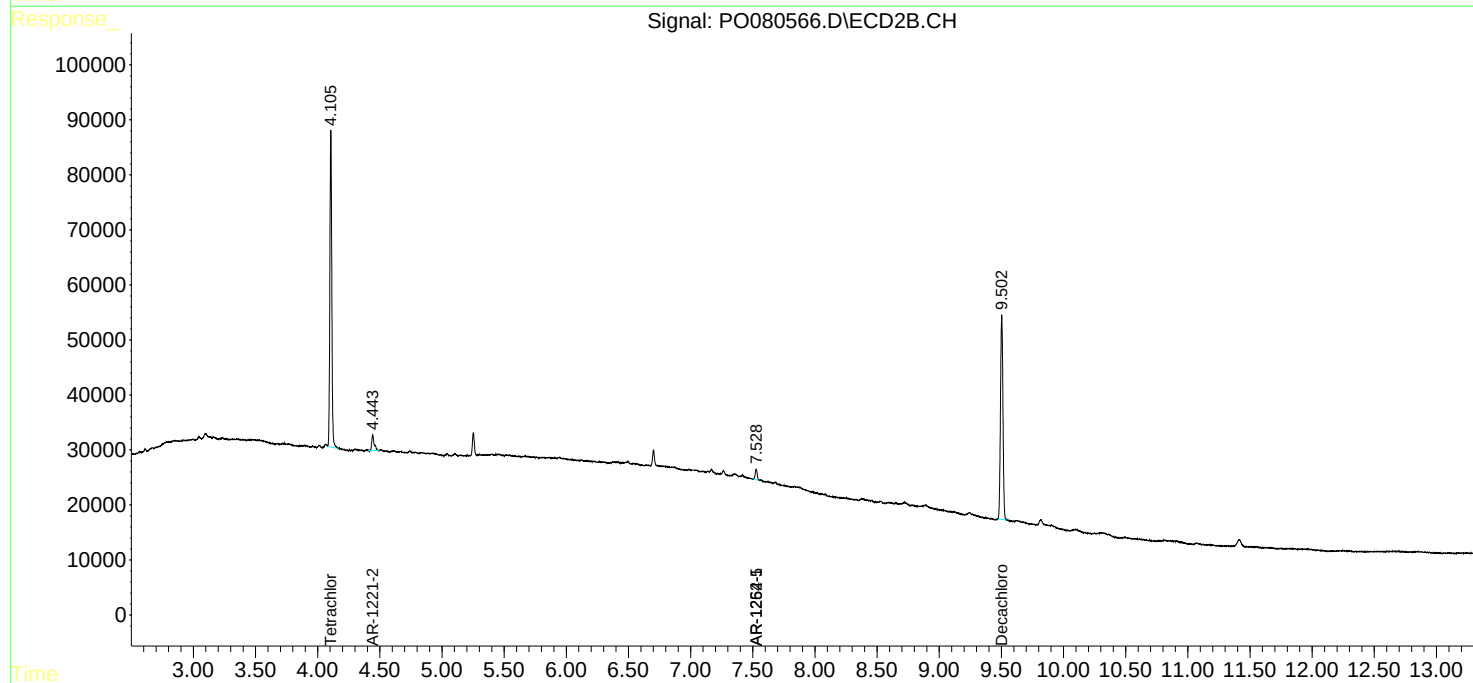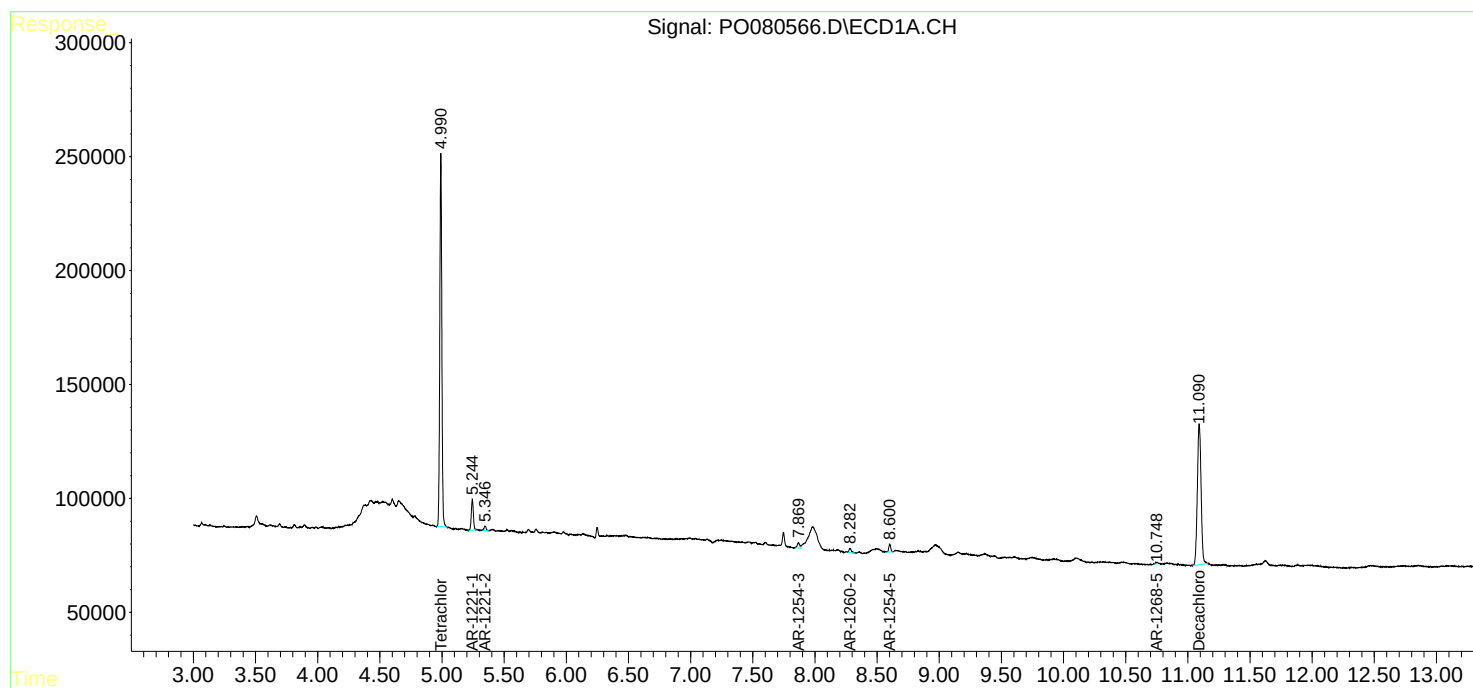


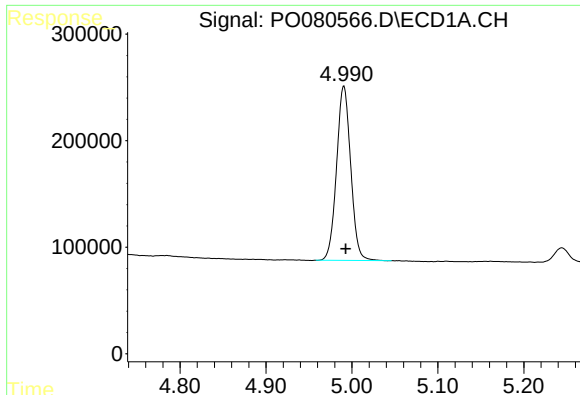

#1 Tetrachloro-m-xylene


R.T.: 4.991 min
Delta R.T.: -0.002 min
Response: 1869877
Conc: 27.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-06-COMP

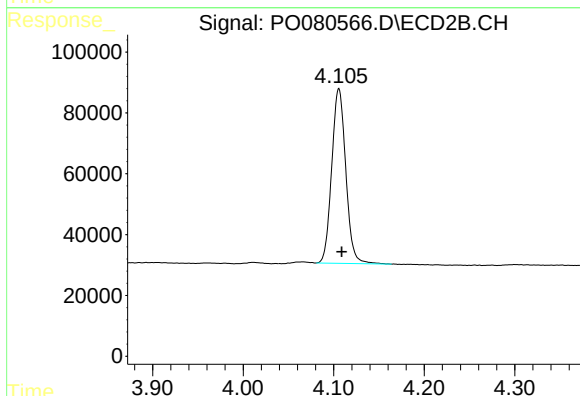


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: -0.003 min
Response: 620474
Conc: 24.89 ng/ml

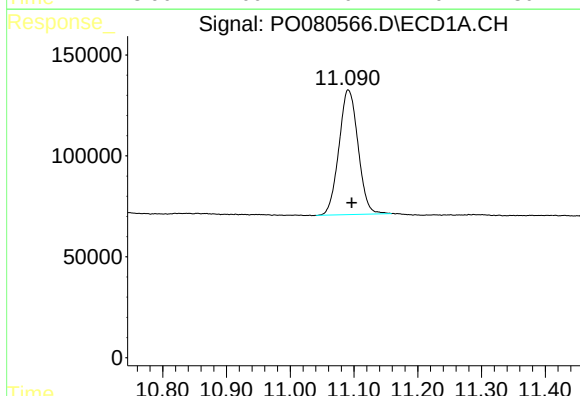


#2 Decachlorobiphenyl

R.T.: 11.091 min
Delta R.T.: -0.006 min
Response: 1287846
Conc: 24.88 ng/ml

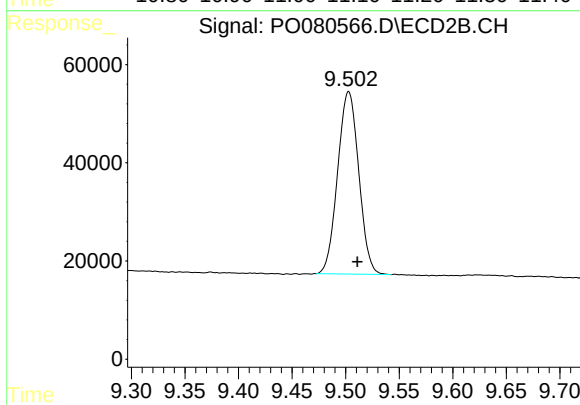

#2 Decachlorobiphenyl


R.T.: 9.503 min
Delta R.T.: -0.008 min
Response: 509538
Conc: 22.46 ng/ml

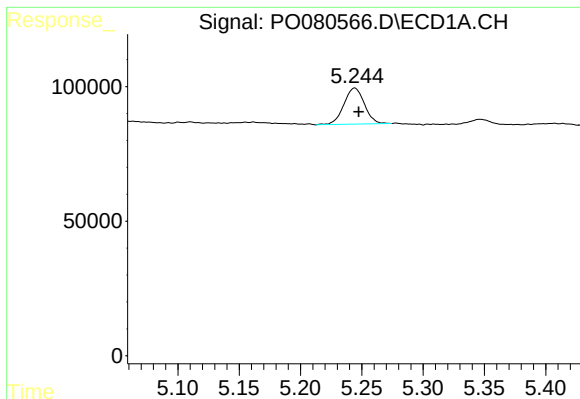

#8 AR-1221-1


R.T.: 5.244 min
Delta R.T.: -0.003 min
Response: 156674
Conc: 196.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-06-COMP

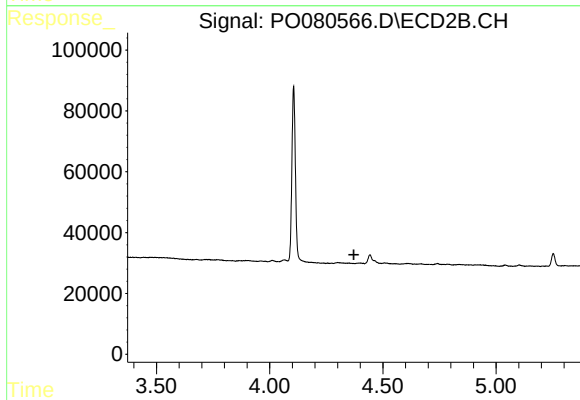


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.372 min
Response: 0
Conc: N.D.

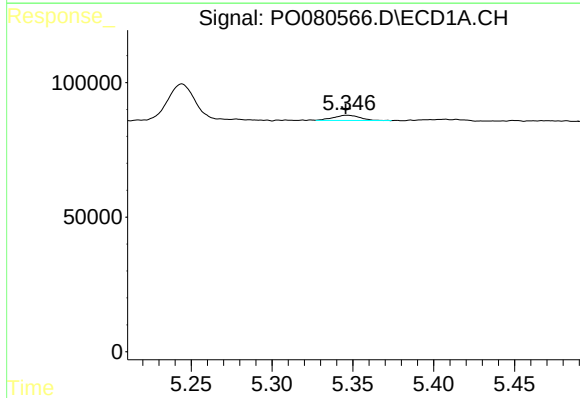


#9 AR-1221-2

R.T.: 5.346 min
Delta R.T.: 0.000 min
Response: 22854
Conc: 41.75 ng/ml

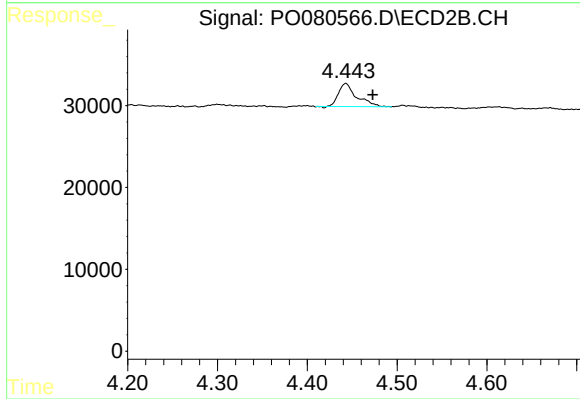

#9 AR-1221-2


R.T.: 4.443 min
Delta R.T.: -0.030 min
Response: 39915
Conc: 171.59 ng/ml

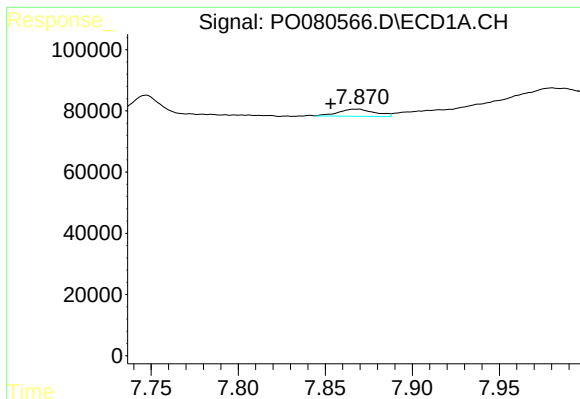

#28 AR-1254-3


R.T.: 7.869 min
Delta R.T.: 0.016 min
Response: 33822
Conc: 8.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-06-COMP

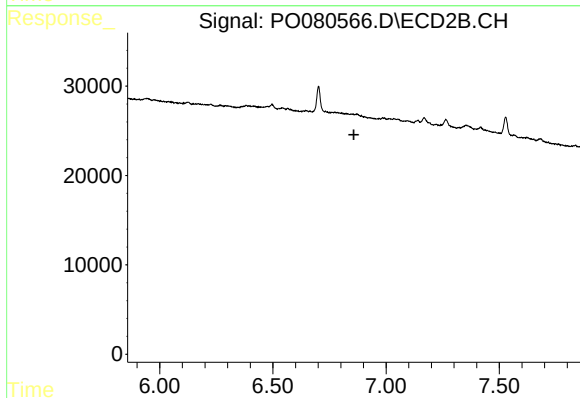


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.858 min
Response: 0
Conc: N.D.

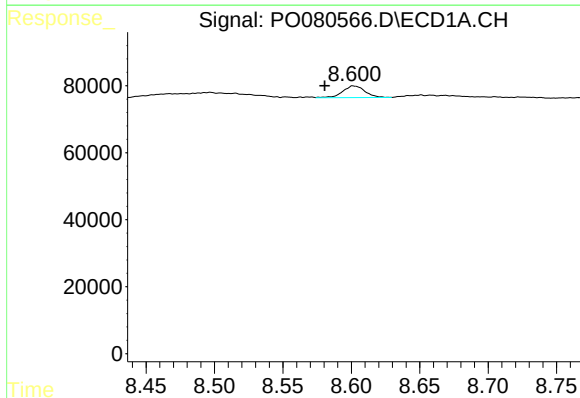


#30 AR-1254-5

R.T.: 8.601 min
Delta R.T.: 0.020 min
Response: 39292
Conc: 12.70 ng/ml

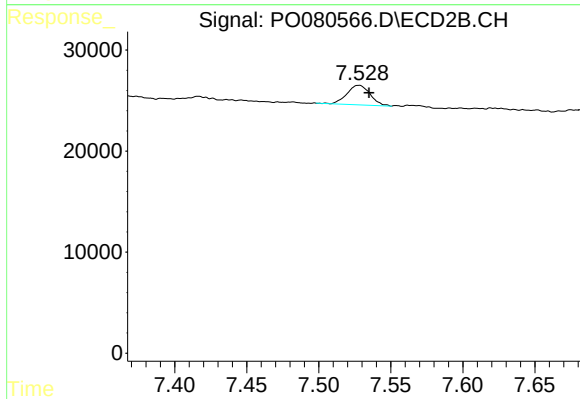

#30 AR-1254-5


R.T.: 7.528 min
Delta R.T.: -0.007 min
Response: 21850
Conc: 12.45 ng/ml

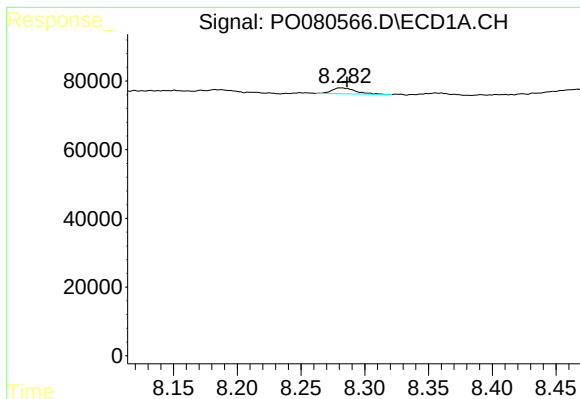

#32 AR-1260-2


R.T.: 8.282 min
Delta R.T.: -0.004 min
Response: 22273
Conc: 6.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-06-COMP

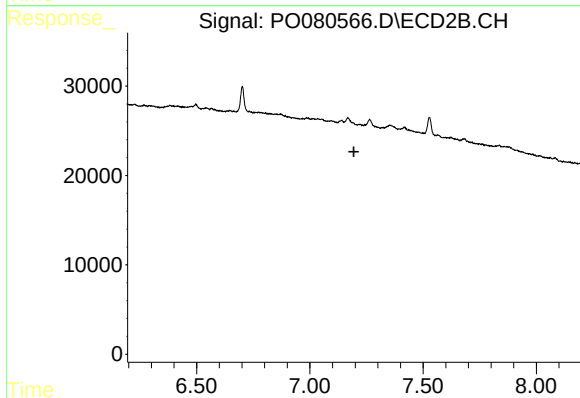


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.194 min
Response: 0
Conc: N.D.

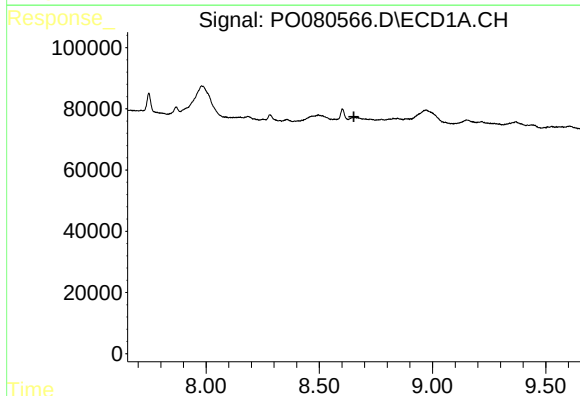


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.652 min
Response: 0
Conc: N.D.

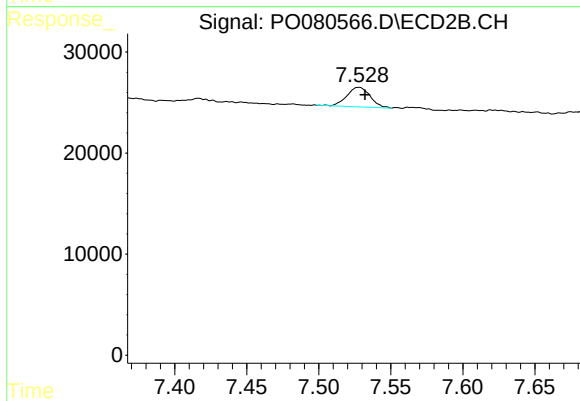

#36 AR-1262-1


R.T.: 7.528 min
Delta R.T.: -0.004 min
Response: 21850
Conc: 21.77 ng/ml

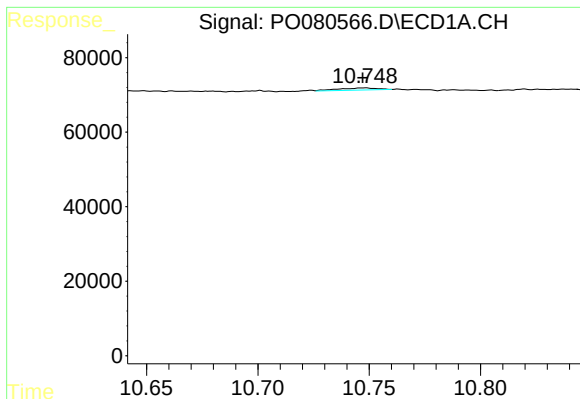

#45 AR-1268-5

R.T.: 10.749 min
Delta R.T.: 0.002 min
Response: 6708
Conc: 0.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-06-COMP

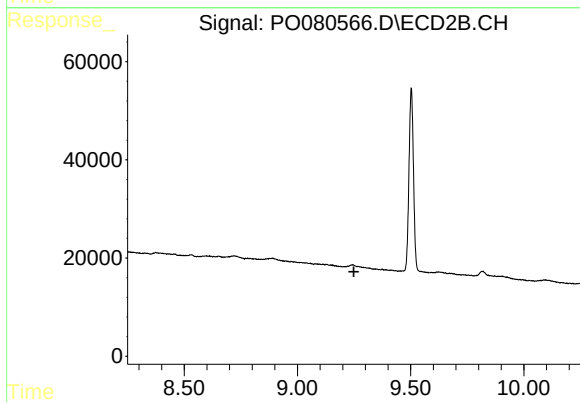

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.249 min
Response: 0
Conc: N.D.