

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081721\
Data File : P0080543.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2021 16:35
Operator : DD\AJ
Sample : M3419-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SWCS-03-1015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 06:00:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.992	4.106	1587253	557968	22.922	22.387
2) SA Decachlor...	11.092	9.504	995620	407868	19.234	17.982

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081721\
Data File : P0080543.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2021 16:35
Operator : DD\AJ
Sample : M3419-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SWCS-03-1015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 06:00:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

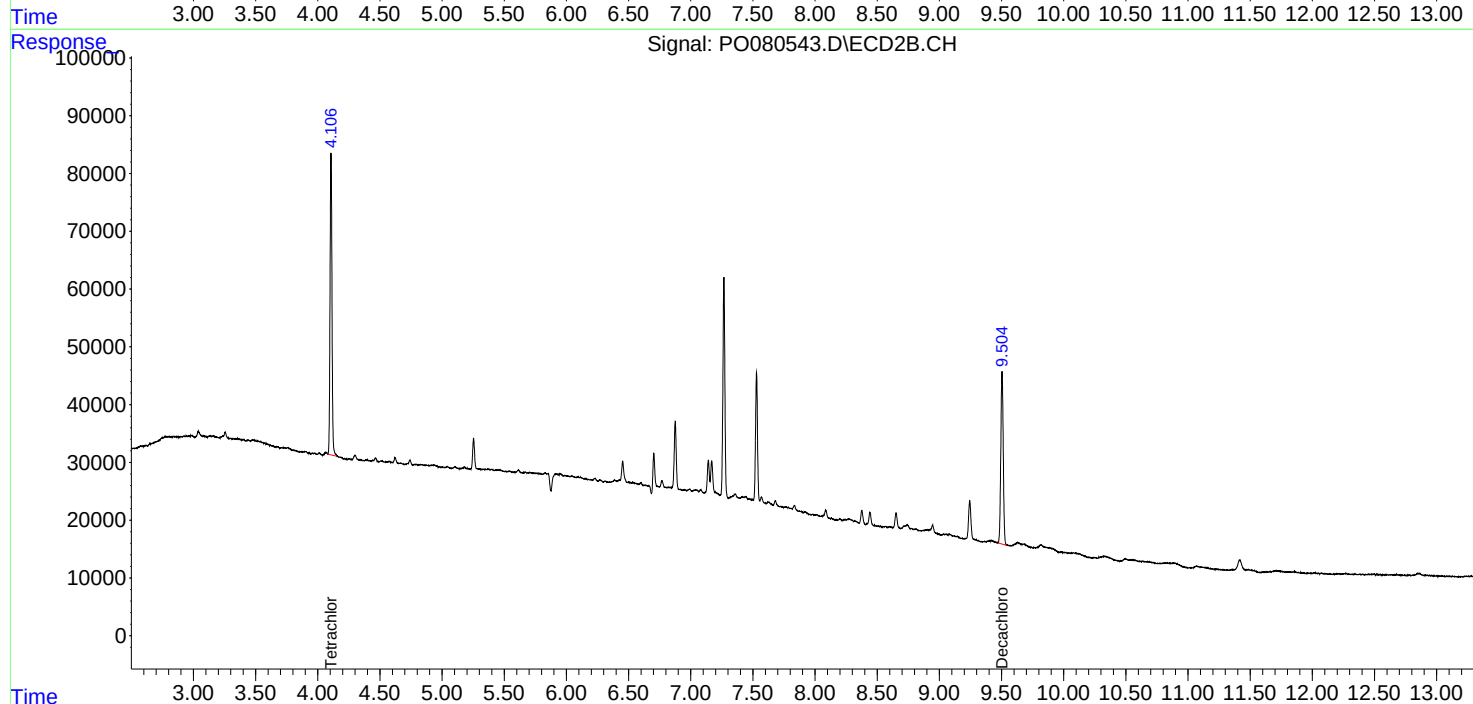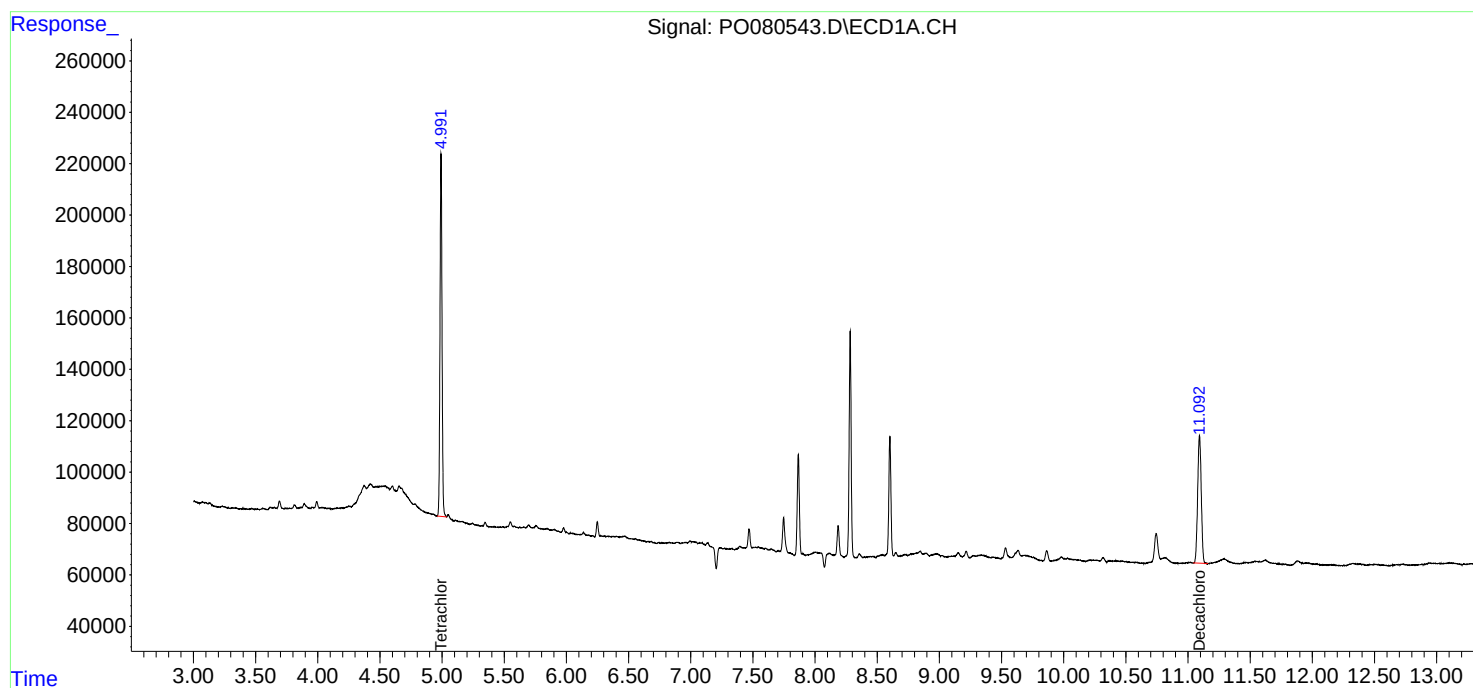


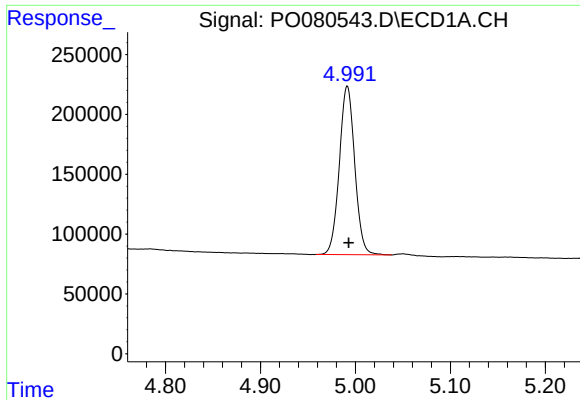

#1 Tetrachloro-m-xylene


R.T.: 4.992 min
Delta R.T.: -0.001 min
Response: 1587253
Conc: 22.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
SWCS-03-1015

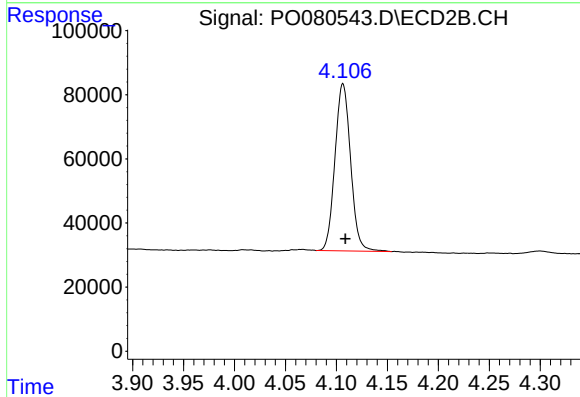


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: -0.002 min
Response: 557968
Conc: 22.39 ng/ml

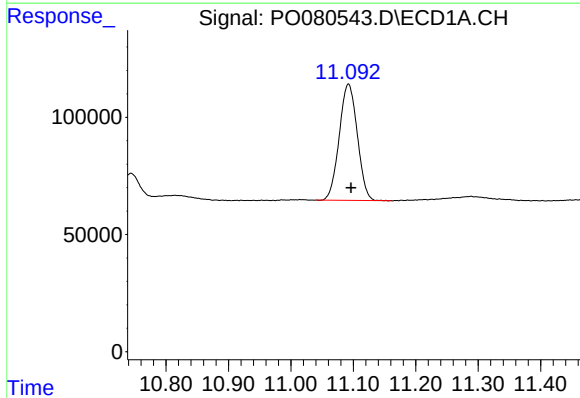

#2 Decachlorobiphenyl

R.T.: 11.092 min
Delta R.T.: -0.004 min
Response: 995620
Conc: 19.23 ng/ml

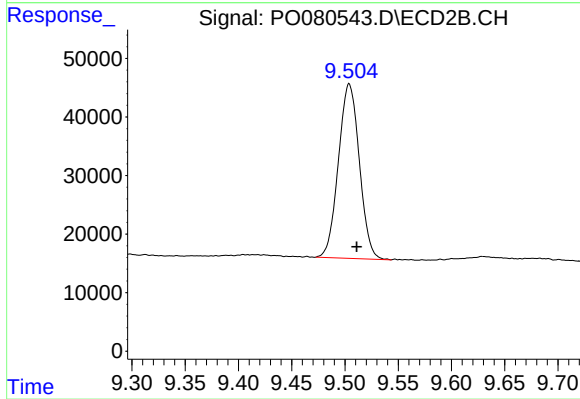

#2 Decachlorobiphenyl

R.T.: 9.504 min
Delta R.T.: -0.007 min
Response: 407868
Conc: 17.98 ng/ml