

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081721\
 Data File : P0080555.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Aug 2021 20:20
 Operator : DD\AJ
 Sample : M3428-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-02-COMP

Manual Integrations
 APPROVED

mohammad
 8/18/2021 2:06:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:37:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.992	4.107	1643493	551796	23.734	22.139m
2) SA Decachlor...	11.094	9.504	1124591	456773	21.726	20.139

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081721\
Data File : P0080555.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2021 20:20
Operator : DD\AJ
Sample : M3428-05
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-02-COMP


Manual Integrations
APPROVED

mohammad
8/18/2021 2:06:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:37:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

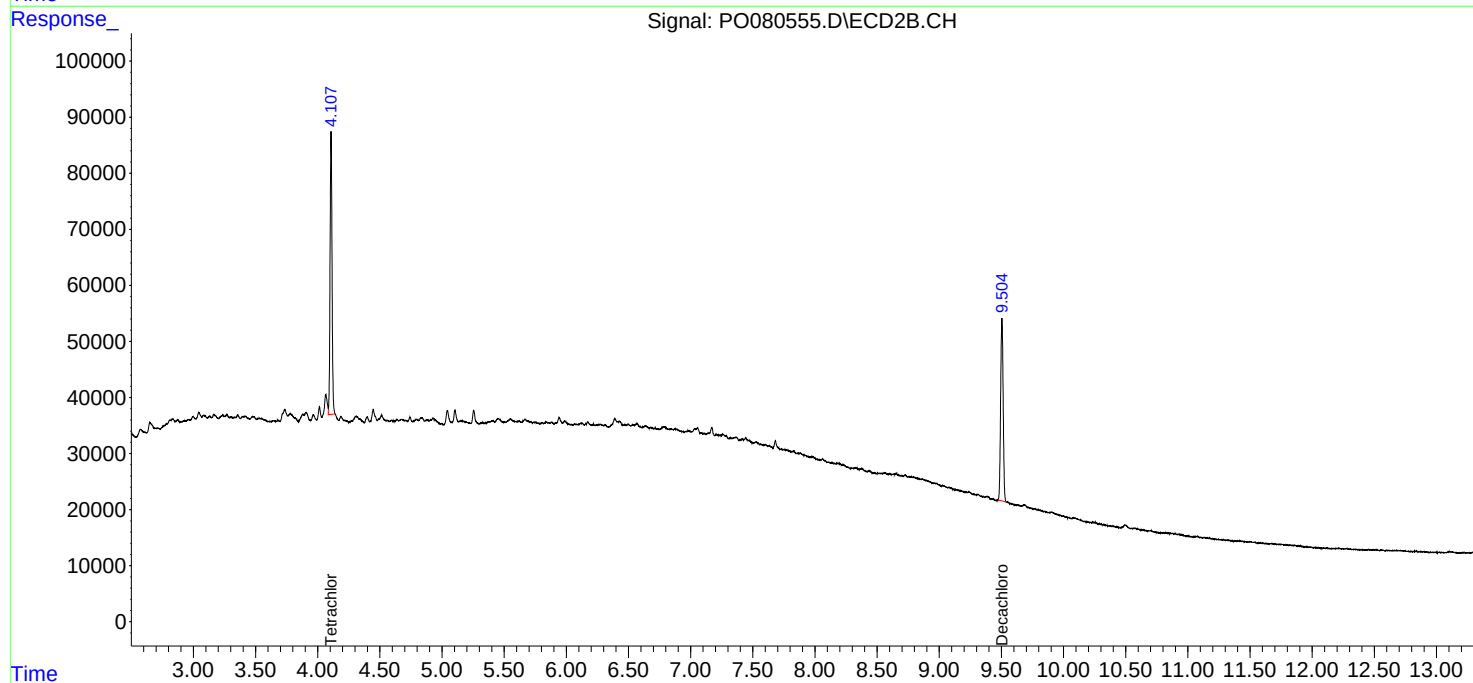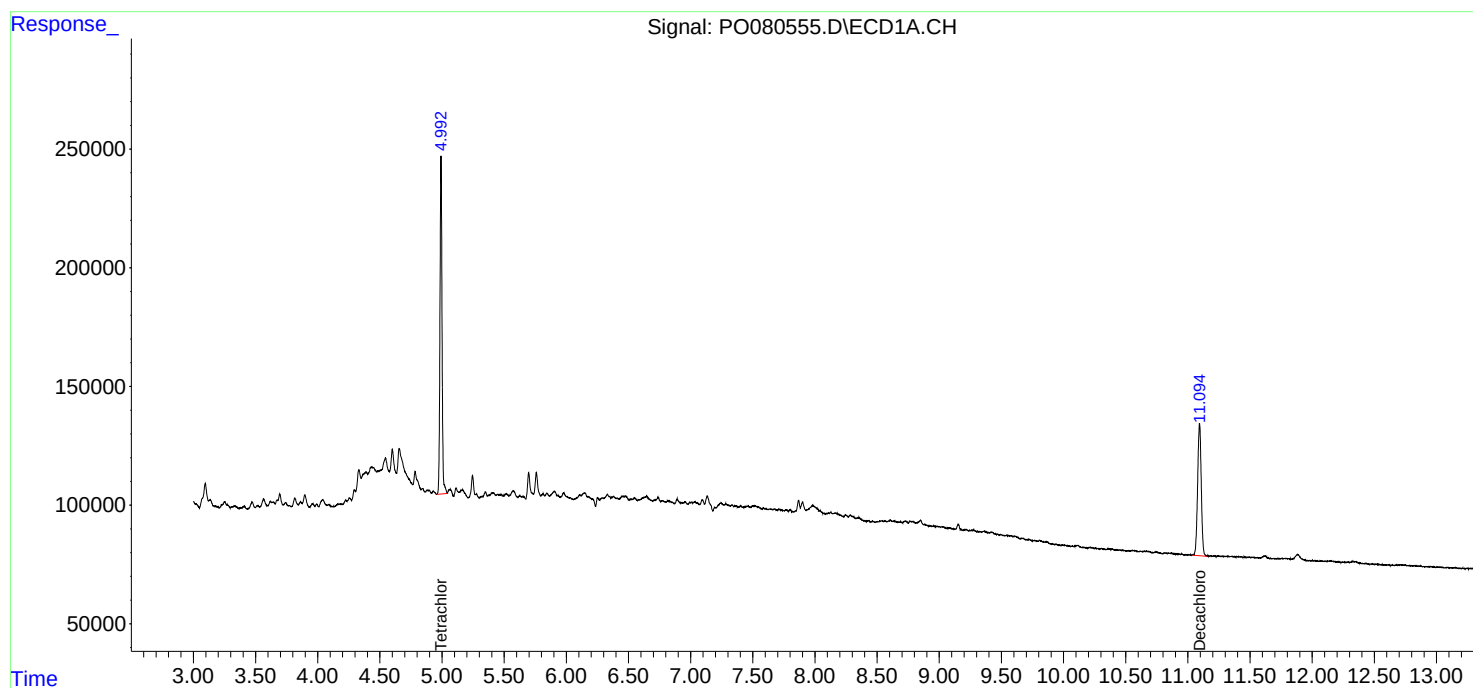

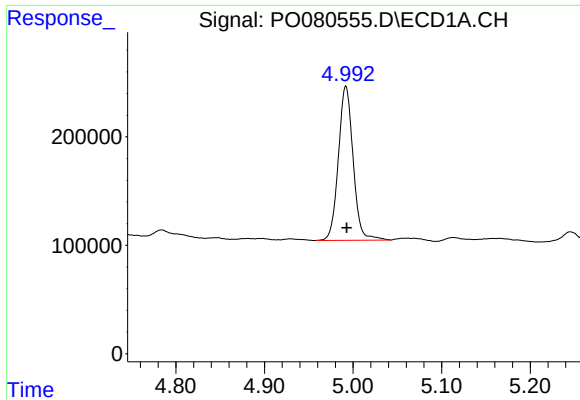


#1 Tetrachloro-m-xylene

R.T.: 4.992 min
Delta R.T.: -0.001 min
Response: 1643493
Conc: 23.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-COMP


Manual Integrations
APPROVED

mohammad
8/18/2021 2:06:30 PM

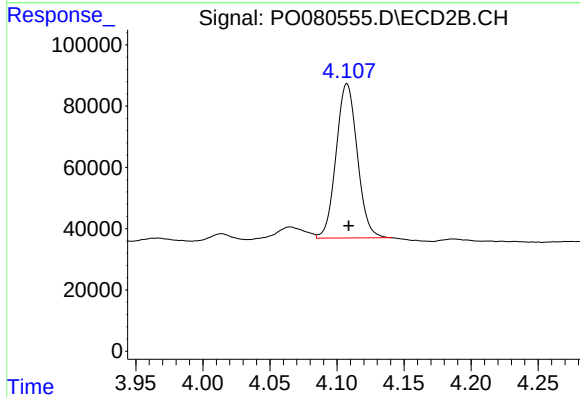


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: -0.002 min
Response: 551796
Conc: 22.14 ng/ml m

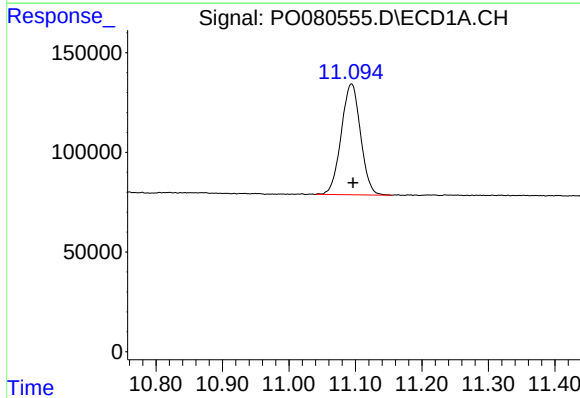

#2 Decachlorobiphenyl

R.T.: 11.094 min
Delta R.T.: -0.002 min
Response: 1124591
Conc: 21.73 ng/ml

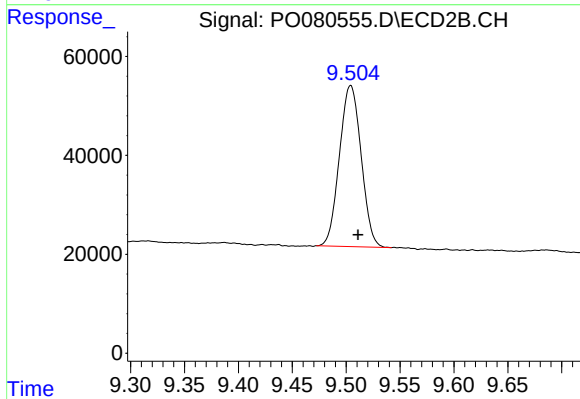

#2 Decachlorobiphenyl

R.T.: 9.504 min
Delta R.T.: -0.007 min
Response: 456773
Conc: 20.14 ng/ml