

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081721\
 Data File : P0080560.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Aug 2021 21:46
 Operator : DD\AJ
 Sample : M3431-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:39:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.990	4.106	1848192	606039	26.690	24.316
2) SA Decachlor...	11.091	9.503	1270203	497438	24.539	21.932

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081721\
Data File : P0080560.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2021 21:46
Operator : DD\AJ
Sample : M3431-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:39:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

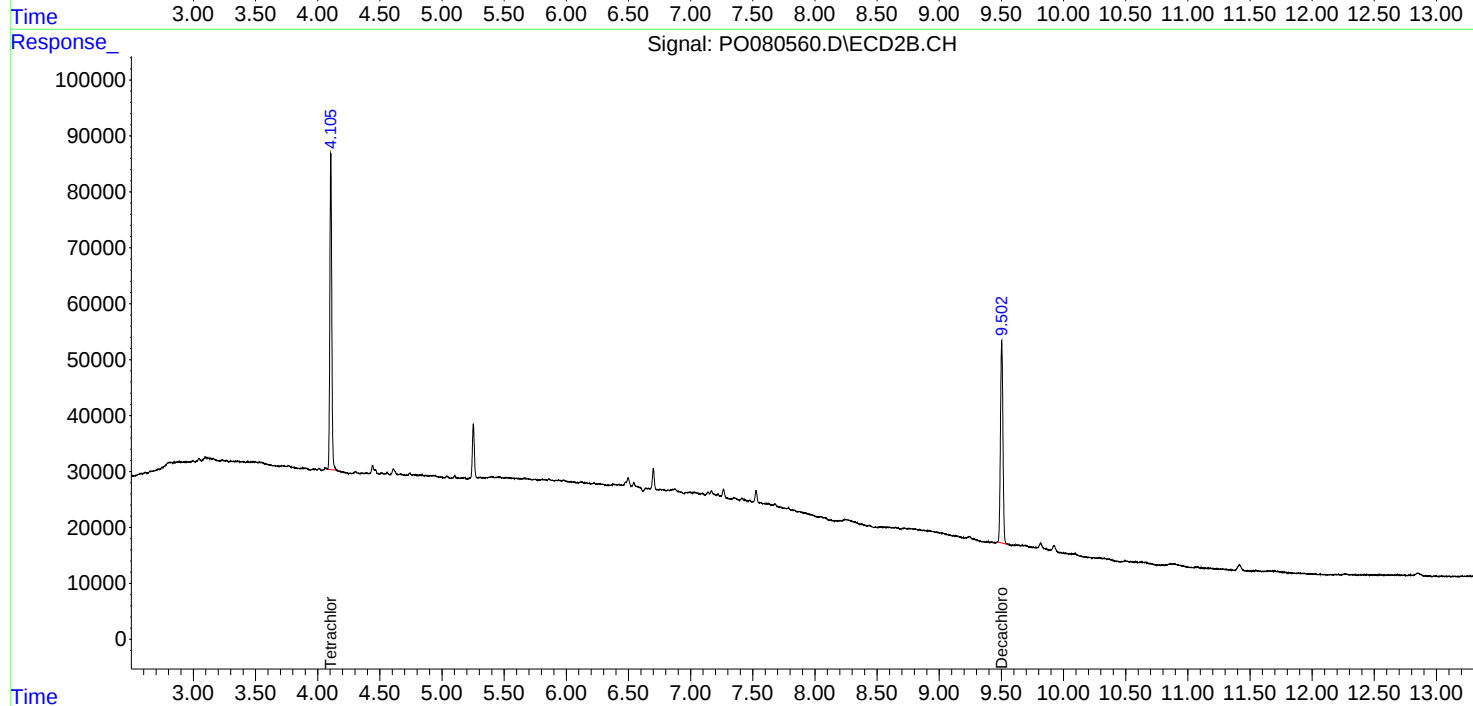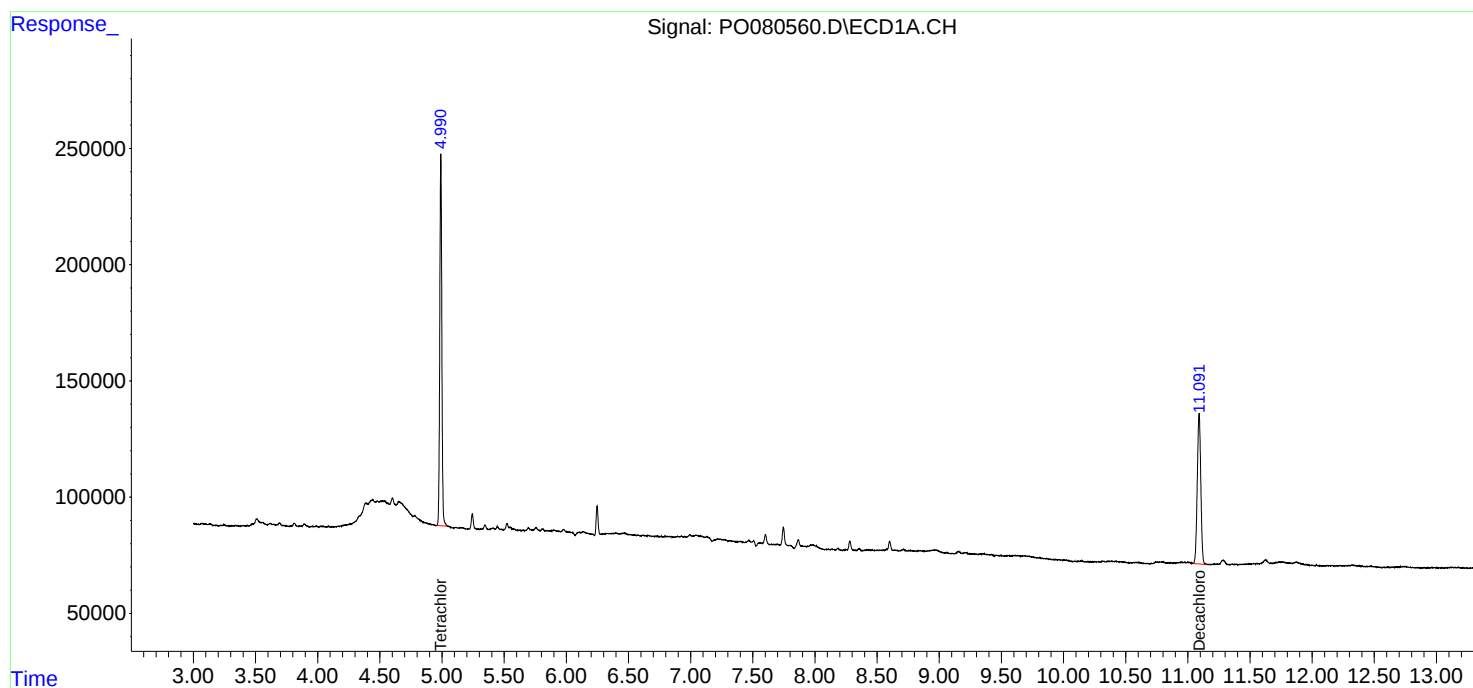


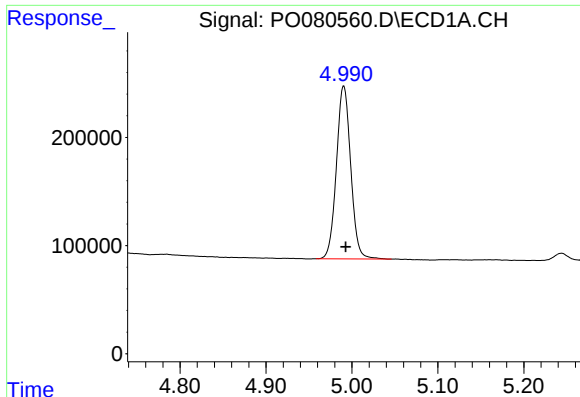

#1 Tetrachloro-m-xylene


R.T.: 4.990 min
Delta R.T.: -0.003 min
Response: 1848192
Conc: 26.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
4

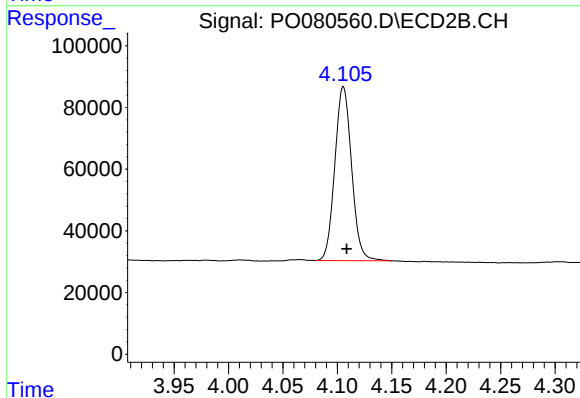


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: -0.003 min
Response: 606039
Conc: 24.32 ng/ml

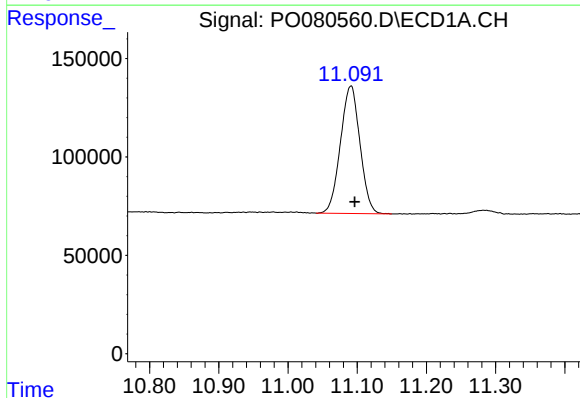

#2 Decachlorobiphenyl

R.T.: 11.091 min
Delta R.T.: -0.005 min
Response: 1270203
Conc: 24.54 ng/ml

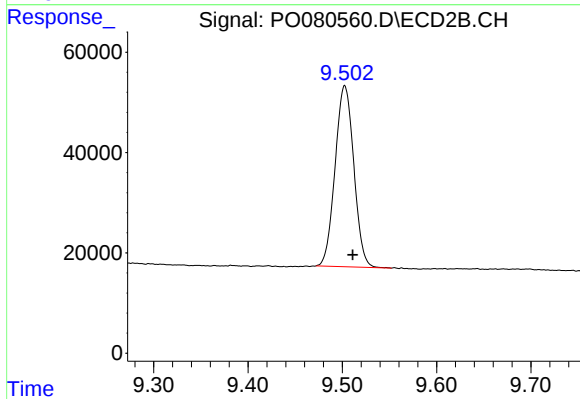

#2 Decachlorobiphenyl

R.T.: 9.503 min
Delta R.T.: -0.009 min
Response: 497438
Conc: 21.93 ng/ml