

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081721\
 Data File : P0080593.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Aug 2021 7:51
 Operator : DD\AJ
 Sample : M3435-35
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2021-08-12-EB-03

Manual Integrations
 APPROVED

mohammad
 8/18/2021 2:07:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 08:35:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.990	4.105	1724226	591649	24.900m	23.738
2) SA Decachlor...	11.088	9.500	1162322	470265	22.455	20.733

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081721\
Data File : PO080593.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Aug 2021 7:51
Operator : DD\AJ
Sample : M3435-35
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2021-08-12-EB-03


Manual Integrations
APPROVED

mohammad
8/18/2021 2:07:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 08:35:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

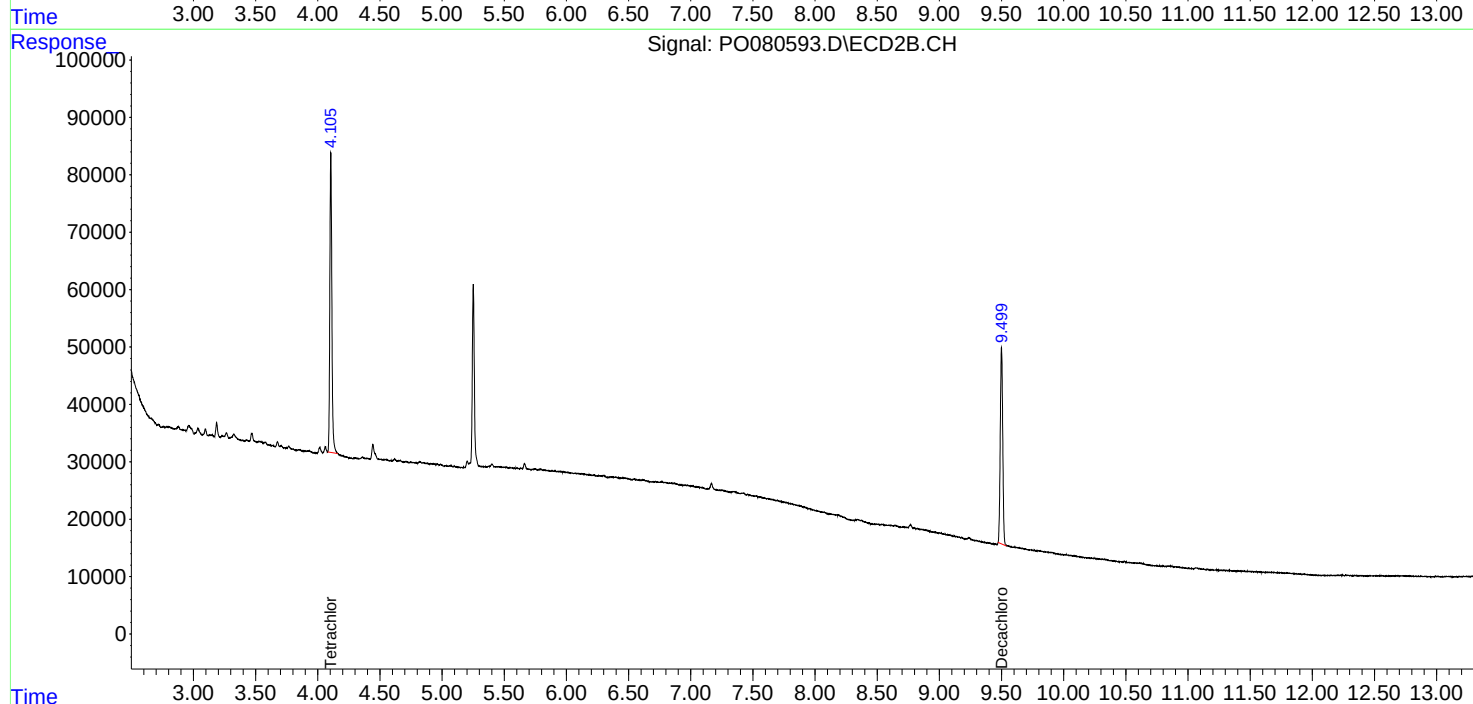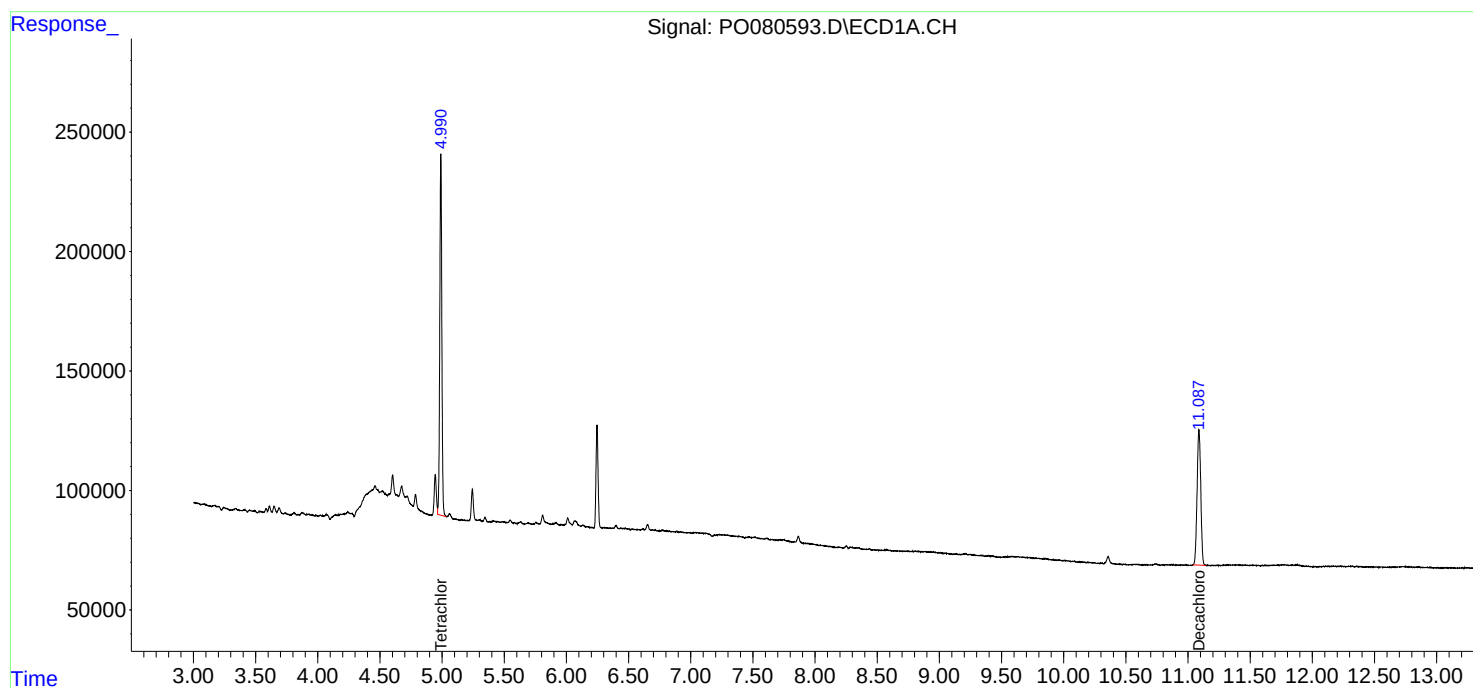

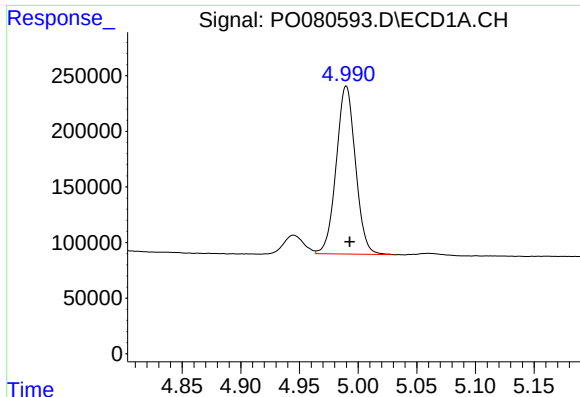


#1 Tetrachloro-m-xylene

R.T.: 4.990 min
Delta R.T.: -0.003 min
Response: 1724226
Conc: 24.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
2021-08-12-EB-03


Manual Integrations
APPROVED

mohammad
8/18/2021 2:07:24 PM

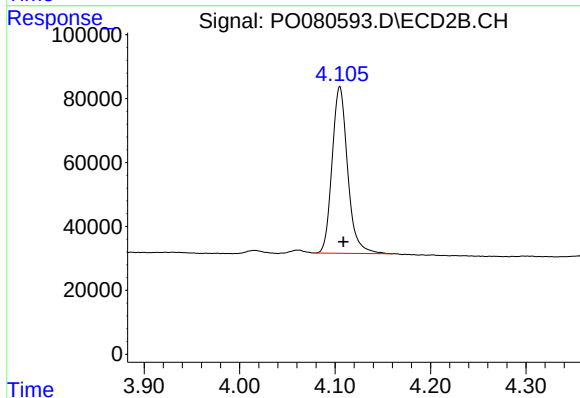


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: -0.004 min
Response: 591649
Conc: 23.74 ng/ml

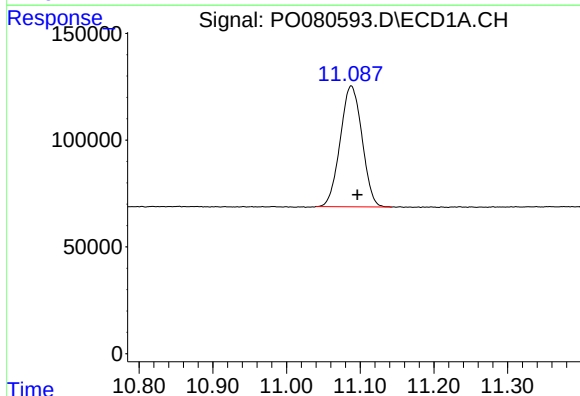

#2 Decachlorobiphenyl

R.T.: 11.088 min
Delta R.T.: -0.009 min
Response: 1162322
Conc: 22.45 ng/ml

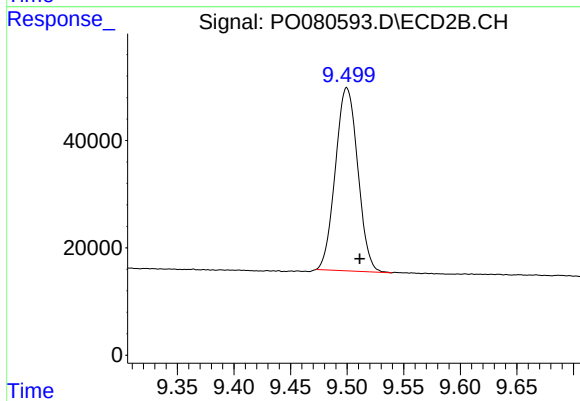

#2 Decachlorobiphenyl

R.T.: 9.500 min
Delta R.T.: -0.011 min
Response: 470265
Conc: 20.73 ng/ml